

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130295

Supervisor / Operator Performing the Verification Procedure:

Name: William A. Mills ✓

ID#: 2688

Date: May 22, 2008 ✓

A. Agency: Hoonah Police Department ✓

Phone #: 945-3655

Instrument Location: 379 Raven Drive, Hoonah

Alco S/N: X124669 ✓

Target Value: .083 ✓ High Pressure: 700 psi

B. Alco Test Value Average: .081 ✓
1st Alco

.081 ✓
2nd Alco

Signature



(OVER)

CSB
6/5/08



Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, William Mills, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

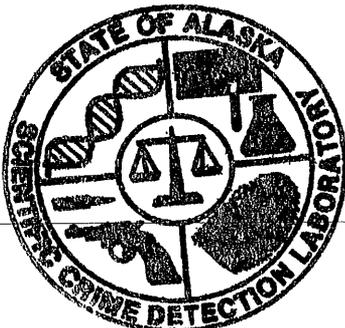

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

Date

6/9/08

MAY 27 2008

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130295

MAY 22, 2008

COB 6/15/08
OPERATOR'S NAME:
MILLS WILLIAM
OPERATOR'S NUMBER: 2608
SUBJECT'S LAST NAME:
VERIFICATION OF
SUBJECT'S FIRST NAME/MI :
CALIBRATION
O.L. #: 1234567890
DEPT/AGENCY: HNH1
CASE/REPORT: 1234567890
TEST TYPE: U
ALCO TARGET VALUE: .083
ALCO S/N: X124669

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 30.55 in
ALCO TARGET .004 20:32
BLANK TEST .000 20:33
INTERNAL STANDARD VERIFIED 20:33
ALCO TV 30.53 in .081 20:33
BLANK TEST .000 20:34
SUBJECT SAMPLE .000 *COB* 20:35
BLANK TEST .000 *6/15/08* 20:36
ALCO TV 30.53 in .081 20:36
BLANK TEST .000 20:37

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130295

MAY 22, 2008
TIME 20:30

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 30.55 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghi jklmno
pqrstuvwxyz{|}~

30:11/16