

VERIFICATION OF CALIBRATION REPORT

DEC 03 2009

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130579</u>
A	Name	<u>Chris RITAN</u>	ID# <u>3791</u> Date <u>11/25/09</u>
	Agency	<u>Anchorage Police Dept.</u>	Phone # <u>786-2140</u>
	Instrument Location	<u>ANCHORAGE Jail</u>	
B	Alco S/N	<u>78995</u>	Target Value <u>081</u> High Pressure <u>1050</u>
	Alco Test Value Average	<u>081</u> 1 st Alco	<u>081</u> 2 nd Alco
	Signature	<u>Chris Ritan</u> / RITAN 1349	

(OVER)

*AMB
12/28/09*

(Do Not write in the area below)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 28th day of Dec, 2009.

Carolyn M. Noland
 Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


DataMaster cdm S/N

130579


(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

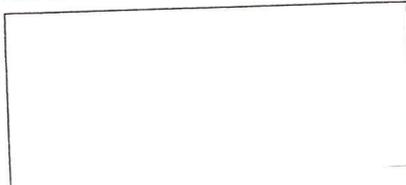

DIAGNOSTIC CHECK

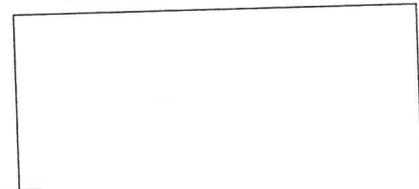

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

NOVEMBER 25, 2009

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

INSTALL NEW ALCO TANK

O.L. #: A

DEPT/AGENCY: ANCL

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: 081

ALCO S/N: 78895

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.31 in ✓
ALCO TARGET .079 16:08
BLANK TEST .000 16:09
INTERNAL STANDARD VERIFIED 16:09
ALCO TV 29.31 in .081 16:09
BLANK TEST .000 16:10
SUBJECT SAMPLE *BMB* .000 16:10
BLANK TEST .000 16:11
ALCO TV 29.31 in *12/28/09* .081 16:12
BLANK TEST .000 16:12

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130579

NOVEMBER 25, 2009
TIME 16:13

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 12/11/08
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.31 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefg
hijklmno
pqrstuvwxyz{|}~^