

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100346

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 03/15/2011

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.33: 0.078
LOT #: 02511080A1
EXPIRATION: 02/01/2013

BLANK TEST	0.000	13:10
INTERNAL STANDARD	VERIFIED	13:10
EXTERNAL STANDARD	0.078	13:10
BLANK TEST	0.000	13:11
EXTERNAL STANDARD	0.077	13:11
BLANK TEST	0.000	13:12
EXTERNAL STANDARD	0.077	13:12
BLANK TEST	0.000	13:13
EXTERNAL STANDARD	0.077	13:13
BLANK TEST	0.000	13:14
EXTERNAL STANDARD	0.076	13:14
BLANK TEST	0.000	13:15

Average = 0.0770
Std Dev = 0.0007

Diagnostic Check

VERSIONS
DMT: 1.01
PIC: 3.01
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
Breath Tube = 38.5°C PASSED

PUMP INFO

Flow Rate = 5.018 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

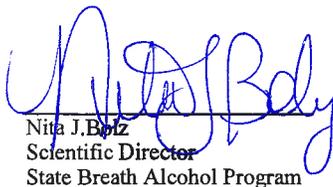
FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.



Nita J. Bolz
Scientific Director
State Breath Alcohol Program

5/13/11

Subscribed and sworn before me this 13 day of MAY, 20 11


Notary Public's Signature
Commission Expires on WITH

KYLE KLOPFER
Notary Name
OFFICE




KMB
5/13/11