

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100348

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 03/15/2011

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.34: 0.078
LOT #: 02511080A1
EXPIRATION: 02/01/2013

BLANK TEST	0.000	13:20
INTERNAL STANDARD	VERIFIED	13:20
EXTERNAL STANDARD	0.079	13:20
BLANK TEST	0.000	13:21
EXTERNAL STANDARD	0.079	13:21
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.079	13:22
BLANK TEST	0.000	13:23
EXTERNAL STANDARD	0.078	13:24
BLANK TEST	0.000	13:24
EXTERNAL STANDARD	0.078	13:25
BLANK TEST	0.000	13:26

Average = 0.0786
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 1.01
PIC: 3.02
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 44.6°C PASSED

PUMP INFO

Flow Rate = 4.881 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

FILTER INFO


Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD

PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

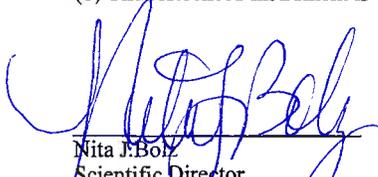
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

4/14/11

Subscribed and sworn before me this 14 day of APRIL, 20 11




Notary Public's Signature
My Commission Expires on WITH OFFICE

KYLE KLOPFER
Notary Name

BMB
3/23/11