

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100359

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 06/29/2012

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.05: 0.080  
LOT #: 07511080A1  
EXPIRATION: 03/01/2013

BLANK TEST	0.000	13:49
INTERNAL STANDARD	VERIFIED	13:49
EXTERNAL STANDARD	0.077	13:49
BLANK TEST	0.000	13:50
EXTERNAL STANDARD	0.077	13:50
BLANK TEST	0.000	13:51
EXTERNAL STANDARD	0.077	13:52
BLANK TEST	0.000	13:53
EXTERNAL STANDARD	0.077	13:53
BLANK TEST	0.000	13:54
EXTERNAL STANDARD	0.077	13:54
BLANK TEST	0.000	13:55

Average = 0.0770  
Std Dev = 0.0000

## Diagnostic Check

### VERSIONS

DMT: 2.00  
PIC: 3.02  
Modem: 2.3  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 46.6°C PASSED

### PUMP INFO

Flow Rate = 4.402 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.


(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.

(5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.

(6) The referenced instrument is certified for evidentiary use in the State of Alaska.

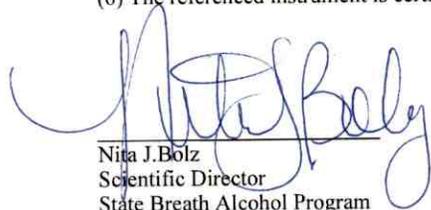
 8/7/2012

Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 7<sup>th</sup> day of Aug. 20 12



Nikki Roth, Notary Public  
My Commission Expires With Office

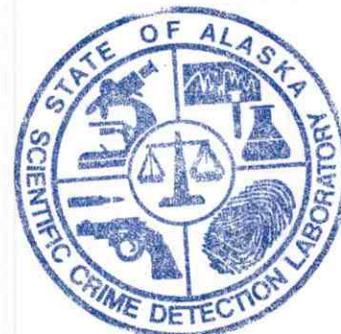

003 7/30/12