

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100364

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 04/14/2011

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.85: 0.079
LOT #: 33609080A1
EXPIRATION: 01/01/2012

BLANK TEST	0.000	09:57
INTERNAL STANDARD	VERIFIED	09:57
EXTERNAL STANDARD	0.079	09:57
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.078	09:59
BLANK TEST	0.000	09:59
EXTERNAL STANDARD	0.078	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.078	10:01
BLANK TEST	0.000	10:02
EXTERNAL STANDARD	0.078	10:02
BLANK TEST	0.000	10:03

Average = 0.0782
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 1.01
PIC: 3.02
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 5.191 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED

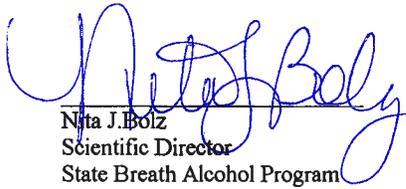
FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

5/13/11

Subscribed and sworn before me this 13 day of MAY, 20 11




Notary Public's Signature
My Commission Expires on W/TH OFFICE
KYLE KLOPFER
Notary Name

CRF
4/14/11