

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument
State of Alaska

Serial #: 100371

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 03/23/2011

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.82: 0.079
LOT #: 02511080A3
EXPIRATION: 02/01/2013

BLANK TEST	0.000	08:20
INTERNAL STANDARD	VERIFIED	08:21
EXTERNAL STANDARD	0.081	08:21
BLANK TEST	0.000	08:22
EXTERNAL STANDARD	0.080	08:22
BLANK TEST	0.000	08:23
EXTERNAL STANDARD	0.080	08:23
BLANK TEST	0.000	08:24
EXTERNAL STANDARD	0.080	08:24
BLANK TEST	0.000	08:25
EXTERNAL STANDARD	0.080	08:25
BLANK TEST	0.000	08:26

Average = 0.0802
Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 1.01
PIC: 3.02
Modem: 2.0
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
Breath Tube = 48.1°C PASSED

PUMP INFO

Flow Rate = 5.217 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
PUMP OFF PASSED


FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

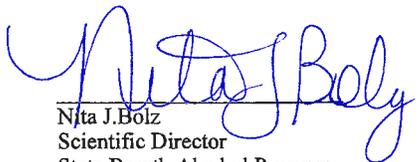
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

5/31/11

Subscribed and sworn before me this 31 day of MAY, 20 11


Notary Public's Signature
My Commission Expires on WITH OFFICE
KYLE KLOPPER
Notary Name




JMB
3/23/11