

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100377

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 09/12/2012

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.46: 0.078  
LOT #: 02012080A1  
EXPIRATION: 03/01/2014

BLANK TEST	0.000	09:00
INTERNAL STANDARD	VERIFIED	09:00
EXTERNAL STANDARD	0.079	09:00
BLANK TEST	0.000	09:01
EXTERNAL STANDARD	0.079	09:02
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.079	09:03
BLANK TEST	0.000	09:04
EXTERNAL STANDARD	0.079	09:04
BLANK TEST	0.000	09:05
EXTERNAL STANDARD	0.079	09:05
BLANK TEST	0.000	09:06

Average = 0.0790  
Std Dev = 0.0000

## Diagnostic Check

VERSIONS  
DMT: 2.00  
PIC: 3.02  
Modem: 2.3  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 49.0°C PASSED  
Breath Tube = 48.1°C PASSED

### PUMP INFO

Flow Rate = 5.114 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED


INTERNAL STANDARD PASSED



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

 10/4/2012  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 4<sup>th</sup> day of Oct, 20 12

  
Nikki Roth, Notary Public  
My Commission Expires With Office

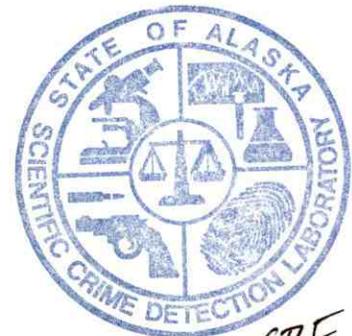

CRF  
9/20/12