

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100384

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 08/29/2012

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 30.08: 0.080  
LOT #: 07511080A1  
EXPIRATION: 03/01/2013

BLANK TEST	0.000	11:07
INTERNAL STANDARD	VERIFIED	11:07
EXTERNAL STANDARD	0.078	11:07
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.076	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.077	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.077	11:11
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.077	11:12
BLANK TEST	0.000	11:13

Average = 0.0770  
Std Dev = 0.0007

## Diagnostic Check

VERSIONS  
DMT: 2.00  
PIC: 3.02  
Modem: 2.3  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.9°C PASSED  
Breath Tube = 46.4°C PASSED

### PUMP INFO

Flow Rate = 4.642 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED


### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

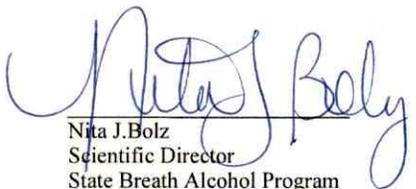 10/4/2012  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 4<sup>th</sup> day of Oct, 20 12

  
Nikki Roth, Notary Public  
My Commission Expires With Office

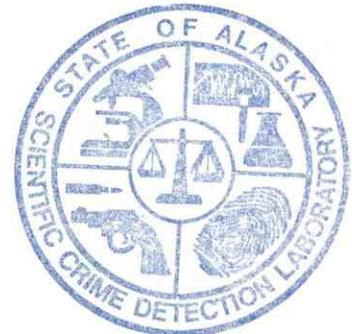

  
8/30/12