

VERIFICATION OF CALIBRATION REPORT

*of DataMaster dmt Breath Test Instrument
State of Alaska*

Serial #: 100667

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 07/18/2012

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 3.080
 TARGET AT 29.54: 0.078
 LOT #: 02J12080A1
 EXPIRATION: 03/01/2014

BLANK TEST	0.000	12:02
INTERNAL STANDARD	VERIFIED	12:02
EXTERNAL STANDARD	0.076	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.077	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.077	12:05
BLANK TEST	0.000	12:06
EXTERNAL STANDARD	0.077	12:06
BLANK TEST	0.000	12:07
EXTERNAL STANDARD	0.077	12:07
BLANK TEST	0.000	12:08

Average = 0.0768
 Std Dev = 0.0004

Diagnostic Check

VERSIONS

DMT: 2.00
 PIC: 3.03
 Modem: 2.3
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
 Breath Tube = 46.1°C PASSED

PUMP INFO

Flow Rate = 5.192 L/M PASSED

DETECTOR INFO

PUMP ON PASSED
 PUMP OFF PASSED

FILTER INFO

Filter 1 PASSED
 Filter 2 PASSED
 Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

8/7/2012

Subscribed and sworn before me this 7th day of Aug. 20 12

Nikki Roth
 Nikki Roth, Notary Public
 My Commission Expires With Office

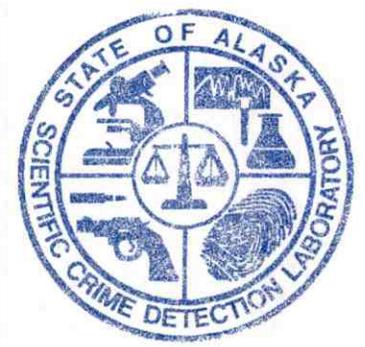

COB 7/31/12