

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100420

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 02/23/2016

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 28.59: 0.076  
LOT #: 09214080A3  
EXPIRATION: 05/01/2016  
TANK PRESSURE: 497 psi

BLANK TEST	0.000	11:11
INTERNAL STANDARD	VERIFIED	11:11
EXTERNAL STANDARD	0.075	11:11
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.075	11:12
BLANK TEST	0.000	11:13
EXTERNAL STANDARD	0.075	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.074	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.075	11:16
BLANK TEST	0.000	11:16

Average = 0.0748  
Std Dev = 0.0004

## Diagnostic Check

### VERSIONS

DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.7°C PASSED  
Breath Tube = 44.5°C PASSED

### PUMP INFO

Flow Rate = 4.814 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED


### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED

I, Charles R. Foster, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist III at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Acting Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.




3/4/16

Charles R. Foster  
Acting Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 4<sup>th</sup> day of Mar. 20 16



Nikki Roth, Notary Public  
My Commission Expires With Office

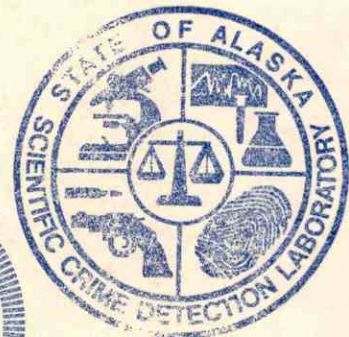

BMB  
2/24/16