




State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100345

Report Issue Date: 03/10/2026
Date Received: 2025-12-16
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

| As-Found Data | | | | | | | | |
|-------------------------|------------------------|------------|------------------|-------|-------|-------|-------|---------------|
| Nominal Values (g/210L) | Target Values (g/210L) | Lot Number | Results (g/210L) | | | | | Mean (g/210L) |
| 0.020 | 0.020 | AG408002 | 0.020 | 0.020 | 0.020 | 0.020 | 0.019 | 0.020 |
| 0.080 | 0.078 | AG436502 | 0.078 | 0.077 | 0.077 | 0.076 | 0.077 | 0.077 |
| 0.300 | 0.293 | AG427706 | 0.289 | 0.287 | 0.287 | 0.287 | 0.288 | 0.288 |

As Found - Evaluation Analyst: Kaija Swisher
 As Found Conditions - Barometric Pressure (inHg): 29.22 Barometer Used: VWR S/N 240680771 Temperature (C): 20.1 Relative Humidity (%): 0
 As-Found Lab Activity Date Range: 12/16/2025 - 12/16/2025

VOC failed twice due to filter wheel errors but passed on the third attempt. Repair is recommended.

| As-Left Data | | | | | | | | | |
|-------------------------|------------------------|------------|------------------|-------|-------|-------|-------|---------------|----------------------|
| Nominal Values (g/210L) | Target Values (g/210L) | Lot Number | Results (g/210L) | | | | | Mean (g/210L) | Uncertainty (g/210L) |
| 0.020 | 0.020 | AG408002 | 0.020 | 0.020 | 0.020 | 0.021 | 0.021 | 0.020 | +/- 0.002 |
| 0.040 | 0.040 | AG407908 | 0.040 | 0.040 | 0.041 | 0.041 | 0.040 | 0.040 | +/- 0.003 |
| 0.080 | 0.080 | AG436502 | 0.080 | 0.080 | 0.080 | 0.080 | 0.080 | 0.080 | +/- 0.004 |
| 0.100 | 0.100 | AG516101 | 0.099 | 0.099 | 0.099 | 0.099 | 0.099 | 0.099 | +/- 0.004 |
| 0.150 | 0.150 | AG515604 | 0.149 | 0.148 | 0.149 | 0.148 | 0.149 | 0.149 | +/- 0.006 |
| 0.300 | 0.300 | AG427706 | 0.301 | 0.300 | 0.300 | 0.300 | 0.301 | 0.300 | +/- 0.012 |

As Left Conditions - Barometric Pressure (inHg): 29.87 Barometer Used: VWR S/N 240680771 Temperature (C): 19.4 Relative Humidity (%): 9
 As-Left Lab Activity Date Range: 02/18/2026 - 02/19/2026

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 03/09/2026

colleen.obryant@alaska.gov

Technically and administratively reviewed by Derek Walton on 03/10/2026

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100345 Analyst or Technician Name: C. O. Bryant

DataMaster DMT Calibration Start Date: 2/18/26

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 10 Sep 2026
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.87 Temperature(C) 19.4 Relative Humidity(%) 9

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
 - Invalid
 - Interference (Volatiles) - *Print with View Details*
 - Maximum Attempts Exceeded
 - Radio Frequency Interference (RFI) 5/18/2026 COB 2026.03.09
1. Acetone Reagent Lot Number: 20260218COB Expiration Date: 10/31/2026
Simulator S/N: 501088 Thermometer Verification Performed? 5/18/2026 COB 2026.03.09
 2. Isopropanol Reagent Lot Number: 20260218COB Expiration Date: 3/19/27
Simulator S/N: 501199 Thermometer Verification Performed?
 3. Negative (Ethanol Only) Lot Number: 25CP41080 Expiration Date: 3/19/27
Simulator S/N: 501177 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 14 Mar 2027

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 2/19/26

Data Interpretation Date (Technician): _____ (if applicable)

Data Interpretation Date (Analyst): 2/19/26

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/18/2026
Time: 12:23:18

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 46.4°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.70 V PASSED
(1.02 V - 2.38 V)
Cooler Voltage = 1.66 V PASSED
(1.00 V - 2.32 V)
Bias Voltage = 80 V PASSED
(48 V - 112 V)
Chopper Fréq = 535 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.9 in

PUMP INFO

Flow Rate = 4.333 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 V <= 0.010 V)
PUMP OFF PASSED
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.090 0.00% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100345

Date: 02/18/2026
Time: 12:35 PM

Temperatures (°C)

Sample Cell: 49.1°C
Breath Tube: 47.3°C

Current Barometer 29.9 in
Volume (Ltr) 1.42

Settings

Lamp: 1.72 V
Bias: 80 V
Cooler: 1.69 V
Chopper: 534 Hz

Voltages (V)

Flow: 1.06 V
Detector: -0.052 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/03/2026
Time: 11:54:06

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca = 0.1000
CAL = 0.990650 0.800 <= CAL < 1.200
b1 = 0.0009 0.0000 <= b1 < 0.0040
b2 = 0.0064 0.0010 <= b2 < 0.0100
b3 = 0.0012 0.0000 <= b3 < 0.0040
Xq = 0.0898 0.0500 <= Xq < 0.2000
a21 = 1.150953 1.050 <= a21 < 1.300
a31 = 0.496050 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/18/2026
Time: 12:37:52

SUBJECT NAME:
TEST TEST
LICENSE #: MIN VOLUME

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1

CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.92: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

| DIAGNOSTIC CHECK | PASSED | 12:38 |
|----------------------------|----------|-------|
| BLANK TEST | 0.000 | 12:39 |
| INTERNAL STANDARD | VERIFIED | 12:39 |
| EXTERNAL STANDARD | 0.080 | 12:39 |
| BLANK TEST | 0.000 | 12:40 |
| SUBJECT SAMPLE (Vol=1.56L) | 0.000 | 12:41 |
| BLANK TEST | 0.000 | 12:42 |
| EXTERNAL STANDARD | 0.080 | 12:42 |
| BLANK TEST | 0.000 | 12:43 |

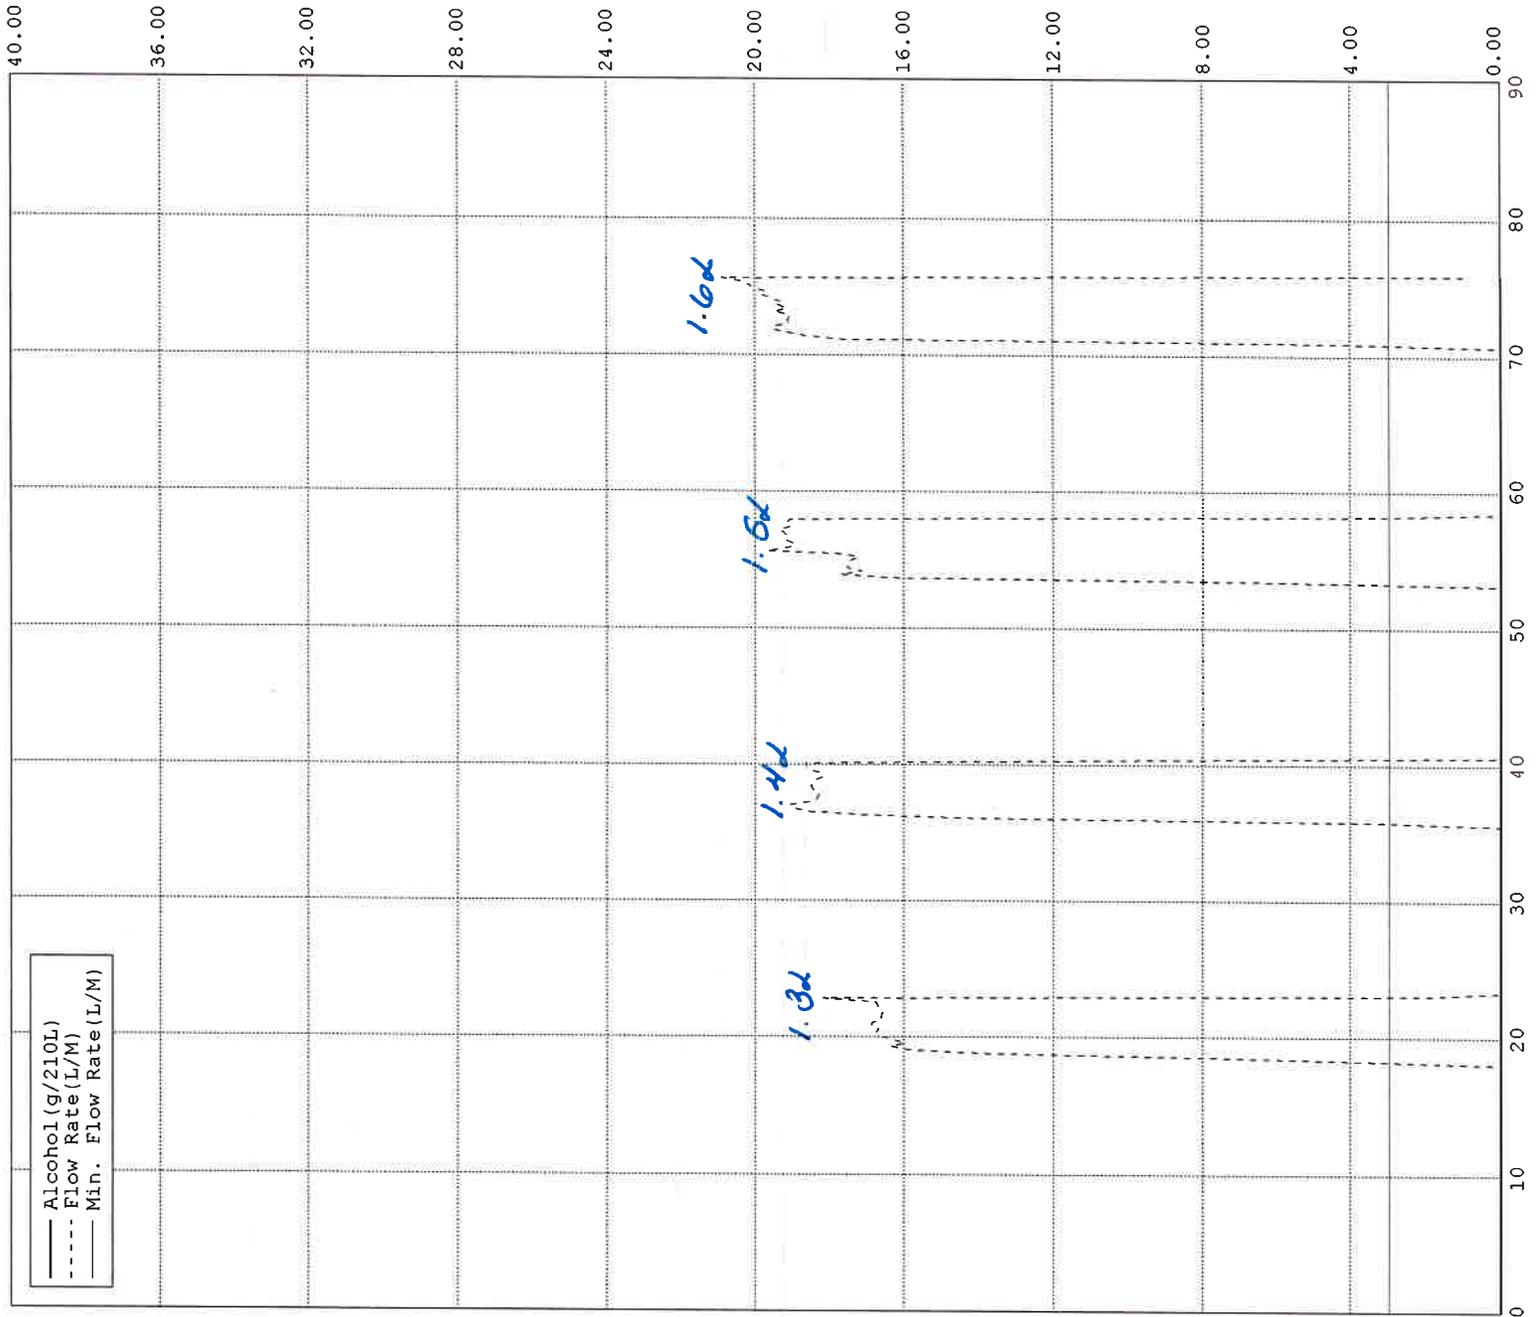

LINEARITY CHECK

 Alaska Department of Public Safety
 DATAMASTER dmt: 100345


Date: 02/19/2026
 Time: 07:06:14

SUPERVISOR NAME:
 COLLEEN S OBRyant
 OPERATOR'S #: 6237

| TARGET | AVERAGE | STD. DEV. |
|--------|---------|-----------|
| 0.020 | 0.0204 | 0.0005 |
| 0.040 | 0.0404 | 0.0005 |
| 0.080 | 0.0800 | 0.0000 |
| 0.100 | 0.0990 | 0.0000 |
| 0.150 | 0.1486 | 0.0005 |
| 0.300 | 0.3004 | 0.0005 |

SLOPE = 0.999457
 R² = 0.999938

CS

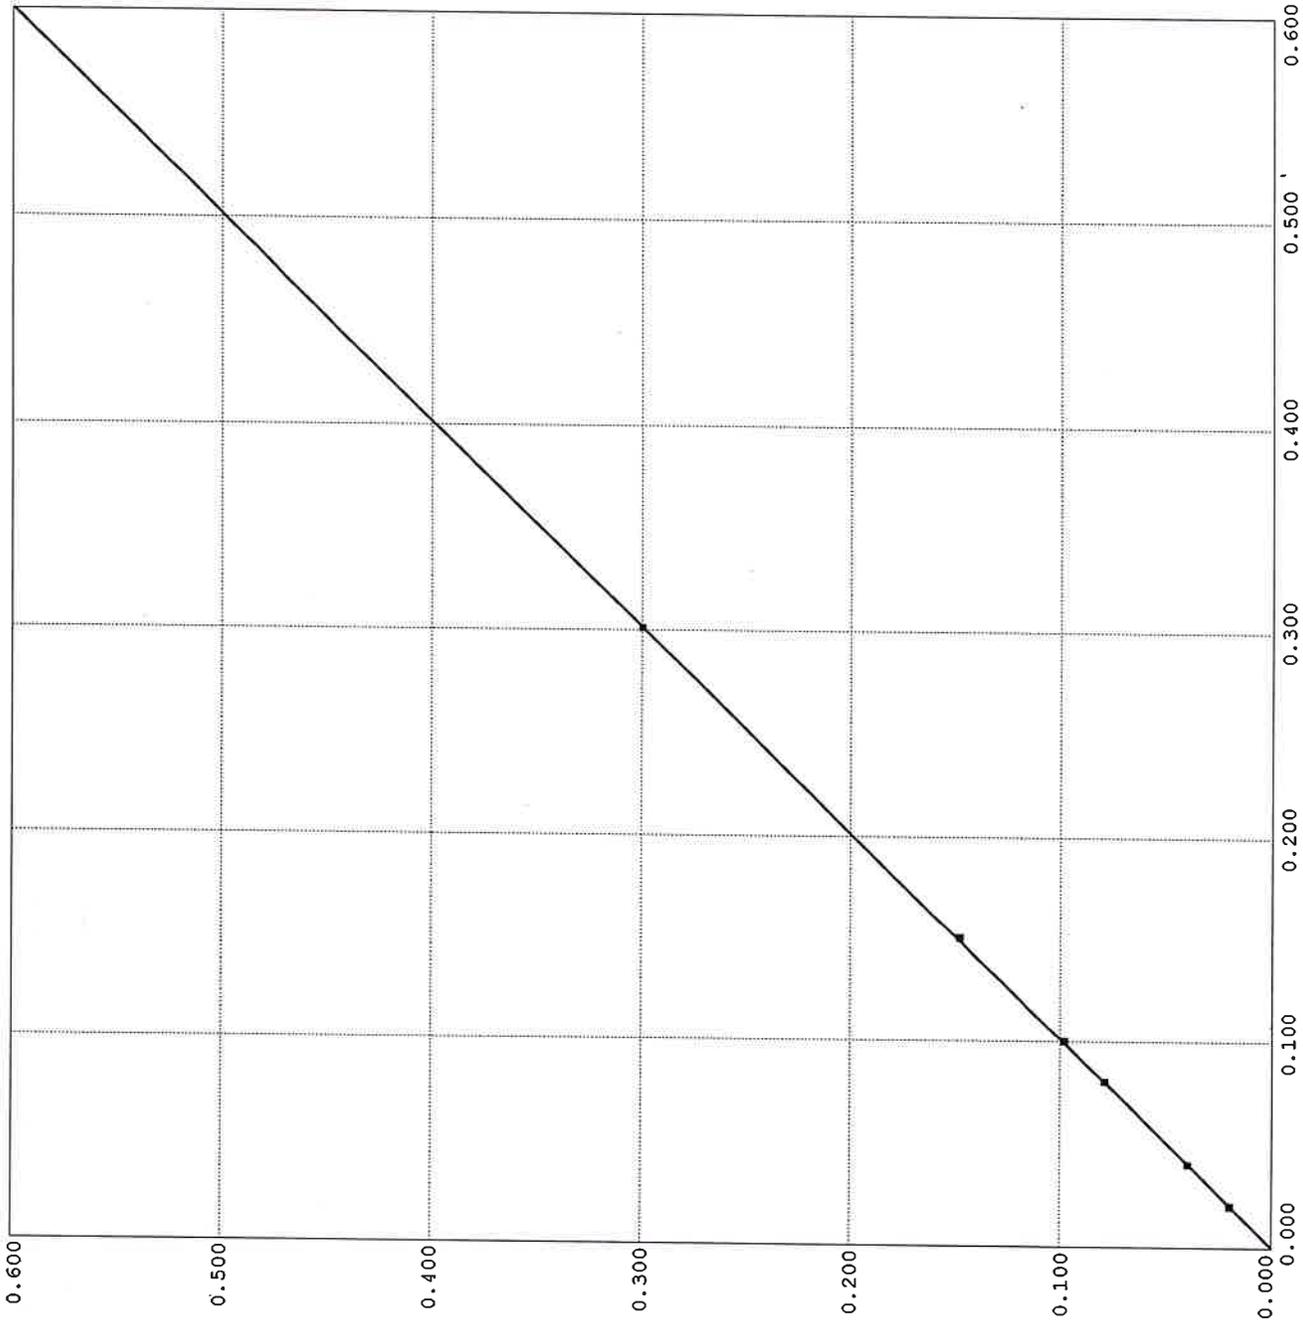

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100345






Date: 02/19/2026
 Time: 07:06:16

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.88: 0.020
 LOT #: AG403002 AG408002 *COB 2/25/26*
 EXPIRATION: 03/20/2026
 TANK PRESSURE: 832 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 07:07 |
| INTERNAL STANDARD | VERIFIED | 07:07 |
| EXTERNAL STANDARD | 0.020 | 07:07 |
| BLANK TEST | 0.000 | 07:08 |
| EXTERNAL STANDARD | 0.020 | 07:08 |
| BLANK TEST | 0.000 | 07:09 |
| EXTERNAL STANDARD | 0.020 | 07:09 |
| BLANK TEST | 0.000 | 07:10 |
| EXTERNAL STANDARD | 0.021 | 07:10 |
| BLANK TEST | 0.000 | 07:11 |
| EXTERNAL STANDARD | 0.021 | 07:11 |
| BLANK TEST | 0.000 | 07:12 |

Average = 0.0204
 Std Dev = 0.0005

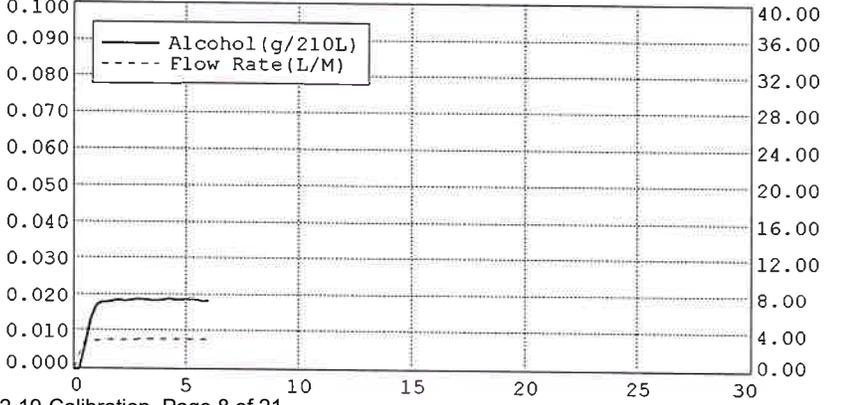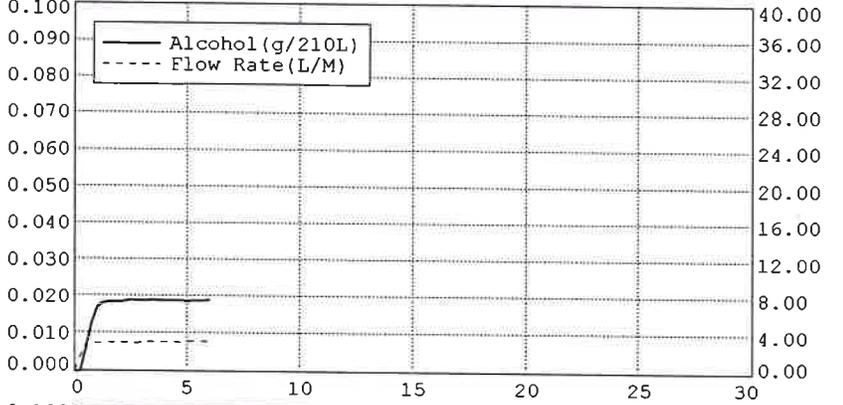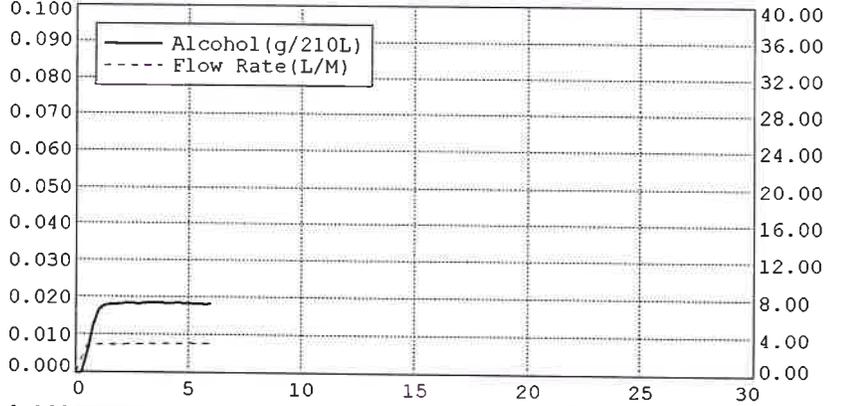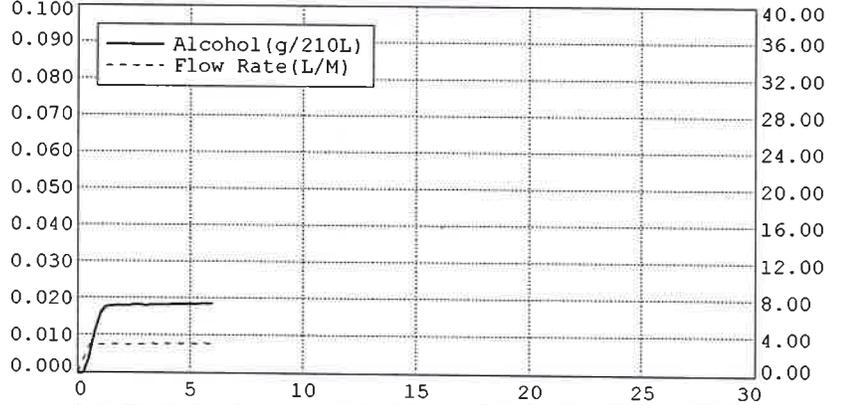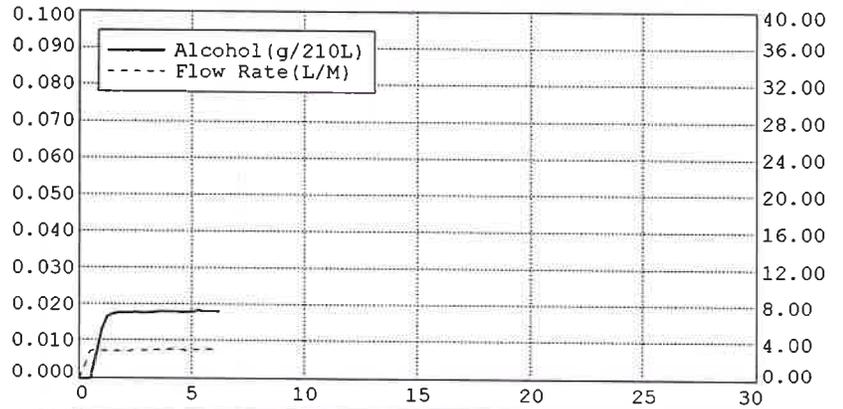

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
 DATAMASTER dmt: 100345






Date: 02/19/2026
 Time: 07:14:50

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
 TARGET AT 29.88: 0.040
 LOT #: AG407908
 EXPIRATION: 03/19/2026
 TANK PRESSURE: 642 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 07:16 |
| INTERNAL STANDARD | VERIFIED | 07:16 |
| EXTERNAL STANDARD | 0.040 | 07:16 |
| BLANK TEST | 0.000 | 07:17 |
| EXTERNAL STANDARD | 0.040 | 07:17 |
| BLANK TEST | 0.000 | 07:18 |
| EXTERNAL STANDARD | 0.041 | 07:18 |
| BLANK TEST | 0.000 | 07:19 |
| EXTERNAL STANDARD | 0.041 | 07:19 |
| BLANK TEST | 0.000 | 07:20 |
| EXTERNAL STANDARD | 0.040 | 07:20 |
| BLANK TEST | 0.000 | 07:21 |

Average = 0.0404
 Std Dev = 0.0005

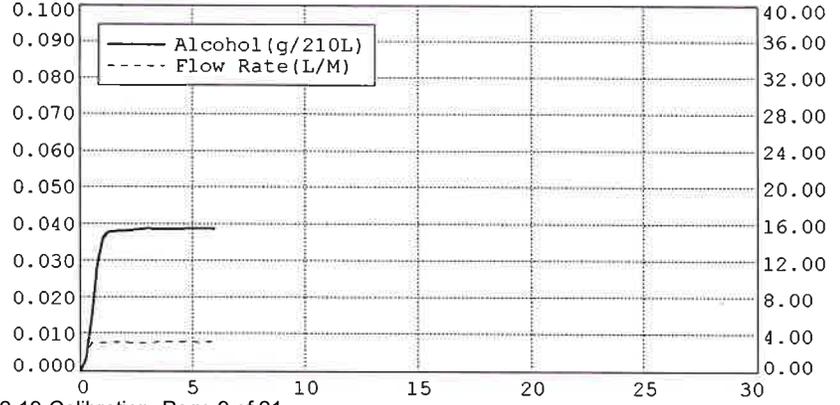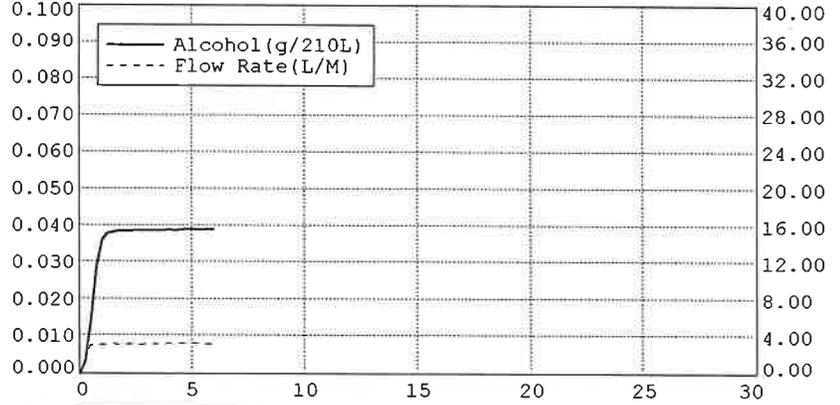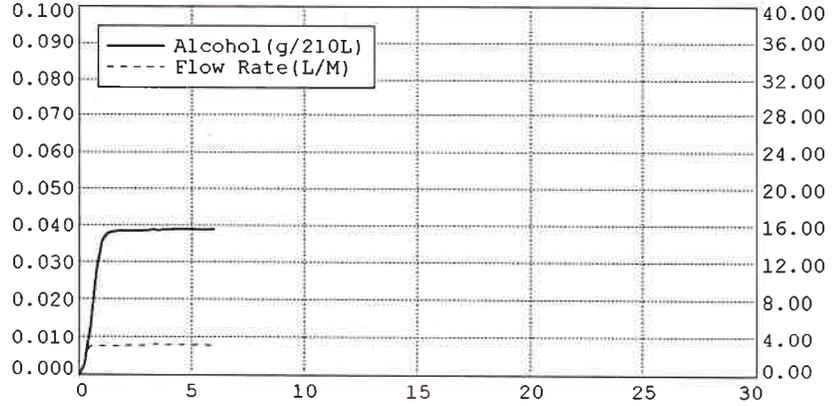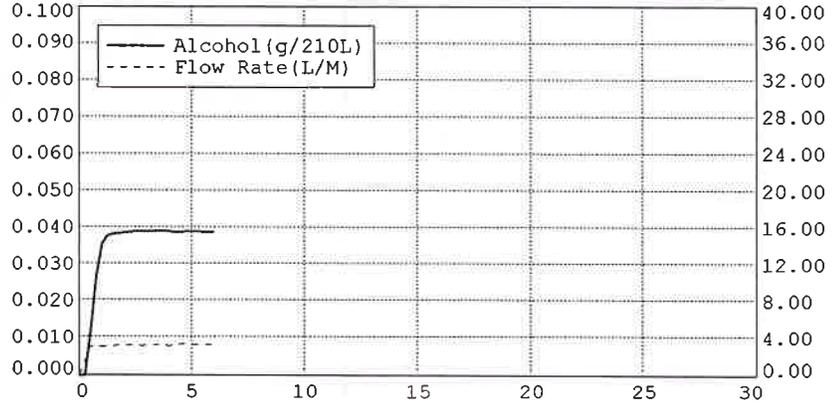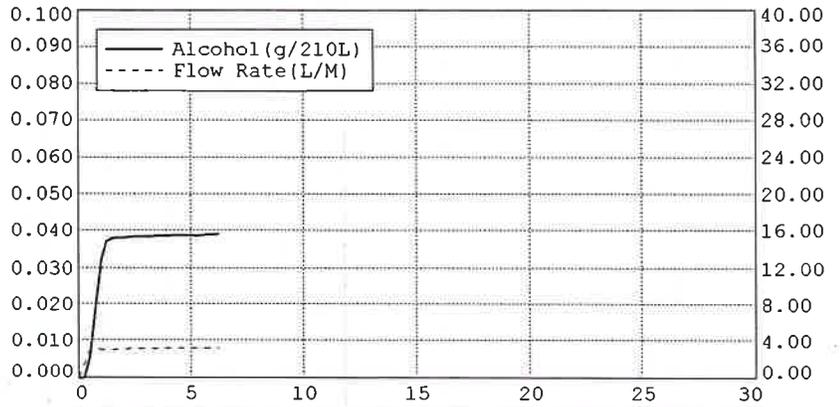

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100345






Date: 02/19/2026
 Time: 07:22:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.87: 0.080
 LOT #: AG436502
 EXPIRATION: 12/30/2026
 TANK PRESSURE: 819 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 07:24 |
| INTERNAL STANDARD | VERIFIED | 07:24 |
| EXTERNAL STANDARD | 0.080 | 07:24 |
| BLANK TEST | 0.000 | 07:25 |
| EXTERNAL STANDARD | 0.080 | 07:25 |
| BLANK TEST | 0.000 | 07:26 |
| EXTERNAL STANDARD | 0.080 | 07:26 |
| BLANK TEST | 0.000 | 07:27 |
| EXTERNAL STANDARD | 0.080 | 07:27 |
| BLANK TEST | 0.000 | 07:28 |
| EXTERNAL STANDARD | 0.080 | 07:28 |
| BLANK TEST | 0.000 | 07:29 |

Average = 0.0800
 Std Dev = 0.0000

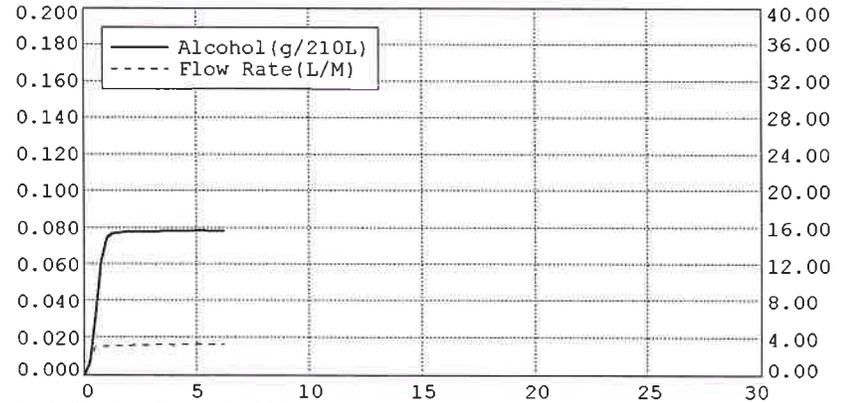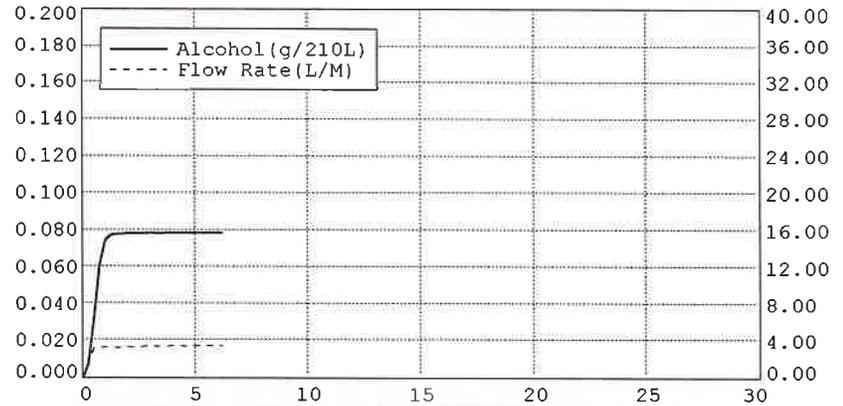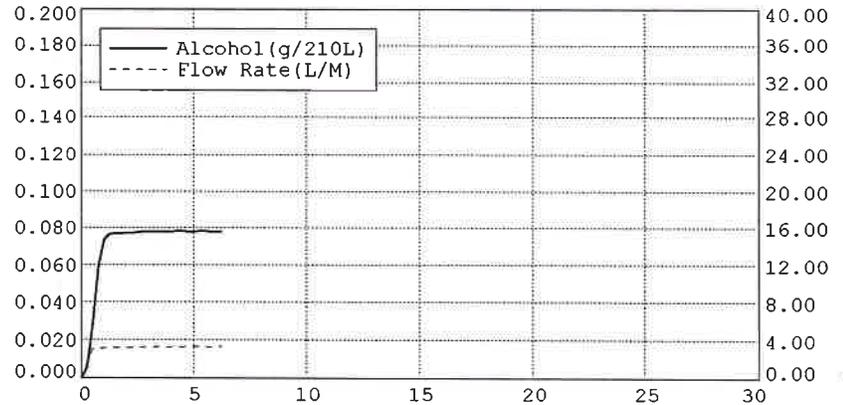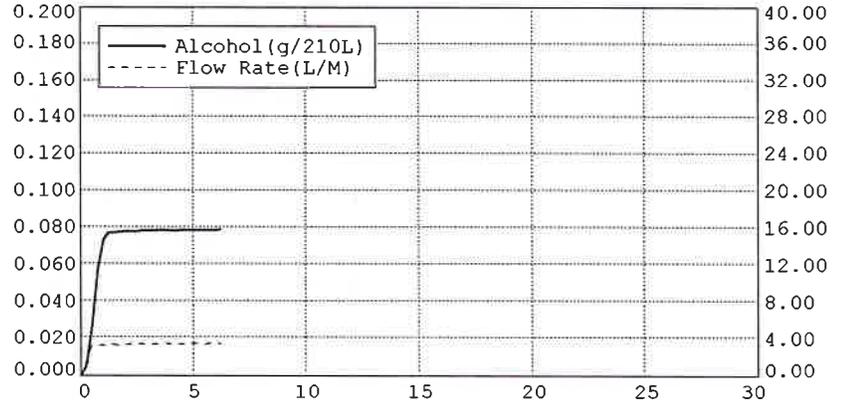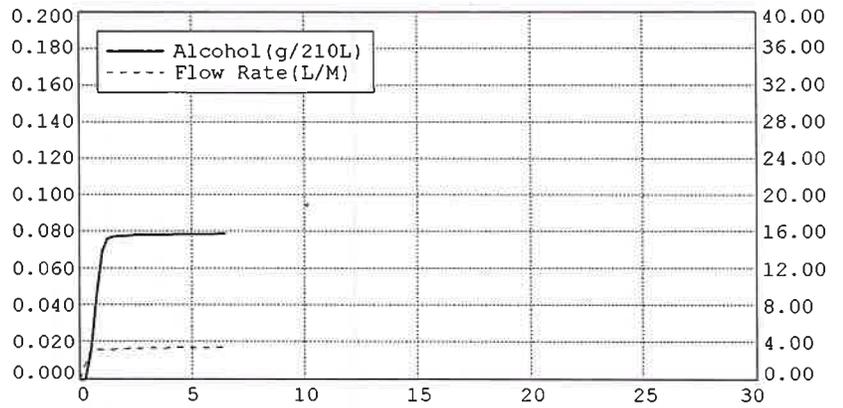

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100345






Date: 02/19/2026
Time: 07:45:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.87: 0.100
LOT #: AG516101
EXPIRATION: 06/10/2027
TANK PRESSURE: 1027 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 07:47 |
| INTERNAL STANDARD | VERIFIED | 07:47 |
| EXTERNAL STANDARD | 0.099 | 07:47 |
| BLANK TEST | 0.000 | 07:48 |
| EXTERNAL STANDARD | 0.099 | 07:48 |
| BLANK TEST | 0.000 | 07:49 |
| EXTERNAL STANDARD | 0.099 | 07:49 |
| BLANK TEST | 0.000 | 07:50 |
| EXTERNAL STANDARD | 0.099 | 07:50 |
| BLANK TEST | 0.000 | 07:51 |
| EXTERNAL STANDARD | 0.099 | 07:51 |
| BLANK TEST | 0.000 | 07:52 |

Average = 0.0990
Std Dev = 0.0000

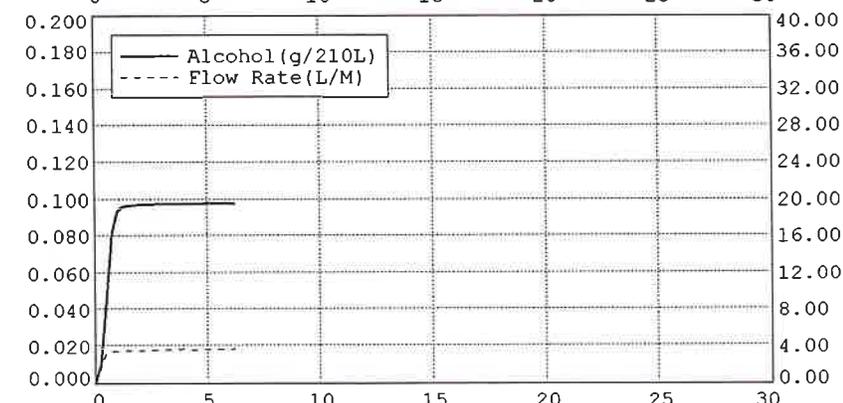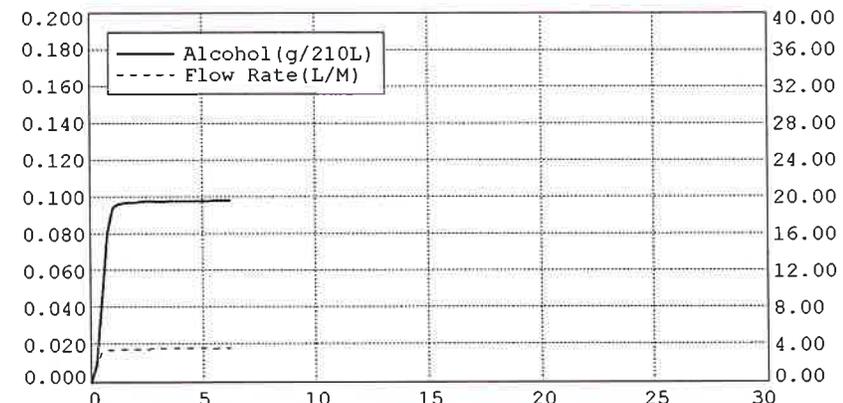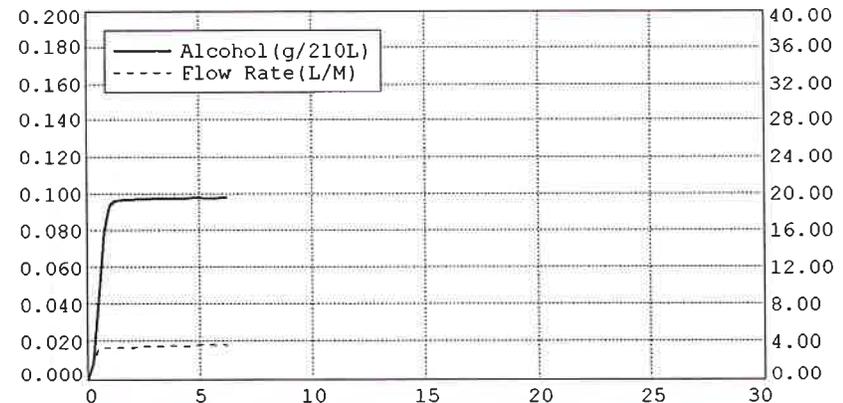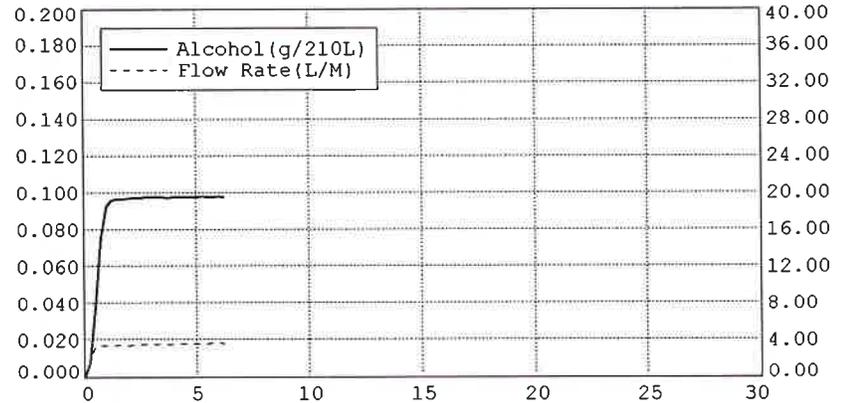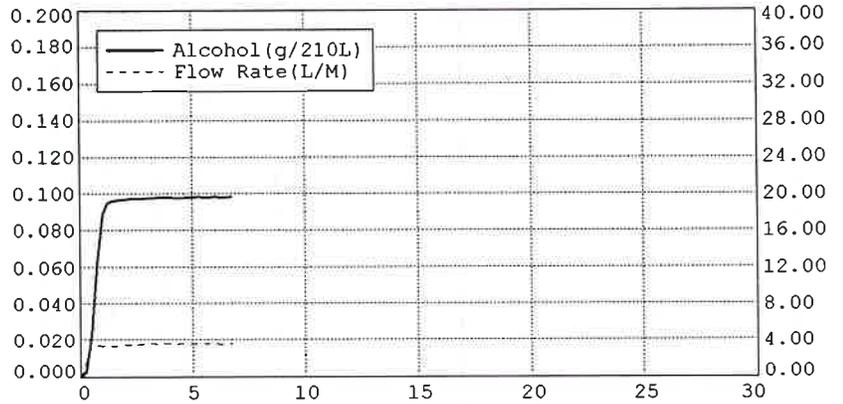

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100345






Date: 02/19/2026
 Time: 07:55:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.88: 0.150
 LOT #: AG515604
 EXPIRATION: 06/05/2027
 TANK PRESSURE: 631 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 07:57 |
| INTERNAL STANDARD | VERIFIED | 07:57 |
| EXTERNAL STANDARD | 0.149 | 07:57 |
| BLANK TEST | 0.000 | 07:58 |
| EXTERNAL STANDARD | 0.148 | 07:58 |
| BLANK TEST | 0.000 | 07:59 |
| EXTERNAL STANDARD | 0.149 | 07:59 |
| BLANK TEST | 0.000 | 08:00 |
| EXTERNAL STANDARD | 0.148 | 08:00 |
| BLANK TEST | 0.000 | 08:01 |
| EXTERNAL STANDARD | 0.149 | 08:01 |
| BLANK TEST | 0.000 | 08:02 |

Average = 0.1486
 Std Dev = 0.0005

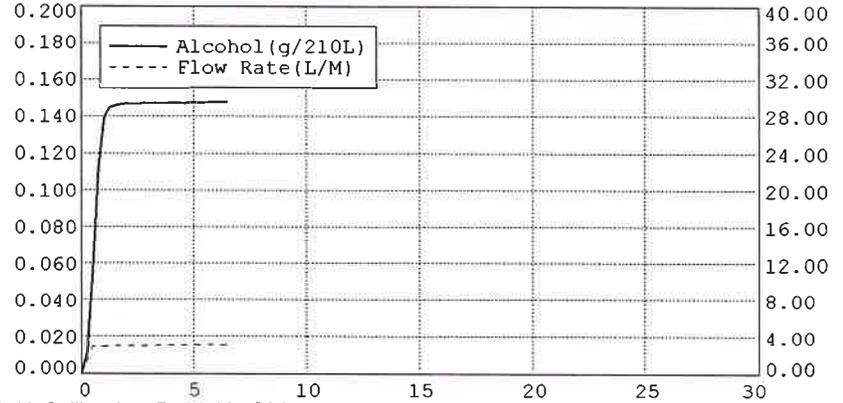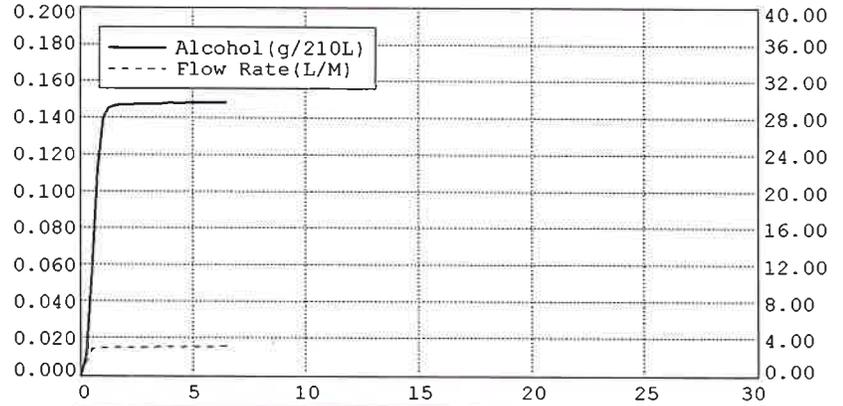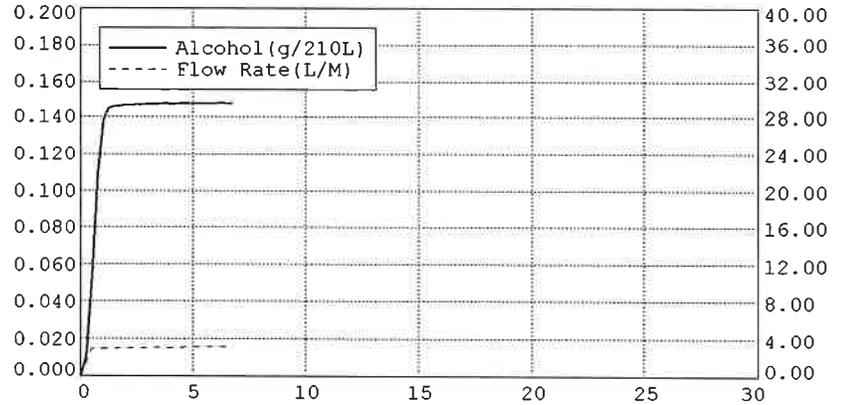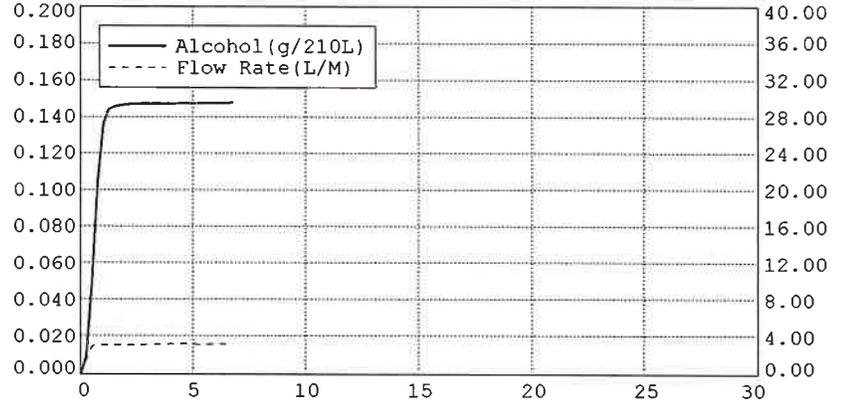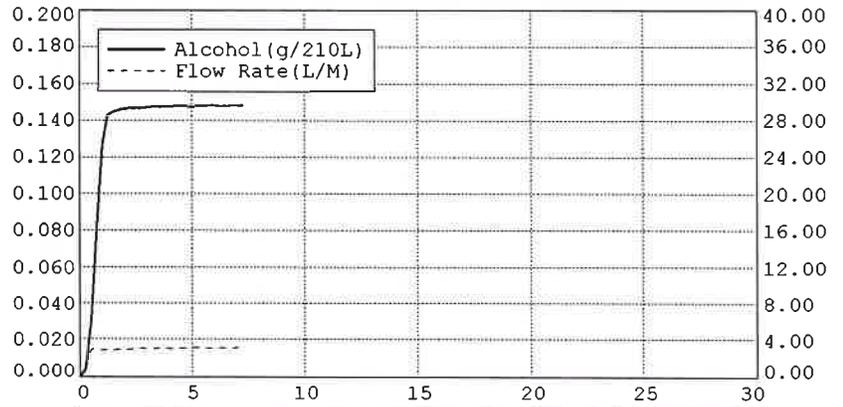

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
 DATAMASTER dmt: 100345






Date: 02/19/2026
 Time: 08:42:30

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
 TARGET AT 29.88: 0.300
 LOT #: AG427706
 EXPIRATION: 10/03/2026
 TANK PRESSURE: 187 psi

| | | |
|-------------------|----------|-------|
| BLANK TEST | 0.000 | 08:43 |
| INTERNAL STANDARD | VERIFIED | 08:43 |
| EXTERNAL STANDARD | 0.301 | 08:44 |
| BLANK TEST | 0.000 | 08:45 |
| EXTERNAL STANDARD | 0.300 | 08:45 |
| BLANK TEST | 0.000 | 08:46 |
| EXTERNAL STANDARD | 0.300 | 08:46 |
| BLANK TEST | 0.000 | 08:47 |
| EXTERNAL STANDARD | 0.300 | 08:47 |
| BLANK TEST | 0.000 | 08:48 |
| EXTERNAL STANDARD | 0.301 | 08:48 |
| BLANK TEST | 0.000 | 08:49 |

Average = 0.3004
 Std Dev = 0.0005

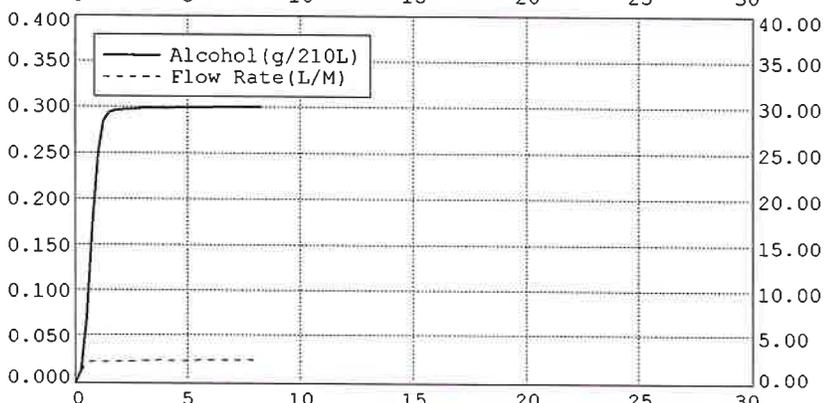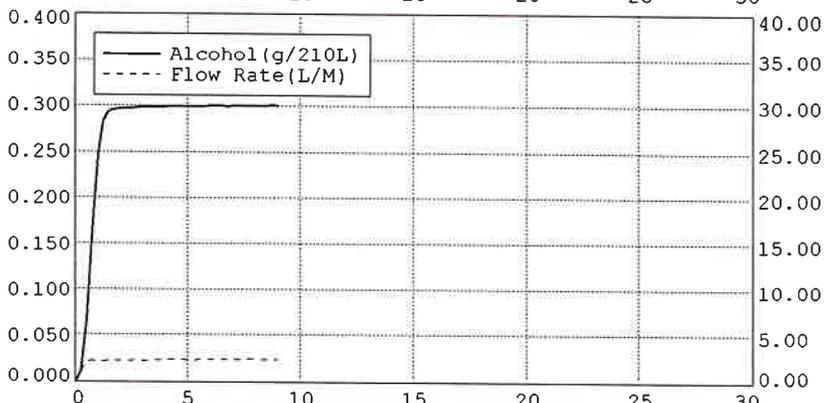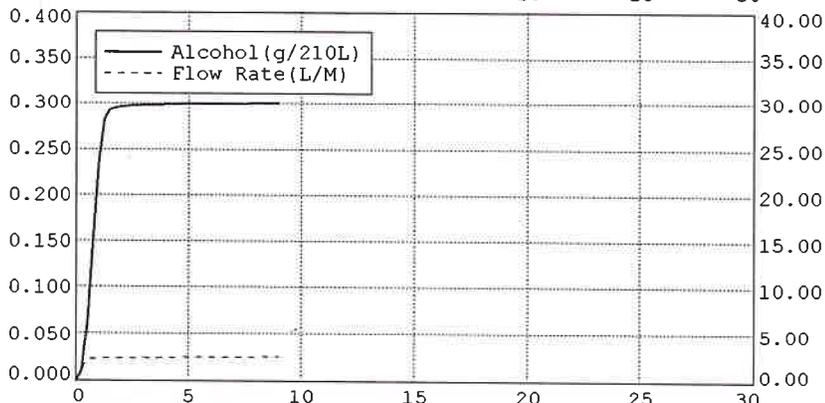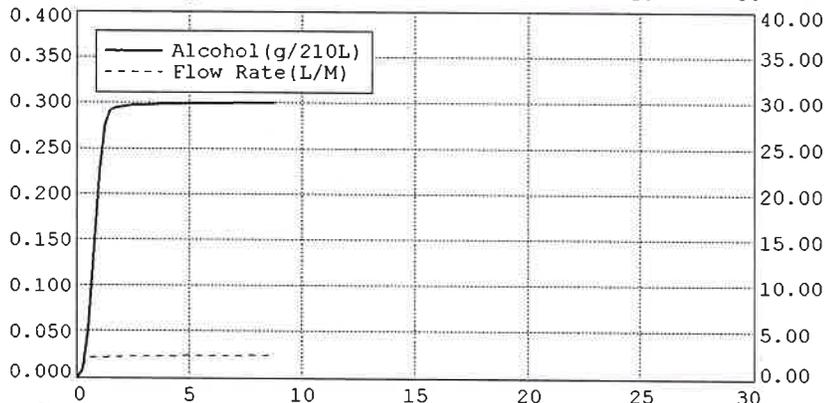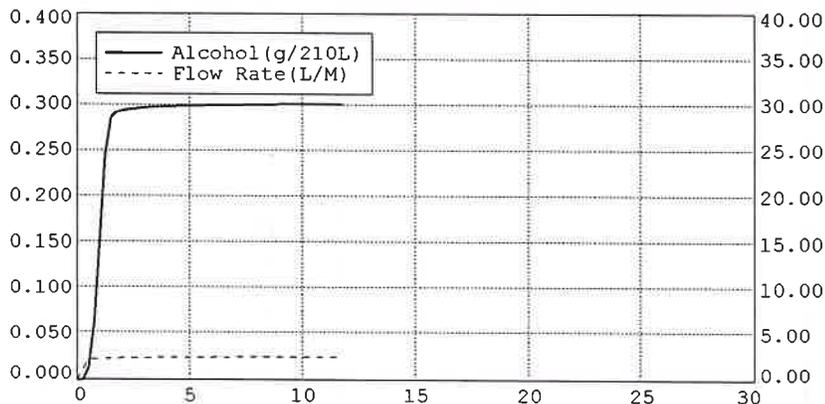

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 09:32:58


SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.86: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 09:57
BLANK TEST 0.000 09:57
INTERNAL STANDARD VERIFIED 09:57
EXTERNAL STANDARD 0.080 09:57
BLANK TEST 0.000 09:58
SUBJECT SAMPLE INCOMPLETE 10:00

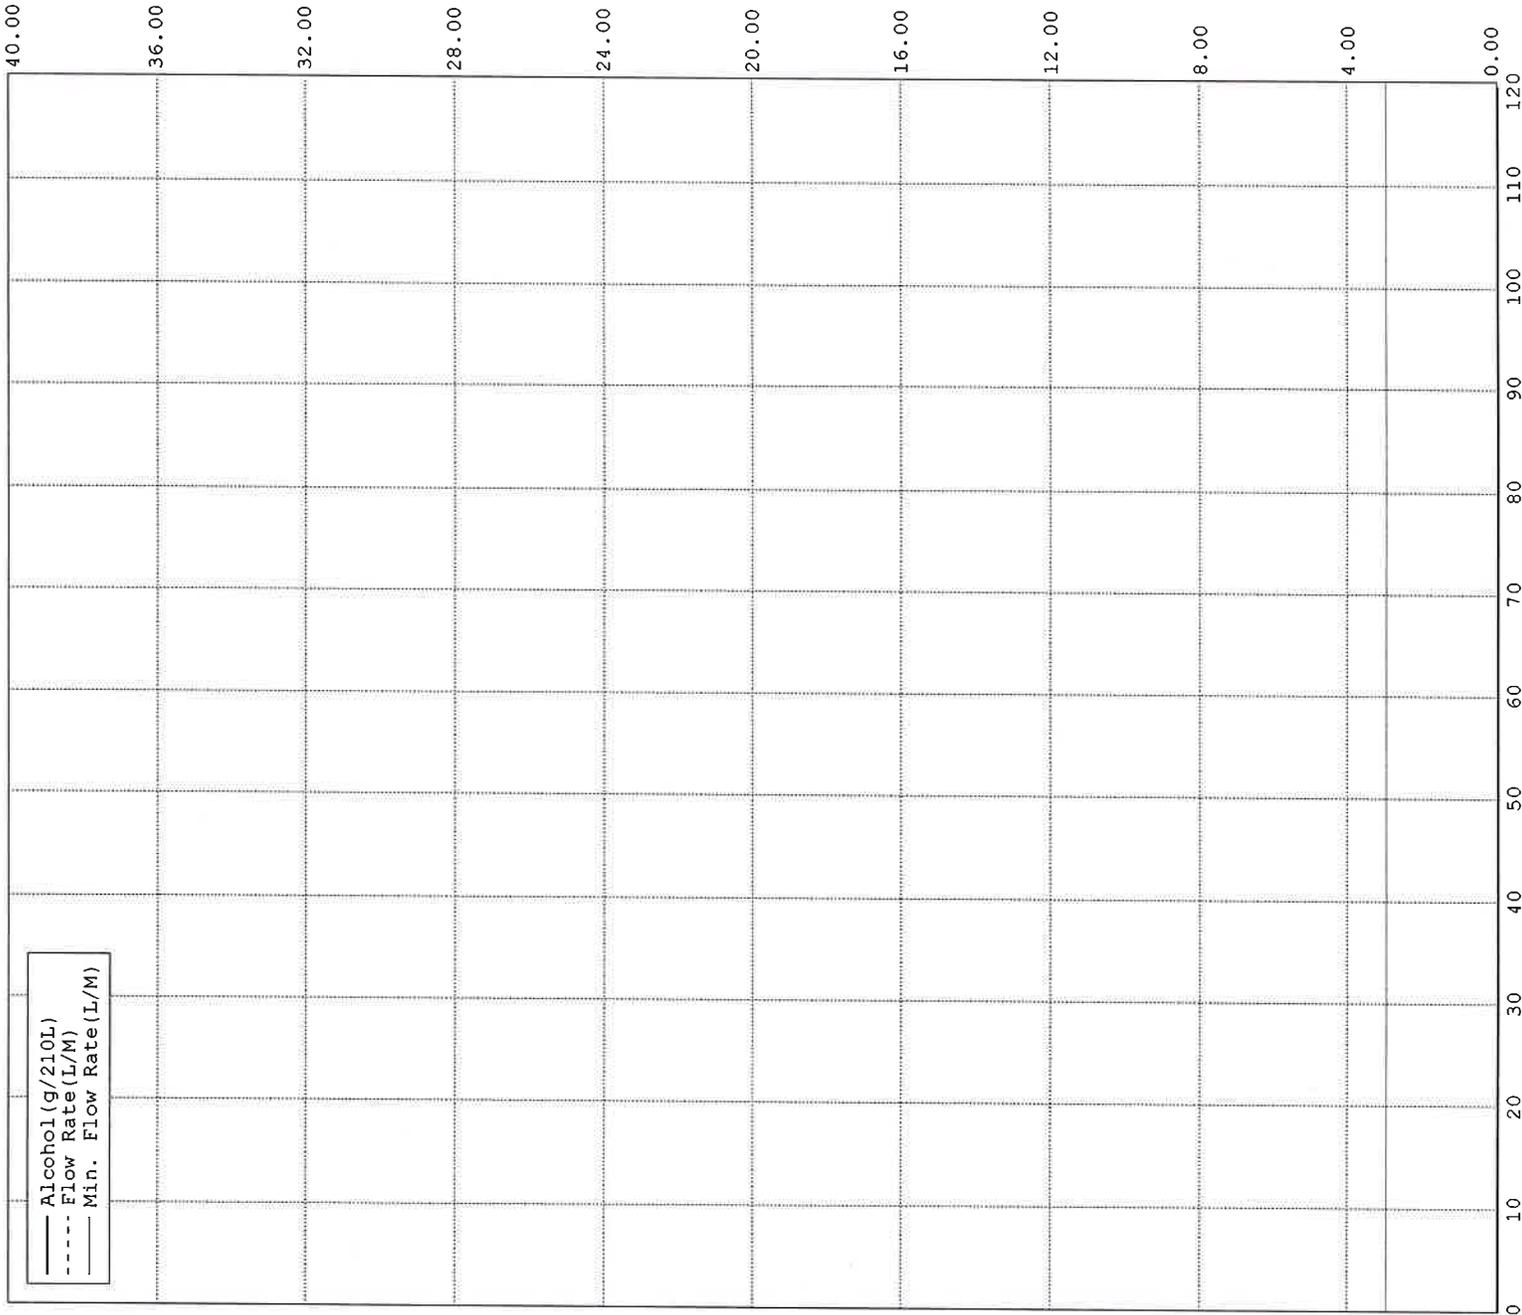

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 11:16:11

SUBJECT NAME:
TEST TEST
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

| | | |
|-------------------|----------|-------|
| DIAGNOSTIC CHECK | PASSED | 11:23 |
| BLANK TEST | 0.000 | 11:23 |
| INTERNAL STANDARD | VERIFIED | 11:23 |
| EXTERNAL STANDARD | 0.080 | 11:23 |
| BLANK TEST | 0.000 | 11:24 |
| SUBJECT SAMPLE | XXX | 11:25 |

Maximum Attempts Exceeded

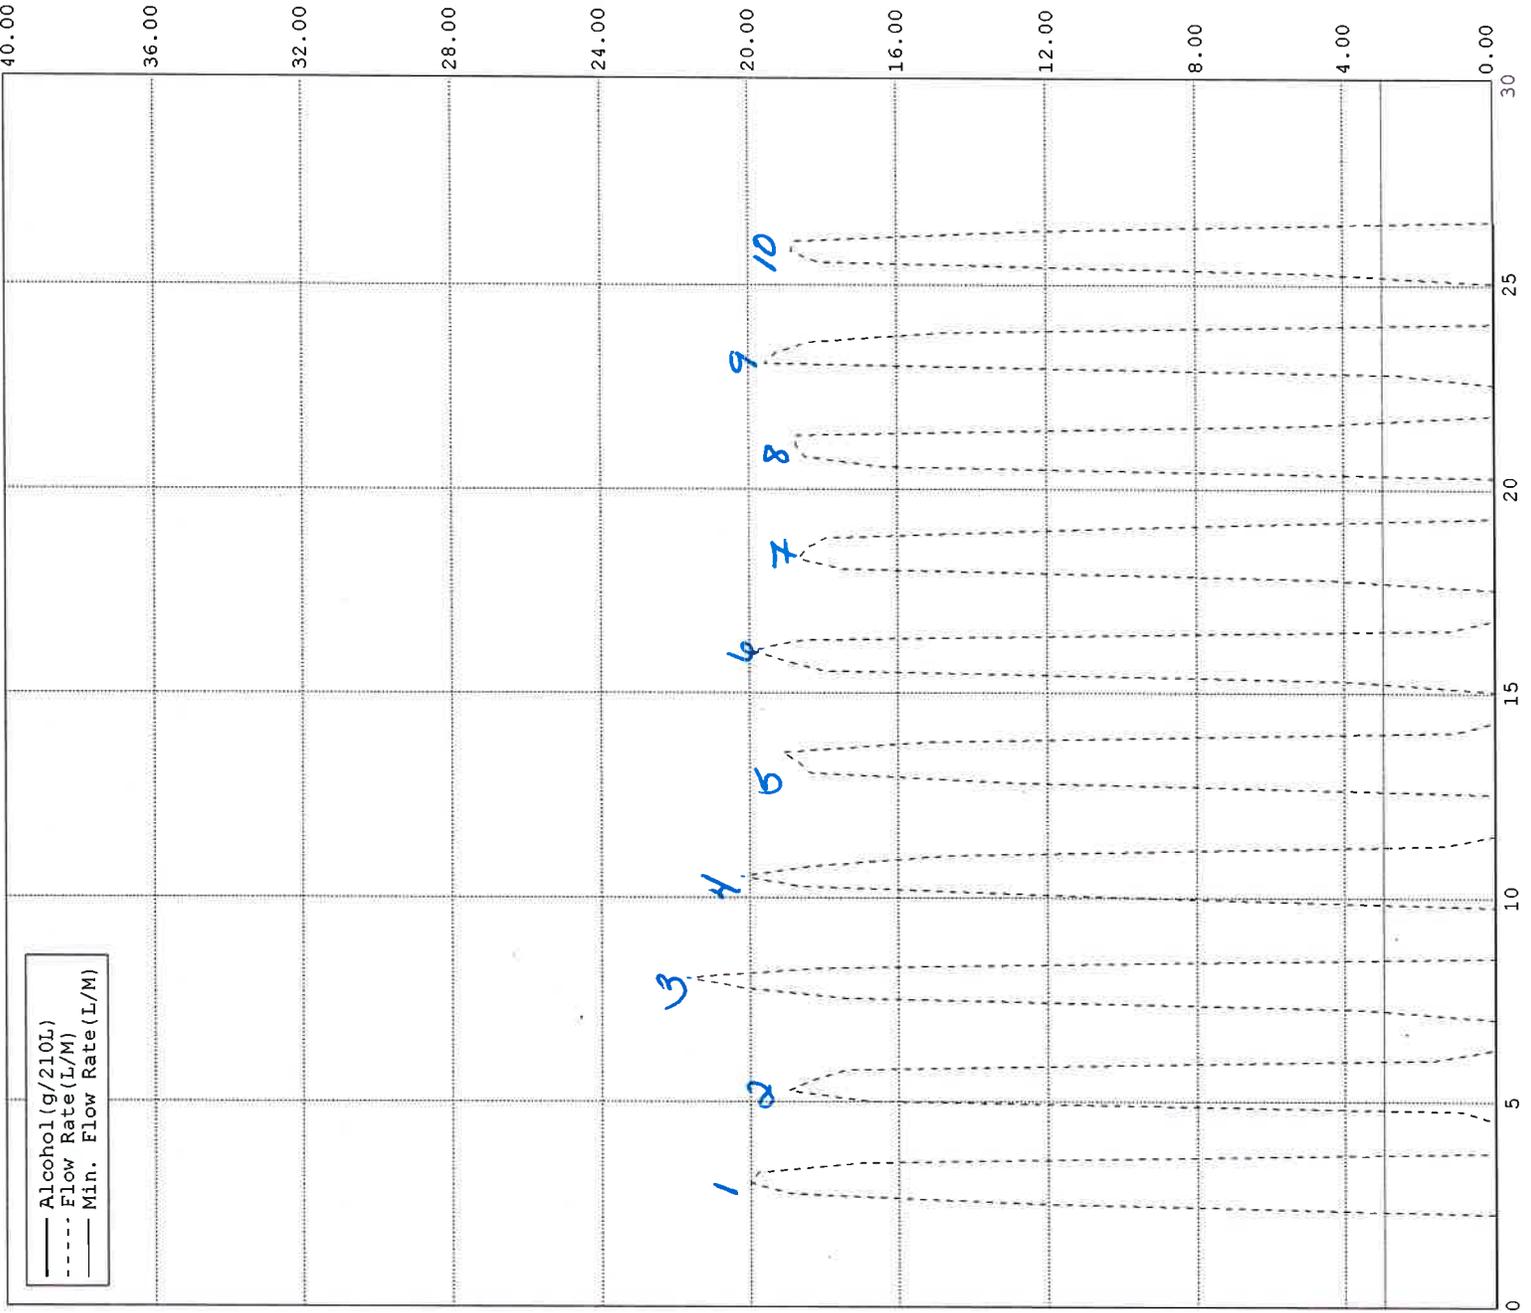

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 11:07:43


SUBJECT NAME:
TEST TEST
LICENSE #: INVALID

OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK
BLANK TEST PASSED 11:10
INTERNAL STANDARD VERIFIED 11:10
EXTERNAL STANDARD 0.080 11:10
BLANK TEST 0.000 11:11
SUBJECT SAMPLE INVALID 11:12

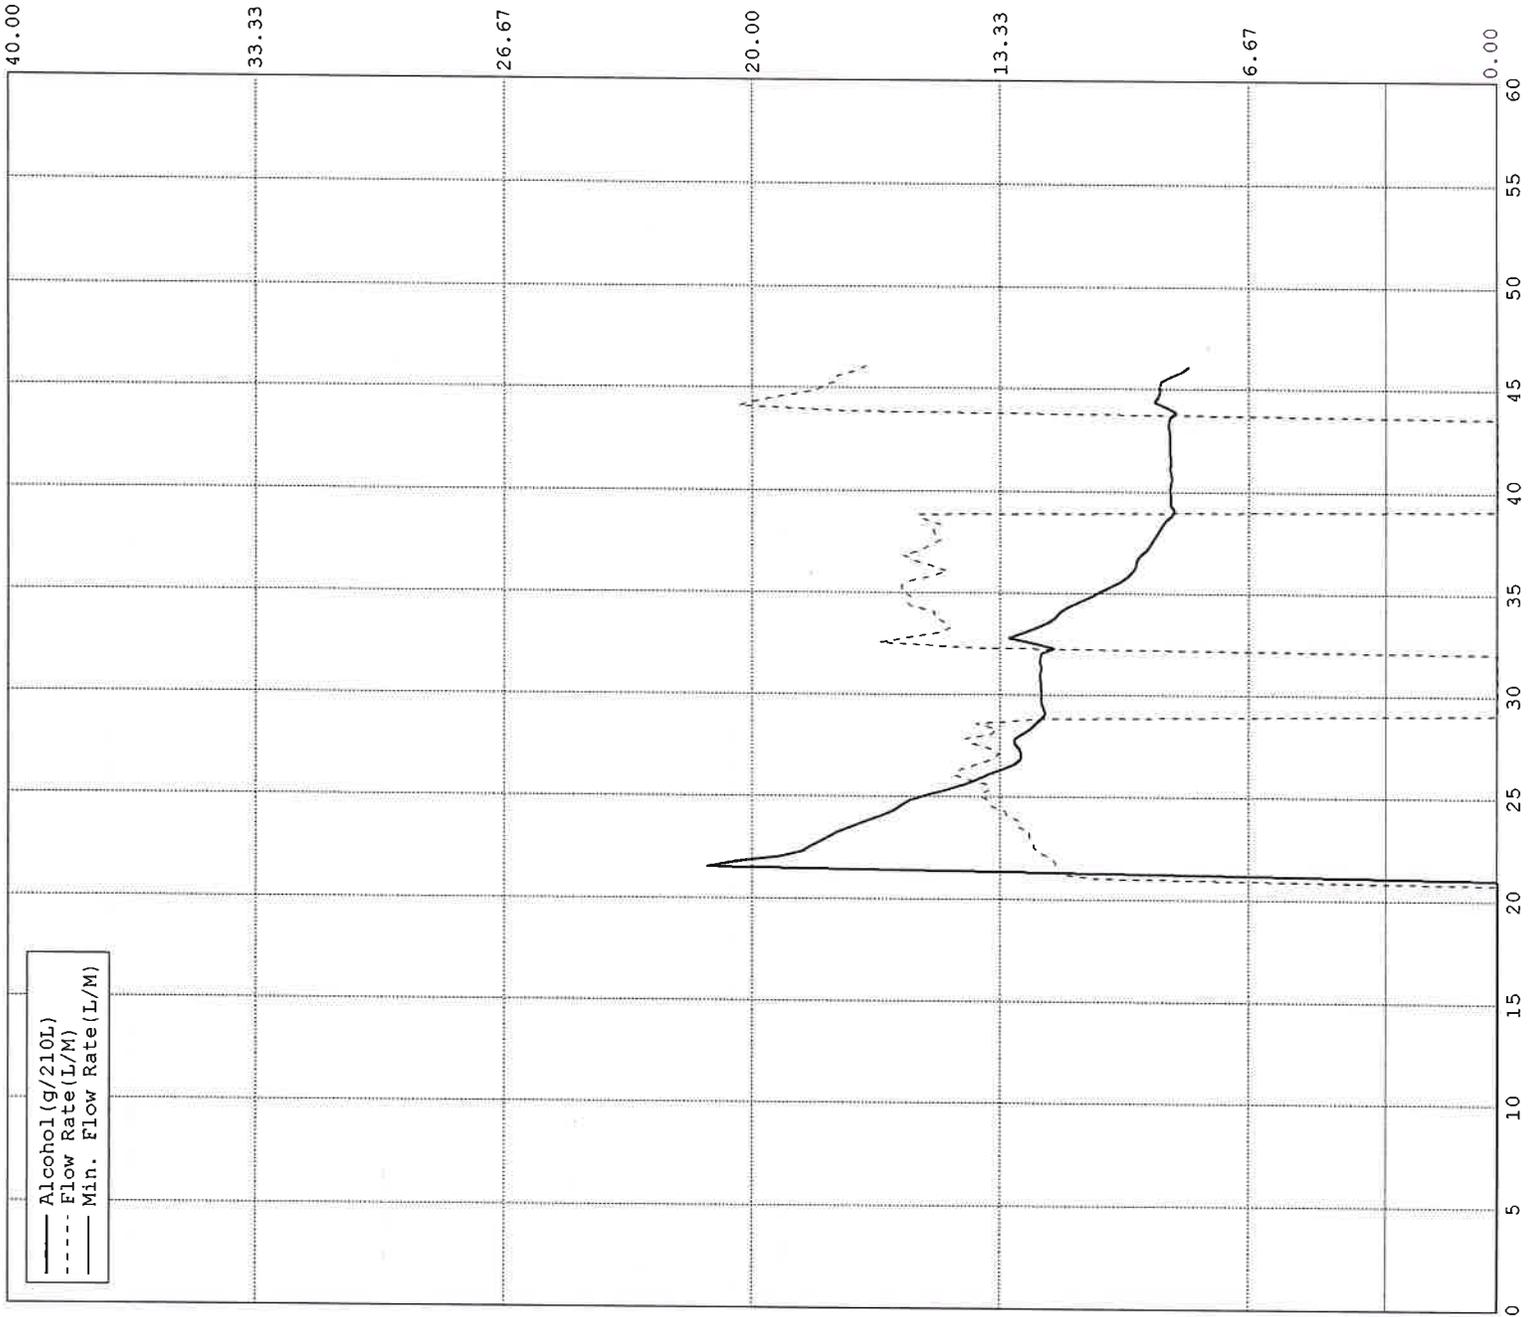

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 11:01:19

SUBJECT NAME:
TEST TEST
LICENSE #: RFI

OPERATOR NAME:
COLLEEN S OBRVANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1


CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.84: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 11:03
BLANK TEST 0.000 11:03
INTERNAL STANDARD VERIFIED 11:03
EXTERNAL STANDARD 0.079 11:03
BLANK TEST 0.000 11:04

RFI DETECTED

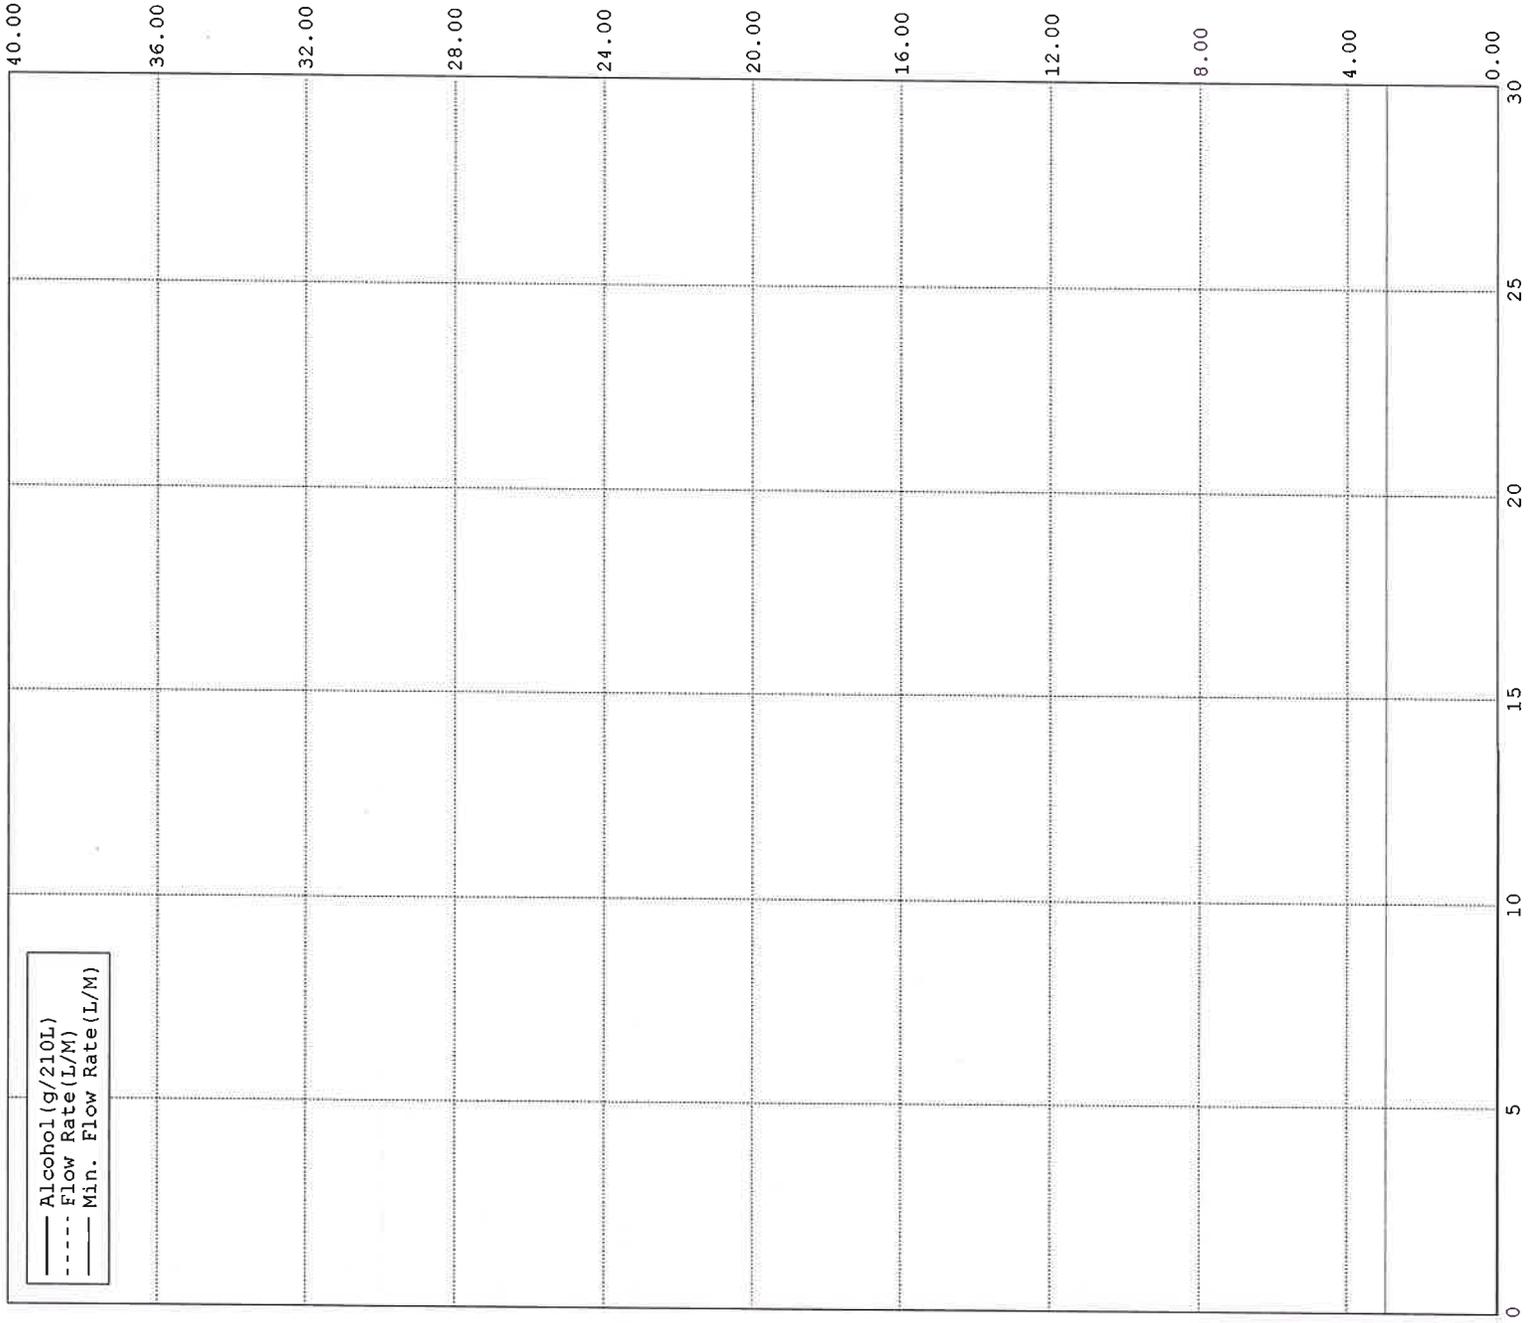

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 09:01:04

SUBJECT NAME:
TEST TEST
LICENSE #: INT-ACETONE

OPERATOR NAME:
COLLEEN S OBRVANT
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.87: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 09:02
BLANK TEST 0.000 09:02
INTERNAL STANDARD VERIFIED 09:02
Xq = 0.090 (0.10%) 0.080 09:02
EXTERNAL STANDARD 0.080 09:02
X[1] = 0.0804 (-0.0010) (0.0016)
BLANK TEST 0.000 09:03
SUBJECT SAMPLE XXX 09:04
X[1] = 0.1112 (-0.0171) (0.0022)

Interference Detected

Filter 2 Avg = -0.0016
Filter 3 Avg = 0.0015

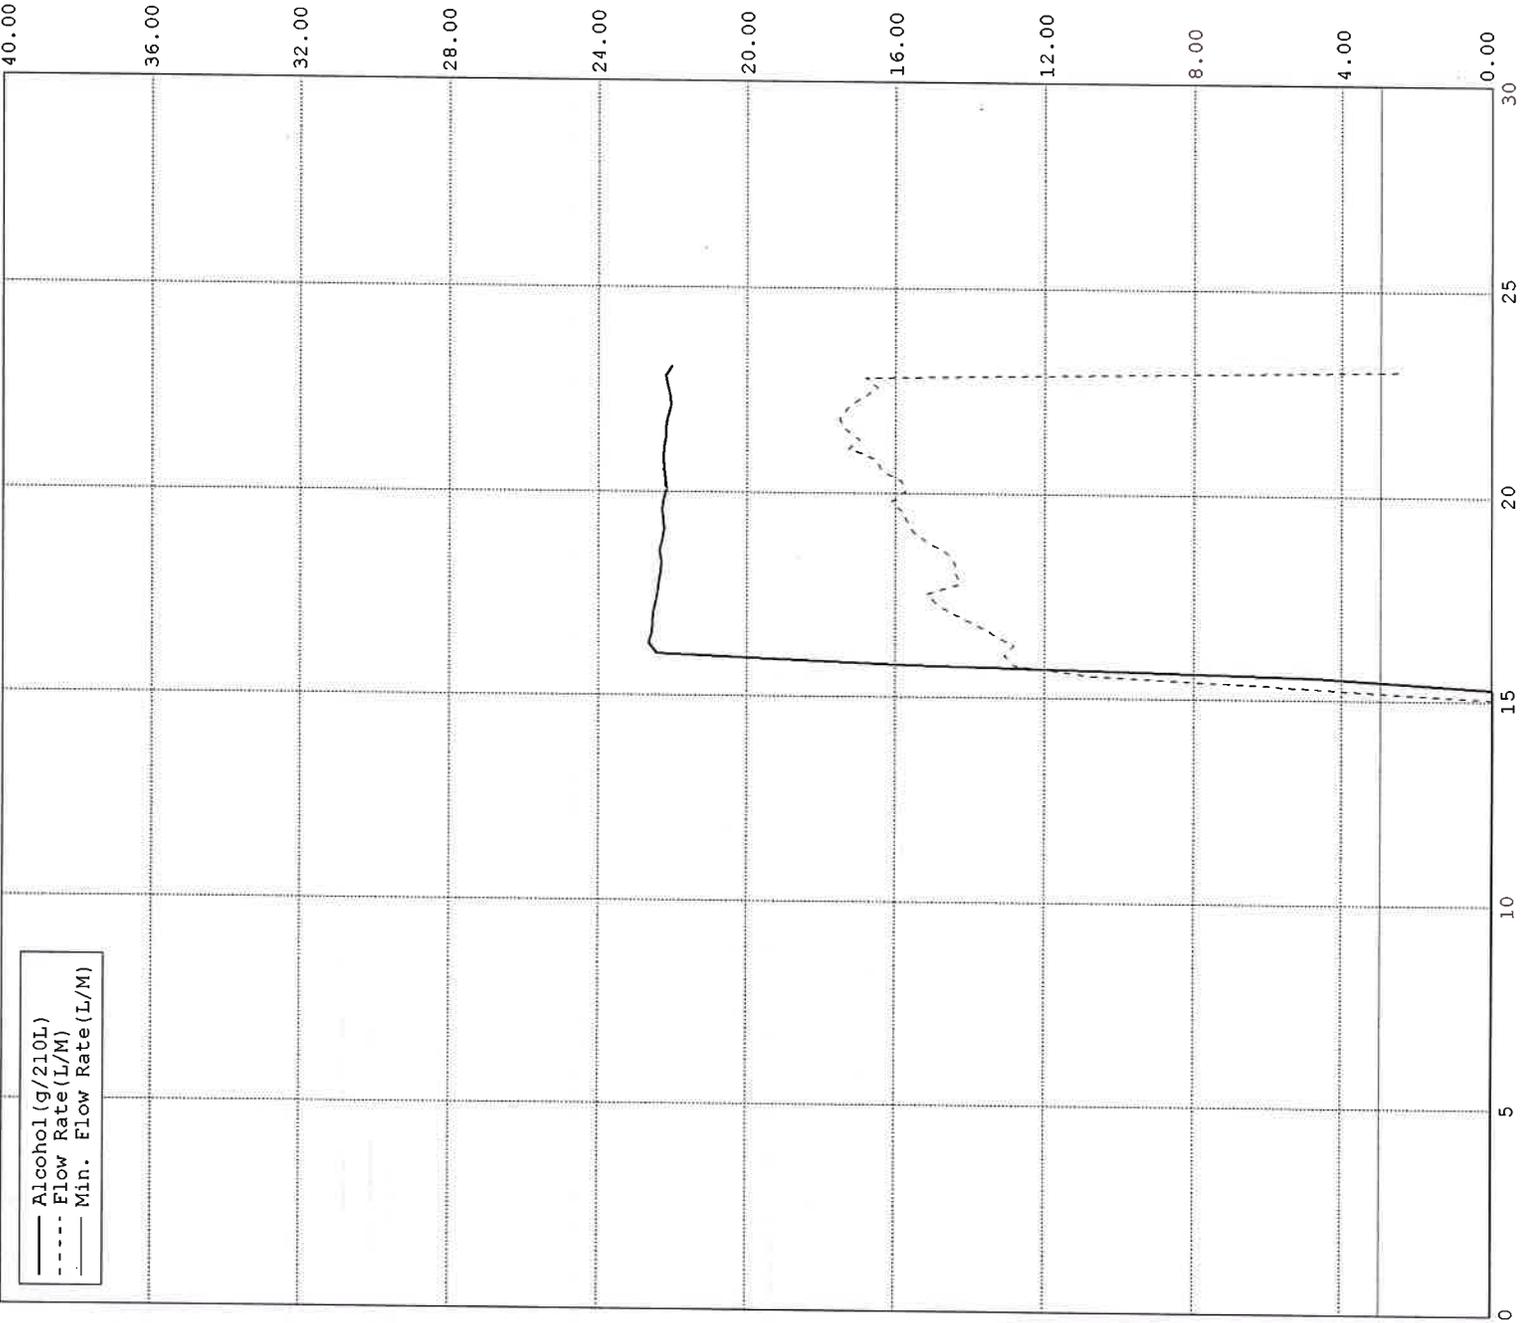

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 09:14:03

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA


OPERATOR NAME:
COLLEEN S OBRyant
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.87: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 09:15
BLANK TEST 0.000 09:15
INTERNAL STANDARD VERIFIED 09:15
Xq = 0.090 (0.10%) 0.080 09:16
EXTERNAL STANDARD X[1] = 0.0802 (-0.0018) (0.0012)
BLANK TEST 0.000 09:17
SUBJECT SAMPLE XXX 09:17
X[1] = 0.1167 (-0.0248) (-0.0001)

Interference Detected

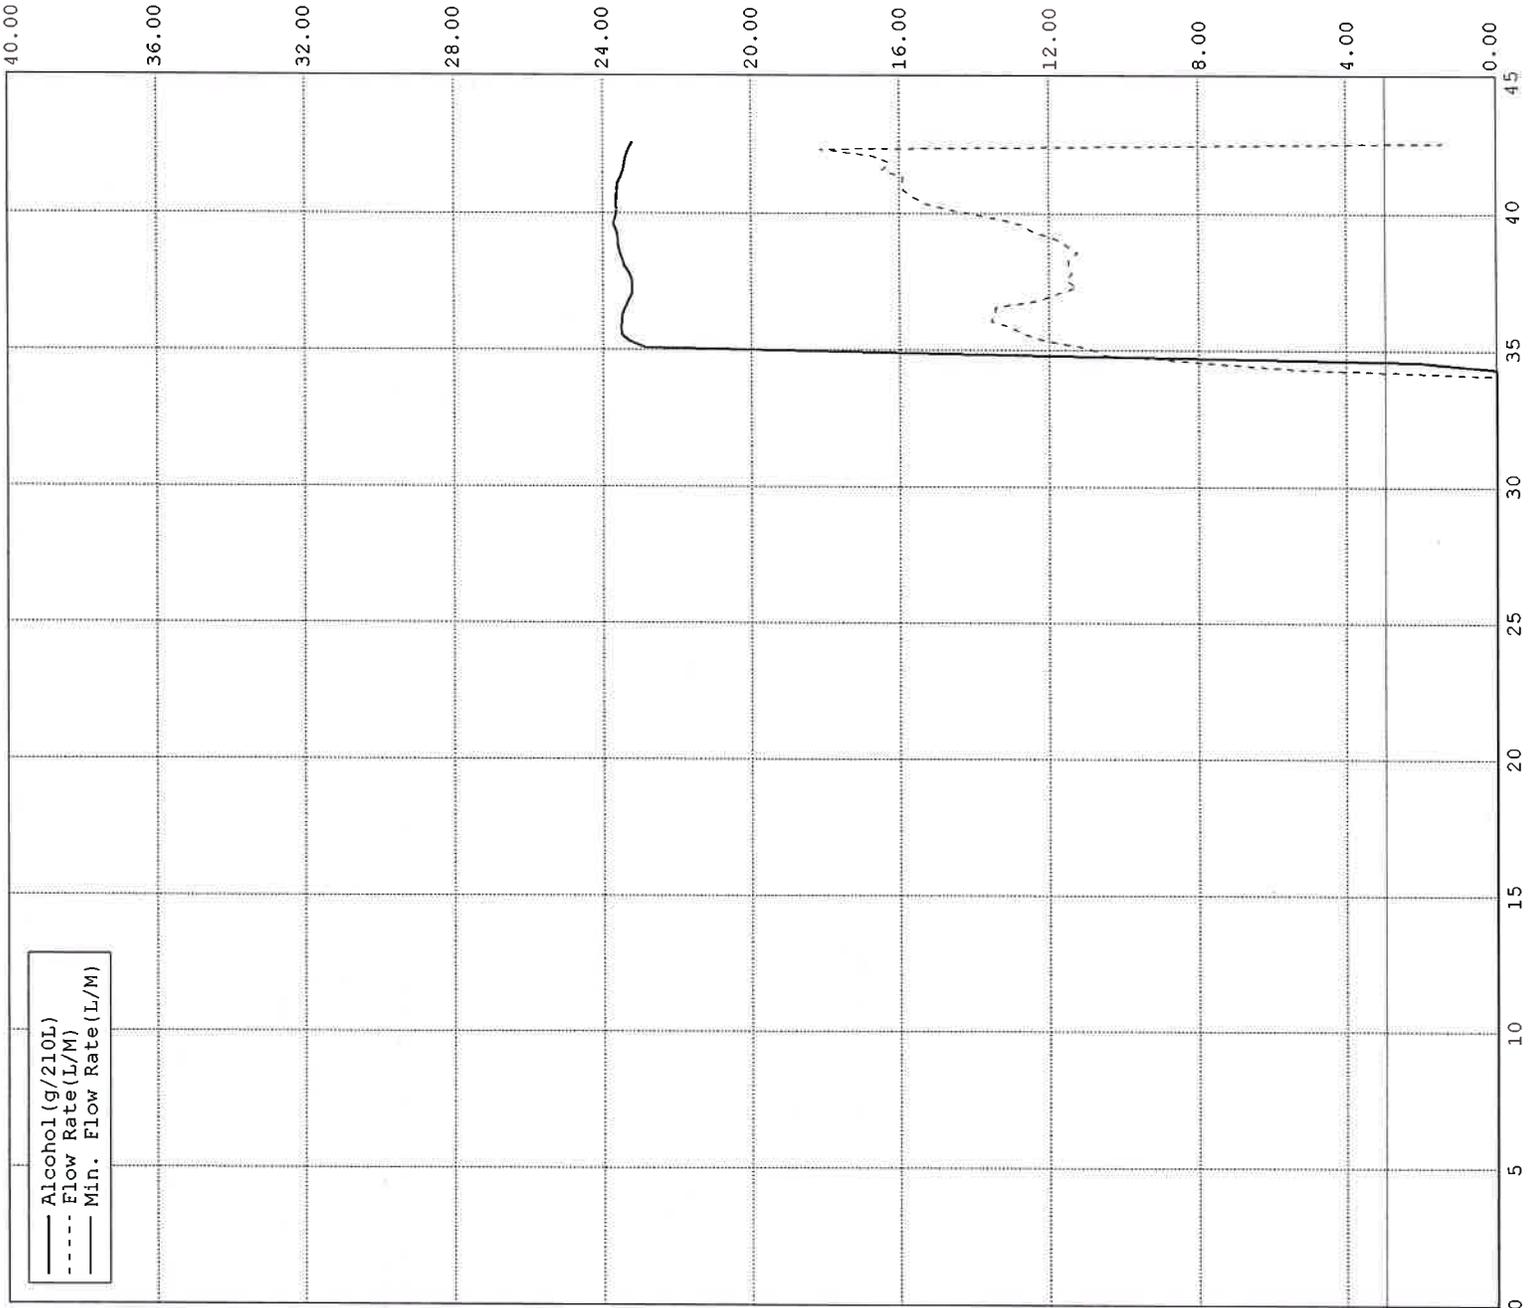

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100345

Date: 02/19/2026
Time: 09:23:01

SUBJECT NAME:
TEST TEST
LICENSE #: INT-NEGATIVE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1

CASE/REPORT: 26-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.87: 0.080
LOT #: AG436502
EXPIRATION: 12/30/2026

| | | |
|----------------------------|----------|-------|
| DIAGNOSTIC CHECK | PASSED | 09:24 |
| BLANK TEST | 0.000 | 09:24 |
| INTERNAL STANDARD | VERIFIED | 09:24 |
| EXTERNAL STANDARD | 0.080 | 09:24 |
| Xg = 0.090 (0.29%) | | |
| X[1] = 0.0800 (-0.0024) | (0.0015) | |
| BLANK TEST | 0.000 | 09:25 |
| SUBJECT SAMPLE (Vol=1.85L) | 0.094 | 09:25 |
| X[1] = 0.0949 (0.0000) | (0.0003) | |
| BLANK TEST | 0.000 | 09:26 |
| EXTERNAL STANDARD | 0.080 | 09:27 |
| X[1] = 0.0797 (-0.0012) | (0.0015) | |
| BLANK TEST | 0.000 | 09:27 |

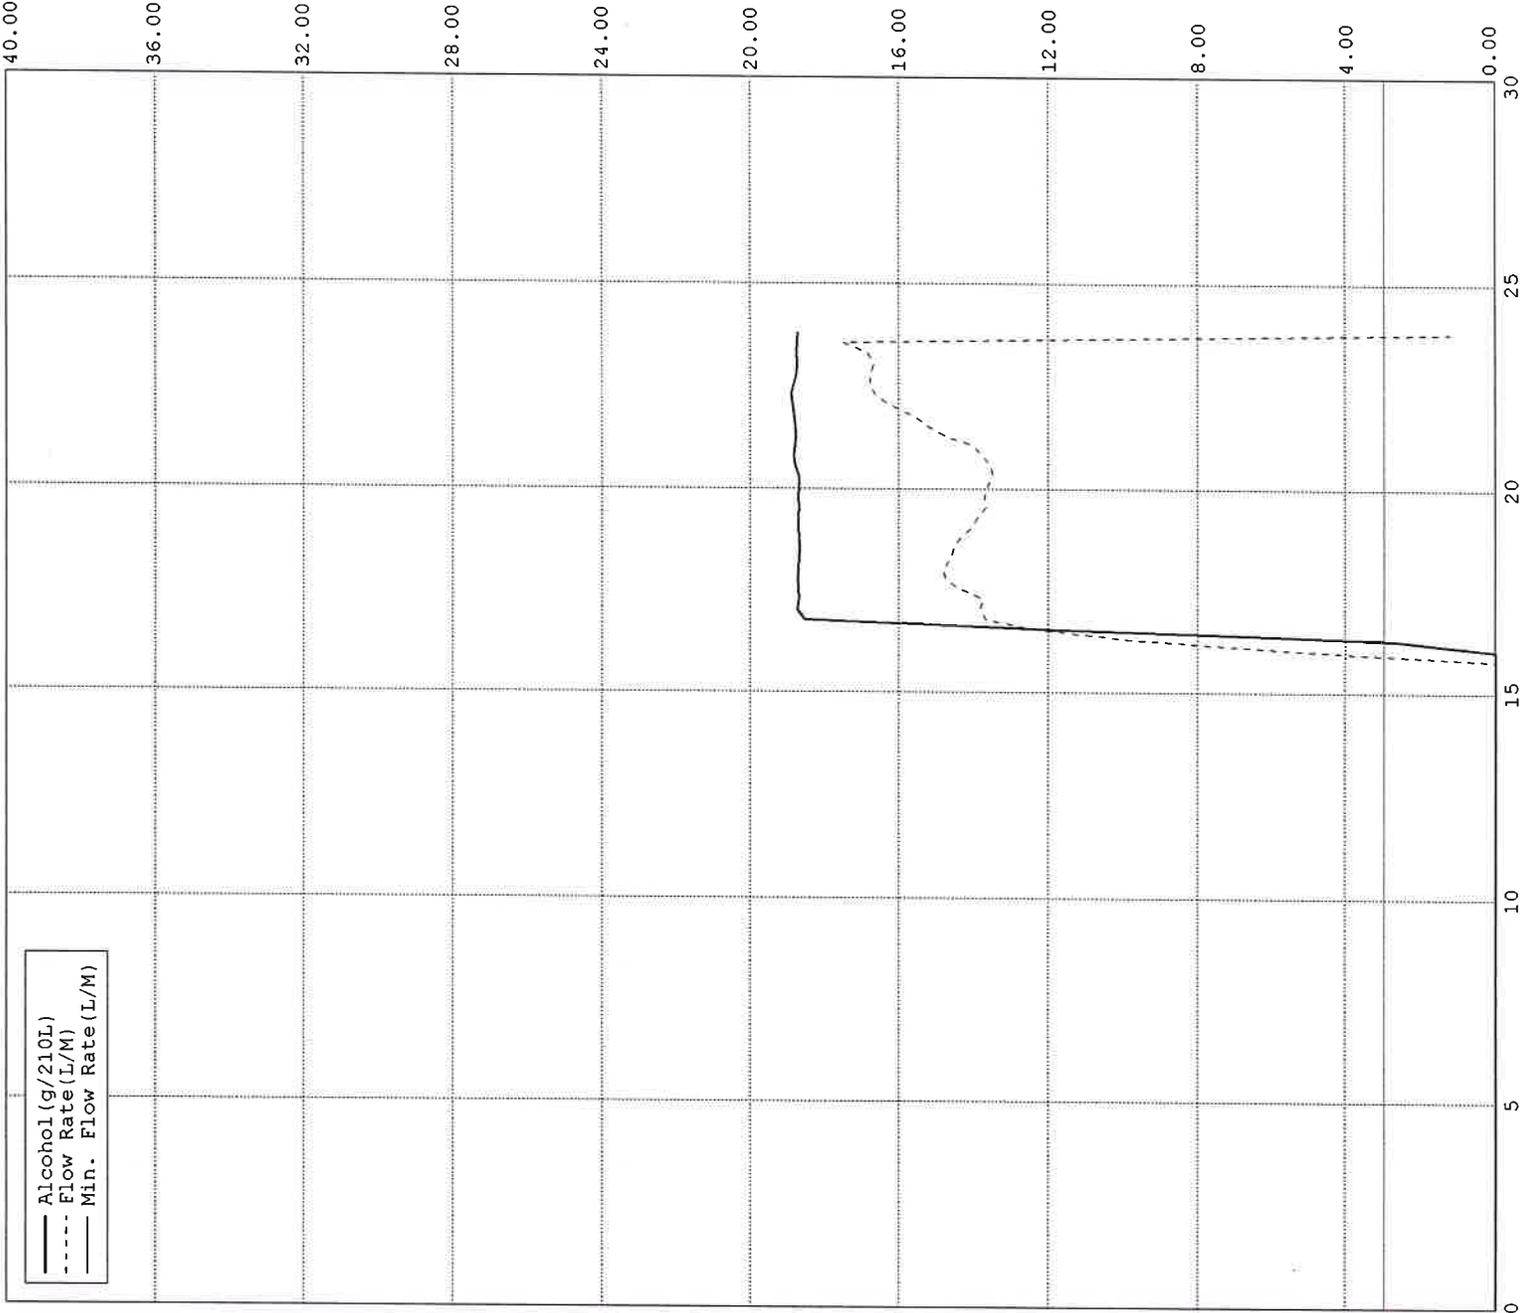

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100345

Date: 02/19/2026
 Time: 11:47:07

SUBJECT NAME:
 TEST TEST
 LICENSE #: NDST
 OPERATOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 26-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.83: 0.080
 LOT #: AG436502
 EXPIRATION: 12/30/2026

| | | |
|----------------------------|----------|-------|
| DIAGNOSTIC CHECK | PASSED | 11:49 |
| BLANK TEST | 0.000 | 11:49 |
| INTERNAL STANDARD | VERIFIED | 11:49 |
| EXTERNAL STANDARD | 0.080 | 11:49 |
| BLANK TEST | 0.000 | 11:50 |
| SUBJECT SAMPLE (Vol=1.88L) | 0.000 | 11:50 |
| BLANK TEST | 0.000 | 11:51 |
| EXTERNAL STANDARD | 0.080 | 11:52 |
| BLANK TEST | 0.000 | 11:52 |

CAS

