



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory
4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100352

Report Issue Date: Not Released
Date Received: 2025-02-19
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.078	AG335202	0.079	0.079	0.079	0.079	0.079	0.079
0.300	0.293	AG427706	0.297	0.297	0.297	0.296	0.296	0.297

As Found - Evaluation Analyst: Kaija Swisher
As Found Conditions - Barometric Pressure (inHg): 29.25 Barometer Used: VWR S/N 240680771 Temperature (C): 22.0 Relative Humidity (%): 14
As-Found Lab Activity Date Range: 02/19/2025 - 02/19/2025

Replaced breath tube holder and O-Ring. First VOC failed due to interference detected. Touch screen seems to be working as normal.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.021	0.020	0.020	0.021	0.021	+/- 0.002
0.040	0.040	AG407908	0.040	0.040	0.040	0.041	0.040	0.040	+/- 0.003
0.080	0.079	AG335202	0.080	0.080	0.080	0.080	0.080	0.080	+/- 0.004
0.100	0.099	AG333401	0.101	0.101	0.101	0.101	0.101	0.101	+/- 0.004
0.150	0.148	AG332004	0.149	0.149	0.149	0.149	0.149	0.149	+/- 0.006
0.300	0.297	AG427706	0.301	0.300	0.301	0.300	0.300	0.300	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.61 Barometer Used: VWR S/N 240680771 Temperature (C): 22.7 Relative Humidity (%): 12
As-Left Lab Activity Date Range: 03/27/2025 - 03/27/2025

Suck back error occurred on the RFI functional test. It was rerun and the correct status message occurred.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Serial Number: 100352

Results authorized by Megan Carlock on 03/27/2025

megan.crouse@alaska.gov

Not Tech/Admin Reviewed

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100352 Analyst or Technician Name: Megan Carlock

DataMaster DMT Calibration Start Date: 3/27/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.61 Temperature(C) 22.7 Relative Humidity(%) 12

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - Print with View Details
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

Suck back error occurred on RFI test, reran and received the correct status message. NWC 3/27/25

1. Acetone Reagent Lot Number: 20250219KS Expiration Date: 5/19/25
Simulator S/N: SD1177 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250219KS Expiration Date: 5/19/25
Simulator S/N: SD1198 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 23IP41233 Expiration Date: 9/20/25
Simulator S/N: SD1199 Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 3/27/25

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 3/27/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 09:35:56

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.0°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 48.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.80 V	PASSED
(1.09 V - 2.55 V)	
Cooler Voltage = 1.72 V	PASSED
(1.08 V - 2.52 V)	
Bias Voltage = 80 V	PASSED
(48 V - 112 V)	
Chopper Freq = 521 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.6 in	

PUMP INFO

Flow Rate = 5.051 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.001 V <= 0.010 V)	
PUMP OFF	PASSED
(0.001 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.087 1.84%	PASSED
(0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100352

Date: 03/27/2025

Time: 9:43 AM

Temperatures (°C)

Sample Cell: 49.4°C

Breath Tube: 48.0°C

Current Barometer 29.6 in

Volume (Ltr) 1.49

Settings

Lamp: 1.85 V

Bias: 80 V

Cooler: 1.60 V

Chopper: 520 Hz

Voltages (V)

Flow: 1.04 V

Detector: -0.012 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 05/24/2021
Time: 06:23:14

OPERATOR NAME:
ST LOUIS INTOX A TECH
CERTIFICATE #: OU812

Ca = 0.1000
CAL = 0.989611 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0054 0.0010 <= b2 < 0.0100
b3 = 0.0007 0.0000 <= b3 < 0.0040
Xq = 0.0854 0.0500 <= Xq < 0.2000
a21 = 1.140227 1.050 <= a21 < 1.300
a31 = 0.456264 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 09:45:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.60: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	09:46
BLANK TEST	0.000	09:46
INTERNAL STANDARD	VERIFIED	09:46
EXTERNAL STANDARD	0.080	09:47
BLANK TEST	0.000	09:48
SUBJECT SAMPLE (Vol=1.59L)	0.000	09:48
BLANK TEST	0.000	09:49
EXTERNAL STANDARD	0.080	09:50
BLANK TEST	0.000	09:50

MNC

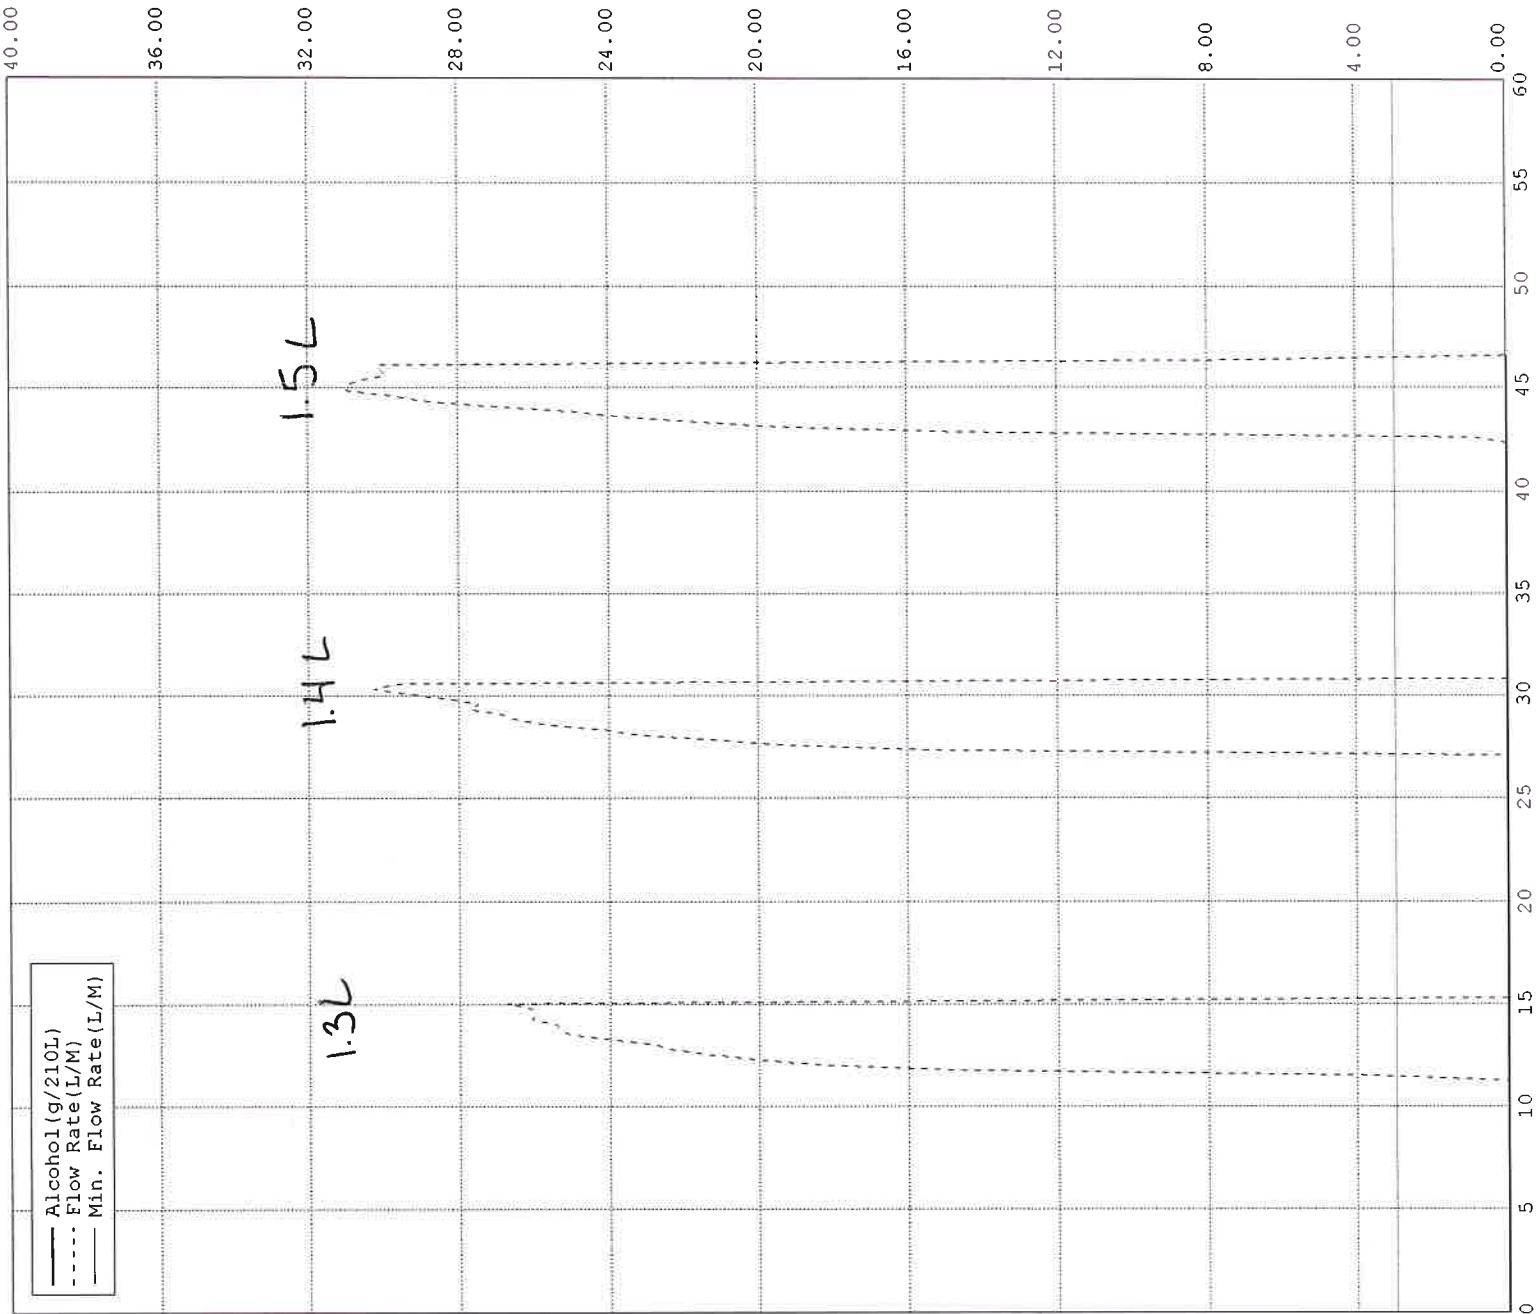

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100352

Date: 03/27/2025
 Time: 09:55:28

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0206	0.0005
0.040	0.0402	0.0004
0.079	0.0800	0.0000
0.099	0.1010	0.0000
0.148	0.1490	0.0000
0.297	0.3004	0.0005

SLOPE
 R^2
 = 1.010343
 = 0.999974

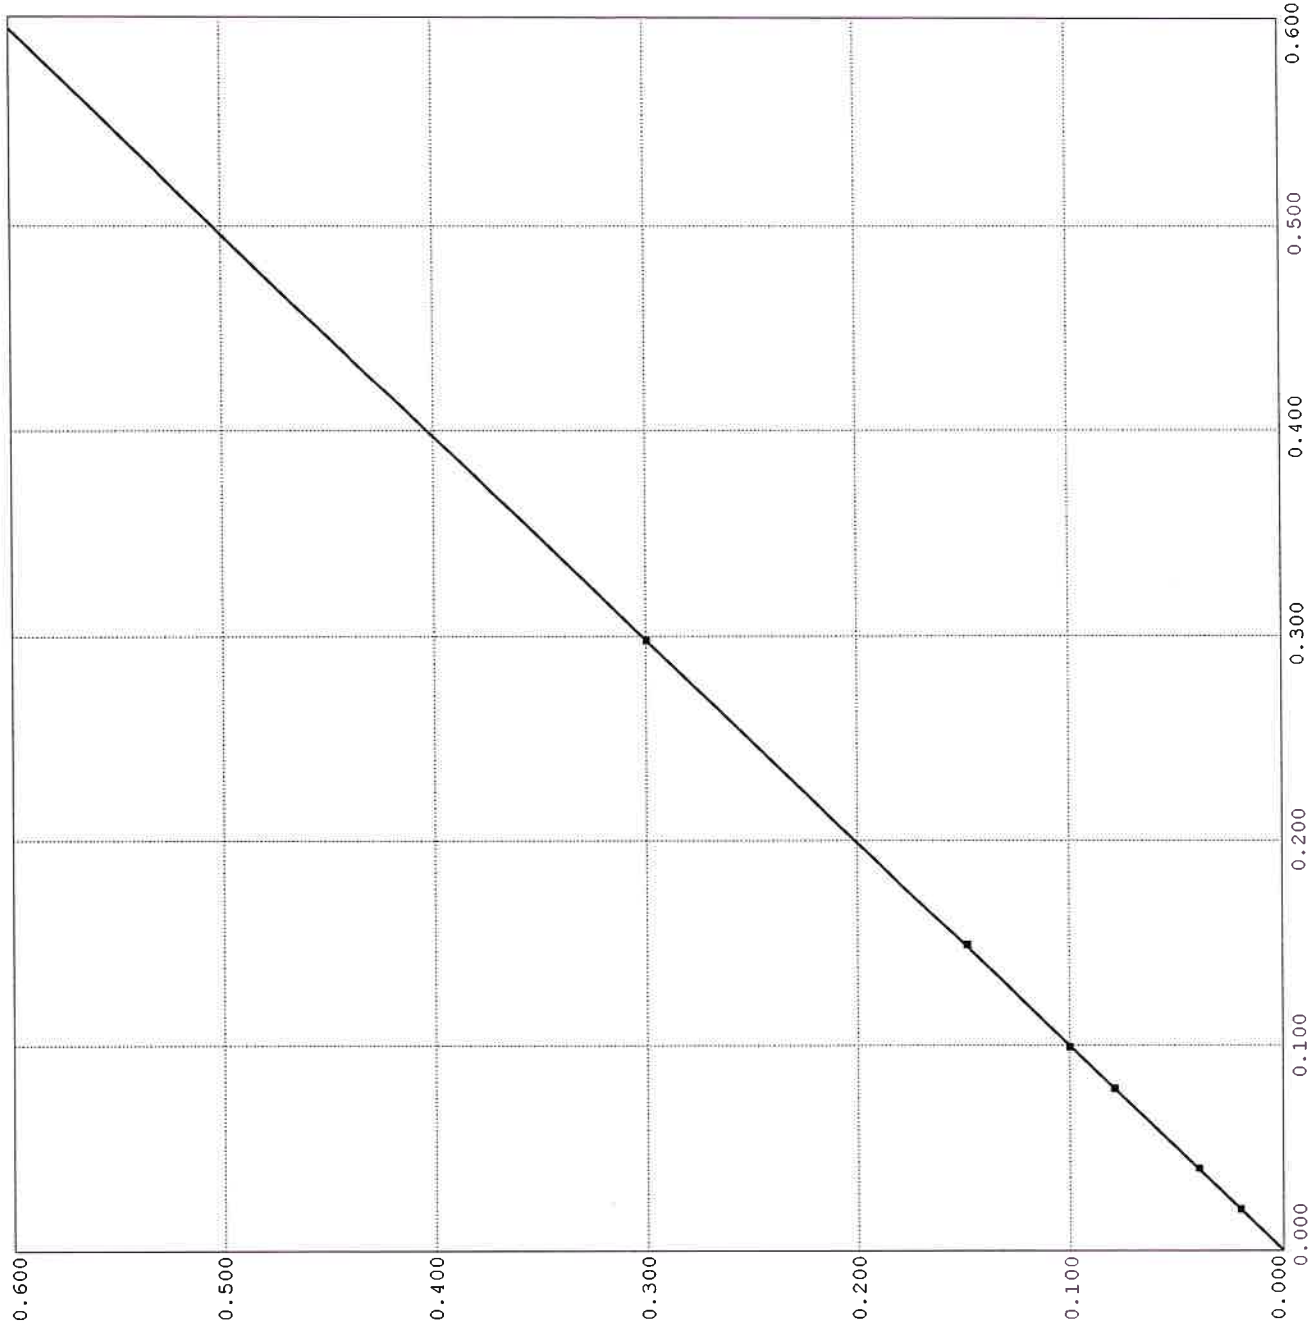

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100352






Date: 03/27/2025
Time: 09:55:30

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.61: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 389 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	09:56
INTERNAL STANDARD	VERIFIED	09:56
EXTERNAL STANDARD	0.021	09:56
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.021	09:58
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.020	09:59
BLANK TEST	0.000	10:00
EXTERNAL STANDARD	0.020	10:00
BLANK TEST	0.000	10:01
EXTERNAL STANDARD	0.021	10:01
BLANK TEST	0.000	10:02

Average = 0.0206
Std Dev = 0.0005

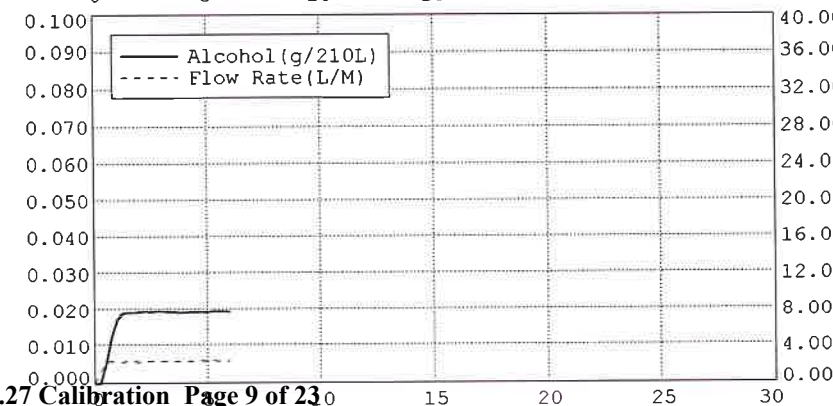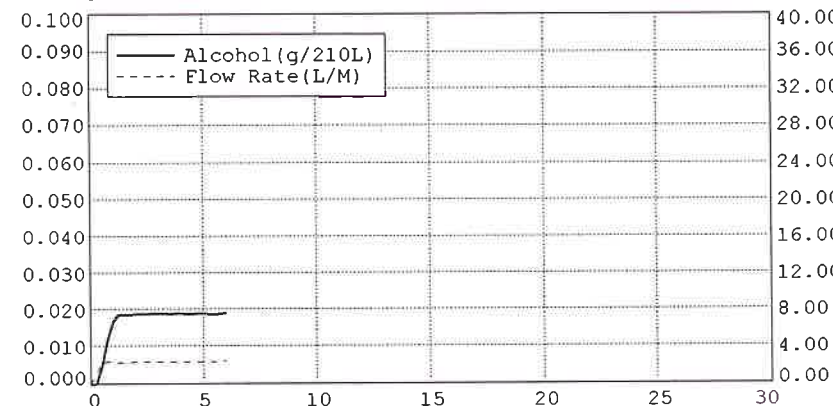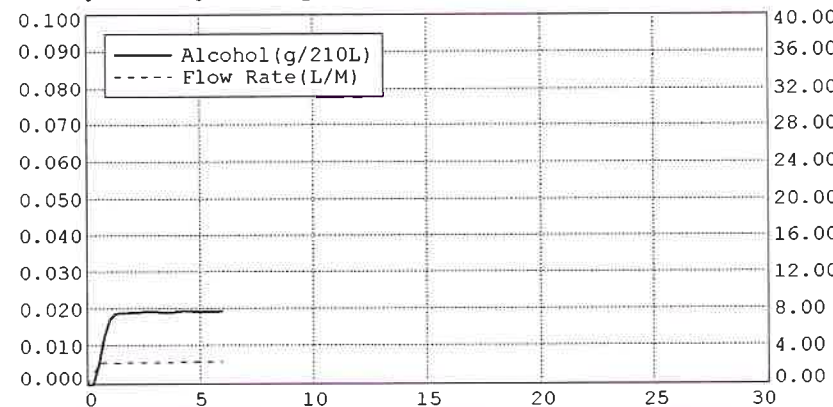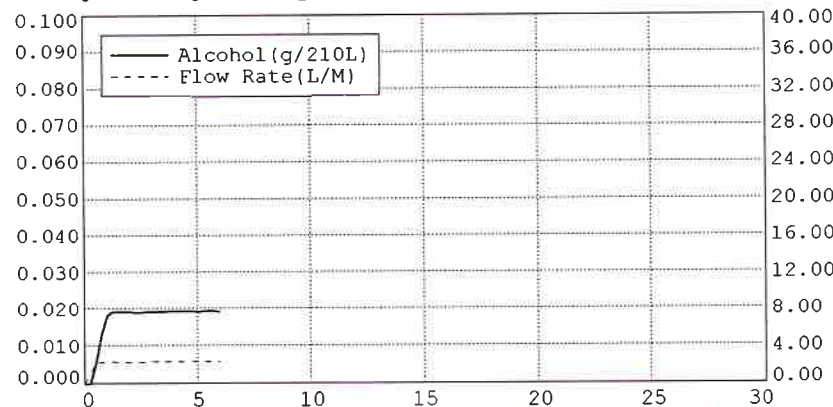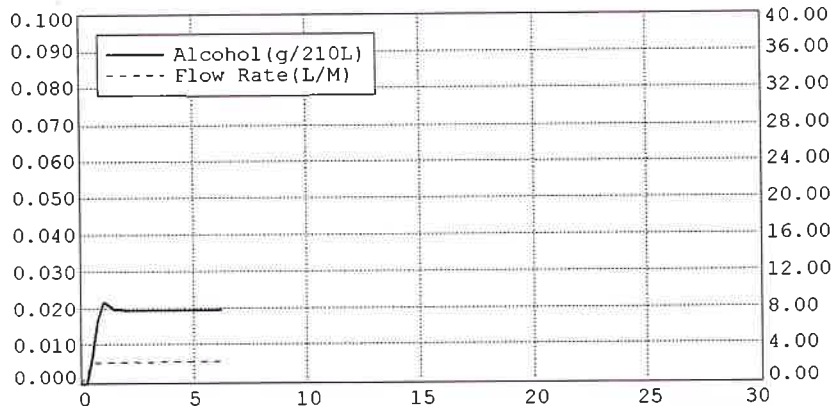

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100352






Date: 03/27/2025
Time: 10:03:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.61: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 866 psi

BLANK TEST	0.000	10:04
INTERNAL STANDARD	VERIFIED	10:04
EXTERNAL STANDARD	0.040	10:04
BLANK TEST	0.000	10:05
EXTERNAL STANDARD	0.040	10:05
BLANK TEST	0.000	10:06
EXTERNAL STANDARD	0.040	10:07
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.041	10:08
BLANK TEST	0.000	10:09
EXTERNAL STANDARD	0.040	10:09
BLANK TEST	0.000	10:10

Average = 0.0402
Std Dev = 0.0004

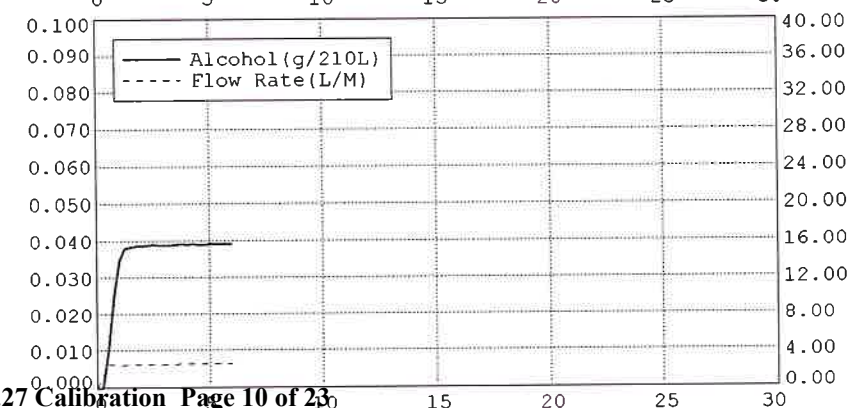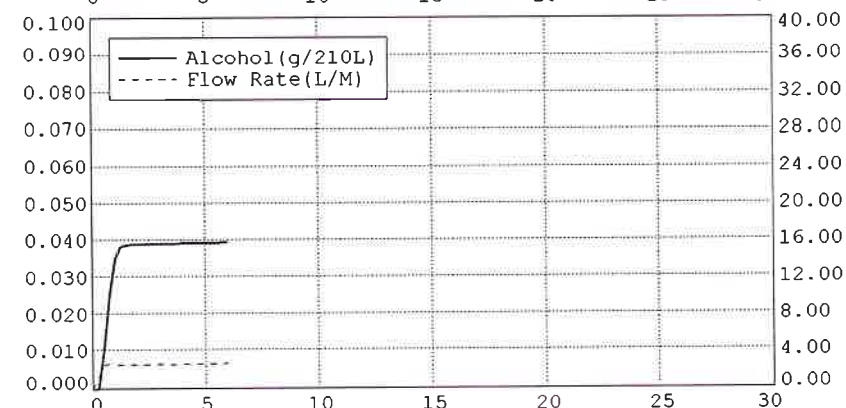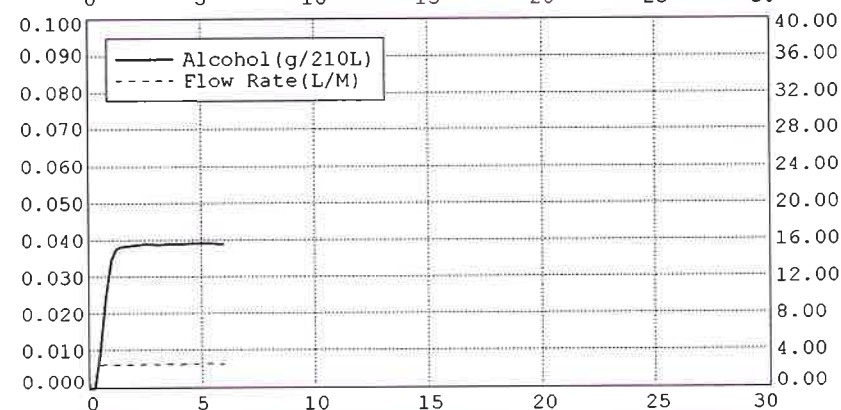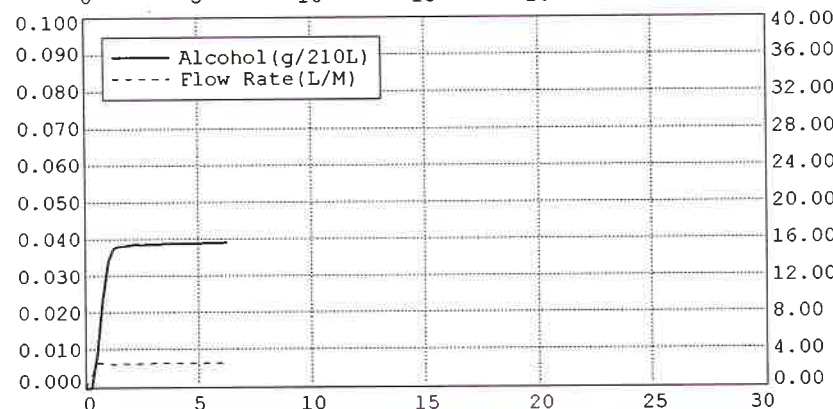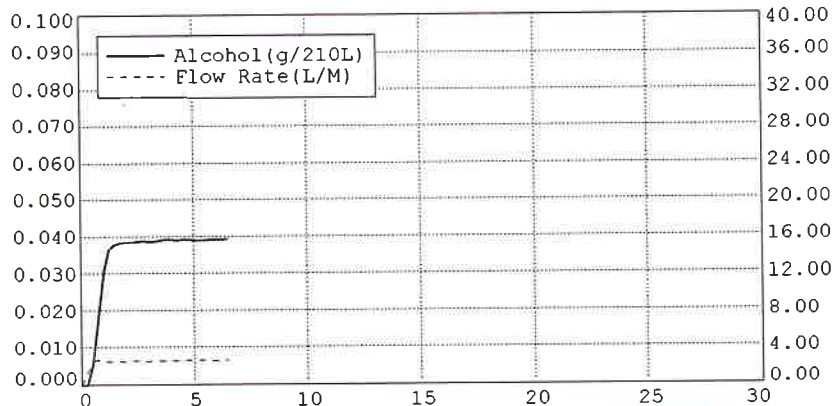

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100352






Date: 03/27/2025
Time: 10:11:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.61: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 583 psi

BLANK TEST	0.000	10:13
INTERNAL STANDARD	VERIFIED	10:13
EXTERNAL STANDARD	0.080	10:13
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.080	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.080	10:15
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.080	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.080	10:17
BLANK TEST	0.000	10:18

Average = 0.0800
Std Dev = 0.0000

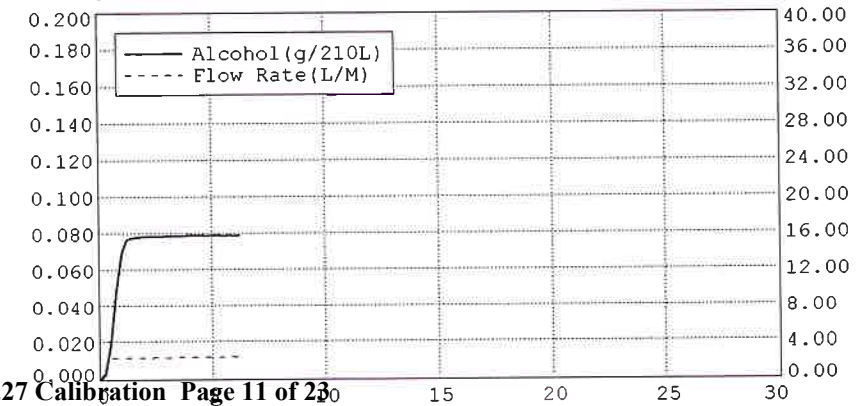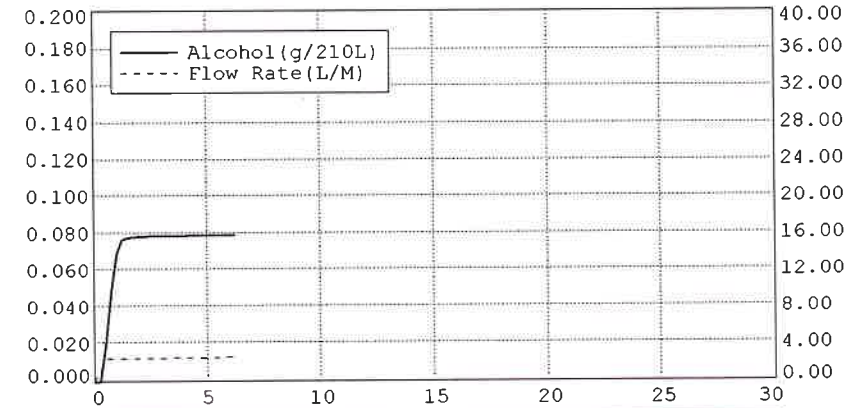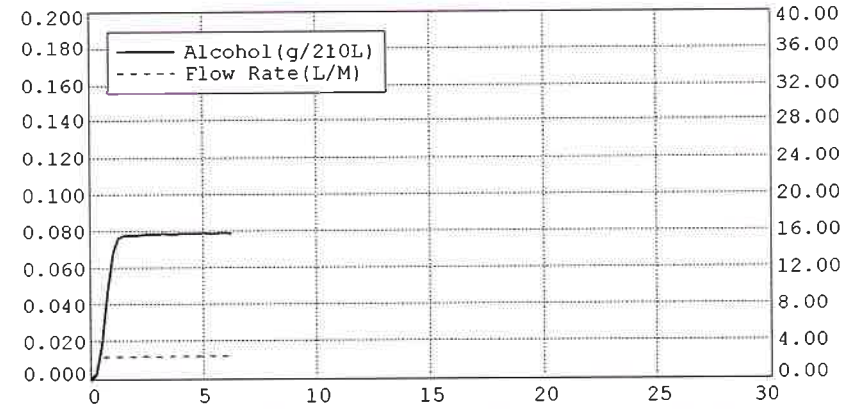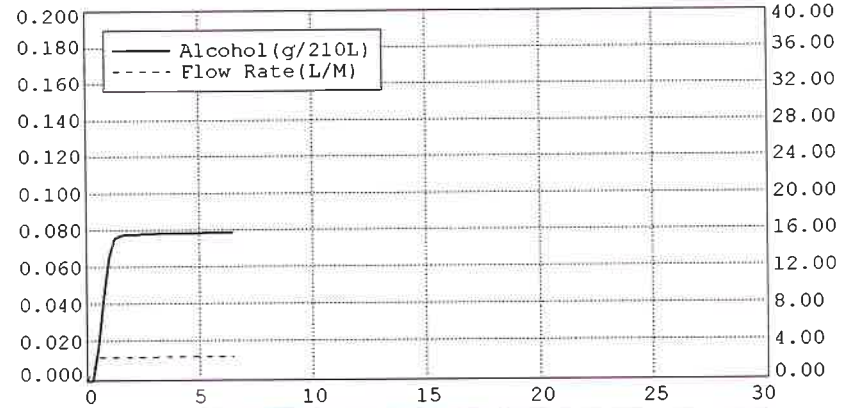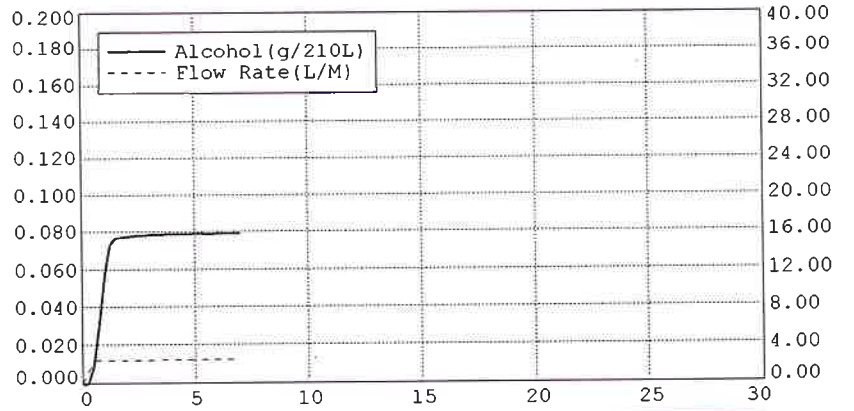

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100352






Date: 03/27/2025
Time: 10:19:48

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.60: 0.099
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 922 psi

BLANK TEST	0.000	10:20
INTERNAL STANDARD	VERIFIED	10:21
EXTERNAL STANDARD	0.101	10:21
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.101	10:22
BLANK TEST	0.000	10:23
EXTERNAL STANDARD	0.101	10:23
BLANK TEST	0.000	10:24
EXTERNAL STANDARD	0.101	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.101	10:25
BLANK TEST	0.000	10:26

Average = 0.1010
Std Dev = 0.0000

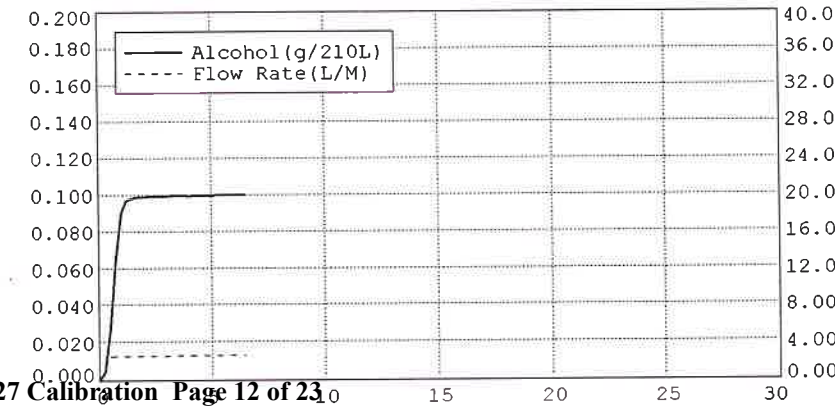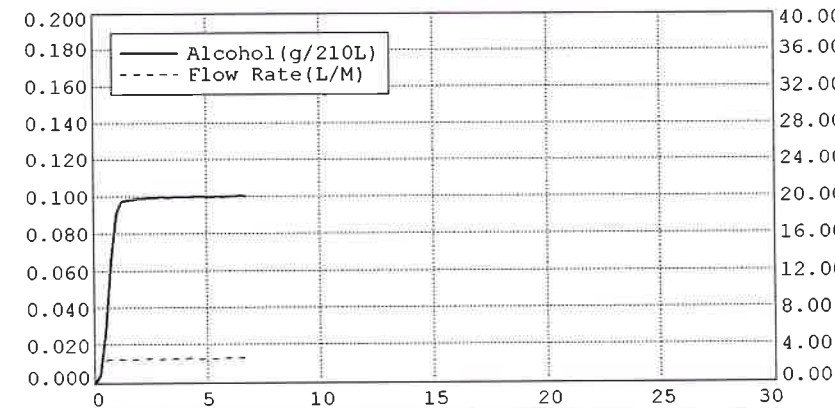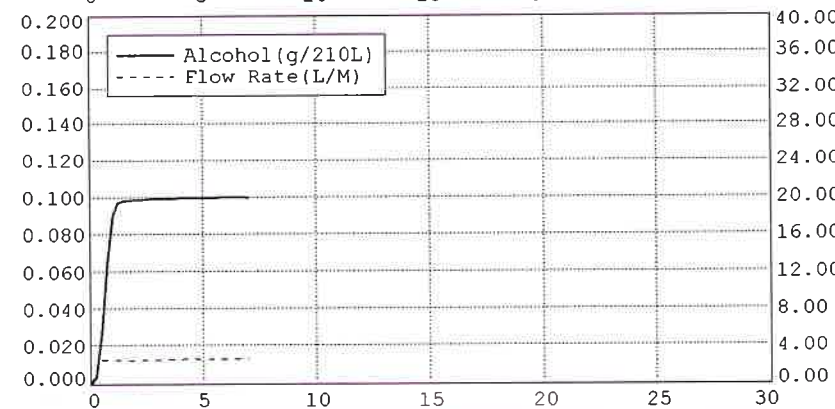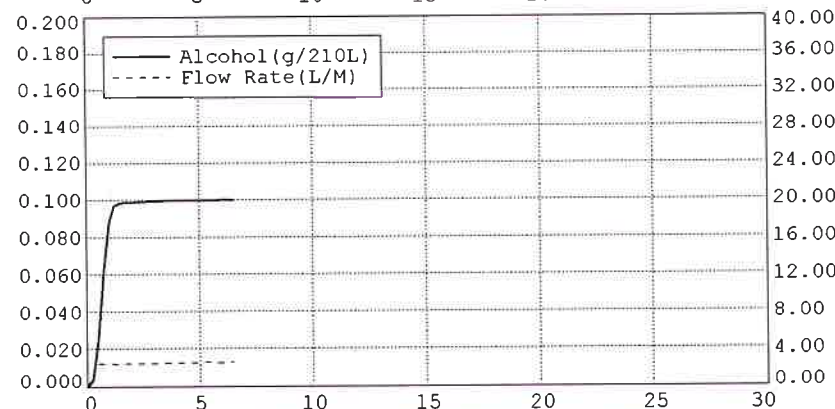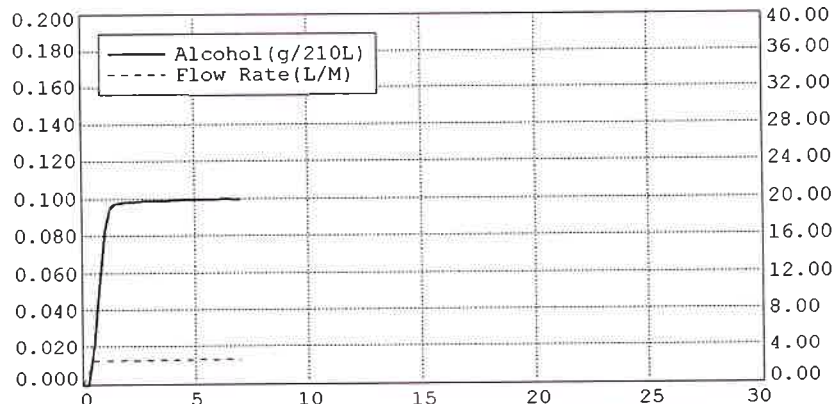

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100352






Date: 03/27/2025
Time: 10:28:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.60: 0.148
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 185 psi

BLANK TEST	0.000	10:29
INTERNAL STANDARD	VERIFIED	10:29
EXTERNAL STANDARD	0.149	10:29
BLANK TEST	0.000	10:30
EXTERNAL STANDARD	0.149	10:31
BLANK TEST	0.000	10:31
EXTERNAL STANDARD	0.149	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.149	10:33
BLANK TEST	0.000	10:34
EXTERNAL STANDARD	0.149	10:34
BLANK TEST	0.000	10:35

Average = 0.1490
Std Dev = 0.0000

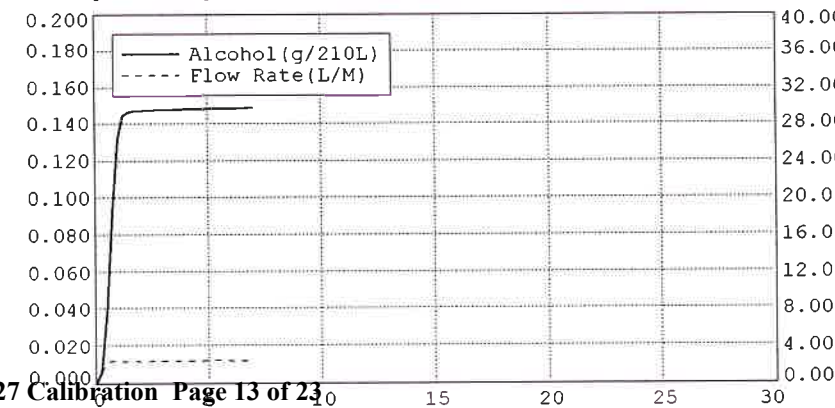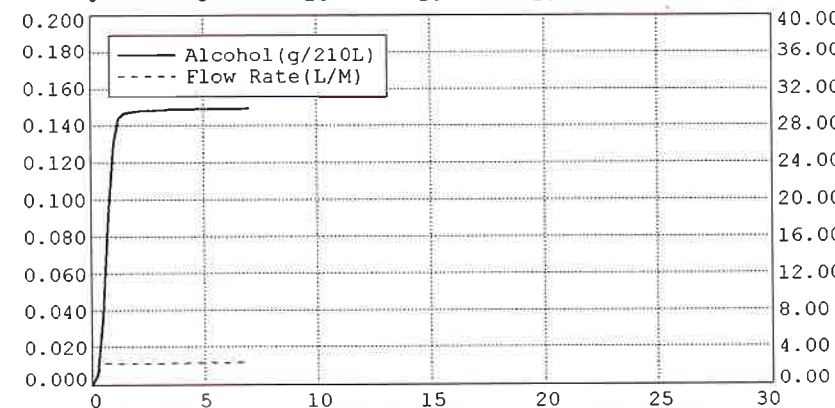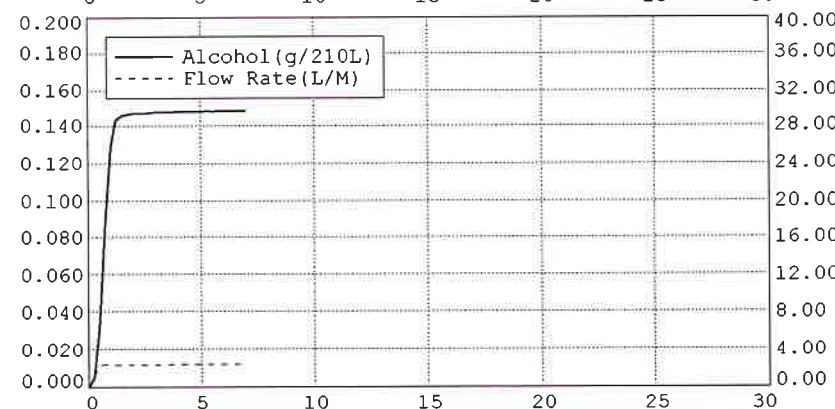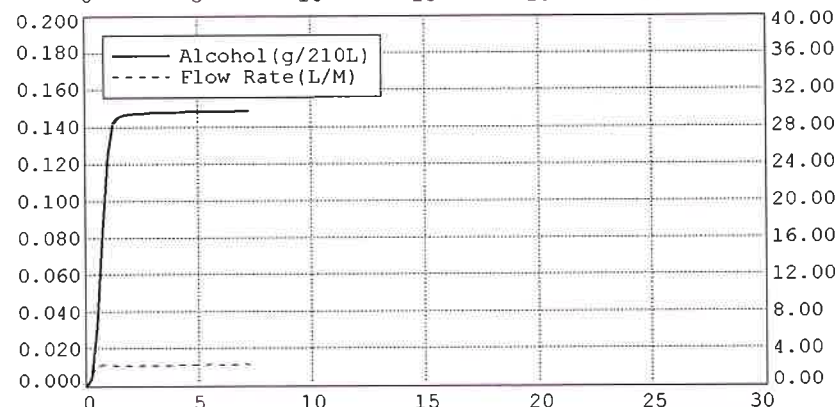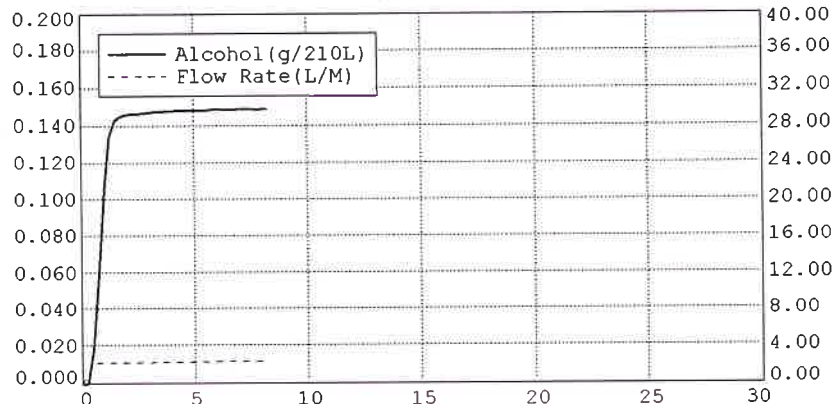

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100352


Date: 03/27/2025
Time: 10:36:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.60: 0.297
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 167 psi

BLANK TEST	0.000	10:38
INTERNAL STANDARD	VERIFIED	10:38
EXTERNAL STANDARD	0.301	10:38
BLANK TEST	0.000	10:39
EXTERNAL STANDARD	0.300	10:39
BLANK TEST	0.000	10:40
EXTERNAL STANDARD	0.301	10:40
BLANK TEST	0.000	10:41
EXTERNAL STANDARD	0.300	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.300	10:43
BLANK TEST	0.000	10:44

Average = 0.3004
Std Dev = 0.0005

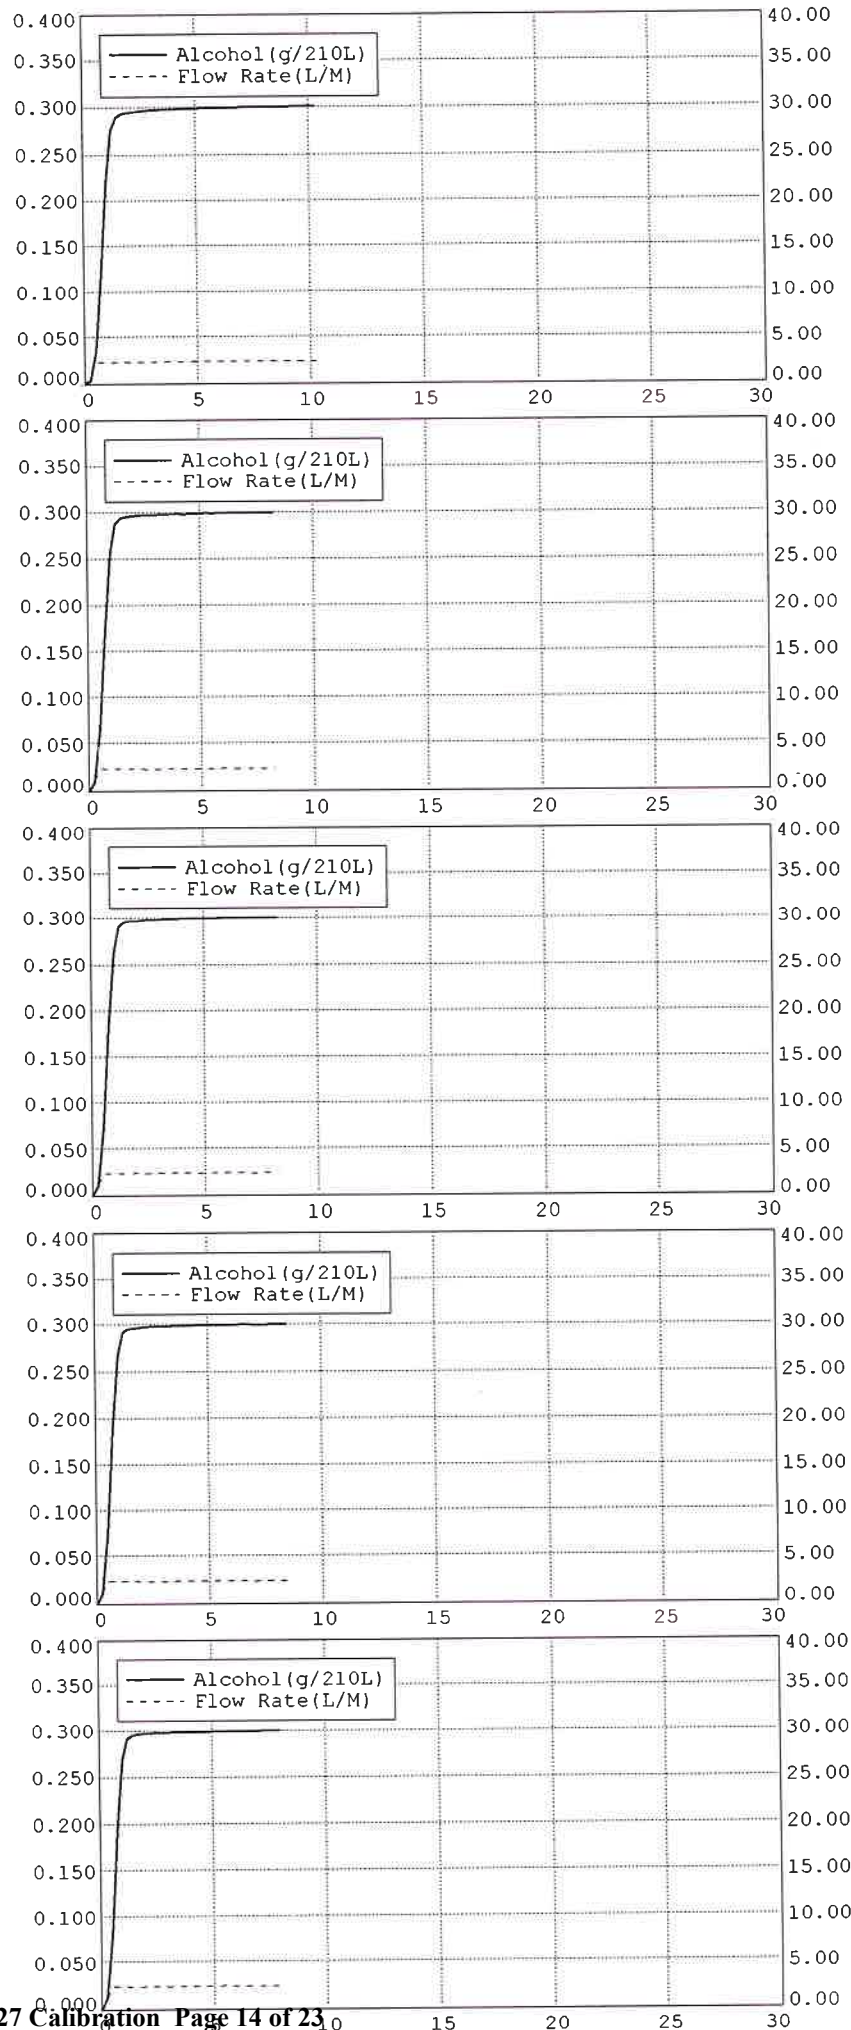

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 11:50:32

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.60: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:51
BLANK TEST	0.000	11:51
INTERNAL STANDARD	VERIFIED	11:51
EXTERNAL STANDARD	0.080	11:51
BLANK TEST	0.000	11:52
SUBJECT SAMPLE	INCOMPLETE	11:54

MNC

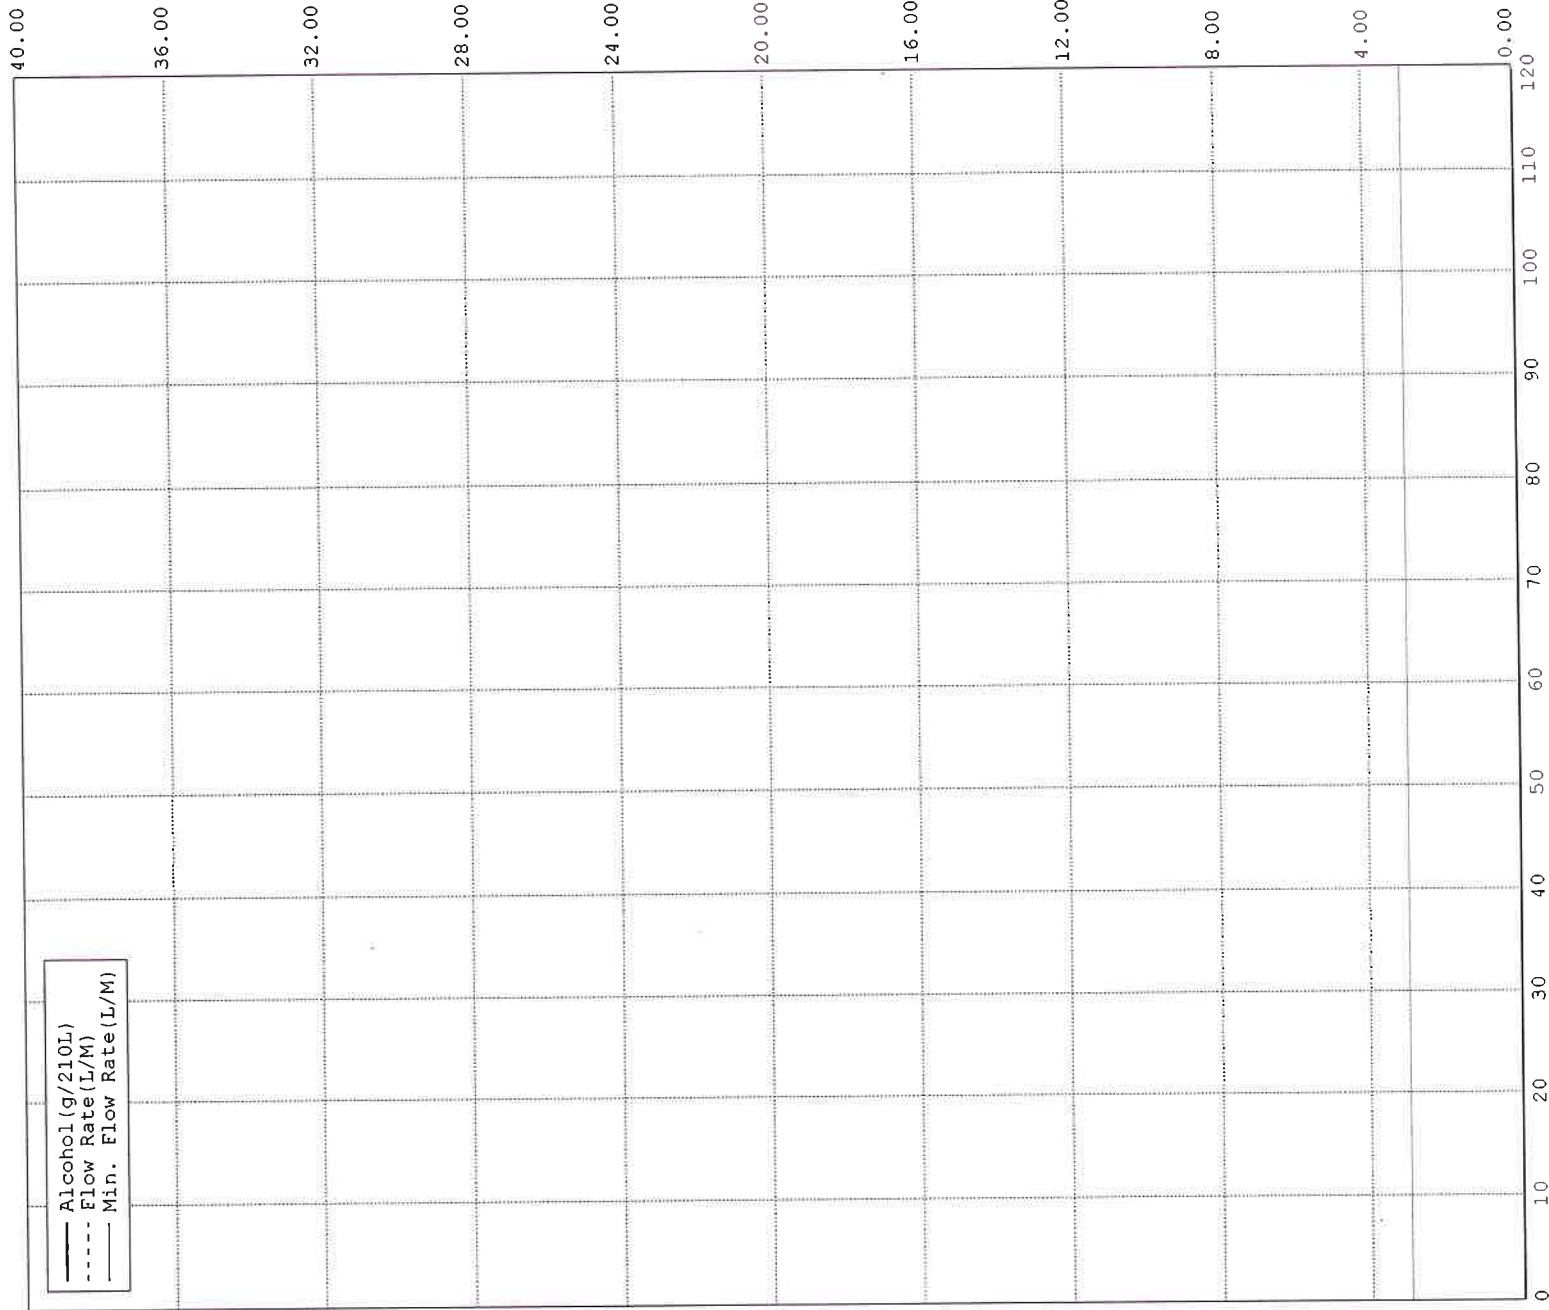

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100352

Date: 03/27/2025
 Time: 11:57:56

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747


DEPT/AGENCY:
 MAXIMUM ATTEMPTS EXCEEDED
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.60: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:59
BLANK TEST	0.000	11:59
INTERNAL STANDARD	VERIFIED	11:59
EXTERNAL STANDARD	0.080	11:59
BLANK TEST	0.000	12:00
SUBJECT SAMPLE	XXX	12:01

Maximum Attempts Exceeded

MNC

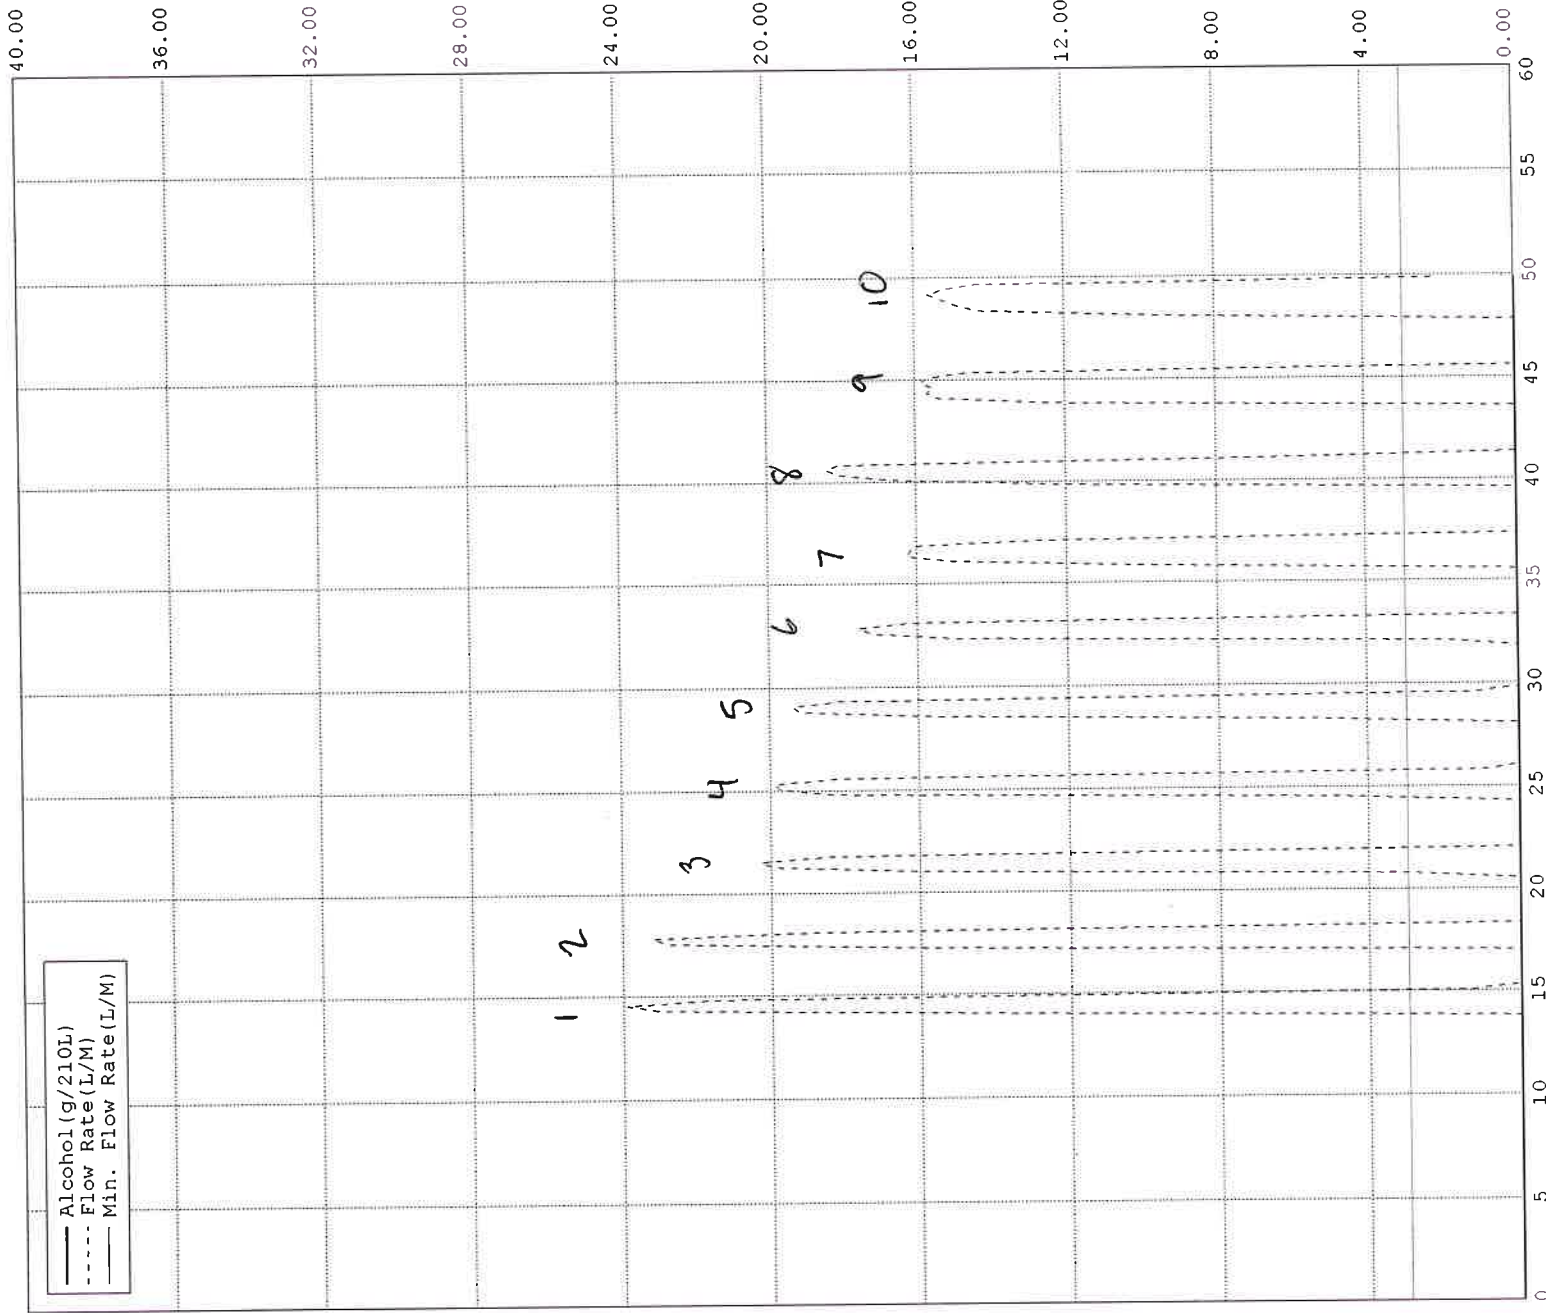

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 12:02:58

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.59: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:04
BLANK TEST	0.000	12:04
INTERNAL STANDARD	VERIFIED	12:04
EXTERNAL STANDARD	0.081	12:04
BLANK TEST	0.000	12:05
SUBJECT SAMPLE	INVALID	12:05

MNC

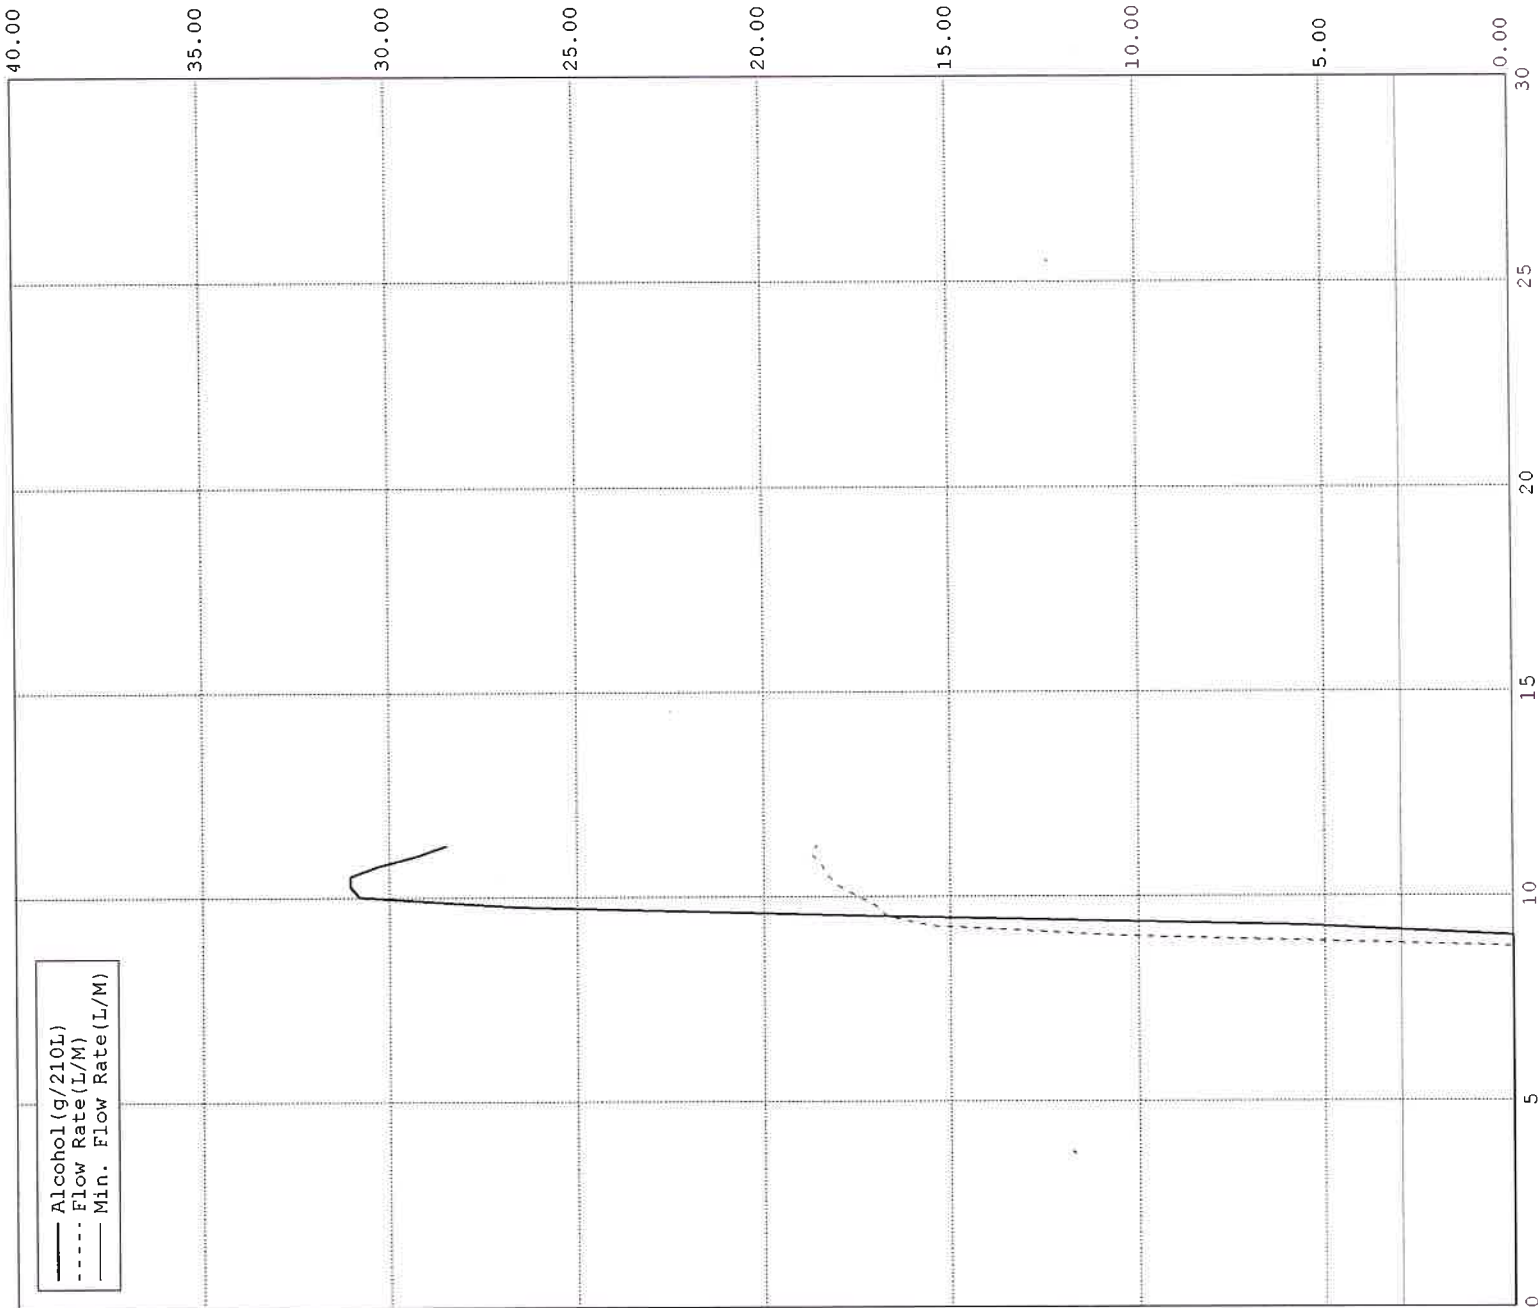

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 12:07:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
RFI

CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.60: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:08
BLANK TEST	0.000	12:09
INTERNAL STANDARD	VERIFIED	12:09
EXTERNAL STANDARD	0.080	12:09
BLANK TEST	0.000	12:10

Suck Back Error

MNC

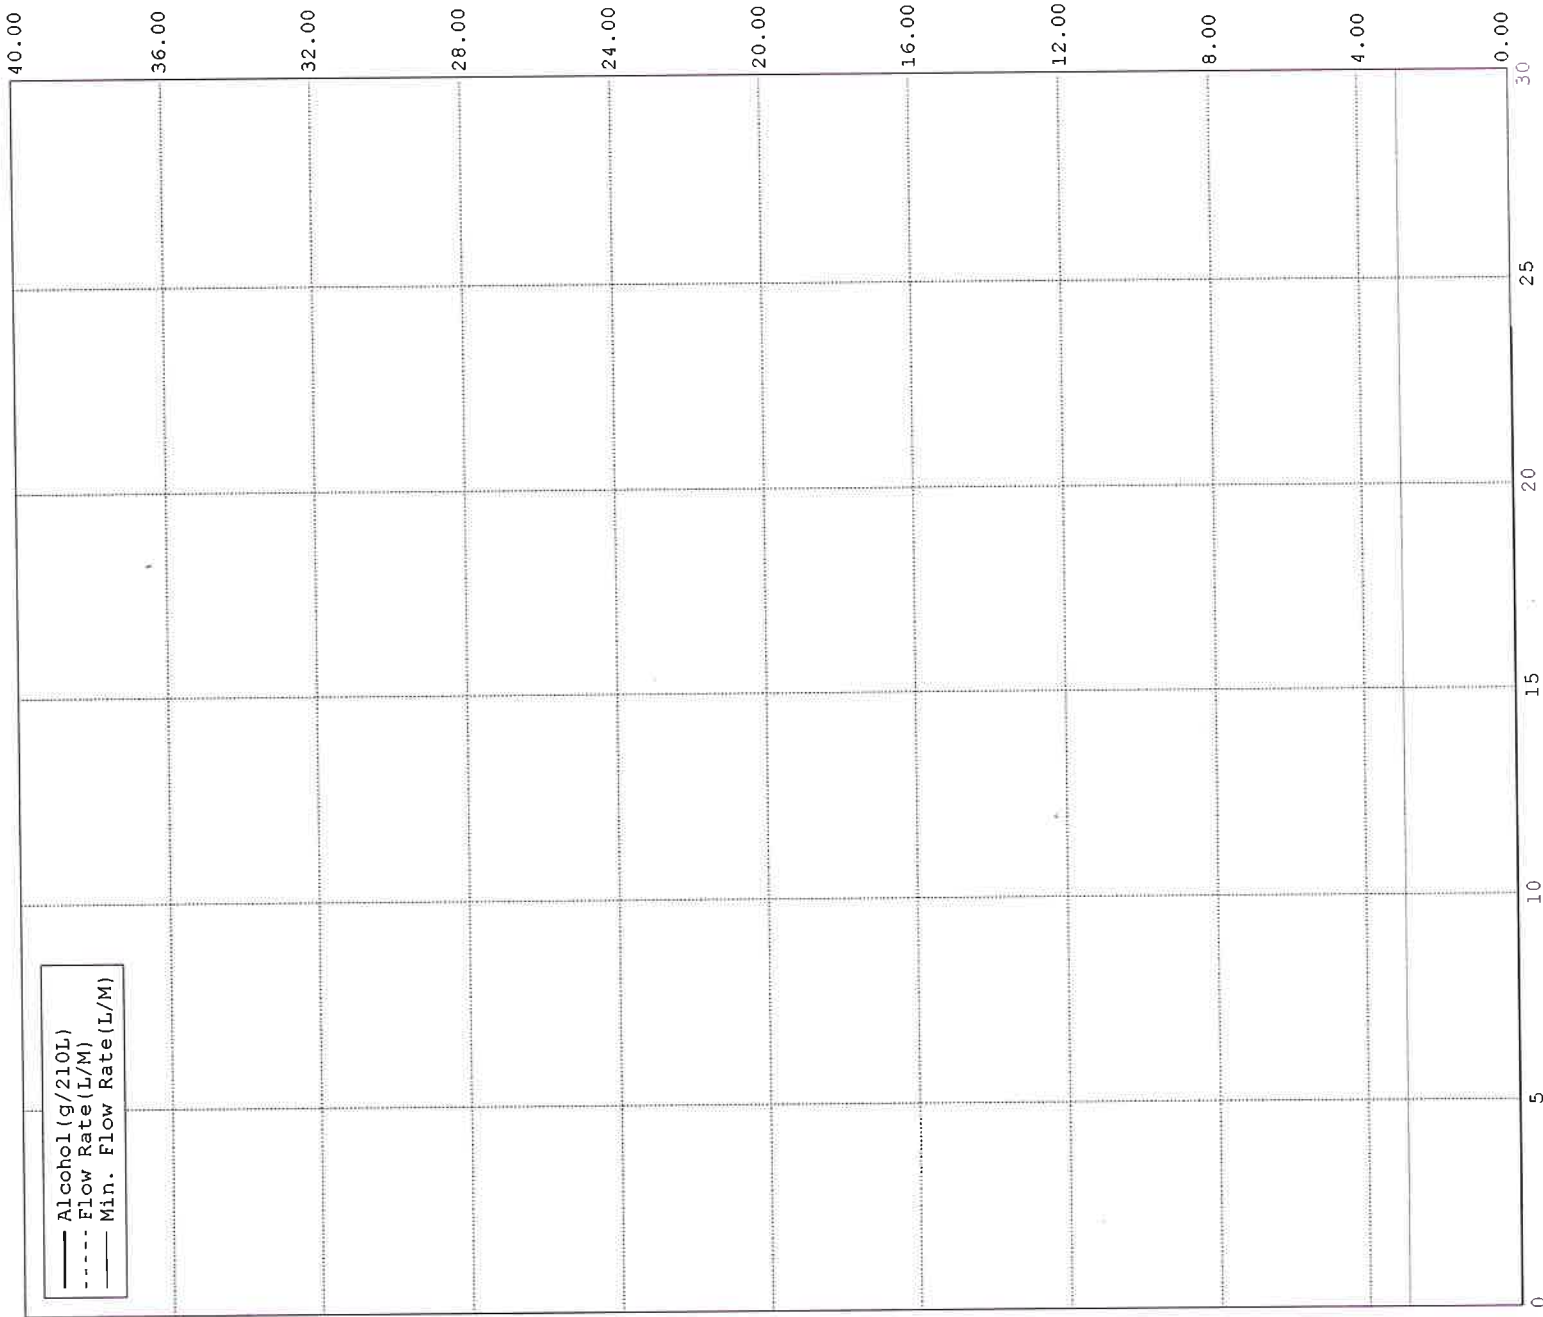

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100352

Date: 03/27/2025
Time: 12:12:49

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.59: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST
INTERNAL STANDARD
EXTERNAL STANDARD
BLANK TEST

PASSED 12:13
0.000 12:13
VERIFIED 12:14
0.080 12:14
0.000 12:15

RFI DETECTED

MNC

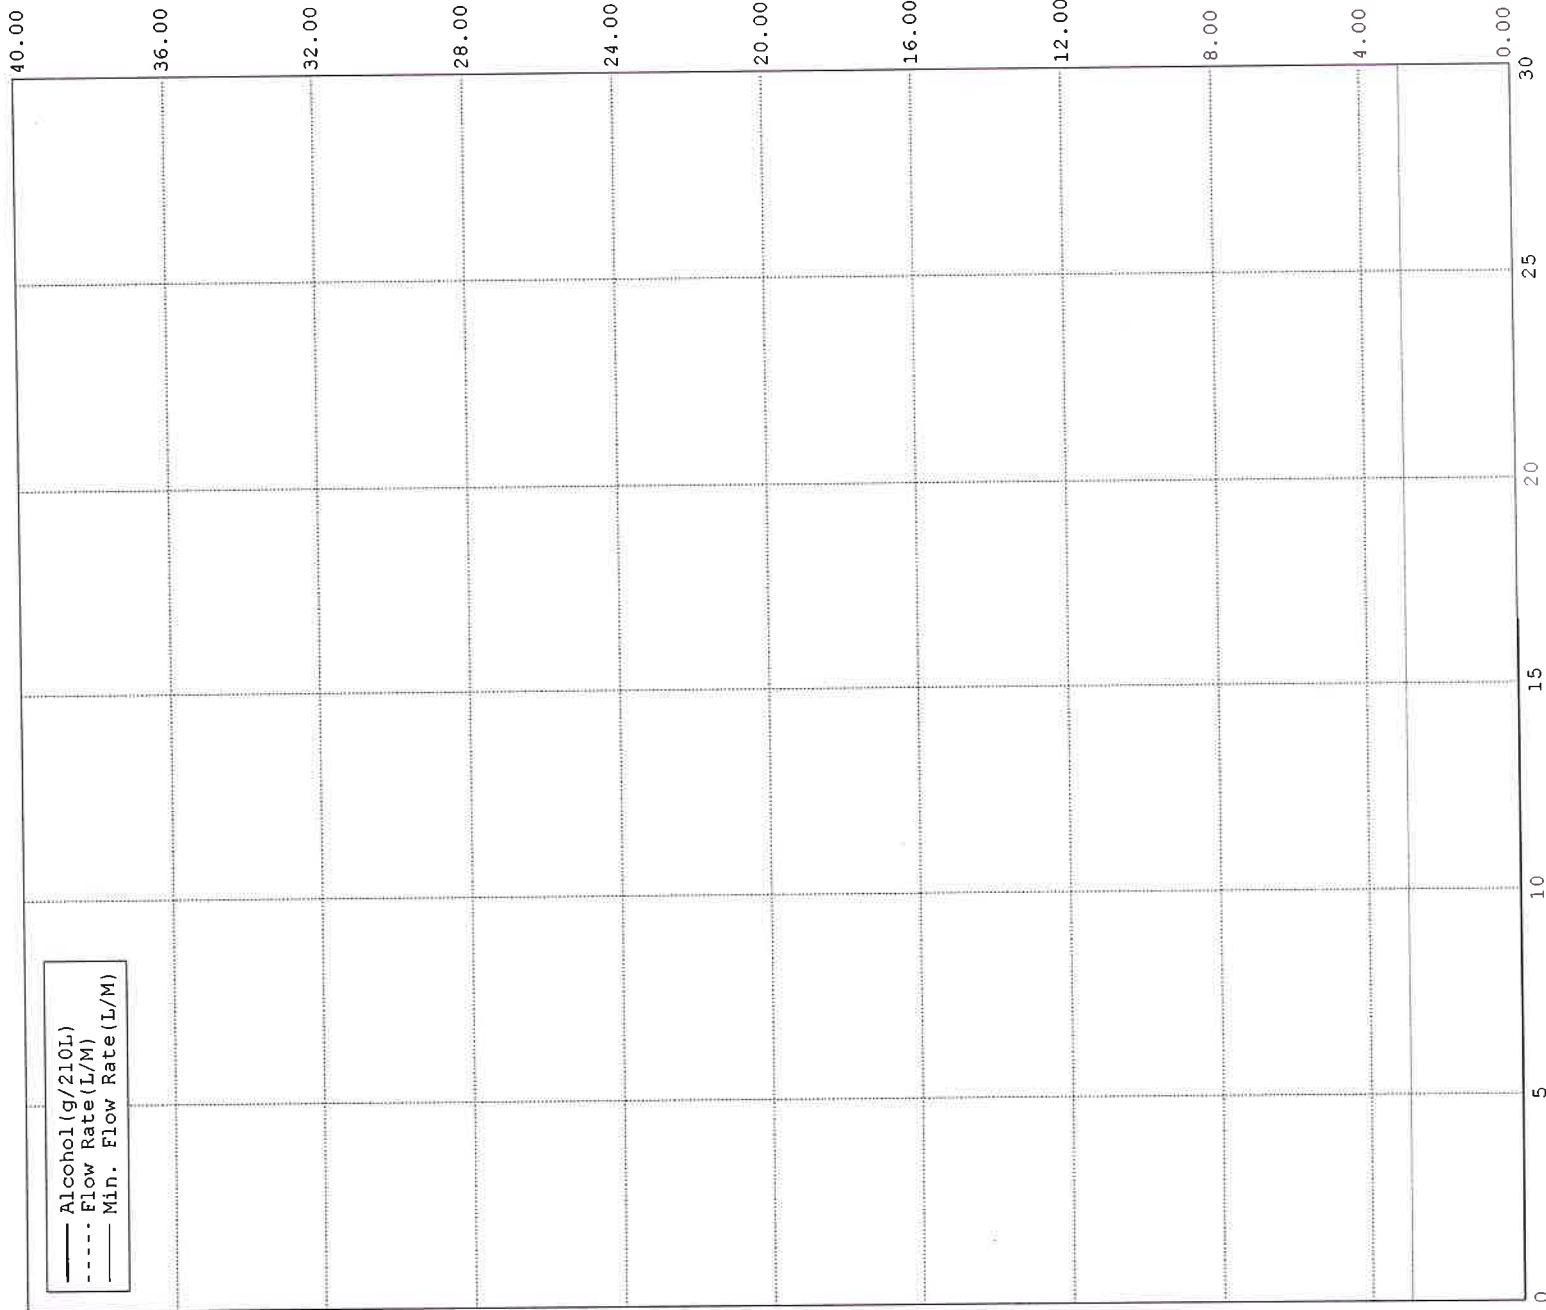

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100352

Date: 03/27/2025
Time: 12:31:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.59: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:32
BLANK TEST	0.000	12:33
INTERNAL STANDARD	VERIFIED	12:33
Xq = 0.088 (2.55%)		
EXTERNAL STANDARD	0.080	12:33
X[1] = 0.0800 (-0.0020)	(0.0021)	
BLANK TEST	0.000	12:34
SUBJECT SAMPLE	XXX	12:34
X[1] = 0.1110 (-0.0147)	(0.0024)	


Interference Detected


Filter 2 Average: -0.0020

Filter 3 Average: 0.0019

NMC 3/27/25

NMC

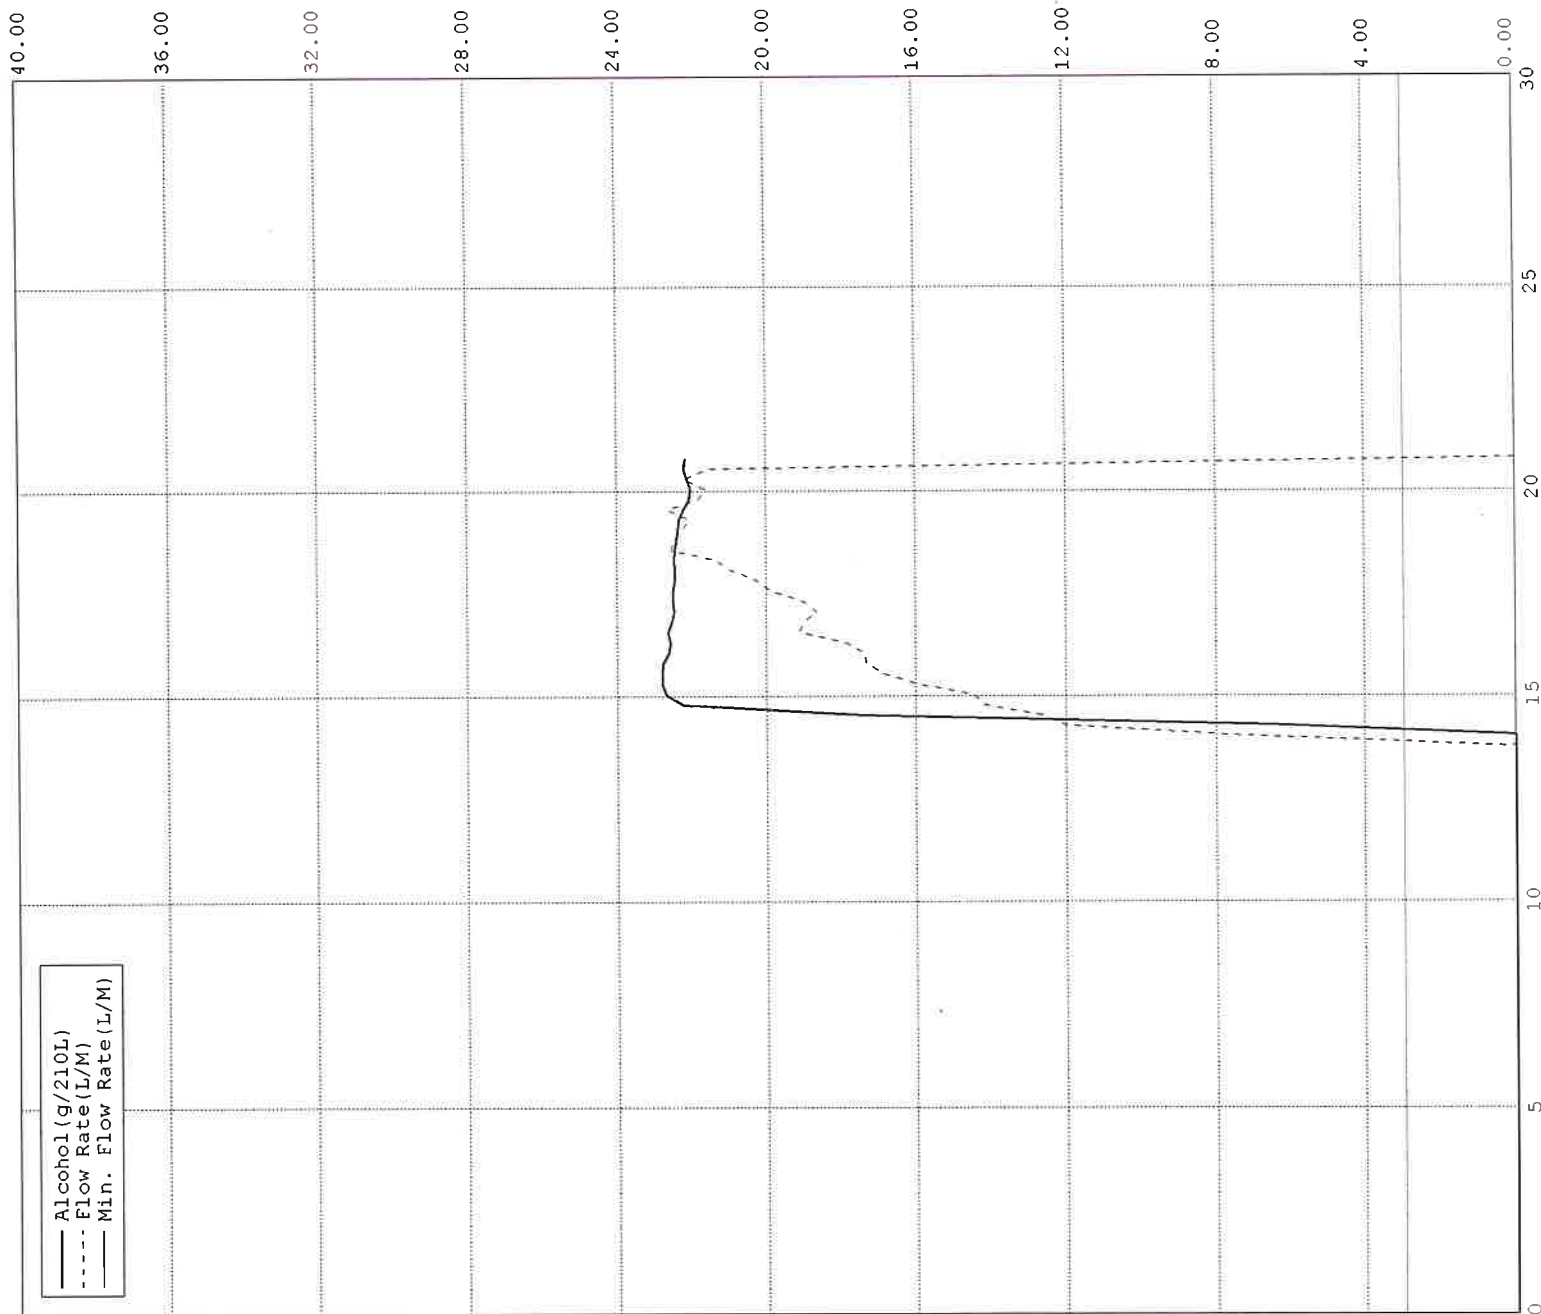

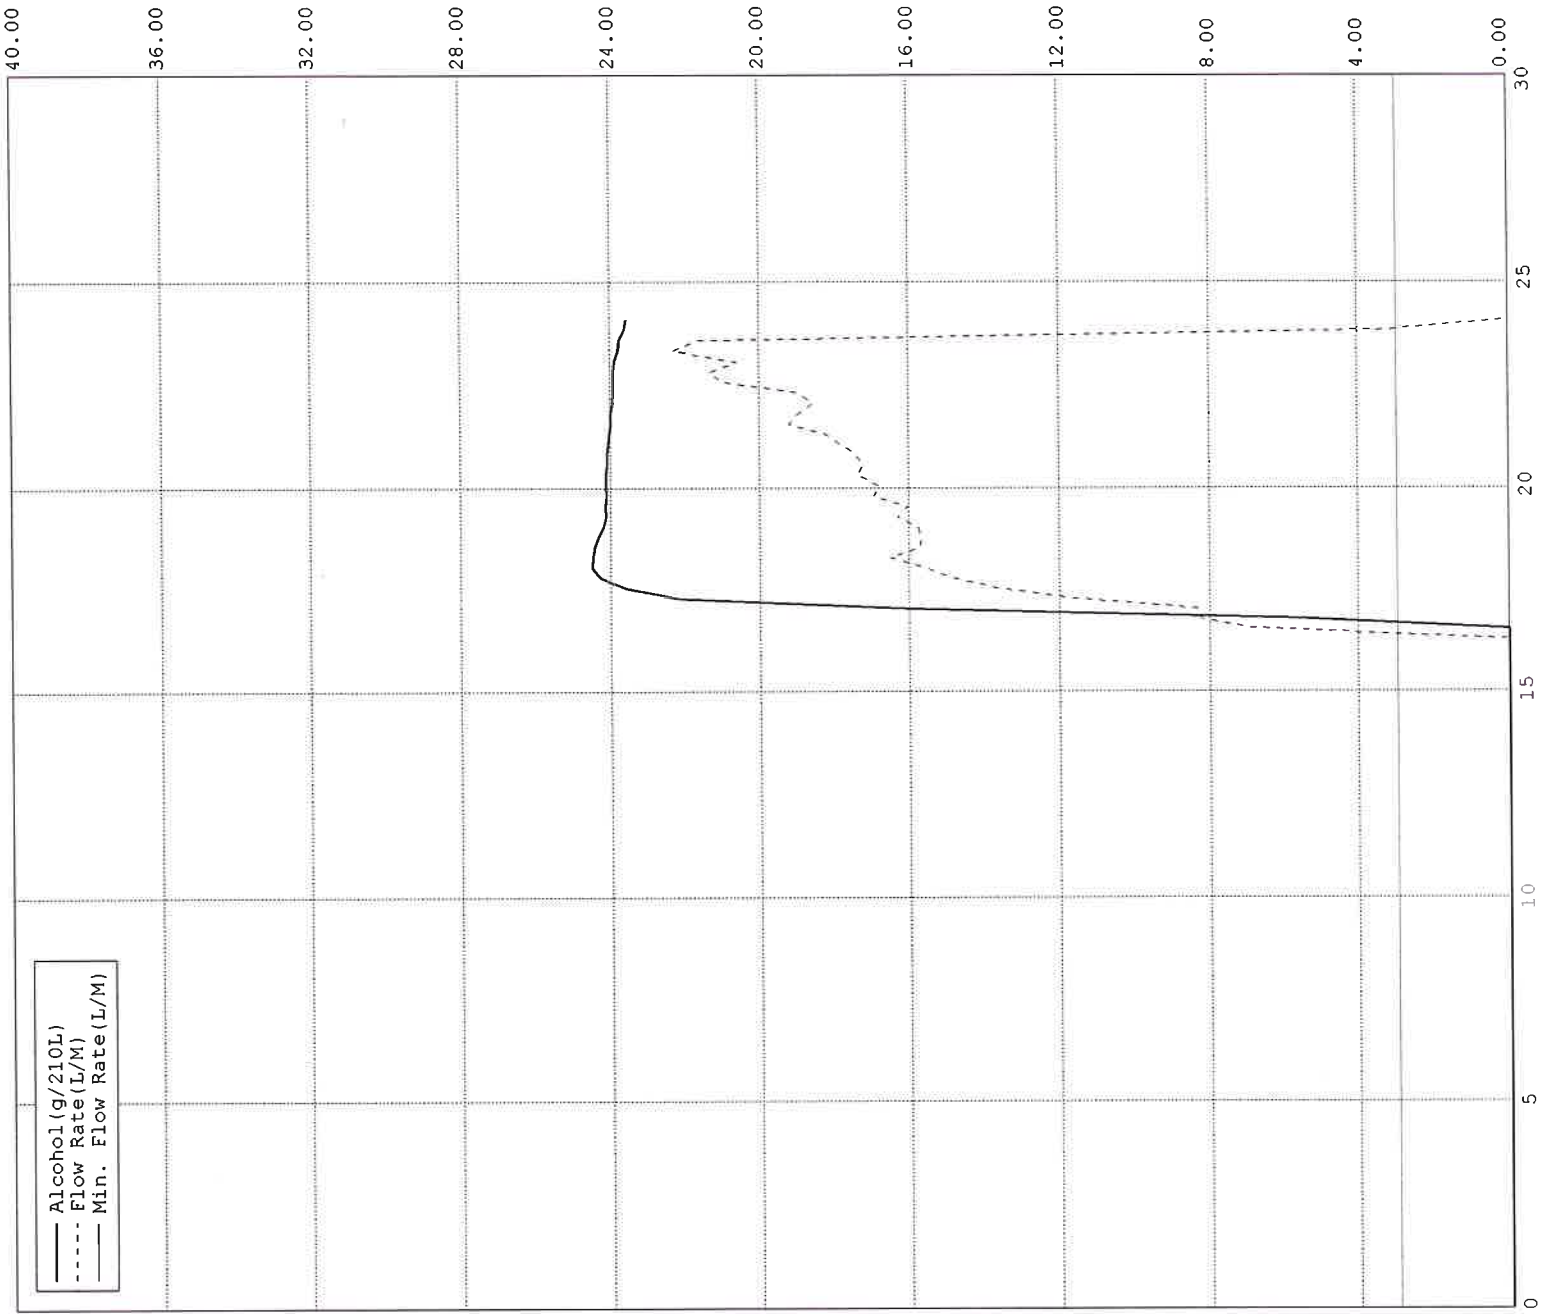

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100352

Date: 03/27/2025

Time: 12:26:55

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - IPA

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.60: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

PASSED 12:27

BLANK TEST

0.000 12:28

INTERNAL STANDARD

VERIFIED 12:28

Xq = 0.087 (2.35%)

EXTERNAL STANDARD

0.080 12:28

X[1] = 0.0798 (-0.0021) (0.0016)

BLANK TEST

0.000 12:29

SUBJECT SAMPLE

XXX 12:29

X[1] = 0.1183 (-0.0261) (0.0021)

Interference Detected

MNC

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 12:17:02

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.60: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:18
BLANK TEST	0.000	12:18
INTERNAL STANDARD	VERIFIED	12:18
$X_q = 0.087$ (2.14%)	0.080	12:18
EXTERNAL STANDARD	$X[1] = 0.0804$ (-0.0022)	(0.0022)
BLANK TEST	0.000	12:19
SUBJECT SAMPLE (Vol=1.97L)	$X[1] = 0.0963$ (-0.0009)	(0.0011)
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	$X[1] = 0.0799$ (-0.0018)	(0.0017)
BLANK TEST	0.000	12:22

MNC

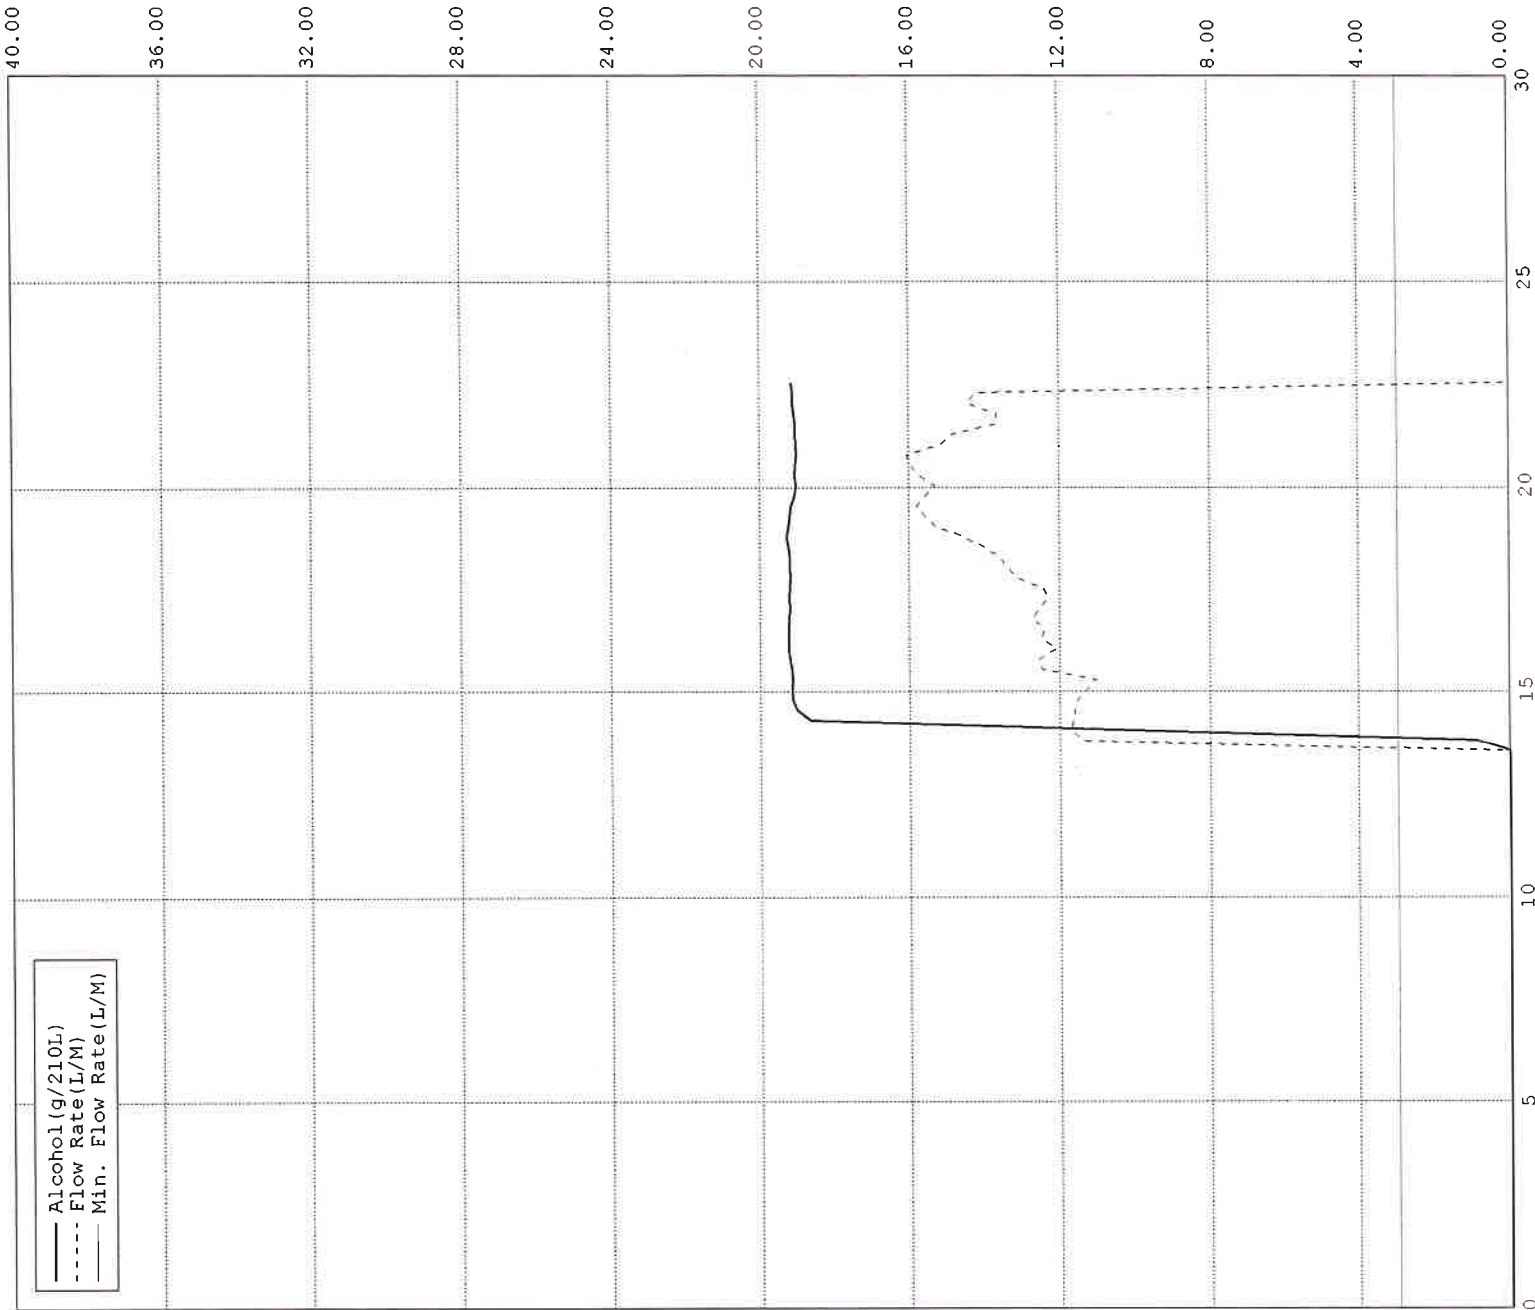

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100352

Date: 03/27/2025
Time: 12:50:00

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.58: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:50
BLANK TEST	0.000	12:51
INTERNAL STANDARD	VERIFIED	12:51
EXTERNAL STANDARD	0.080	12:51
BLANK TEST	0.000	12:52
SUBJECT SAMPLE (Vol=2.02L)	0.000	12:52
BLANK TEST	0.000	12:53
EXTERNAL STANDARD	0.080	12:53
BLANK TEST	0.000	12:54

MNC

