

VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100403

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/17/2017

External Standard Test Values

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.18: 0.078
LOT #: AG634001
EXPIRATION: 12/05/2018
TANK PRESSURE: 1023 psi

BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:42
EXTERNAL STANDARD	0.080	10:43
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.080	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.080	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.079	10:46
BLANK TEST	0.000	10:47
EXTERNAL STANDARD	0.079	10:47
BLANK TEST	0.000	10:48

Average = 0.0796
Std Dev = 0.0005

Diagnostic Check

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C	PASSED
Breath Tube = 44.9°C	PASSED

PUMP INFO

Flow Rate = 4.709 L/M	PASSED
-----------------------	--------

DETECTOR INFO

PUMP ON	PASSED
PUMP OFF	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED


INTERNAL STANDARD	PASSED
-------------------	--------



I, Charles R. Foster, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Charles R. Foster
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 9 day of Nov, 20 17


Kyle Klopfer, Notary Public
My Commission Expires With Office

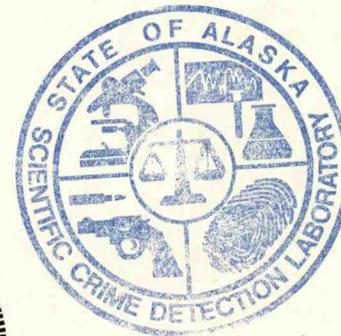


10/19/17