




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100687

Report Issue Date: 12/22/2025
Date Received: 2025-11-18
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.079	AG335202	0.078	0.078	0.077	0.078	0.078	0.078
0.300	0.295	AG427706	0.289	0.288	0.288	0.289	0.289	0.289

As Found - Evaluation Analyst: Kaija Swisher

As Found Conditions - Barometric Pressure (inHg): 29.39 Barometer Used: VWR S/N 240680771 Temperature (C): 20.9 Relative Humidity (%): 16

As-Found Lab Activity Date Range: 11/18/2025 - 11/18/2025

Internal standard greater than 3%. Recommend adjustment.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.078	AG335202	0.078	0.078	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.098	AG516101	0.097	0.097	0.097	0.096	0.096	0.097	+/- 0.004
0.150	0.147	AG515604	0.145	0.144	0.145	0.145	0.145	0.145	+/- 0.006
0.300	0.294	AG427706	0.291	0.290	0.291	0.290	0.290	0.290	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.27 Barometer Used: VWR S/N 240680771 Temperature (C): 21.6 Relative Humidity (%): 4

As-Left Lab Activity Date Range: 12/08/2025 - 12/08/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Carlie Glaister on 12/19/2025

carlie.glaister@alaska.gov

Technically and administratively reviewed by Kaija Swisher on 12/22/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100687 Analyst or Technician Name: Charlie Glaister

DataMaster DMT Calibration Start Date: 12/8/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.27 Temperature(C) 21.6 Relative Humidity(%) 4

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250922K5 Expiration Date: 12/22/25
Simulator S/N: DR4178 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250922K5 Expiration Date: 12/22/25
Simulator S/N: DR4177 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 3/19/27 $\rightarrow$ shn.
Simulator S/N: DR4163 Thermometer Verification Performed? ☒ 12/22/25 $\rightarrow$ pref.

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 12/8/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 12/8/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 11:47:11

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 44.5°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.56 V	PASSED
(0.94 V - 2.18 V)	
Cooler Voltage = 1.56 V	PASSED
(0.94 V - 2.18 V)	
Bias Voltage = 80 V	PASSED
(48 V - 112 V)	
Chopper Freq = 540 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.2 in	

PUMP INFO

Flow Rate = 4.422 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.003 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.094 0.37%	PASSED
(0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100687

Date: 12/08/2025

Time: 11:55 AM

Temperatures (°C)

Sample Cell: 49.4°C

Breath Tube: 44.5°C

Current Barometer 29.3 in

Volume (litr) 1.54

Settings

Lamp: 1.56 V

Bias: 80 V

Cooler: 1.56 V

Chopper: 538 Hz

Voltages (V)

Flow: 1.06 V

Detector: -0.004 V


CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 10:59:28

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca	=	0.1000		
CAL	=	1.001978	0.800	<= CAL < 1.200
b1	=	0.0005	0.0000	<= b1 < 0.0040
b2	=	0.0058	0.0010	<= b2 < 0.0100
b3	=	0.0006	0.0000	<= b3 < 0.0040
Xq	=	0.0938	0.0500	<= Xq < 0.2000
a21	=	1.157053	1.050	<= a21 < 1.300
a31	=	0.530116	0.300	<= a31 < 0.800

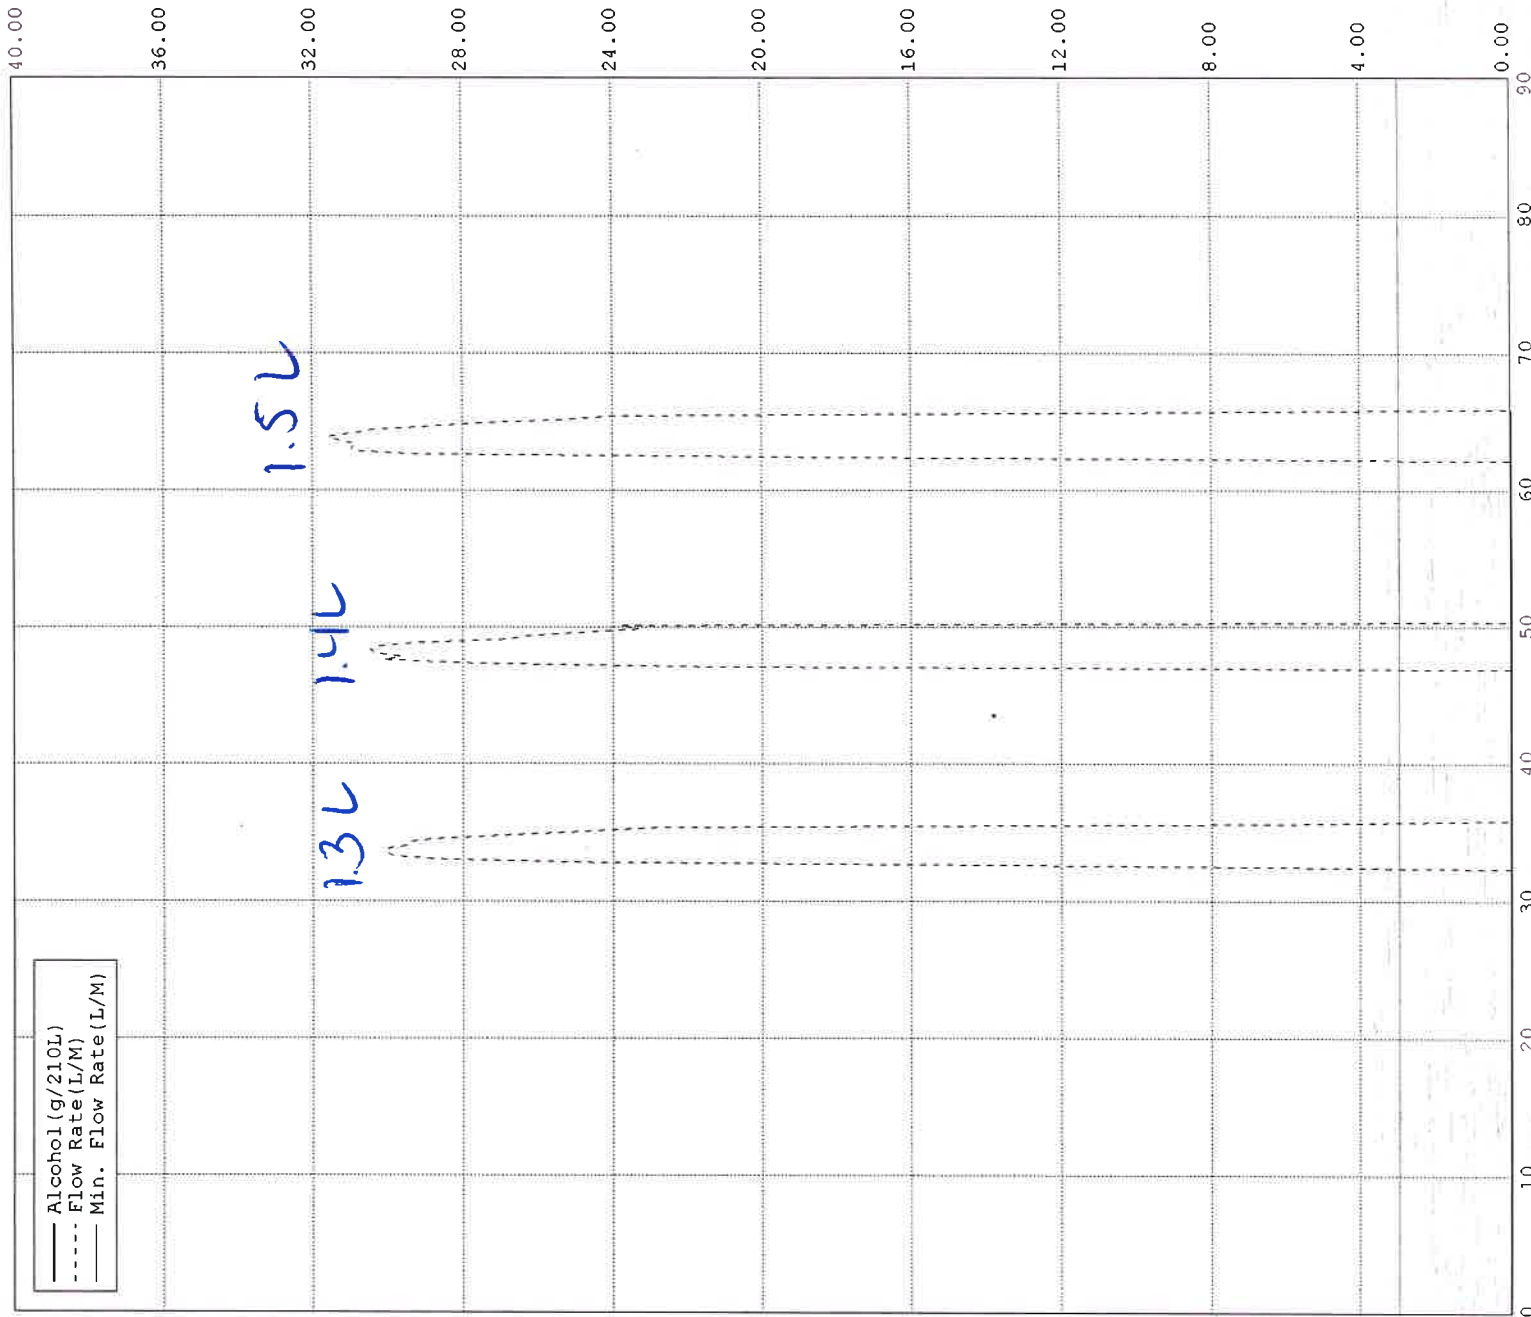

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 11:58:02

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:59
BLANK TEST	0.000	11:59
INTERNAL STANDARD	VERIFIED	11:59
EXTERNAL STANDARD	0.078	11:59
BLANK TEST	0.000	12:00
SUBJECT SAMPLE (Vol=1.59L)	0.000	12:01
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.078	12:02
BLANK TEST	0.000	12:03

CX65

LINEARITY CHECK


Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 12:09:53

SUPERVISOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0390	0.0000
0.078	0.0780	0.0000
0.098	0.0966	0.0005
0.147	0.1448	0.0004
0.294	0.2904	0.0005

SLOPE = 0.985699
R² = 0.999979

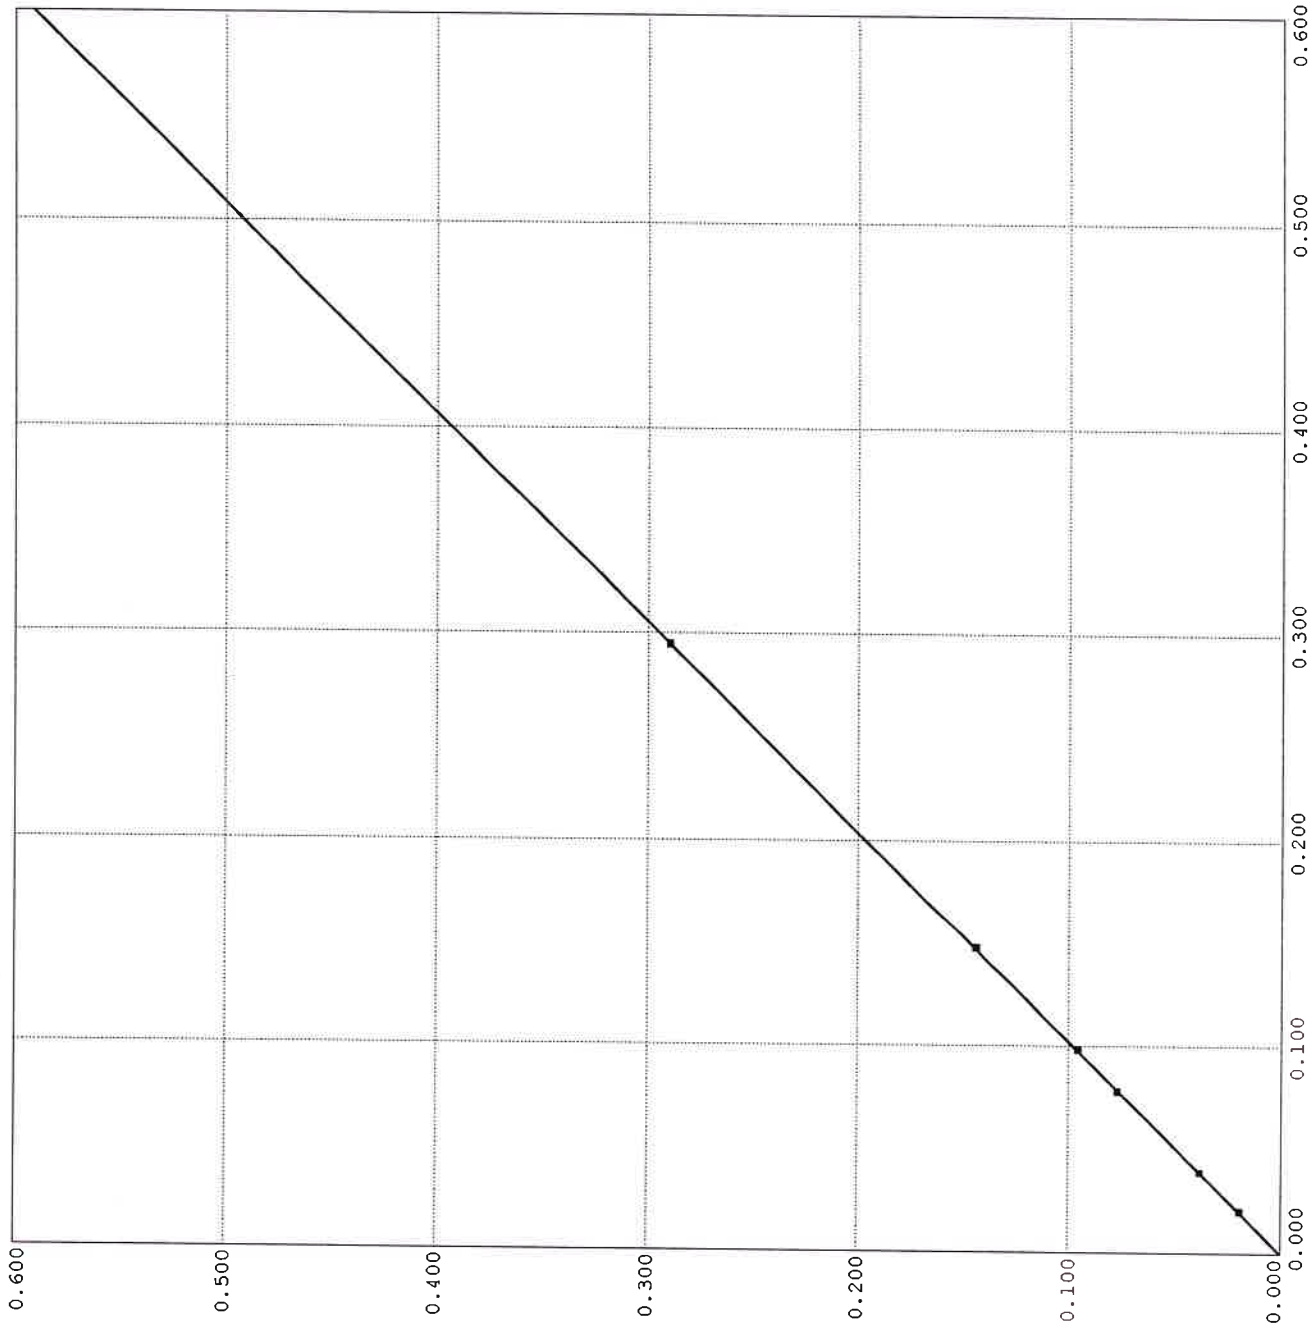

A filter wheel error occurred on 1st attempt of 0.300. DMG-12/8/25
This instrument does not have a recent history of filter wheel errors. Error was not repeated during calibration. DMG 12/8/25

DMG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100687






Date: 12/08/2025
Time: 12:09:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.27: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 779 psi

BLANK TEST	0.000	12:11
INTERNAL STANDARD	VERIFIED	12:11
EXTERNAL STANDARD	0.020	12:11
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.020	12:12
BLANK TEST	0.000	12:13
EXTERNAL STANDARD	0.020	12:13
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.020	12:14
BLANK TEST	0.000	12:15
EXTERNAL STANDARD	0.020	12:15
BLANK TEST	0.000	12:16

Average = 0.0200
Std Dev = 0.0000

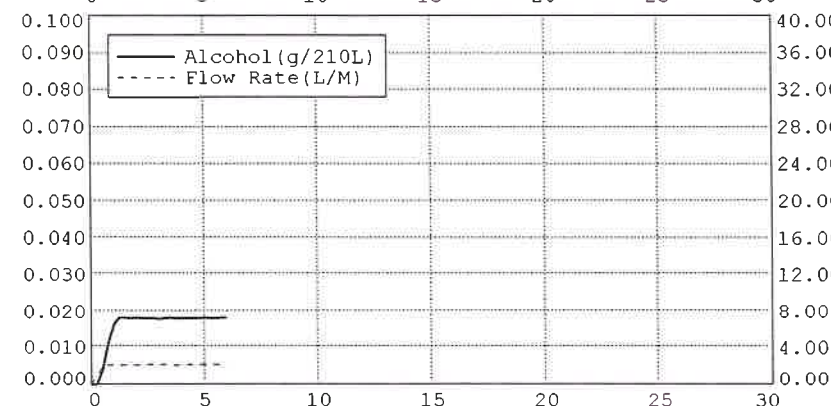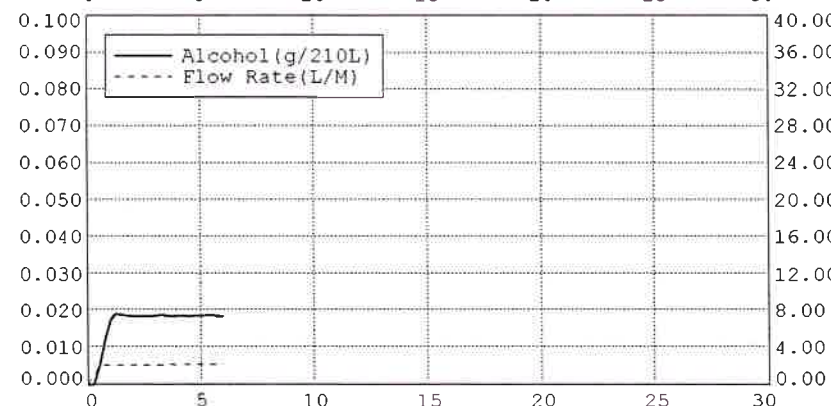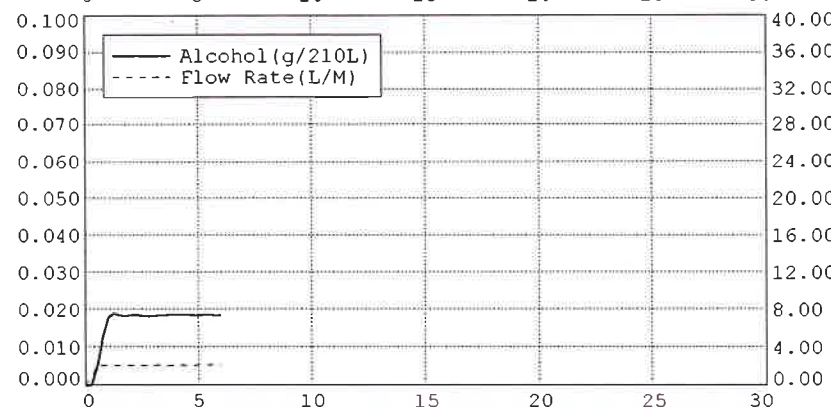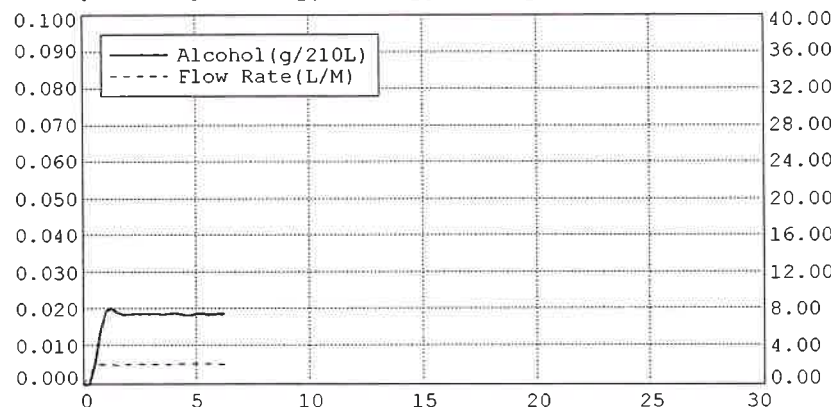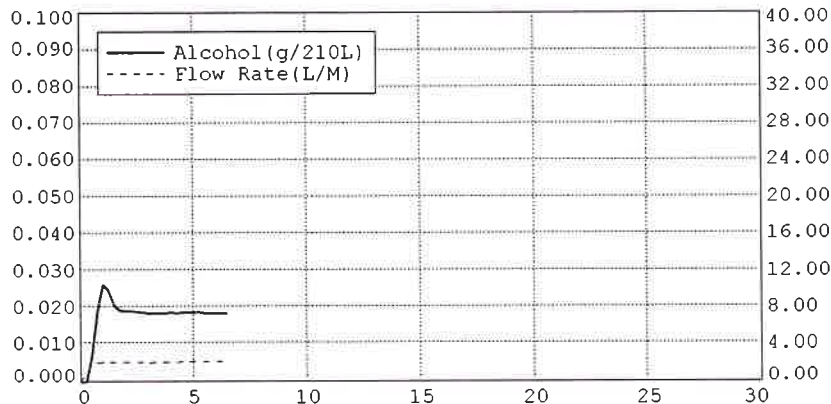

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100687






Date: 12/08/2025
Time: 12:18:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.28: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 701 psi

BLANK TEST	0.000	12:20
INTERNAL STANDARD	VERIFIED	12:20
EXTERNAL STANDARD	0.039	12:20
BLANK TEST	0.000	12:21
EXTERNAL STANDARD	0.039	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.039	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.039	12:23
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.039	12:24
BLANK TEST	0.000	12:25

Average = 0.0390
Std Dev = 0.0000

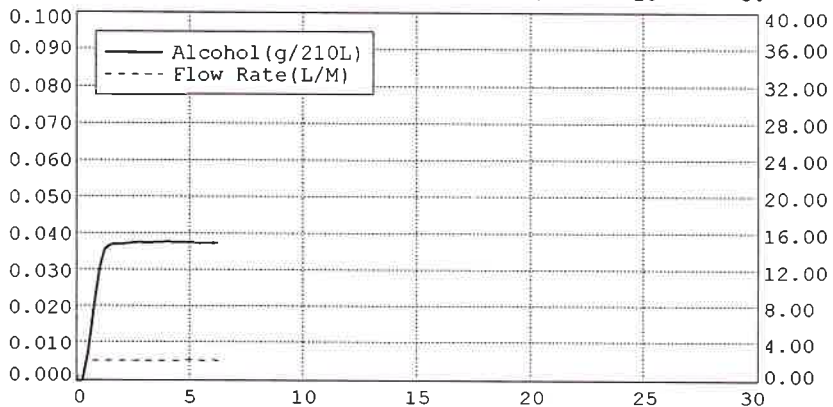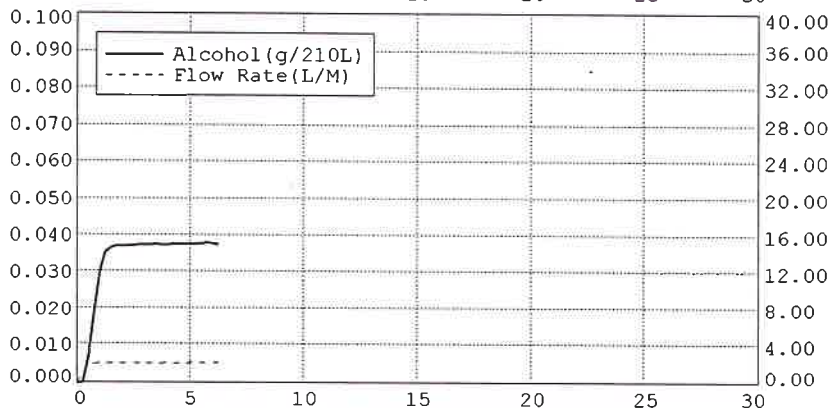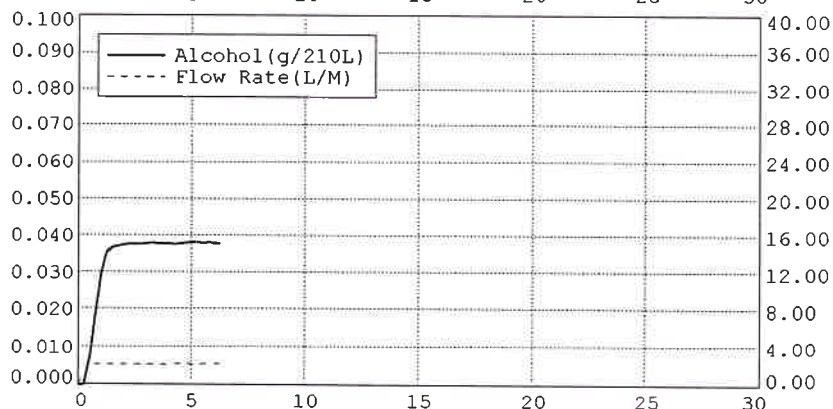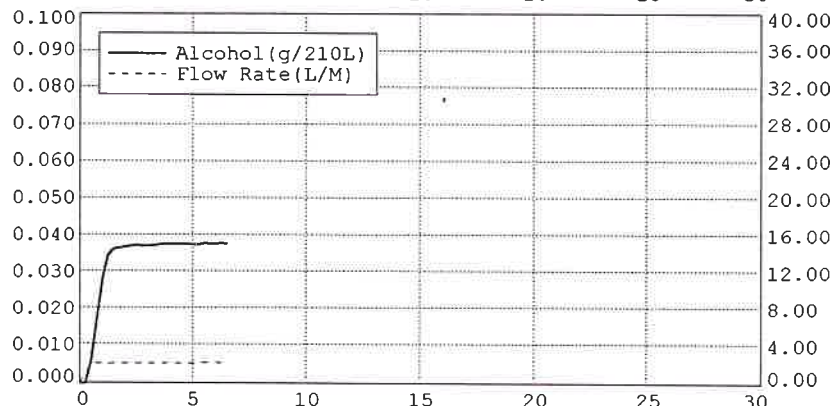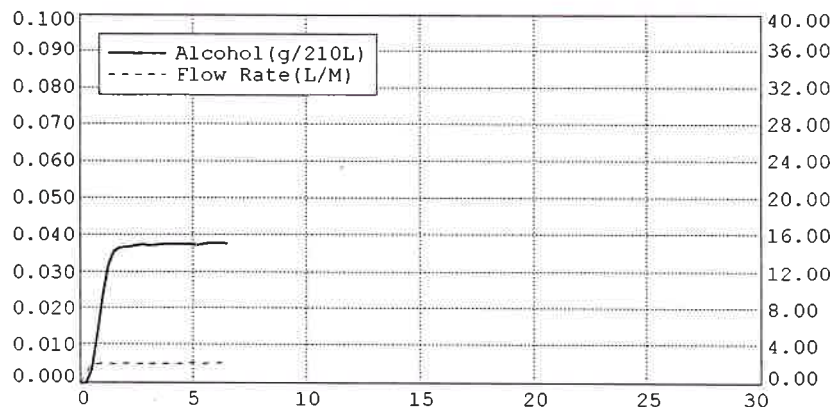

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025

Time: 12:26:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.28: 0.078

LOT #: AG335202






EXPIRATION: 12/18/2025

TANK PRESSURE: 1043 psi

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:27
EXTERNAL STANDARD	0.078	12:28
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.078	12:29
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.078	12:30
BLANK TEST	0.000	12:31
EXTERNAL STANDARD	0.078	12:31
BLANK TEST	0.000	12:32
EXTERNAL STANDARD	0.078	12:32
BLANK TEST	0.000	12:33

Average = 0.0780

Std Dev = 0.0000

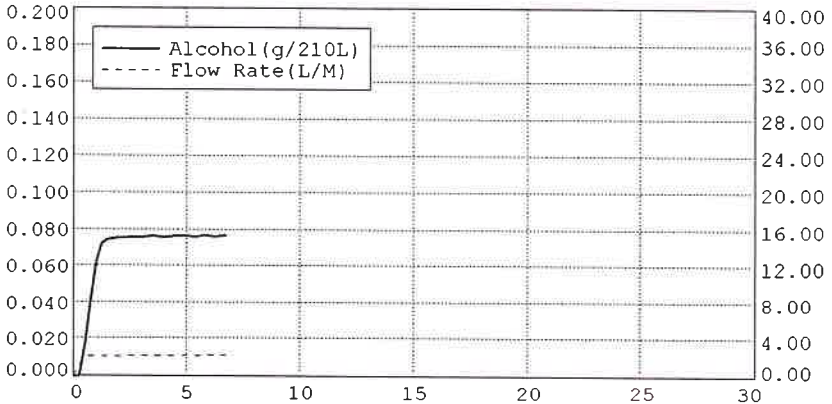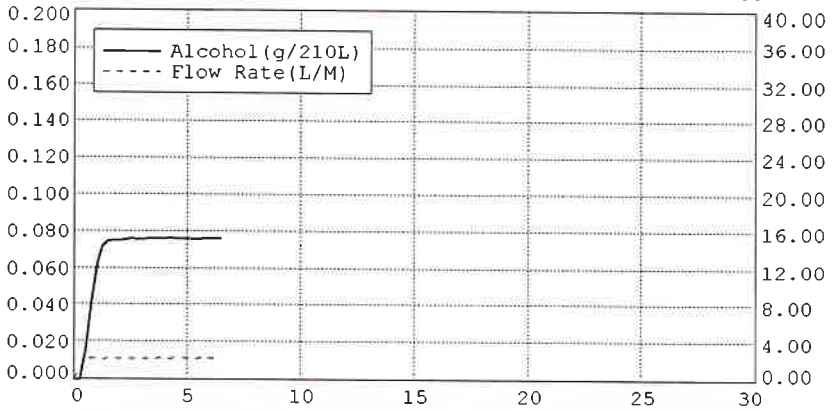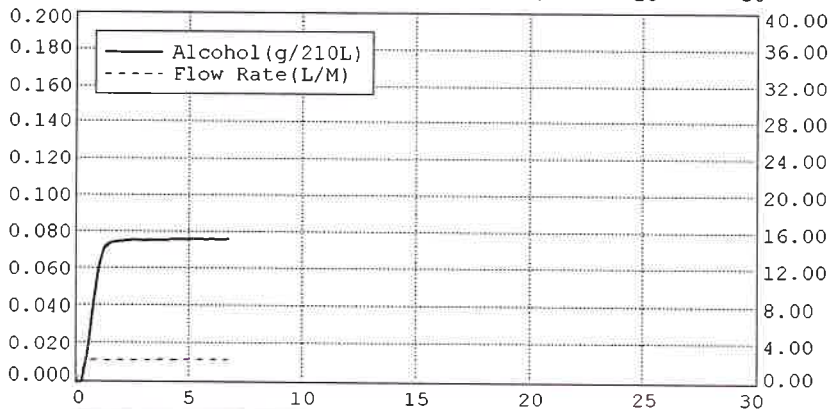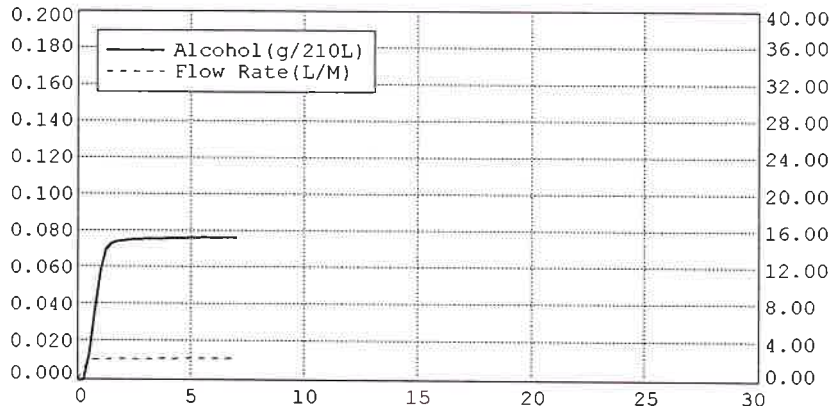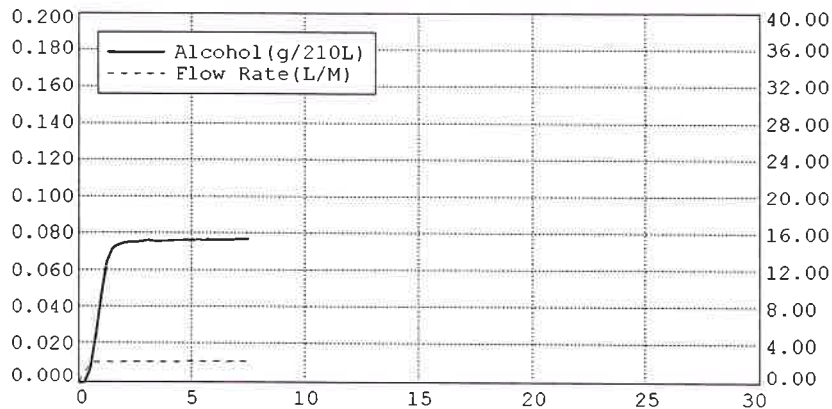

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025

Time: 12:33:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100

TARGET AT 29.27: 0.098

LOT #: AG516101






EXPIRATION: 06/10/2027

TANK PRESSURE: 1189 psi

BLANK TEST	0.000	12:34
INTERNAL STANDARD	VERIFIED	12:35
EXTERNAL STANDARD	0.097	12:35
BLANK TEST	0.000	12:36
EXTERNAL STANDARD	0.097	12:36
BLANK TEST	0.000	12:37
EXTERNAL STANDARD	0.097	12:37
BLANK TEST	0.000	12:38
EXTERNAL STANDARD	0.096	12:38
BLANK TEST	0.000	12:39
EXTERNAL STANDARD	0.096	12:39
BLANK TEST	0.000	12:40

Average = 0.0966

Std Dev = 0.0005

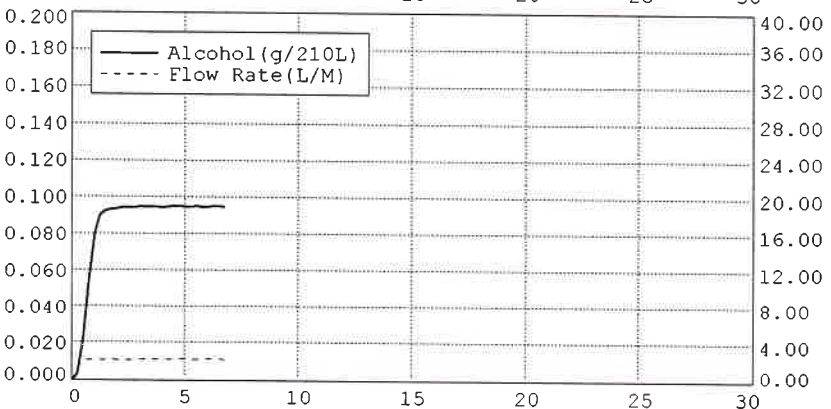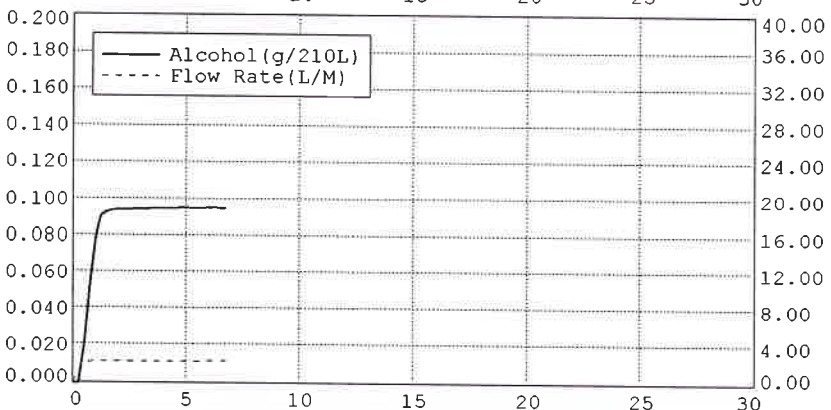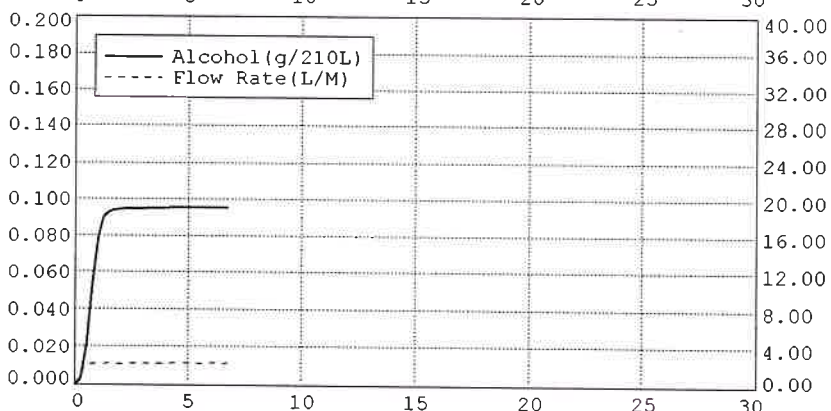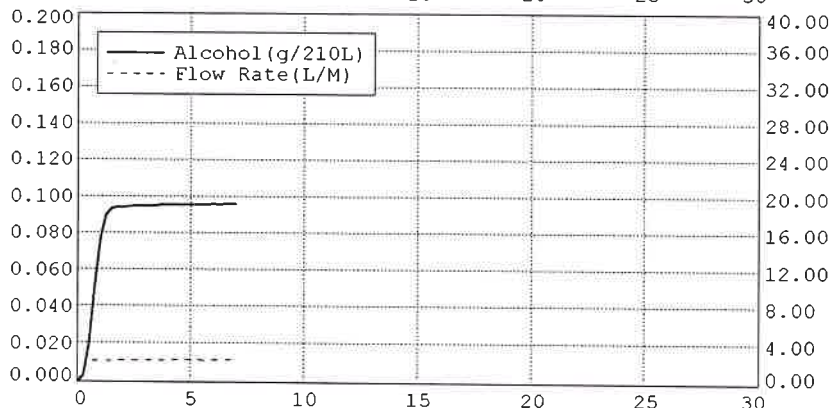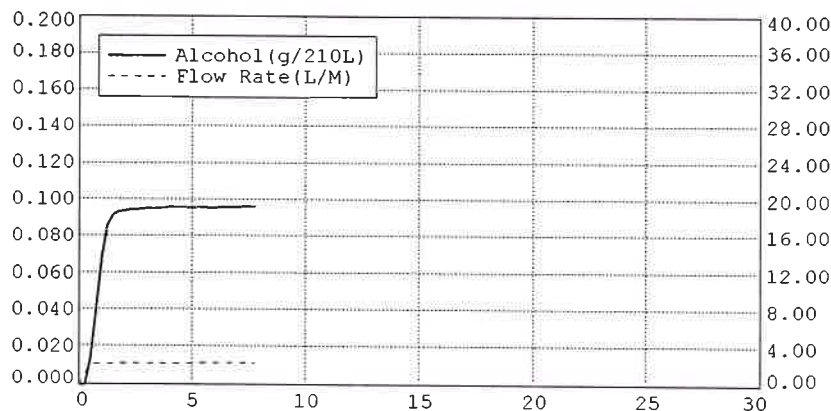

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100687






Date: 12/08/2025
Time: 12:43:36

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.28: 0.147
LOT #: AG515604
EXPIRATION: 06/05/2027
TANK PRESSURE: 700 psi

BLANK TEST	0.000	12:45
INTERNAL STANDARD	VERIFIED	12:45
EXTERNAL STANDARD	0.145	12:45
BLANK TEST	0.000	12:46
EXTERNAL STANDARD	0.144	12:46
BLANK TEST	0.000	12:47
EXTERNAL STANDARD	0.145	12:47
BLANK TEST	0.000	12:48
EXTERNAL STANDARD	0.145	12:48
BLANK TEST	0.000	12:49
EXTERNAL STANDARD	0.145	12:49
BLANK TEST	0.000	12:50

Average = 0.1448
Std Dev = 0.0004

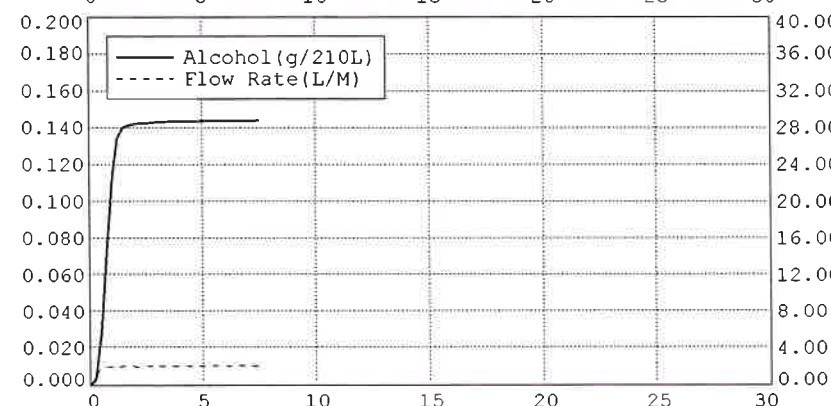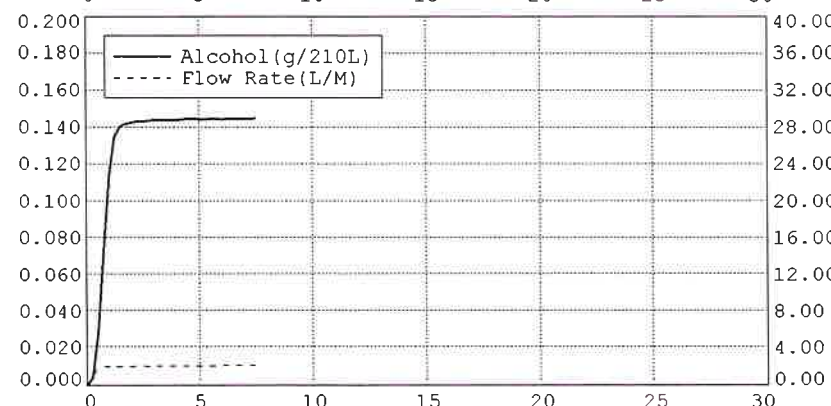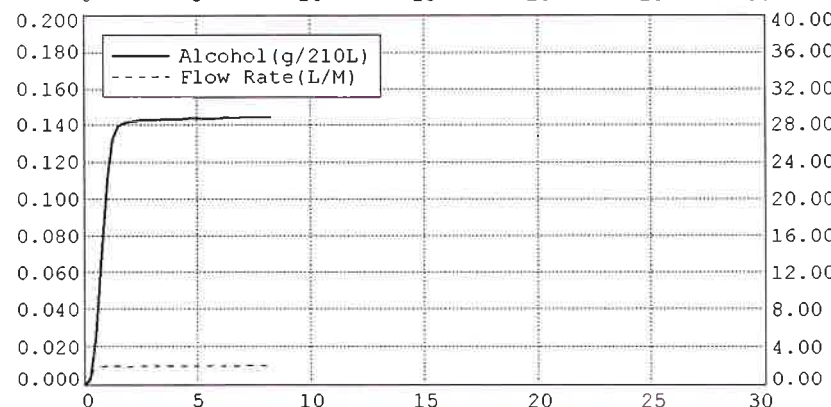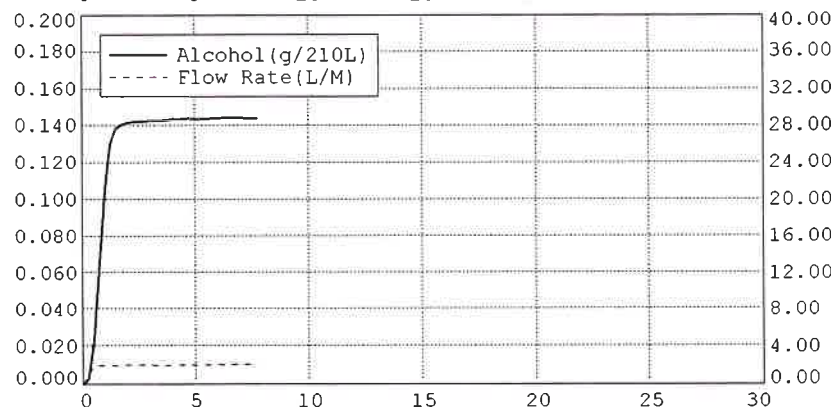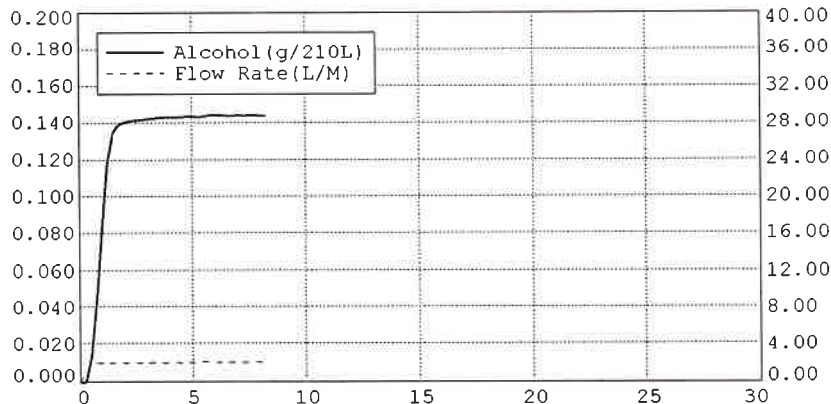

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100687






Date: 12/08/2025
Time: 12:56:24

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.28: 0.294
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 199 psi

BLANK TEST	0.000	12:57
INTERNAL STANDARD	VERIFIED	12:57
EXTERNAL STANDARD	0.291	12:58
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.290	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.291	13:00
BLANK TEST	0.000	13:01
EXTERNAL STANDARD	0.290	13:01
BLANK TEST	0.000	13:02
EXTERNAL STANDARD	0.290	13:02
BLANK TEST	0.000	13:03

Average = 0.2904
Std Dev = 0.0005

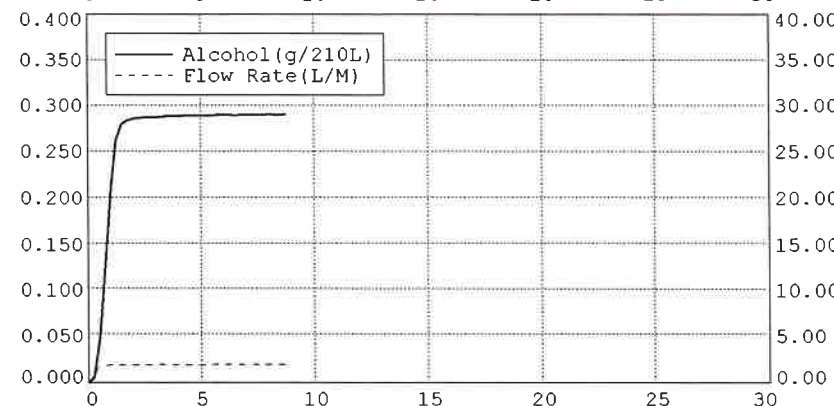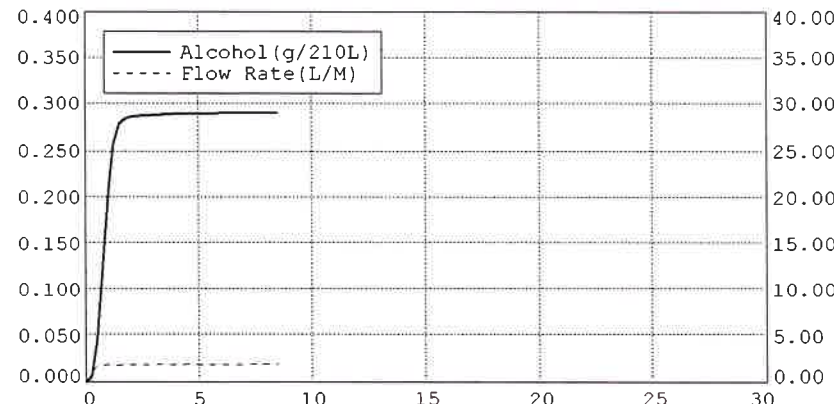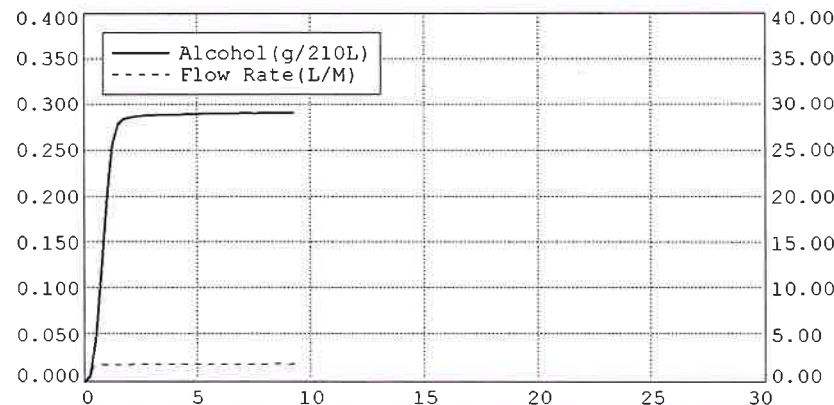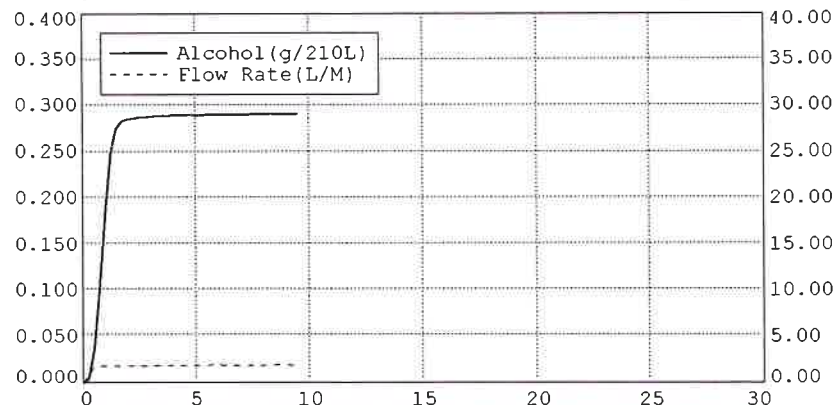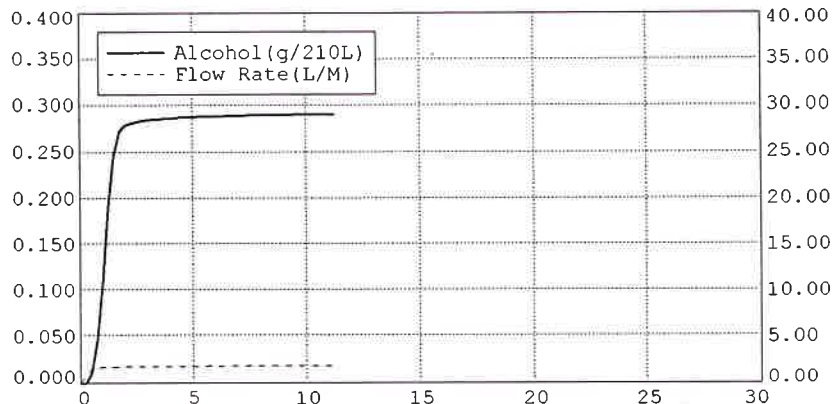

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 13:08:47

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.28: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:10
BLANK TEST	0.000	13:10
INTERNAL STANDARD	VERIFIED	13:10
EXTERNAL STANDARD	0.079	13:10
BLANK TEST	0.000	13:11
SUBJECT SAMPLE	INCOMPLETE	13:13

[Handwritten signature]

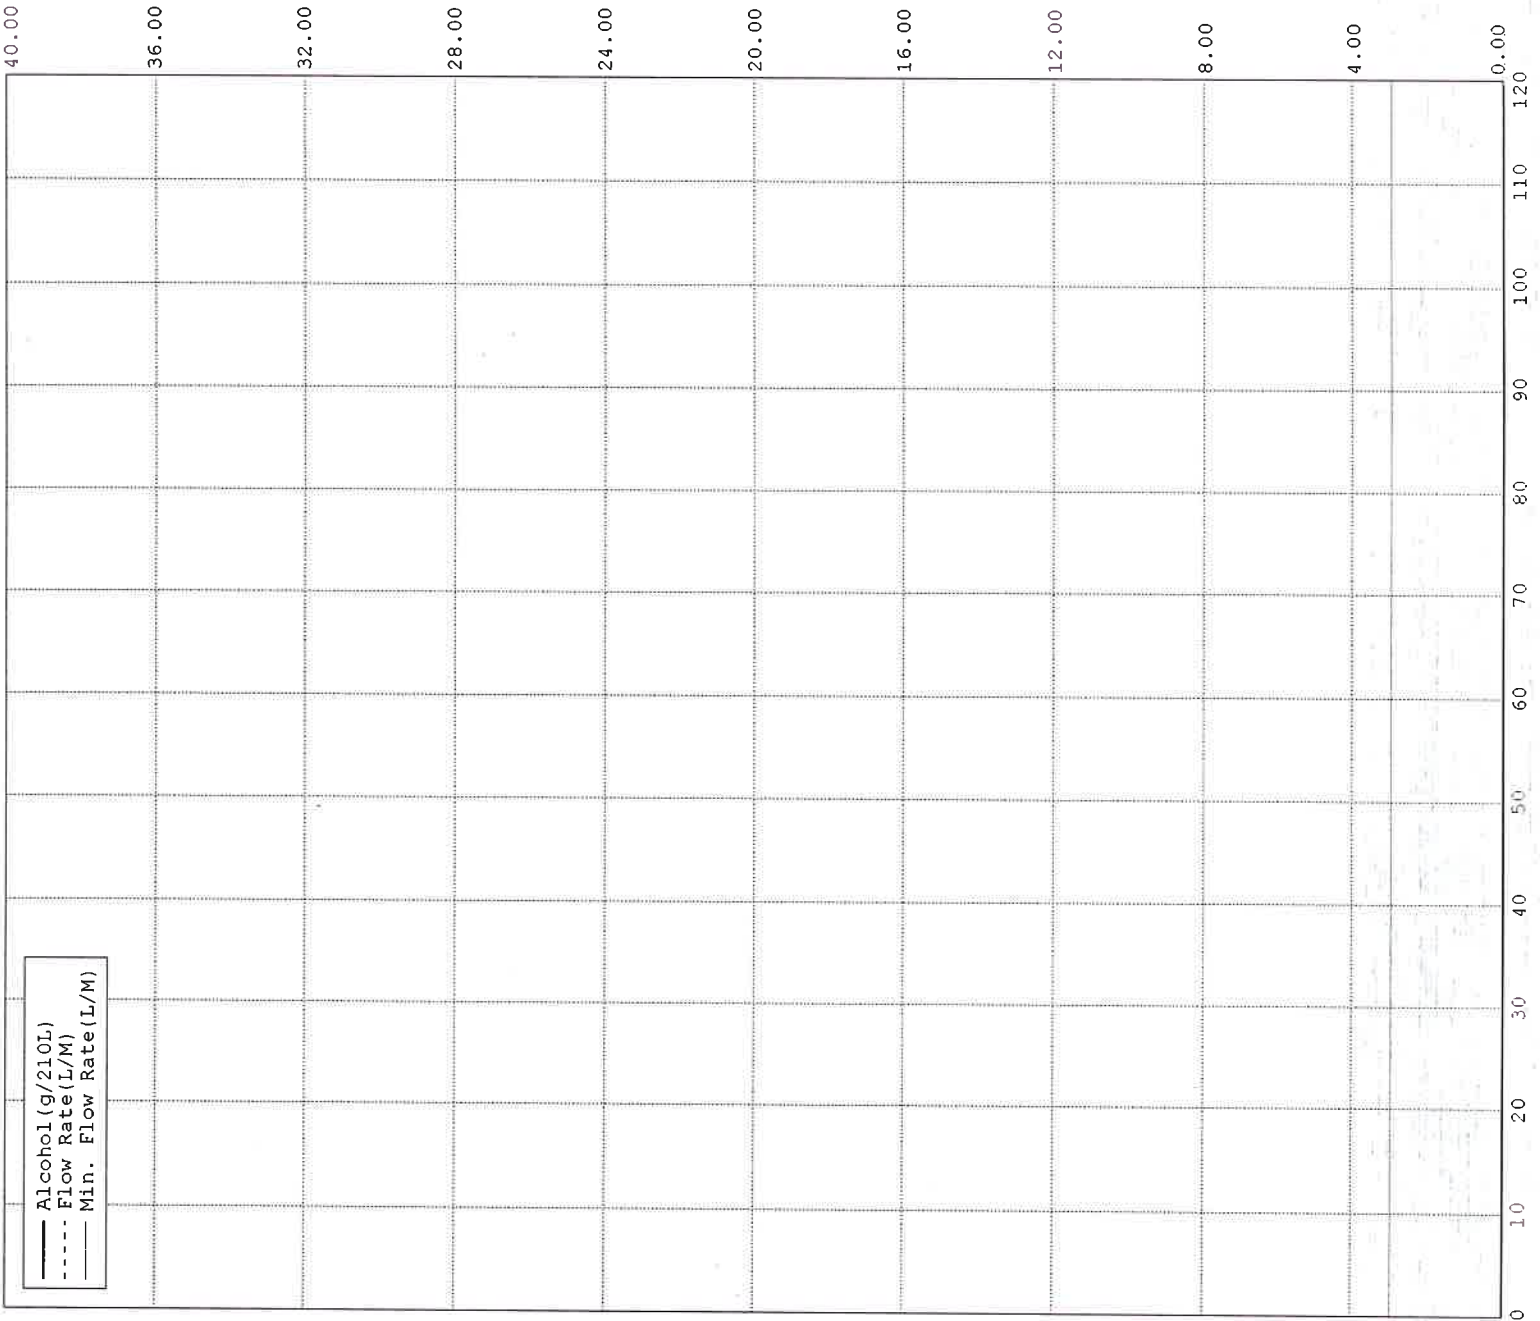

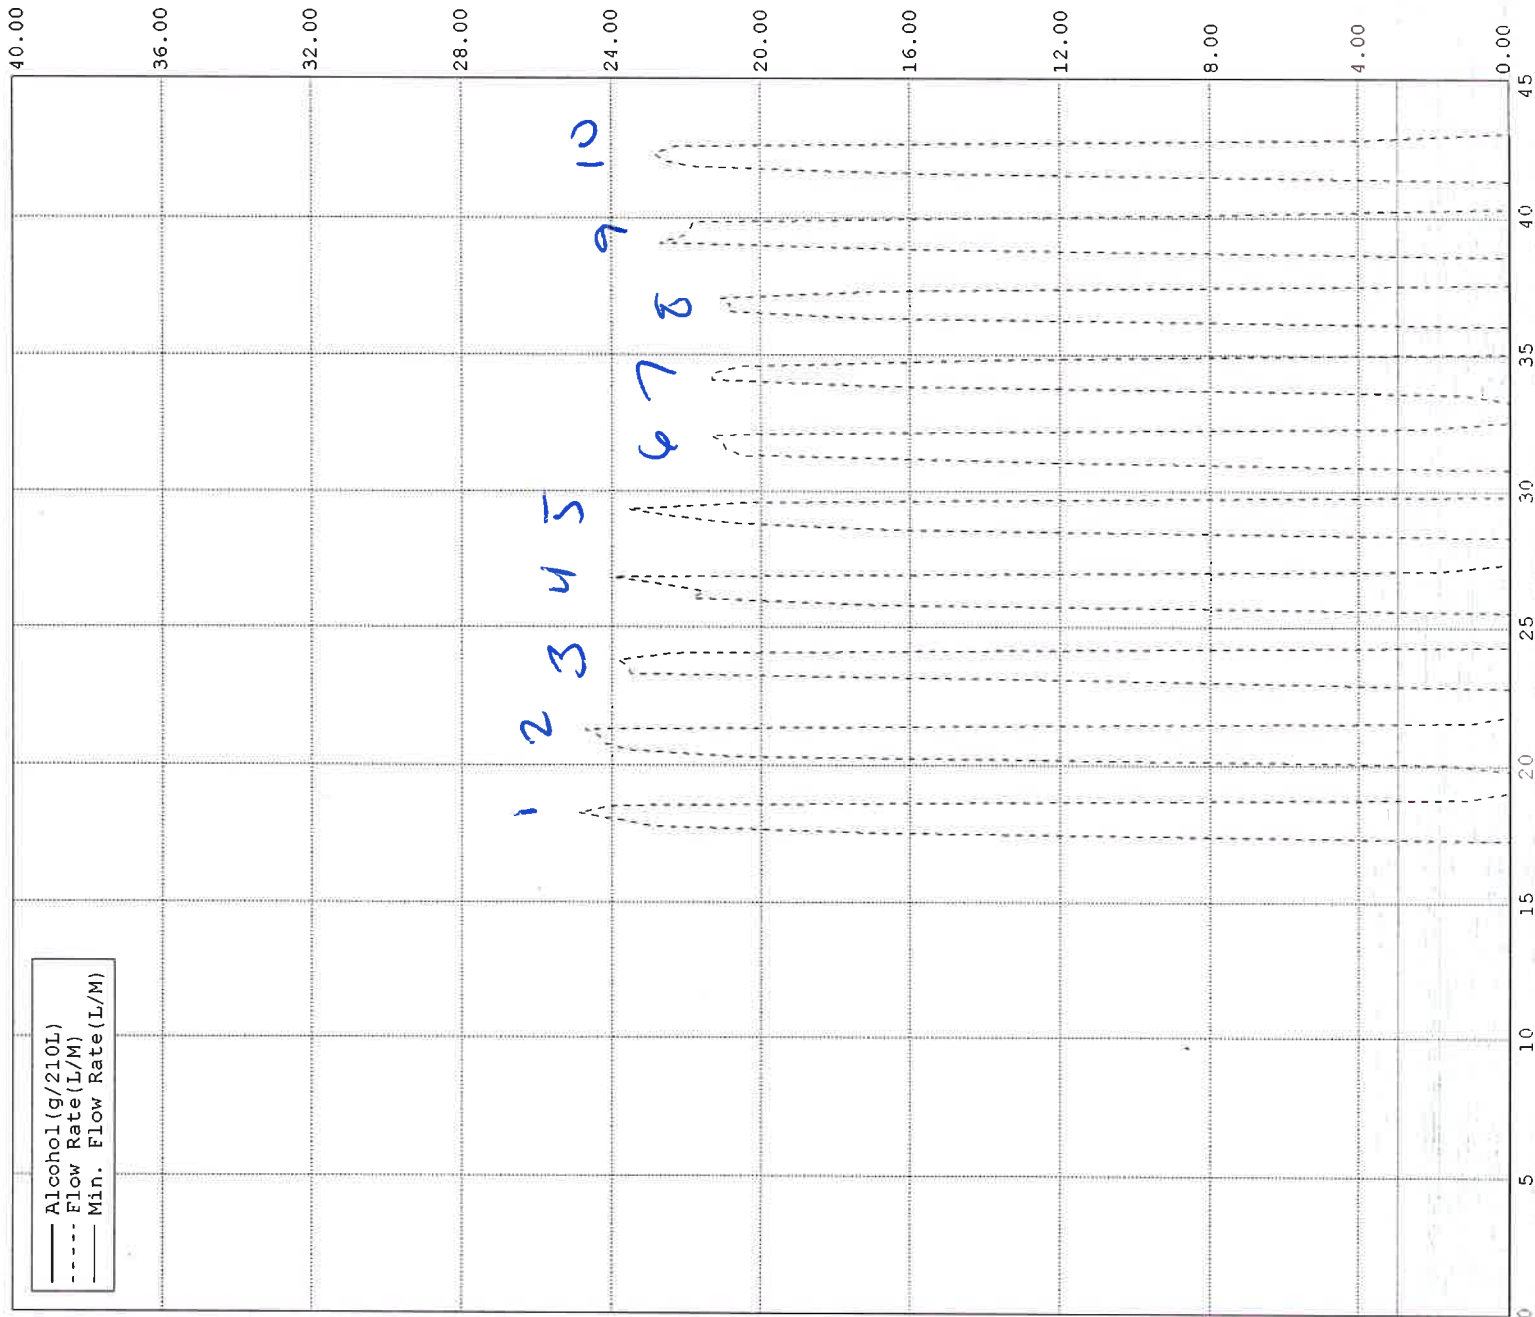

SUBJECT TEST	
Alaska Department of Public Safety DATA MASTER dmt: 100687	
Date: 12/08/2025 Time: 13:16:08	
SUBJECT NAME: TEST TEST LICENSE #: XXXX	
OPERATOR NAME: CARLIE GLAISTER OPERATOR'S #: 10436	
DEPT/AGENCY: MAX ATTEMPTS EXCEEDED CASE/REPORT: XXXX TEST TYPE: TEST	
EXTERNAL STANDARD INFORMATION NOMINAL: 0.080 TARGET AT 29.28: 0.078 LOT #: AG335202 EXPIRATION: 12/18/2025	
DIAGNOSTIC CHECK BLANK TEST INTERNAL STANDARD EXTERNAL STANDARD BLANK TEST SUBJECT SAMPLE	PASSED 0.000 VERIFIED 0.079 0.000 XXX 13:17 13:17 13:17 13:18 13:19 13:19
Maximum Attempts Exceeded	

006

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100687

Date: 12/08/2025

Time: 14:10:16

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INVALID

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.26: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 14:11


0.000 14:11

VERIFIED 14:11

0.079 14:11

0.000 14:12

INVALID 14:13

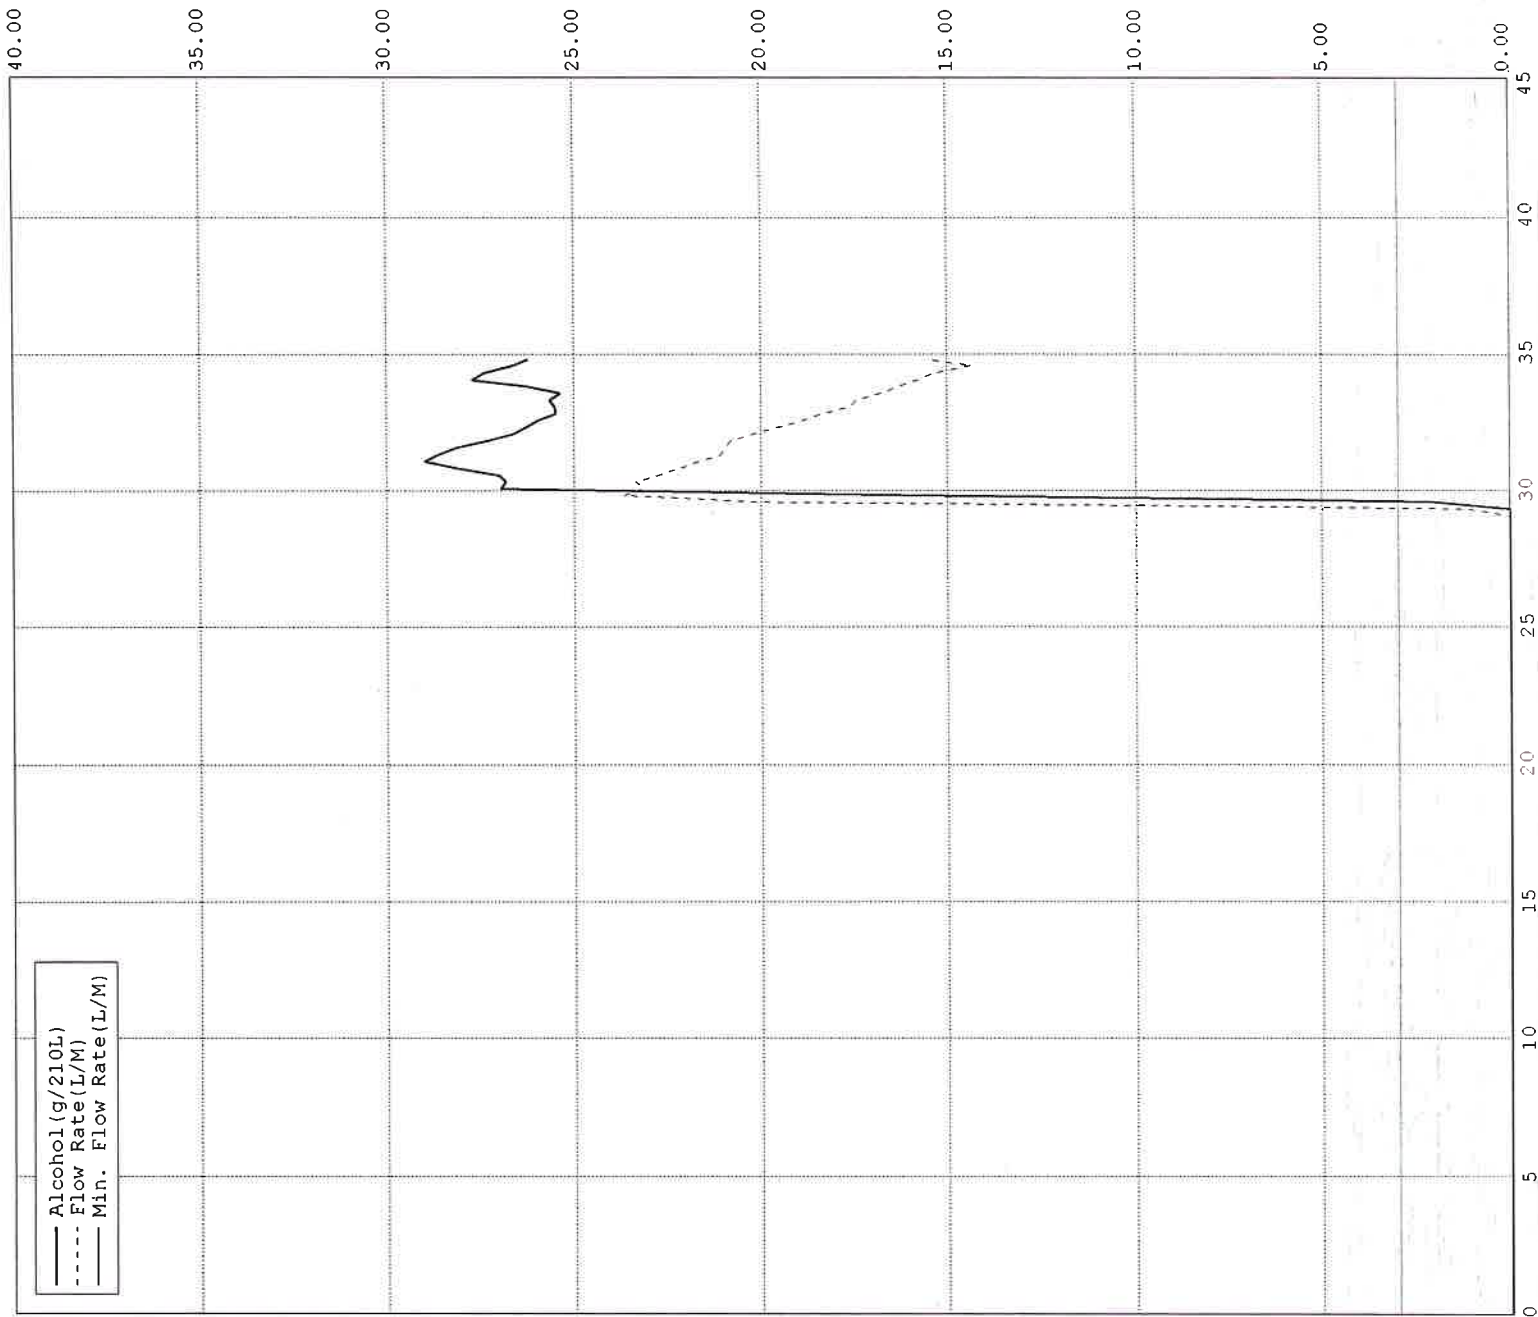

URG

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 14:15:44

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
RFI
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.26: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 14:17
BLANK TEST 0.000 14:17
INTERNAL STANDARD VERIFIED 14:17
EXTERNAL STANDARD 0.078 14:18
BLANK TEST 0.000 14:19


RFI DETECTED

CMS

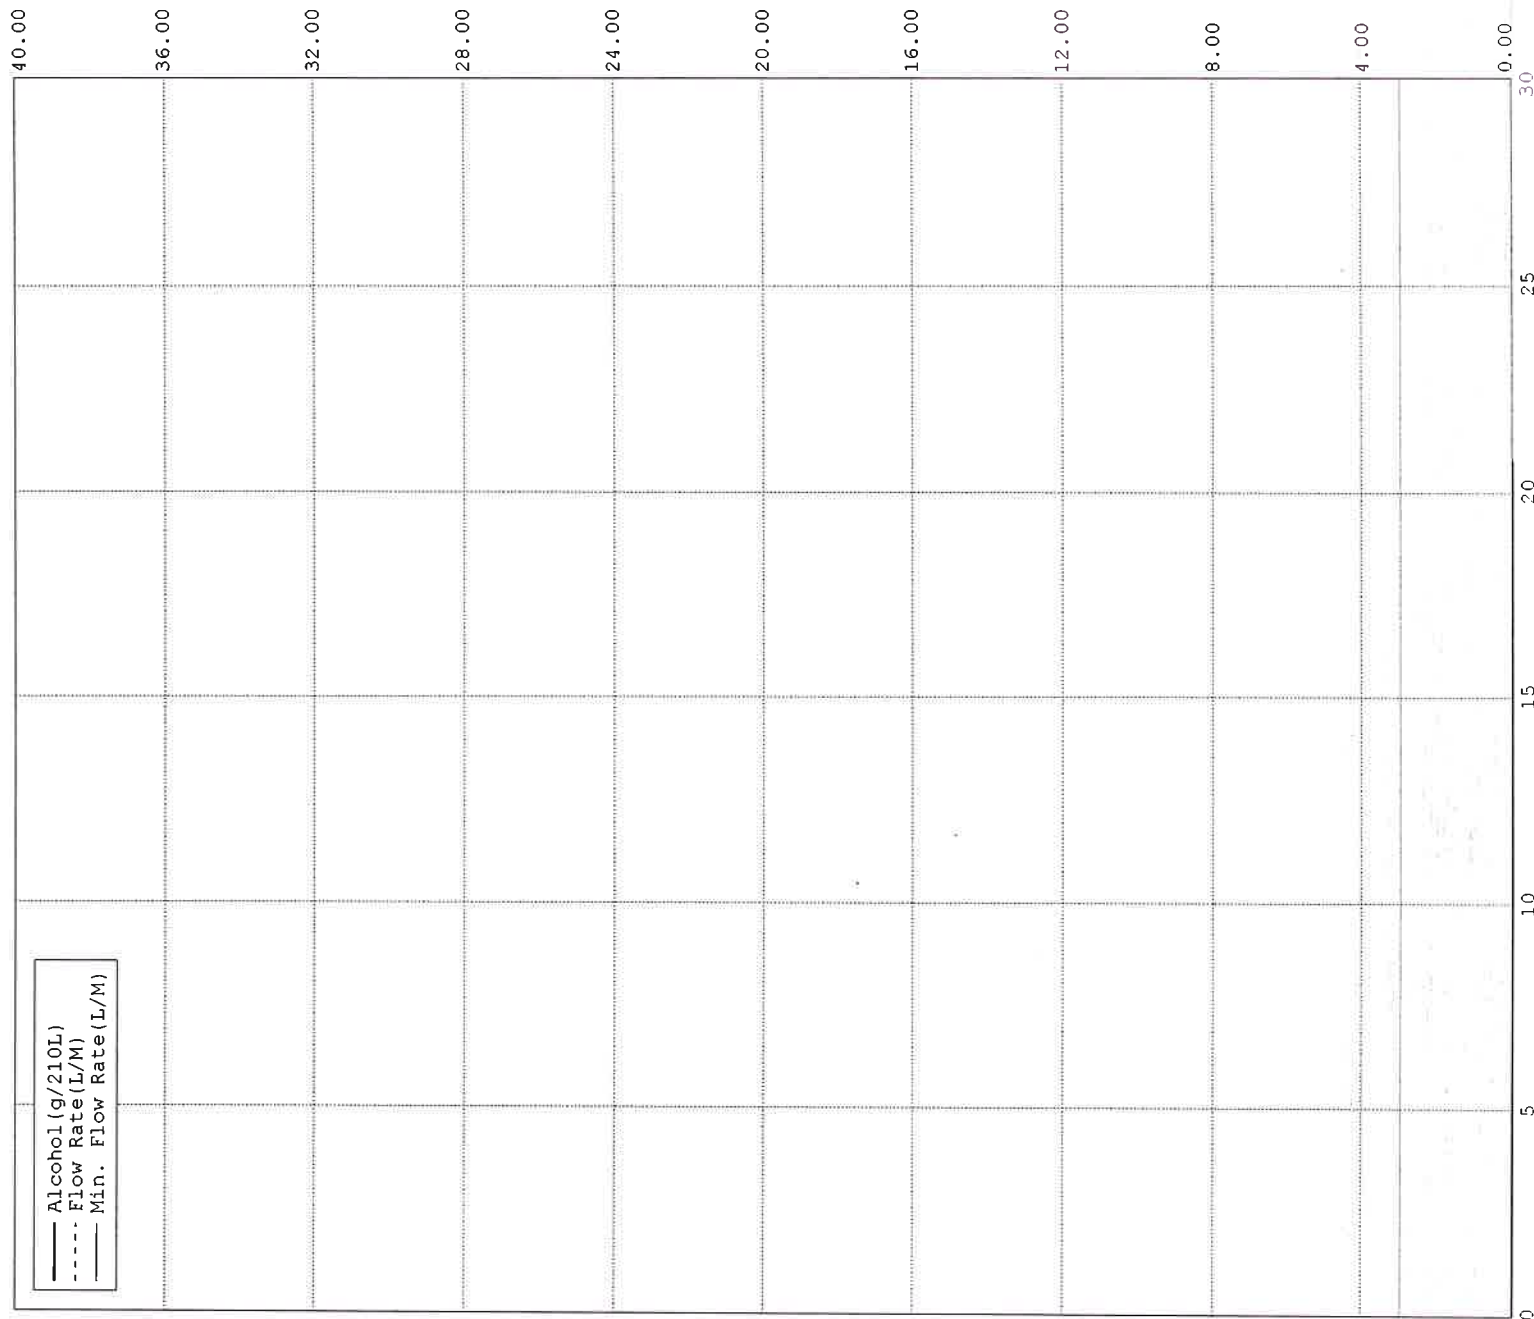

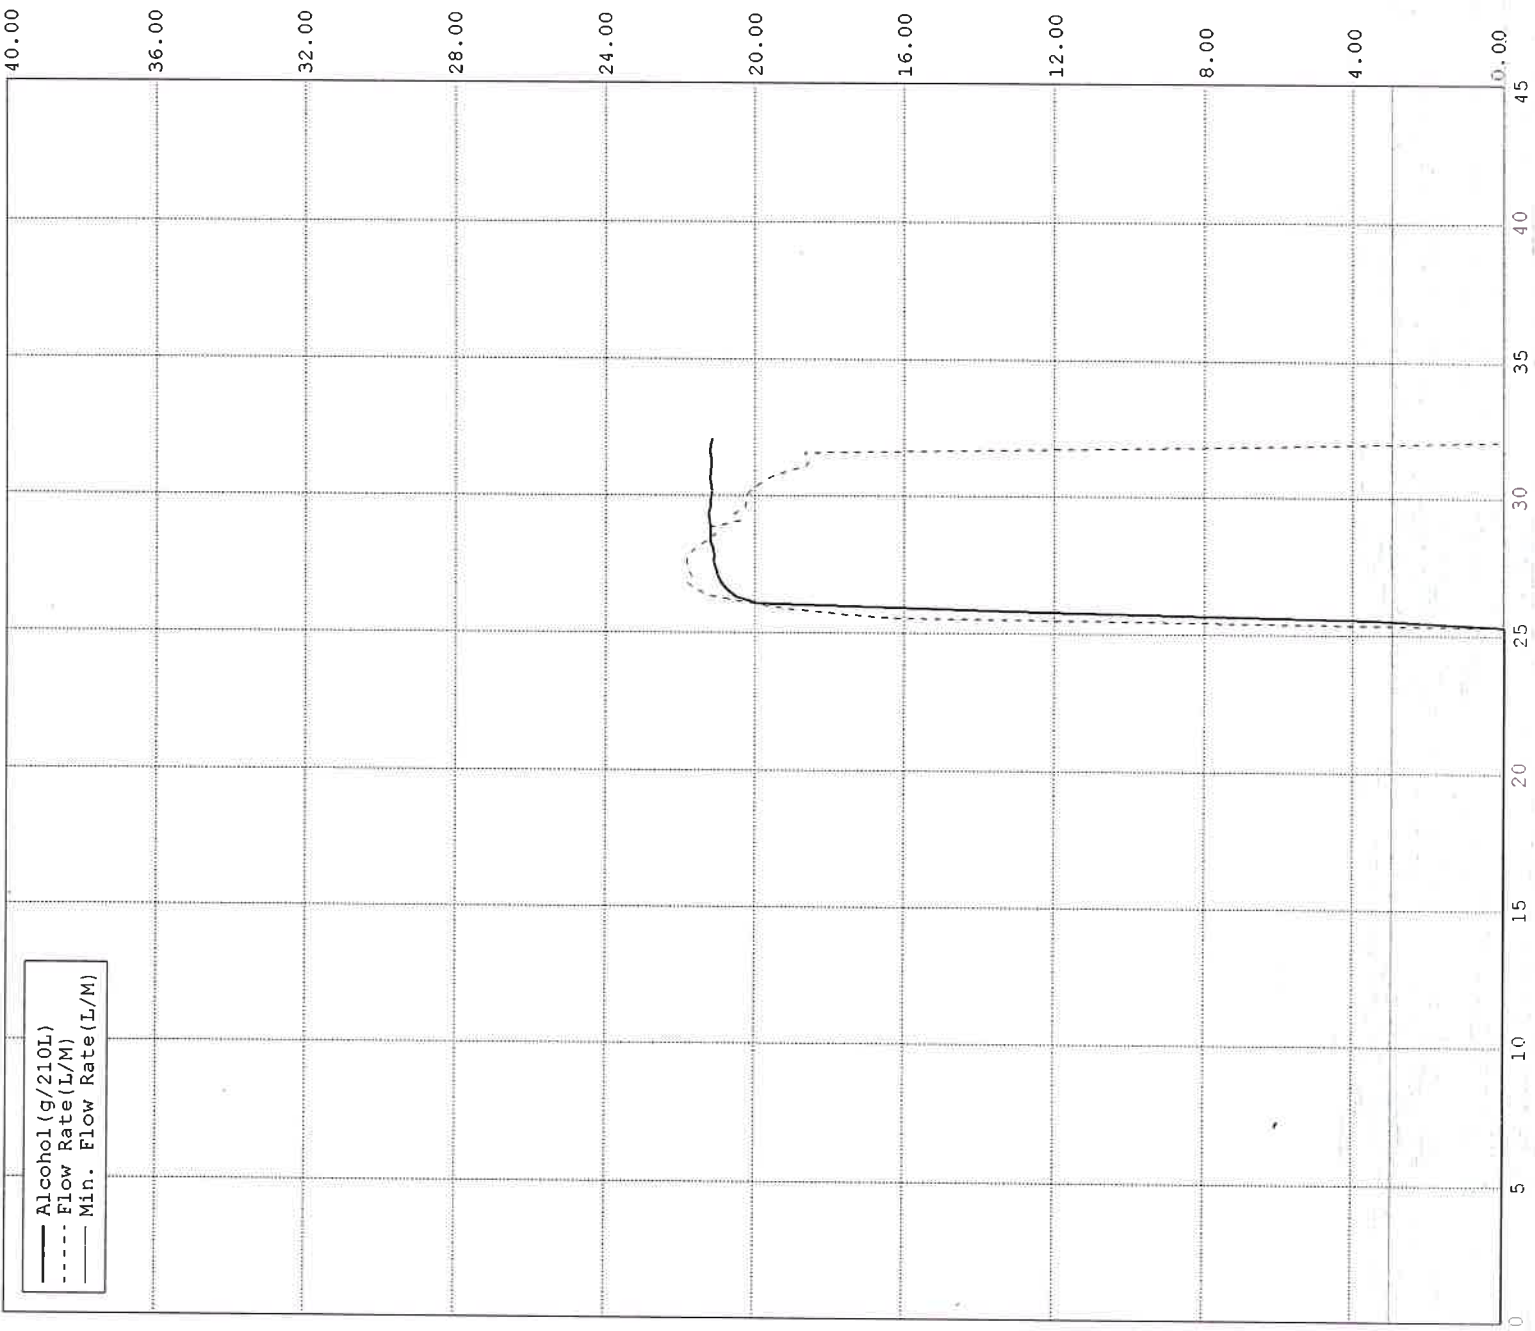

SUBJECT TEST	
Alaska Department of Public Safety DATAMASTER dmt: 100687	
Date: 12/08/2025 Time: 13:24:10	
SUBJECT NAME: TEST TEST LICENSE #: XXXX	
OPERATOR NAME: CARLIE GLAISTER OPERATOR'S #: 10436	
DEPT/AGENCY: INTERFERENCE - ACETONE CASE/REPORT: XXXX TEST TYPE: TEST	
EXTERNAL STANDARD INFORMATION NOMINAL: 0.080 TARGET AT 29.29: 0.078 LOT #: AG335202 EXPIRATION: 12/18/2025	
DIAGNOSTIC CHECK	PASSED 13:31
BLANK TEST	0.000 13:31
INTERNAL STANDARD	VERIFIED 13:31
Xq = 0.094 (0.19%)	
EXTERNAL STANDARD	0.079 13:31
X[1] = 0.0789 (-0.0009) (0.0024)	
BLANK TEST	0.000 13:32
SUBJECT SAMPLE	XXX 13:33
X[1] = 0.1057 (-0.0188) (0.0006)	
Interference Detected	
Filter 2 Avg: -0.0009	
Filter 3 Avg: 0.0027	
QWB 12/8/25	
OK	

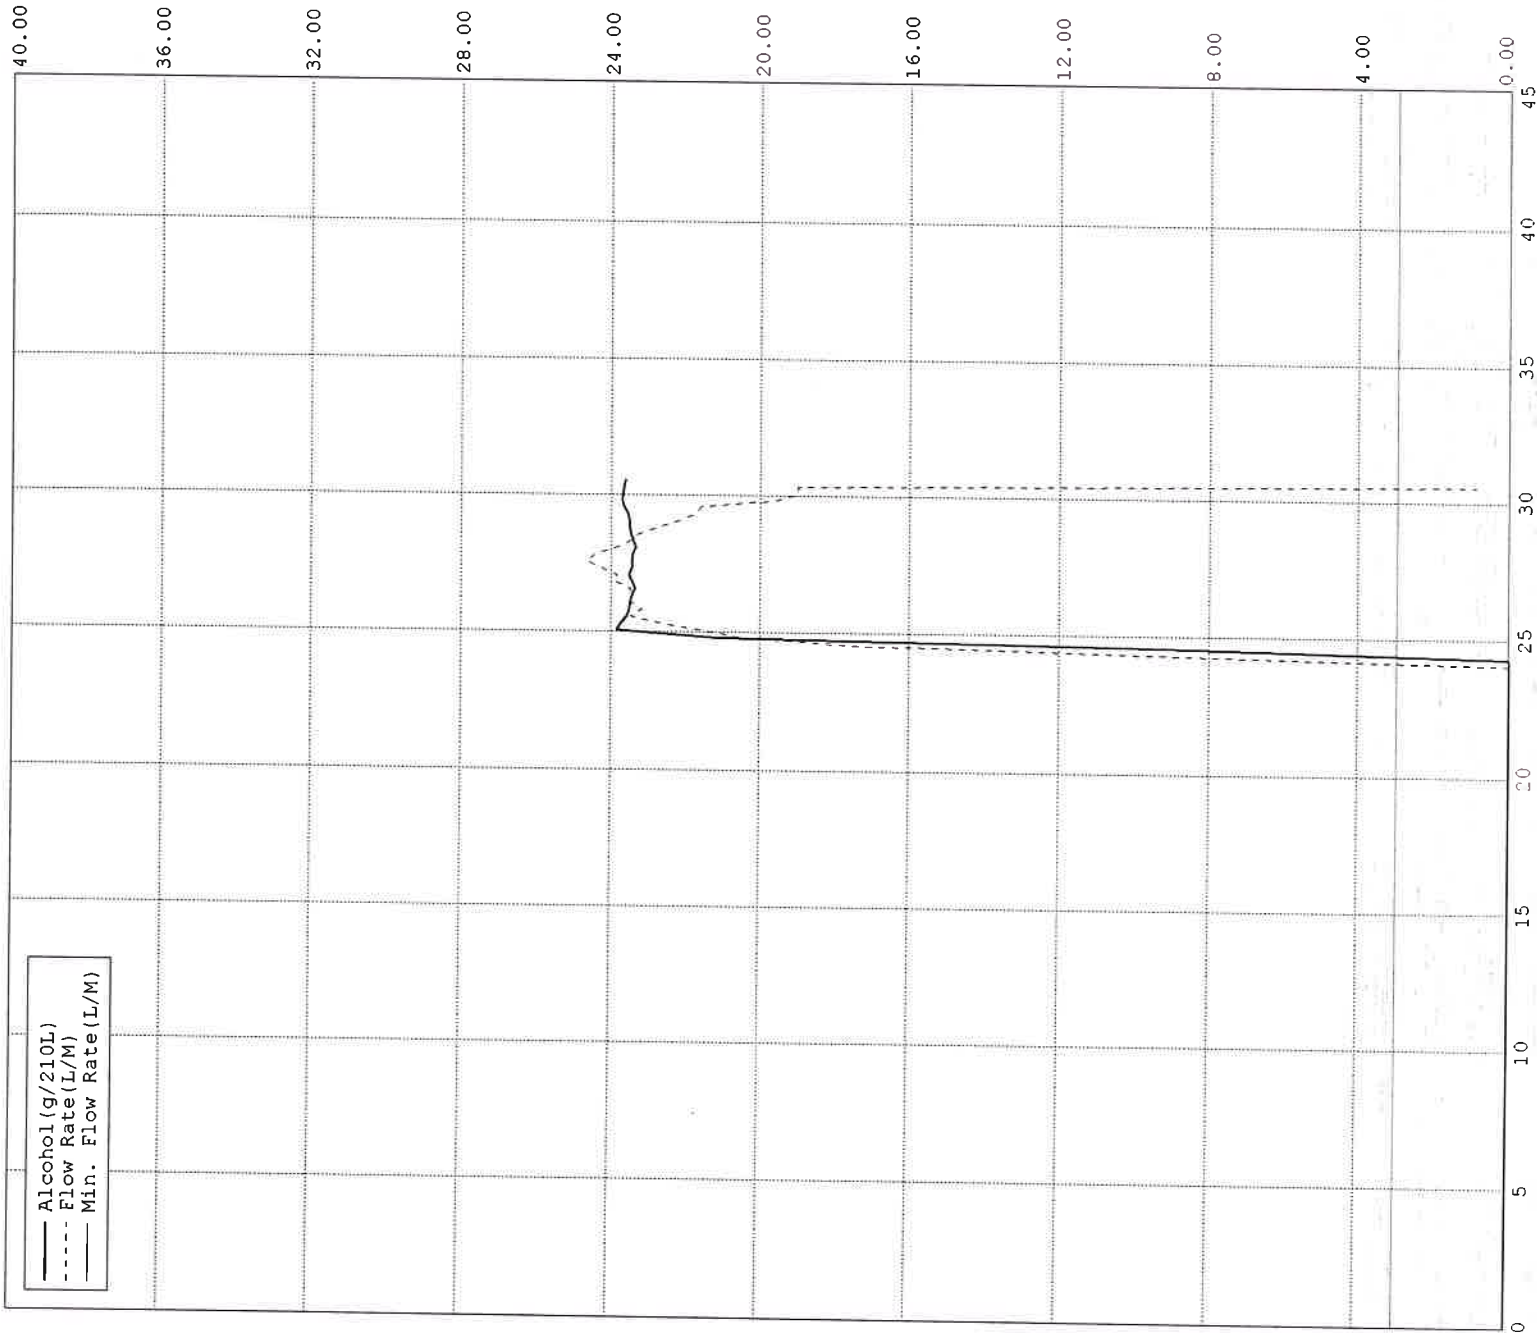

SUBJECT TEST																												
----- Alaska Department of Public Safety DATA MASTER dmt: 100687 ----- Date: 12/08/2025 Time: 13:36:17 SUBJECT NAME: TEST TEST LICENSE #: XXXX OPERATOR NAME: CARLIE GLAISTER OPERATOR'S #: 10436 DEPT/AGENCY: INTERFERENCE - IPA CASE/REPORT: XXXX TEST TYPE: TEST EXTERNAL STANDARD INFORMATION NOMINAL: 0.080 TARGET AT 29.28: 0.078 LOT #: AG335202 EXPIRATION: 12/18/2025 <table border="0"> <tr> <td>DIAGNOSTIC CHECK</td> <td>PASSED</td> <td>13:37</td> </tr> <tr> <td>BLANK TEST</td> <td>0.000</td> <td>13:37</td> </tr> <tr> <td>INTERNAL STANDARD</td> <td>VERIFIED</td> <td>13:37</td> </tr> <tr> <td colspan="3">$x_q = 0.094$ (0.65%)</td> </tr> <tr> <td>EXTERNAL STANDARD</td> <td>0.079</td> <td>13:37</td> </tr> <tr> <td>$x[1] = 0.0786$ (-0.0006)</td> <td>(0.0031)</td> <td></td> </tr> <tr> <td>BLANK TEST</td> <td>0.000</td> <td>13:38</td> </tr> <tr> <td>SUBJECT SAMPLE</td> <td>XXX</td> <td>13:39</td> </tr> <tr> <td>$x[1] = 0.1174$ (-0.0220)</td> <td>(0.0025)</td> <td></td> </tr> </table> Interference Detected		DIAGNOSTIC CHECK	PASSED	13:37	BLANK TEST	0.000	13:37	INTERNAL STANDARD	VERIFIED	13:37	$x_q = 0.094$ (0.65%)			EXTERNAL STANDARD	0.079	13:37	$x[1] = 0.0786$ (-0.0006)	(0.0031)		BLANK TEST	0.000	13:38	SUBJECT SAMPLE	XXX	13:39	$x[1] = 0.1174$ (-0.0220)	(0.0025)	
DIAGNOSTIC CHECK	PASSED	13:37																										
BLANK TEST	0.000	13:37																										
INTERNAL STANDARD	VERIFIED	13:37																										
$x_q = 0.094$ (0.65%)																												
EXTERNAL STANDARD	0.079	13:37																										
$x[1] = 0.0786$ (-0.0006)	(0.0031)																											
BLANK TEST	0.000	13:38																										
SUBJECT SAMPLE	XXX	13:39																										
$x[1] = 0.1174$ (-0.0220)	(0.0025)																											

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100687

Date: 12/08/2025
Time: 13:42:07

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.27: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:43
BLANK TEST	0.000	13:43
INTERNAL STANDARD	VERIFIED	13:43
$X_q = 0.093$ (0.47%)		
EXTERNAL STANDARD	0.078	13:43
$X[1] = 0.0776$ (-0.0012) (0.0026)	0.000	13:44
BLANK TEST	0.000	13:44
SUBJECT SAMPLE (Vol=2.22L)	0.091	13:44
$X[1] = 0.0911$ (0.0008) (0.0010)	0.000	13:45
BLANK TEST	0.000	13:45
EXTERNAL STANDARD	0.078	13:46
$X[1] = 0.0776$ (-0.0009) (0.0027)	0.000	13:47
BLANK TEST	0.000	13:47

CMG

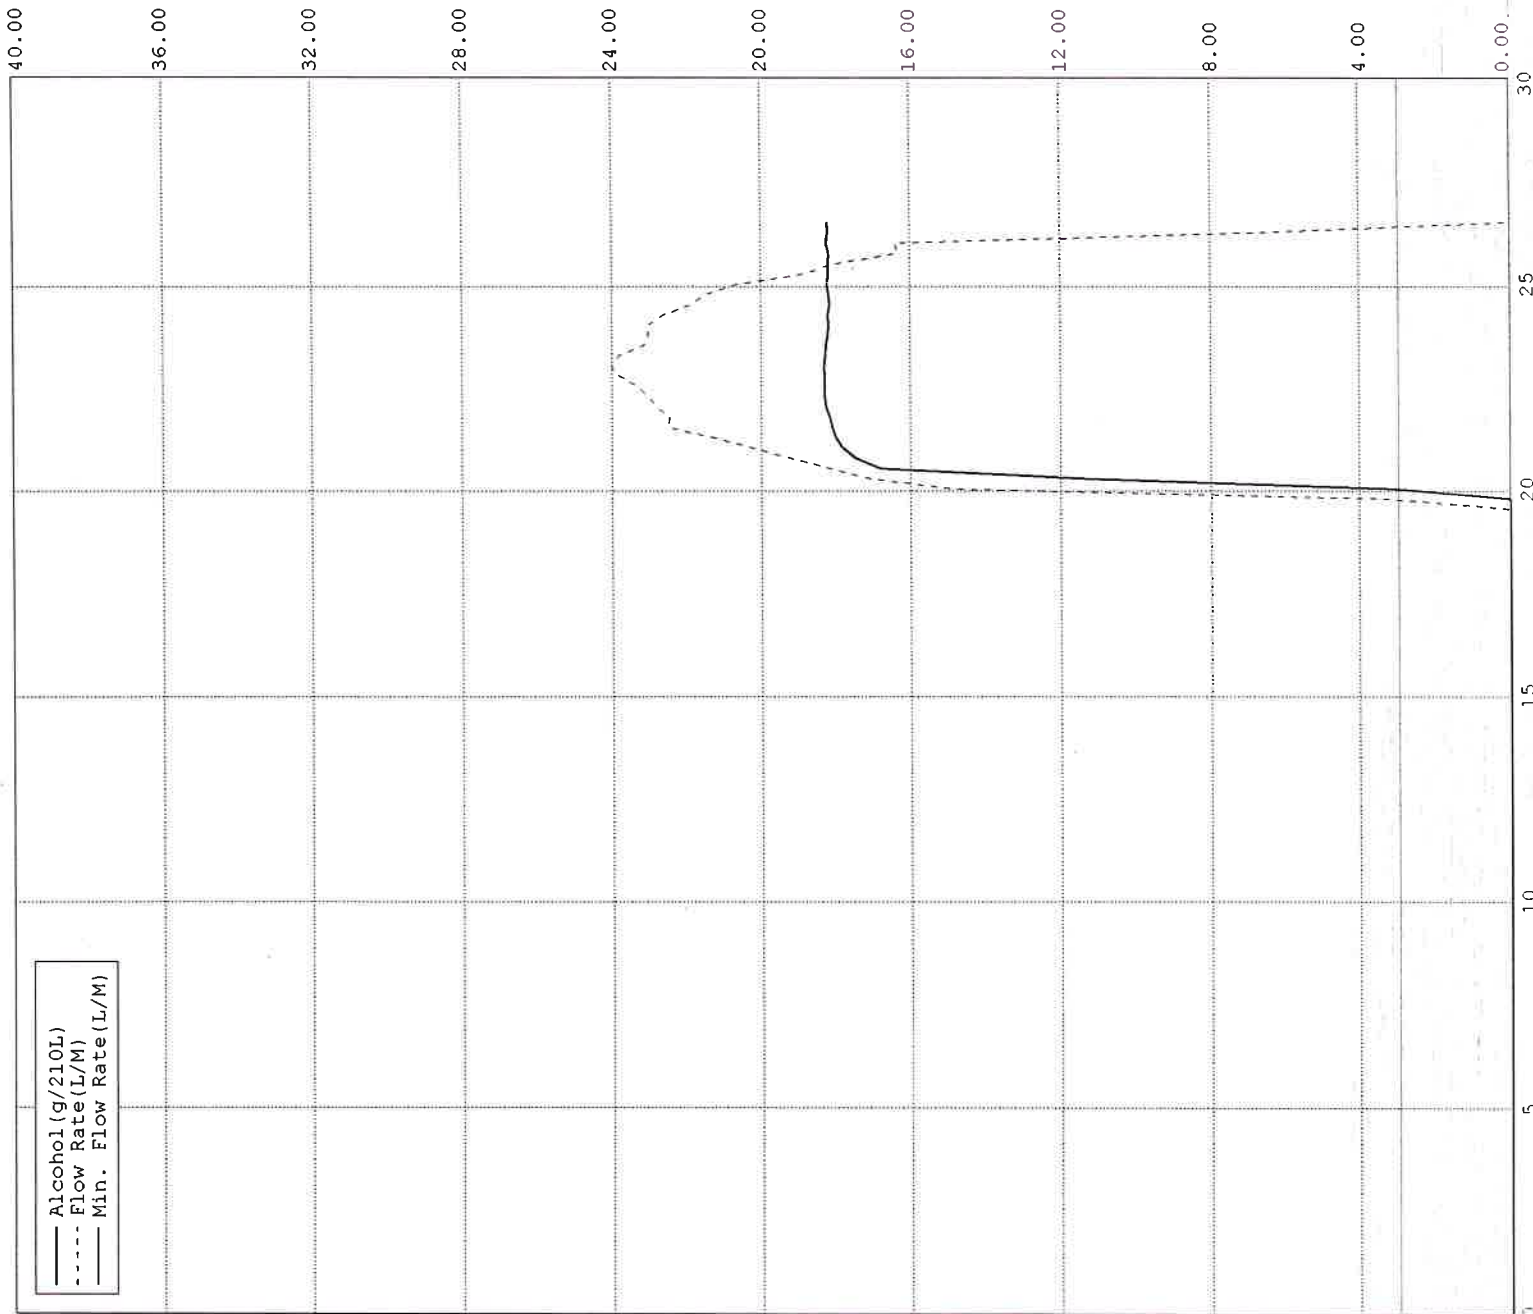

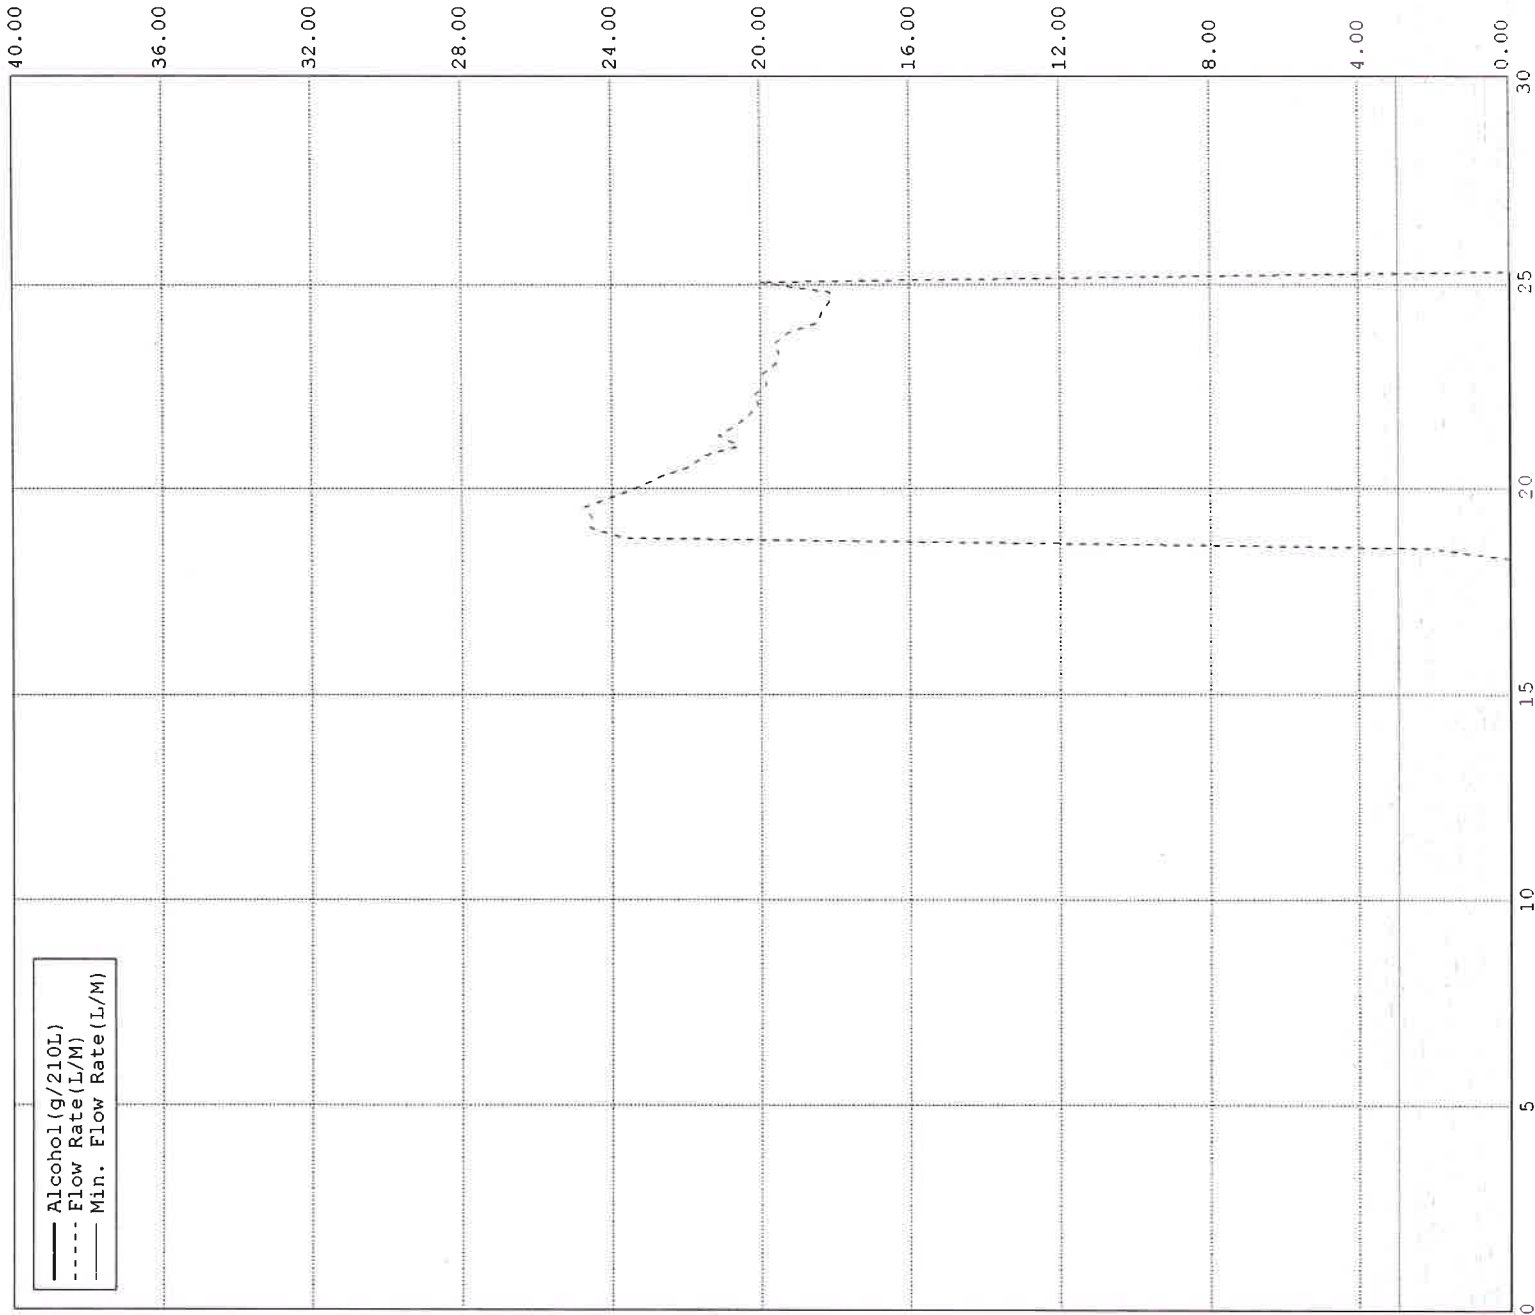

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100687

Date: 12/08/2025

Time: 14:46:33

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.26: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

PASSED

14:49

INTERNAL STANDARD

0.000

14:49

EXTERNAL STANDARD

0.077

14:50

BLANK TEST

0.000

14:51

SUBJECT SAMPLE (Vol=2.27L)

0.000

14:51

BLANK TEST

0.000

14:52

EXTERNAL STANDARD

0.079

14:52

BLANK TEST

0.000

14:53

CMA