




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory
4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100376

Report Issue Date: 06/12/2025
Date Received: 2025-05-19
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.021	0.021	0.020	0.021	0.021	0.021
0.080	0.079	AG335202	0.078	0.078	0.078	0.078	0.078	0.078
0.300	0.298	AG427706	0.297	0.296	0.296	0.296	0.297	0.296

As Found - Evaluation Analyst: Carlie Glaister
As Found Conditions - Barometric Pressure (inHg): 29.74 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 21
As-Found Lab Activity Date Range: 05/22/2025 - 05/22/2025

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.079	AG335202	0.077	0.077	0.077	0.077	0.077	0.077	+/- 0.004
0.100	0.098	AG333401	0.098	0.099	0.099	0.098	0.099	0.099	+/- 0.004
0.150	0.148	AG332004	0.145	0.144	0.145	0.145	0.145	0.145	+/- 0.006
0.300	0.295	AG427706	0.291	0.291	0.292	0.292	0.292	0.292	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.44 Barometer Used: VWR S/N 240680771 Temperature (C): 22.9 Relative Humidity (%): 29
As-Left Lab Activity Date Range: 06/04/2025 - 06/05/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 06/12/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 06/12/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100376 Analyst or Technician Name: Kaija Swisher

DataMaster DMT Calibration Start Date: 6/4/25

Diagnostic Test

☒ Perform Diagnostic Test (View Details)

☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

☒ Adjust Voltages (if needed)

- Lamp (2.60 V Maximum)
- Bias
- Cooler (2.00 V Maximum)
- Chopper Frequency
- Detector Voltage (-0.100V to 0.100V)

☒ Set RFI Sensitivity

☒ Adjust internal barometer reading to match NIST-traceable barometer

Barometer/Thermometer/Hygrometer S/N: 290680771

Calibration Due Date: 9/10/26

☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed

☒ Print Technician Screen

☒ Print "Cal Factors"

Minimum Volume Test

☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.44 ^{KS 6/4/25} Temperature(C) 22.7 Relative Humidity(%) 29

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

☒ Incomplete

☒ Invalid

☒ Maximum Attempts Exceeded

☒ Radio Frequency Interference (RFI)

☒ Interference (Volatiles) - *Print with View Details*

• 1. Acetone Reagent Lot Number: 20250603KS Expiration Date: 7/27/25

Simulator S/N: SD1200 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250603KS Expiration Date: 9/3/25

Simulator S/N: SD1198 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 9/3/25

Simulator S/N: SD1199 Thermometer Verification Performed? ☒

0.100 solution exp: 9/20/2025
KS 06/05/2025

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/25

Administrative

☒ Verify Stylus Calibration

☒ Reset Options

☒ Clear Memory

☒ Verification of Calibration (VOC)

☒ Perform Non-Drinking Subject Test

☒ Upload Instrument

☒ Remove Dry Gas Tank Before Shutdown

☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/4/25

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 6/5/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100376

Date: 06/04/2025
Time: 11:28:09

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C (44.0°C - 52.0°C)	PASSED
Breath Tube = 48.1°C (38.0°C - 50.0°C)	PASSED

SETTINGS

Lamp Voltage = 1.64 V (0.98 V - 2.30 V)	PASSED
Cooler Voltage = 1.66 V (1.00 V - 2.32 V)	PASSED
Bias Voltage = 80 V (48 V - 112 V)	PASSED
Chopper Freq = 536 Hz (475 Hz - 575 Hz)	PASSED
Barometer = 29.4 in	

PUMP INFO

Flow Rate = 3.936 L/M (3.500 L/M - 6.500 L/M)	PASSED
--	--------

DETECTOR INFO

PUMP ON (0.002 V <= 0.010 V)	PASSED
PUMP OFF (0.002 V <= 0.010 V)	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.077 1.25% (0.00% - 4.00%)	PASSED
----------------------------------	--------

Technician Screen

DATAMASTER dmt: 100376

Date: 06/04/2025

Time: 11:32 AM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 47.4°C

Current Barometer 29.4 in

Volume (Ltr) 1.47

Settings

Lamp: 1.67 V

Bias: 80 V

Cooler: 1.66 V

Chopper: 535 Hz

Voltages (V)

Flow: 1.06 V

Detector: -0.050 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100376

Date: 12/29/2021
Time: 12:08:56

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.974499 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0064 0.0010 <= b2 < 0.0100
b3 = 0.0001 0.0000 <= b3 < 0.0040
Xq = 0.0762 0.0500 <= Xq < 0.2000
a21 = 1.177238 1.050 <= a21 < 1.300
a31 = 0.378082 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100376

Date: 06/04/2025
Time: 11:35:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAJIA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MIN VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.45: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:36
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	VERIFIED	11:37
BLANK TEST	0.076	11:37
BLANK TEST	0.000	11:38
SUBJECT SAMPLE (Vol=1.51L)	0.000	11:39
BLANK TEST	0.000	11:40
EXTERNAL STANDARD	0.077	11:40
BLANK TEST	0.000	11:41

KS

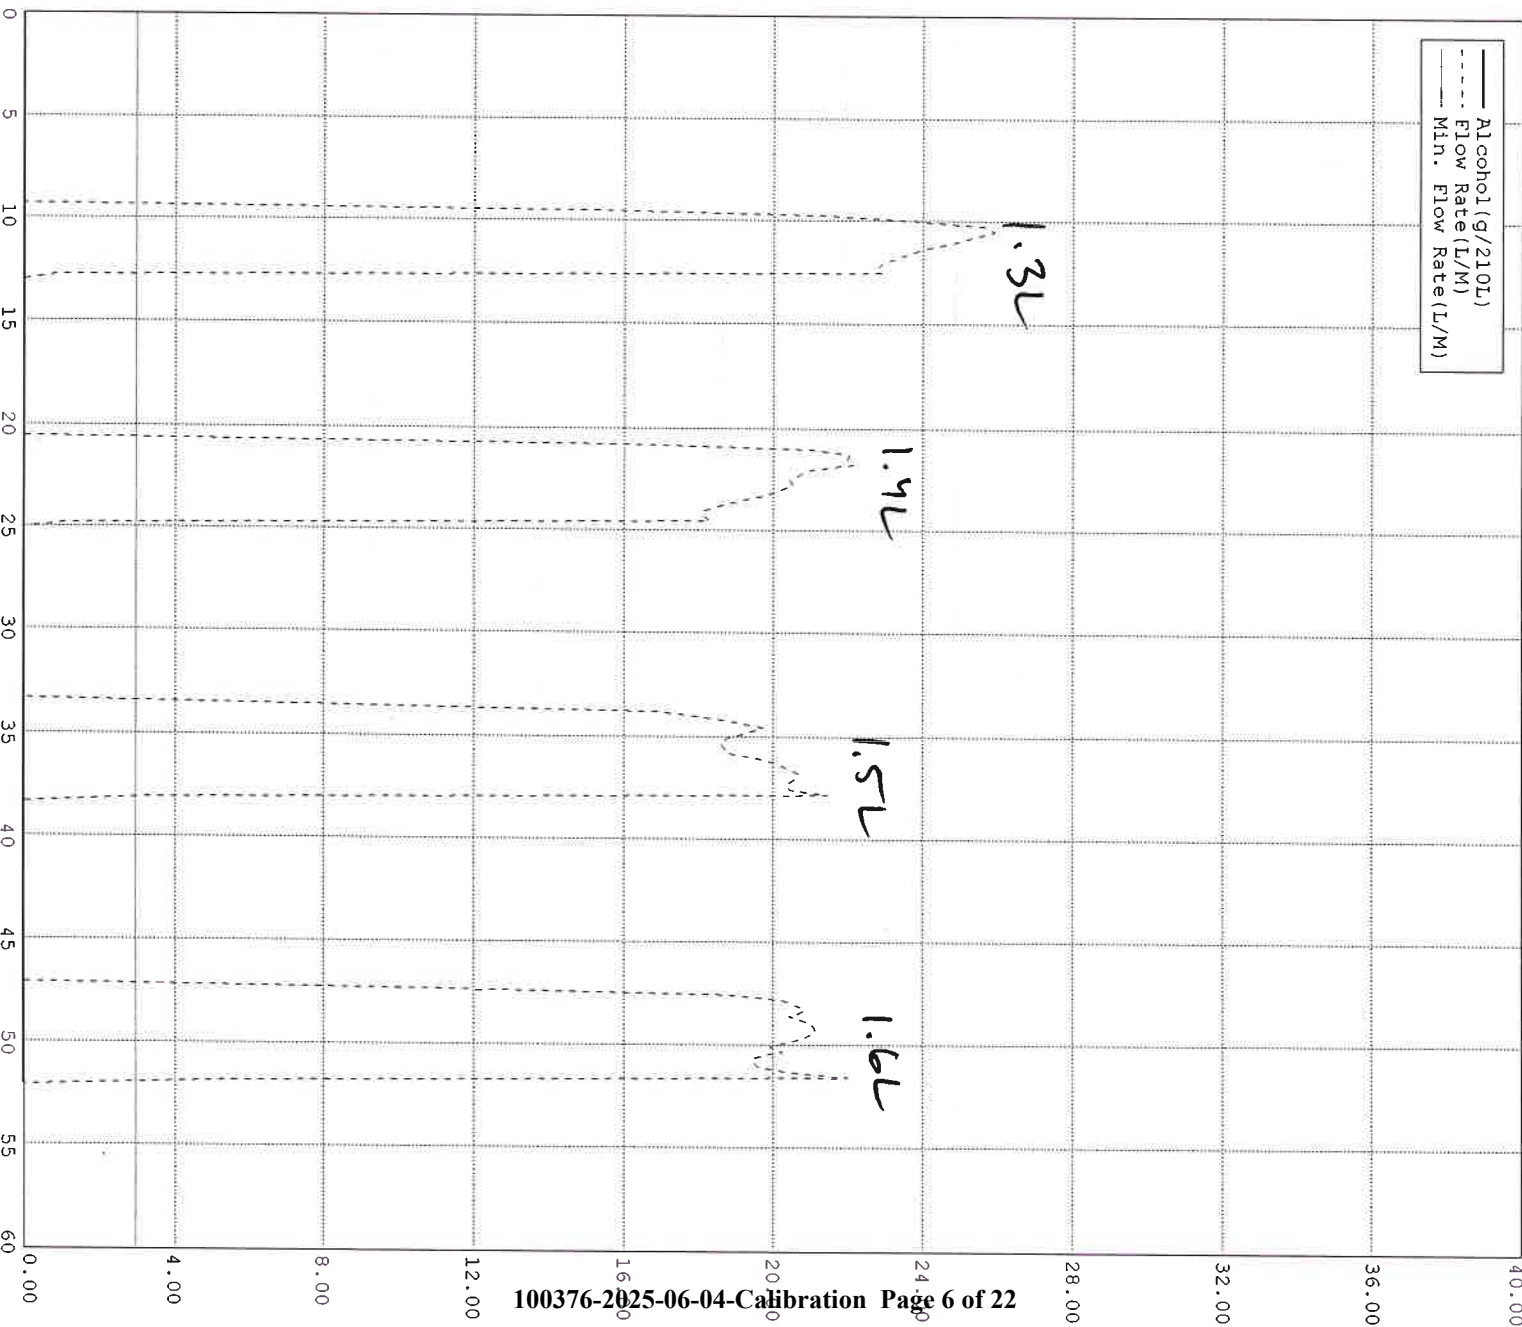


LINEARITY CHECK

Alaska Department of Public Safety
 DATAMASTER dmt: 100376

Date: 06/04/2025
 Time: 11:43:09

SUPERVISOR NAME:
 KAITA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0200	0.0000
0.039	0.0398	0.0004
0.079	0.0770	0.0000
0.098	0.0986	0.0005
0.148	0.1448	0.0004
0.295	0.2916	0.0005
SLOPE	= 0.985361	
R ²	= 0.999846	

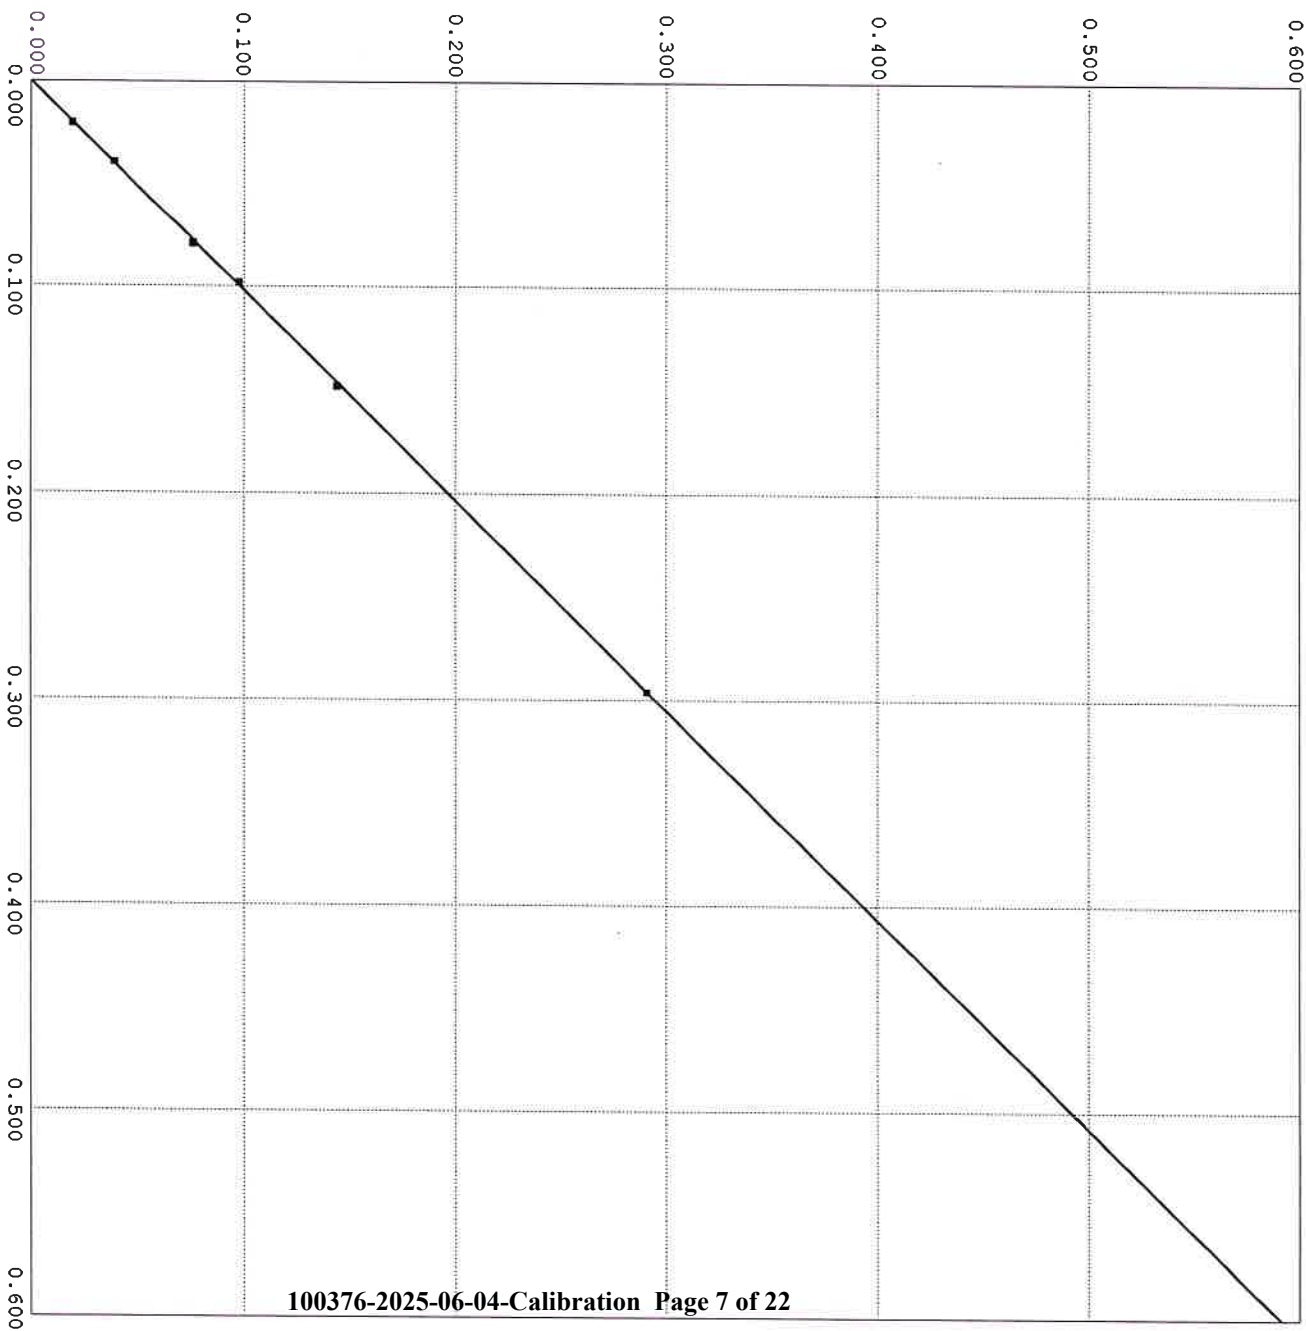

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100376






Date: 06/04/2025
Time: 11:43:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.44: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 0 psi KS 06/12/2025
PSI above 100, screwed tank in while running test.

BLANK TEST	0.000	11:45
INTERNAL STANDARD	VERIFIED	11:45
EXTERNAL STANDARD	0.020	11:45
BLANK TEST	0.000	11:46
EXTERNAL STANDARD	0.020	11:47
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.020	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.020	11:49
BLANK TEST	0.000	11:50
EXTERNAL STANDARD	0.020	11:50
BLANK TEST	0.000	11:51

Average = 0.0200
Std Dev = 0.0000

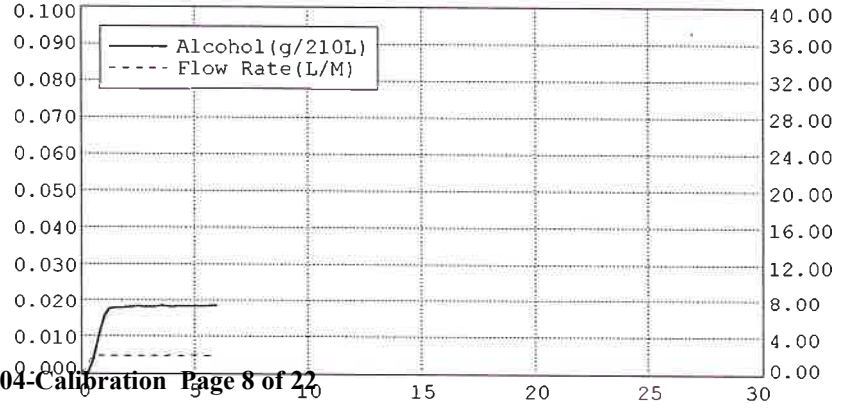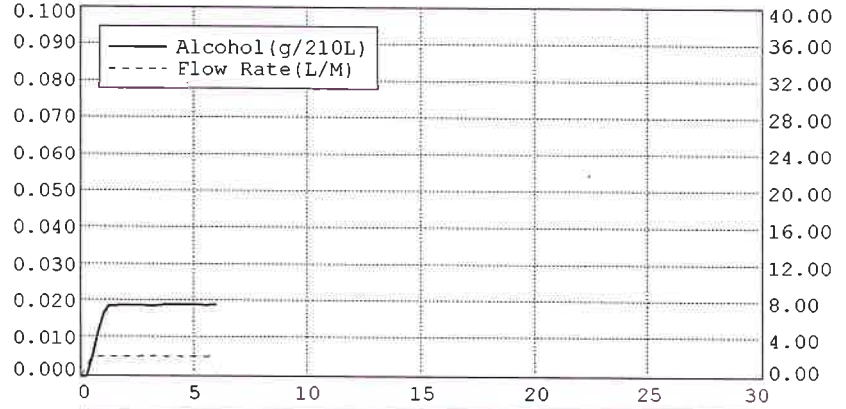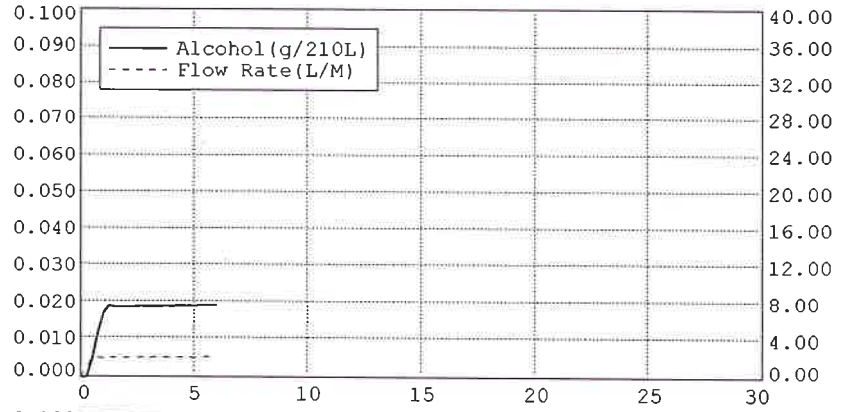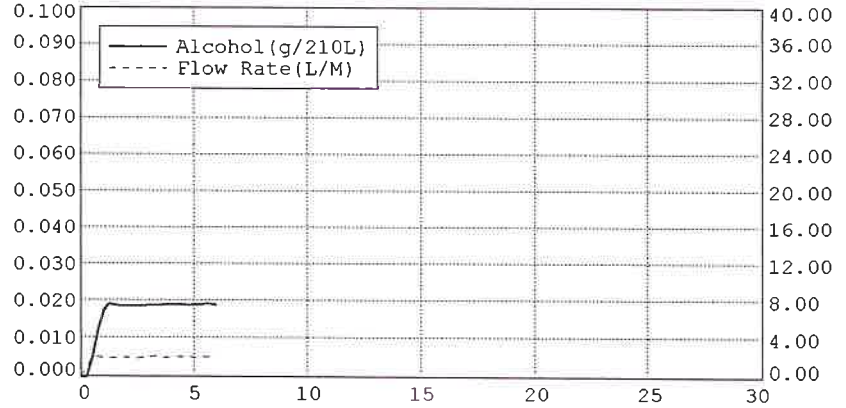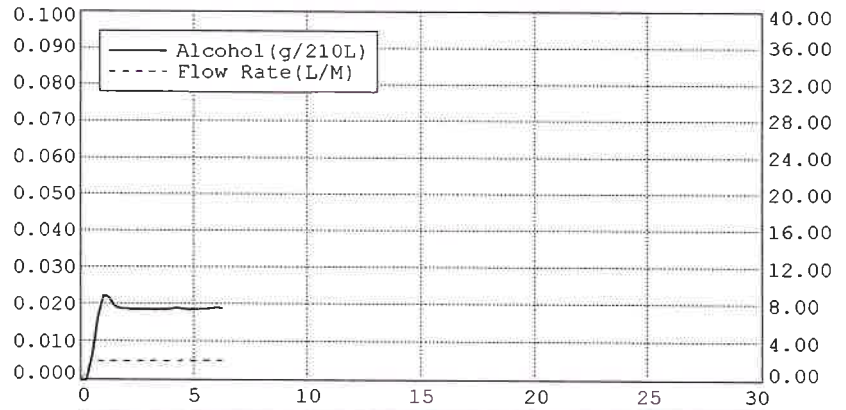

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100376






Date: 06/04/2025
Time: 11:52:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.44: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 857 psi

BLANK TEST	0.000	11:53
INTERNAL STANDARD	VERIFIED	11:53
EXTERNAL STANDARD	0.039	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.040	11:54
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.040	11:55
BLANK TEST	0.000	11:56
EXTERNAL STANDARD	0.040	11:57
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.040	11:58
BLANK TEST	0.000	11:59

Average = 0.0398
Std Dev = 0.0004

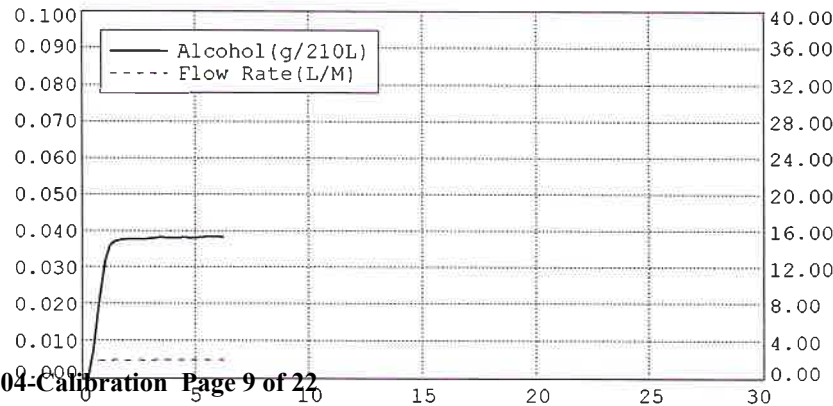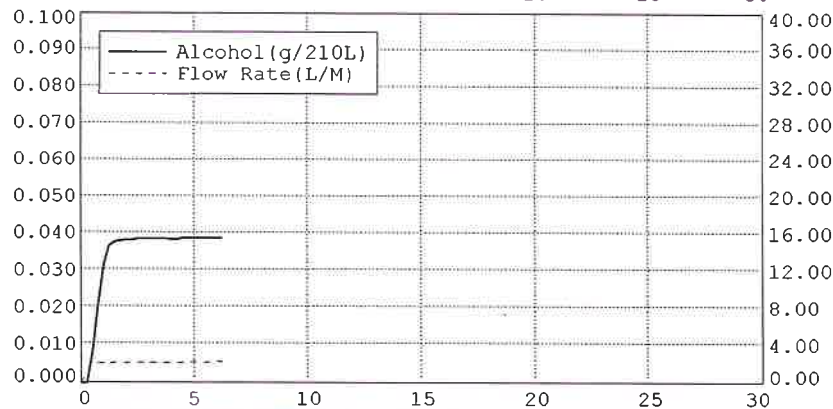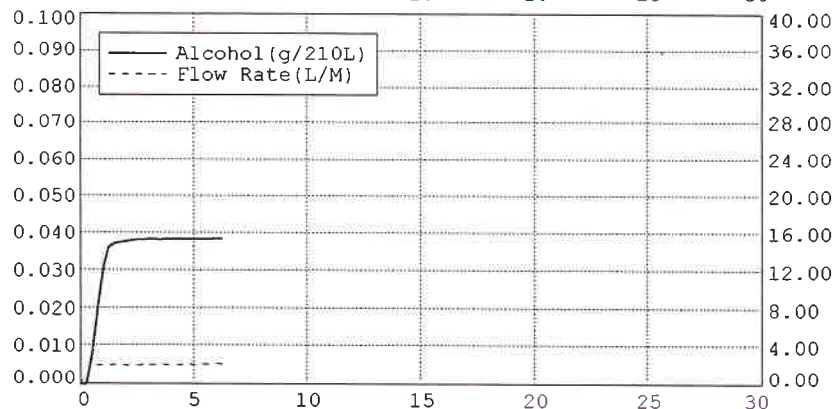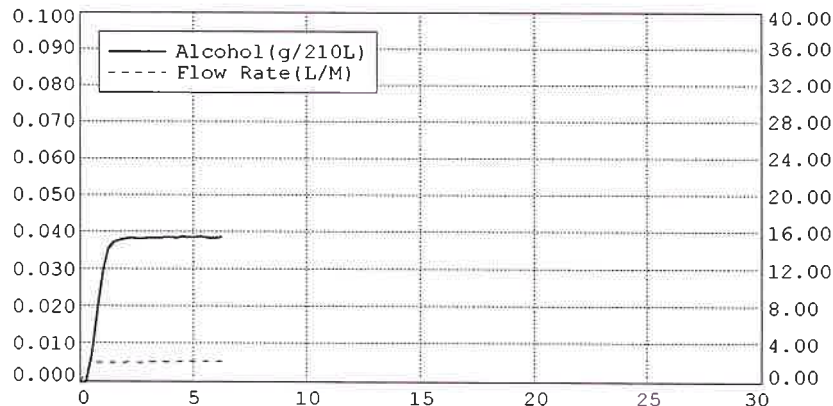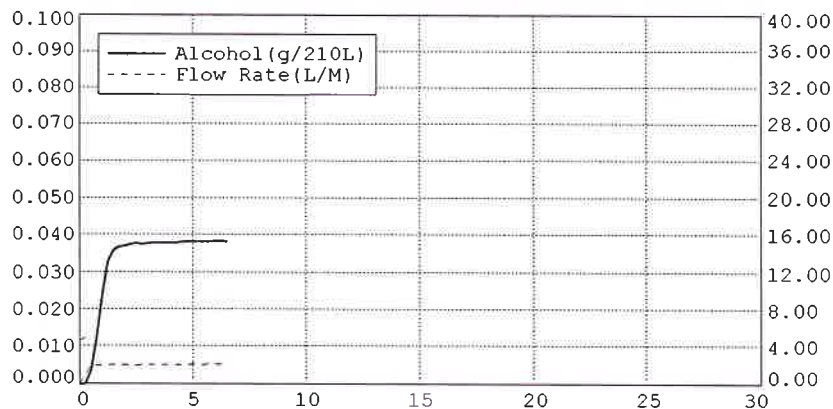

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100376






Date: 06/04/2025
Time: 11:59:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.43: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 616 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	12:01
INTERNAL STANDARD	VERIFIED	12:01
EXTERNAL STANDARD	0.077	12:01
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.077	12:02
BLANK TEST	0.000	12:03
EXTERNAL STANDARD	0.077	12:03
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.077	12:05
BLANK TEST	0.000	12:05
EXTERNAL STANDARD	0.077	12:06
BLANK TEST	0.000	12:07

Average = 0.0770
Std Dev = 0.0000

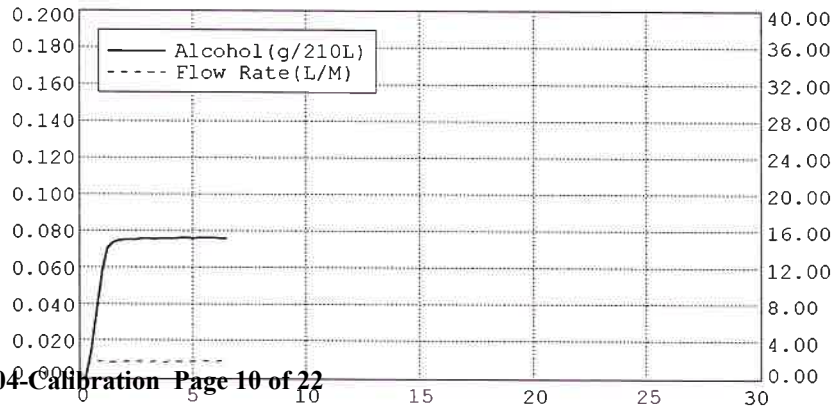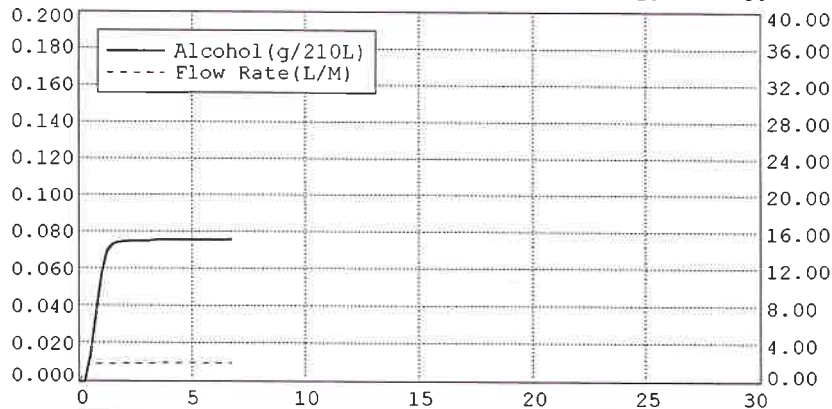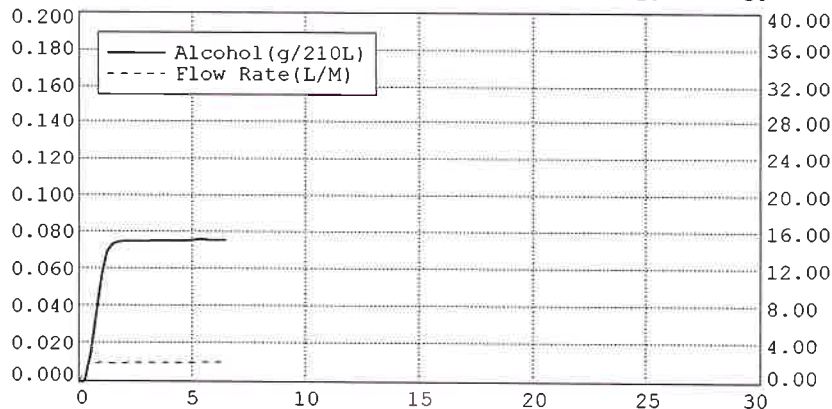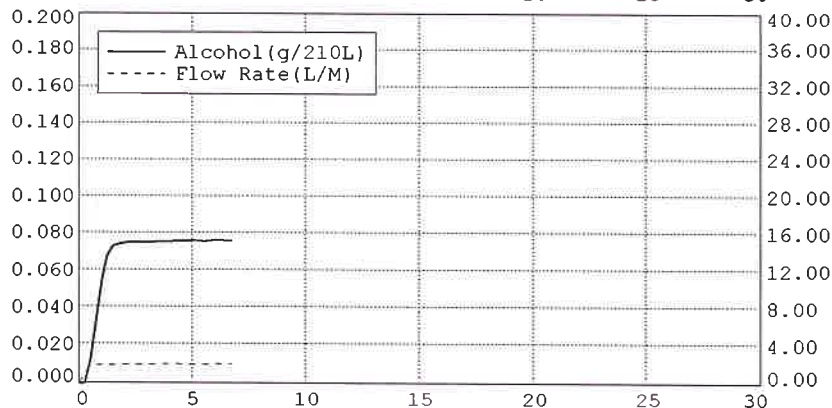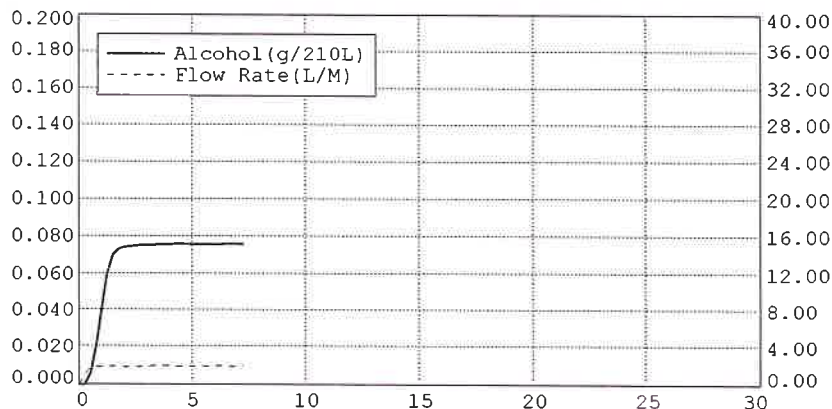

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100376






Date: 06/04/2025
Time: 12:08:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.43: 0.098
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 992 psi

BLANK TEST	0.000	12:10
INTERNAL STANDARD	VERIFIED	12:10
EXTERNAL STANDARD	0.098	12:10
BLANK TEST	0.000	12:11
EXTERNAL STANDARD	0.099	12:11
BLANK TEST	0.000	12:12
EXTERNAL STANDARD	0.099	12:12
BLANK TEST	0.000	12:13
EXTERNAL STANDARD	0.098	12:14
BLANK TEST	0.000	12:14
EXTERNAL STANDARD	0.099	12:15
BLANK TEST	0.000	12:16

Average = 0.0986
Std Dev = 0.0005

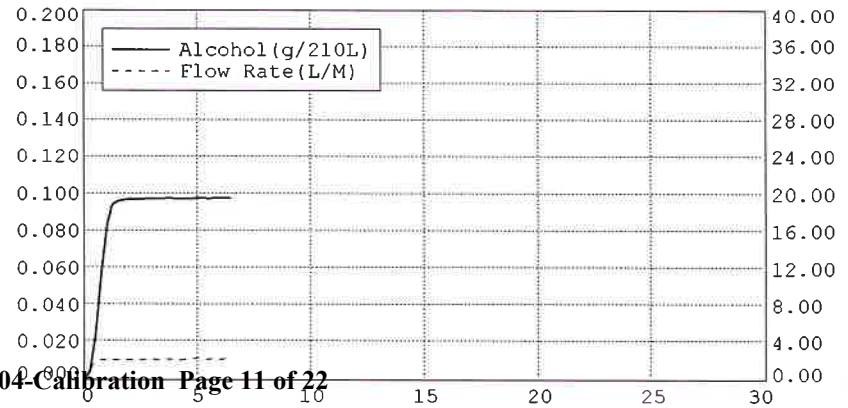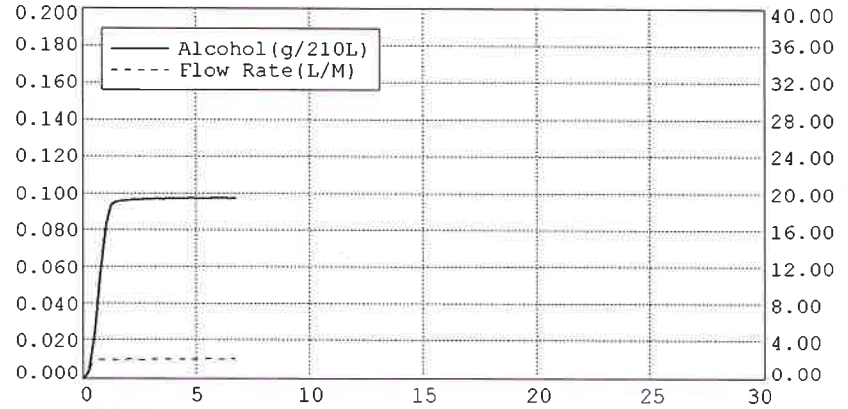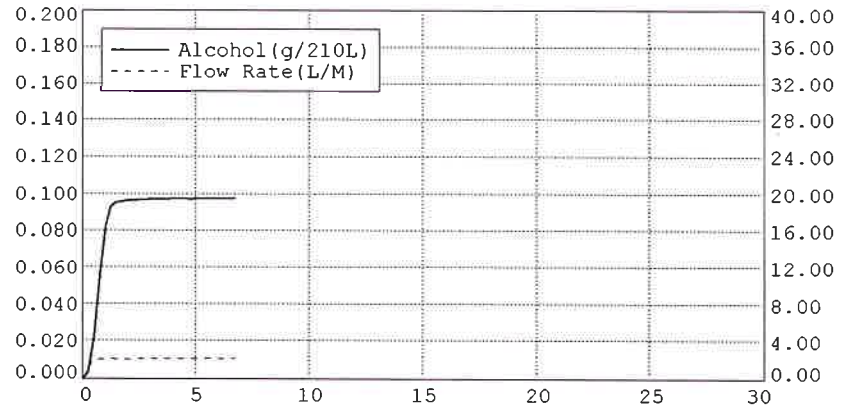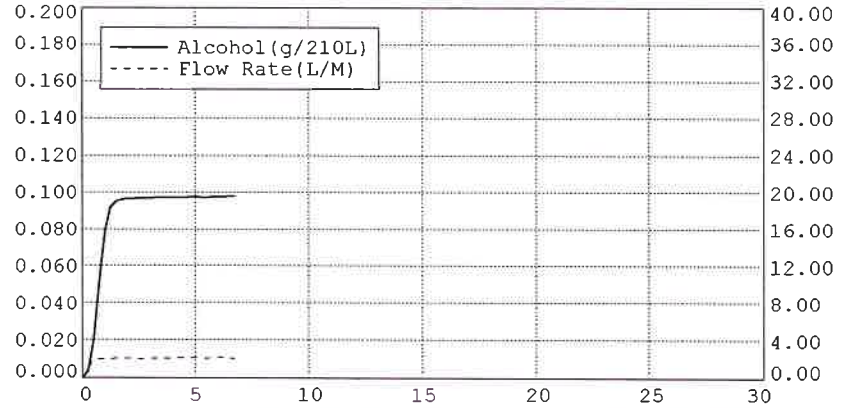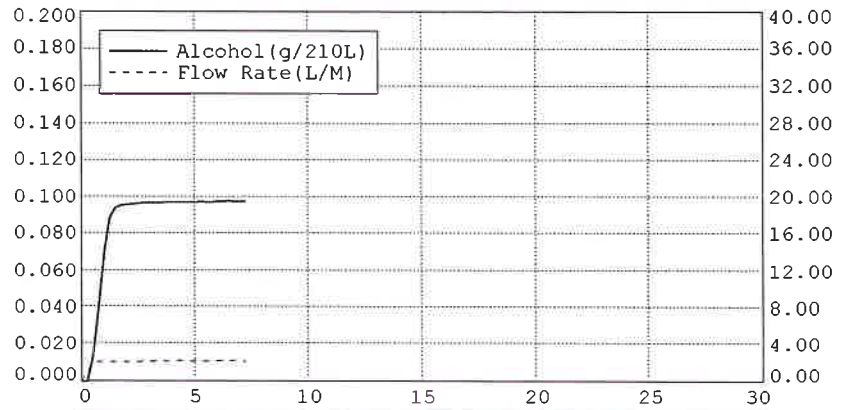

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100376






Date: 06/04/2025
Time: 12:17:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.44: 0.148
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 280 psi

BLANK TEST	0.000	12:19
INTERNAL STANDARD	VERIFIED	12:19
EXTERNAL STANDARD	0.145	12:20
BLANK TEST	0.000	12:20
EXTERNAL STANDARD	0.144	12:21
BLANK TEST	0.000	12:22
EXTERNAL STANDARD	0.145	12:22
BLANK TEST	0.000	12:23
EXTERNAL STANDARD	0.145	12:23
BLANK TEST	0.000	12:24
EXTERNAL STANDARD	0.145	12:24
BLANK TEST	0.000	12:25

Average = 0.1448
Std Dev = 0.0004

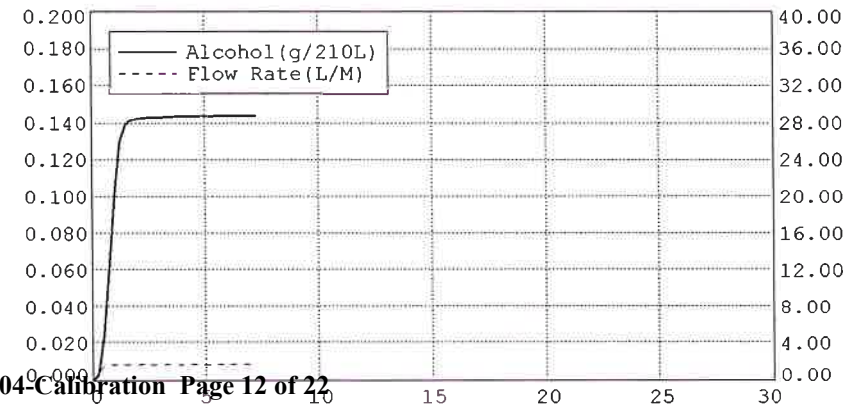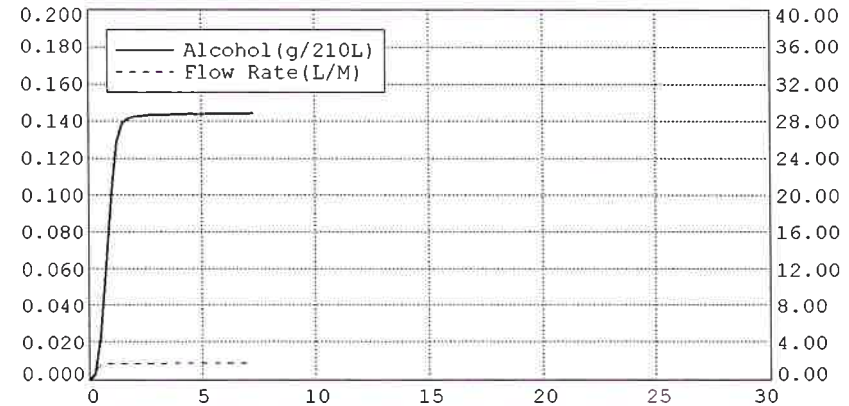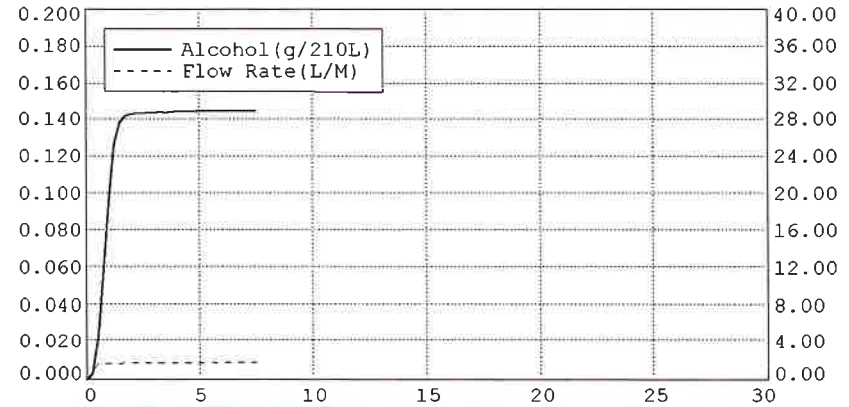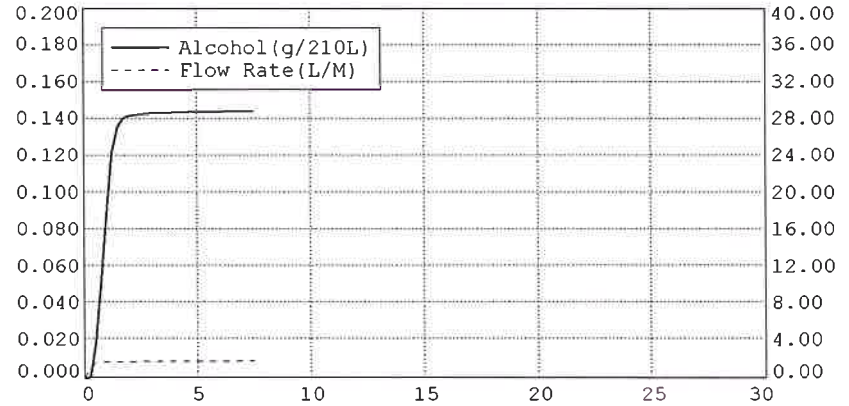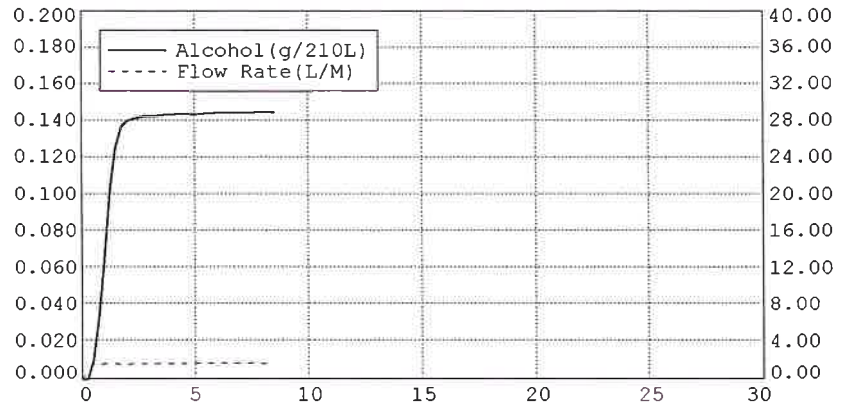

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100376






Date: 06/04/2025
Time: 13:28:21

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.43: 0.295
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 287 psi

BLANK TEST	0.000	13:29
INTERNAL STANDARD	VERIFIED	13:30
EXTERNAL STANDARD	0.291	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.291	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.292	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.292	13:33
BLANK TEST	0.000	13:34
EXTERNAL STANDARD	0.292	13:34
BLANK TEST	0.000	13:35

Average = 0.2916
Std Dev = 0.0005

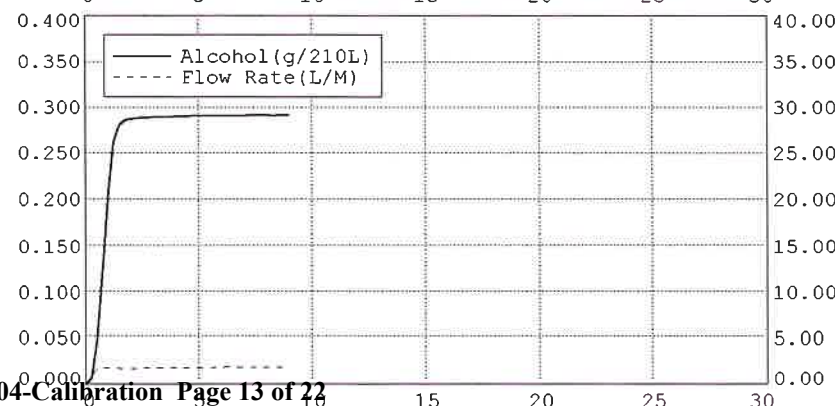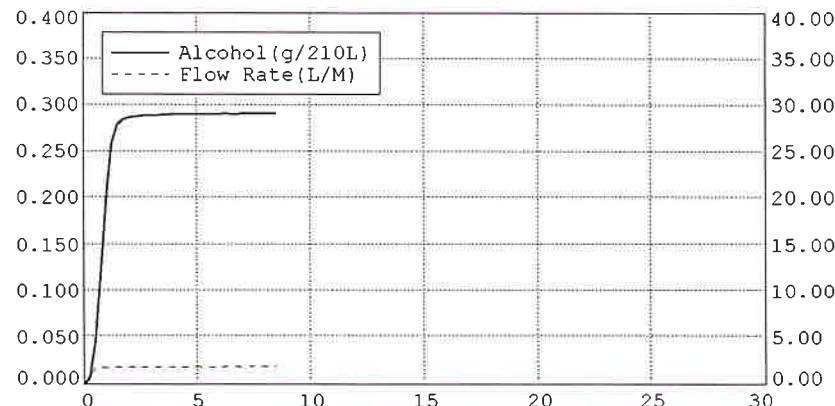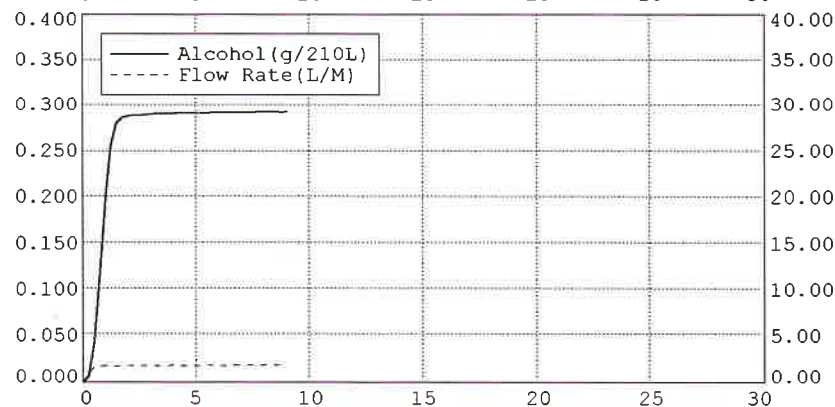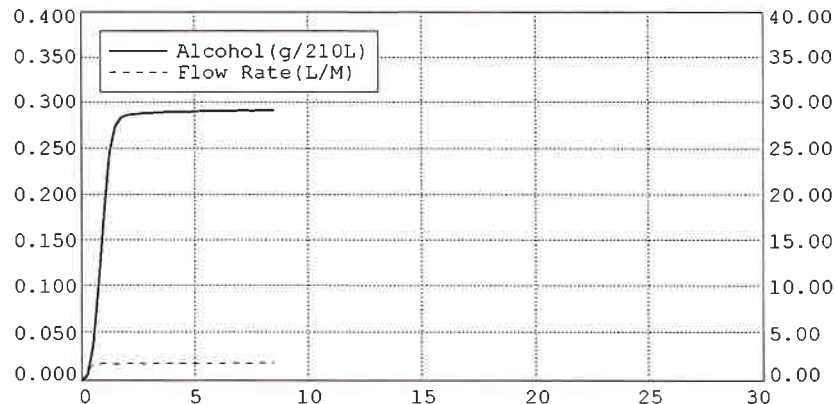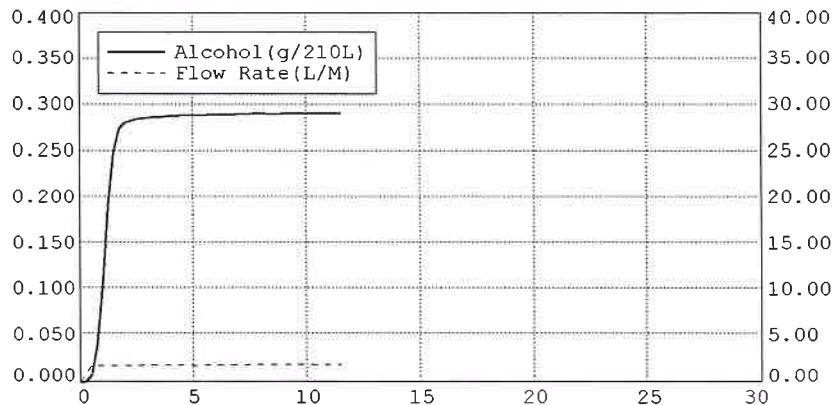

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100376

Date: 06/04/2025
Time: 13:48:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAITA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:49
BLANK TEST	0.000	13:49
INTERNAL STANDARD	VERIFIED	13:50
EXTERNAL STANDARD	0.078	13:50
BLANK TEST	0.000	13:51
SUBJECT SAMPLE	INCOMPLETE	13:53

KS

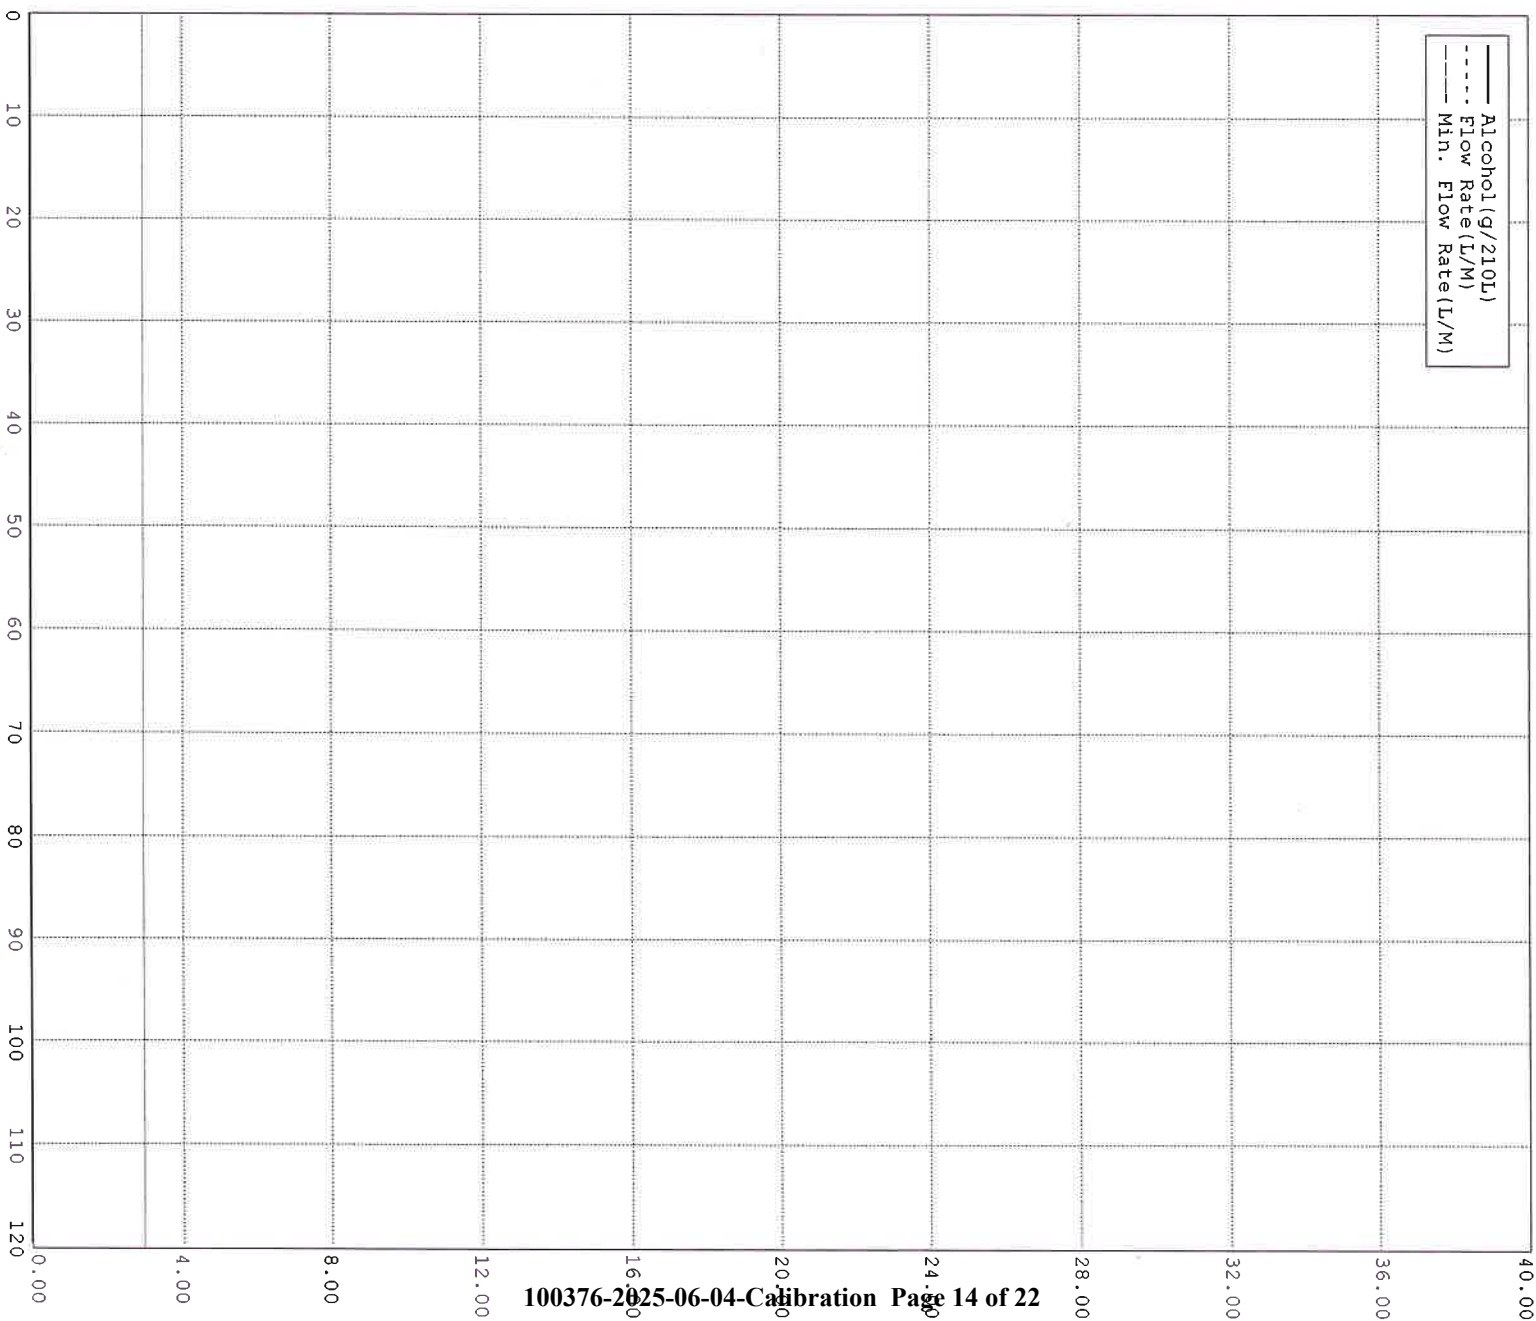

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100376

Date: 06/04/2025
Time: 13:57:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:59
BLANK TEST	0.000	13:59
INTERNAL STANDARD	VERIFIED	13:59
EXTERNAL STANDARD	0.077	13:59
BLANK TEST	0.000	14:00
SUBJECT SAMPLE	XXX	14:01

Maximum Attempts Exceeded

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

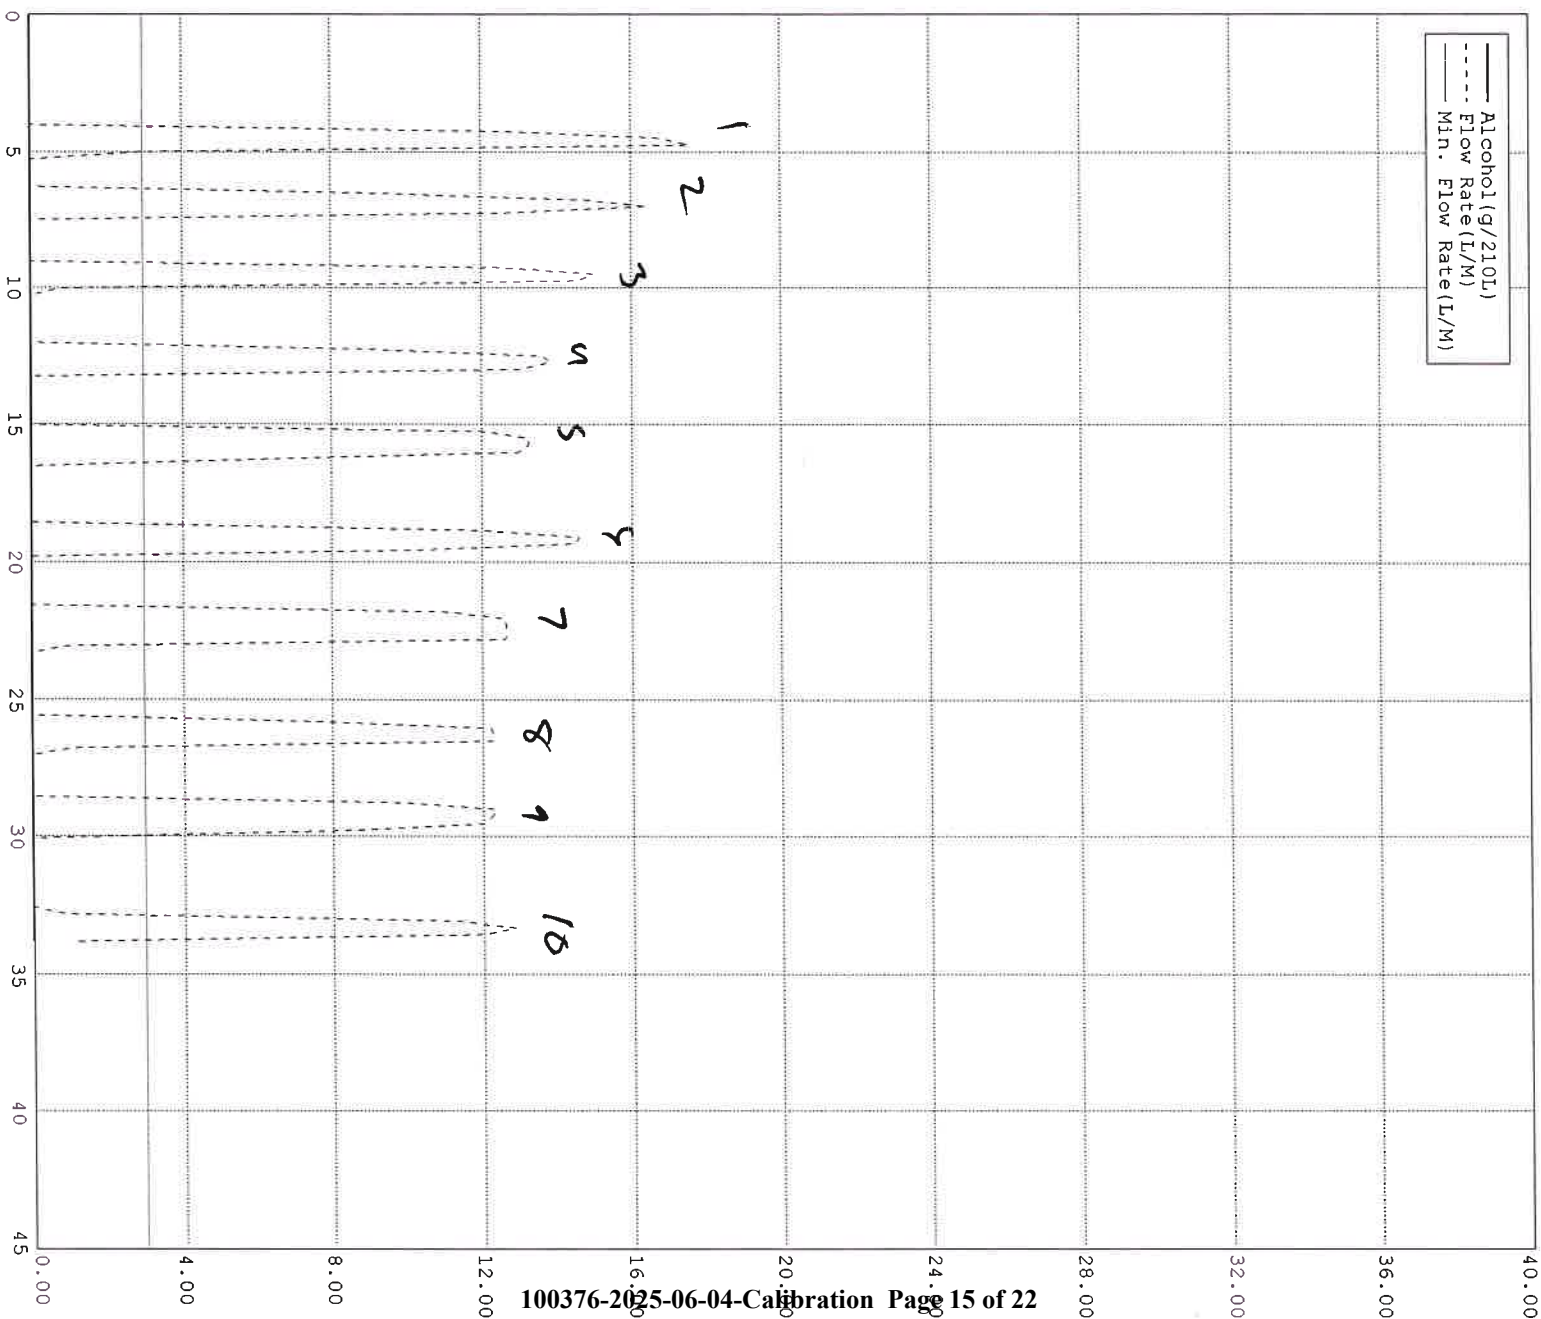

KS

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100376

Date: 06/04/2025
Time: 14:03:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	
BLANK TEST	PASSED 14:04
INTERNAL STANDARD	0.000 14:04
EXTERNAL STANDARD	VERIFIED 14:04
BLANK TEST	0.078 14:04
SUBJECT SAMPLE	0.000 14:05
	INVALID 14:06

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

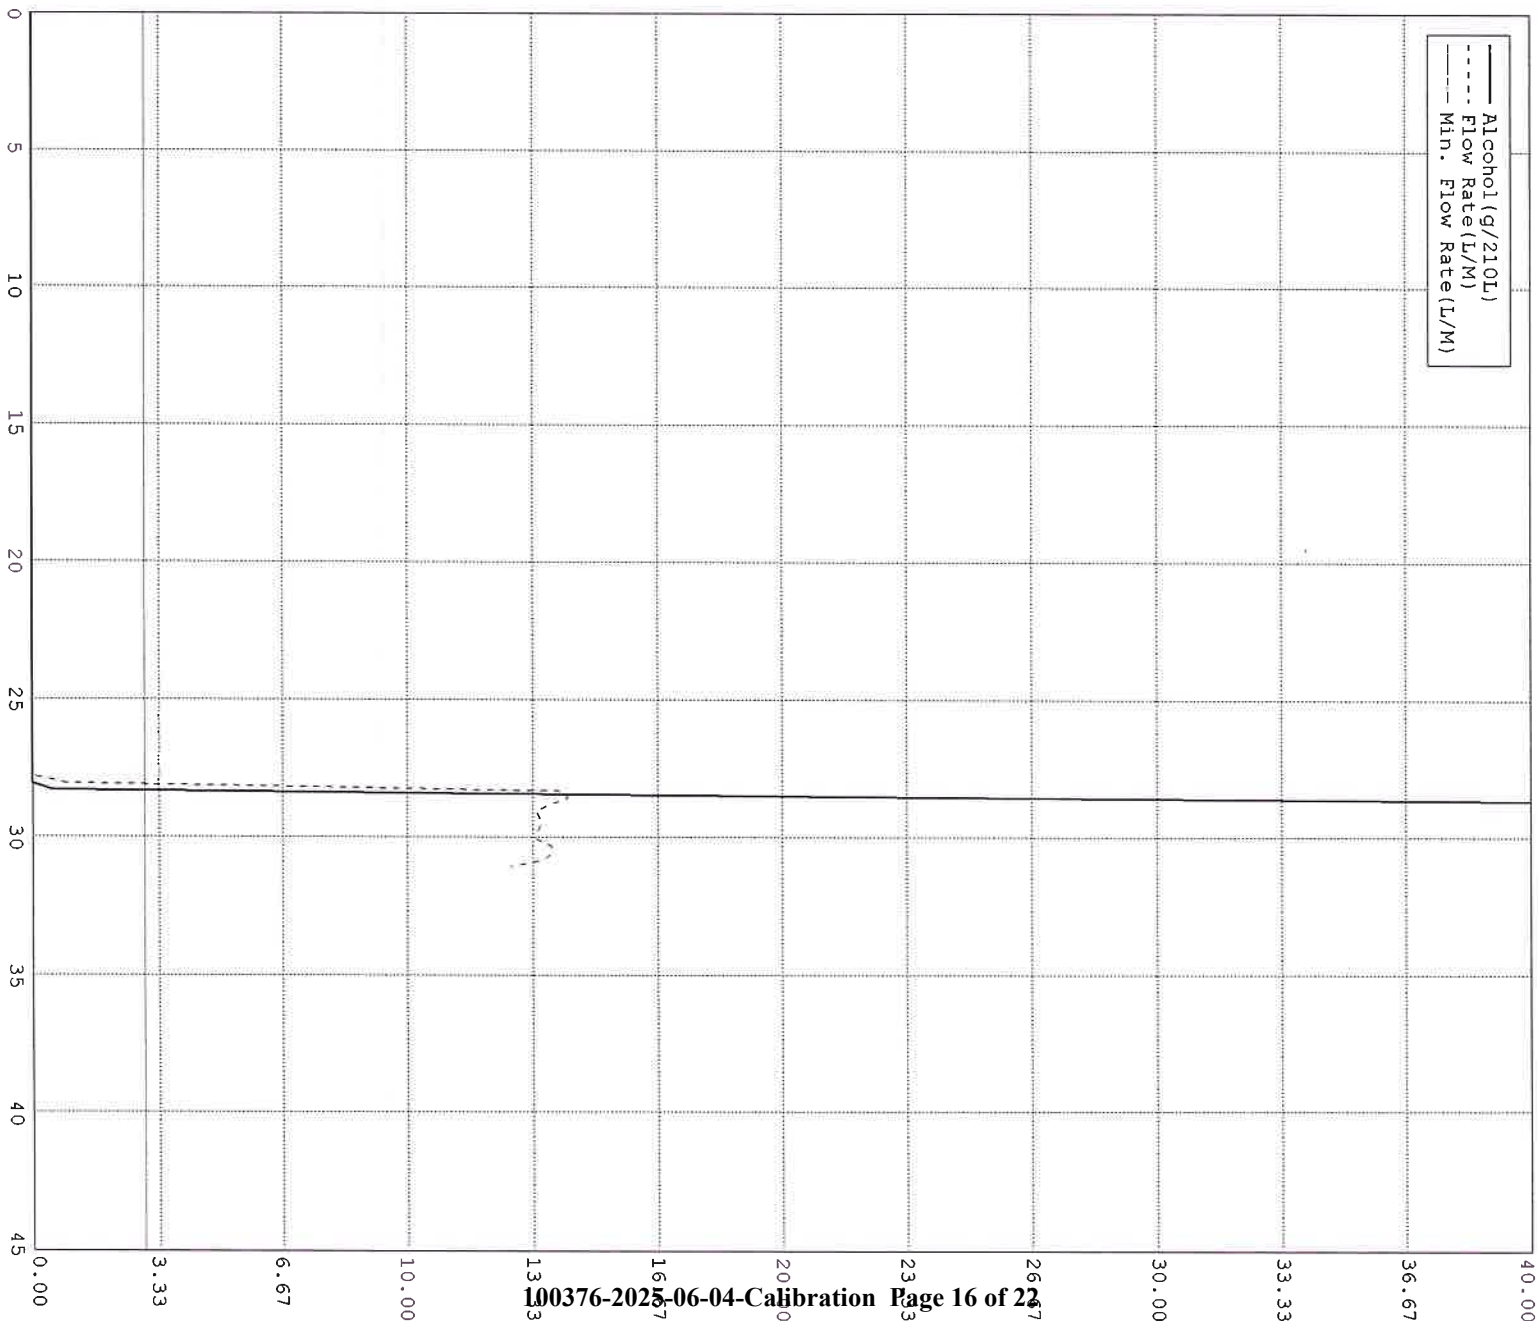

KS

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100376

Date: 06/12/2025
Time: 08:18:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.89: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:20
BLANK TEST	0.000	08:20
INTERNAL STANDARD	VERIFIED	08:20
EXTERNAL STANDARD	0.078	08:20
BLANK TEST	0.000	08:21
SUBJECT SAMPLE	INVALID	08:21

*Invalid Completed on 6/12/25
to show slope.
KS 6/12/25*

KS

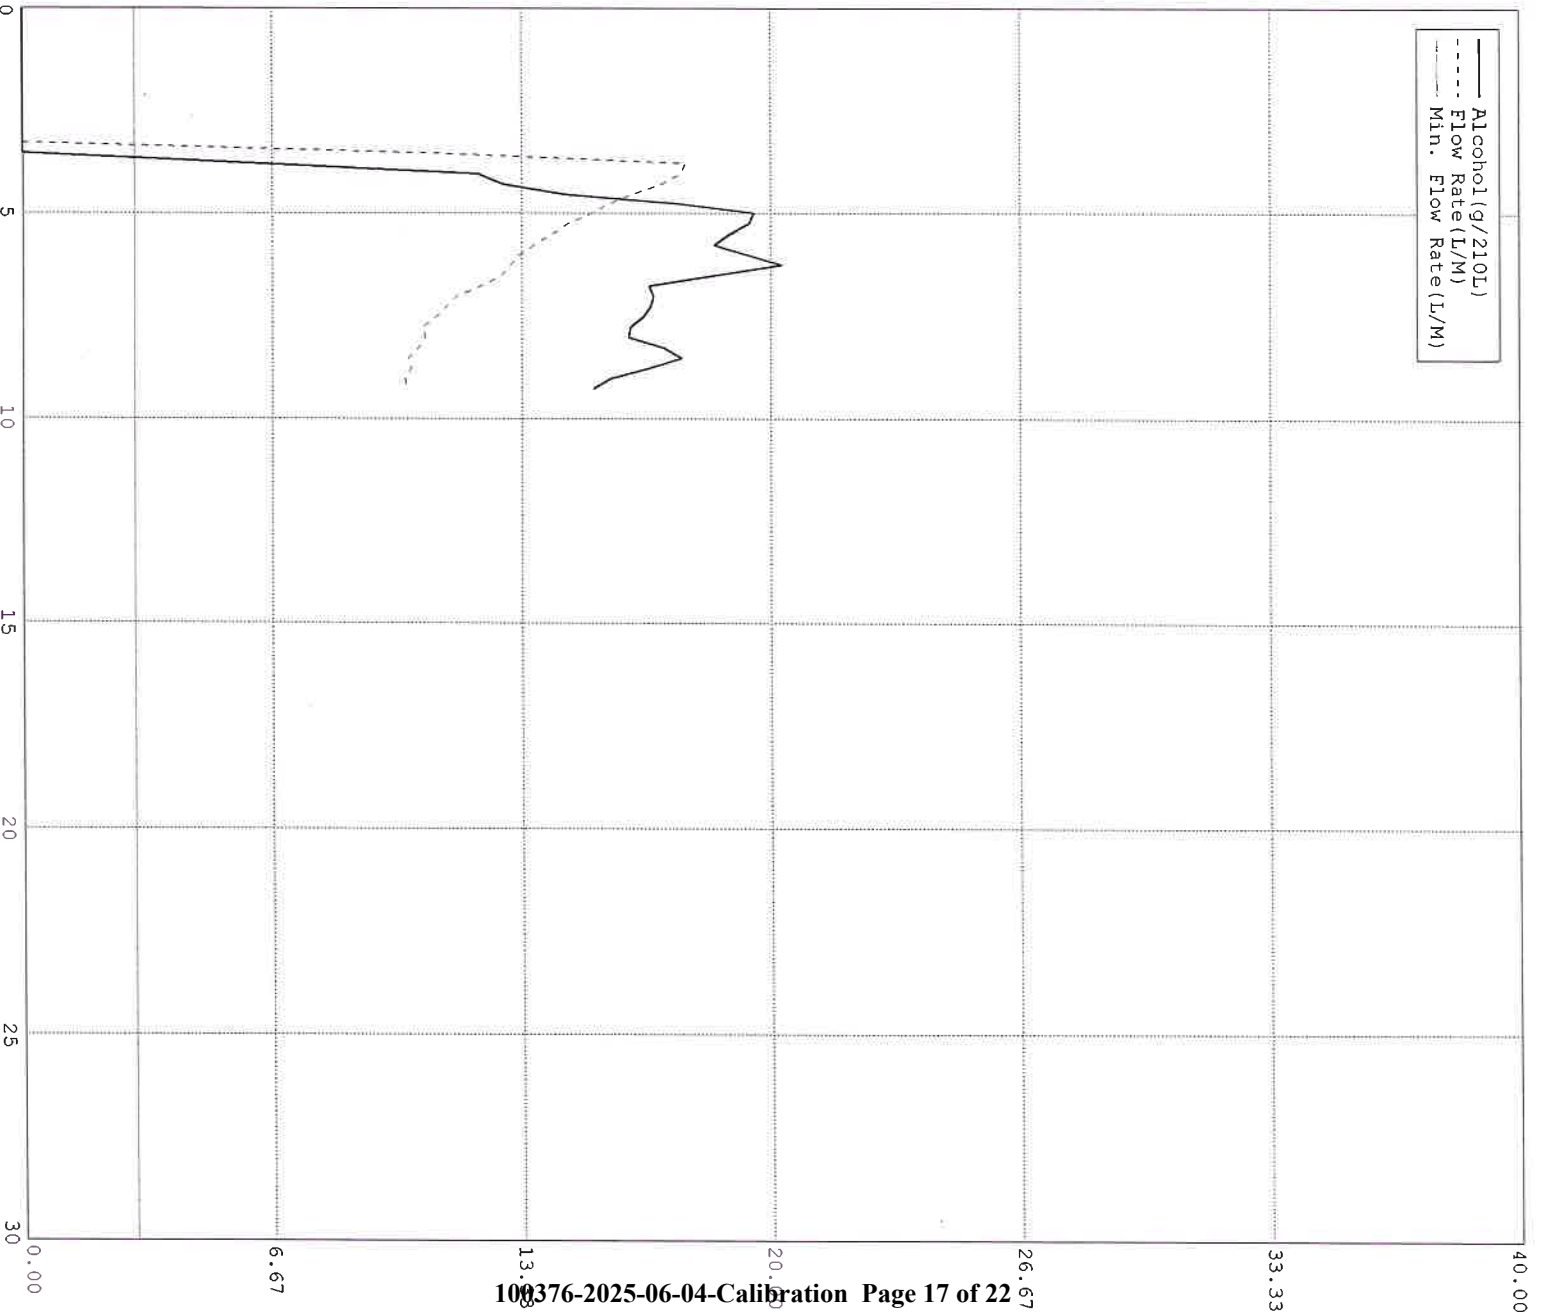

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100376

Date: 06/04/2025
Time: 13:39:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAJIA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:40
BLANK TEST	0.000	13:40
INTERNAL STANDARD	VERIFIED	13:40
EXTERNAL STANDARD	0.078	13:40
BLANK TEST	0.000	13:41

RFI DETECTED

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

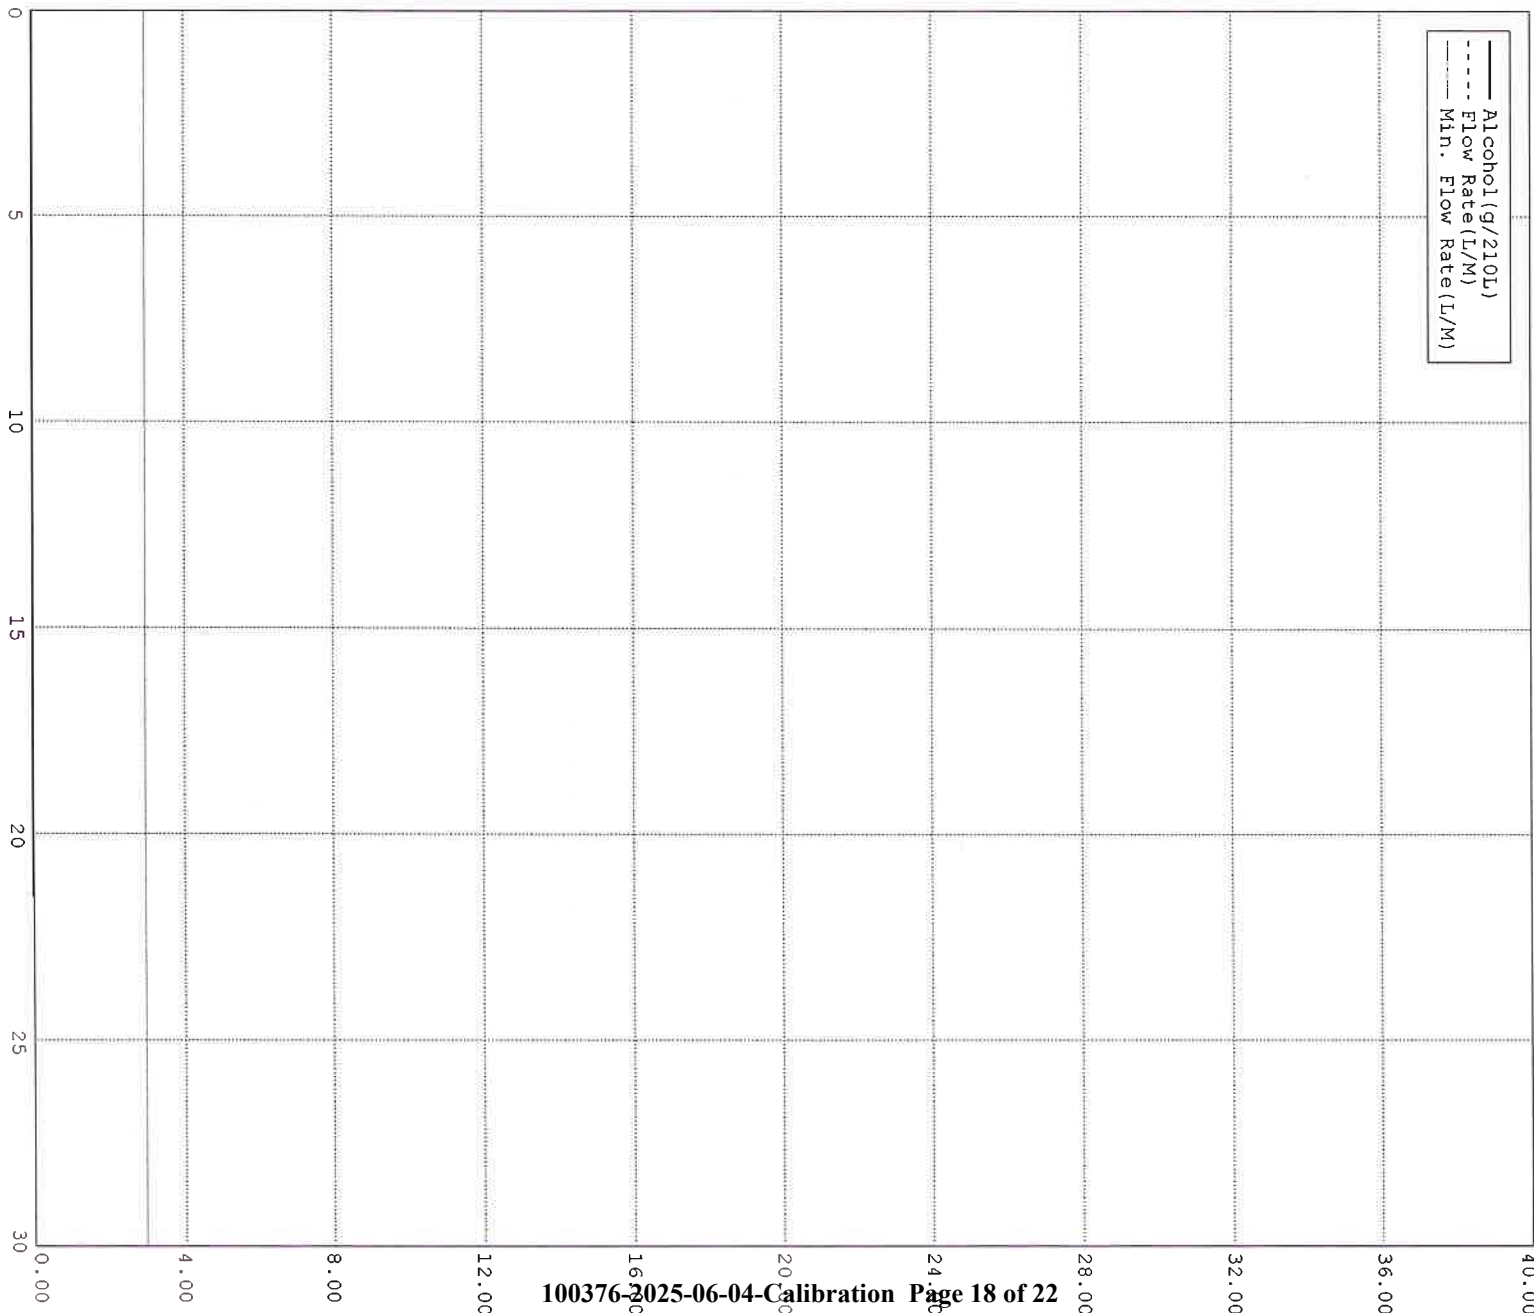

KS

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100376

Date: 06/04/2025
Time: 14:10:18

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.45: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:11
BLANK TEST	0.000	14:11
INTERNAL STANDARD	VERIFIED	14:11
Xq = 0.078 (2.62%)	0.077	14:11
EXTERNAL STANDARD	X[1] = 0.0772 (-0.0004)	(0.0030)
BLANK TEST	0.000	14:12
SUBJECT SAMPLE	XXX	14:13
X[1] = 0.1132 (-0.0158)	(0.0023)	

Interference Detected

F2 average: -0.0007

F3 average: 0.0023

KS 6/5/25

KS



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100376

Date: 06/04/2025
Time: 14:15:23

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:16
BLANK TEST	0.000	14:16
INTERNAL STANDARD	VERIFIED	14:16
Xq = 0.077 (1.48%)	0.077	14:17
EXTERNAL STANDARD	0.0020	14:18
X[1] = 0.0769 (-0.0013)	0.000	14:18
BLANK TEST	XXX	14:18
SUBJECT SAMPLE	X[1] = 0.1202 (-0.0275) (0.0017)	

Interference Detected

KS

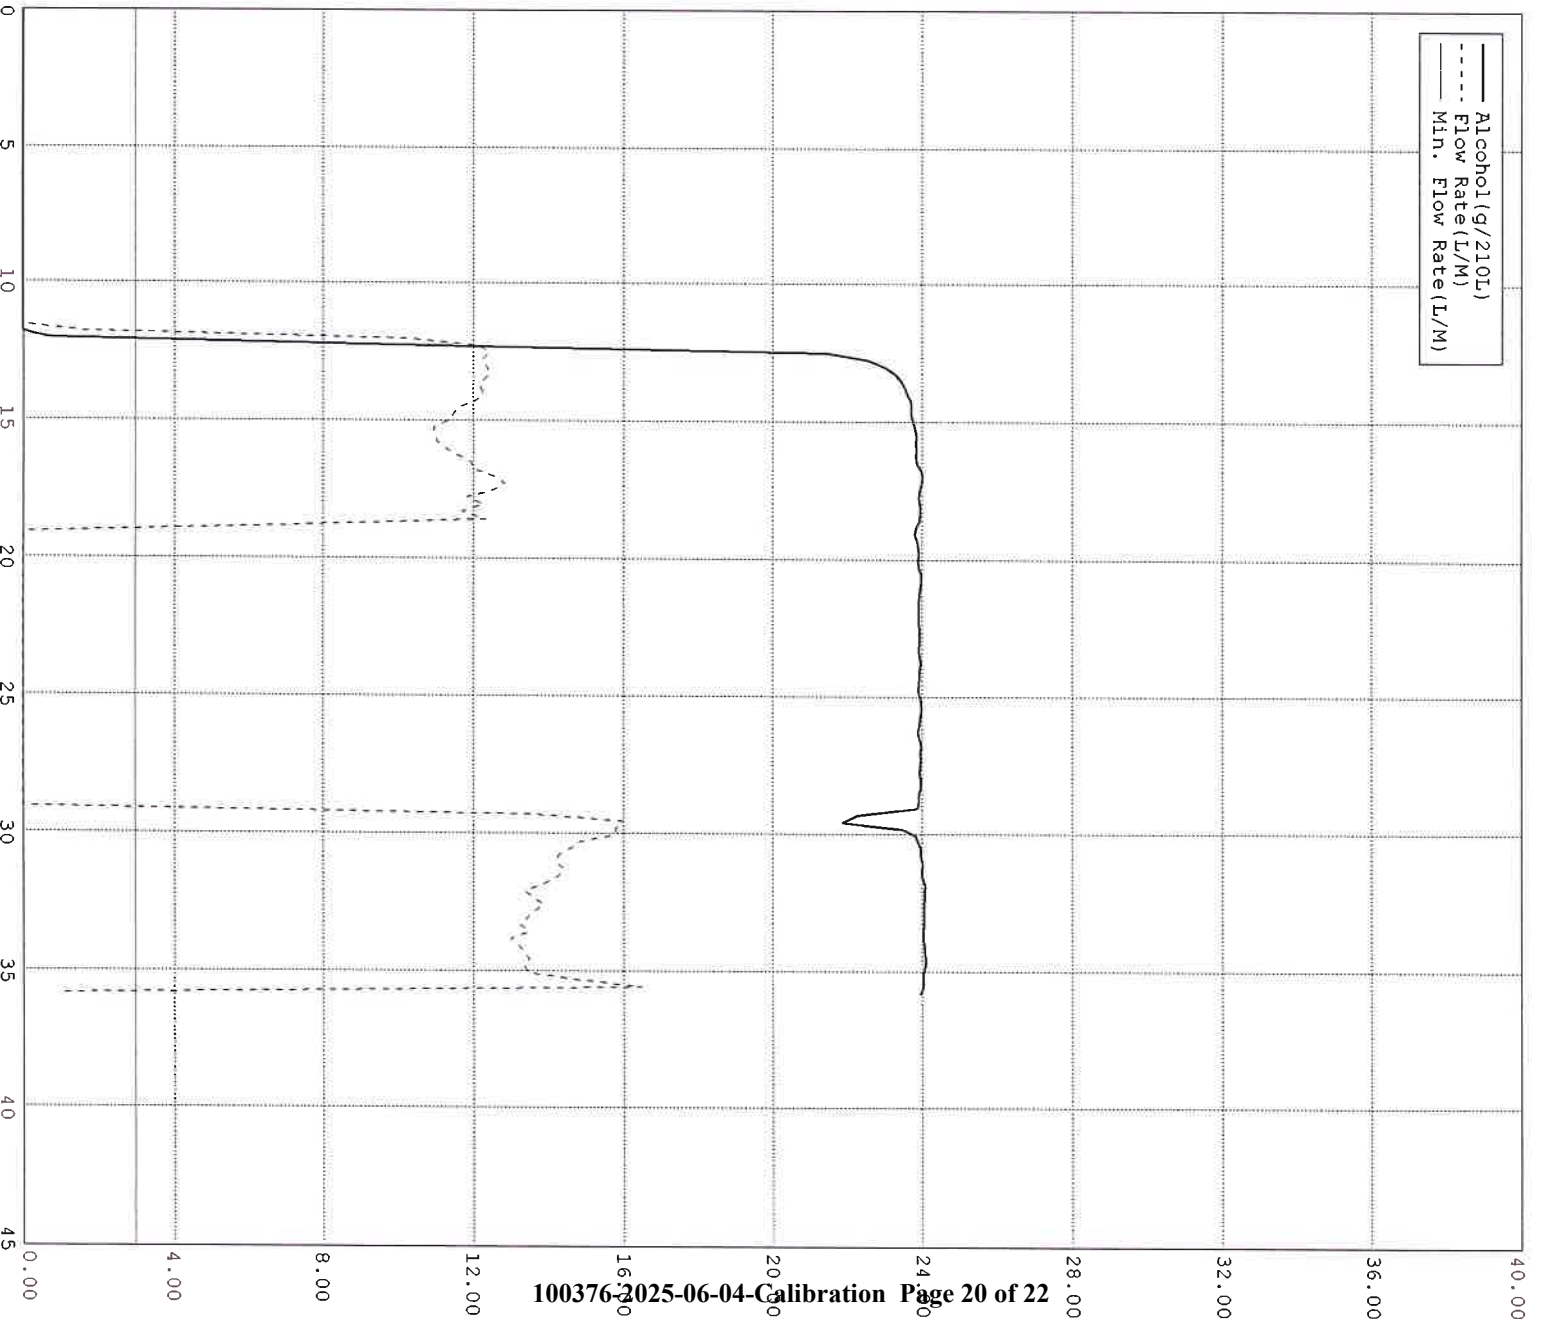

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100376

Date: 06/04/2025
Time: 14:20:32

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.45: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 14:21
INTERNAL STANDARD VERIFIED 14:21
Xq = 0.078 (2.28%) 0.077 14:22
EXTERNAL STANDARD X[1] = 0.0771 (-0.0008) (0.0023) 14:22
BLANK TEST 0.000 14:22
SUBJECT SAMPLE (Vol=1.57L) 0.095 14:24
X[1] = 0.0952 (-0.0004) (0.0010) 14:25
BLANK TEST 0.000 14:25
EXTERNAL STANDARD 0.076 14:25
X[1] = 0.0761 (-0.0004) (0.0020) 14:26
BLANK TEST 0.000 14:26

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

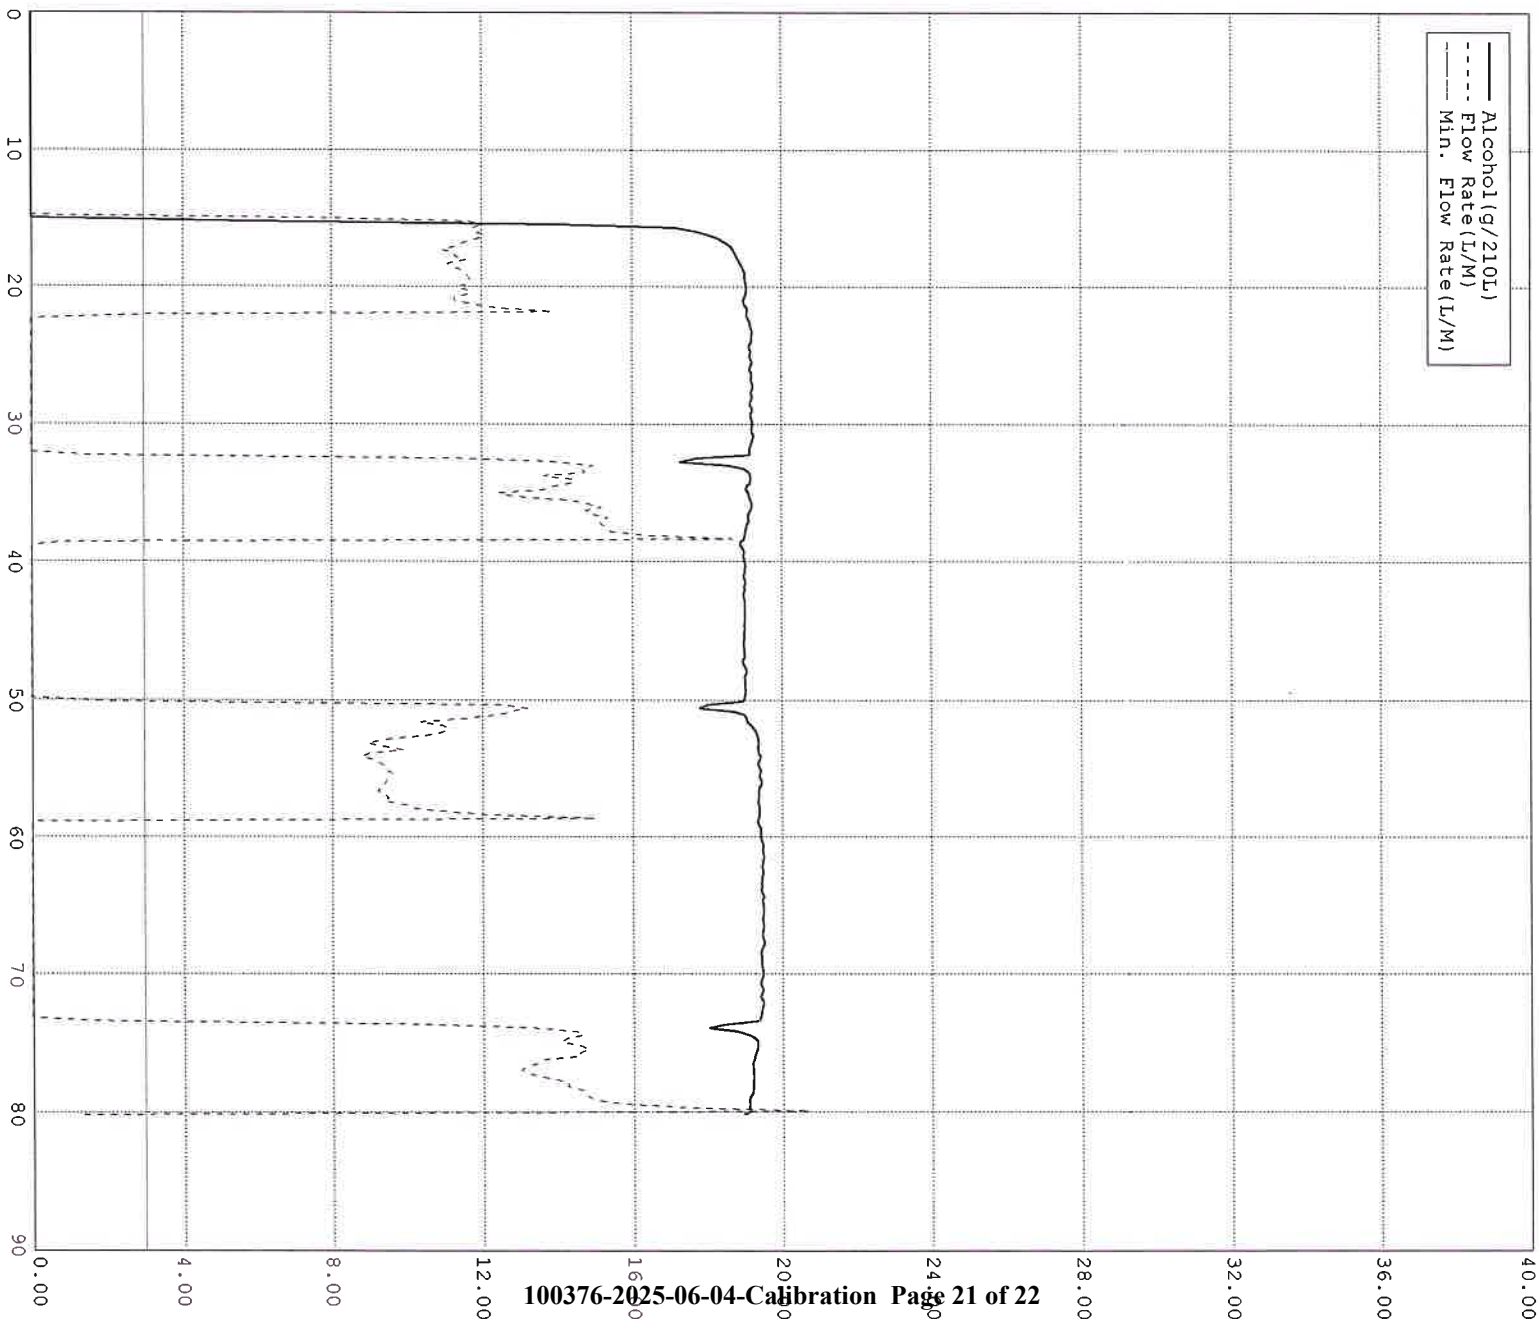

KS

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100376

Date: 06/04/2025
Time: 14:40:06

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.44: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:41
BLANK TEST	0.000	14:41
INTERNAL STANDARD	VERIFIED	14:41
EXTERNAL STANDARD	0.078	14:41
BLANK TEST	0.000	14:42
SUBJECT SAMPLE (Vol=1.89L)	0.000	14:42
BLANK TEST	0.000	14:43
EXTERNAL STANDARD	0.077	14:43
BLANK TEST	0.000	14:44

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

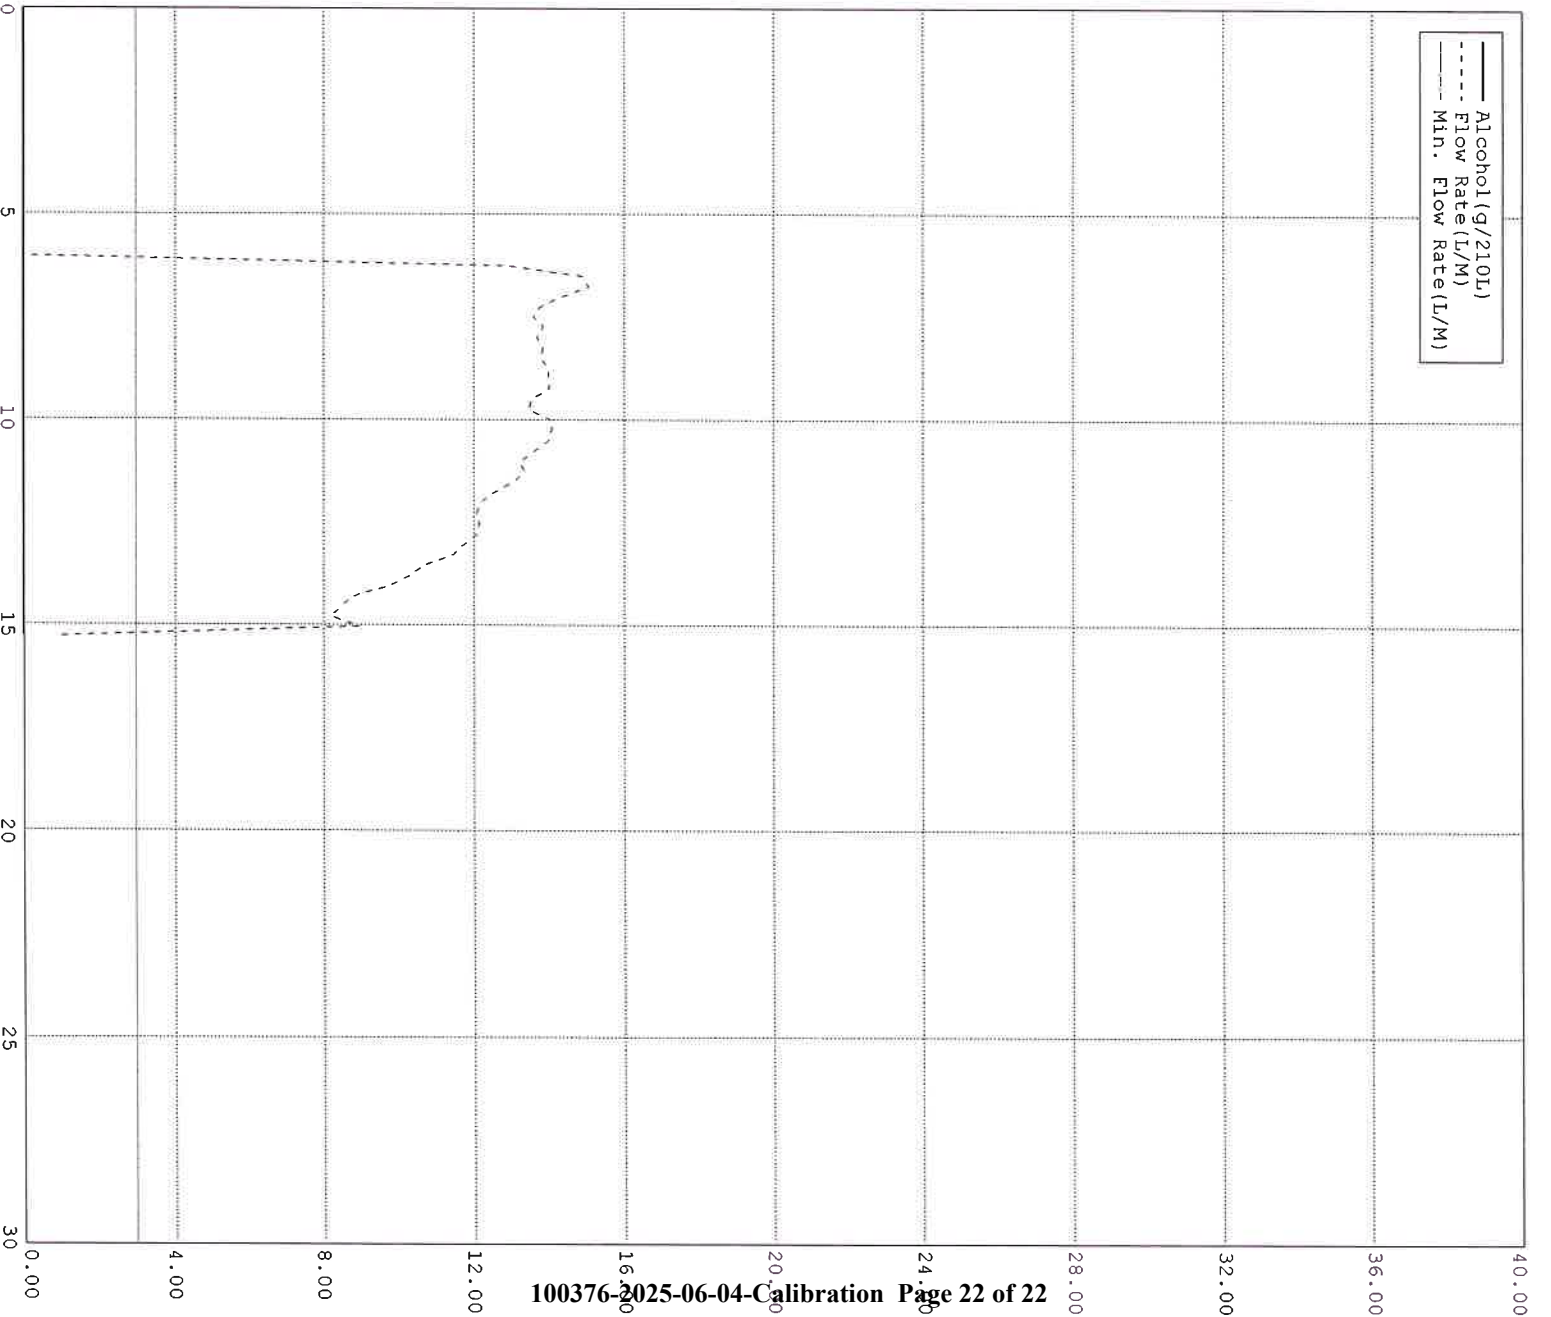

KS