



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories

**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100361

**Report Issue Date:** 10/16/2023  
**Date Received:** 2023-04-05  
**Condition of Item:** Needs Repair

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

**Start Date 04/10/2023** - As Found - **End Date 04/11/2023** As Found - Evaluation Analyst: Tatiana Malnoske  
 As Found Conditions - Barometric Pressure (inHg): 29.58 Barometer Used: Fisher S/N 221250180 Temperature (C): 22.9  
 Relative Humidity (%): 10%

As-Found Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.019	0.019	0.020	0.019	
0.080	0.079	AG135004	0.079	0.078	0.078	0.078	0.078	0.078	
0.300	0.297	AG217903	0.299	0.298	0.298	0.298	0.298	0.298	

The values on the linearity testing and VOC looks good. They all passed and I did not get a status message during the evaluation. While printing the paperwork for the linearity testing on 04/10/2023, the screen froze. I restarted the DMT and once on, the screen was just blank. I restarted it a second time and that seemed to have fixed the issue.

**Start Date 09/26/2023** - As Left - **End Date 09/27/2023**

As Left Conditions - Barometric Pressure (inHg): 29.30 Barometer Used: Fisher S/N 221250180 Temperature (C): 23.5 Relative Humidity (%): 31

As-Left Data										
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)	
0.020	0.020	AG217902	0.019	0.019	0.019	0.019	0.020	0.019	+/- 0.002	
0.040	0.039	AG217904	0.039	0.039	0.040	0.039	0.039	0.039	+/- 0.003	
0.080	0.078	AG135004	0.078	0.077	0.079	0.077	0.078	0.078	+/- 0.004	
0.100	0.098	AG211003	0.098	0.098	0.098	0.098	0.097	0.098	+/- 0.004	
0.150	0.147	AG134205	0.147	0.147	0.147	0.147	0.147	0.147	+/- 0.005	
0.300	0.294	AG217903	0.296	0.295	0.295	0.295	0.295	0.295	+/- 0.011	

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**



State of Alaska  
Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
Anchorage, Alaska 99507  
David Kanaris, Chief, Forensic Laboratories

---

**Serial Number:** 100361

---

Results authorized by Carlie Glaister on 09/27/2023

[carlie.glaister@alaska.gov](mailto:carlie.glaister@alaska.gov)

Technically and administratively reviewed by Colleen O'Bryant on 10/16/2023

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 10/10/2022

Version: 3.0

Instrument #: 100361 Analyst: Carlisle Glaister Start Date: 9/26/2023

- Diagnostic Test (attached)
- Adjust voltages, if needed
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
- Internal Standard value  $\leq 3.00\%$ 
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
- Adjust volume setting, if needed (1.50 L +/- 0.10 L)
- Print Technician Screen (attached)
- Print Calibration Factors (attached)
- Minimum Volume Test 1.5 L (1.3L to 1.7L)

As Left Conditions:

Barometric Pressure (in Hg): 29.30 Temperature (C): 23.5 Relative Humidity (%) 31

Linearity Test (attached)

0.020g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217902</u>	Exp: <u>6/28/24</u>
0.040g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217904</u>	Exp: <u>6/28/24</u>
0.080g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-135004</u>	Exp: <u>12/16/23</u>
0.100g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-211003</u>	Exp: <u>4/20/24</u>
0.150g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-134205</u>	Exp: <u>12/8/23</u>
0.300g/210L Mnf: <u>Airgas</u>	Lot: <u>AG-217903</u>	Exp: <u>6/28/24</u>

Functional Tests (attached)

- Incomplete
- Maximum Attempts Exceeded
- Interference (Volatiles)
- Invalid
- Radio Frequency Interference (RFI)

Acetone Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR4176 Verification Performed?

Isopropanol Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR4177 Verification Performed?

Neg. Control Mnf: Lifloc Lot: 22HP41201 Level: 0.100 Exp: 8/24/24

Simulator S/N: DR6267 Verification Performed?

Calibrated External Thermometer:

Thermometer S/N: 210958384 Calibration Due Date: 11/9/2023

- Verify stylus is calibrated
  - Reset Options
  - Clear Memory
  - Verification of Calibration (VOC)
  - Non-Drinking Subject Test
  - Upload
  - Remove Tank Prior to Shutdown
- Calibration End Date: 9/27/2023

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 09/26/2023  
Time: 08:22:34

VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C            PASSED  
(44.0°C - 52.0°C)  
Breath Tube       = 43.8°C        PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage     = 1.87 V           PASSED  
(1.17 V - 2.73 V)  
Cooler Voltage   = 1.89 V           PASSED  
(1.01 V - 2.35 V)  
Bias Voltage     = 79 V            PASSED  
(48 V - 112 V)  
Chopper Freq    = 528 Hz            PASSED  
(475 Hz - 575 Hz)  
Barometer        = 29.3 in

PUMP INFO

Flow Rate = 4.414 L/M            PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON                            PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF                           PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1                           PASSED  
Filter 2                           PASSED  
Filter 3                           PASSED

INTERNAL STANDARD

Xq = 0.088 0.30% (0.00% - 4.00%)            PASSED

Technician Screen

-----  
DATAMASTER dmt: 100361  
-----

Date: 09/26/2023  
Time: 9:22 AM

Temperatures (°C)

Sample Cell: 48.7°C  
Breath Tube: 45.3°C

Current Barometer 29.3 in  
Volume (Ltr) 1.51

Settings

Lamp: 1.87 V  
Bias: 79 V  
Cooler: 1.89 V  
Chopper: 528 Hz

Voltages (V)

Flow: 1.04 V  
Detector: 0.064 V


CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 04/23/2021  
Time: 09:19:31

OPERATOR NAME:  
NPAS TECH  
CERTIFICATE #: G12921/20490

Ca = 0.1000  
CAL = 0.999458 0.800 <= CAL < 1.200  
b1 = 0.0003 0.0000 <= b1 < 0.0040  
b2 = 0.0060 0.0010 <= b2 < 0.0100  
b3 = 0.0001 0.0000 <= b3 < 0.0040  
Xq = 0.0877 0.0500 <= Xq < 0.2000  
a21 = 1.187326 1.050 <= a21 < 1.300  
a31 = 0.501823 0.300 <= a31 < 0.800



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 09/26/2023  
Time: 09:30:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080 *Lot# AG135004*  
TARGET AT 29.32: 0.078 *Exp. 12/16/23*

DIAGNOSTIC CHECK PASSED 09:32  
BLANK TEST 0.000 09:32  
INTERNAL STANDARD VERIFIED 09:32  
EXTERNAL STANDARD 0.078 09:33  
BLANK TEST 0.000 09:34  
SUBJECT SAMPLE (Vol=1.58L) 0.000 09:35  
BLANK TEST 0.000 09:36  
EXTERNAL STANDARD 0.078 09:36  
BLANK TEST 0.000 09:37

*CVL*

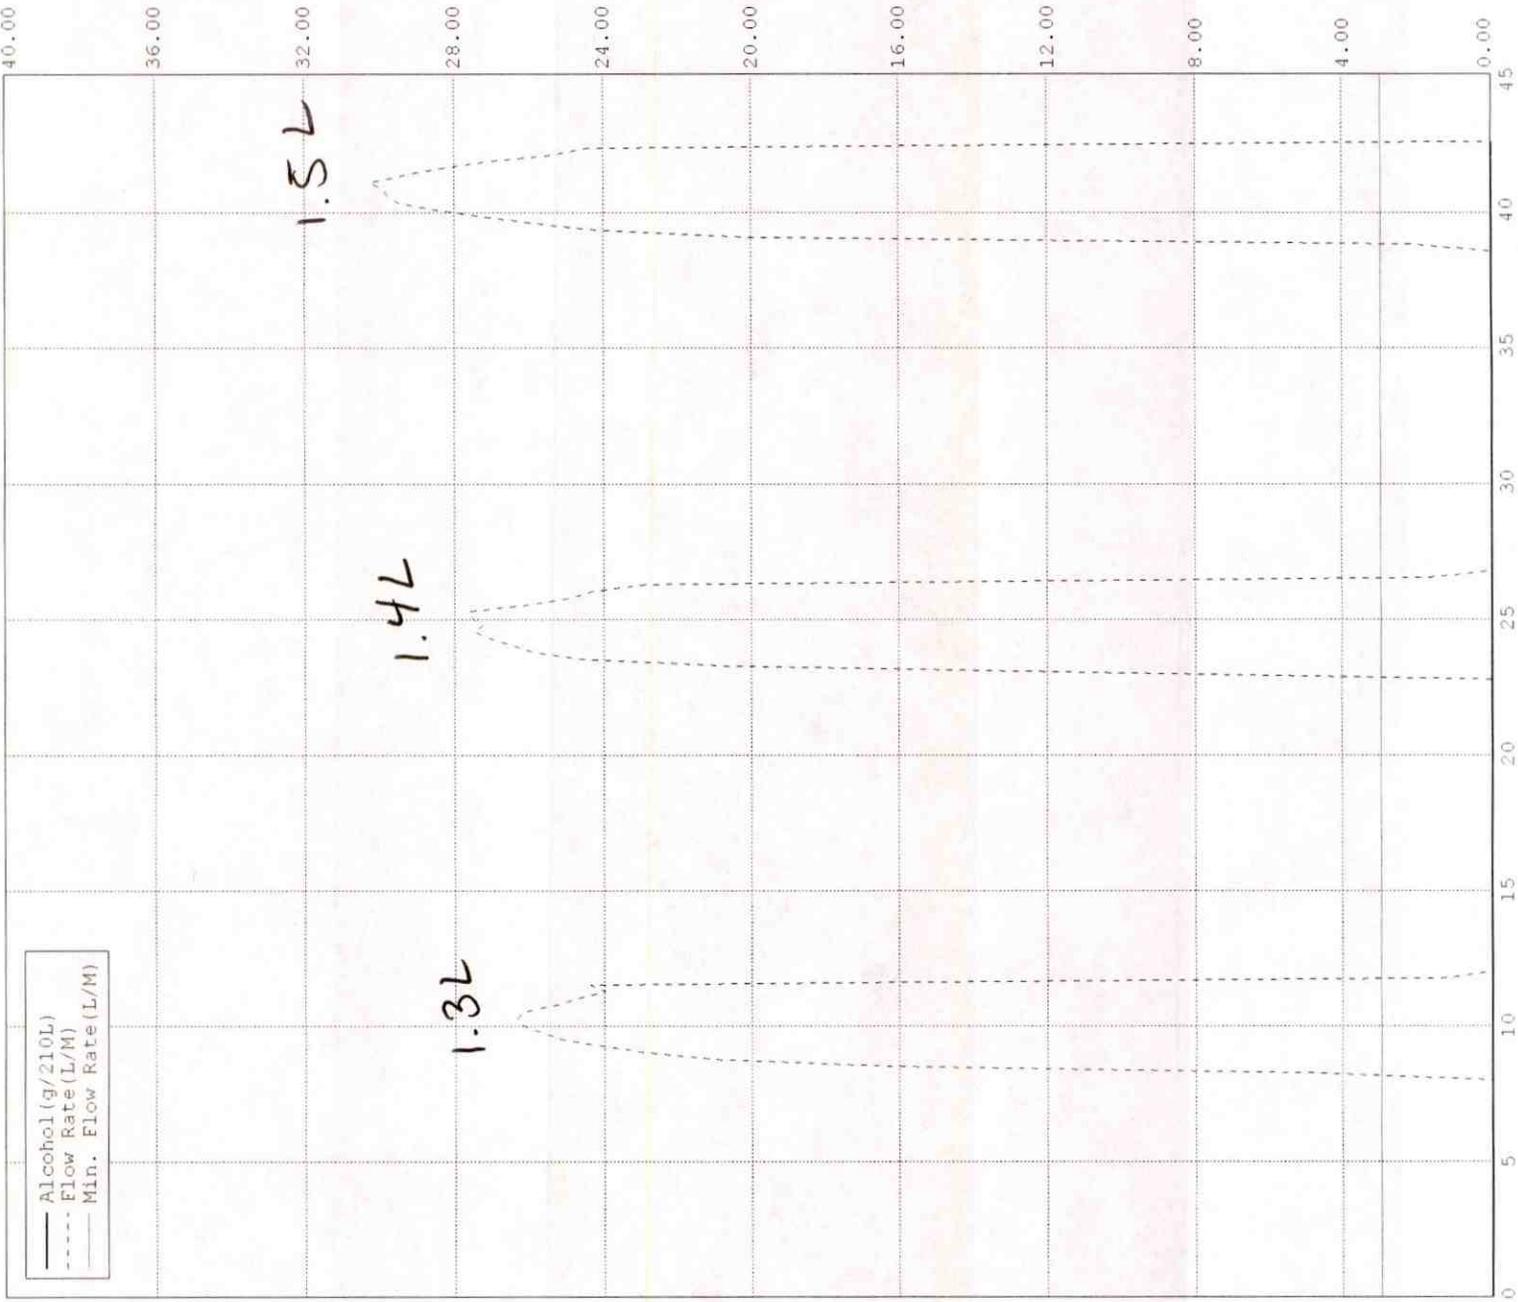

LINEARITY CHECK


-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100361  
 -----

Date: 09/26/2023  
 Time: 13:27:25

SUPERVISOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0192	0.0004
0.039	0.0392	0.0004
0.078	0.0778	0.0008
0.098	0.0978	0.0004
0.147	0.1470	0.0000
0.294	0.2952	0.0004

SLOPE = 1.005796  
 R<sup>2</sup> = 0.999989

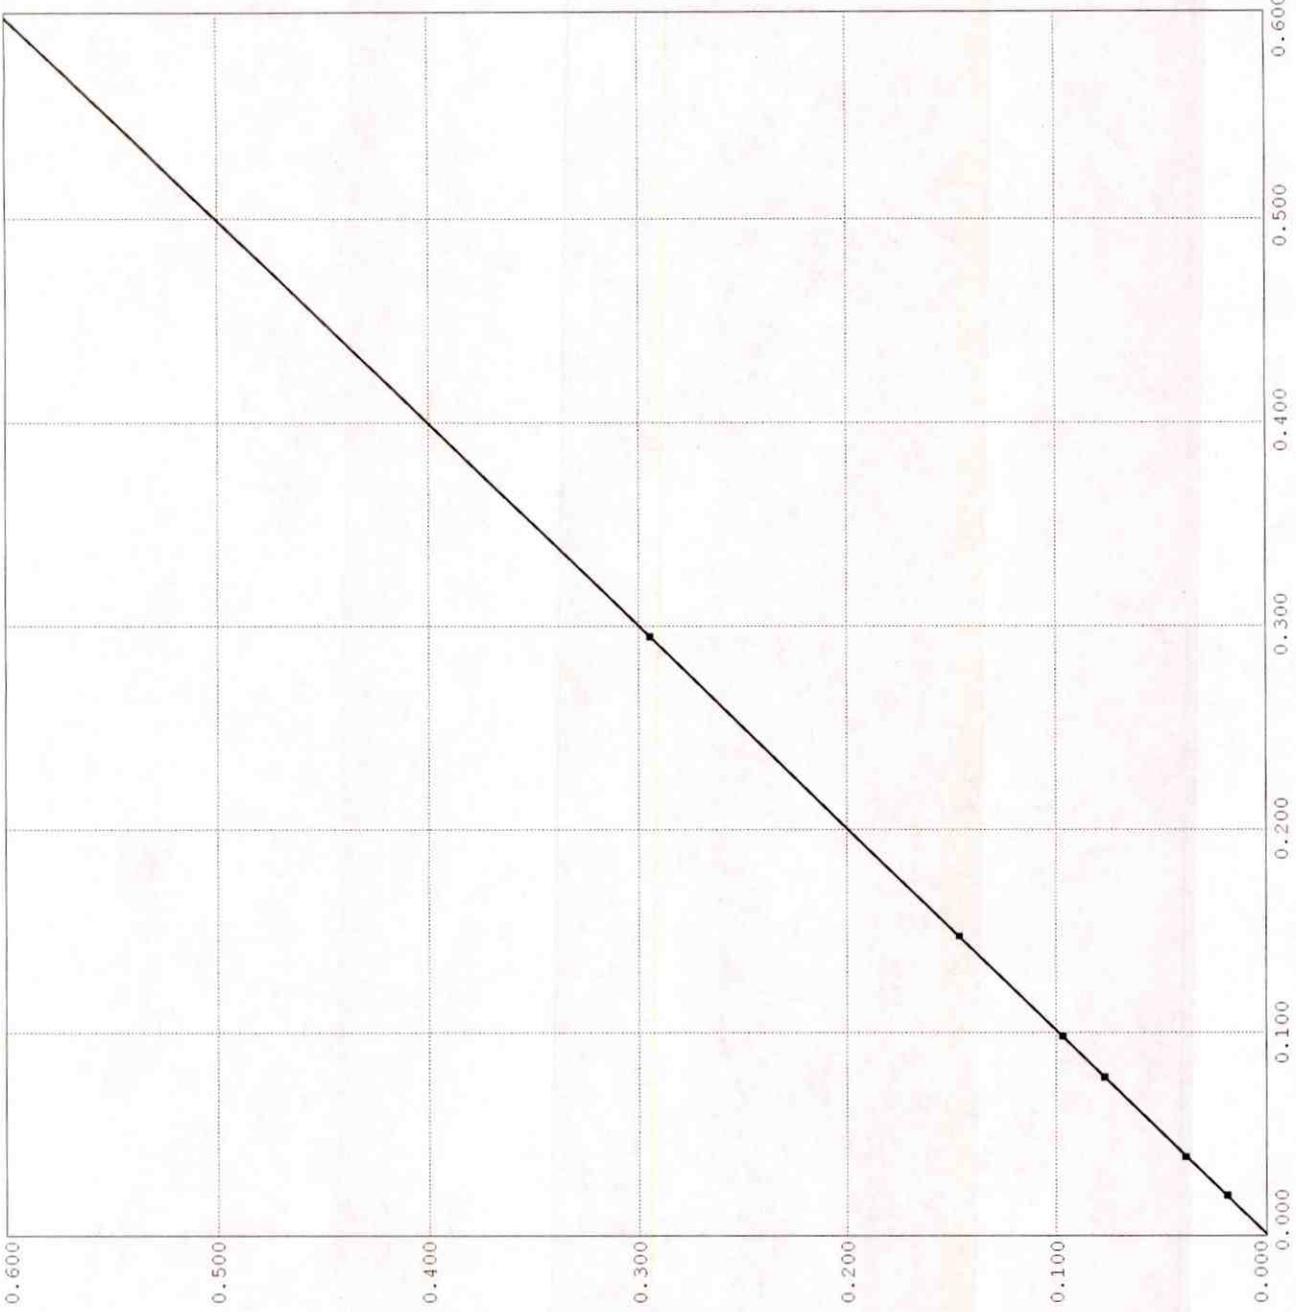

CKG

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 09/26/2023  
 Time: 13:27:28

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.30: 0.020  
 LOT #: AG217902  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 769 psi

BLANK TEST	0.000	13:28
INTERNAL STANDARD	VERIFIED	13:29
EXTERNAL STANDARD	0.019	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.019	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.019	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.019	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.020	13:33
BLANK TEST	0.000	13:34

Average = 0.0192  
 Std Dev = 0.0004

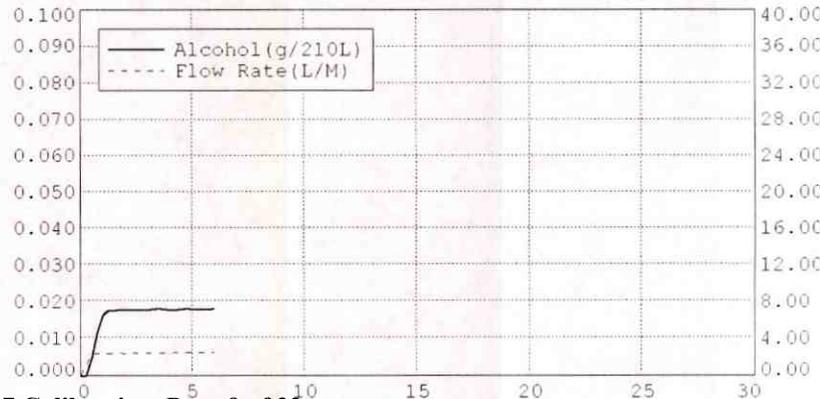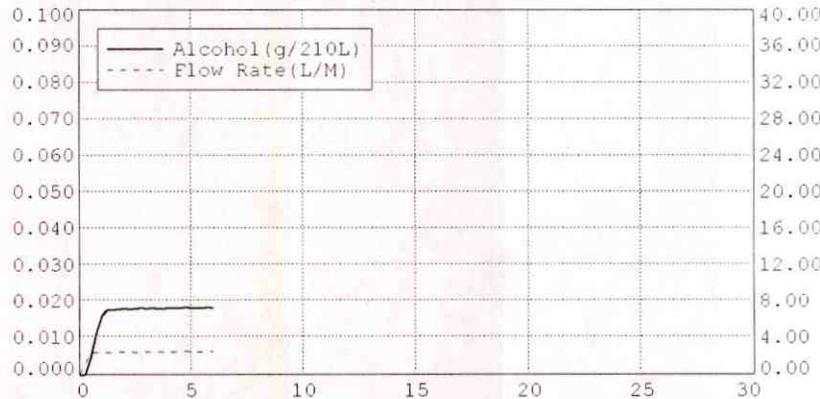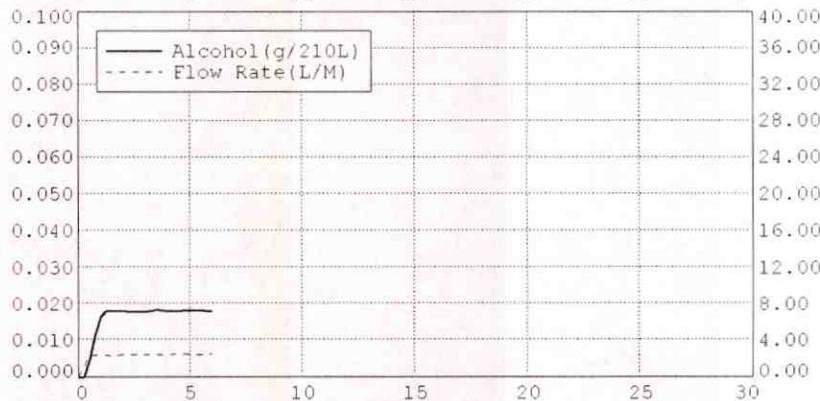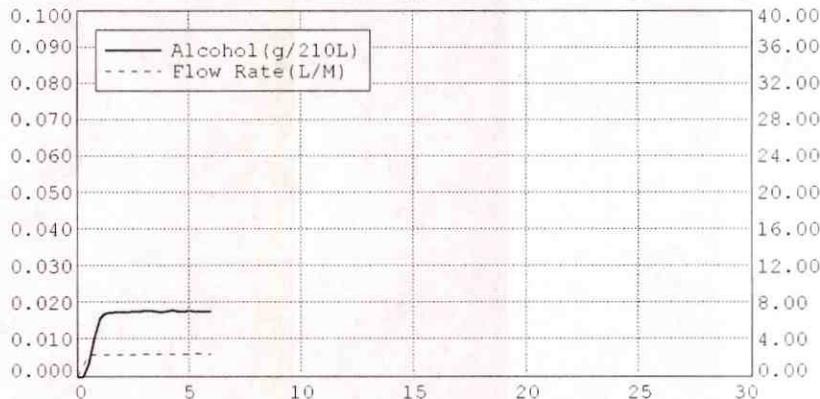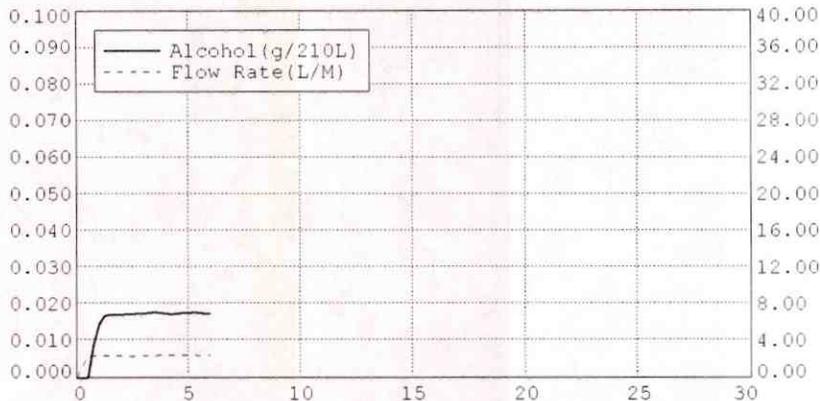

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 09/26/2023  
 Time: 13:35:21

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.30: 0.039  
 LOT #: AG217904  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 997 psi

BLANK TEST	0.000	13:36
INTERNAL STANDARD	VERIFIED	13:36
EXTERNAL STANDARD	0.039	13:37
BLANK TEST	0.000	13:37
EXTERNAL STANDARD	0.039	13:38
BLANK TEST	0.000	13:39
EXTERNAL STANDARD	0.040	13:39
BLANK TEST	0.000	13:40
EXTERNAL STANDARD	0.039	13:40
BLANK TEST	0.000	13:41
EXTERNAL STANDARD	0.039	13:41
BLANK TEST	0.000	13:42

Average = 0.0392  
 Std Dev = 0.0004

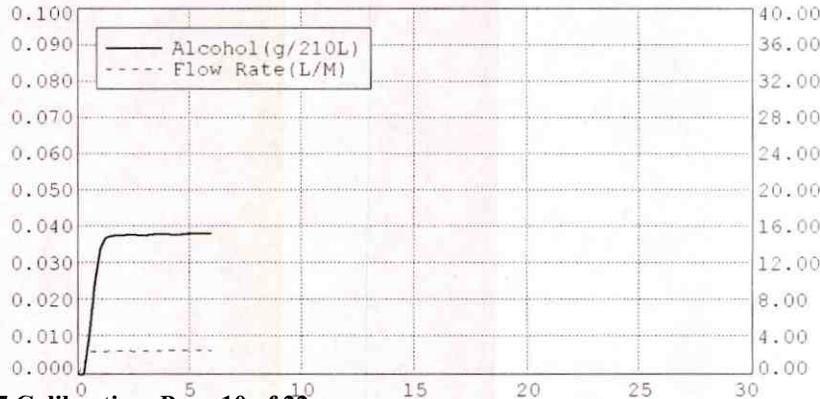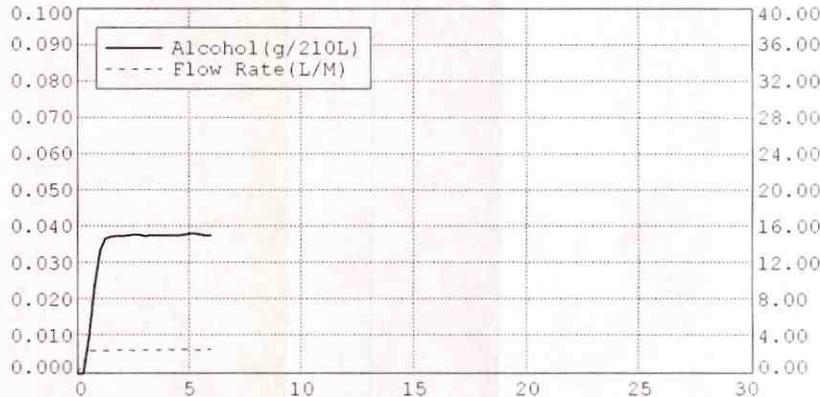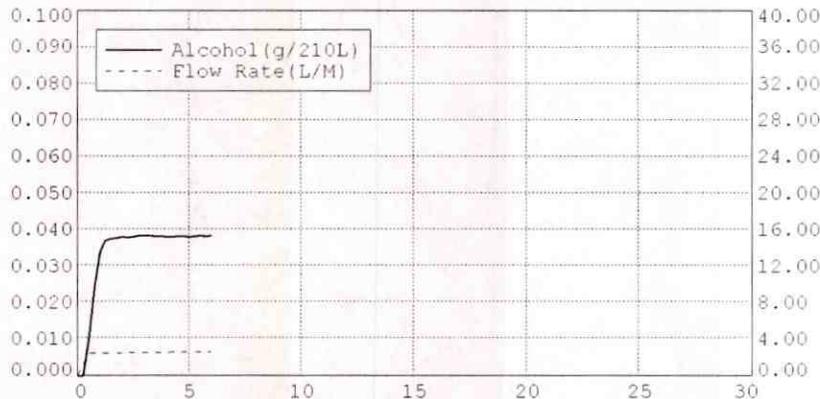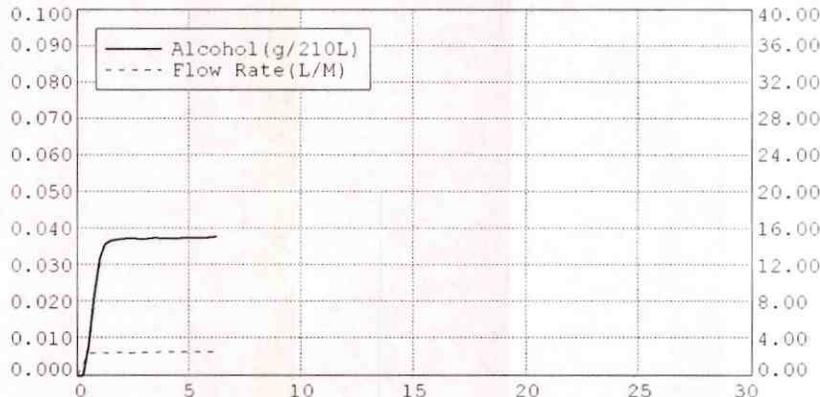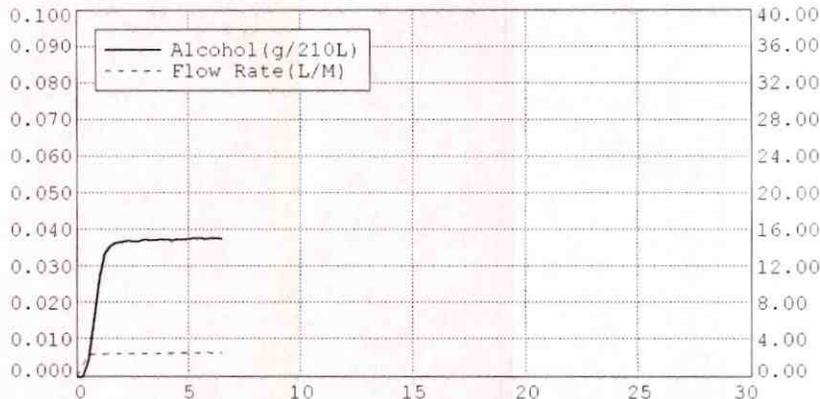

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 09/26/2023  
 Time: 13:43:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.30: 0.078  
 LOT #: AG135004  
 EXPIRATION: 12/16/2023  
 TANK PRESSURE: 287 psi

BLANK TEST	0.000	13:45
INTERNAL STANDARD	VERIFIED	13:45
EXTERNAL STANDARD	0.078	13:45
BLANK TEST	0.000	13:46
EXTERNAL STANDARD	0.077	13:46
BLANK TEST	0.000	13:47
EXTERNAL STANDARD	0.079	13:47
BLANK TEST	0.000	13:48
EXTERNAL STANDARD	0.077	13:48
BLANK TEST	0.000	13:49
EXTERNAL STANDARD	0.078	13:49
BLANK TEST	0.000	13:50

Average = 0.0778  
 Std Dev = 0.0008

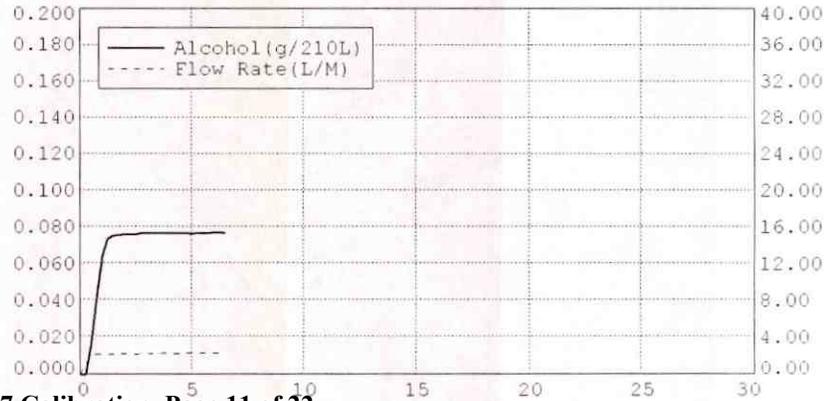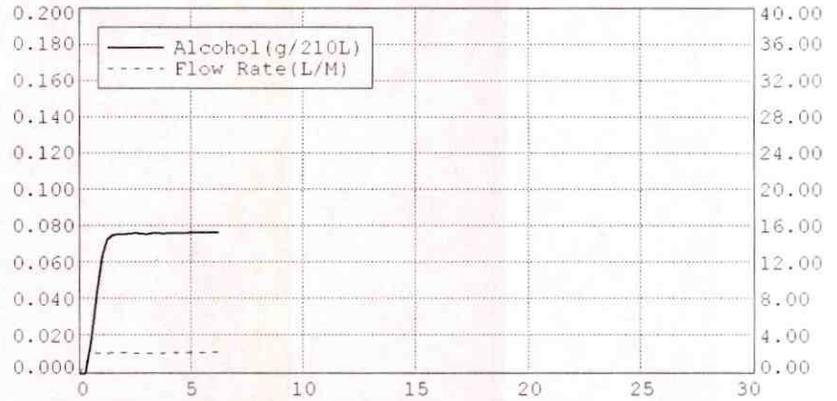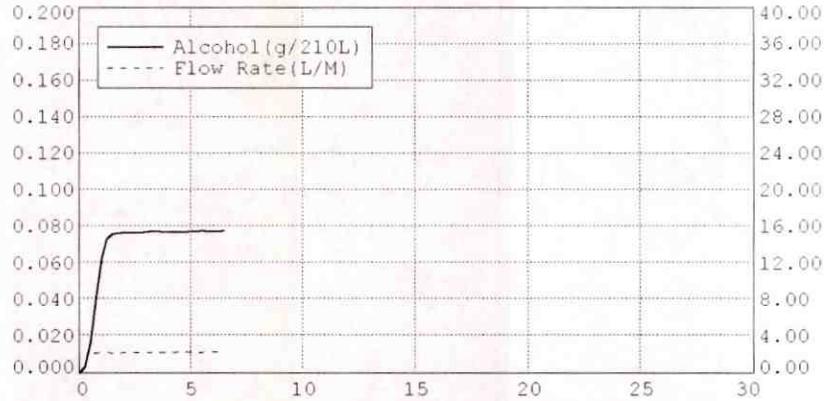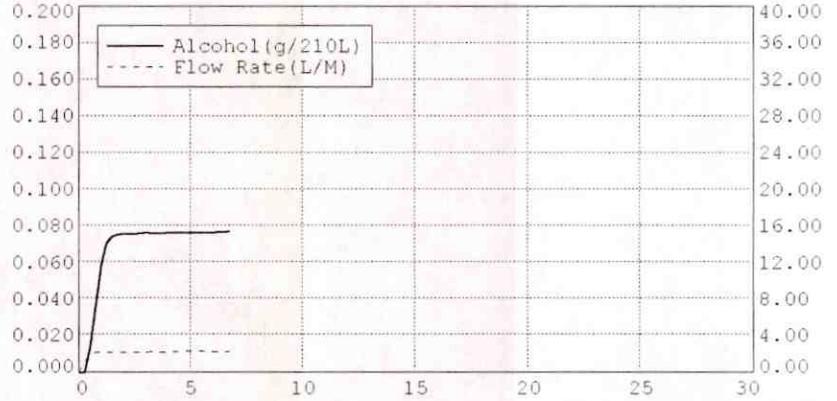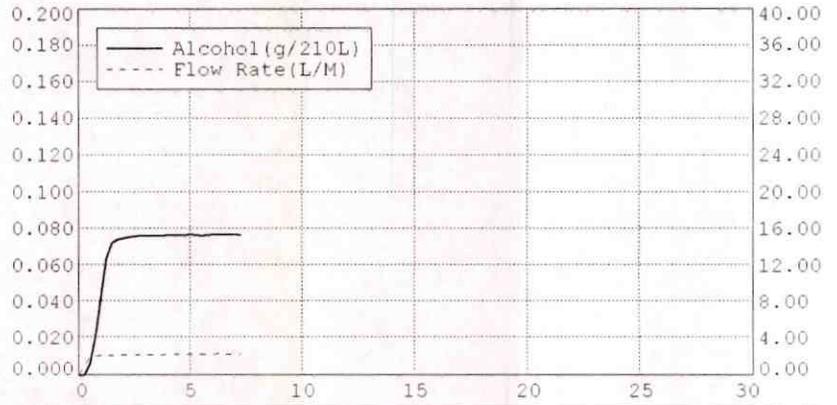

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
DATAMASTER dmt: 100361






Date: 09/26/2023  
Time: 13:52:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
TARGET AT 29.30: 0.098  
LOT #: AG211003  
EXPIRATION: 04/20/2024  
TANK PRESSURE: 847 psi

BLANK TEST	0.000	13:54
INTERNAL STANDARD	VERIFIED	13:54
EXTERNAL STANDARD	0.098	13:54
BLANK TEST	0.000	13:55
EXTERNAL STANDARD	0.098	13:55
BLANK TEST	0.000	13:56
EXTERNAL STANDARD	0.098	13:57
BLANK TEST	0.000	13:57
EXTERNAL STANDARD	0.098	13:58
BLANK TEST	0.000	13:59
EXTERNAL STANDARD	0.097	13:59
BLANK TEST	0.000	14:00

Average = 0.0978  
Std Dev = 0.0004

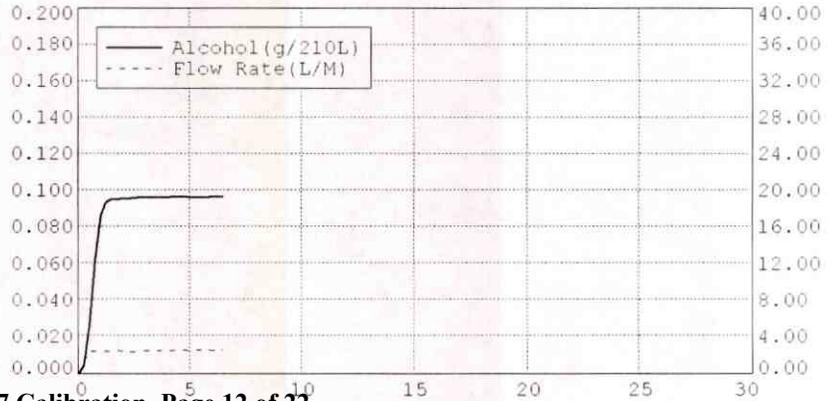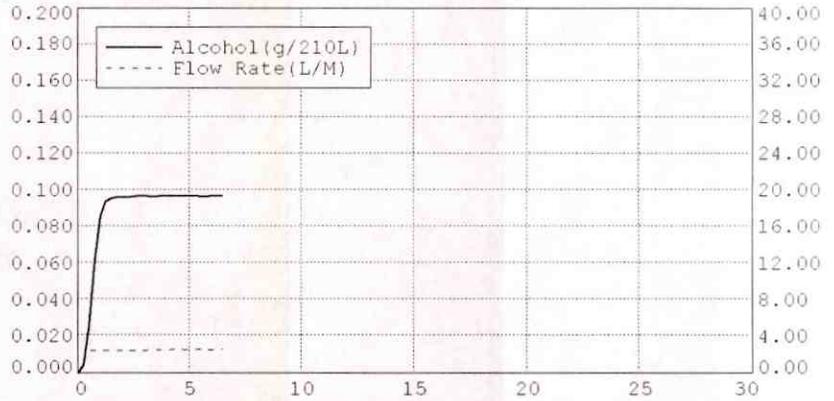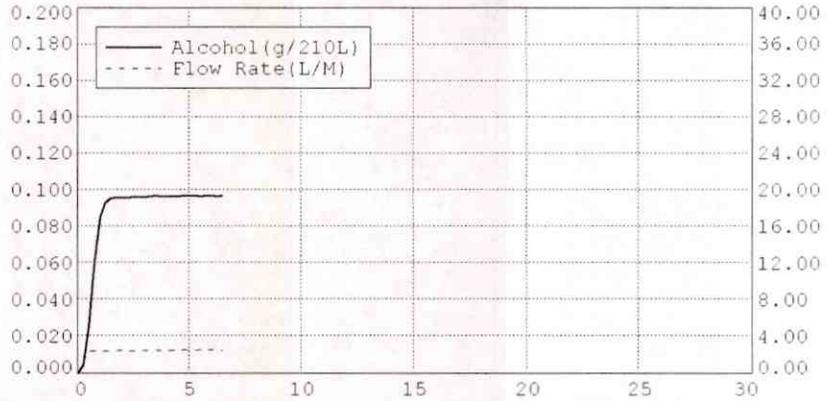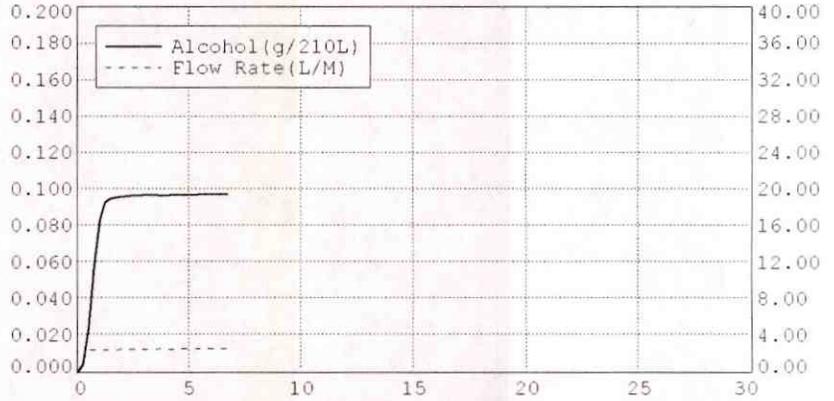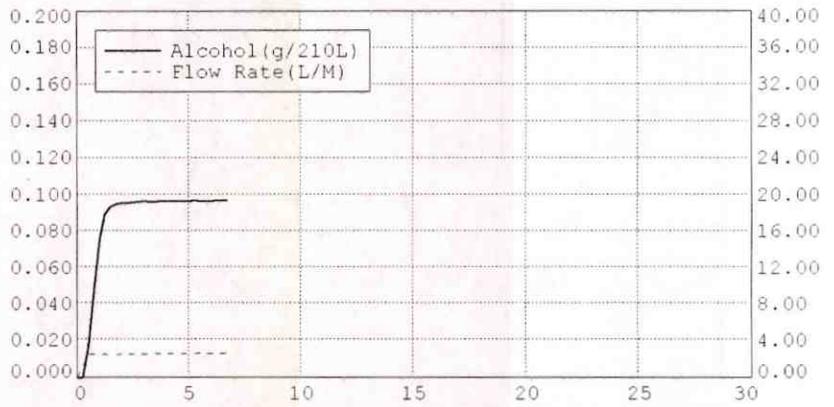

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 09/26/2023  
 Time: 14:01:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.30: 0.147  
 LOT #: AG134205  
 EXPIRATION: 12/08/2023  
 TANK PRESSURE: 936 psi

BLANK TEST	0.000	14:02
INTERNAL STANDARD	VERIFIED	14:02
EXTERNAL STANDARD	0.147	14:02
BLANK TEST	0.000	14:03
EXTERNAL STANDARD	0.147	14:04
BLANK TEST	0.000	14:04
EXTERNAL STANDARD	0.147	14:05
BLANK TEST	0.000	14:06
EXTERNAL STANDARD	0.147	14:06
BLANK TEST	0.000	14:07
EXTERNAL STANDARD	0.147	14:07
BLANK TEST	0.000	14:08

Average = 0.1470  
 Std Dev = 0.0000

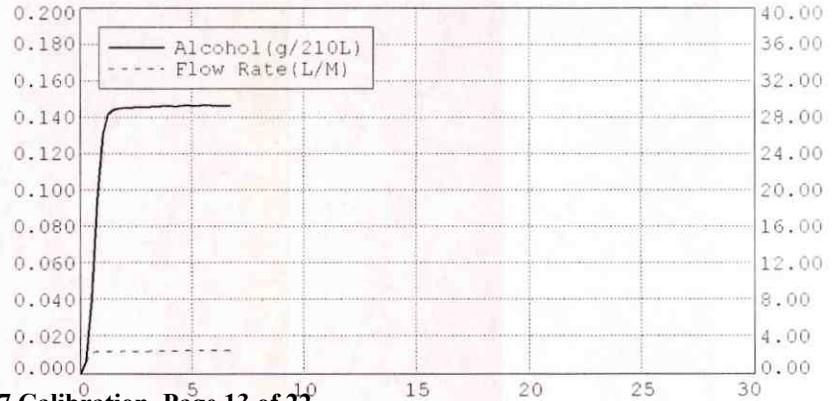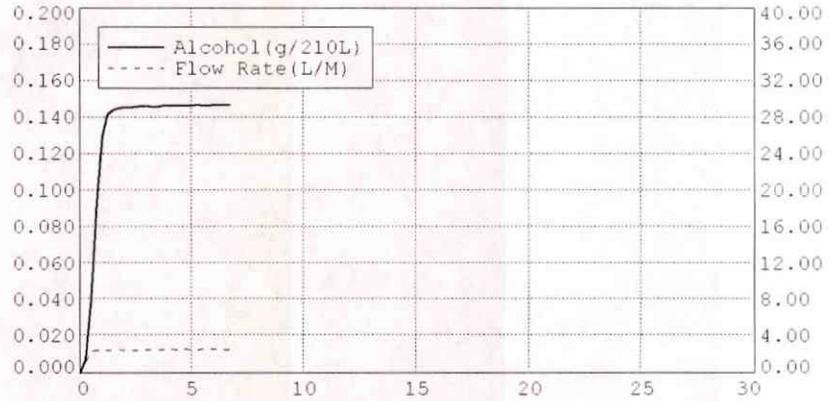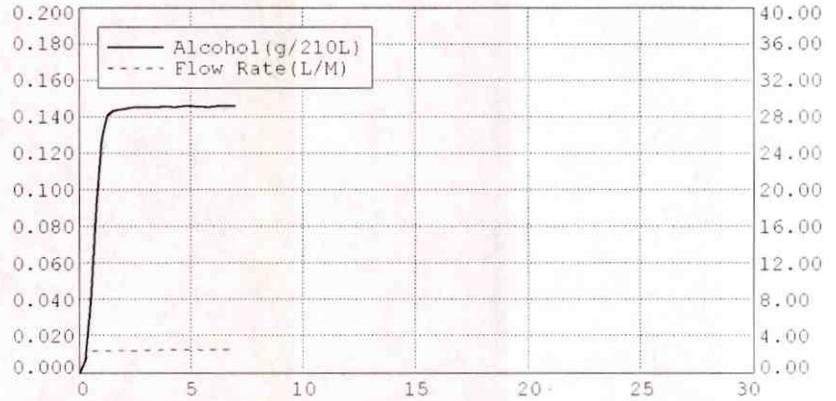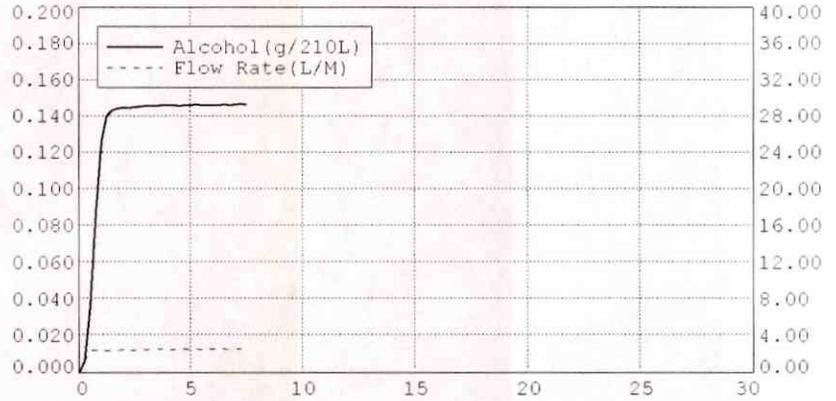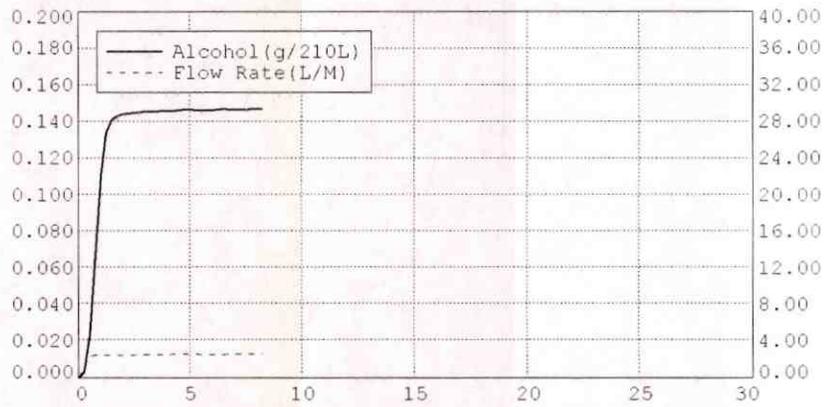

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100361






Date: 09/26/2023  
 Time: 14:10:54

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.30: 0.294  
 LOT #: AG217903  
 EXPIRATION: 06/28/2024  
 TANK PRESSURE: 213 psi

BLANK TEST	0.000	14:12
INTERNAL STANDARD	VERIFIED	14:12
EXTERNAL STANDARD	0.296	14:12
BLANK TEST	0.000	14:13
EXTERNAL STANDARD	0.295	14:13
BLANK TEST	0.000	14:14
EXTERNAL STANDARD	0.295	14:15
BLANK TEST	0.000	14:15
EXTERNAL STANDARD	0.295	14:16
BLANK TEST	0.000	14:17
EXTERNAL STANDARD	0.295	14:17
BLANK TEST	0.000	14:18

Average = 0.2952  
 Std Dev = 0.0004

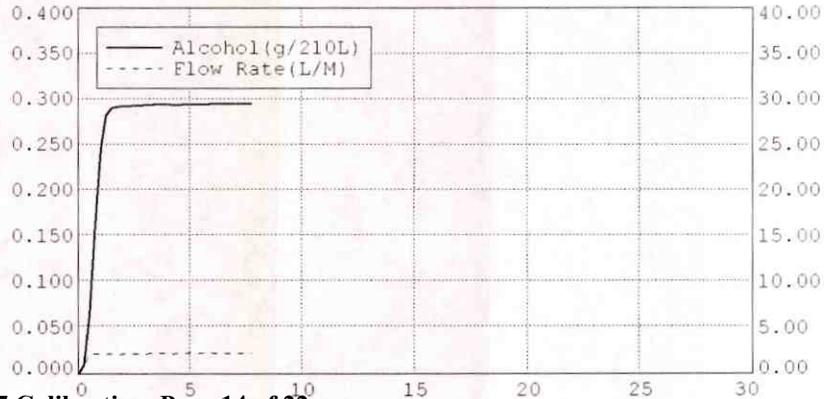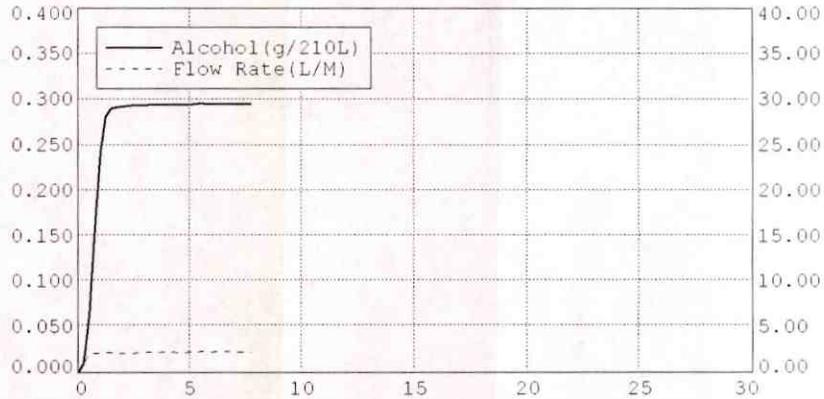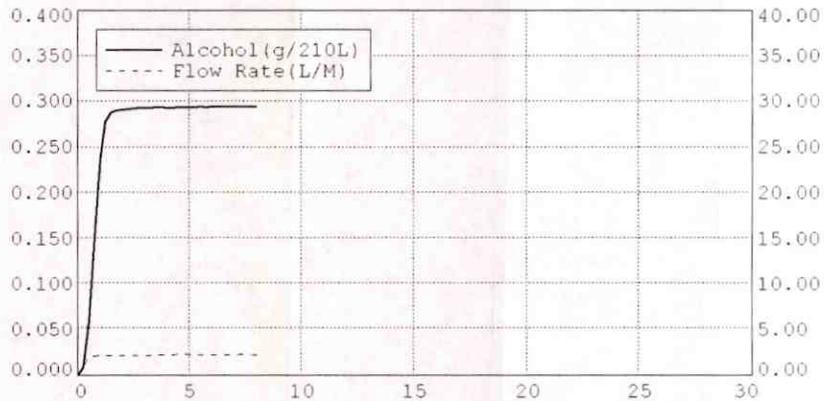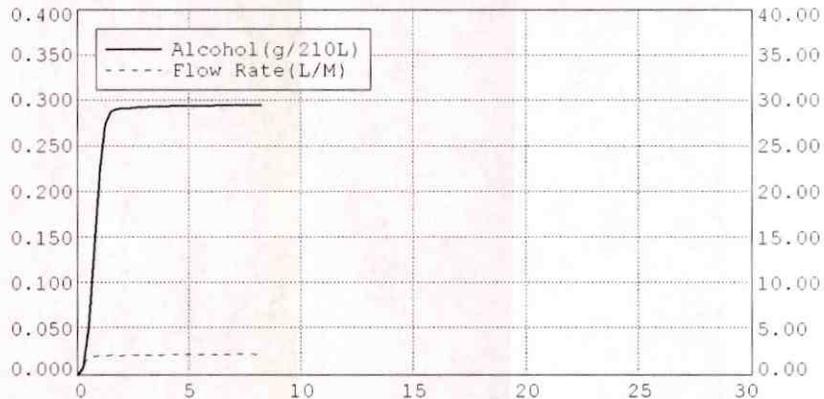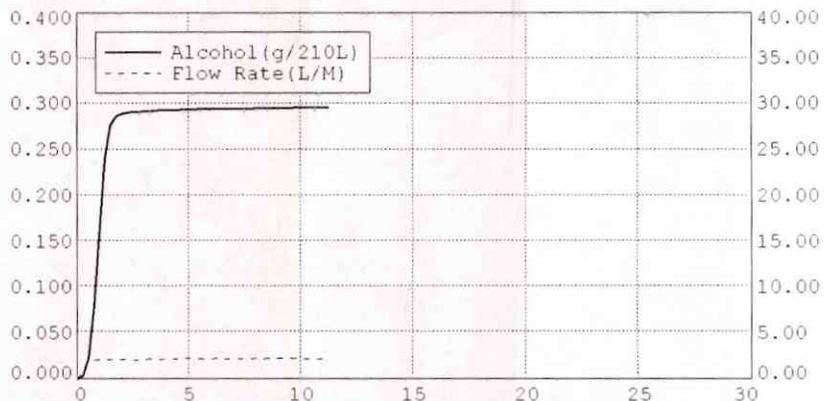

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 09/26/2023  
Time: 14:28:32

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080 Lot # AG-135004  
TARGET AT 29.30: 0.078 Exp: 12/16/23

DIAGNOSTIC CHECK PASSED 14:30  
BLANK TEST 0.000 14:30  
INTERNAL STANDARD VERIFIED 14:31  
EXTERNAL STANDARD 0.079 14:31  
BLANK TEST 0.000 14:32  
SUBJECT SAMPLE INCOMPLETE 14:34

CKG

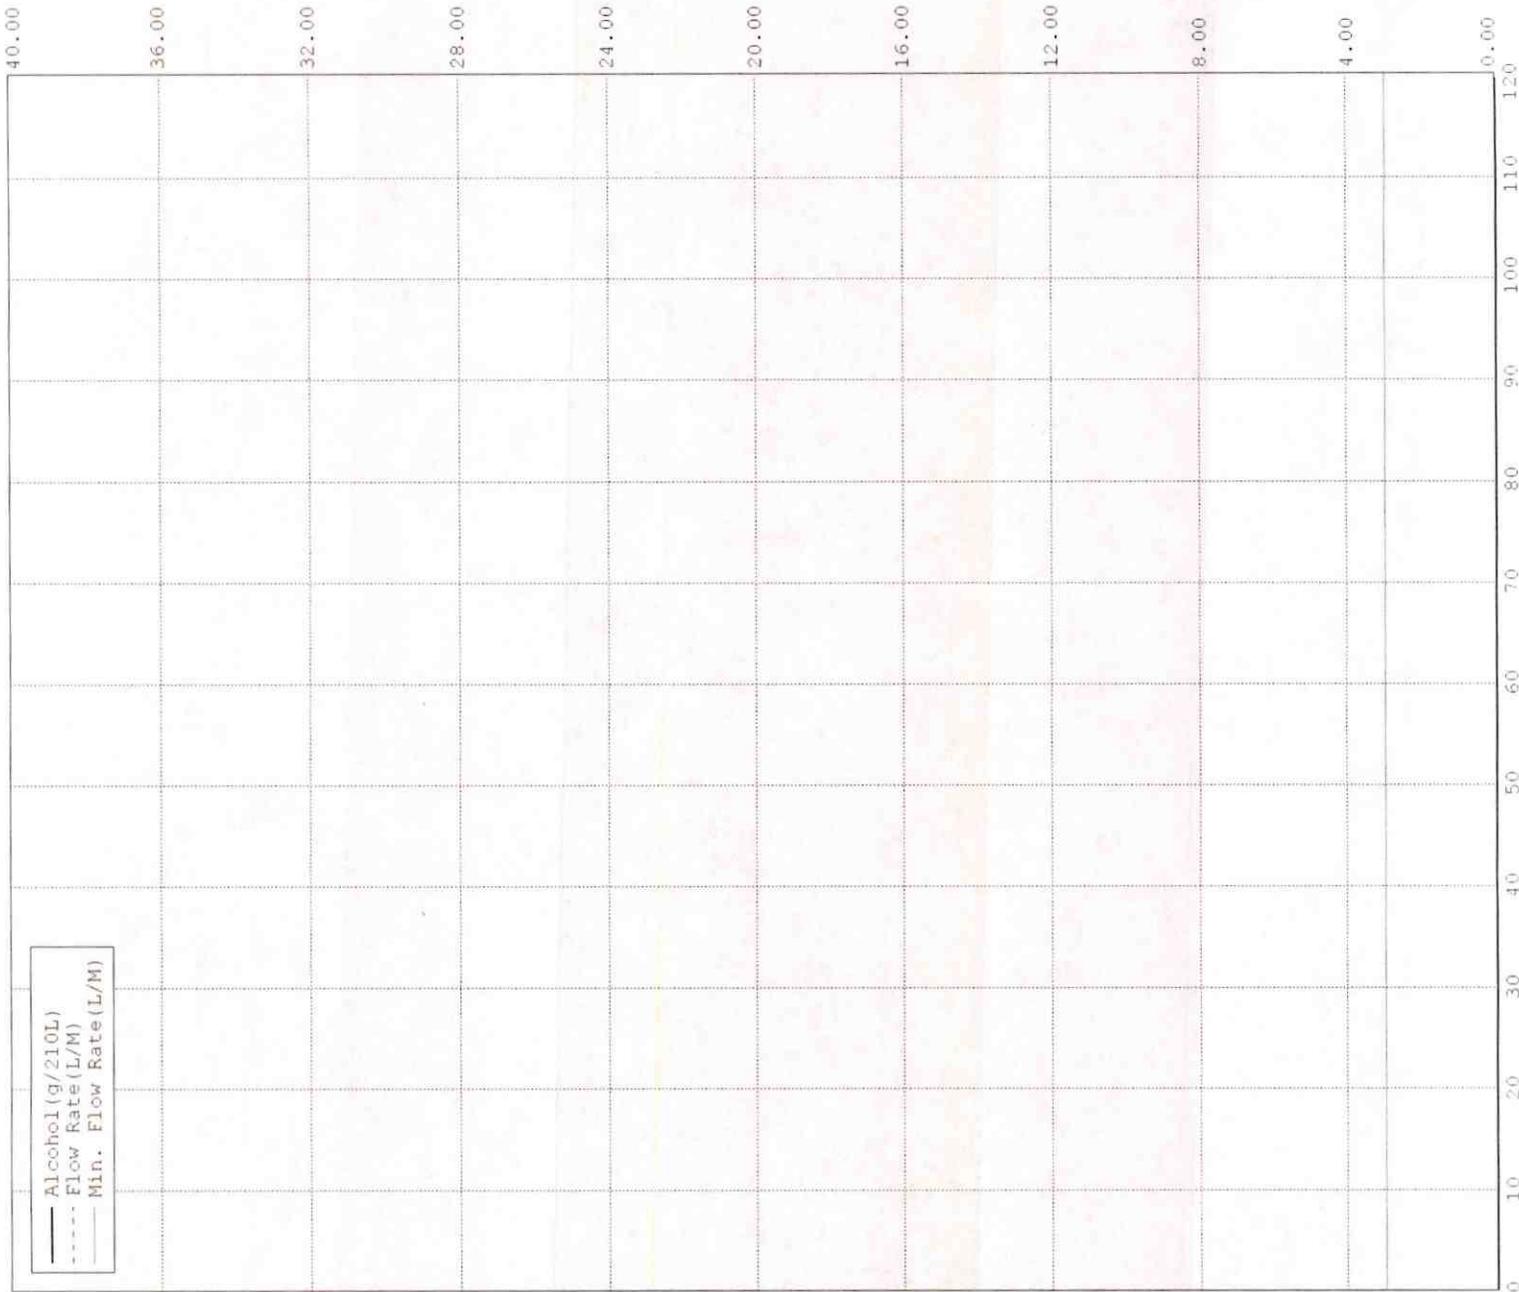

SUBJECT TEST

Alaska Department of Public Safety  
DATA MASTER dmt: 100361

Date: 09/26/2023  
Time: 14:37:18

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
MAXIMUM ATTEMPTS EXCEEDED  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080 Lot # 196-135004  
TARGET AT 29.30: 0.078 Exp: 12/16/23

DIAGNOSTIC CHECK PASSED 14:38  
BLANK TEST 0.000 14:38  
INTERNAL STANDARD VERIFIED 14:38  
EXTERNAL STANDARD 0.078 14:38  
BLANK TEST 0.000 14:39  
SUBJECT SAMPLE XXX 14:41

Maximum Attempts Exceeded

OKG

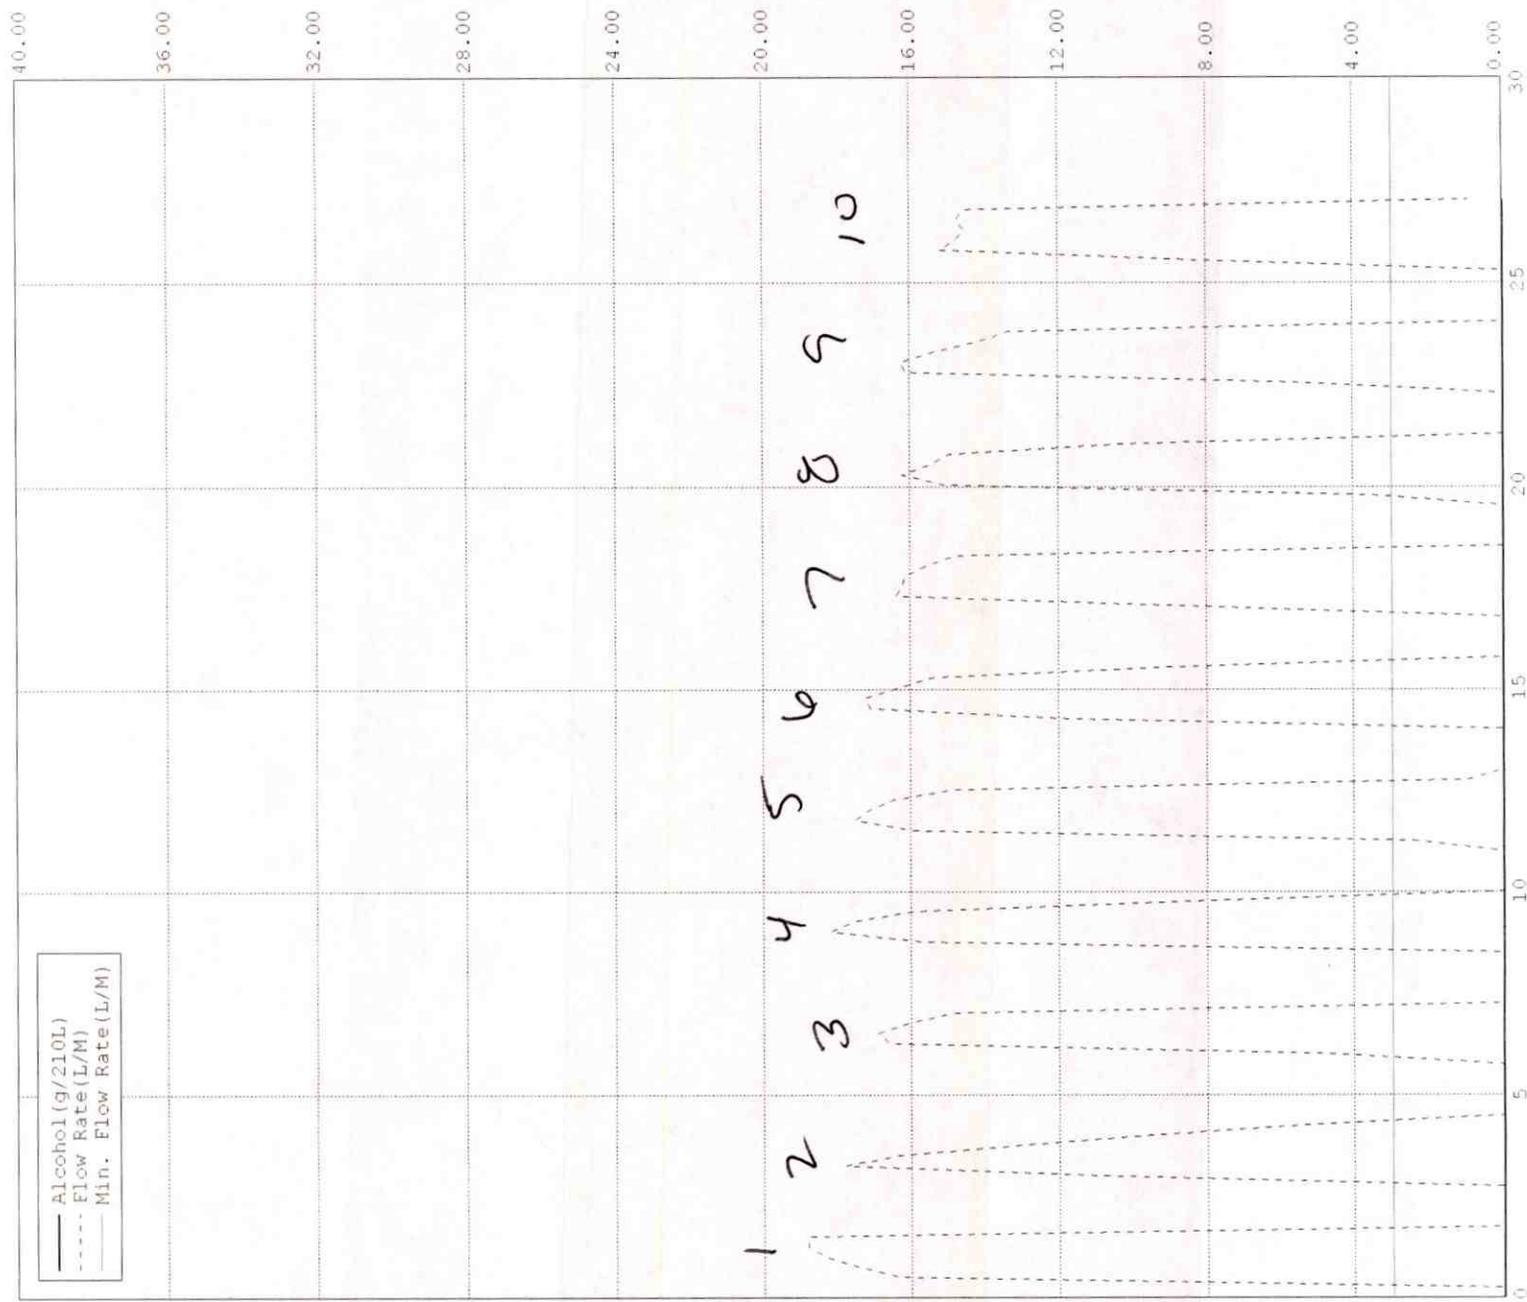

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 09/26/2023  
Time: 15:20:11

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.30: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 15:21  
BLANK TEST 0.000 15:21  
INTERNAL STANDARD VERIFIED 15:21  
EXTERNAL STANDARD 0.078 15:21  
BLANK TEST 0.000 15:22  
SUBJECT SAMPLE INVALID 15:25

OK

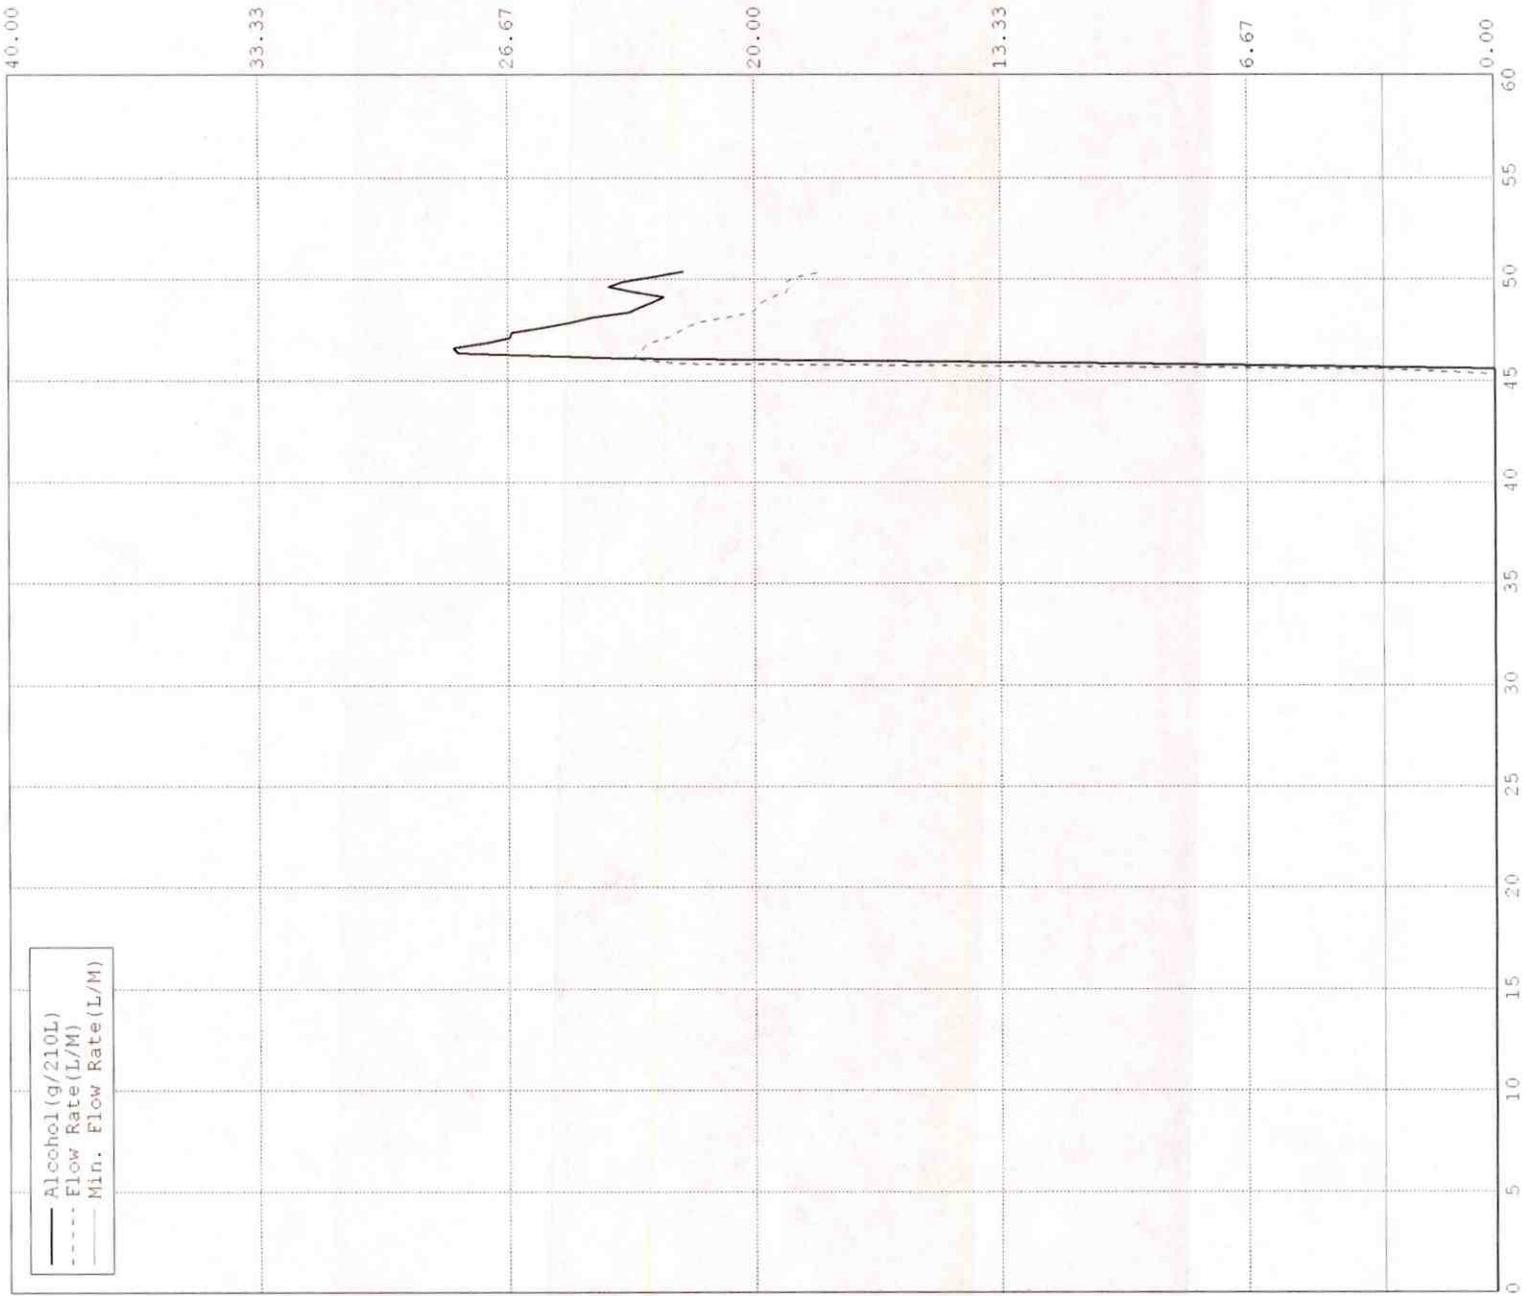

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 09/26/2023  
Time: 14:50:23

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
RFI  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.30: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK PASSED 14:51  
BLANK TEST 0.000 14:51  
INTERNAL STANDARD VERIFIED 14:51  
EXTERNAL STANDARD 0.077 14:52  
BLANK TEST 0.000 14:52

RFI DETECTED

CKG

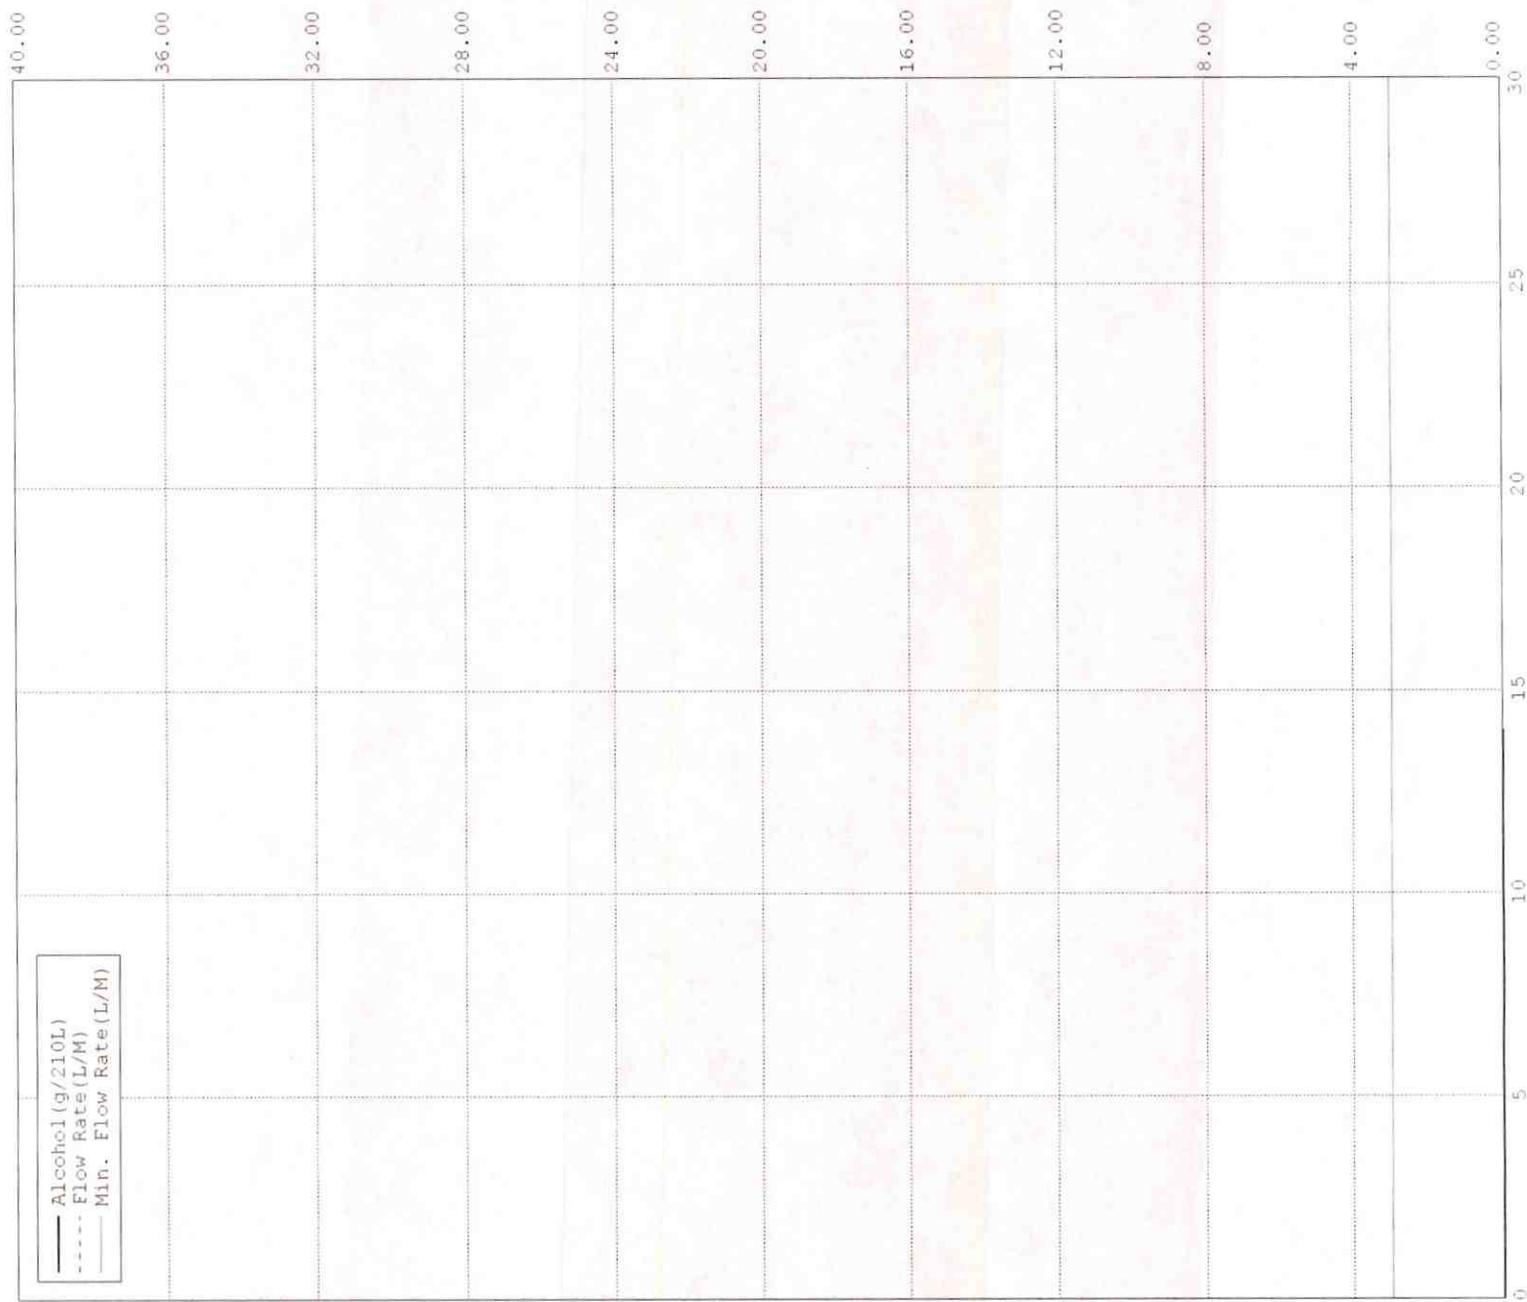

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 09/26/2023  
Time: 15:37:26

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - ACETONE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080  
TARGET AT 29.30: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	15:38
BLANK TEST	0.000	15:38
INTERNAL STANDARD	VERIFIED	15:38
Xg = 0.089 (1.49%)		
EXTERNAL STANDARD	0.078	15:39
X[1] = 0.0779 (-0.0012) (0.0026)		
BLANK TEST	0.000	15:40
SUBJECT SAMPLE	XXX	15:40
X[1] = 0.1115 (-0.0239) (0.0002)		

Interference Detected

Filter 2 Average = -0.0011  
Filter 3 Average = 0.0027  
OMG 9/27/23

CKG

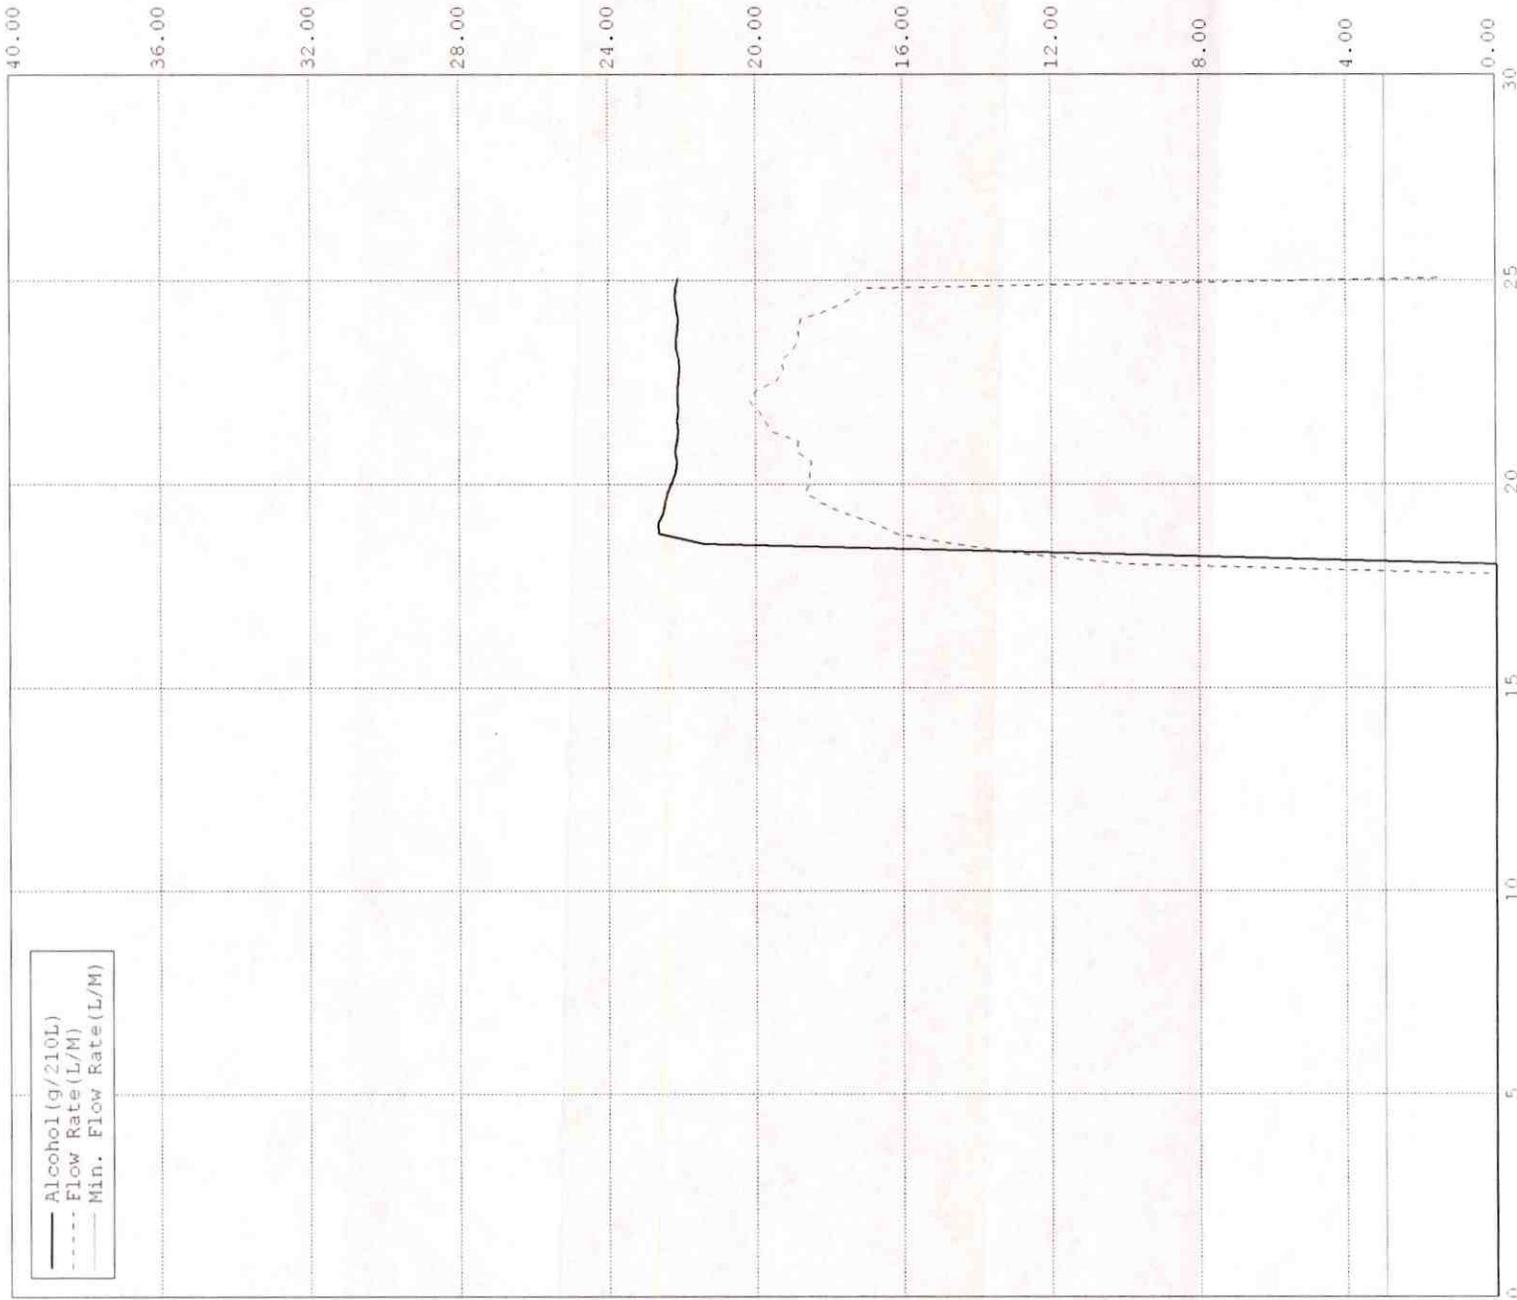

SUBJECT TEST

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100361  
-----

Date: 09/26/2023  
Time: 15:30:45

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX

OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436

DEPT/AGENCY:  
INTERFERENCE - IPA  
CASE/REPORT: XXXX  
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.30: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	15:32
BLANK TEST	0.000	15:32
INTERNAL STANDARD	VERIFIED	15:32
Xq = 0.088 (0.10%)		
EXTERNAL STANDARD	0.077	15:32
X[1] = 0.0774 (-0.0009)	(0.0028)	
BLANK TEST	0.000	15:33
SUBJECT SAMPLE	XXX	15:34
X[1] = 0.1261 (-0.0314)	(0.0026)	

Interference Detected

CXB

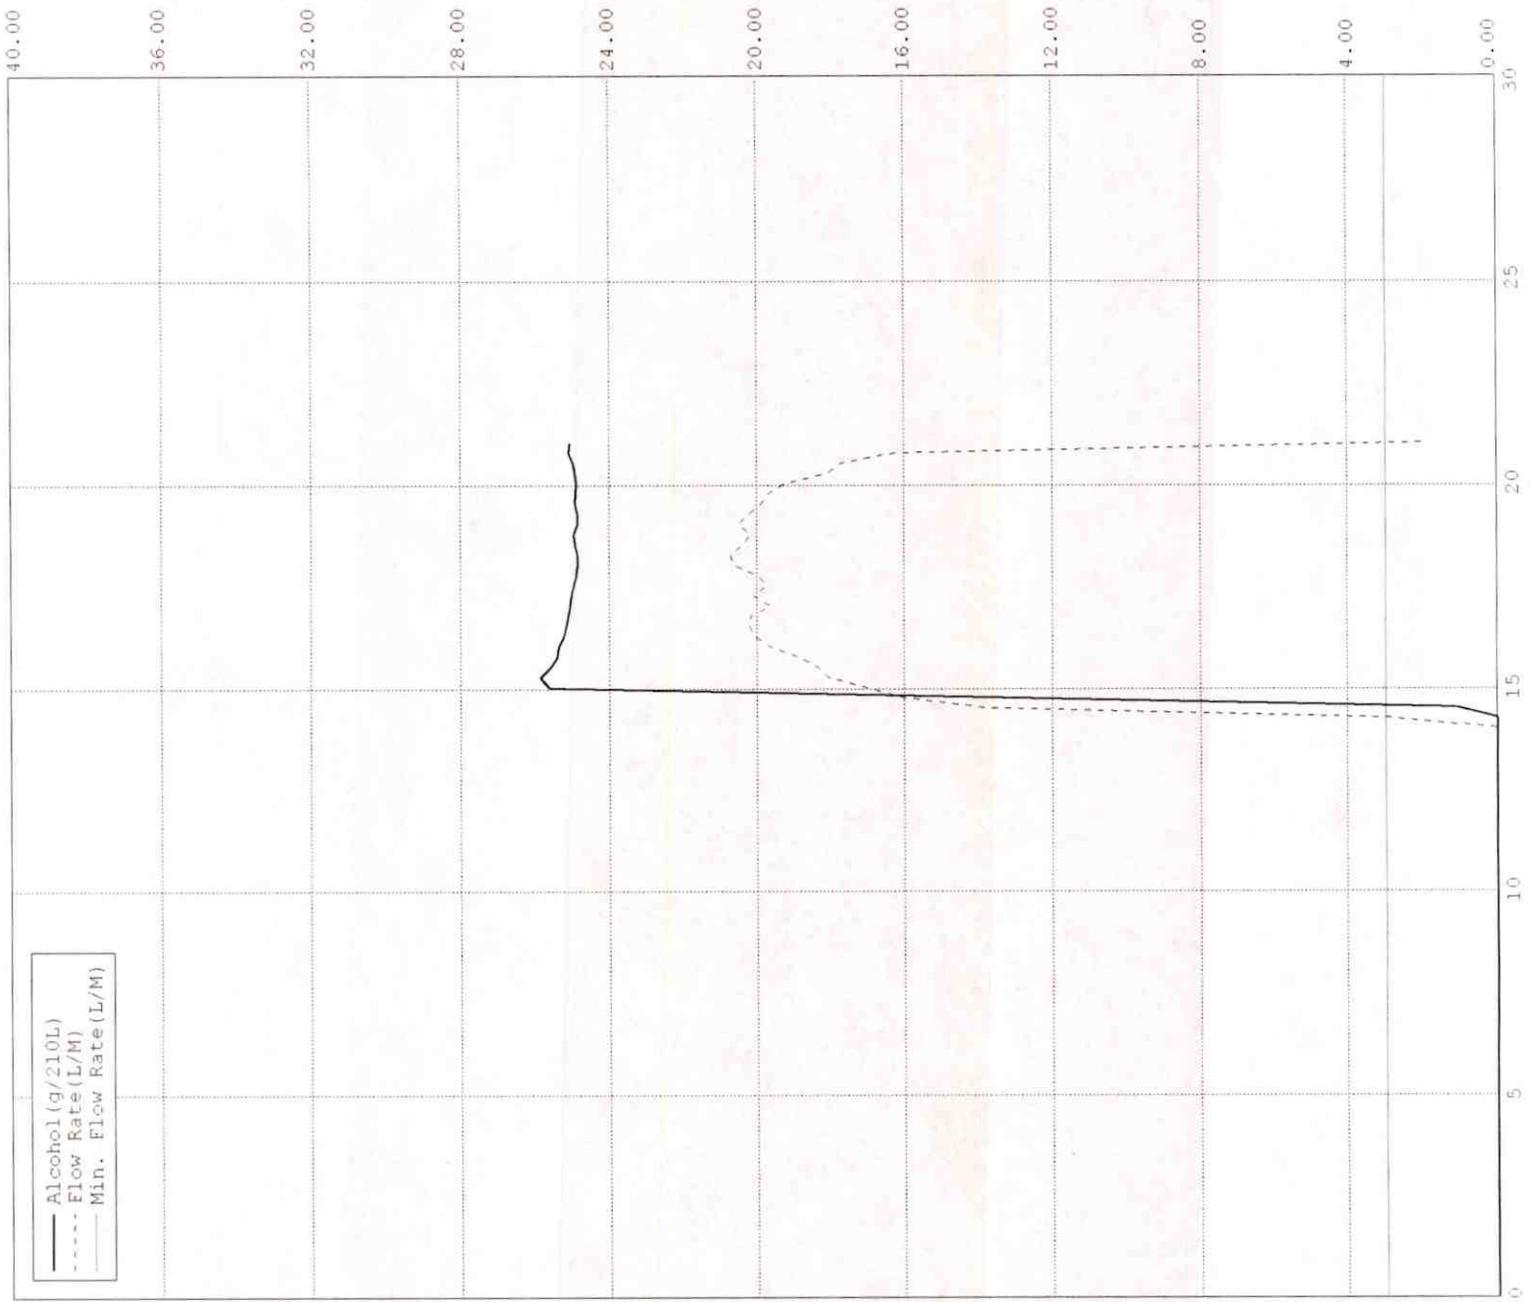

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100361

Date: 09/26/2023  
Time: 15:43:02

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXXX


OPERATOR NAME:  
CARLIE GLAISTER  
OPERATOR'S #: 10436


DEPT/AGENCY:  
INTERFERENCE - NEGATIVE  
CASE/REPORT: XXXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.30: 0.078  
LOT #: AG135004  
EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	15:44
BLANK TEST	0.000	15:44
INTERNAL STANDARD	VERIFIED	15:44
Xq = 0.088 (0.50%)	0.078	15:44
X[1] = 0.0780 (-0.0010)	(0.0025)	15:45
BLANK TEST	0.000	15:46
SUBJECT SAMPLE (Vol=2.10L)	0.096	15:46
X[1] = 0.0969 (-0.0003)	(0.0014)	15:47
BLANK TEST	0.000	15:47
EXTERNAL STANDARD	0.077	15:47
X[1] = 0.0766 (-0.0011)	(0.0028)	15:48
BLANK TEST	0.000	15:48

Q166

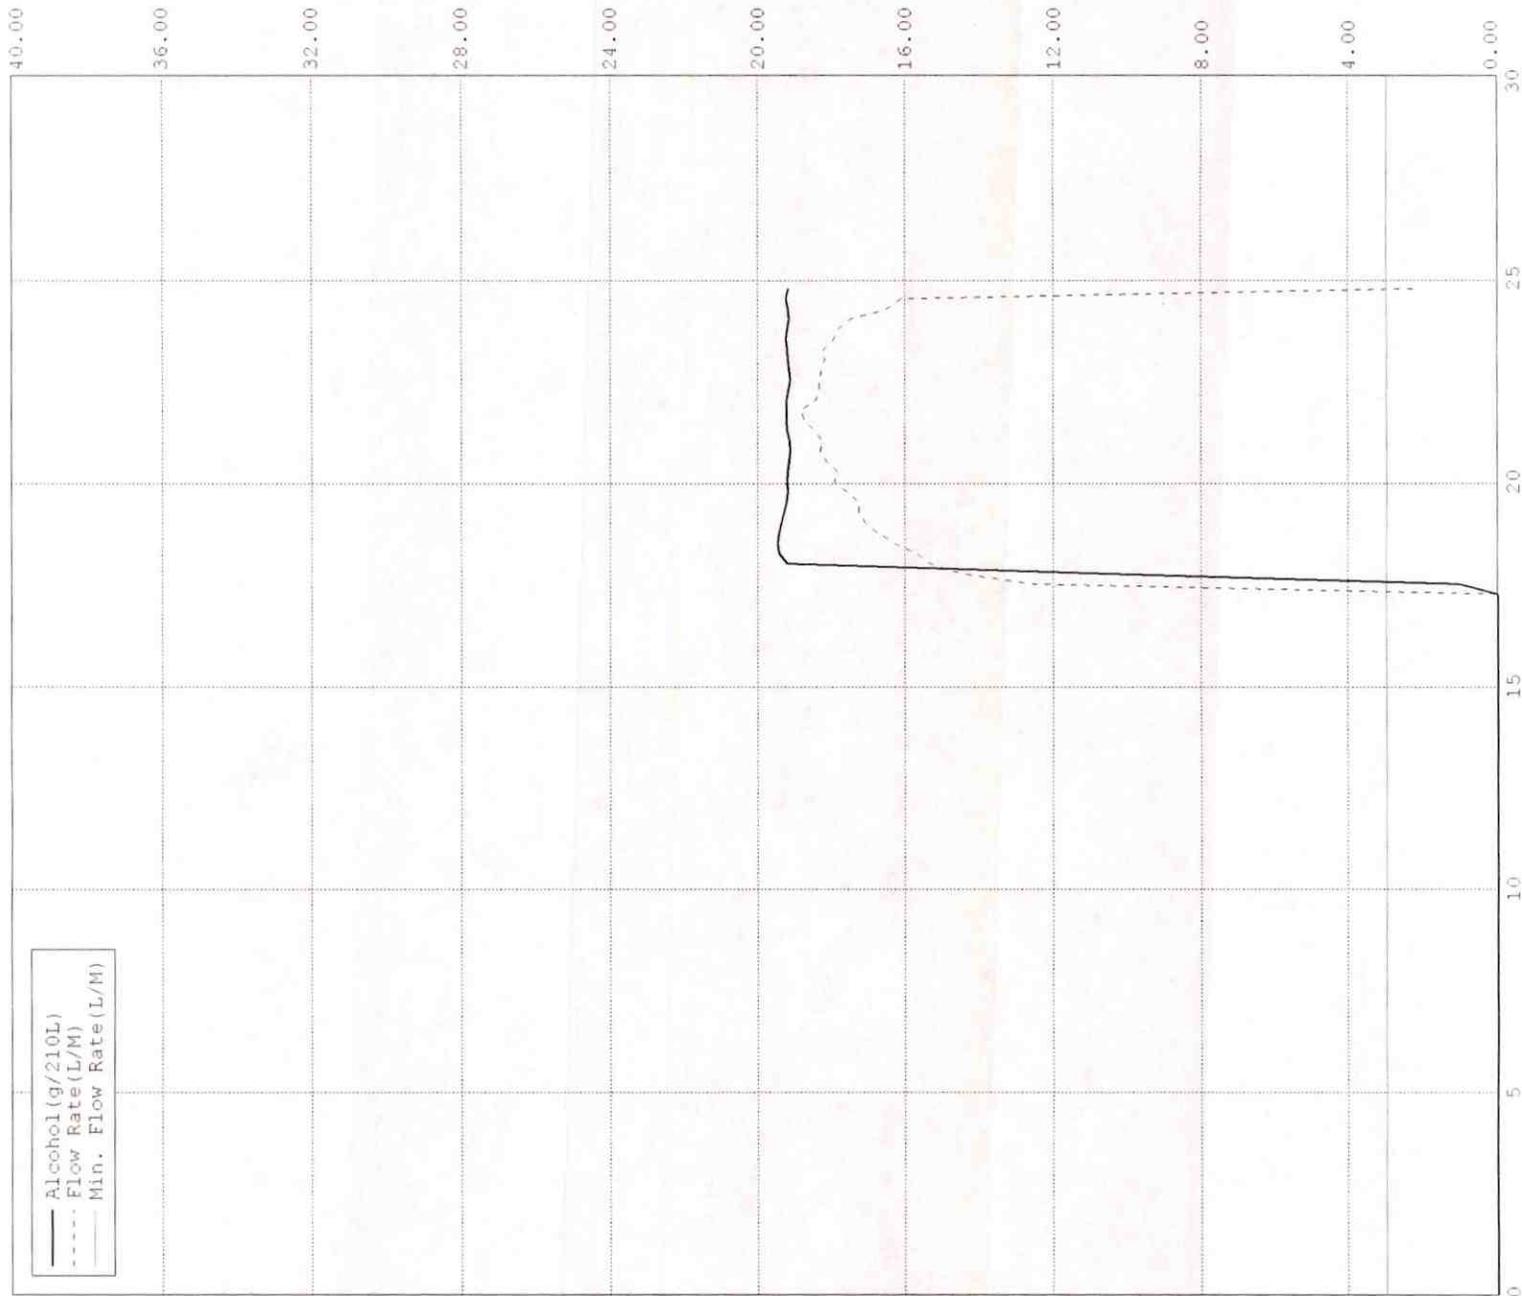

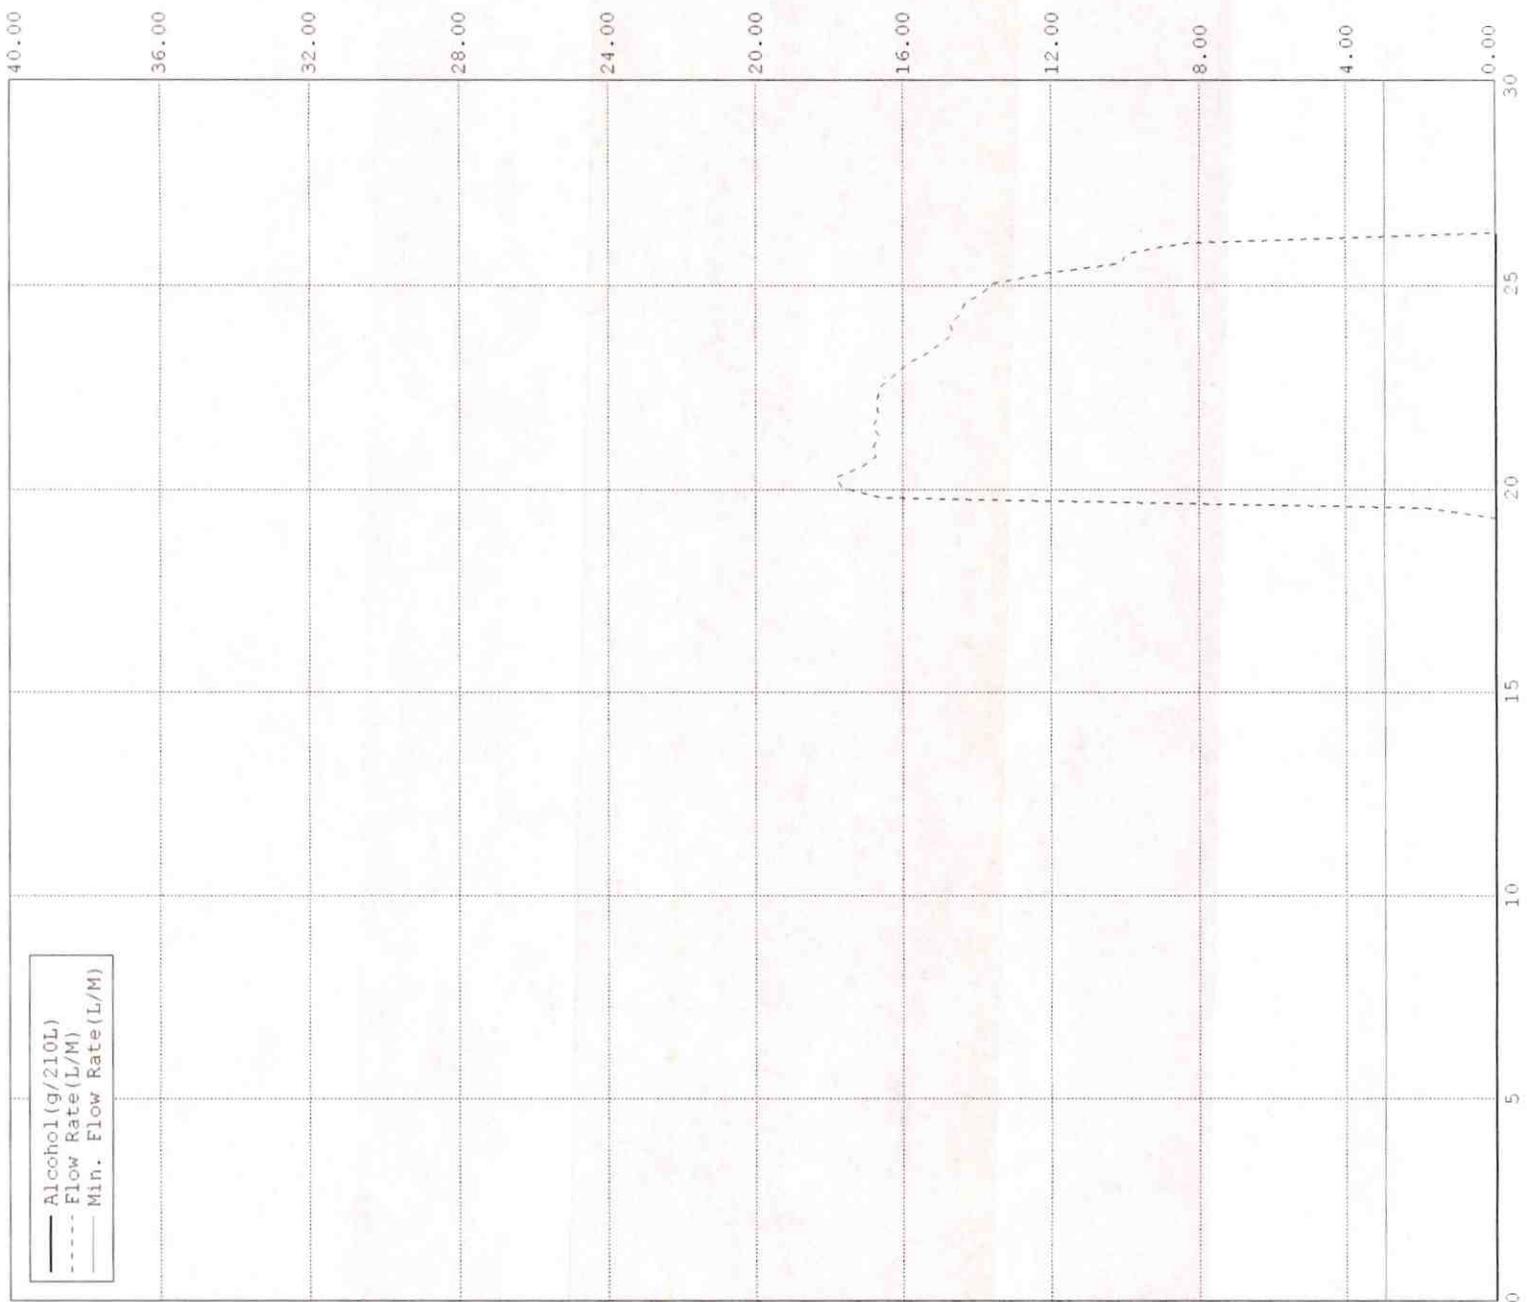

Alcohol (g/210L)  
 - - - - Flow Rate (L/M)  
 Min. Flow Rate (L/M)

SUBJECT TEST

-----  
 Alaska Department of Public Safety  
 DATAMASTER dmt: 100361  
 -----  
 Date: 09/27/2023  
 Time: 11:20:50

SUBJECT NAME:  
 TEST TEST  
 LICENSE #: XXXX

OPERATOR NAME:  
 CARLIE GLAISTER  
 OPERATOR'S #: 10436

DEPT/AGENCY:  
 NON-DRINKING SUBJECT TEST  
 CASE/REPORT: XXXX  
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
 NOMINAL: 0.080  
 TARGET AT 29.52: 0.079  
 LOT #: AG135004  
 EXPIRATION: 12/16/2023

DIAGNOSTIC CHECK	PASSED	11:22
BLANK TEST	0.000	11:22
INTERNAL STANDARD	VERIFIED	11:22
EXTERNAL STANDARD	0.078	11:22
BLANK TEST	0.000	11:23
SUBJECT SAMPLE (Vol=1.63L)	0.000	11:24
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.078	11:25
BLANK TEST	0.000	11:26

CKG