




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100415

Report Issue Date: Not Released
Date Received: 2025-01-08
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.019	0.021	0.020	0.020
0.080	0.079	AG335202	0.080	0.079	0.079	0.079	0.079	0.079
0.300	0.298	AG427706	0.297	0.298	0.297	0.297	0.297	0.297

As Found - Evaluation Analyst: Megan Carlock

As Found Conditions - Barometric Pressure (inHg): 29.17 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.7 Relative Humidity (%): 16

As-Found Lab Activity Date Range: 01/08/2025 - 01/08/2025

Replaced double sided tape on double check valve. Replaced O-ring.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.020	0.020	0.020	0.020	0.019	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.040	0.039	0.039	+/- 0.003
0.080	0.078	AG335202	0.078	0.077	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.097	AG333401	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.146	AG332004	0.145	0.145	0.144	0.145	0.145	0.145	+/- 0.006
0.300	0.292	AG427706	0.293	0.292	0.292	0.292	0.292	0.292	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.16 Barometer Used: VWR S/N 240680771 Temperature (C): 22.4 Relative Humidity (%): 14

As-Left Lab Activity Date Range: 02/20/2025 - 02/20/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 02/21/2025

kaija.swisher@alaska.gov

Not Tech/Admin Reviewed

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100415 Analyst or Technician Name: Kaia Swisher

DataMaster DMT Calibration Start Date: 2/20/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 10 Sep 2026
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.16 Temperature(C) 22.4 Relative Humidity(%) 14
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)
- ☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20250219KS Expiration Date: 5/19/25

Simulator S/N: SD11987 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250219KS Expiration Date: 5/19/25

Simulator S/N: SD1198 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 5/19/25

Simulator S/N: SD1199 Thermometer Verification Performed? ☒

Exp of ethanol solution
9/20/25
KS 2/20/25

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 19 Sep 2025

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 2/20/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 2/20/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100415

Date: 02/20/2025
 Time: 08:48:53

VERSIONS

DMT: 3.02
 PIC: 3.02
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 49.1°C PASSED
 (44.0°C - 52.0°C)
 Breath Tube = 45.6°C PASSED
 (38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.86 V PASSED
 (1.04 V - 2.42 V)
 Cooler Voltage = 1.75 V PASSED
 (1.04 V - 2.42 V)
 Bias Voltage = 79 V PASSED
 (47 V - 111 V)
 Chopper Freq = 528 Hz PASSED
 (475 Hz - 575 Hz)
 Barometer = 29.1 in

PUMP INFO

Flow Rate = 4.891 L/M PASSED
 (3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
 (0.003 V <= 0.010 V)
 PUMP OFF PASSED
 (0.002 V <= 0.010 V)

FILTER INFO

Filter 1 PASSED
 Filter 2 PASSED
 Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.101 0.09% PASSED
 (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100415

Date: 02/20/2025

Time: 9:03 AM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 45.9°C

Current Barometer 29.2 in

Volume (Ltr) 1.48

Settings

Lamp: 1.92 V

Bias: 79 V

Cooler: 1.81 V

Chopper: 526 Hz

Voltages (V)

Flow: 1.06 V

Detector: 0.087 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 06/21/2019
Time: 09:39:06

OPERATOR NAME:
DEREK WALTON
CERTIFICATE #: 9508

Ca = 0.1000
CAL = 0.995204 0.800 <= CAL < 1.200
b1 = 0.0001 0.0000 <= b1 < 0.0040
b2 = 0.0046 0.0010 <= b2 < 0.0100
b3 = 0.0003 0.0000 <= b3 < 0.0040
Xq = 0.1015 0.0500 <= Xq < 0.2000
a21 = 1.185899 1.050 <= a21 < 1.300
a31 = 0.416230 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 09:04:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.17: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	09:05
BLANK TEST	0.000	09:05
INTERNAL STANDARD	VERIFIED	09:06
EXTERNAL STANDARD	0.077	09:06
BLANK TEST	0.000	09:07
SUBJECT SAMPLE (Vol=1.55L)	0.000	09:08
BLANK TEST	0.000	09:09
EXTERNAL STANDARD	0.078	09:09
BLANK TEST	0.000	09:10

KS

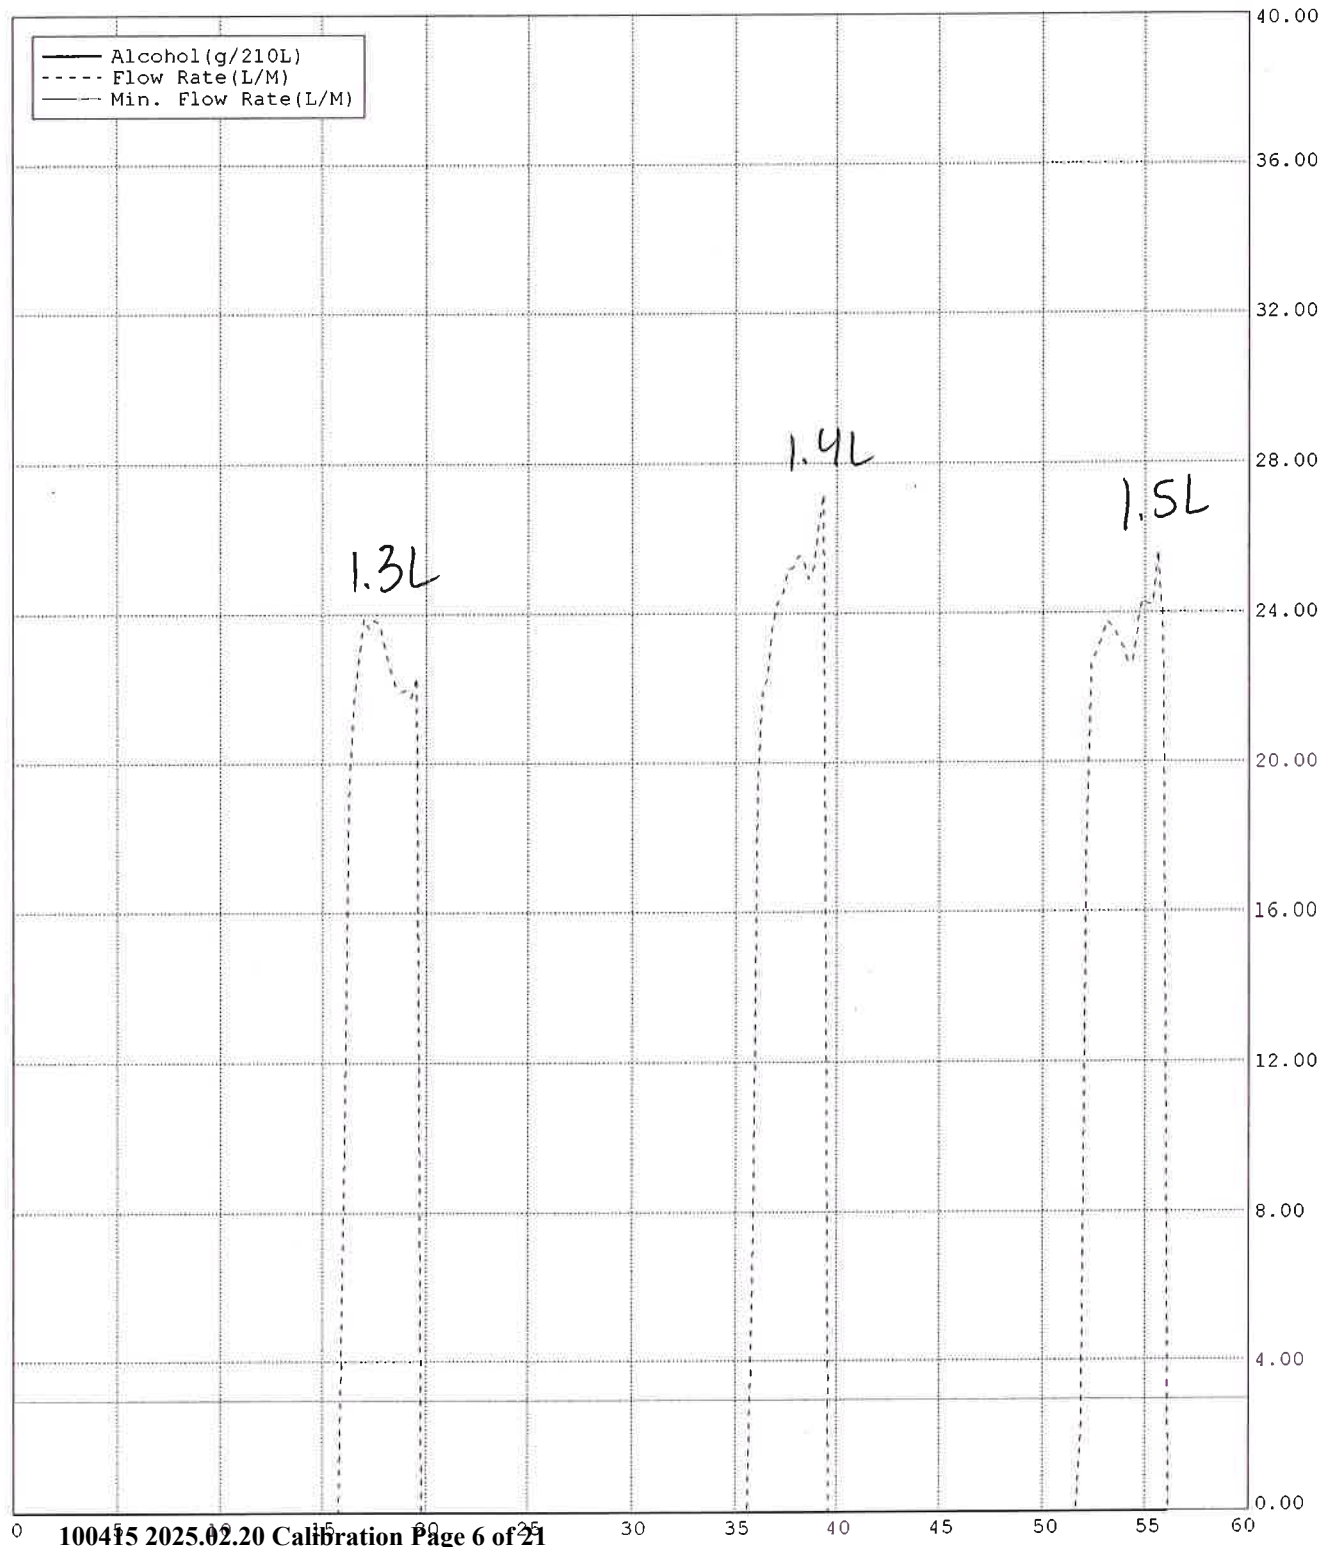

LINEARITY CHECK

Alaska Department of Public Safety
DATAMASTER dmt: 100415


Date: 02/20/2025
Time: 09:22:37

SUPERVISOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0198	0.0004
0.039	0.0392	0.0004
0.078	0.0778	0.0004
0.097	0.0980	0.0000
0.146	0.1448	0.0004
0.292	0.2922	0.0004

SLOPE = 0.997917
R² = 0.999941

KS

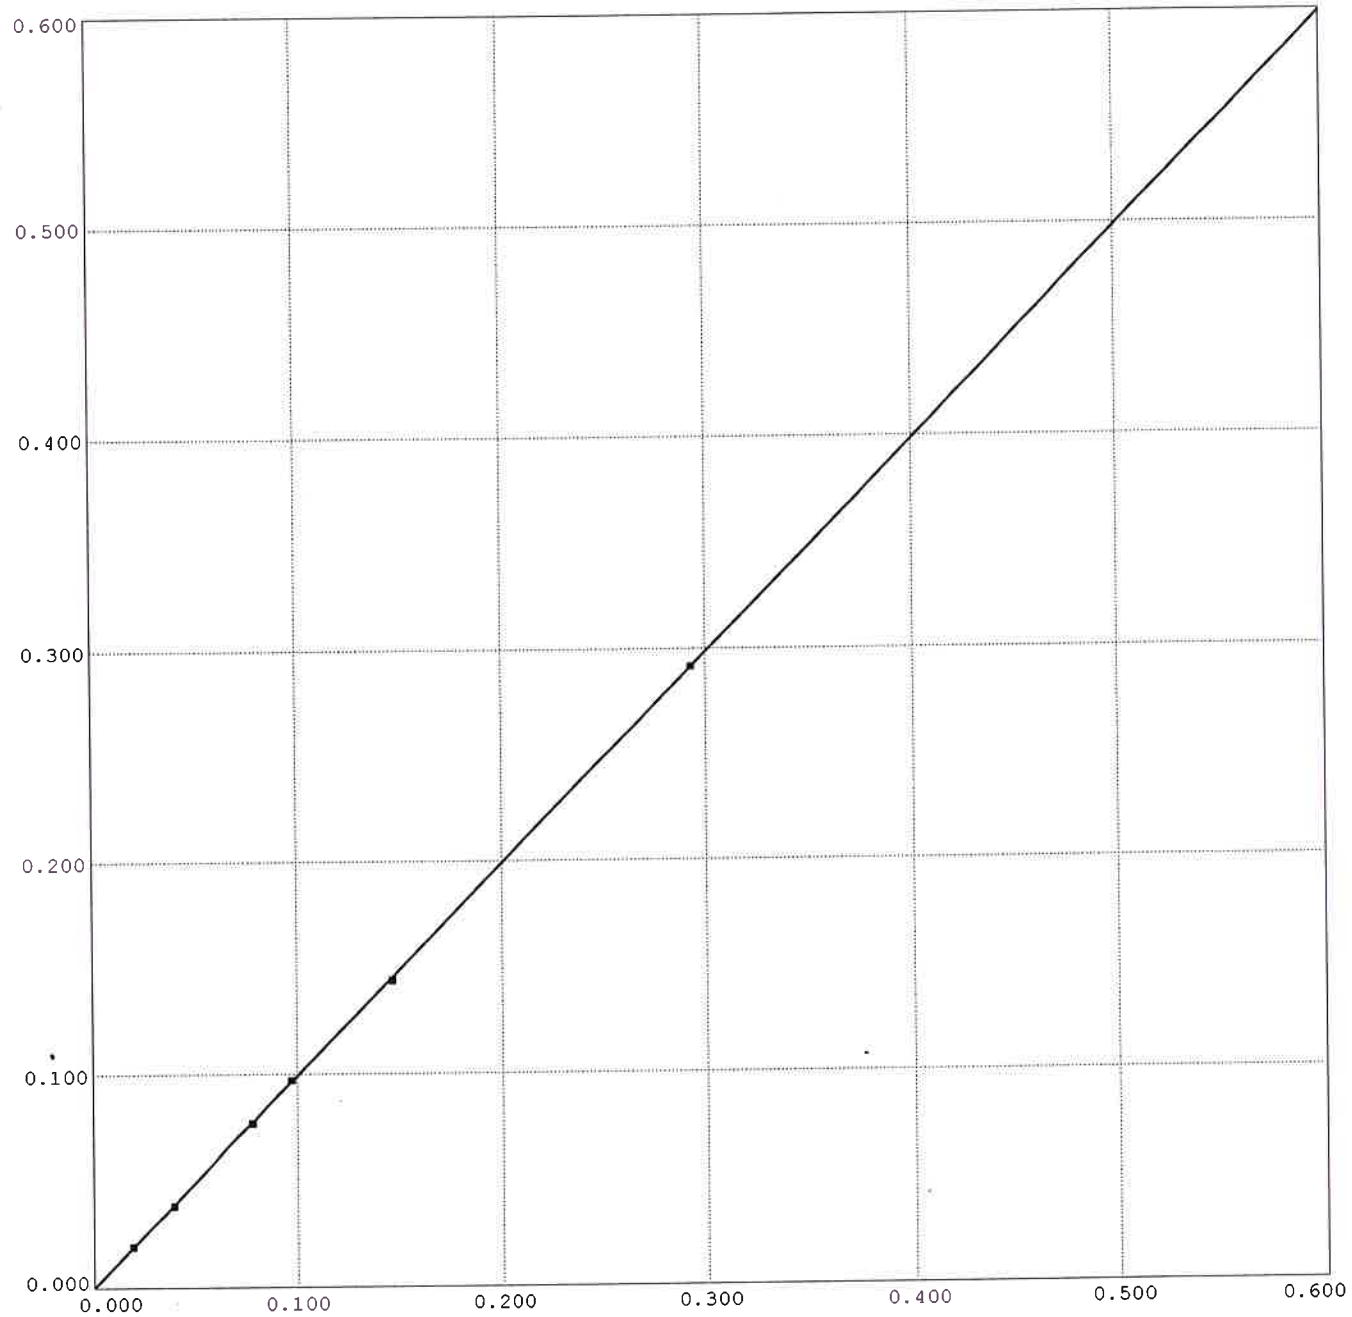

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100415






Date: 02/20/2025
Time: 09:23:32

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.17: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 516 psi

BLANK TEST	0.000	09:24
INTERNAL STANDARD	VERIFIED	09:25
EXTERNAL STANDARD	0.020	09:25
BLANK TEST	0.000	09:26
EXTERNAL STANDARD	0.020	09:26
BLANK TEST	0.000	09:27
EXTERNAL STANDARD	0.020	09:27
BLANK TEST	0.000	09:28
EXTERNAL STANDARD	0.020	09:28
BLANK TEST	0.000	09:29
EXTERNAL STANDARD	0.019	09:29
BLANK TEST	0.000	09:30

Average = 0.0198
Std Dev = 0.0004

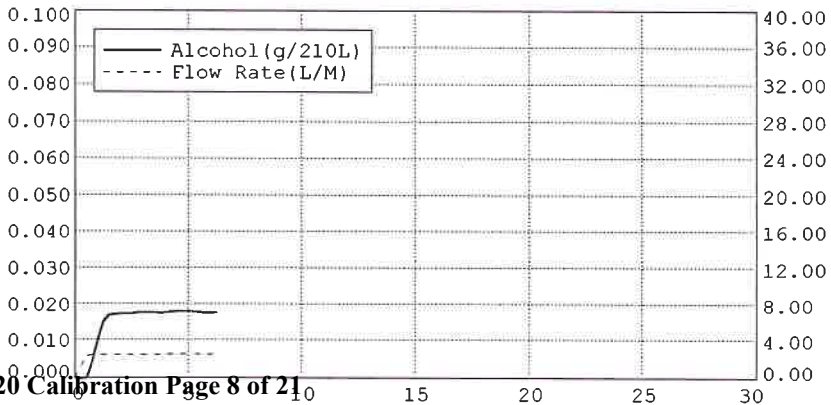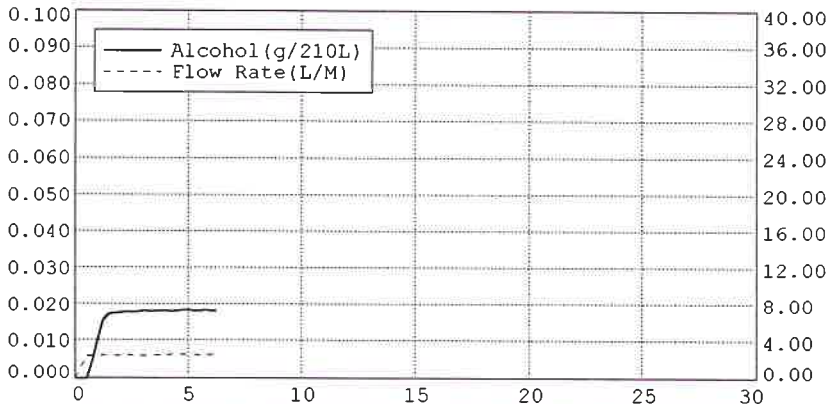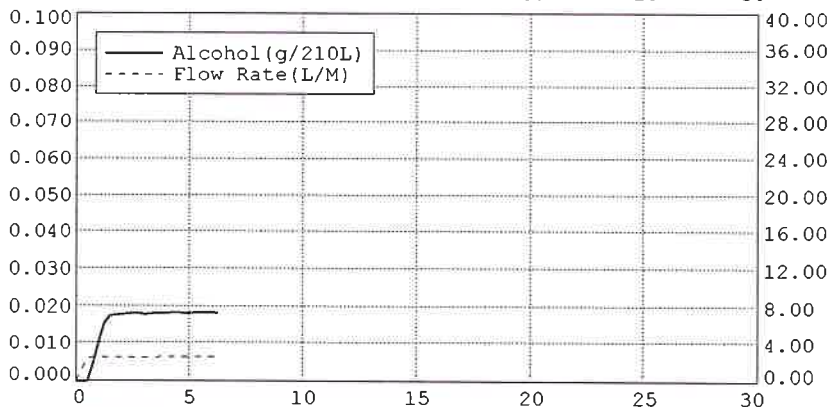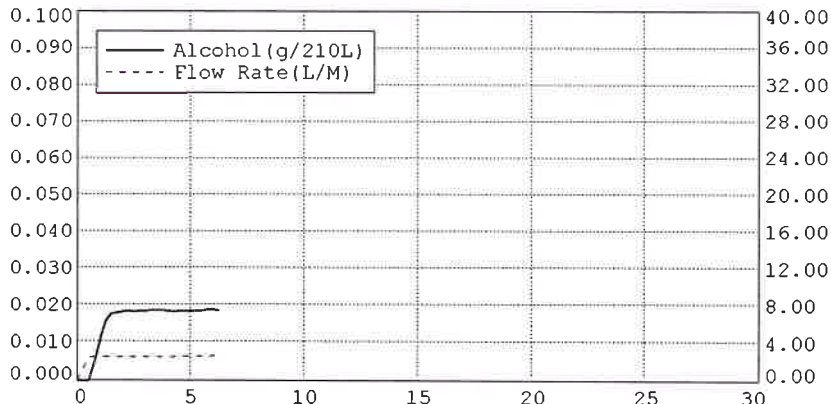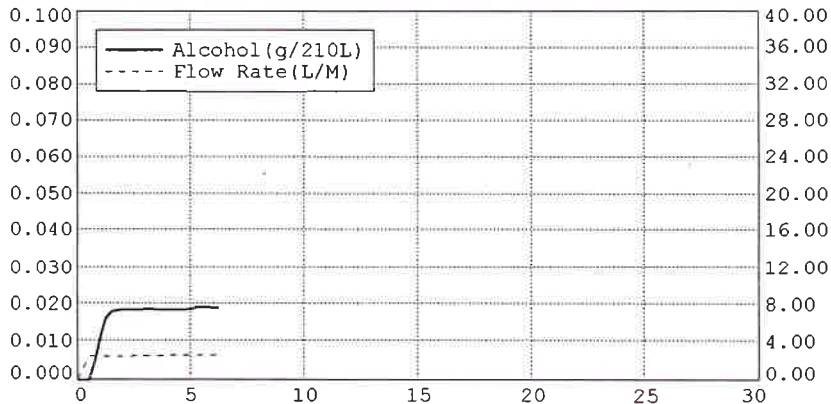

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100415






Date: 02/20/2025
Time: 09:33:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.17: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 913 psi

BLANK TEST	0.000	09:35
INTERNAL STANDARD	VERIFIED	09:35
EXTERNAL STANDARD	0.039	09:35
BLANK TEST	0.000	09:36
EXTERNAL STANDARD	0.039	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.039	09:37
BLANK TEST	0.000	09:38
EXTERNAL STANDARD	0.040	09:38
BLANK TEST	0.000	09:39
EXTERNAL STANDARD	0.039	09:40
BLANK TEST	0.000	09:40

Average = 0.0392
Std Dev = 0.0004

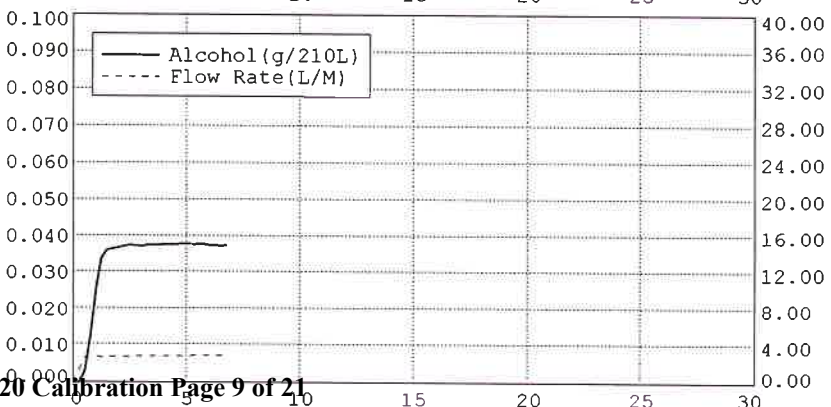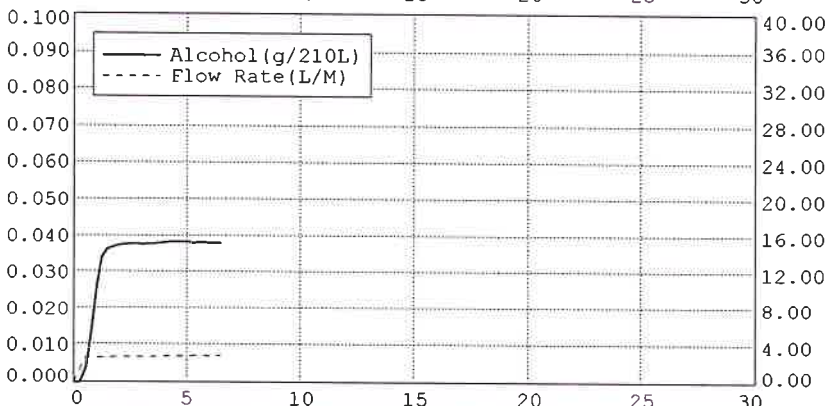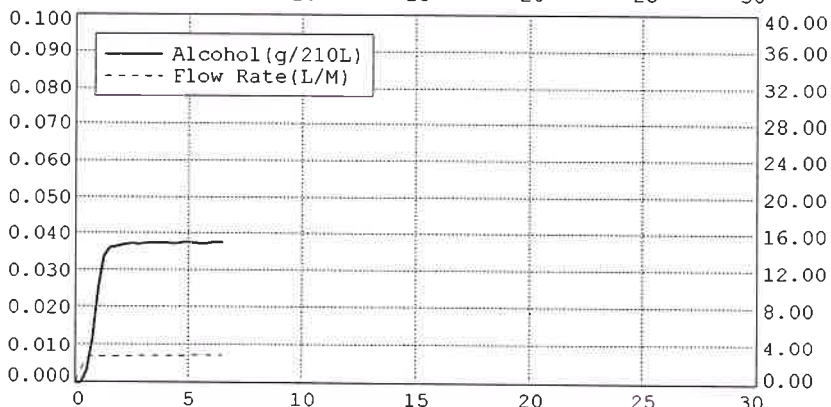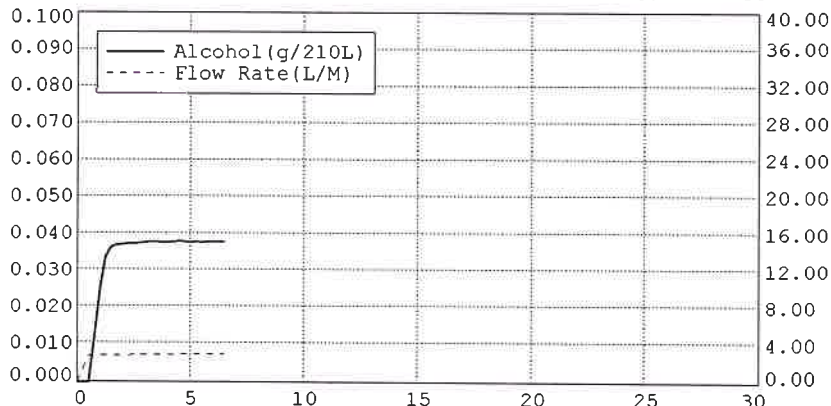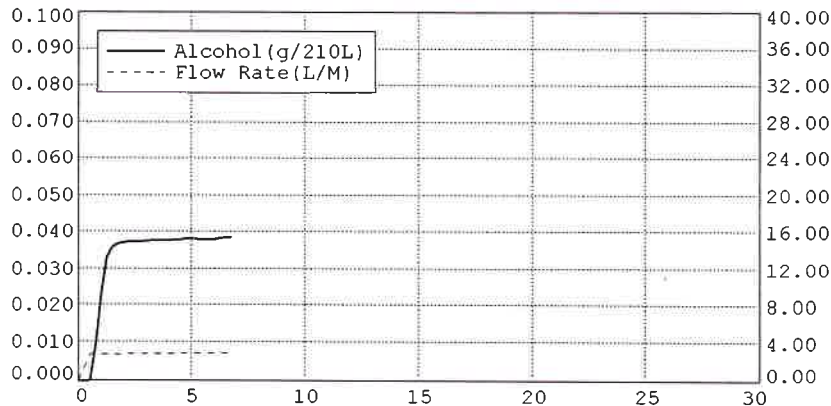

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100415






Date: 02/20/2025
Time: 09:43:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.16: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 537 psi

BLANK TEST	0.000	09:44
INTERNAL STANDARD	VERIFIED	09:44
EXTERNAL STANDARD	0.078	09:44
BLANK TEST	0.000	09:45
EXTERNAL STANDARD	0.077	09:46
BLANK TEST	0.000	09:47
EXTERNAL STANDARD	0.078	09:47
BLANK TEST	0.000	09:48
EXTERNAL STANDARD	0.078	09:48
BLANK TEST	0.000	09:49
EXTERNAL STANDARD	0.078	09:49
BLANK TEST	0.000	09:50

Average = 0.0778
Std Dev = 0.0004

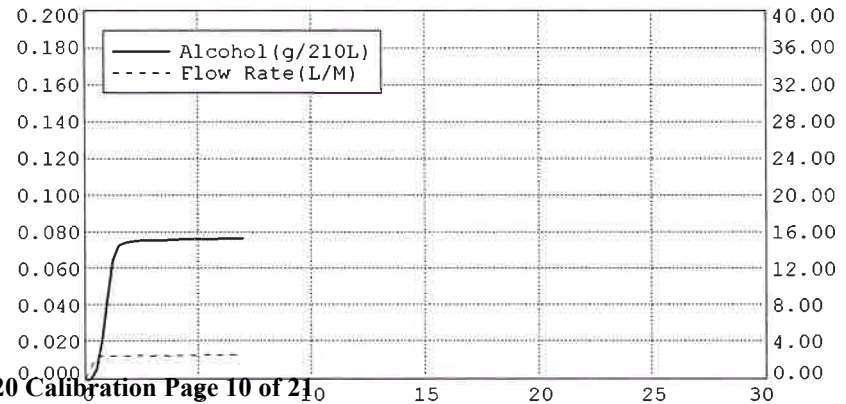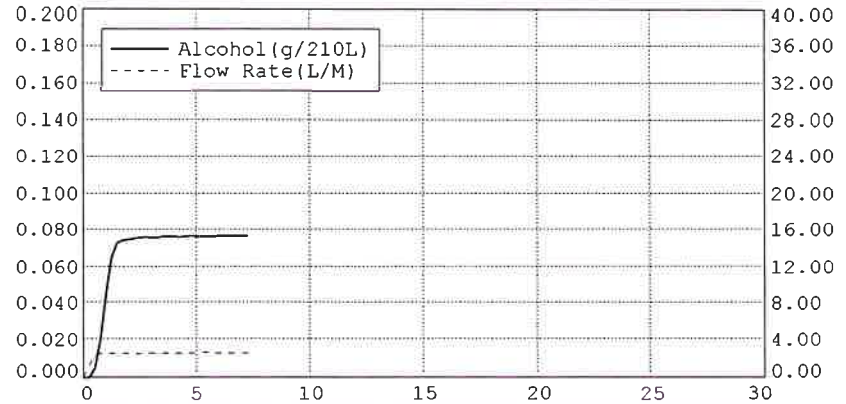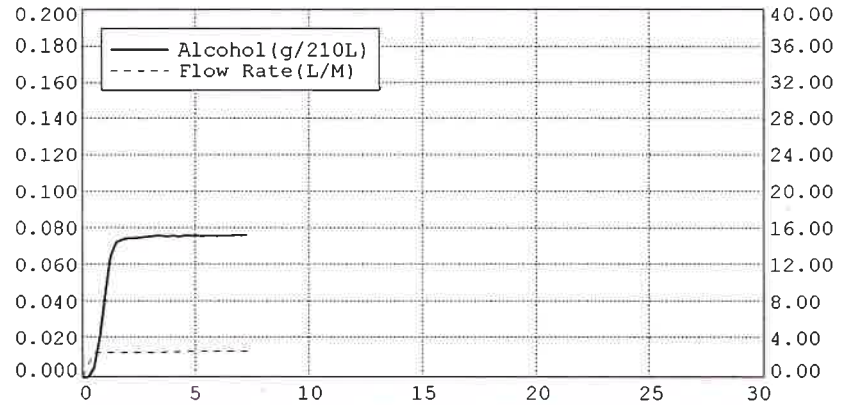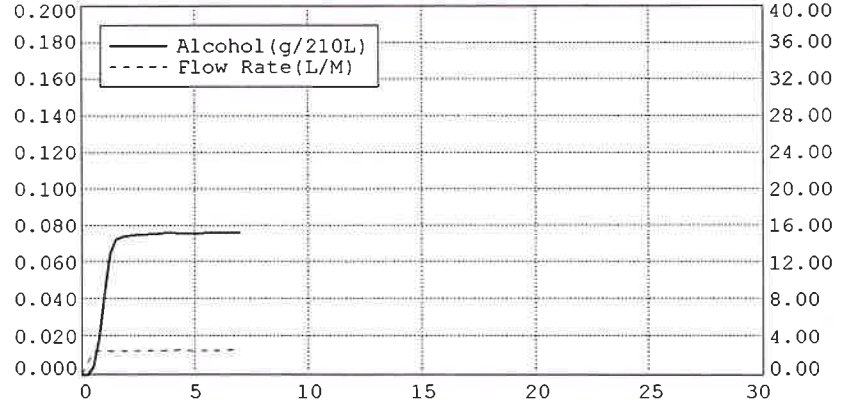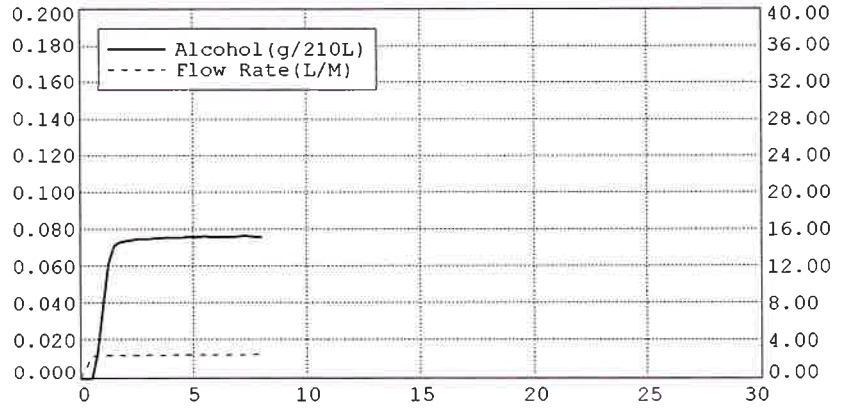

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100415






Date: 02/20/2025
Time: 09:52:09

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.16: 0.097
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 647 psi

BLANK TEST	0.000	09:53
INTERNAL STANDARD	VERIFIED	09:53
EXTERNAL STANDARD	0.098	09:53
BLANK TEST	0.000	09:54
EXTERNAL STANDARD	0.098	09:55
BLANK TEST	0.000	09:56
EXTERNAL STANDARD	0.098	09:56
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.098	09:57
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.098	09:58
BLANK TEST	0.000	09:59

Average = 0.0980
Std Dev = 0.0000

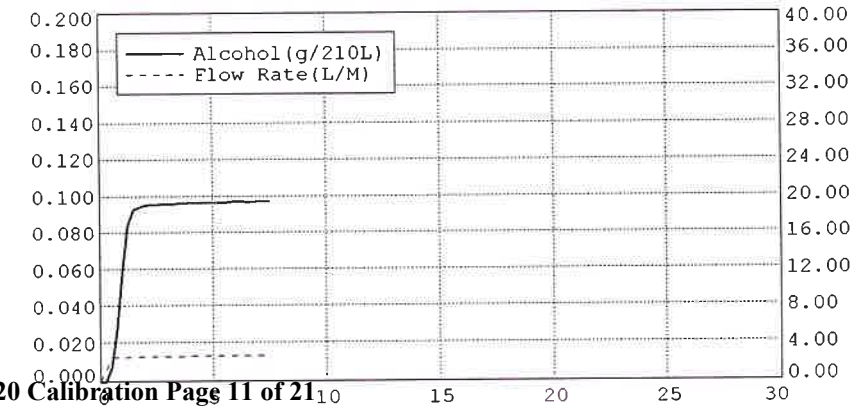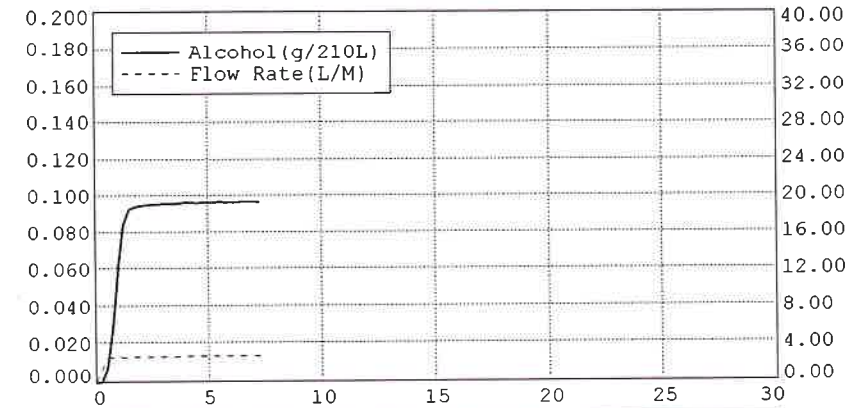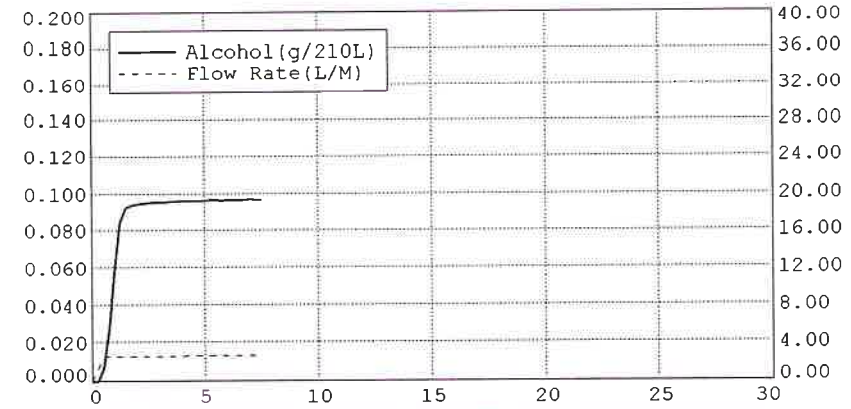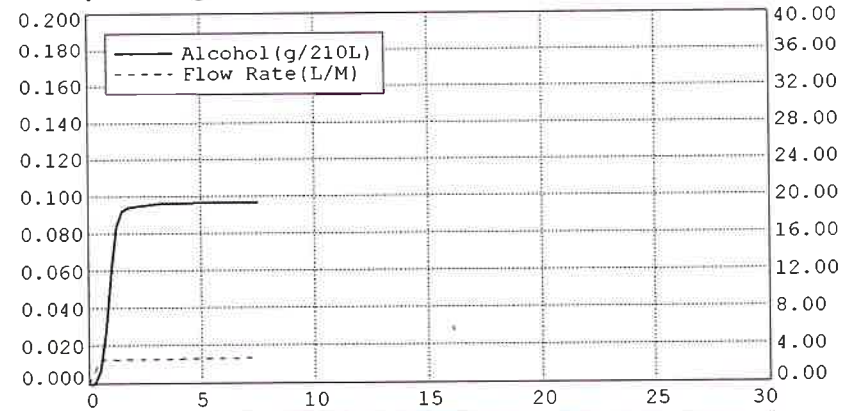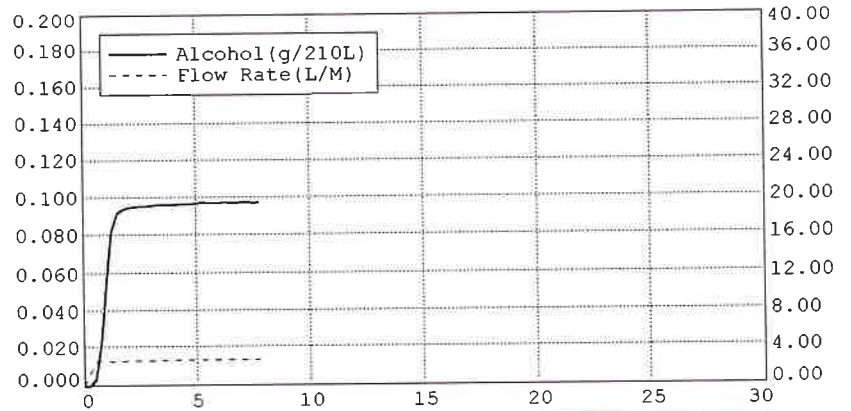

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100415






Date: 02/20/2025
Time: 10:00:38

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.16: 0.146
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 256 psi

BLANK TEST	0.000	10:01
INTERNAL STANDARD	VERIFIED	10:02
EXTERNAL STANDARD	0.145	10:02
BLANK TEST	0.000	10:03
EXTERNAL STANDARD	0.145	10:03
BLANK TEST	0.000	10:04
EXTERNAL STANDARD	0.144	10:04
BLANK TEST	0.000	10:05
EXTERNAL STANDARD	0.145	10:06
BLANK TEST	0.000	10:07
EXTERNAL STANDARD	0.145	10:07
BLANK TEST	0.000	10:08

Average = 0.1448
Std Dev = 0.0004

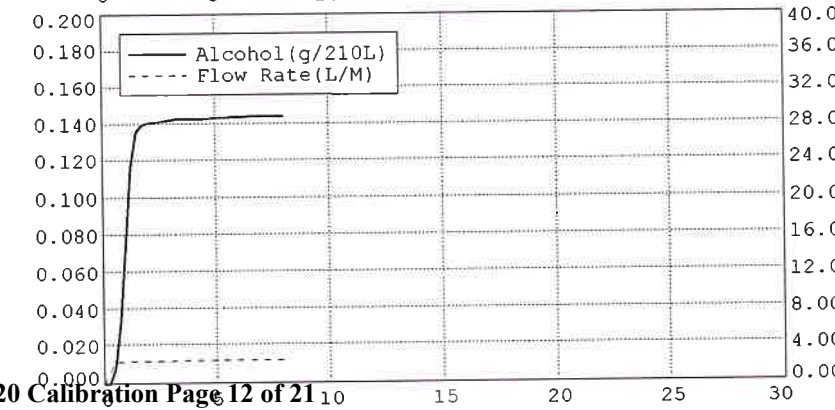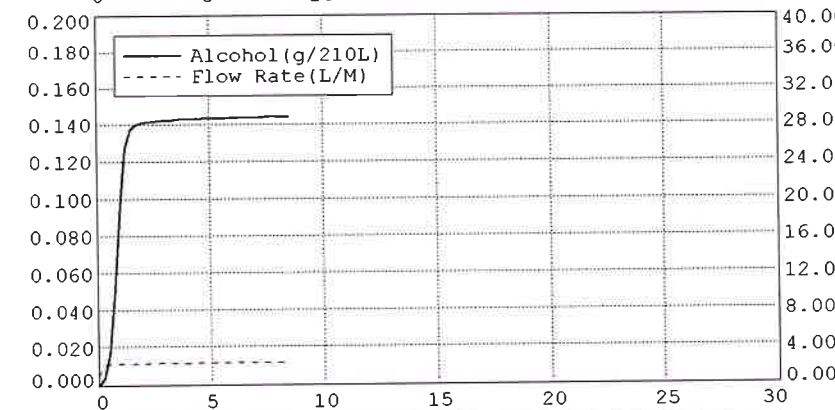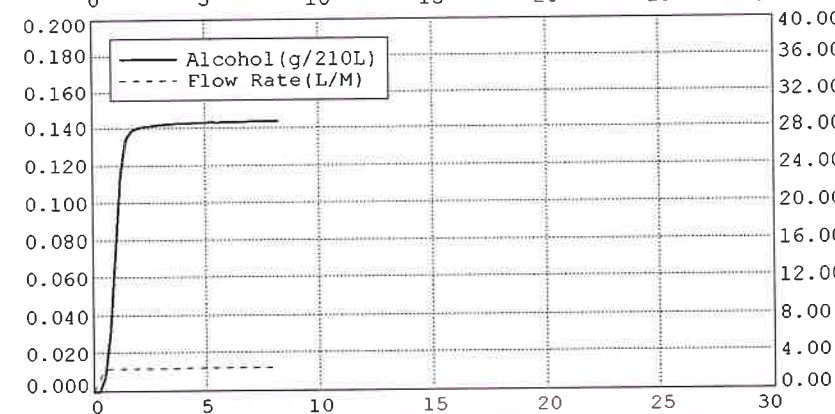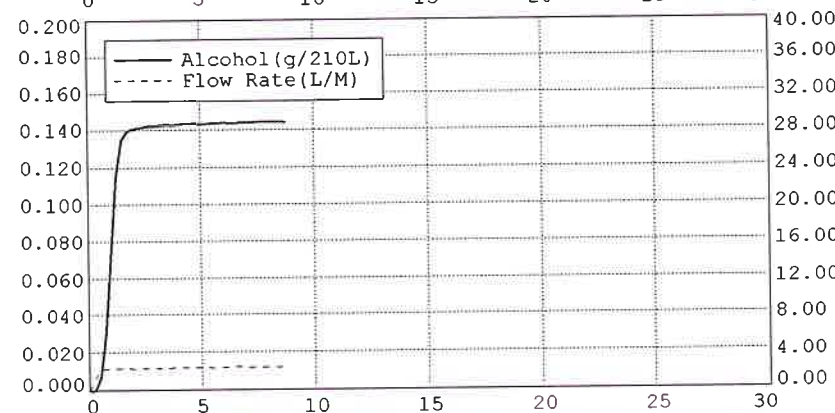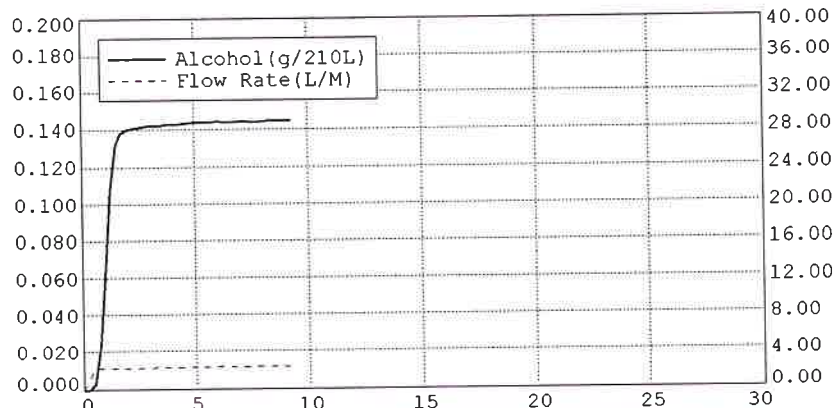

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100415






Date: 02/20/2025
Time: 10:11:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.15: 0.292
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 404 psi

BLANK TEST	0.000	10:12
INTERNAL STANDARD	VERIFIED	10:12
EXTERNAL STANDARD	0.293	10:12
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.292	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.292	10:15
BLANK TEST	0.000	10:16
EXTERNAL STANDARD	0.292	10:16
BLANK TEST	0.000	10:17
EXTERNAL STANDARD	0.292	10:18
BLANK TEST	0.000	10:19

Average = 0.2922
Std Dev = 0.0004

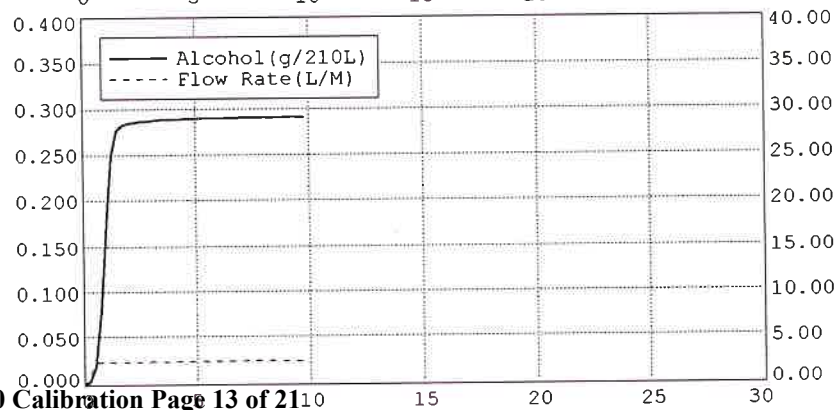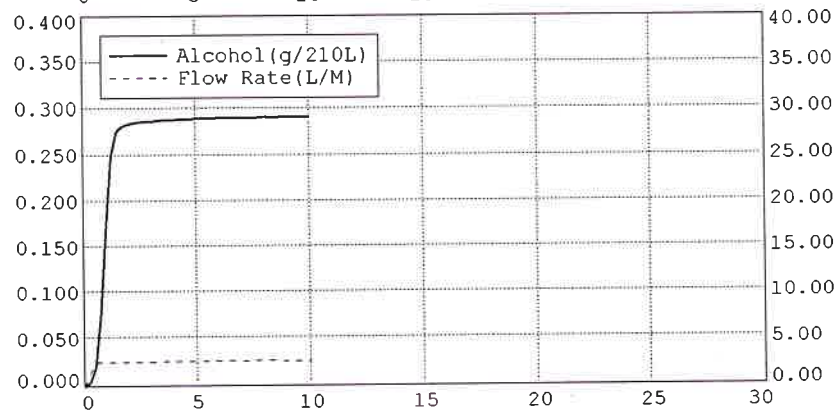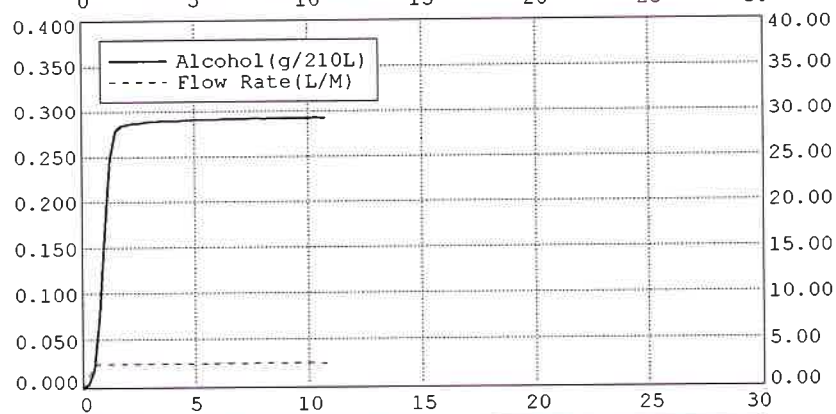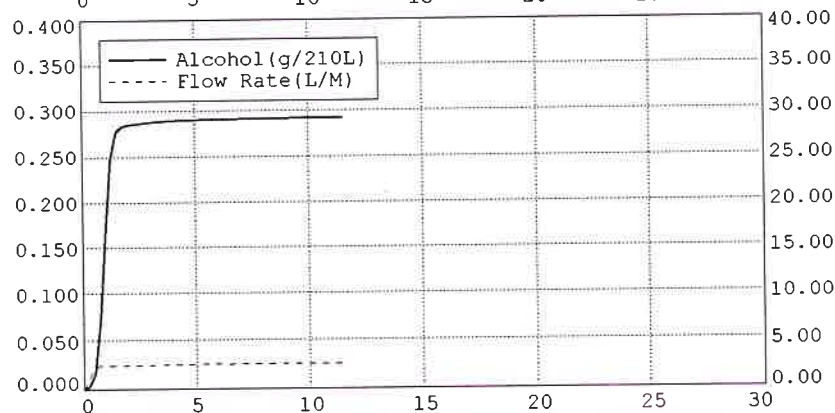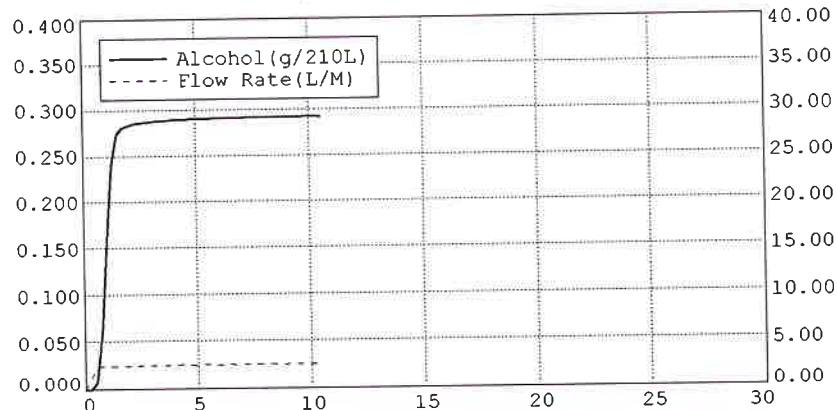

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 10:50:35

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:52
BLANK TEST	0.000	10:52
INTERNAL STANDARD	VERIFIED	10:52
EXTERNAL STANDARD	0.077	10:52
BLANK TEST	0.000	10:53
SUBJECT SAMPLE	INCOMPLETE	10:55

K5

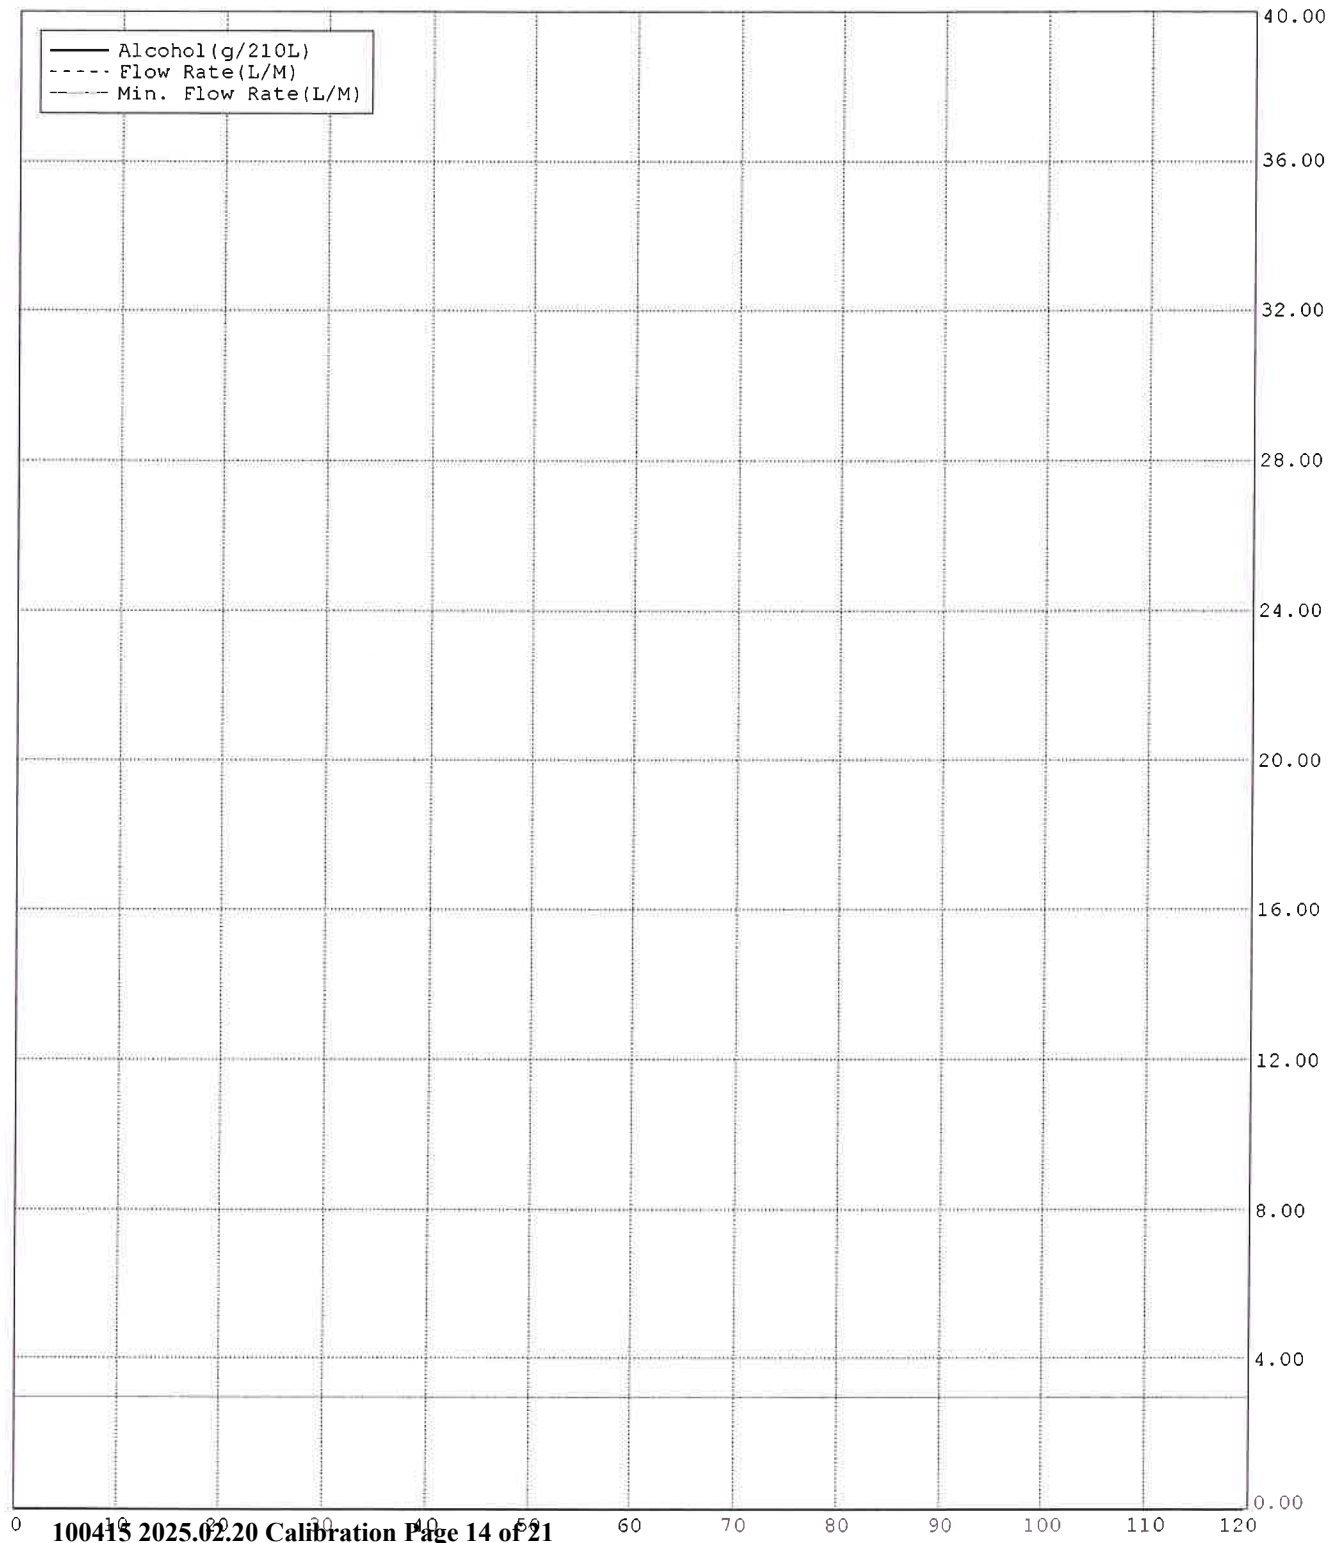

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 11:02:08

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAX ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:03
BLANK TEST	0.000	11:03
INTERNAL STANDARD	VERIFIED	11:03
EXTERNAL STANDARD	0.078	11:03
BLANK TEST	0.000	11:04
SUBJECT SAMPLE	XXX	11:05

Maximum Attempts Exceeded

KS

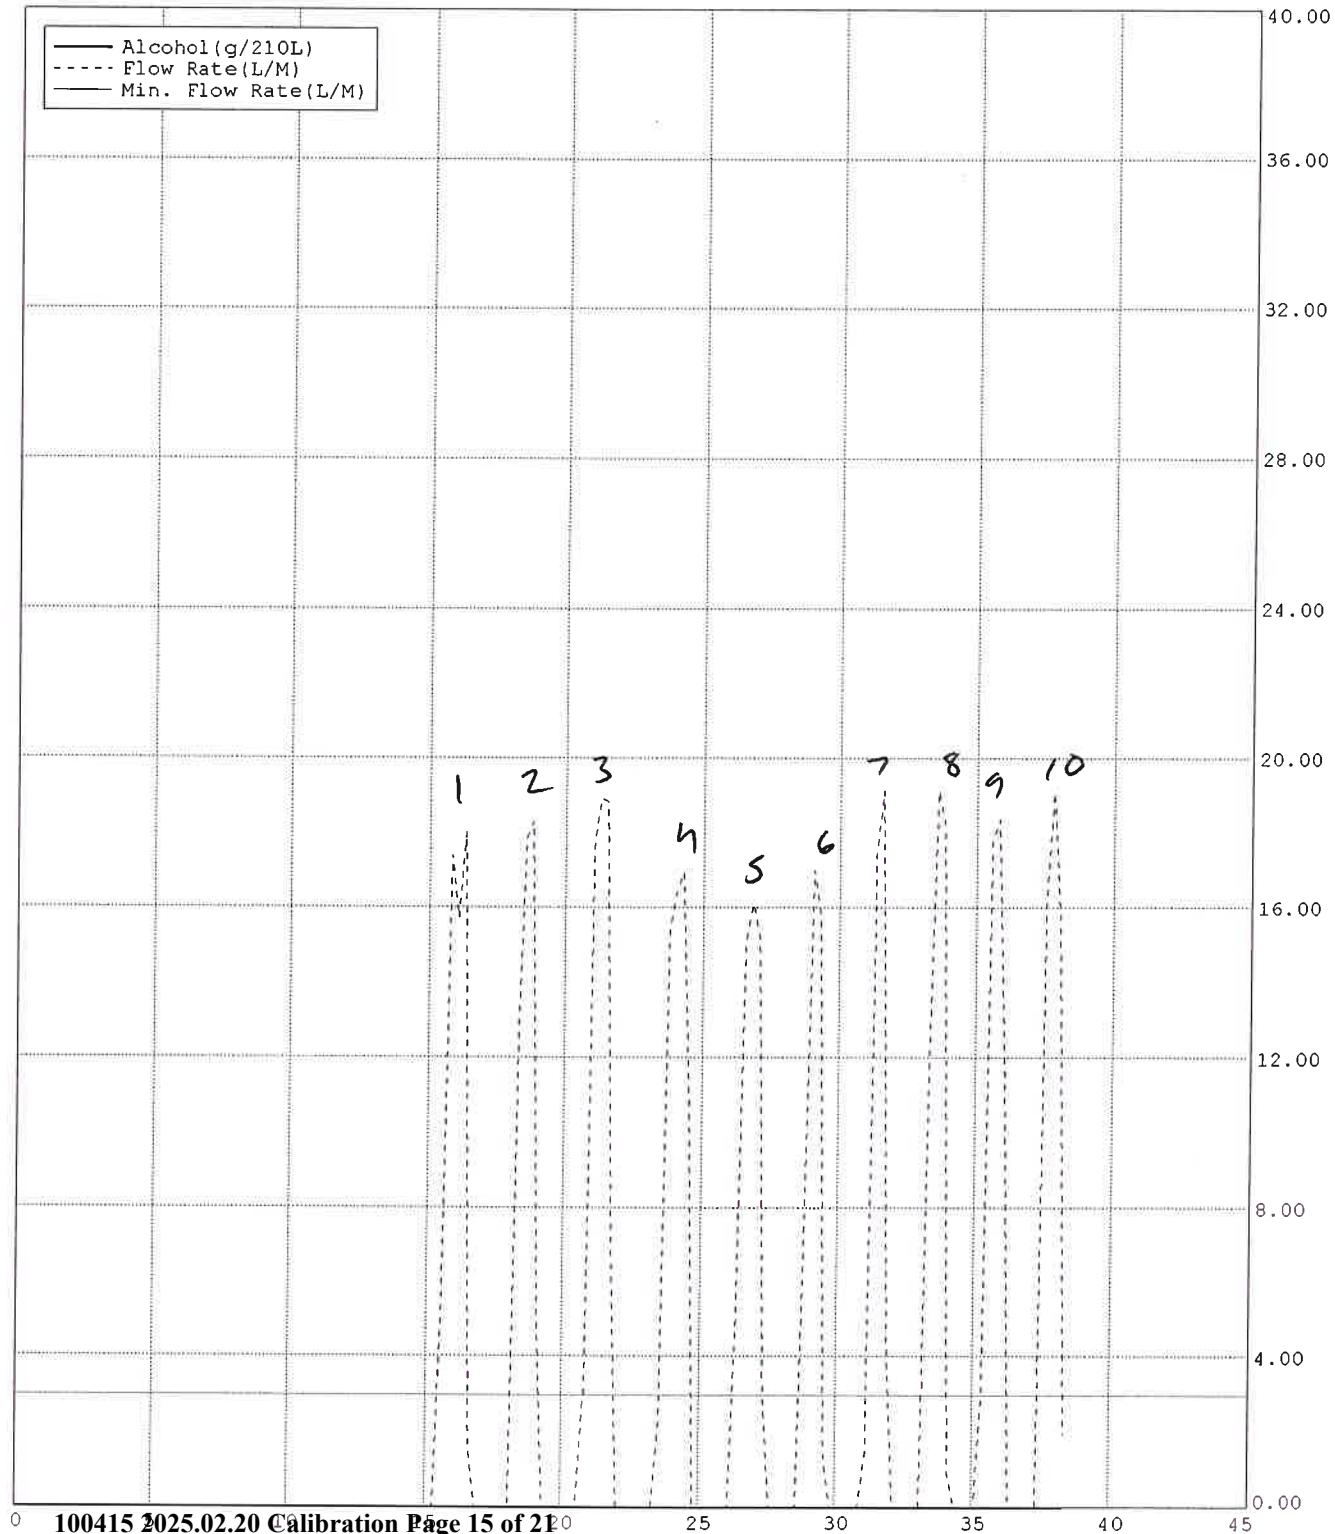

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 11:09:02

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:11
BLANK TEST	0.000	11:11
INTERNAL STANDARD	VERIFIED	11:11
EXTERNAL STANDARD	0.078	11:12
BLANK TEST	0.000	11:13
SUBJECT SAMPLE	INVALID	11:13

KS

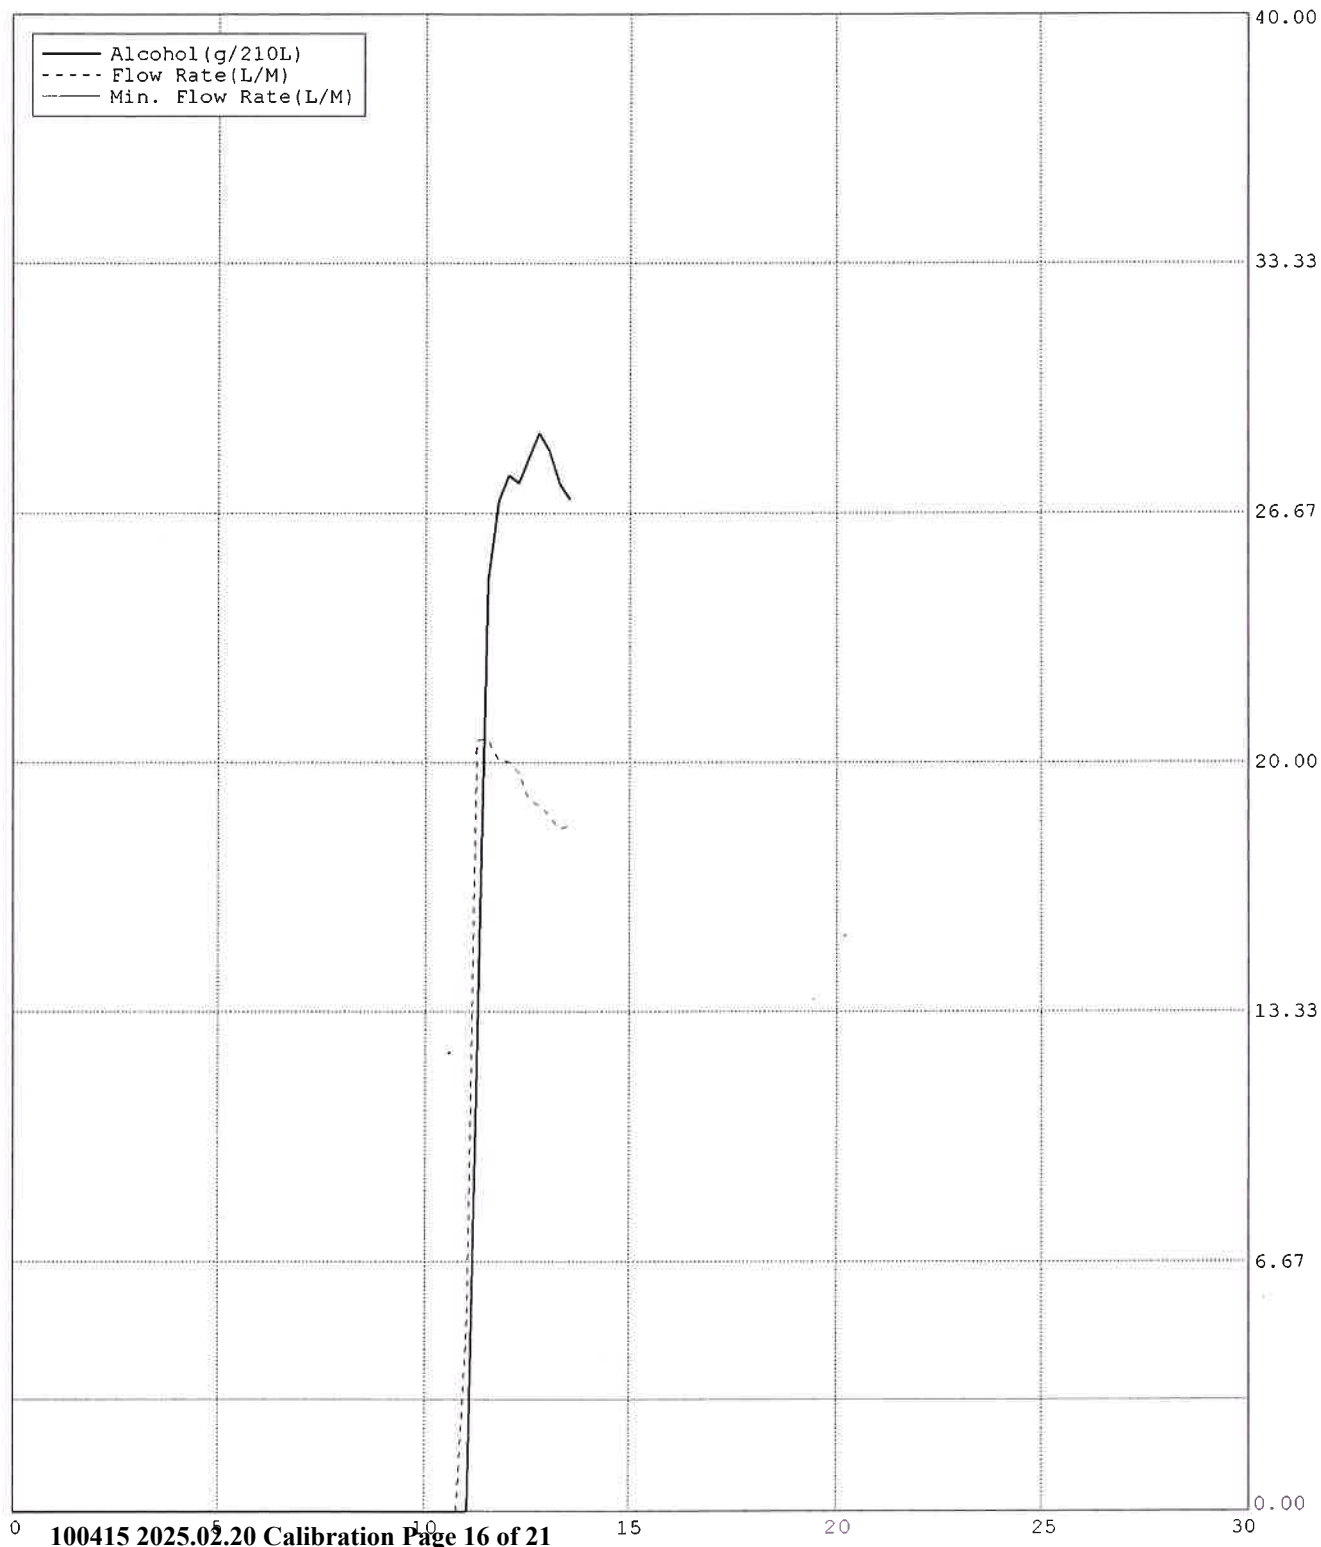

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 11:14:45

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.15: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:16
BLANK TEST	0.000	11:16
INTERNAL STANDARD	VERIFIED	11:16
EXTERNAL STANDARD	0.078	11:17
BLANK TEST	0.000	11:18

RFI DETECTED

KS

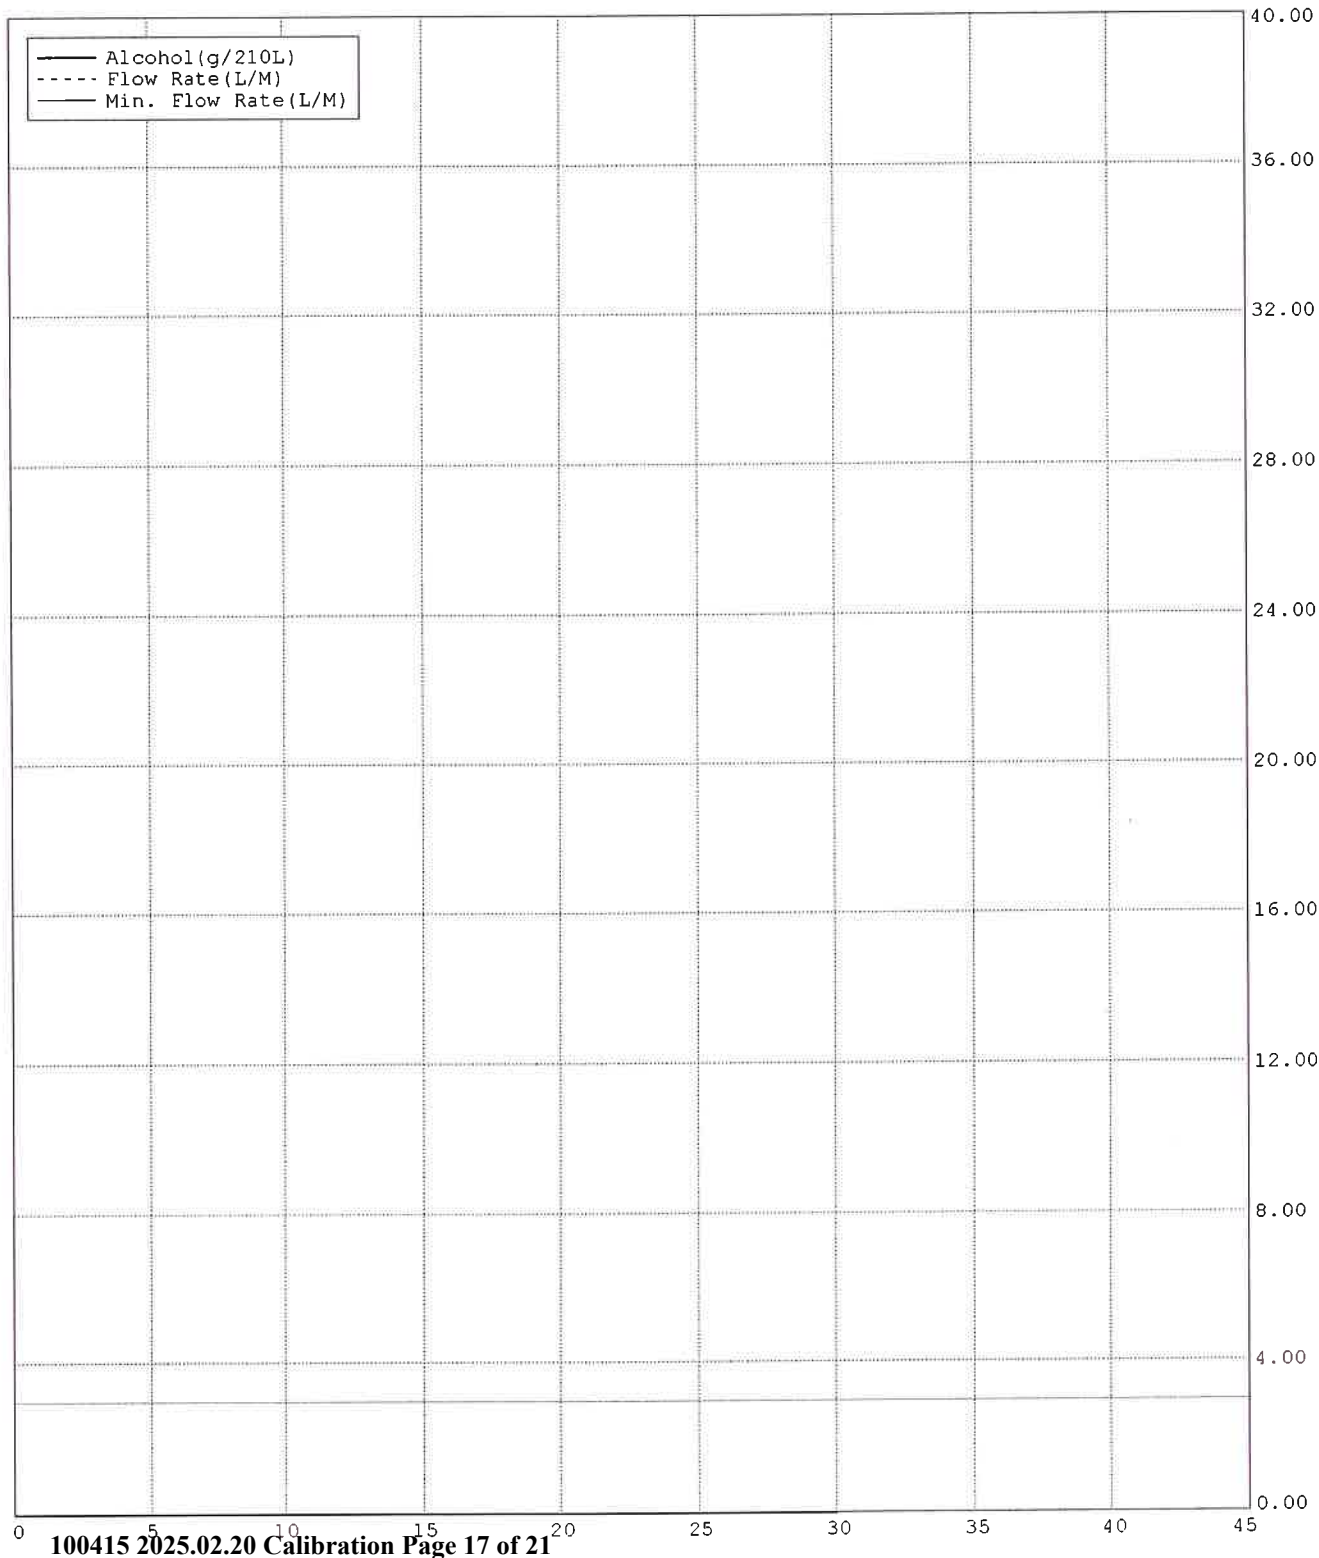

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 13:30:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.11: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:31
BLANK TEST	0.000	13:31
INTERNAL STANDARD	VERIFIED	13:31
Xq = 0.102 (0.52%)		
EXTERNAL STANDARD	0.078	13:31
X[1] = 0.0776 (-0.0010) (0.0011)		
BLANK TEST	0.000	13:32
SUBJECT SAMPLE	XXX	13:33
X[1] = 0.1139 (-0.0166) (0.0005)		

Interference Detected

Filter 2 average: -0.0012
Filter 3 average: 0.0013
KS 2/20/2025

KS

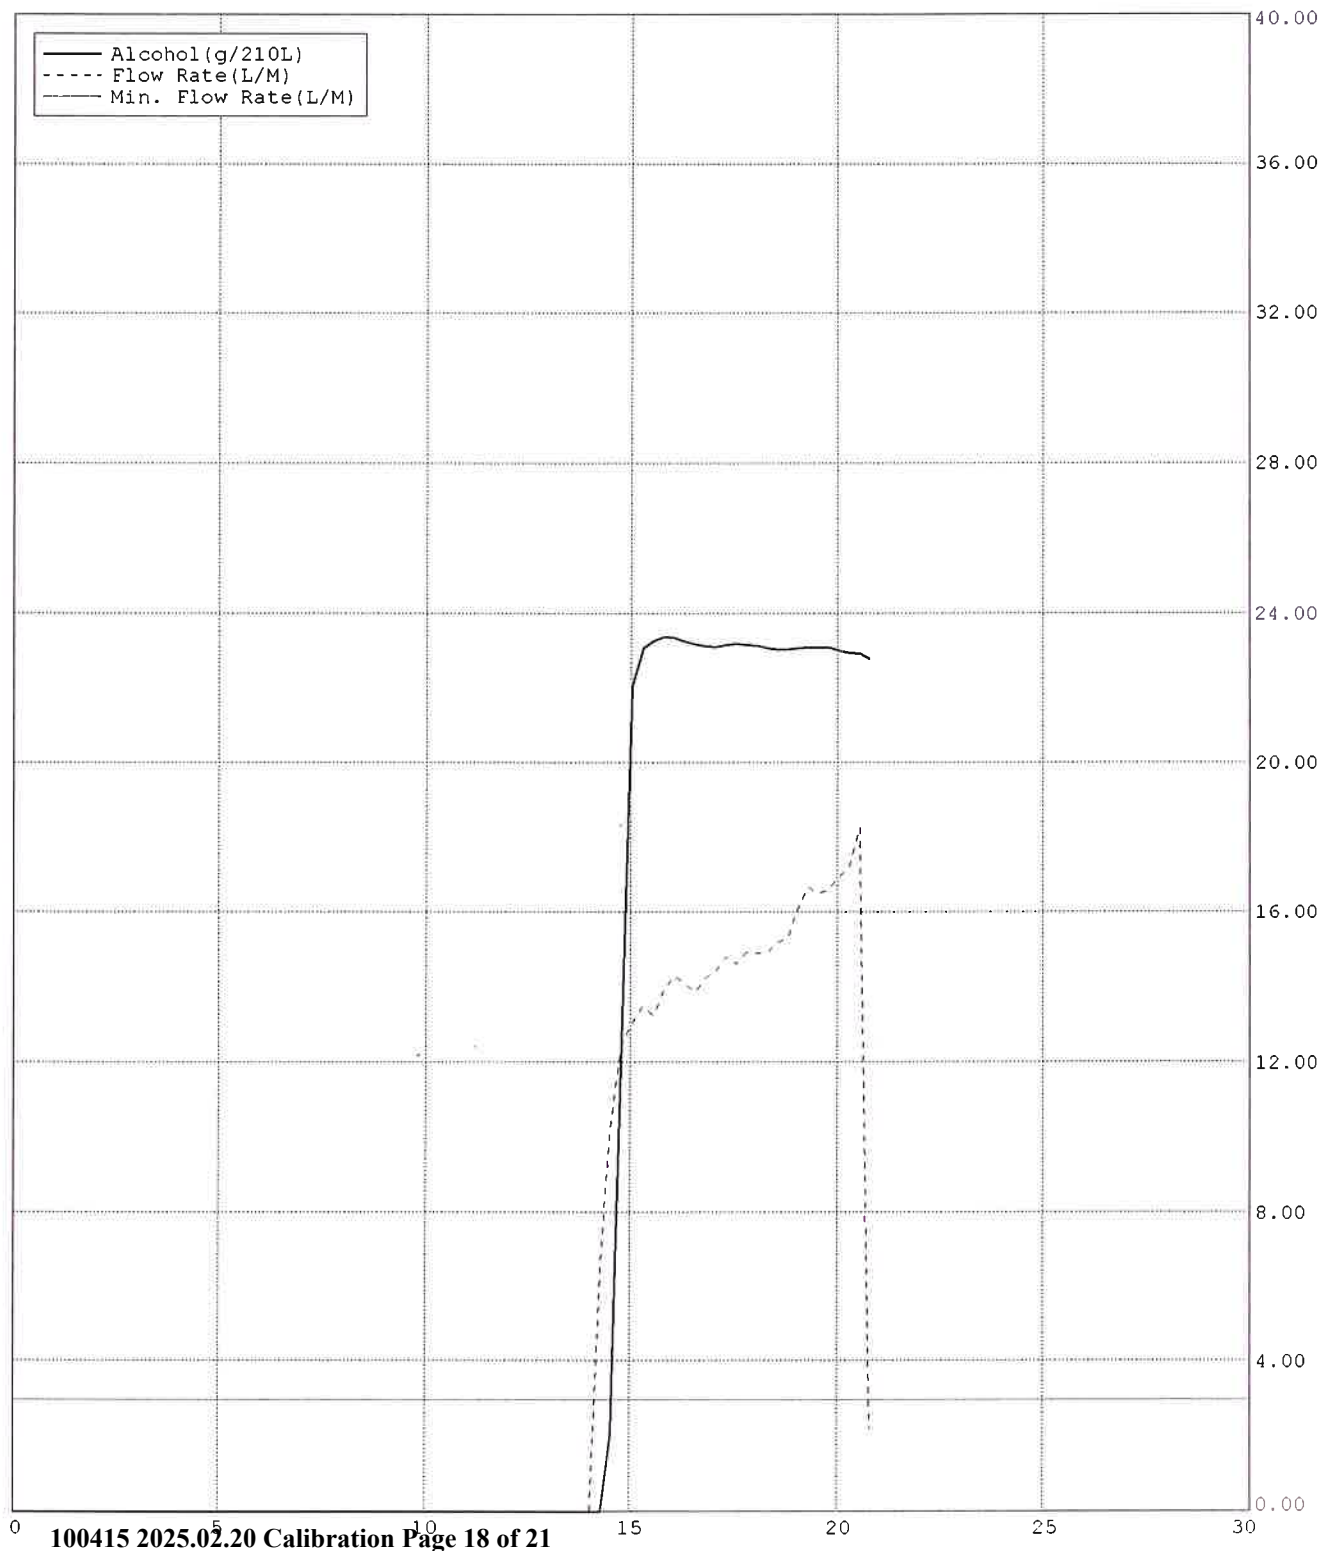

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 13:24:43

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.11: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:25
BLANK TEST	0.000	13:25
INTERNAL STANDARD	VERIFIED	13:25
Xq = 0.101 (0.43%)		
EXTERNAL STANDARD	0.077	13:26
X[1] = 0.0768 (-0.0016) (0.0018)		
BLANK TEST	0.000	13:27
SUBJECT SAMPLE	XXX	13:27
X[1] = 0.1215 (-0.0313) (0.0003)		

Interference Detected

KS

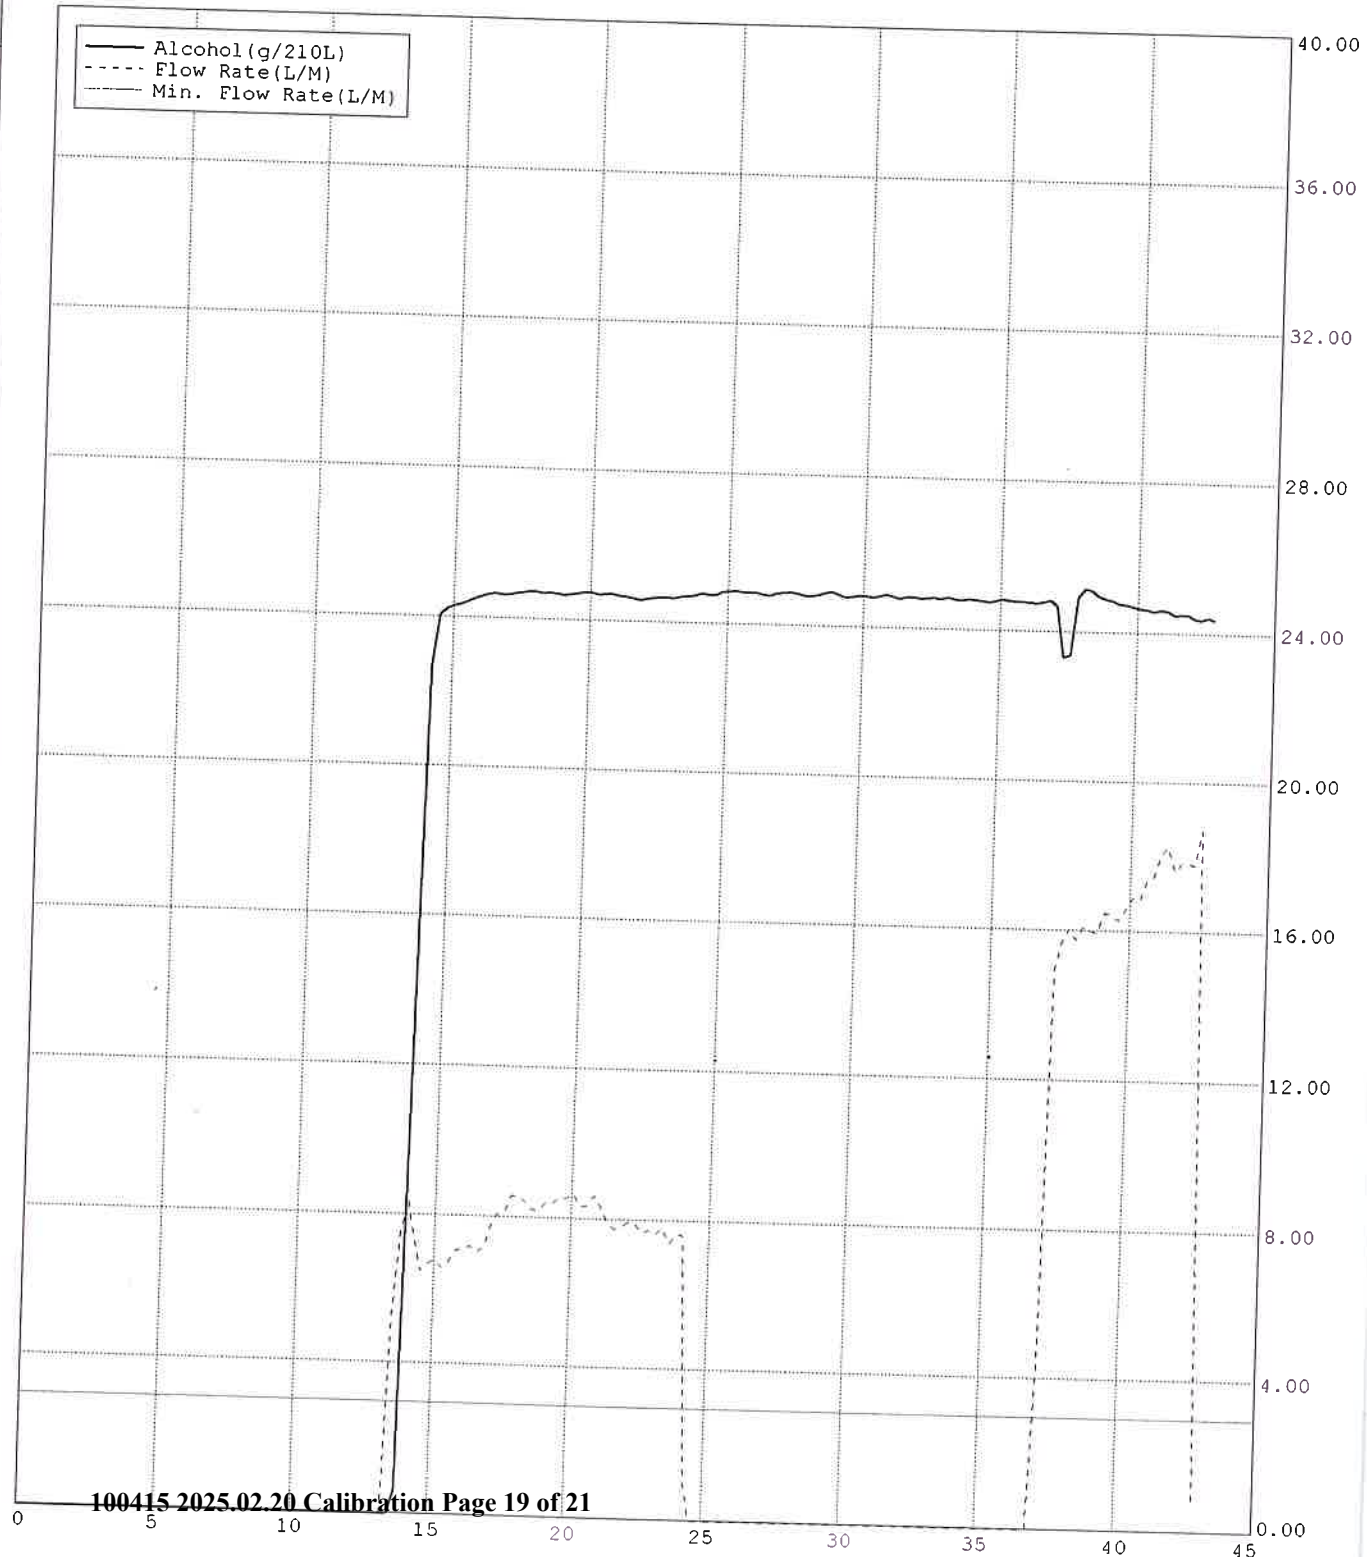

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 13:35:48

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.11: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:37
BLANK TEST	0.000	13:37
INTERNAL STANDARD	VERIFIED	13:37
Xq = 0.102 (0.78%)		
EXTERNAL STANDARD	0.077	13:37
X[1] = 0.0771 (-0.0014) (0.0017)		
BLANK TEST	0.000	13:38
SUBJECT SAMPLE (Vol=1.57L)	0.095	13:39
X[1] = 0.0957 (-0.0016) (-0.0003)		
BLANK TEST	0.000	13:40
EXTERNAL STANDARD	0.077	13:40
X[1] = 0.0774 (-0.0006) (0.0007)		
BLANK TEST	0.000	13:41

KS

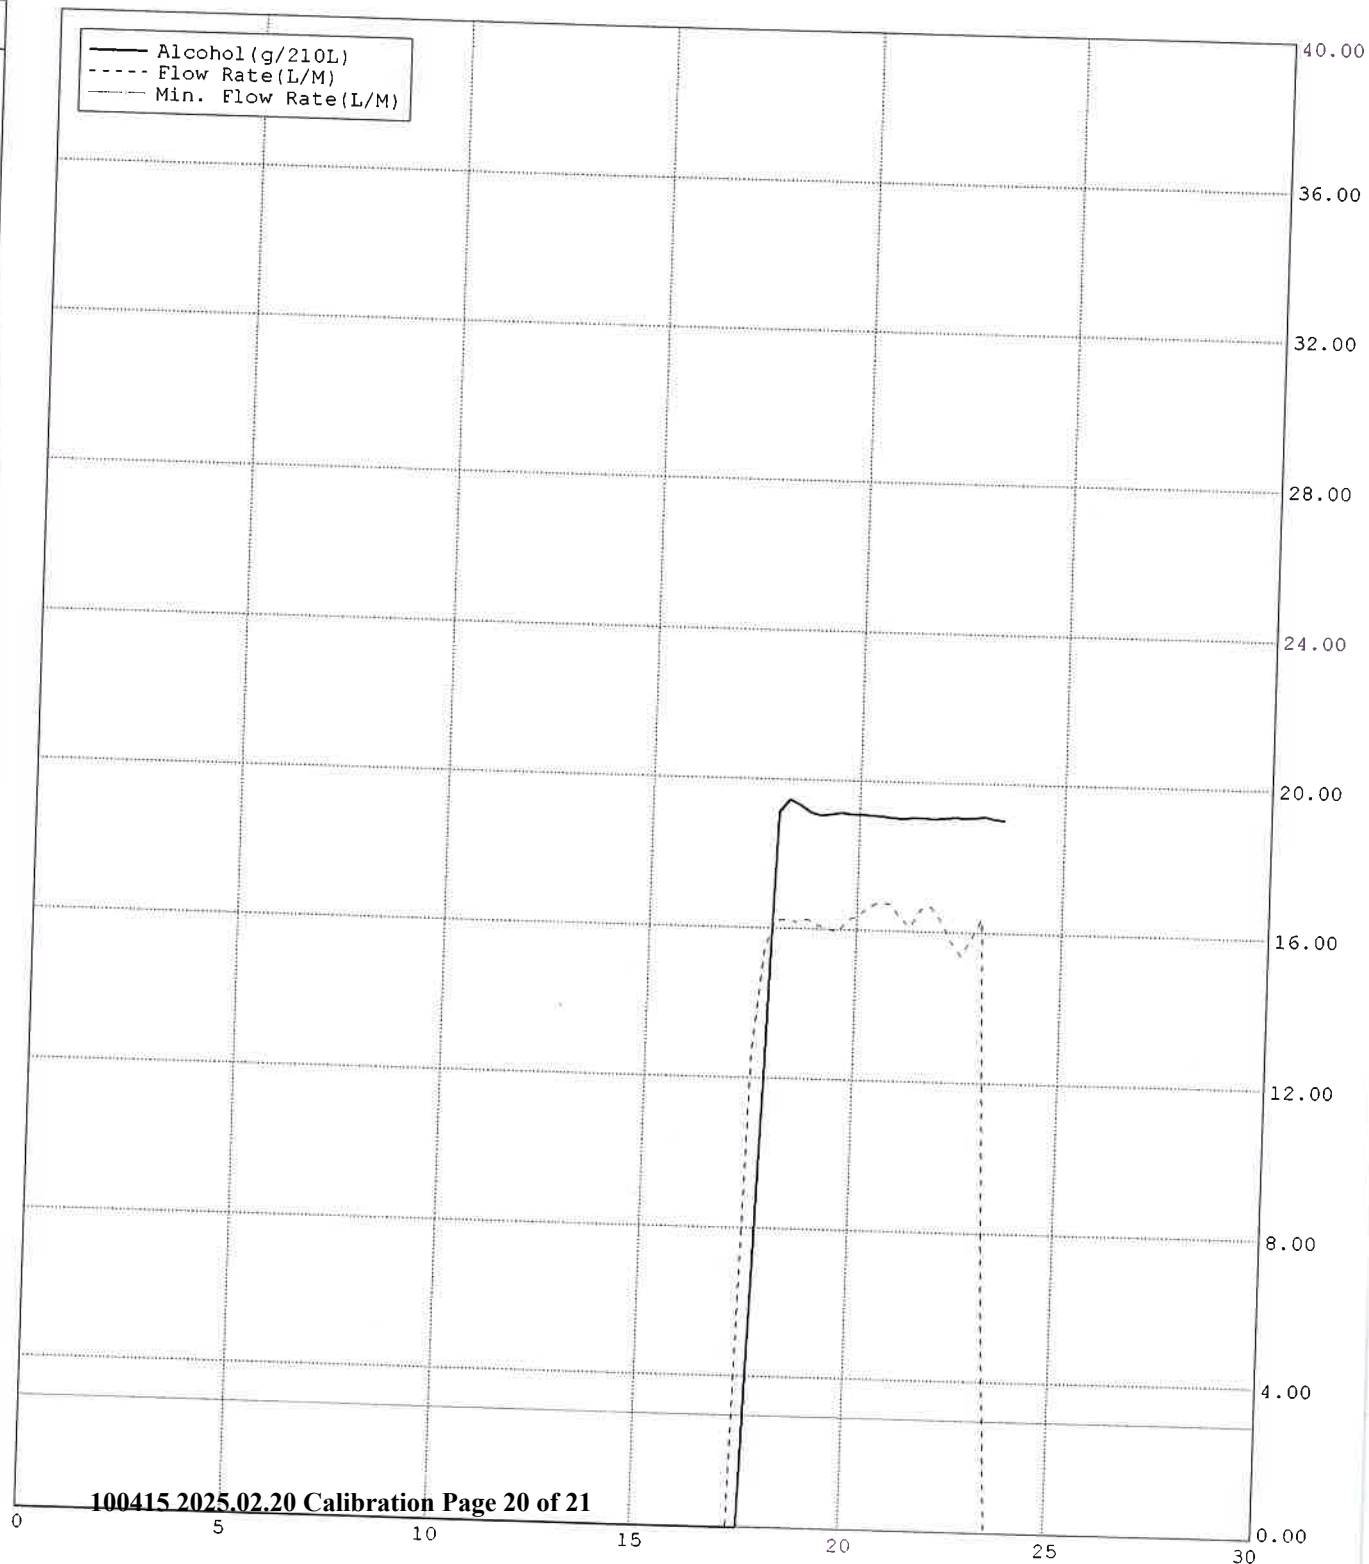

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100415

Date: 02/20/2025
Time: 14:02:33

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:03
BLANK TEST	0.000	14:04
INTERNAL STANDARD	VERIFIED	14:04
EXTERNAL STANDARD	0.077	14:04
BLANK TEST	0.000	14:05
SUBJECT SAMPLE (Vol=1.71L)	0.000	14:05
BLANK TEST	0.000	14:06
EXTERNAL STANDARD	0.078	14:06
BLANK TEST	0.000	14:07

KS

