

State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory
4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100375

Report Issue Date: 07/02/2025
Date Received: Not Recorded
Condition of Item: Not Recorded

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

No As-Found Data Collected

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.021	0.021	0.021	0.021	0.021	+/- 0.002
0.040	0.040	AG407908	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.079	AG335202	0.080	0.080	0.080	0.079	0.079	0.080	+/- 0.004
0.100	0.099	AG333401	0.100	0.099	0.100	0.100	0.100	0.100	+/- 0.004
0.150	0.149	AG332004	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.006
0.300	0.297	AG427706	0.294	0.294	0.293	0.293	0.294	0.294	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.66 Barometer Used: VWR S/N 240680771 Temperature (C): 21.7 Relative Humidity (%): 45
As-Left Lab Activity Date Range: 07/01/2025 - 07/02/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Carlie Glaister

Results authorized by Carlie Glaister on 07/02/2025

carlie.glaister@alaska.gov

Technically and administratively reviewed by Derek Walton on 07/02/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100375 Analyst or Technician Name: Carlie Glaister

DataMaster DMT Calibration Start Date: 7/1/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/2026
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.64 Temperature(C) 21.7 Relative Humidity(%) 45
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) – *Print with View Details*
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250603KS Expiration Date: 7/27/25
Simulator S/N: SD1200 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250603KS Expiration Date: 9/3/25
Simulator S/N: SD1198 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 9/20/25
Simulator S/N: SD1199 Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 230631096
Calibration Due Date: 9/19/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 7/1/25
Data Interpretation Date (Technician): NA (if applicable)
Data Interpretation Date (Analyst): 7/1/25

*In house
instrument
(Salmon)
CAG 7/1/25*

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100375

Date: 07/01/2025
 Time: 12:39:28

VERSIONS

DMT: 3.02
 PIC: 3.02
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.6°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 48.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.49 V	PASSED
(0.92 V - 2.16 V)	
Cooler Voltage = 1.67 V	PASSED
(0.92 V - 2.16 V)	
Bias Voltage = 79 V	PASSED
(47 V - 111 V)	
Chopper Freq = 518 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.6 in	

PUMP INFO

Flow Rate = 4.016 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

	PASSED
Xq = 0.091 0.19% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100375

Date: 07/01/2025

Time: 12:44 PM

Temperatures (°C)

Sample Cell: 48.9°C

Breath Tube: 47.8°C

Current Barometer 29.7 in

Volume (Ltr) 1.49

Settings

Lamp: 1.52 V

Bias: 79 V

Cooler: 1.73 V

Chopper: 519 Hz

Voltages (V)

Flow: 1.05 V

Detector: -0.002 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 04/12/2011
Time: 13:58:30

OPERATOR NAME:
COLLEEN S OBRYANT
CERTIFICATE #: 6237

LOT #: GUTH100
BOTTLE #: 10260
EXPIRATION: 10/25/2012

Ca = 0.1000
CAL = 0.979715 0.800 <= CAL < 1.200
b1 = 0.0001 0.0000 <= b1 < 0.0040
b2 = 0.0041 0.0010 <= b2 < 0.0100
b3 = 0.0003 0.0000 <= b3 < 0.0040
Xq = 0.0913 0.0500 <= Xq < 0.2000
a21 = 1.104953 1.050 <= a21 < 1.300
a31 = 0.439751 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 07/01/2025
Time: 12:46:14

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST
INTERNAL STANDARD
EXTERNAL STANDARD
BLANK TEST
SUBJECT SAMPLE (Vol=1.58L)
BLANK TEST
EXTERNAL STANDARD
BLANK TEST

PASSED
0.000
VERIFIED
0.079
0.000
0.000
0.000
0.080
0.000

12:47
12:47
12:47
12:47
12:48
12:49
12:50
12:51
12:52

CXG

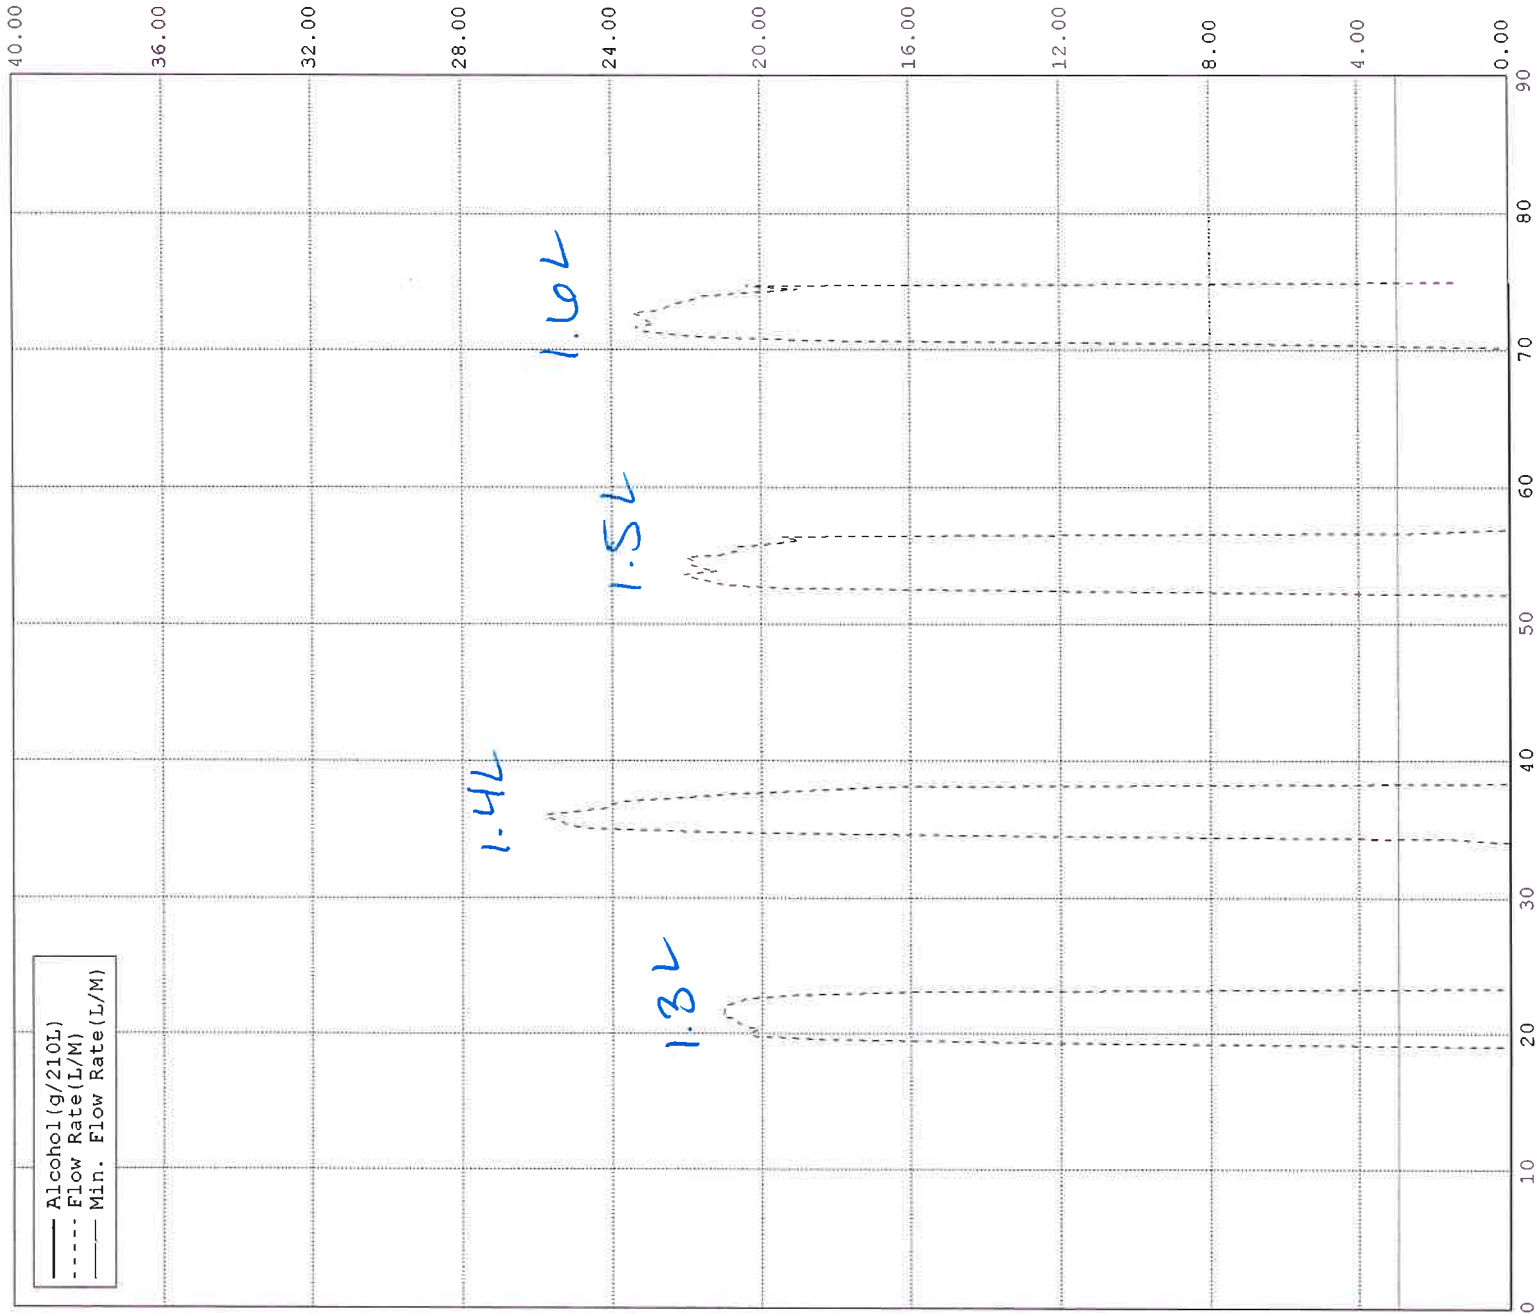

LINEARITY CHECK

Alaska Department of Public Safety
 DATAMASTER dnt: 100375


Date: 07/01/2025
 Time: 12:55:15

SUPERVISOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

TARGET	AVERAGE	STD. DEV.
0.020	0.0208	0.0004
0.040	0.0400	0.0000
0.079	0.0796	0.0005
0.099	0.0998	0.0004
0.149	0.1460	0.0000
0.297	0.2936	0.0005

SLOPE = 0.983450
 R² = 0.999889

CKG

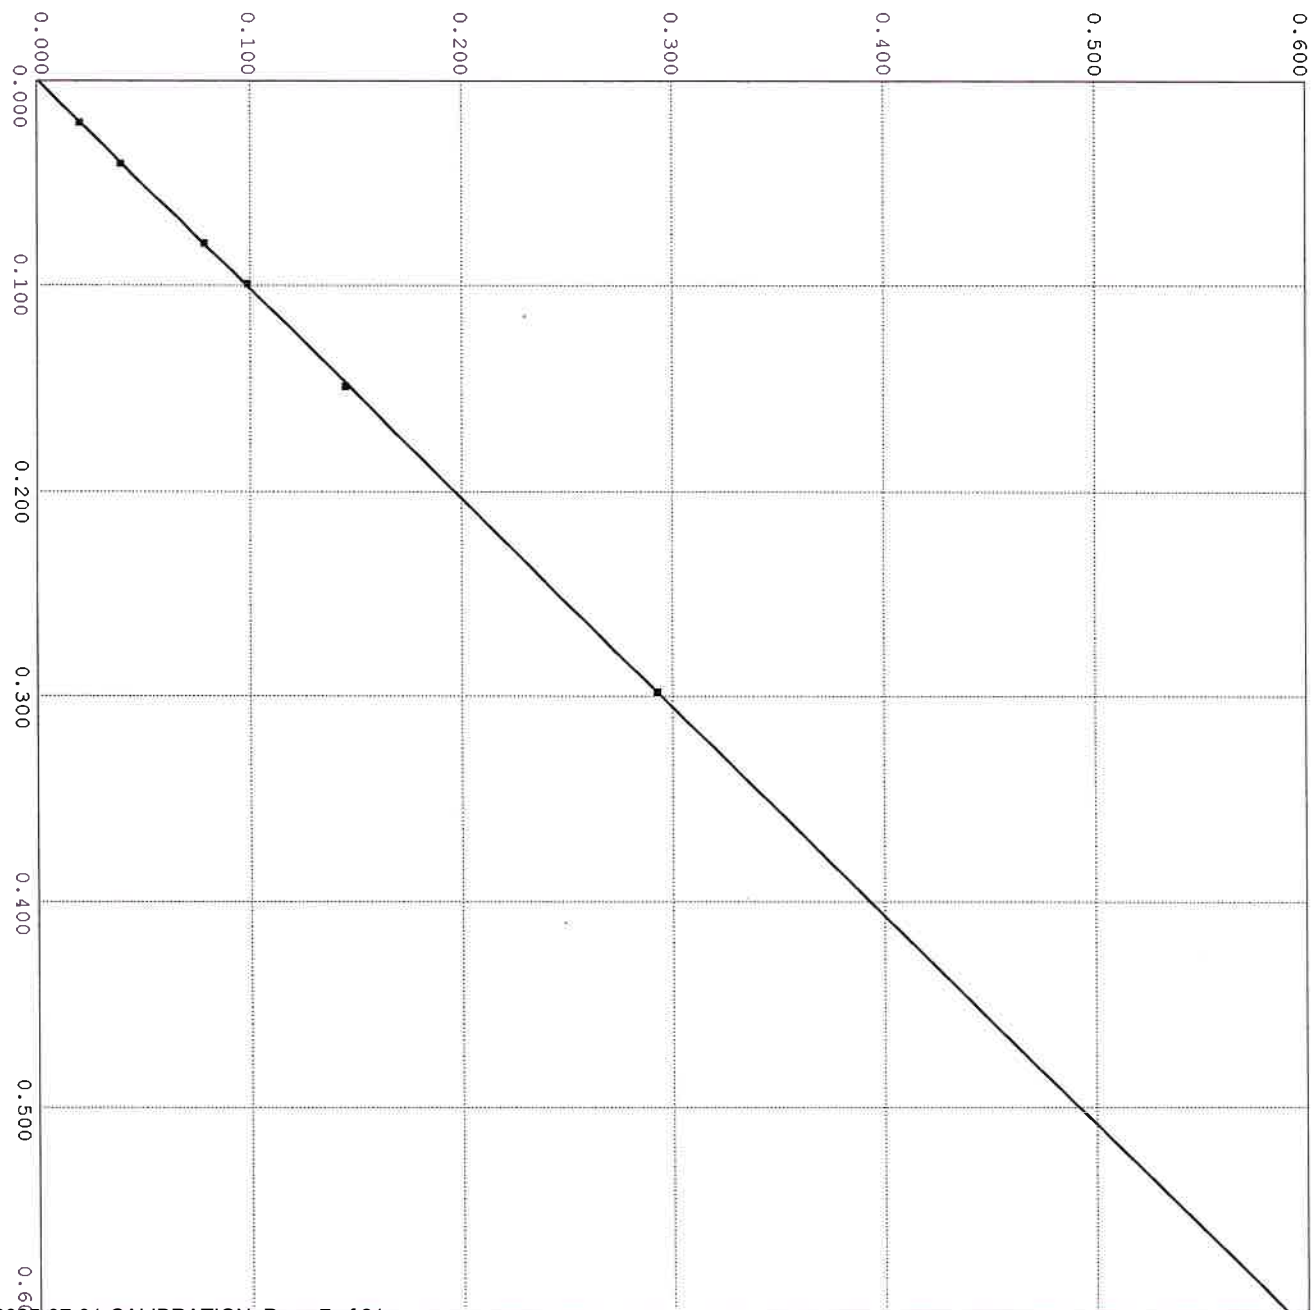

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 07/01/2025
Time: 12:55:17

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.65: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 628 psi

BLANK TEST	0.000	12:56
INTERNAL STANDARD	VERIFIED	12:56
EXTERNAL STANDARD	0.020	12:56
BLANK TEST	0.000	12:57
EXTERNAL STANDARD	0.021	12:58
BLANK TEST	0.000	12:58
EXTERNAL STANDARD	0.021	12:59
BLANK TEST	0.000	13:00
EXTERNAL STANDARD	0.021	13:00
BLANK TEST	0.000	13:01
EXTERNAL STANDARD	0.021	13:01
BLANK TEST	0.000	13:02

Average = 0.0208
Std Dev = 0.0004

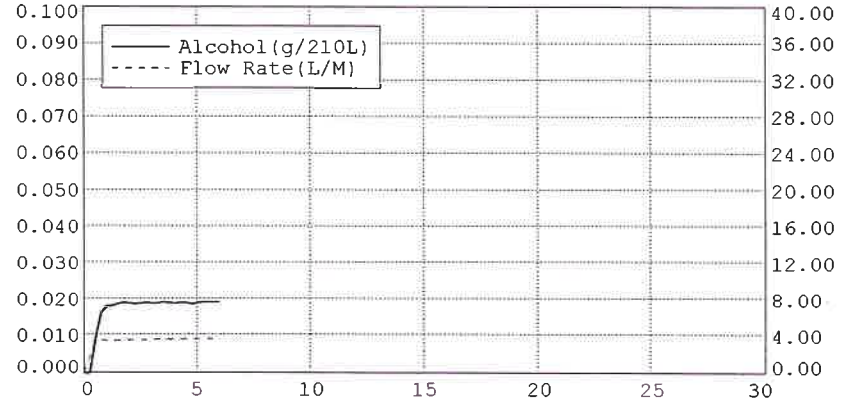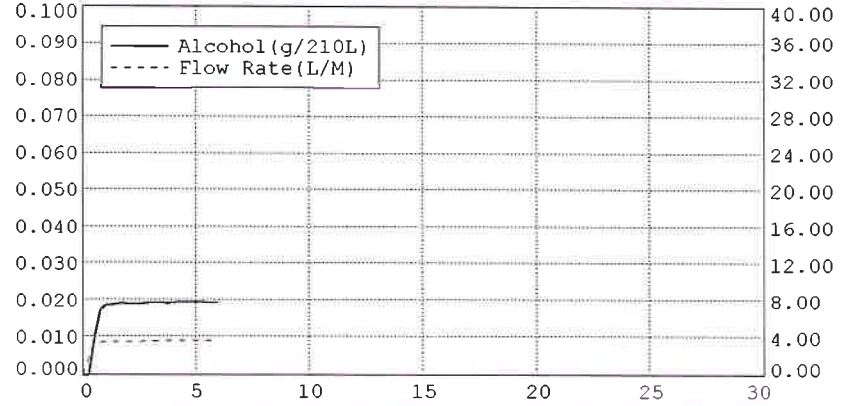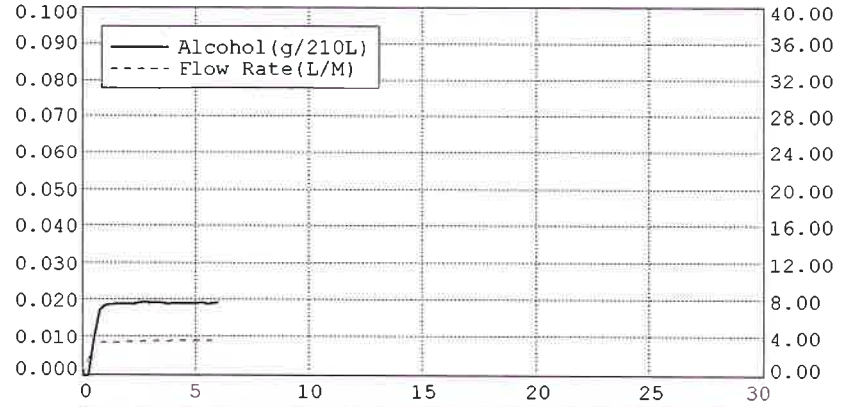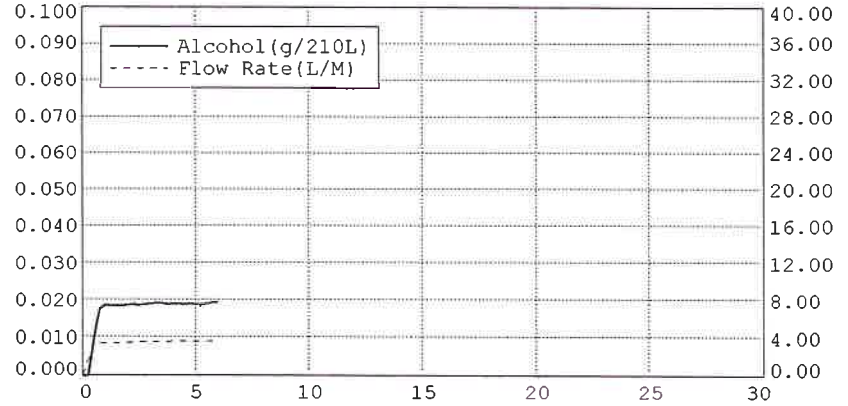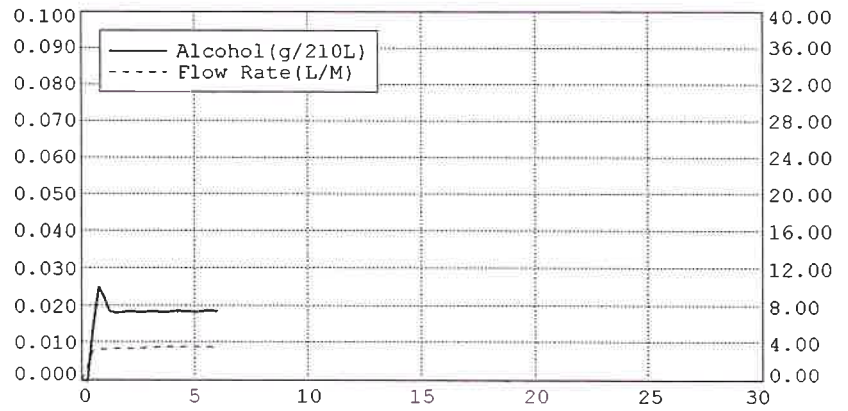

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 07/01/2025
Time: 13:02:57

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.65: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 985 psi

BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.040	13:04
BLANK TEST	0.000	13:05
EXTERNAL STANDARD	0.040	13:05
BLANK TEST	0.000	13:06
EXTERNAL STANDARD	0.040	13:06
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.040	13:07
BLANK TEST	0.000	13:08
EXTERNAL STANDARD	0.040	13:08
BLANK TEST	0.000	13:09

Average = 0.0400
Std Dev = 0.0000

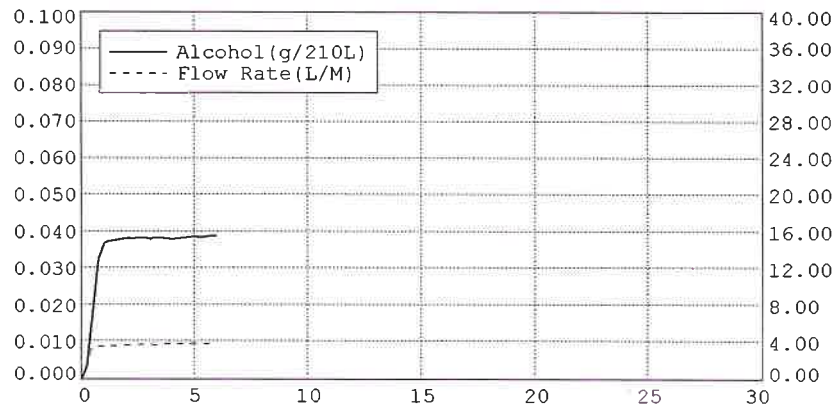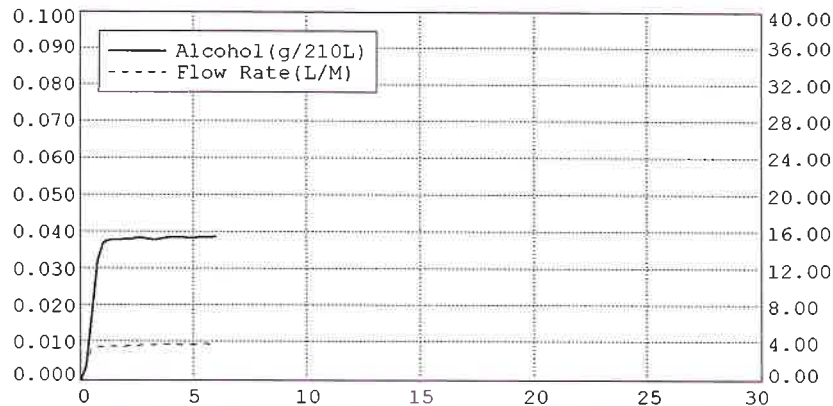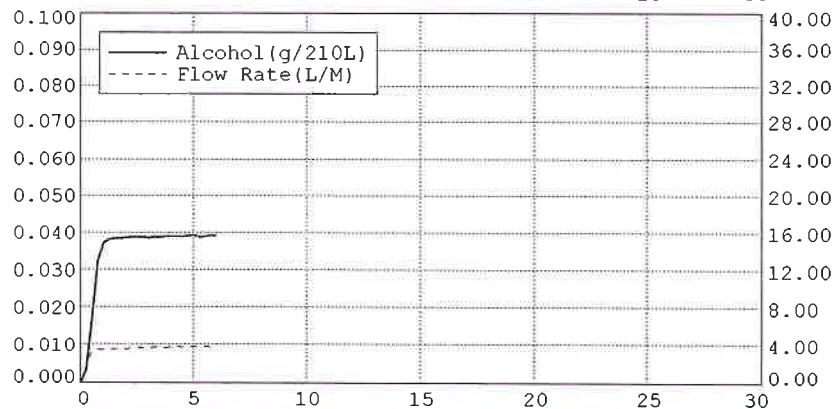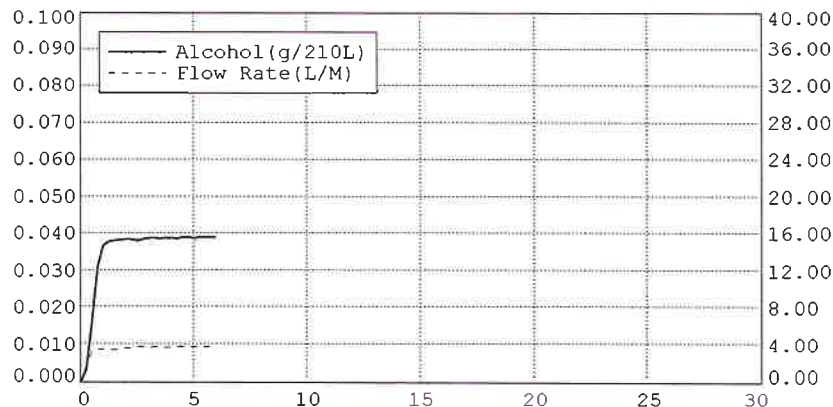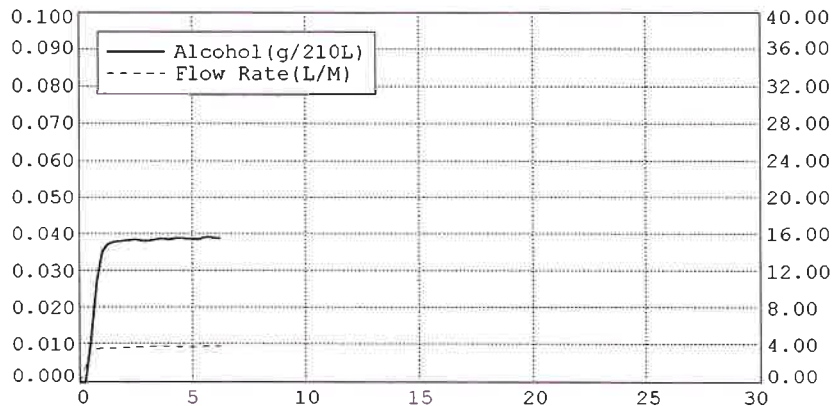

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 07/01/2025
Time: 13:10:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 828 psi

BLANK TEST	0.000	13:12
INTERNAL STANDARD	VERIFIED	13:12
EXTERNAL STANDARD	0.080	13:12
BLANK TEST	0.000	13:13
EXTERNAL STANDARD	0.080	13:13
BLANK TEST	0.000	13:14
EXTERNAL STANDARD	0.080	13:14
BLANK TEST	0.000	13:15
EXTERNAL STANDARD	0.079	13:15
BLANK TEST	0.000	13:16
EXTERNAL STANDARD	0.079	13:16
BLANK TEST	0.000	13:17

Average = 0.0796
Std Dev = 0.0005

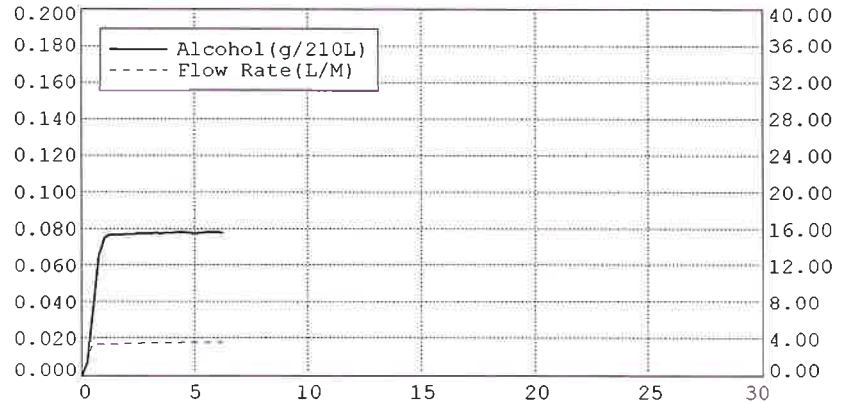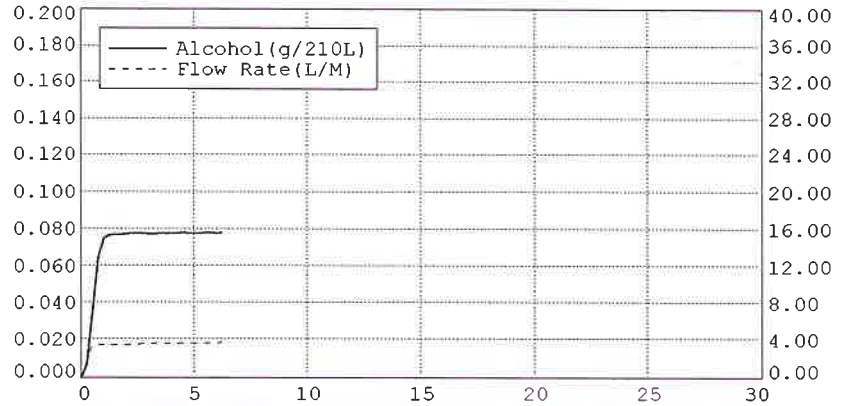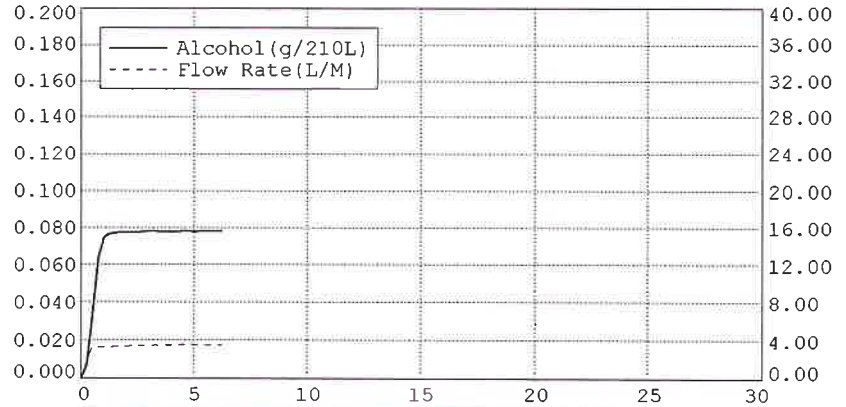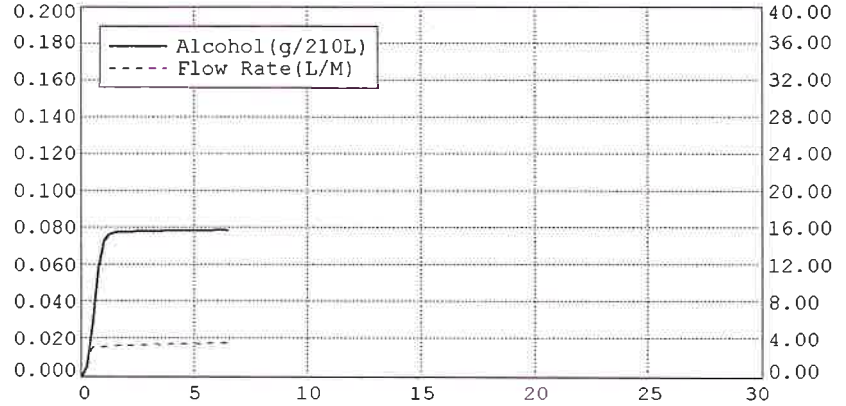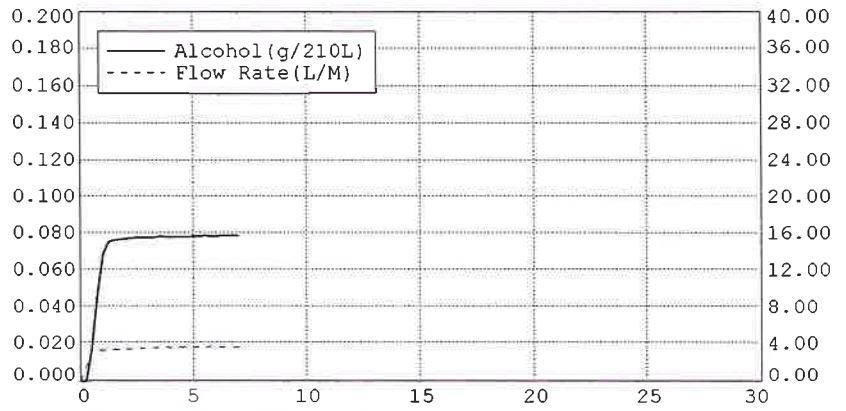

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 07/01/2025
Time: 13:18:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.65: 0.099
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 912 psi

BLANK TEST	0.000	13:20
INTERNAL STANDARD	VERIFIED	13:20
EXTERNAL STANDARD	0.100	13:20
BLANK TEST	0.000	13:21
EXTERNAL STANDARD	0.099	13:21
BLANK TEST	0.000	13:22
EXTERNAL STANDARD	0.100	13:22
BLANK TEST	0.000	13:23
EXTERNAL STANDARD	0.100	13:23
BLANK TEST	0.000	13:24
EXTERNAL STANDARD	0.100	13:24
BLANK TEST	0.000	13:25

Average = 0.0998
Std Dev = 0.0004

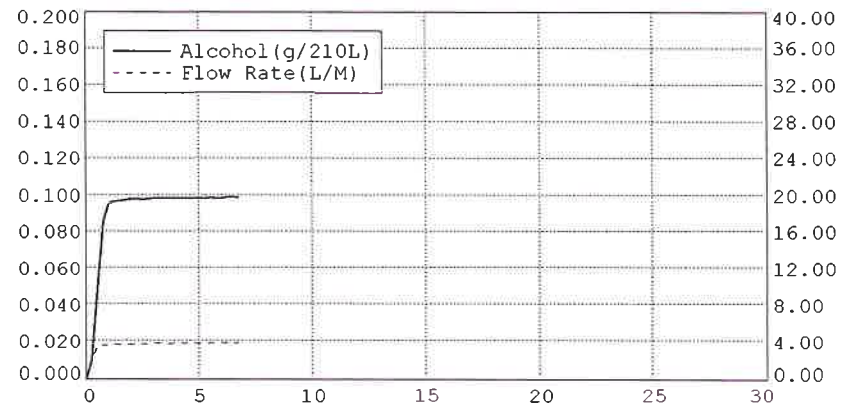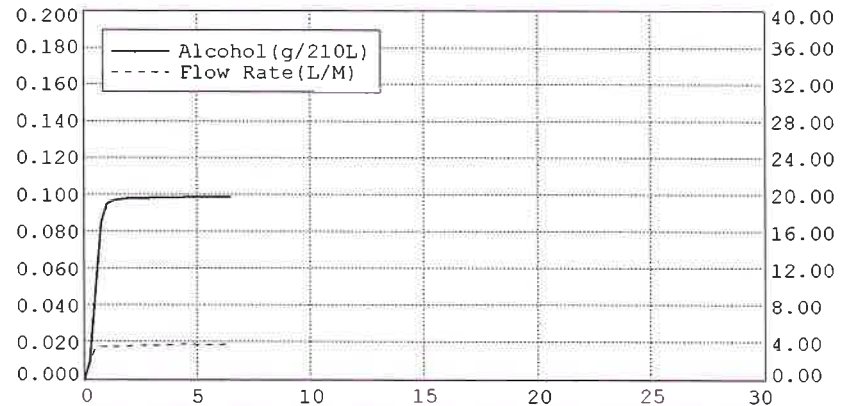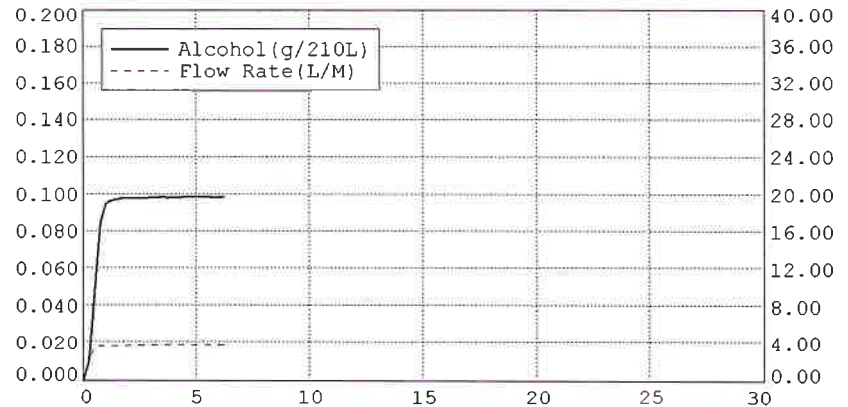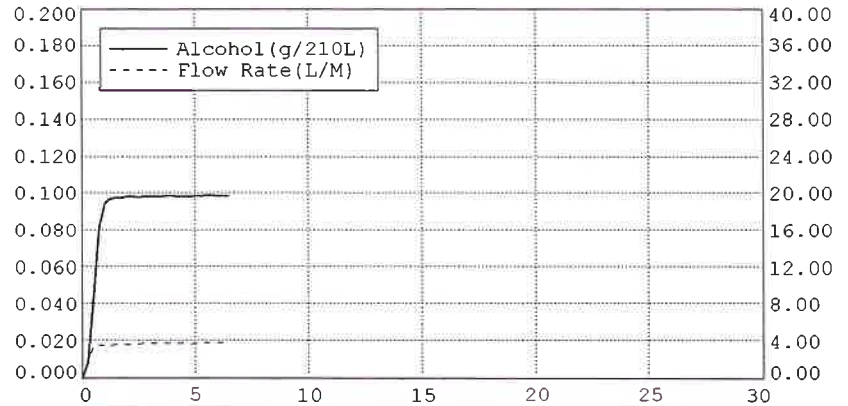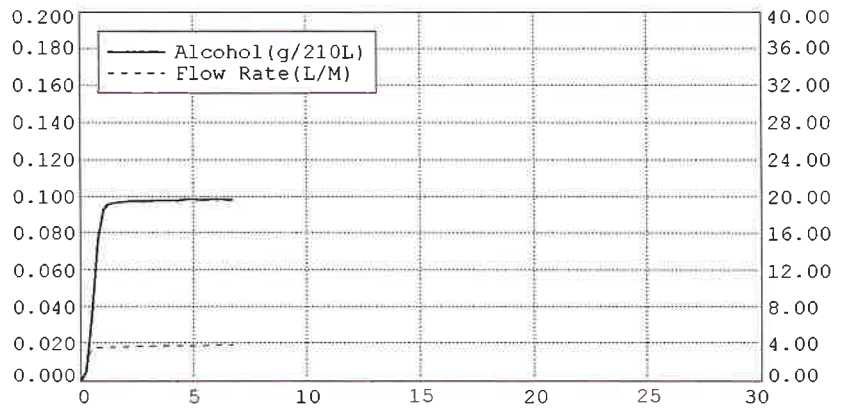

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 07/01/2025
Time: 13:27:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.65: 0.149
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 162 psi

BLANK TEST	0.000	13:29
INTERNAL STANDARD	VERIFIED	13:29
EXTERNAL STANDARD	0.146	13:29
BLANK TEST	0.000	13:30
EXTERNAL STANDARD	0.146	13:30
BLANK TEST	0.000	13:31
EXTERNAL STANDARD	0.146	13:31
BLANK TEST	0.000	13:32
EXTERNAL STANDARD	0.146	13:32
BLANK TEST	0.000	13:33
EXTERNAL STANDARD	0.146	13:33
BLANK TEST	0.000	13:34

Average = 0.1460
Std Dev = 0.0000

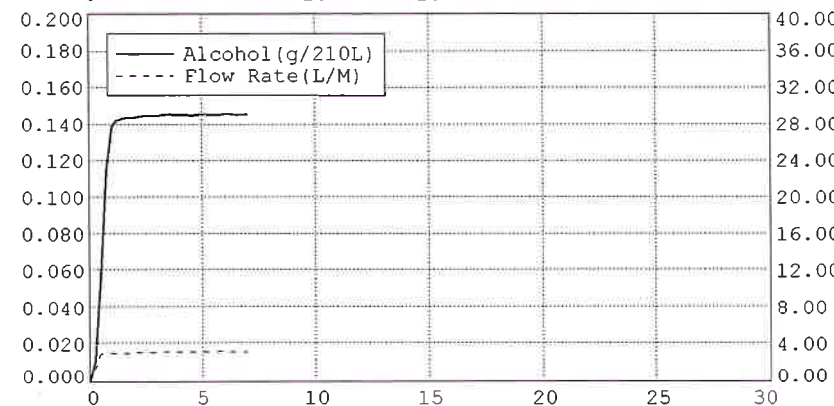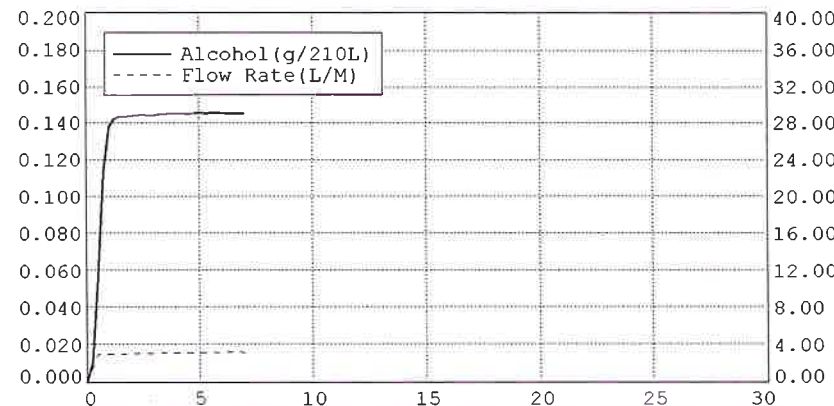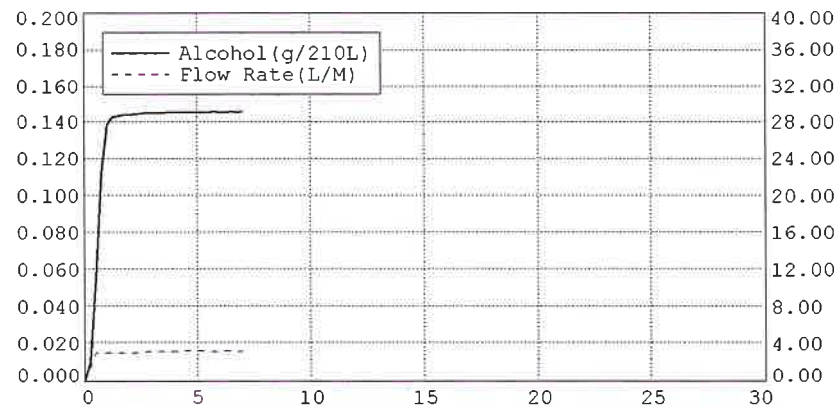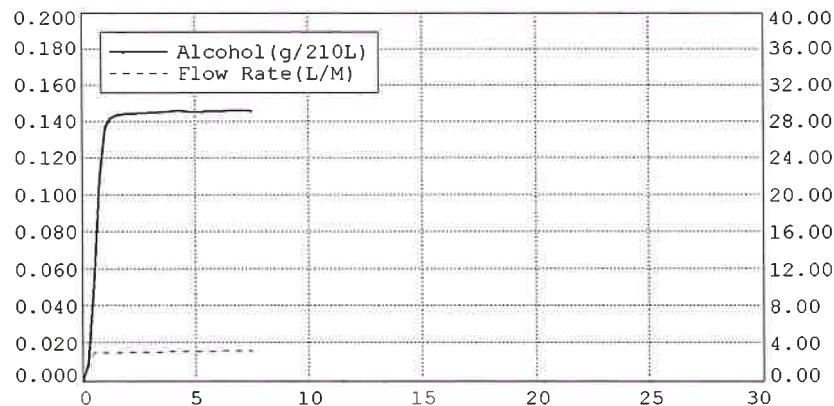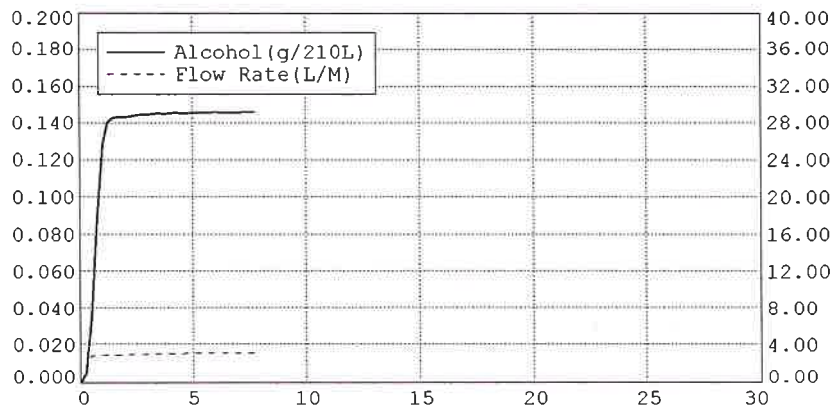

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100375






Date: 07/01/2025
Time: 13:35:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.65: 0.297
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 175 psi

BLANK TEST	0.000	13:37
INTERNAL STANDARD	VERIFIED	13:37
EXTERNAL STANDARD	0.294	13:37
BLANK TEST	0.000	13:38
EXTERNAL STANDARD	0.294	13:38
BLANK TEST	0.000	13:39
EXTERNAL STANDARD	0.293	13:39
BLANK TEST	0.000	13:40
EXTERNAL STANDARD	0.293	13:41
BLANK TEST	0.000	13:42
EXTERNAL STANDARD	0.294	13:42
BLANK TEST	0.000	13:43

Average = 0.2936
Std Dev = 0.0005

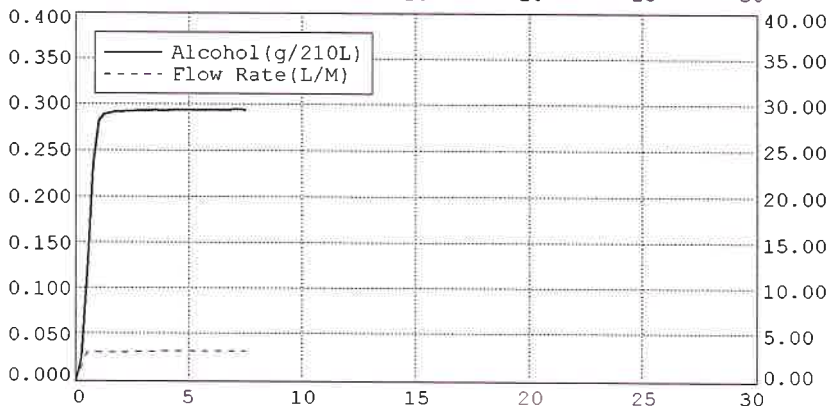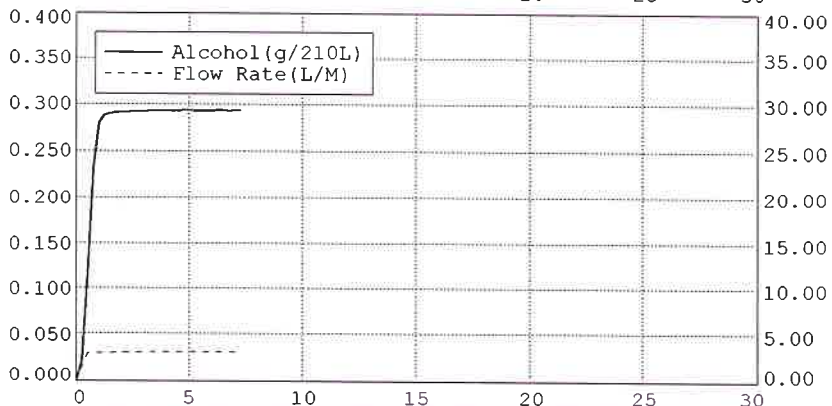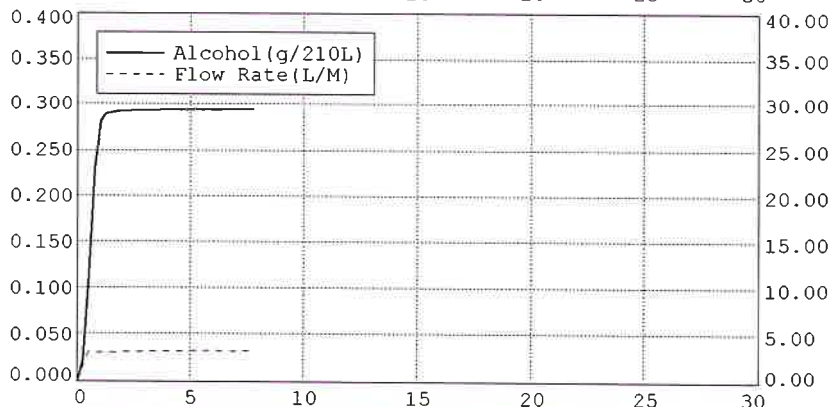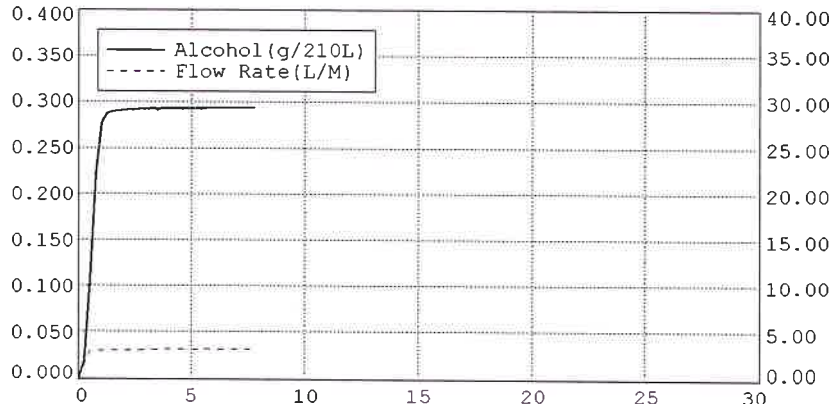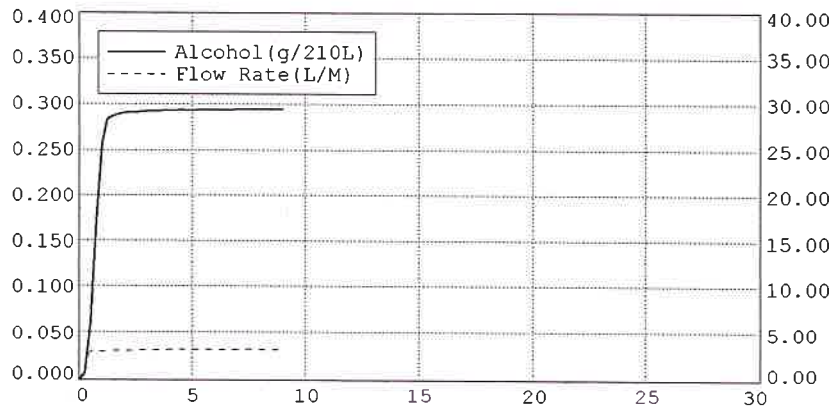

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100375

Date: 07/01/2025
Time: 13:47:54

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.65: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:49
BLANK TEST	0.000	13:49
INTERNAL STANDARD	VERIFIED	13:49
EXTERNAL STANDARD	0.079	13:49
BLANK TEST	0.000	13:50
SUBJECT SAMPLE	INCOMPLETE	13:52

CLG

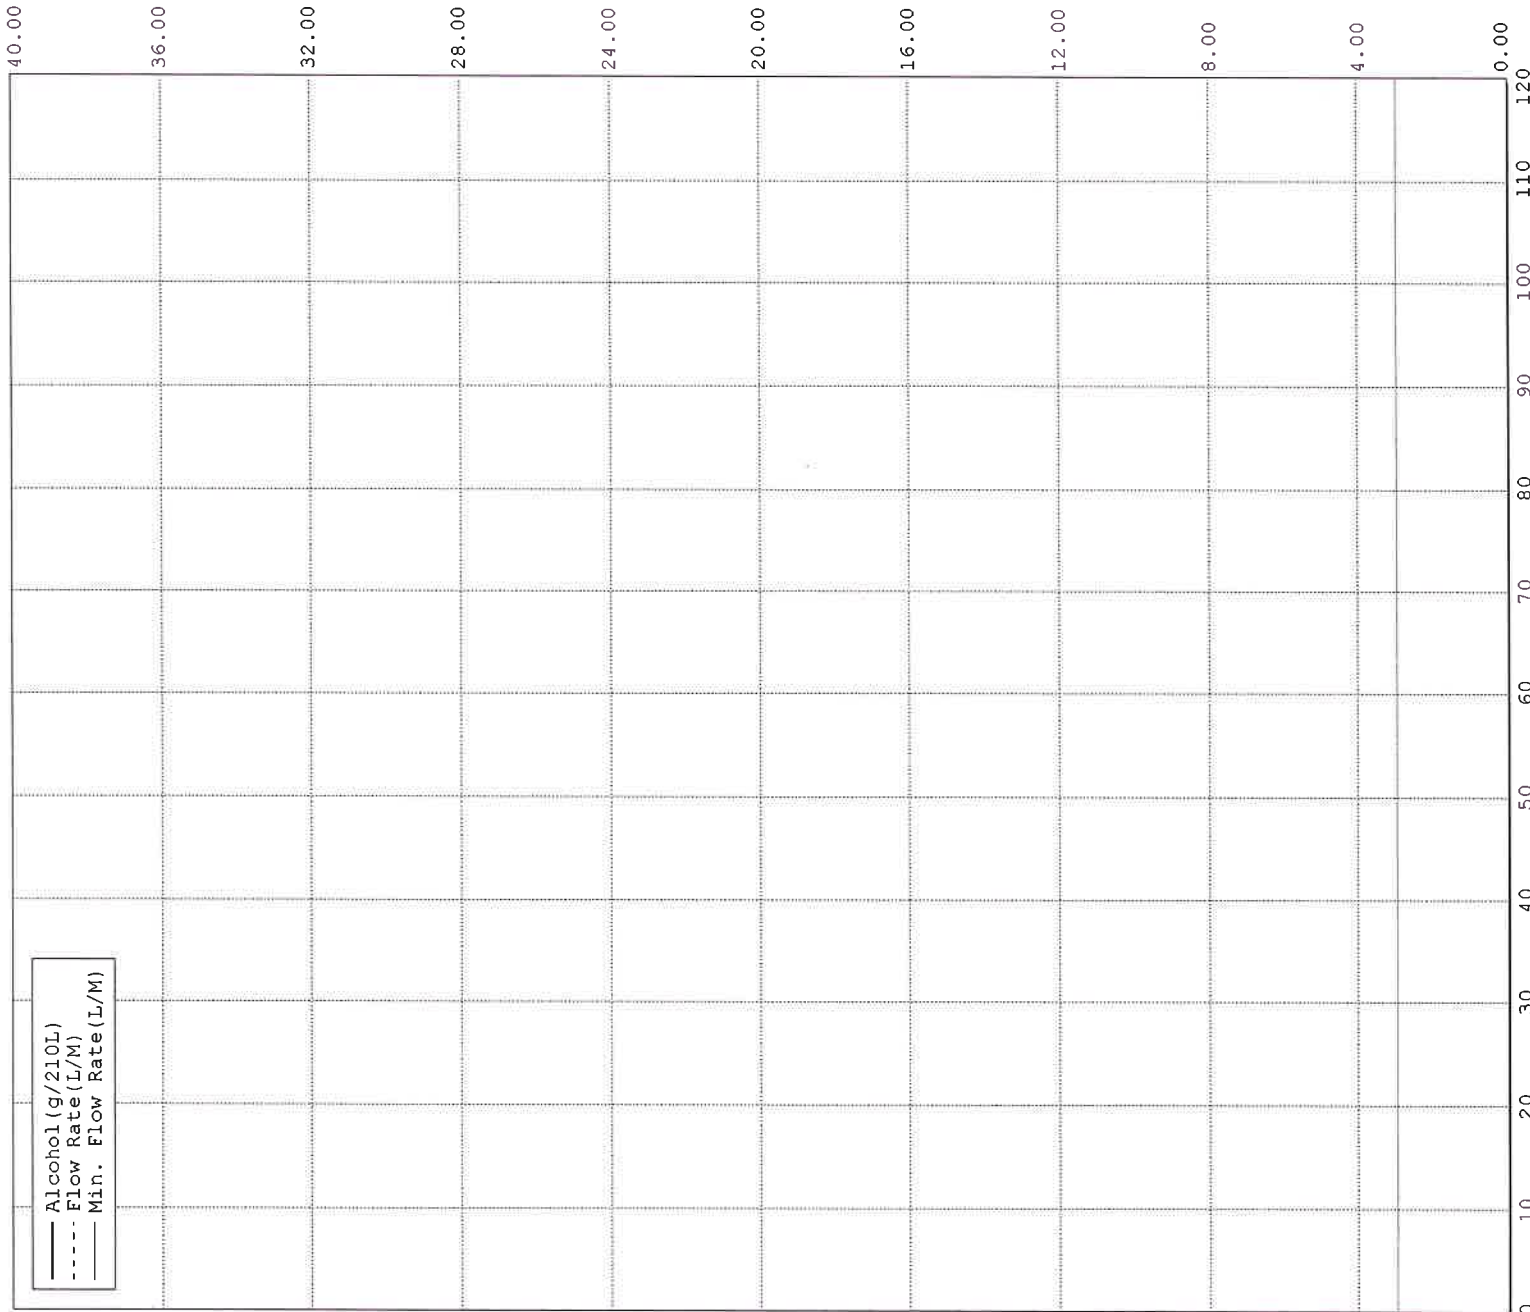

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 07/01/2025
Time: 14:11:58

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:14
BLANK TEST	0.000	14:14
INTERNAL STANDARD	VERIFIED	14:14
EXTERNAL STANDARD	0.079	14:14
BLANK TEST	0.000	14:15
SUBJECT SAMPLE	XXX	14:16

Maximum Attempts Exceeded

OKG

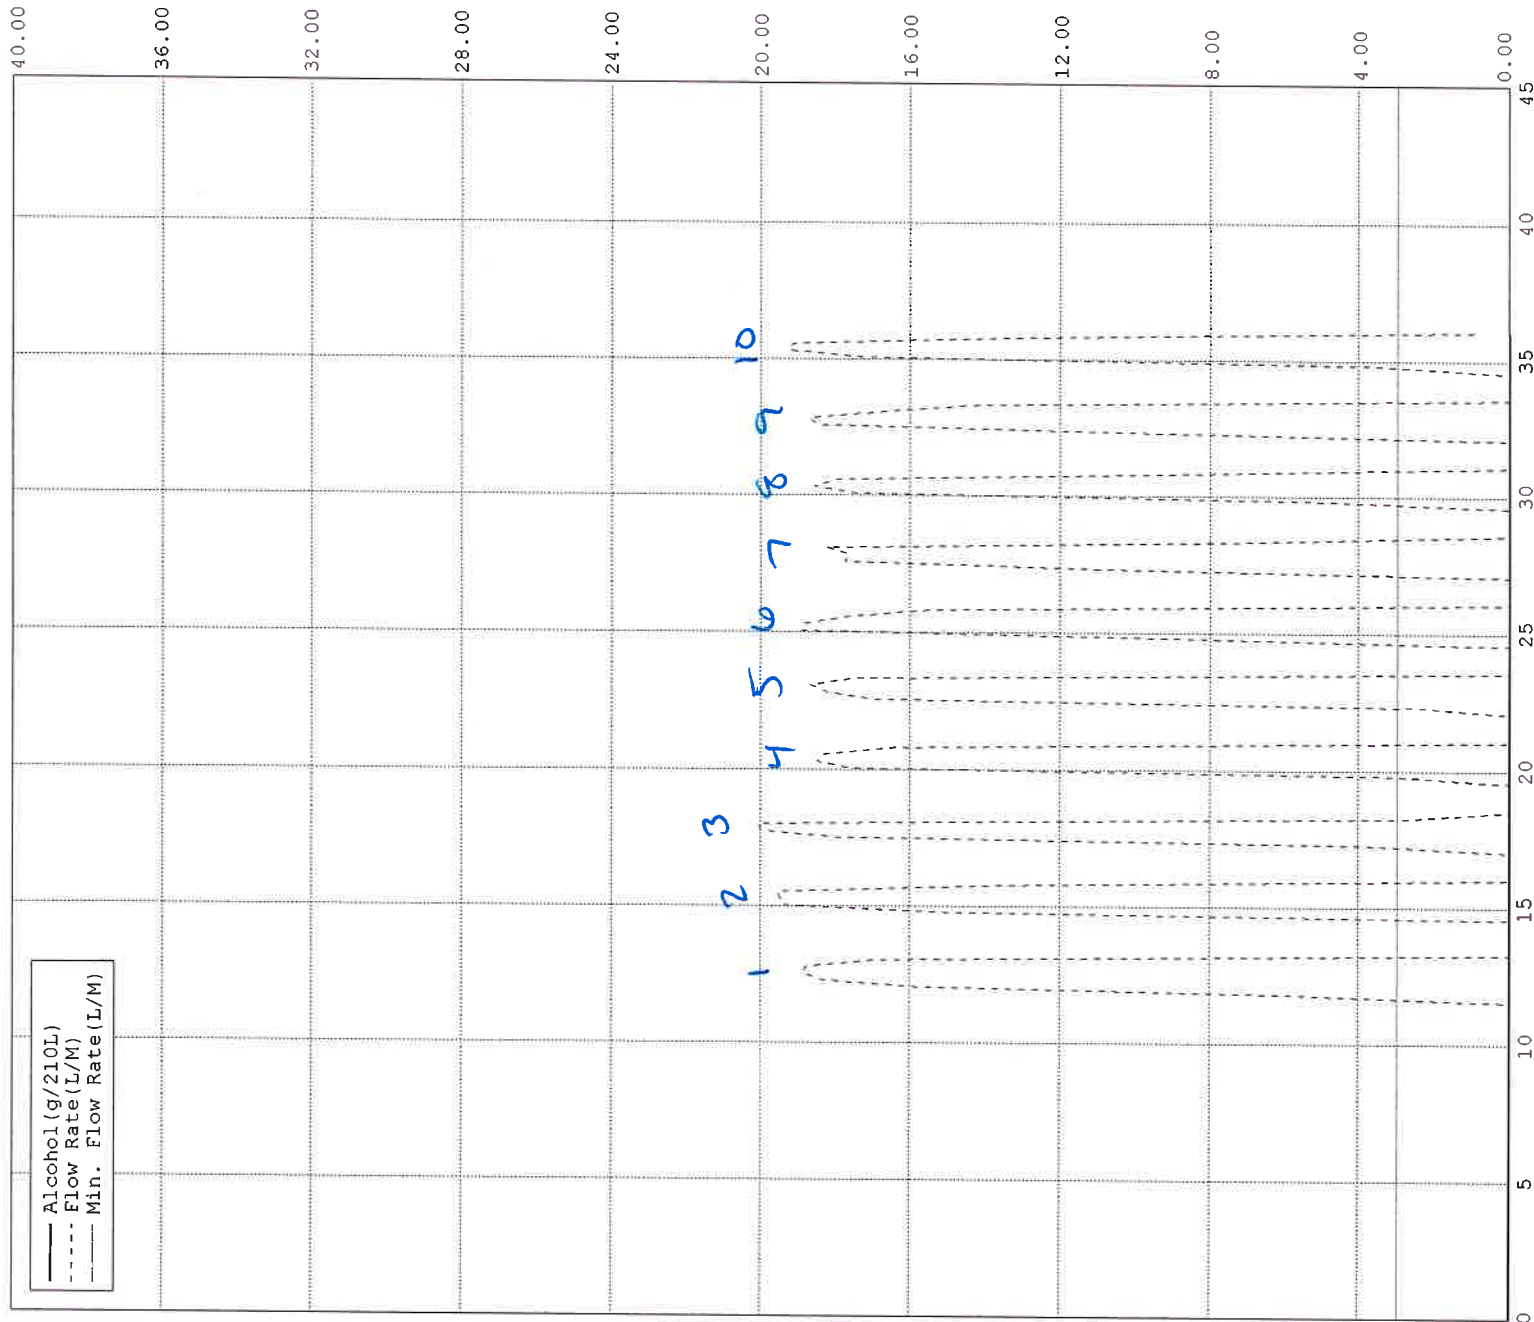

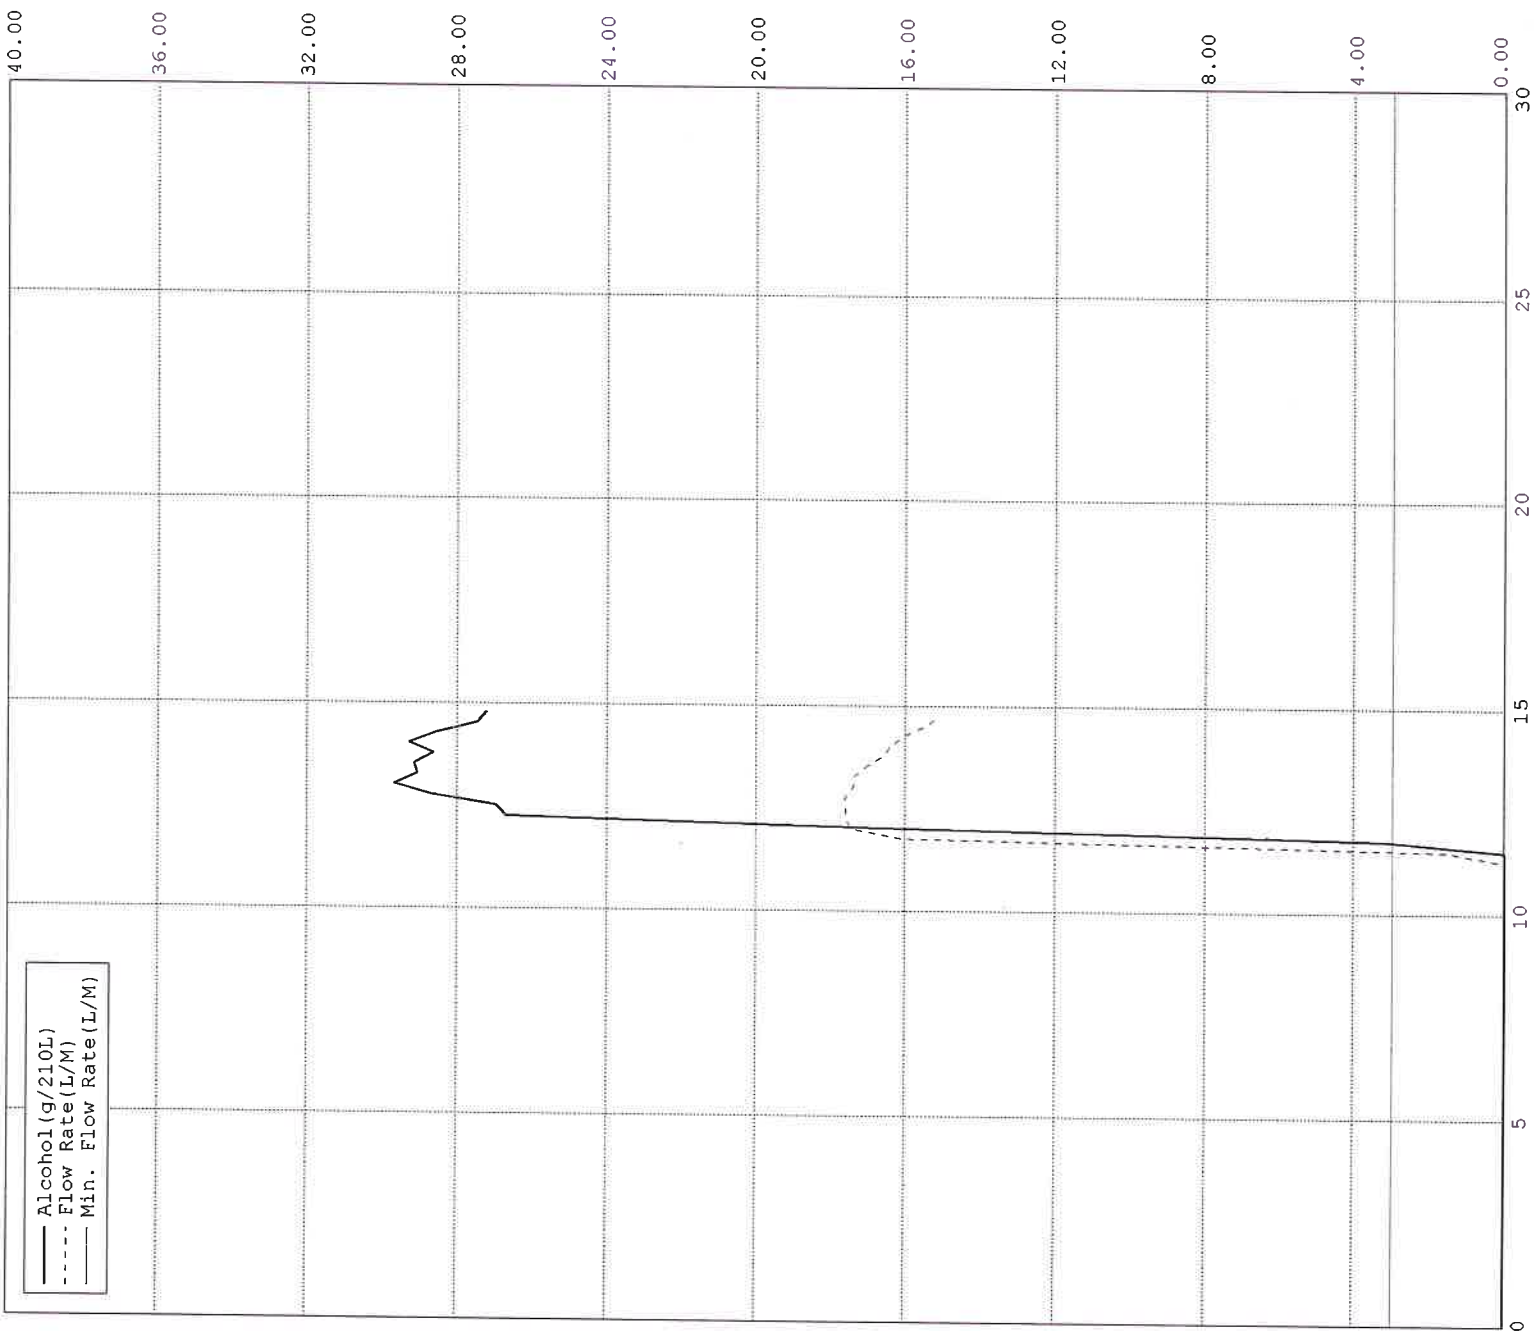

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 07/01/2025
Time: 14:18:45

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
INVALID

CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	14:19
BLANK TEST	0.000	14:20
INTERNAL STANDARD	VERIFIED	14:20
EXTERNAL STANDARD	0.079	14:20
BLANK TEST	0.000	14:21
SUBJECT SAMPLE	INVALID	14:21

OXG

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100375

Date: 07/01/2025

Time: 14:24:03

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

RFI

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.64: 0.079

LOT #: AG335202


EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:25
BLANK TEST	0.000	14:25
INTERNAL STANDARD	VERIFIED	14:25
EXTERNAL STANDARD	0.079	14:25
BLANK TEST	0.000	14:26

RFI DETECTED

0165

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

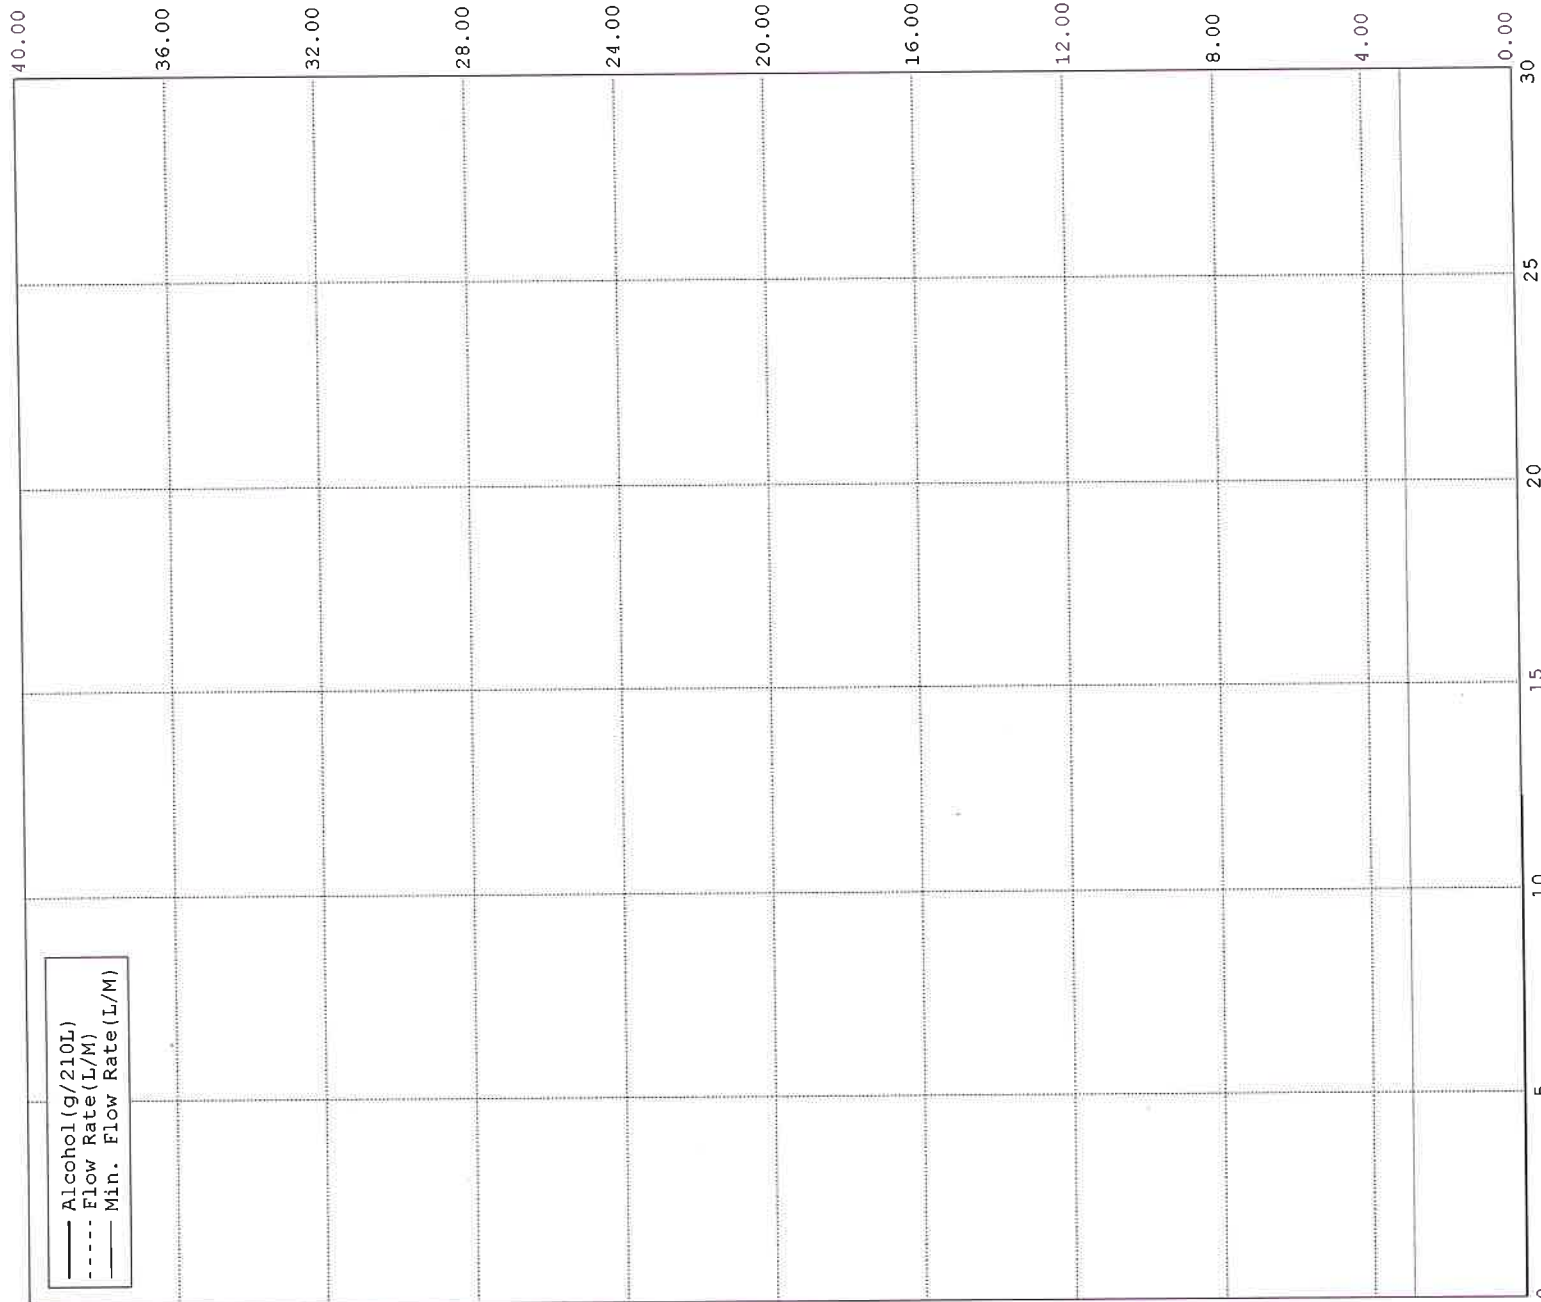

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100375

Date: 07/01/2025
 Time: 14:30:09

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXXX

OPERATOR NAME:
 CARLIE GLAISTER
 OPERATOR'S #: 10436

DEPT/AGENCY:
 INTERFERENCE - ACETONE
 CASE/REPORT: XXXX
 TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.65: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:31
BLANK TEST	0.000	14:31
INTERNAL STANDARD	VERIFIED	14:31
Xq = 0.091 (0.10%)		
EXTERNAL STANDARD	0.079	14:31
X[1] = 0.0792 (0.0001)	(0.0013)	
BLANK TEST	0.000	14:32
SUBJECT SAMPLE	XXX	14:33
X[1] = 0.1071 (-0.0189)	(0.0008)	

Interference Detected

Filter 2 Avg: 0.0001
 Filter 3 Avg: 0.0012
 ONV-711125

CVG

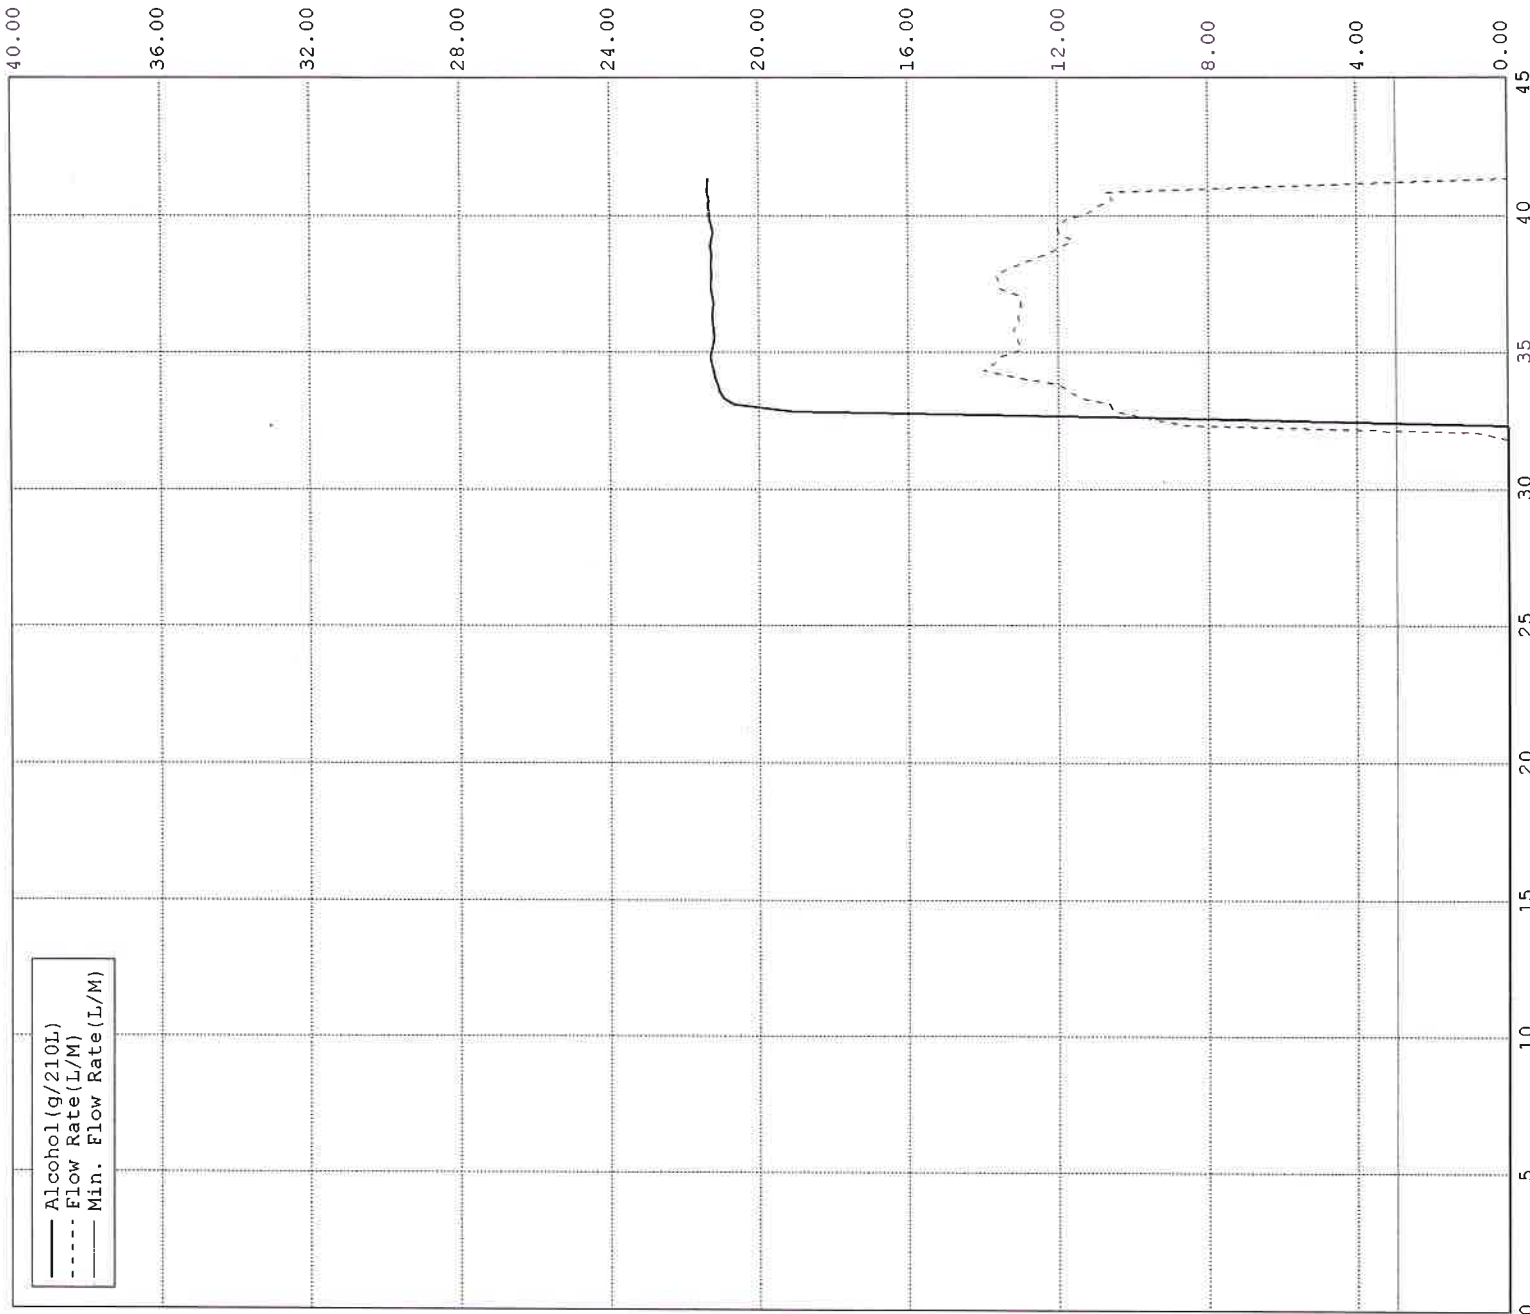

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100375

Date: 07/01/2025
Time: 14:35:02

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - IPA

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.65: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 14:36

BLANK TEST 0.000 14:37

INTERNAL STANDARD VERIFIED 14:37

$X_q = 0.091$ (0.38%)

EXTERNAL STANDARD 0.079 14:37

$X[1] = 0.0789$ (-0.0006) (0.0009)


BLANK TEST 0.000 14:38

SUBJECT SAMPLE XXX 14:38

$X[1] = 0.1161$ (-0.0174) (0.0029)

Interference Detected

OKG

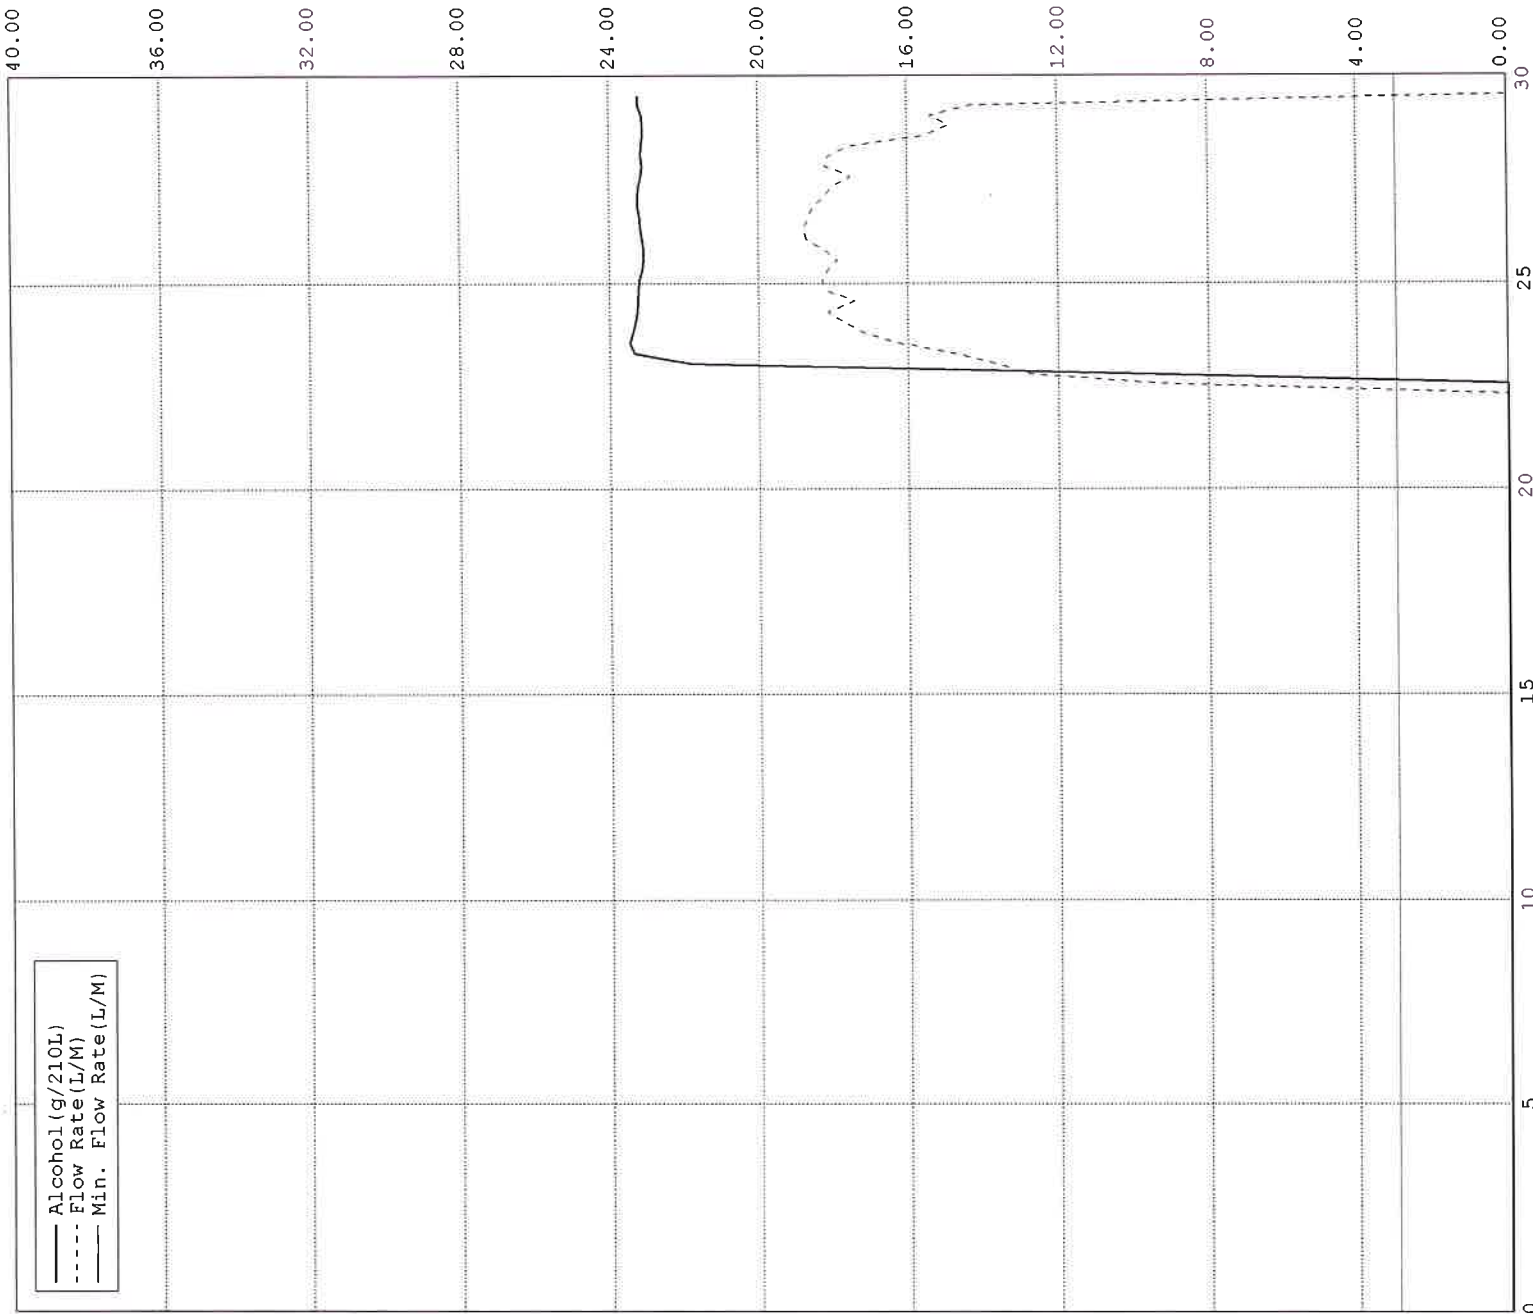

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100375

Date: 07/01/2025

Time: 14:41:21

SUBJECT NAME:

TEST TEST

LICENSE #: XXXX

OPERATOR NAME:

CARLIE GLAISTER

OPERATOR'S #: 10436

DEPT/AGENCY:

INTERFERENCE - NEGATIVE

CASE/REPORT: XXXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 29.64: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:43
BLANK TEST	0.000	14:43
INTERNAL STANDARD	VERIFIED	14:43
$x_q = 0.091$ (0.19%)	0.079	14:43
EXTERNAL STANDARD	(0.0012)	
$x[1] = 0.0791$ (0.0009)	0.000	14:44
BLANK TEST	0.000	14:45
SUBJECT SAMPLE (Vol=1.86L)	0.091	
$x[1] = 0.0917$ (0.0008)	(0.0003)	
BLANK TEST	0.000	14:46
EXTERNAL STANDARD	0.079	14:46
$x[1] = 0.0790$ (0.0001)	(0.0014)	
BLANK TEST	0.000	14:47

CMS

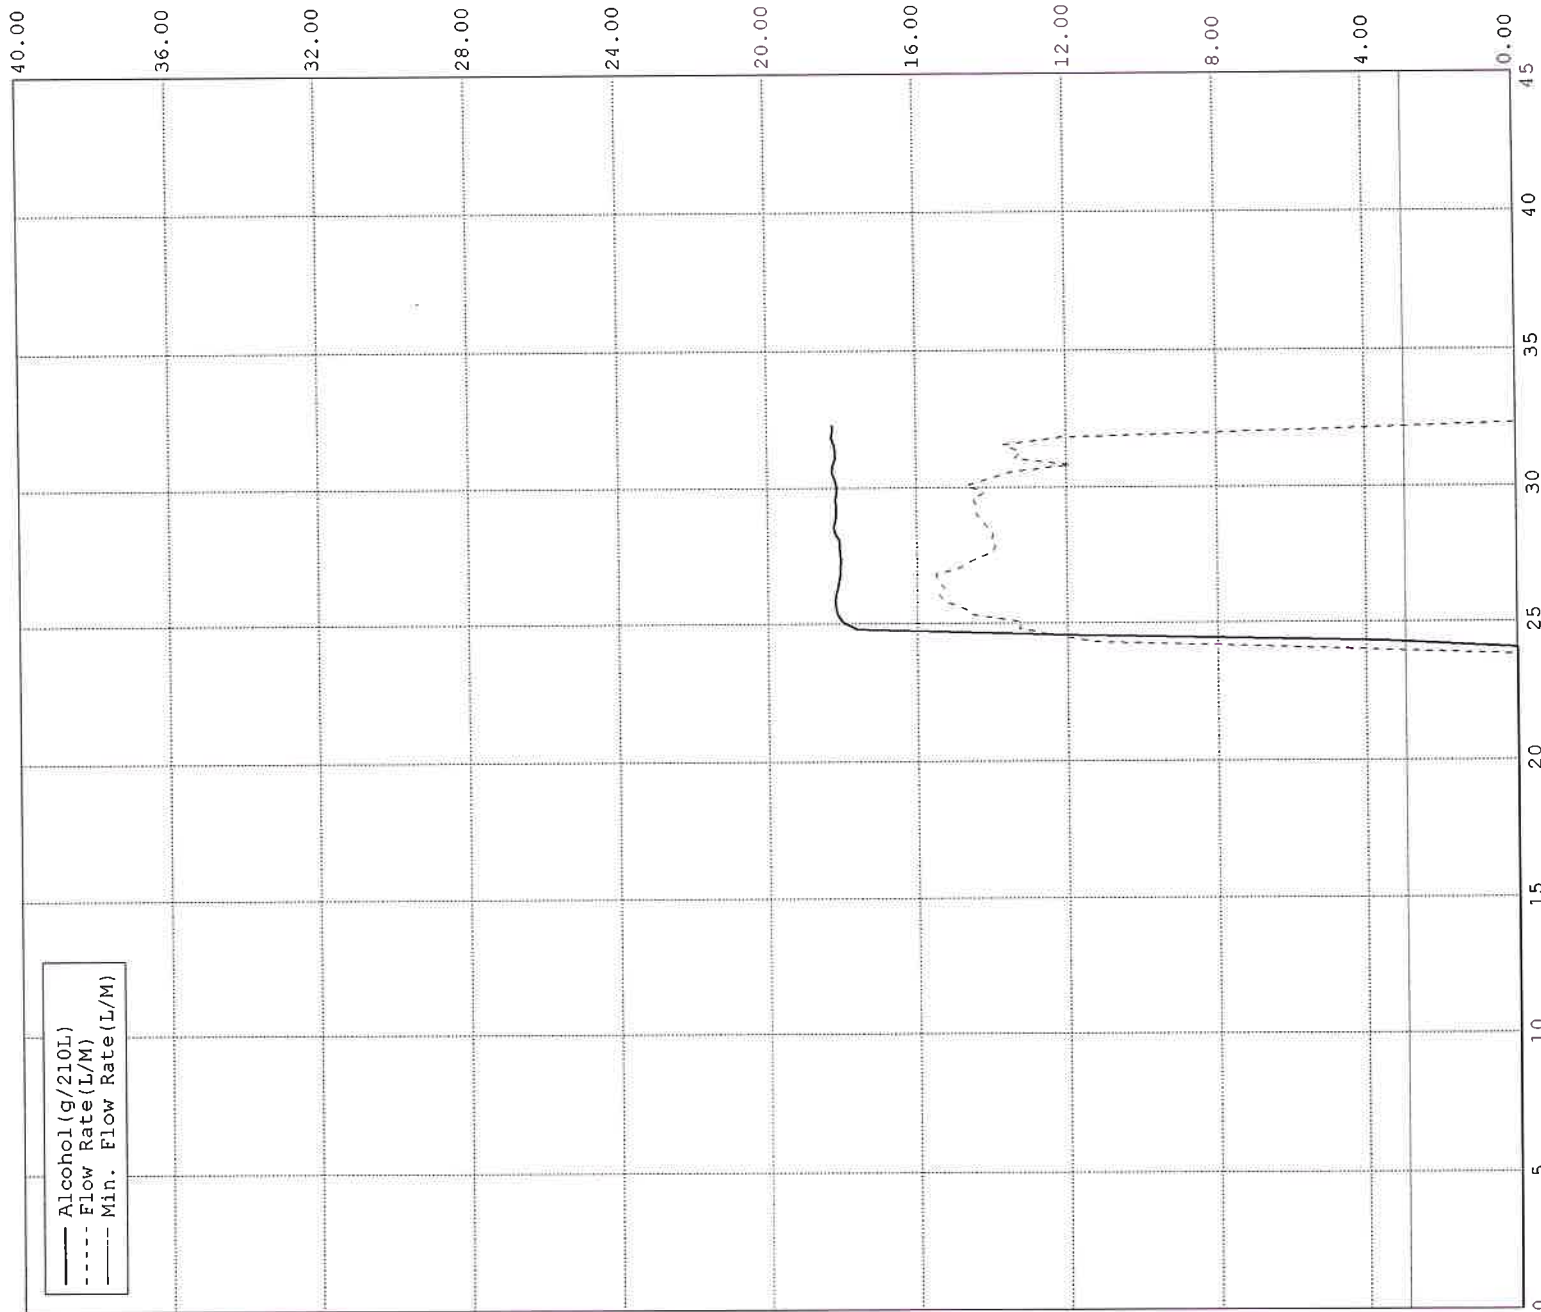

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100375

Date: 07/01/2025
Time: 15:02:54

SUBJECT NAME:
TEST TEST
LICENSE #: XXXX

OPERATOR NAME:
CARLIE GLAISTER
OPERATOR'S #: 10436

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	15:04
BLANK TEST	0.000	15:04
INTERNAL STANDARD	VERIFIED	15:04
EXTERNAL STANDARD	0.079	15:05
BLANK TEST	0.000	15:06
SUBJECT SAMPLE (Vol=1.59L)	0.000	15:06
BLANK TEST	0.000	15:07
EXTERNAL STANDARD	0.079	15:07
BLANK TEST	0.000	15:08

CKG

