




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100699

Report Issue Date: 06/23/2025
Date Received: 2024-10-07
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.018	0.021	0.020	0.020	0.020	0.020
0.080	0.079	AG310901	0.079	0.078	0.079	0.078	0.078	0.078
0.300	0.295	AG427706	0.294	0.293	0.291	0.291	0.291	0.292

As Found - Evaluation Analyst: Megan Carlock

As Found Conditions - Barometric Pressure (inHg): 29.48 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.7 Relative Humidity (%): 16

As-Found Lab Activity Date Range: 10/28/2024 - 10/29/2024

Changed O-ring. The first VOC ran had an Interference Detected status message.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.020	0.020	0.021	0.020	0.020	+/- 0.002
0.040	0.040	AG407908	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG335202	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.100	AG333401	0.100	0.100	0.101	0.101	0.100	0.100	+/- 0.004
0.150	0.150	AG332004	0.150	0.148	0.147	0.148	0.148	0.148	+/- 0.006
0.300	0.300	AG427706	0.300	0.298	0.298	0.299	0.299	0.299	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 30.00 Barometer Used: VWR S/N 240680771 Temperature (C): 23.9 Relative Humidity (%): 27

As-Left Lab Activity Date Range: 06/11/2025 - 06/12/2025

Blank error occurred twice during the minimum volume test. The tank was changed, and the test was completed.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock

Results authorized by Megan Carlock on 06/23/2025

megan.crouse@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 06/23/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100699 Analyst or Technician Name: Megan Carlock

DataMaster DMT Calibration Start Date: 6/11/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/2026
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

Blank error occurred twice, tank was changed and minimum volume test was completed.

As Left Linearity Testing

Barometric Pressure (in Hg) 30.00 Temperature(C) 23.9 Relative Humidity(%) 27

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - Print with View Details
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

- Acetone Reagent Lot Number: 2025060315 Expiration Date: 7/27/25
Simulator S/N: SD1200 Thermometer Verification Performed? ☒
- Isopropanol Reagent Lot Number: 2025060315 Expiration Date: 9/3/25
Simulator S/N: SD1198 Thermometer Verification Performed? ☒
- Negative (Ethanol Only) Lot Number: 23IP41233 Expiration Date: 9/20/25
Simulator S/N: SD1199 Thermometer Verification Performed? ☒

MNC 6/23/25

9/3/25

sim exp: 9/10/25

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/2025

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/11/25

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 6/12/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100699

Date: 06/11/2025
 Time: 08:30:29

VERSIONS
 DMT: 3.02
 PIC: 3.03
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 44.2°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.53 V	PASSED
(0.94 V - 2.18 V)	
Cooler Voltage = 1.54 V	PASSED
(0.91 V - 2.11 V)	
Bias Voltage = 80 V	PASSED
(48 V - 112 V)	
Chopper Freq = 531 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 30.0 in	

PUMP INFO

Flow Rate = 4.183 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.004 V <= 0.010 V)	
PUMP OFF	PASSED
(0.001 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.079 0.00%	PASSED
(0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100699

Date: 06/11/2025

Time: 9:59 AM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 44.3°C

Current Barometer 30.0 in

Volume (Ltr) 1.52

Settings

Lamp: 1.53 V

Bias: 80 V

Cooler: 1.56 V

Chopper: 531 Hz

Voltages (V)

Flow: 1.05 V

Detector: -0.010 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 11/06/2024
Time: 14:08:01

OPERATOR NAME:
KAIJA SWISHER
CERTIFICATE #: 10746

Ca = 0.1000
CAL = 0.982224 0.800 <= CAL < 1.200
b1 = 0.0008 0.0000 <= b1 < 0.0040
b2 = 0.0052 0.0010 <= b2 < 0.0100
b3 = 0.0005 0.0000 <= b3 < 0.0040
Xq = 0.0787 0.0500 <= Xq < 0.2000
a21 = 1.175117 1.050 <= a21 < 1.300
a31 = 0.408176 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 06/11/2025
Time: 10:40:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.99: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:42
BLANK TEST	0.000	10:42
INTERNAL STANDARD	VERIFIED	10:42
EXTERNAL STANDARD	0.079	10:42
BLANK TEST	0.000	10:43
SUBJECT SAMPLE (Vol=1.59L)	XXX	10:44

Blank Error

MNC

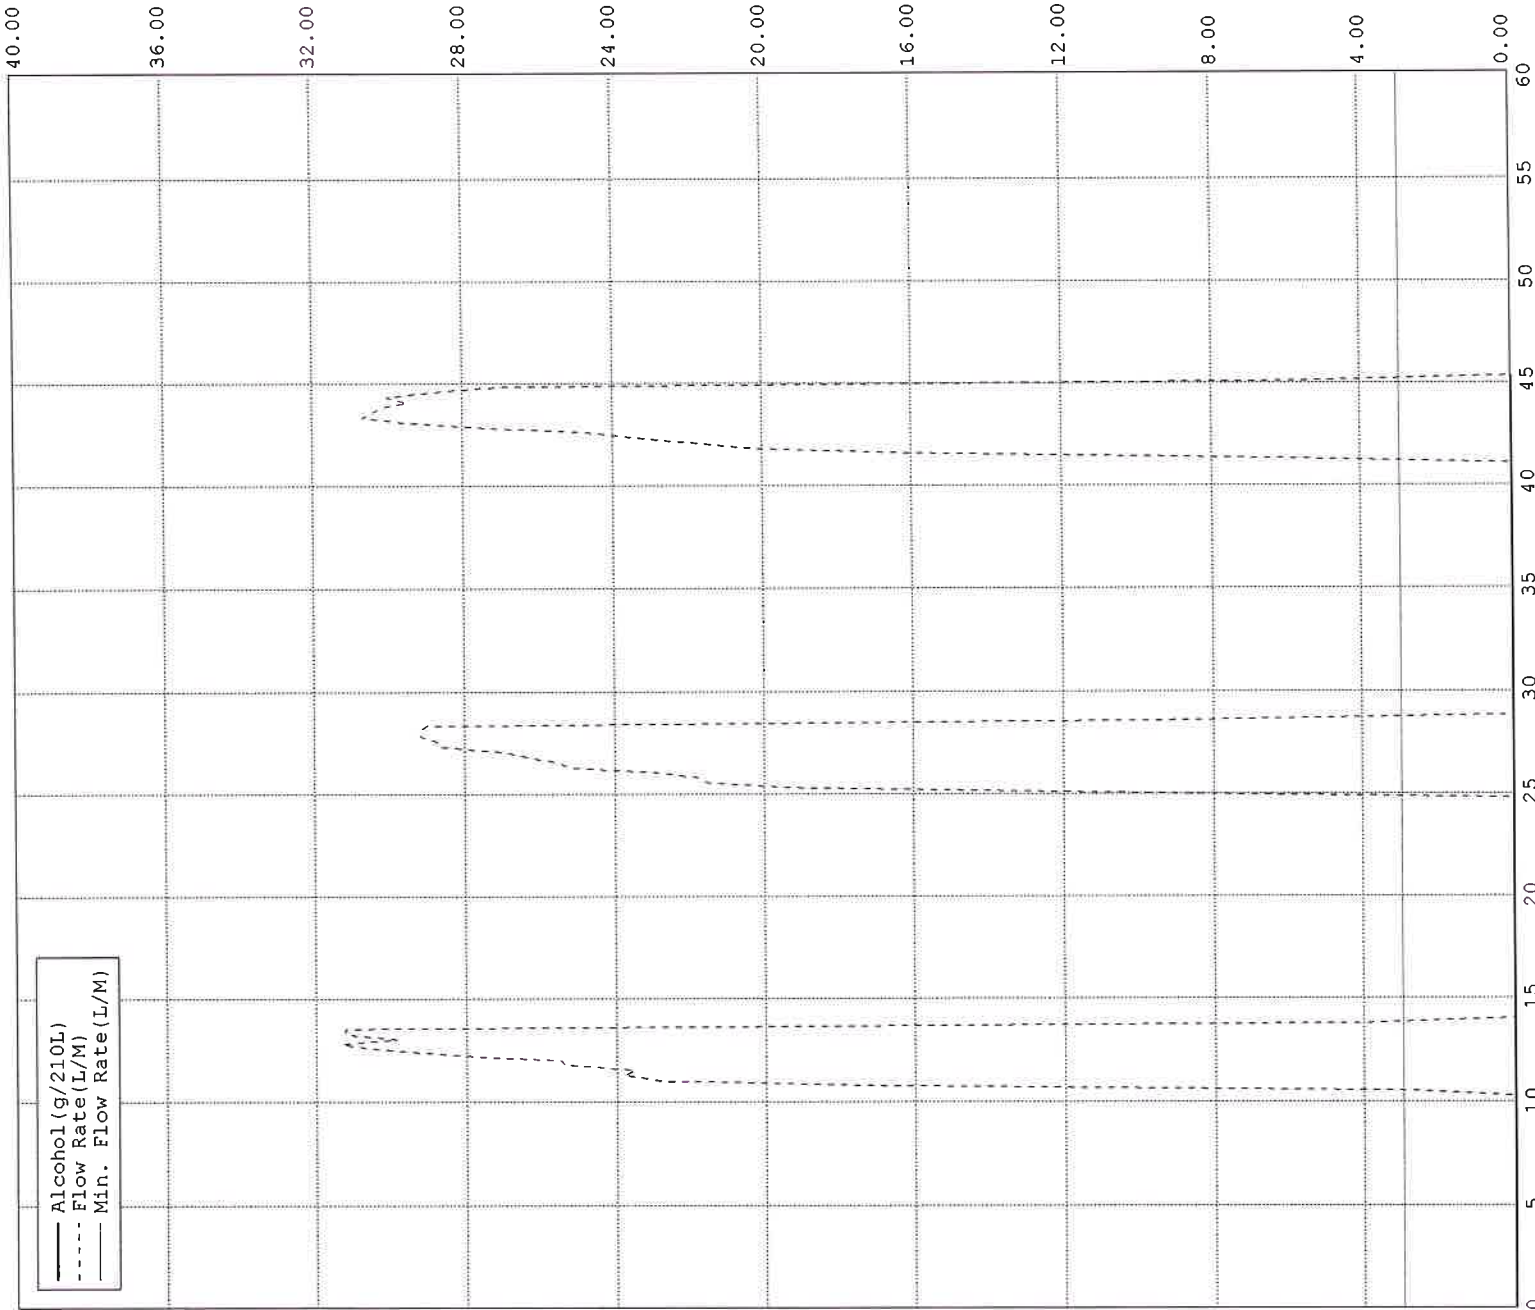

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100699

Date: 06/11/2025

Time: 10:51:57

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.98: 0.080


LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:52
BLANK TEST	0.000	10:53
INTERNAL STANDARD	VERIFIED	10:53
EXTERNAL STANDARD	0.080	10:53
BLANK TEST	0.000	10:54
SUBJECT SAMPLE (Vol=1.67L)	XXX	10:55

Blank Error

MNC

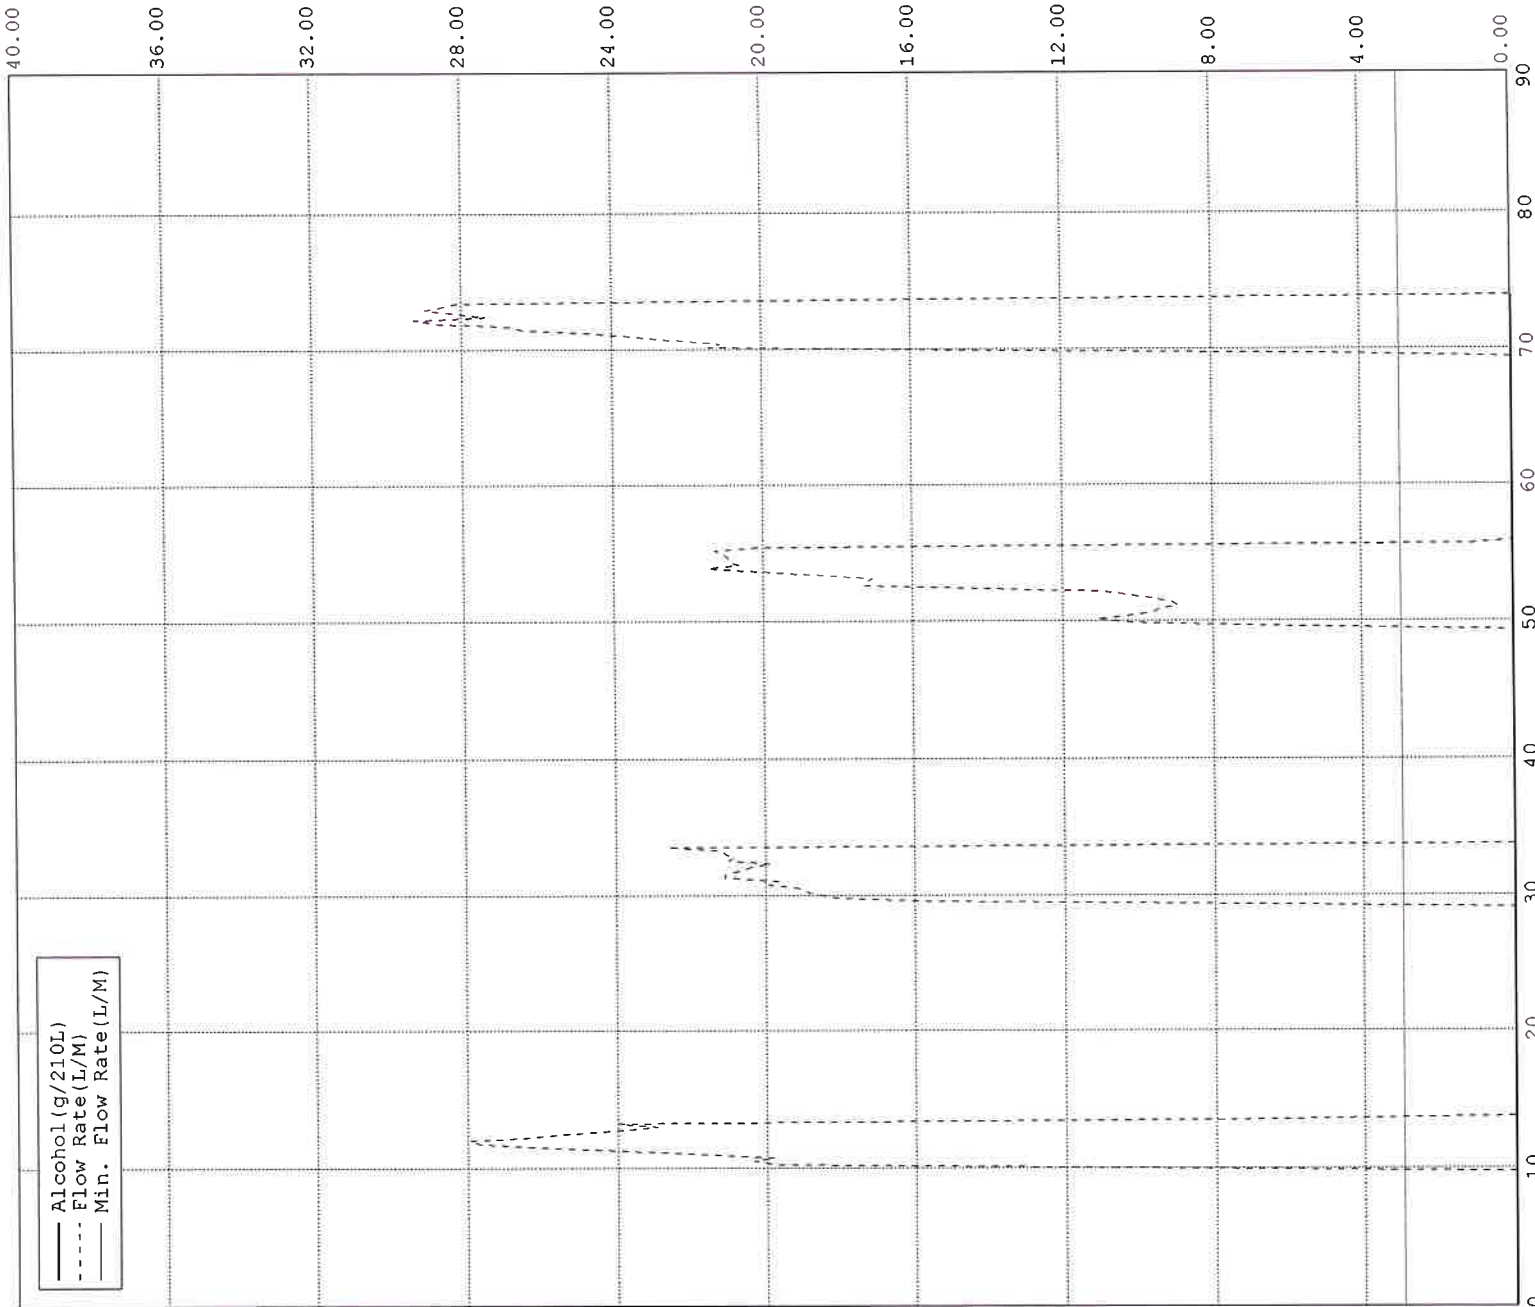

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 06/11/2025
Time: 10:59:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:00
BLANK TEST	0.000	11:00
INTERNAL STANDARD	VERIFIED	11:01
EXTERNAL STANDARD	0.082	11:01
BLANK TEST	0.000	11:02
SUBJECT SAMPLE (Vol=1.53L)	0.000	11:03
BLANK TEST	0.000	11:04
EXTERNAL STANDARD	0.080	11:04
BLANK TEST	0.000	11:05

MNC

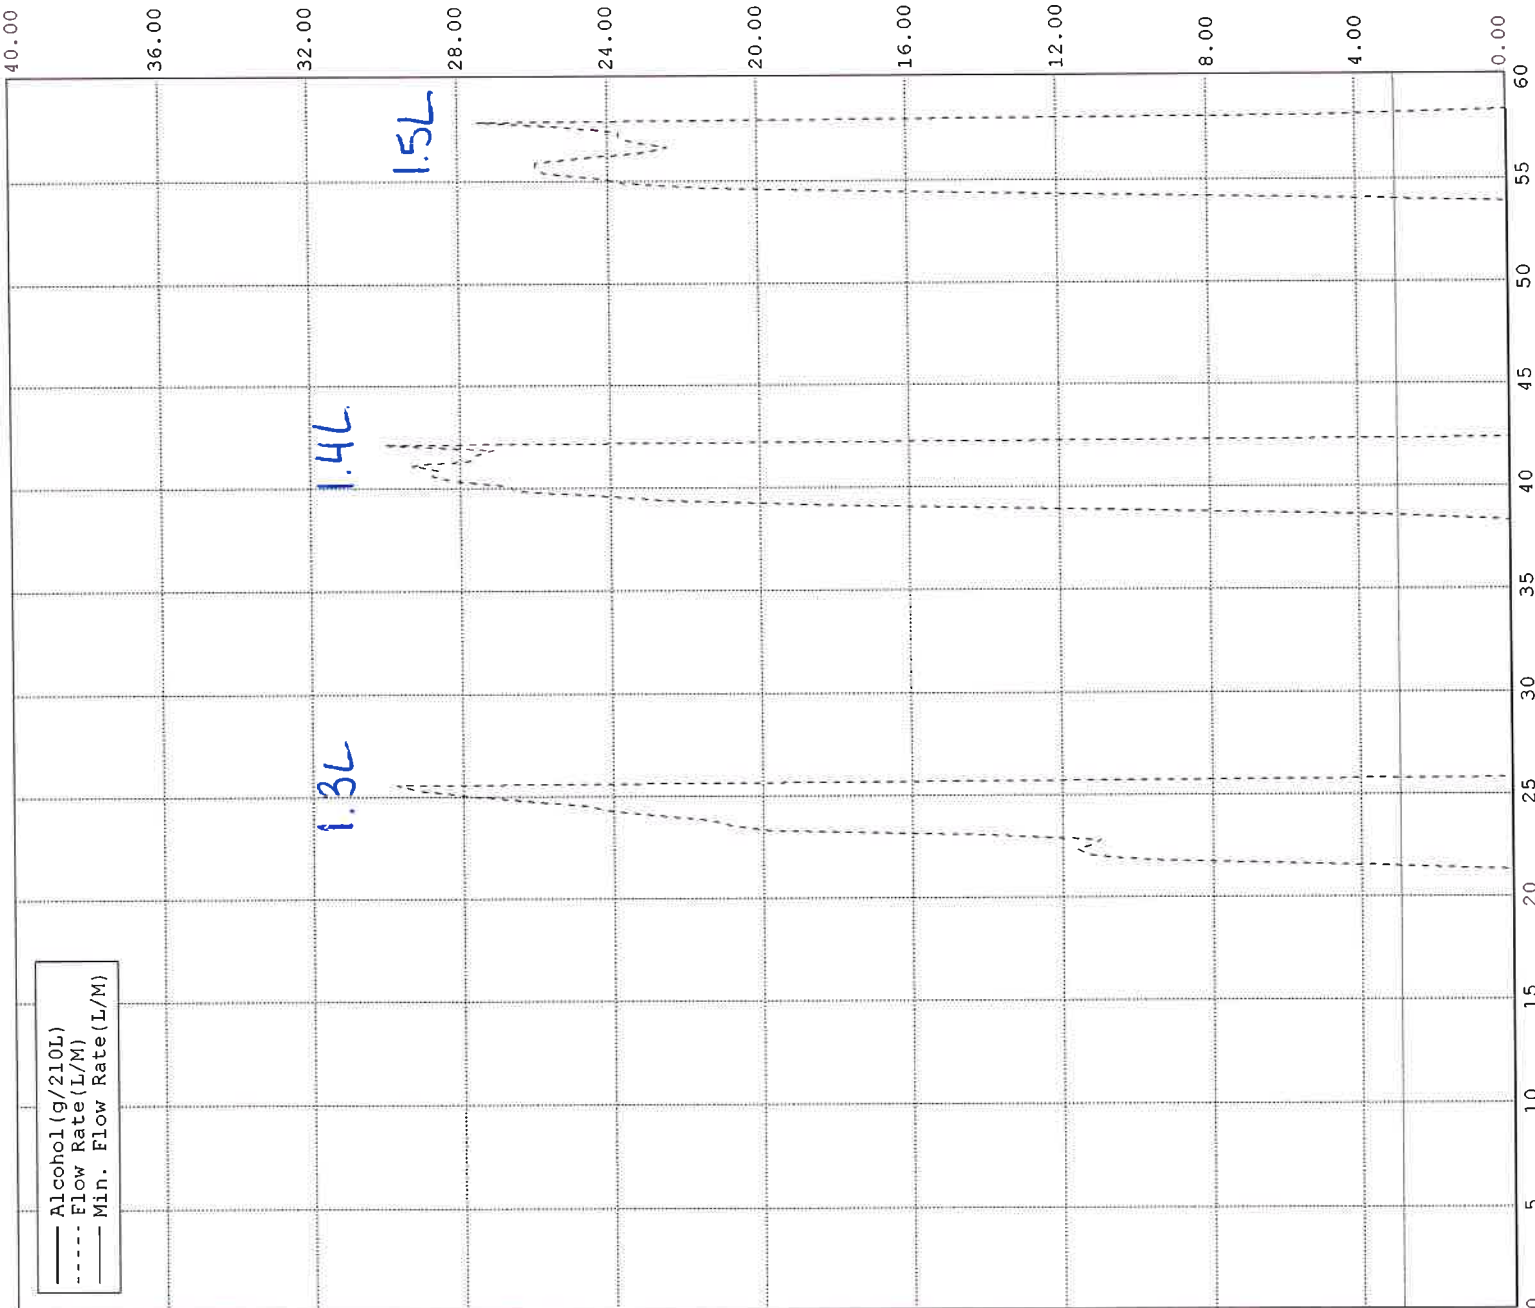

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100699

Date: 06/11/2025
 Time: 11:09:49

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0204	0.0005
0.040	0.0400	0.0000
0.080	0.0790	0.0000
0.100	0.1004	0.0005
0.150	0.1482	0.0011
0.300	0.2988	0.0008

SLOPE = 0.994297
 R² = 0.999949

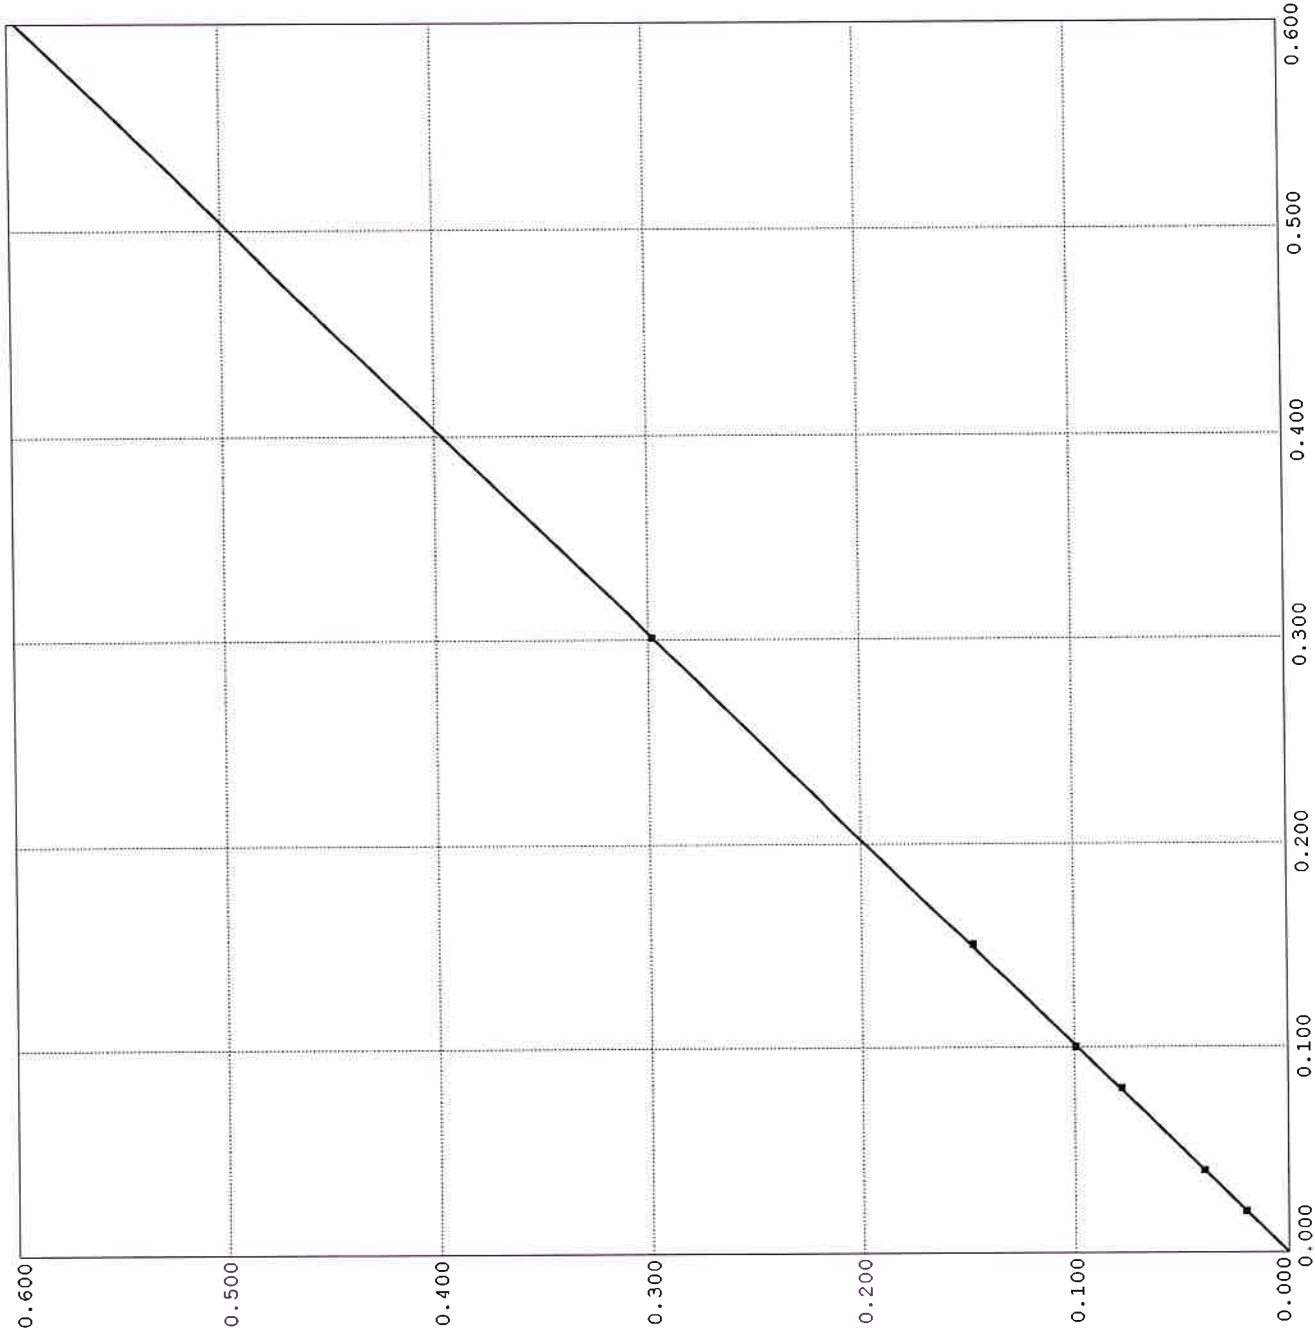

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 06/11/2025
Time: 11:09:51

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.97: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 1132 psi

BLANK TEST	0.000	11:11
INTERNAL STANDARD	VERIFIED	11:11
EXTERNAL STANDARD	0.021	11:11
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.020	11:12
BLANK TEST	0.000	11:13
EXTERNAL STANDARD	0.020	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.021	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.020	11:15
BLANK TEST	0.000	11:16

Average = 0.0204
Std Dev = 0.0005

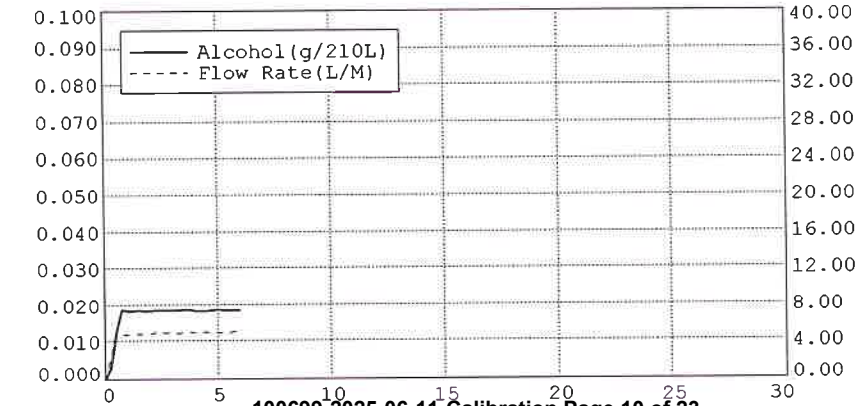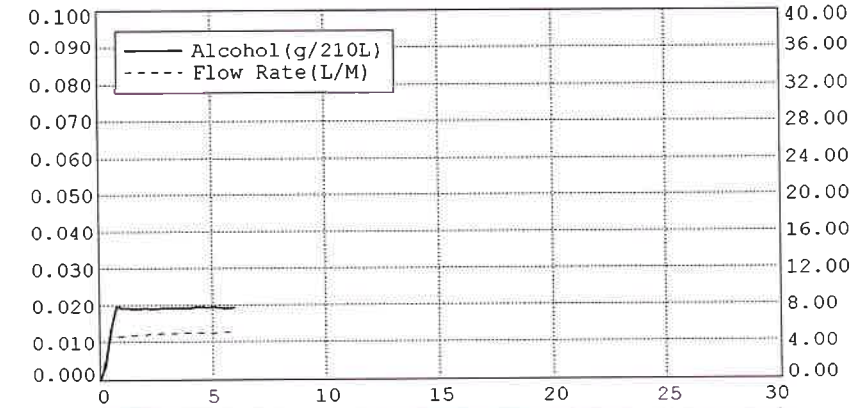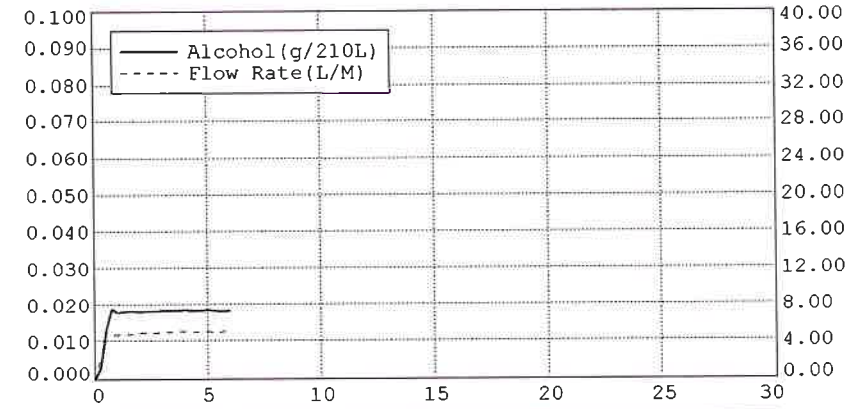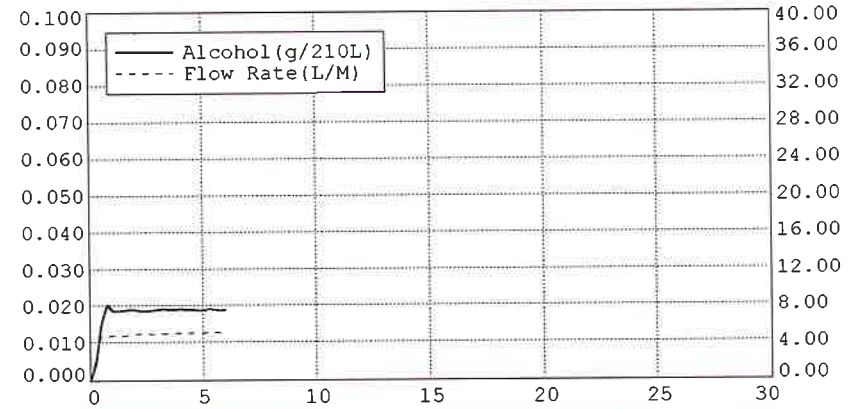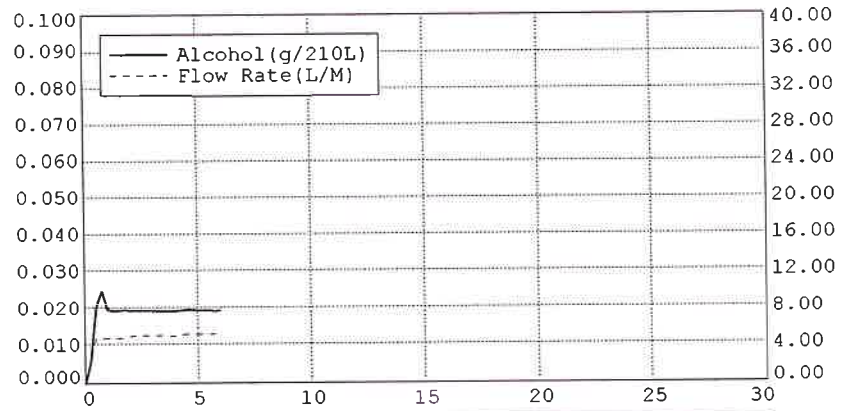

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 06/11/2025
Time: 11:17:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.97: 0.040
LOT #: ~~AG704908~~ AG407908 MJC 6/12/25
EXPIRATION: 03/19/2026
TANK PRESSURE: 1064 psi

TEST TYPE	VALUE	TIME
BLANK TEST	0.000	11:19
INTERNAL STANDARD	VERIFIED	11:19
EXTERNAL STANDARD	0.040	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.040	11:20
BLANK TEST	0.000	11:21
EXTERNAL STANDARD	0.040	11:21
BLANK TEST	0.000	11:22
EXTERNAL STANDARD	0.040	11:22
BLANK TEST	0.000	11:23
EXTERNAL STANDARD	0.040	11:24
BLANK TEST	0.000	11:25

Average = 0.0400
Std Dev = 0.0000

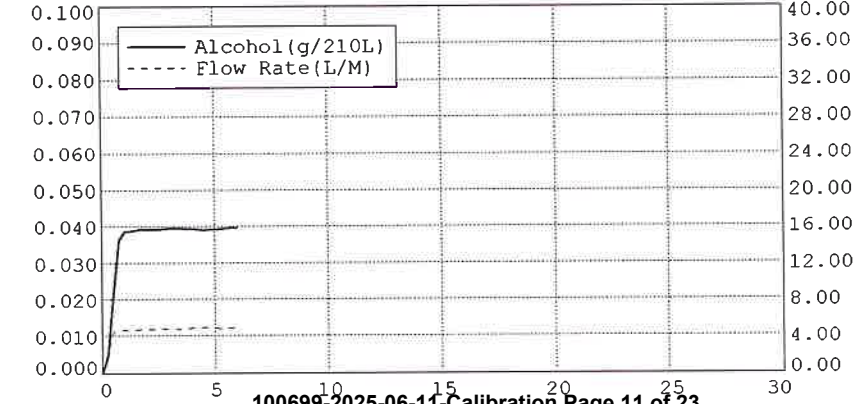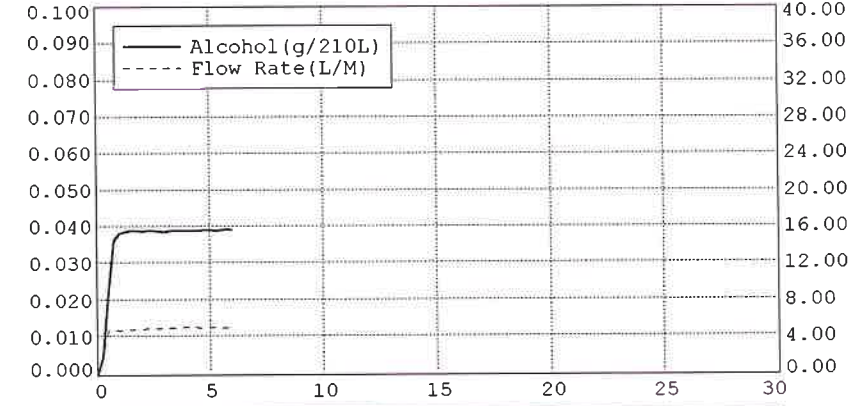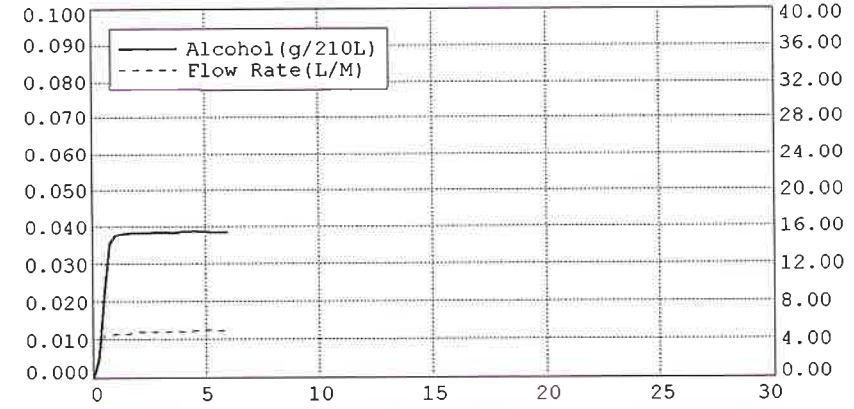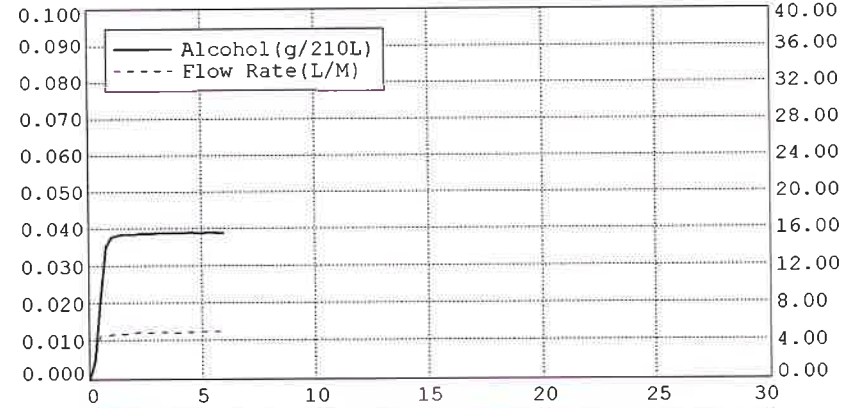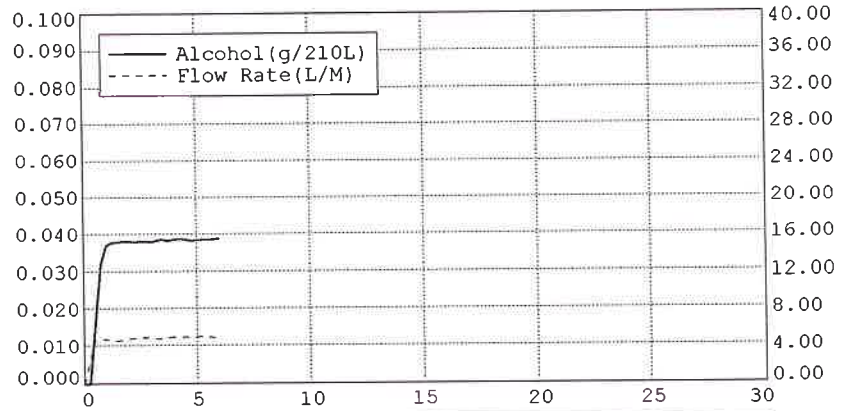

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 06/11/2025
Time: 11:26:41

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 792 psi

BLANK TEST	0.000	11:27
INTERNAL STANDARD	VERIFIED	11:27
EXTERNAL STANDARD	0.079	11:28
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.079	11:29
BLANK TEST	0.000	11:30
EXTERNAL STANDARD	0.079	11:30
BLANK TEST	0.000	11:31
EXTERNAL STANDARD	0.079	11:31
BLANK TEST	0.000	11:32
EXTERNAL STANDARD	0.079	11:32
BLANK TEST	0.000	11:33

Average = 0.0790
Std Dev = 0.0000

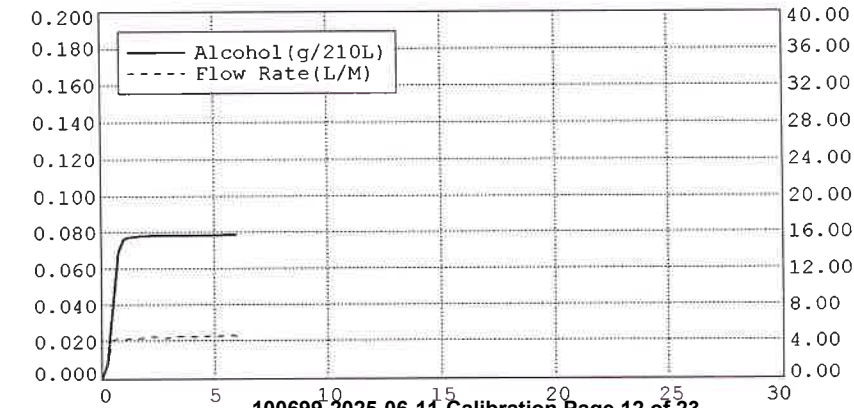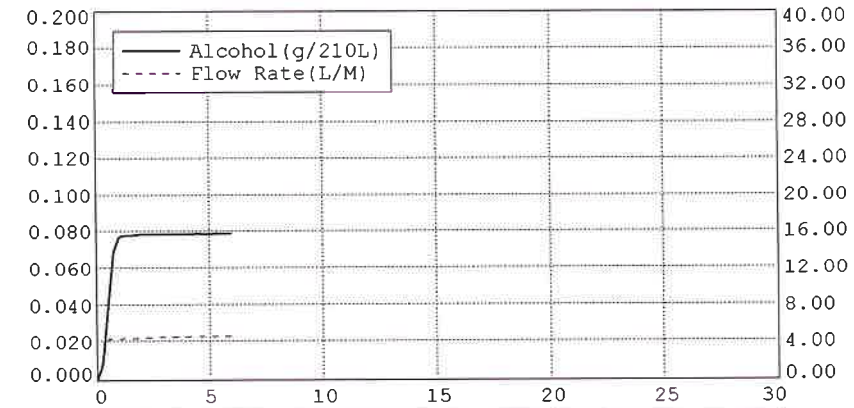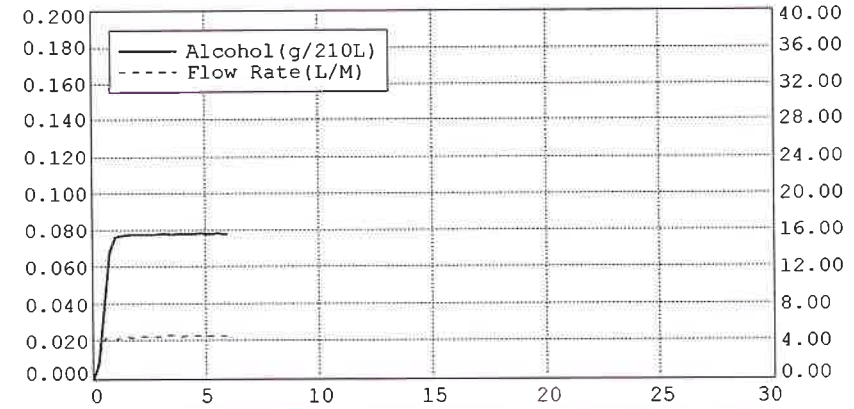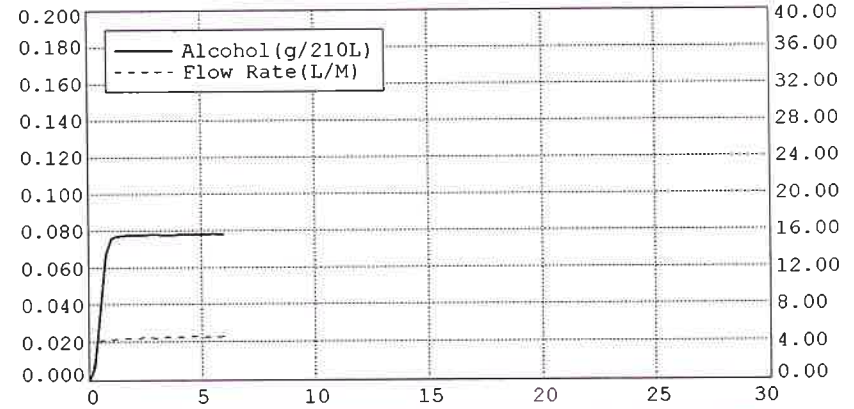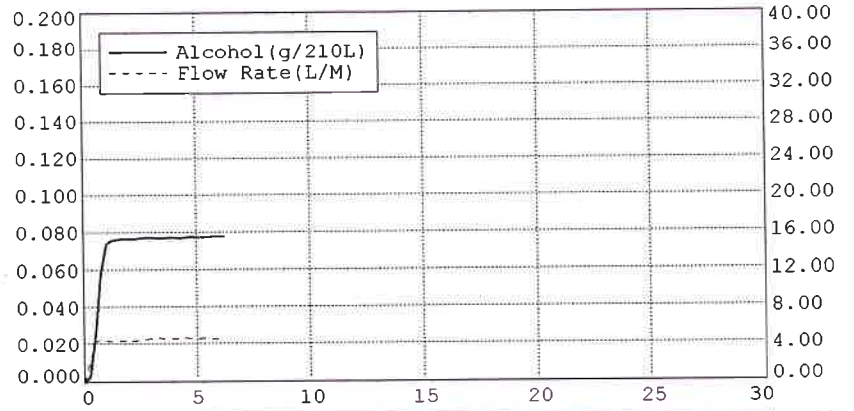

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 06/11/2025
Time: 11:34:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.97: 0.100
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 997 psi

BLANK TEST	0.000	11:36
INTERNAL STANDARD	VERIFIED	11:36
EXTERNAL STANDARD	0.100	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.100	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.101	11:38
BLANK TEST	0.000	11:39
EXTERNAL STANDARD	0.101	11:40
BLANK TEST	0.000	11:40
EXTERNAL STANDARD	0.100	11:41
BLANK TEST	0.000	11:42

Average = 0.1004
Std Dev = 0.0005

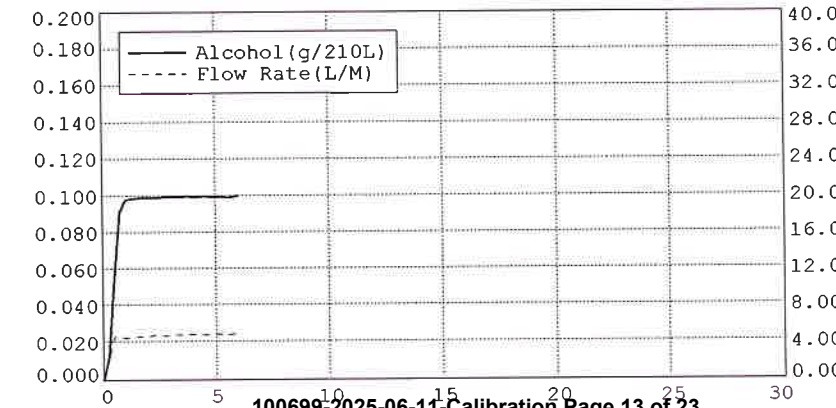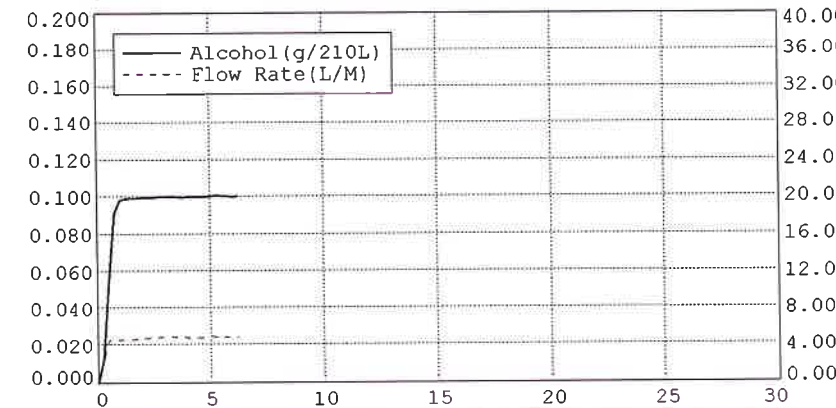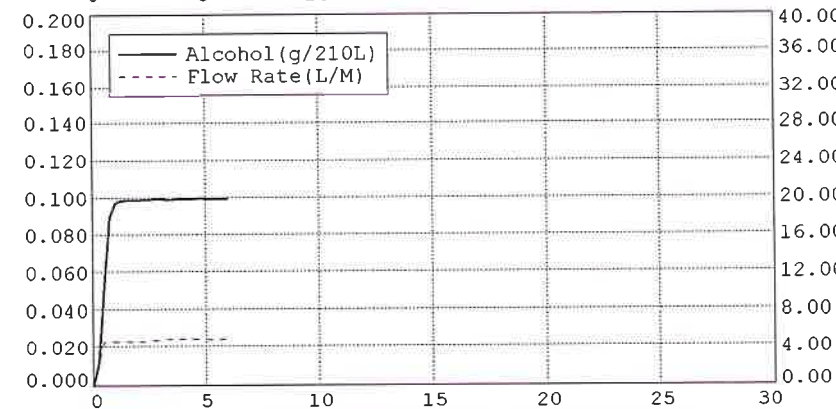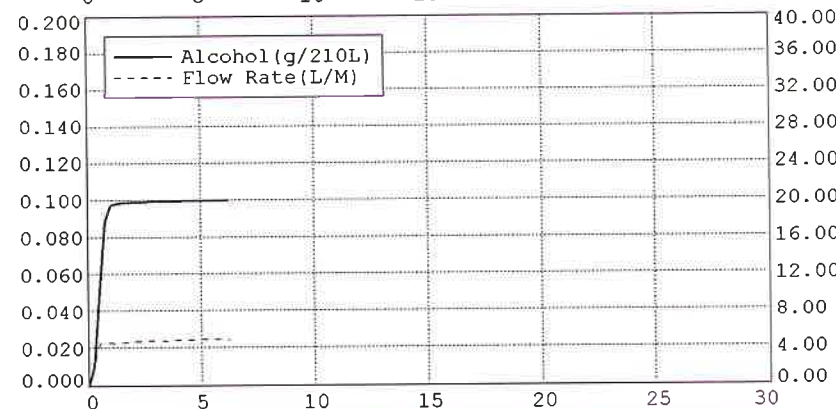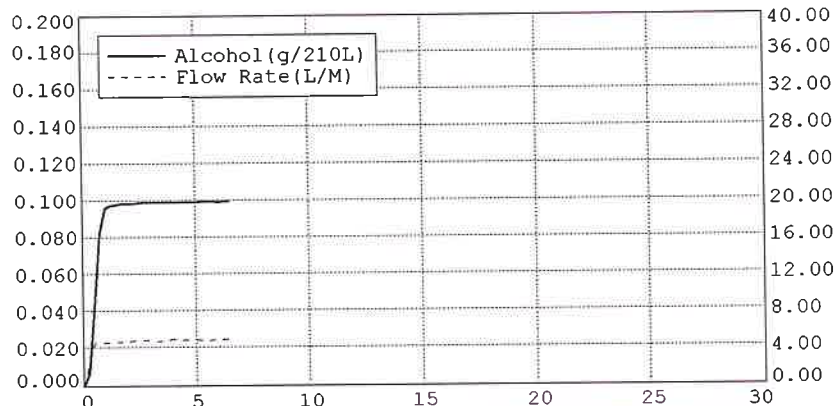

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 06/11/2025
Time: 11:43:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.97: 0.150
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 232 psi

BLANK TEST	0.000	11:44
INTERNAL STANDARD	VERIFIED	11:44
EXTERNAL STANDARD	0.150	11:44
BLANK TEST	0.000	11:46
EXTERNAL STANDARD	0.148	11:46
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.147	11:47
BLANK TEST	0.000	11:48
EXTERNAL STANDARD	0.148	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.148	11:49
BLANK TEST	0.000	11:51

Average = 0.1482
Std Dev = 0.0011

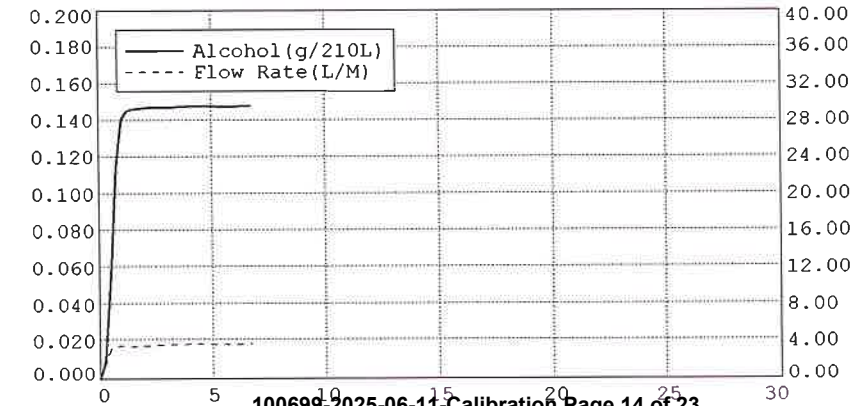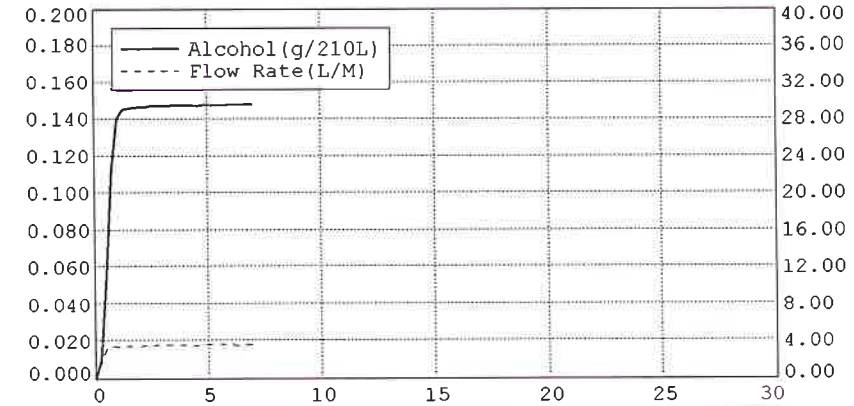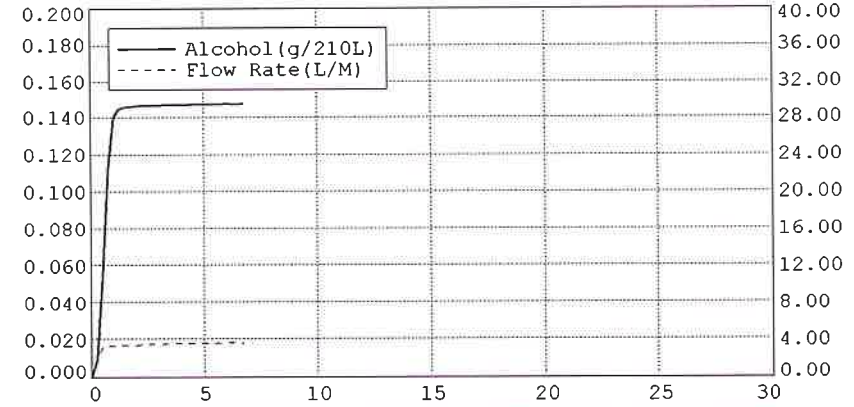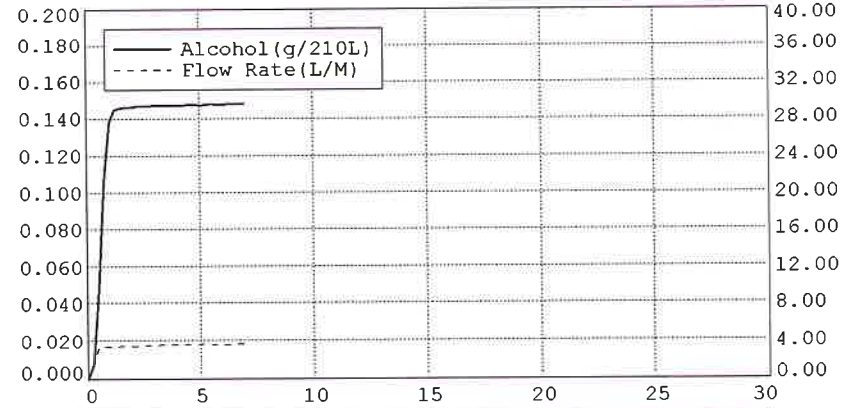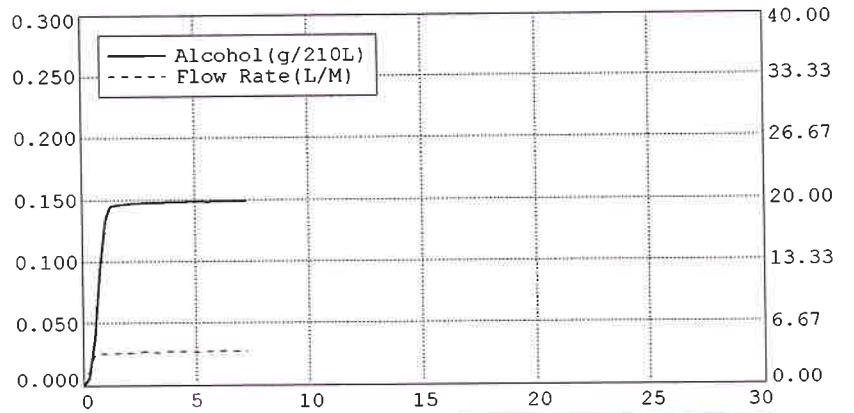

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100699






Date: 06/11/2025
Time: 11:55:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.97: 0.300
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 247 psi

BLANK TEST	0.000	11:57
INTERNAL STANDARD	VERIFIED	11:57
EXTERNAL STANDARD	0.300	11:57
BLANK TEST	0.000	11:58
EXTERNAL STANDARD	0.298	11:58
BLANK TEST	0.000	11:59
EXTERNAL STANDARD	0.298	11:59
BLANK TEST	0.000	12:00
EXTERNAL STANDARD	0.299	12:00
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.299	12:02
BLANK TEST	0.000	12:03

Average = 0.2988
Std Dev = 0.0008

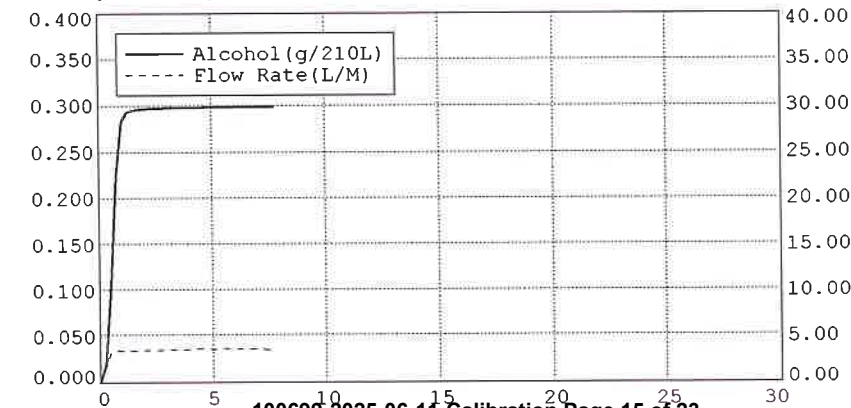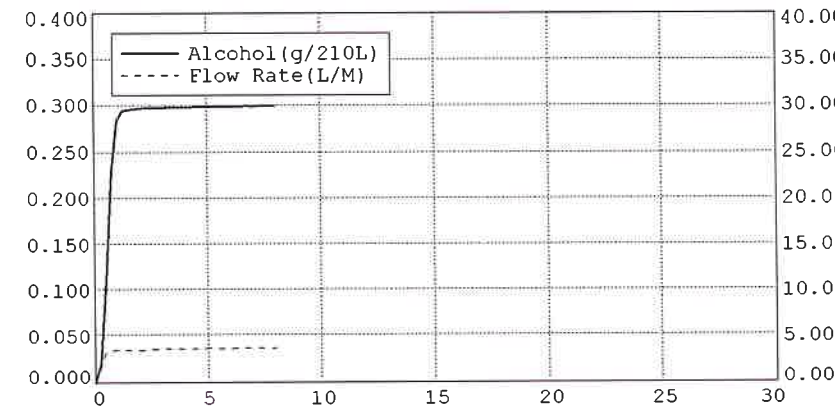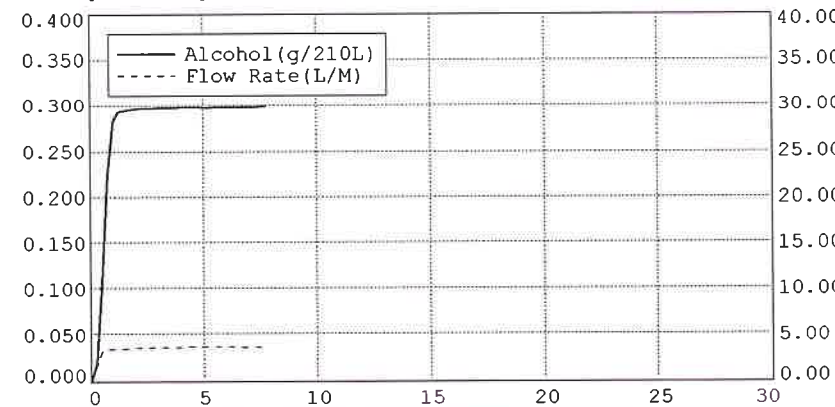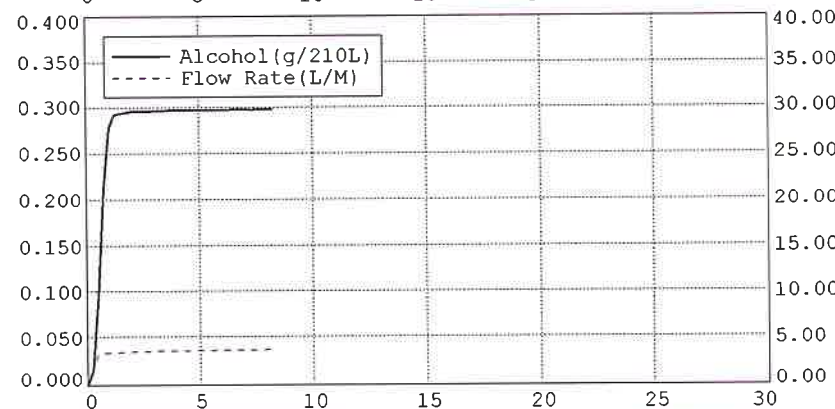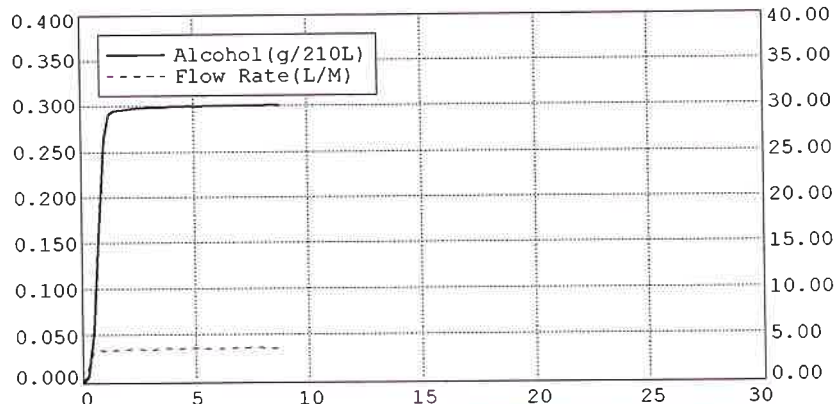

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100699

Date: 06/11/2025

Time: 12:12:50

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INCOMPLETE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.97: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED

0.000

VERIFIED

0.082

0.000

INCOMPLETE

12:13

12:13


12:14

12:14

12:15

12:17

MNC

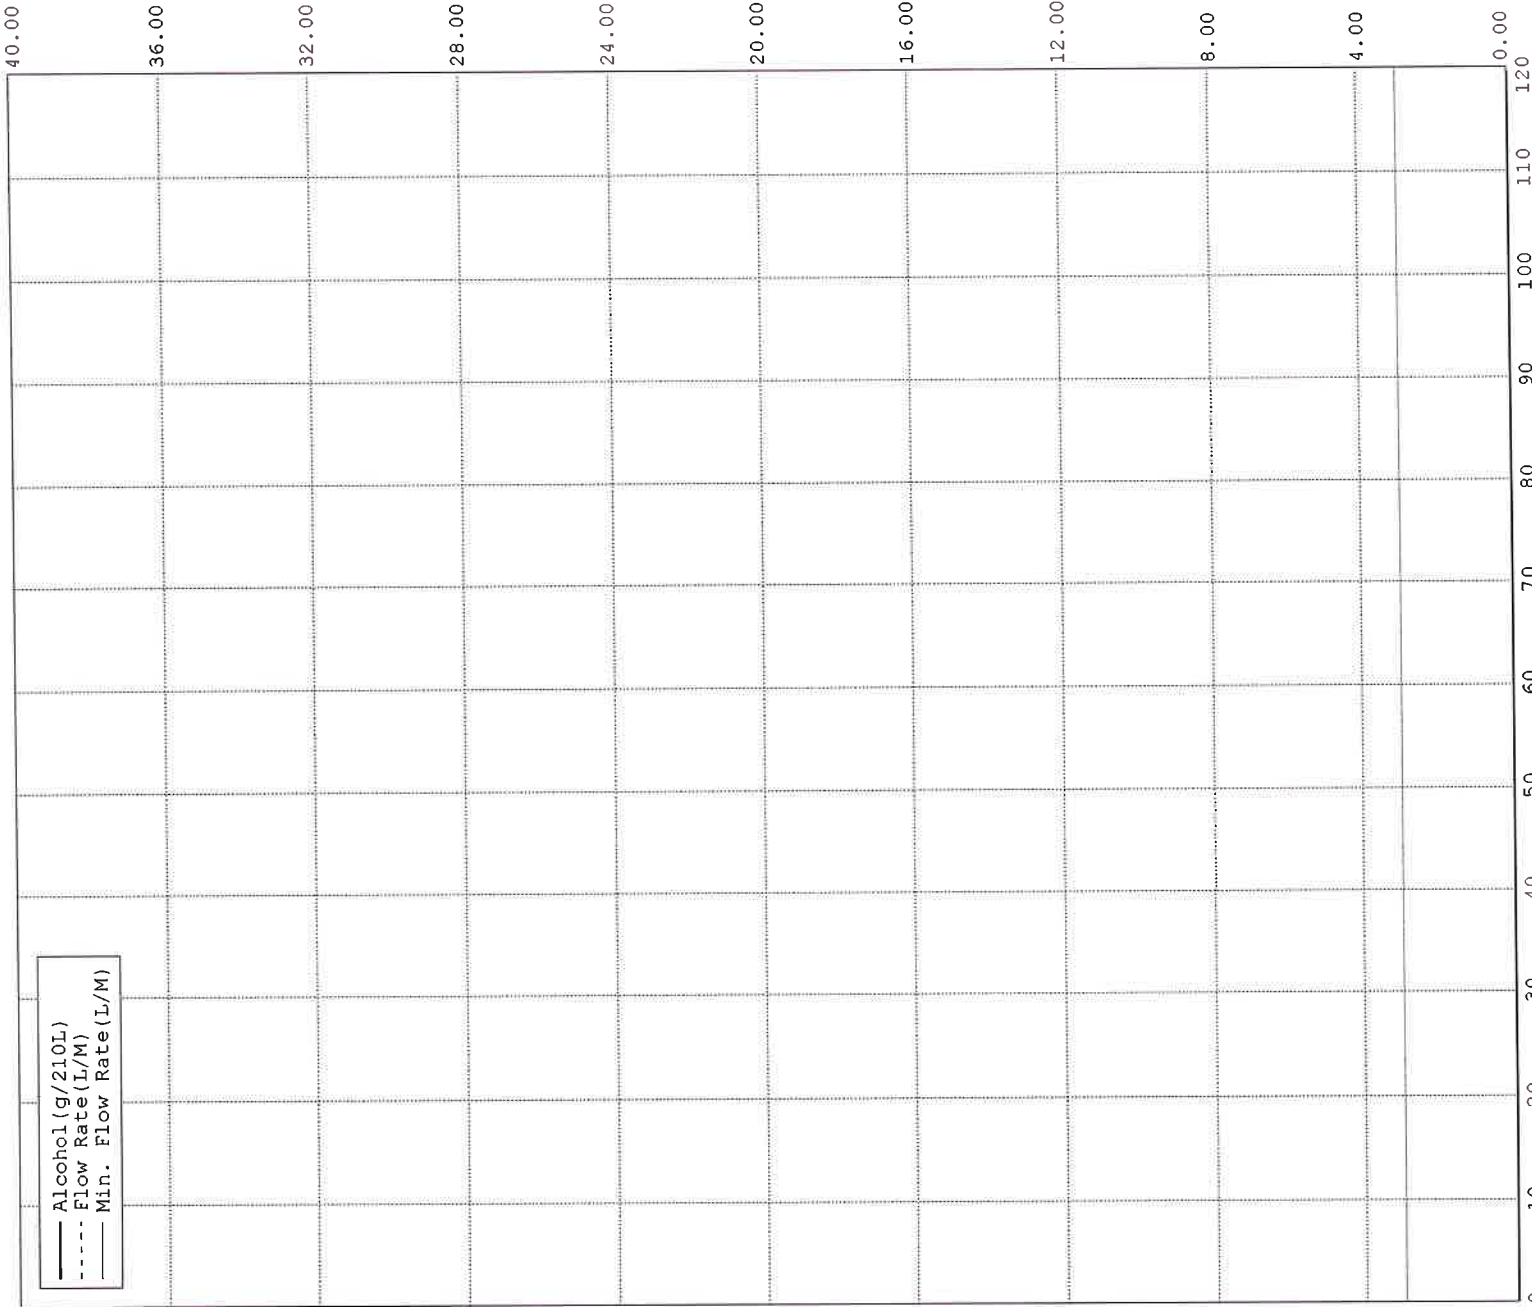

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100699

Date: 06/11/2025

Time: 14:15:11

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

MAXIMUM ATTEMPTS EXCEEDED

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.95: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 14:16

0.000 14:16

VERIFIED 14:16


0.079 14:16

0.000 14:17

XXX 14:18

Maximum Attempts Exceeded

MNC

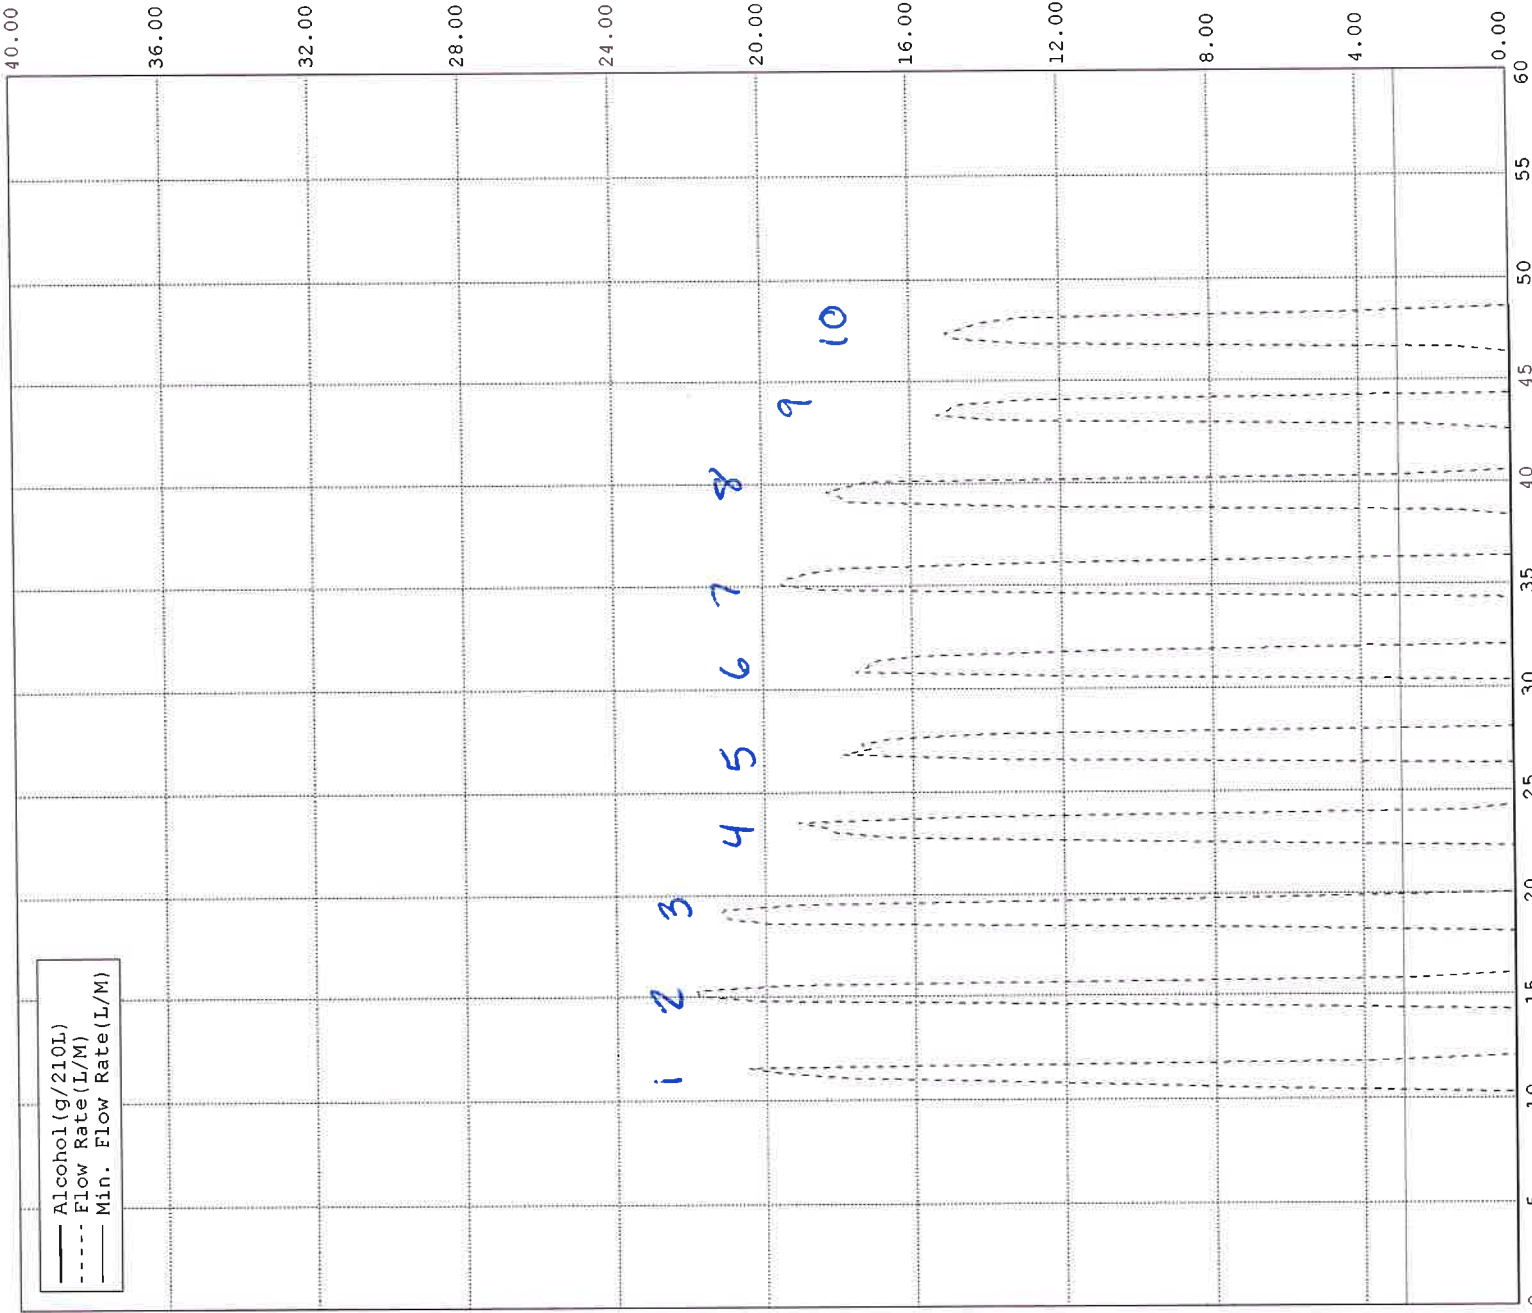

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 06/11/2025
Time: 14:20:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.96: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:23
BLANK TEST	0.000	14:23
INTERNAL STANDARD	VERIFIED	14:24
EXTERNAL STANDARD	0.081	14:24
BLANK TEST	0.000	14:25
SUBJECT SAMPLE	INVALID	14:25

MNC

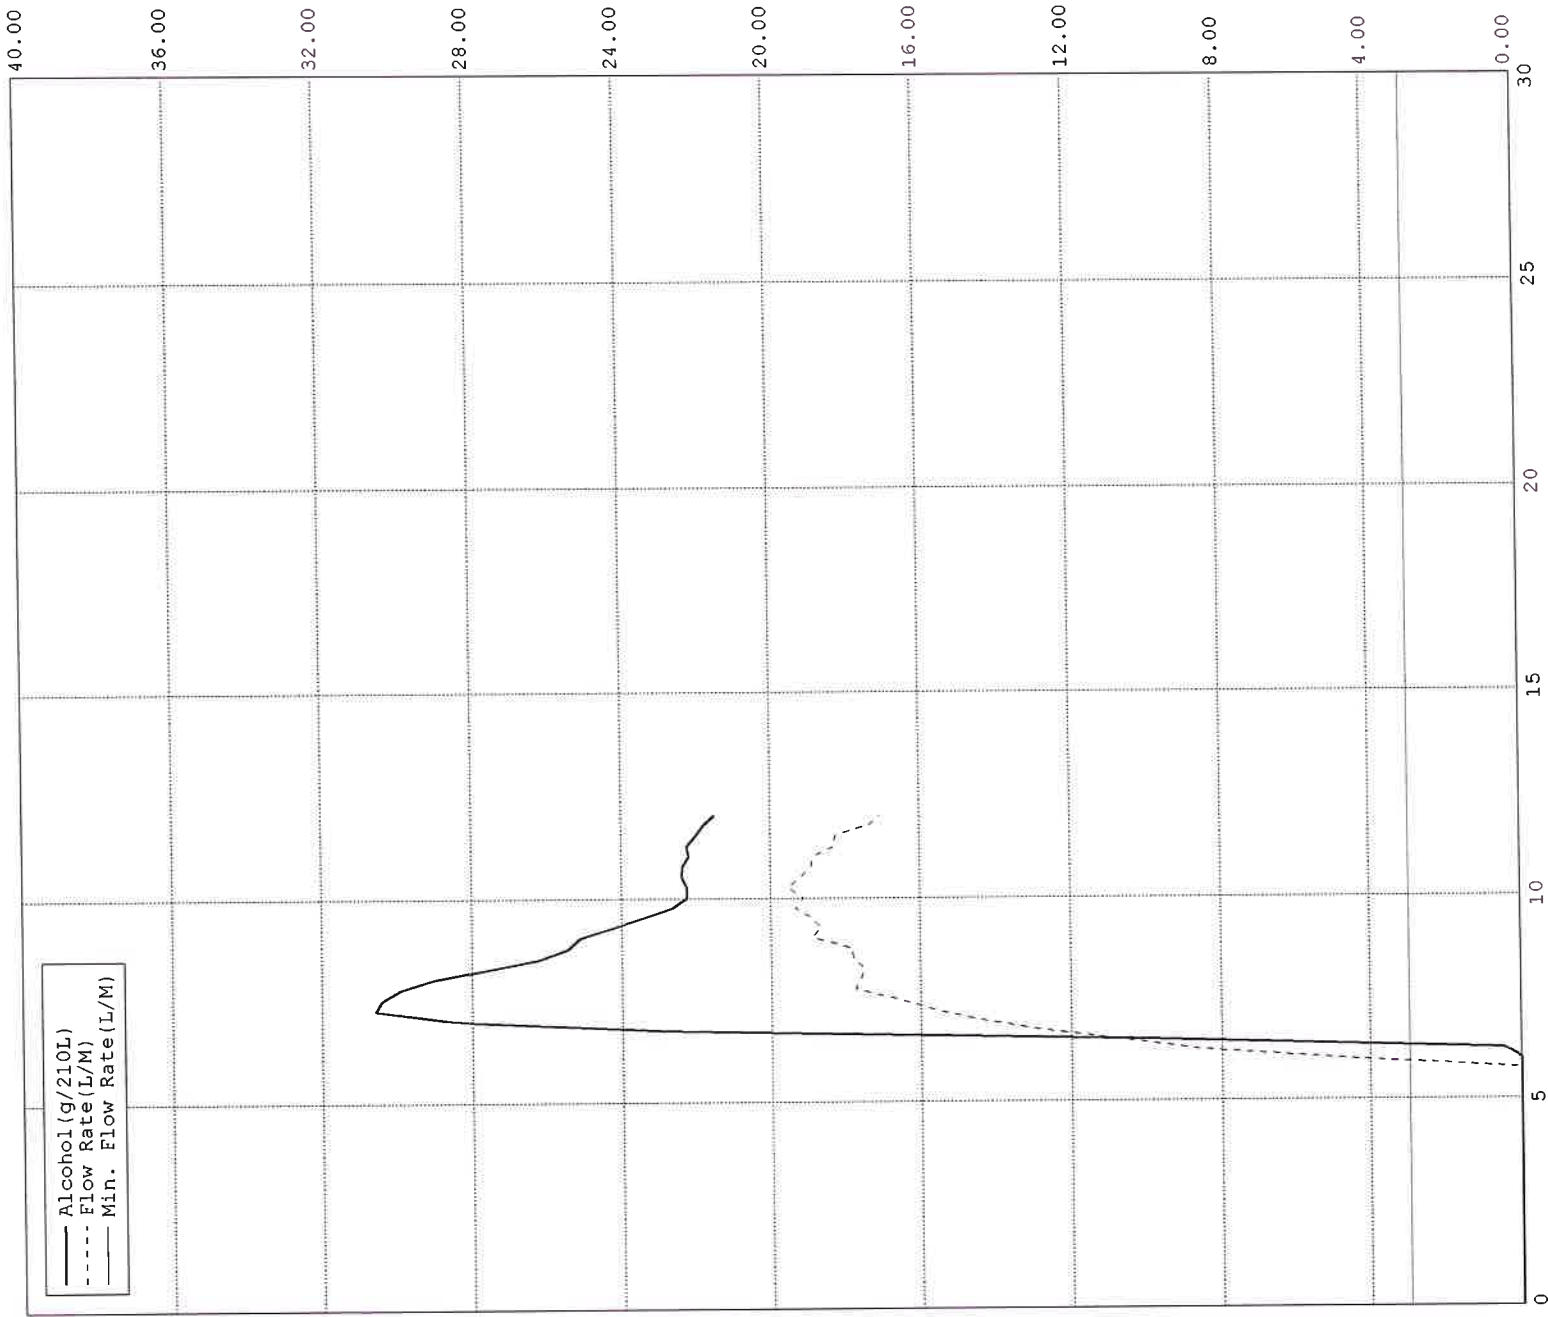

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 06/11/2025
Time: 12:07:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.97: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:08
BLANK TEST	0.000	12:08
INTERNAL STANDARD	VERIFIED	12:08
EXTERNAL STANDARD	0.081	12:08
BLANK TEST	0.000	12:09

RFI DETECTED

MNC

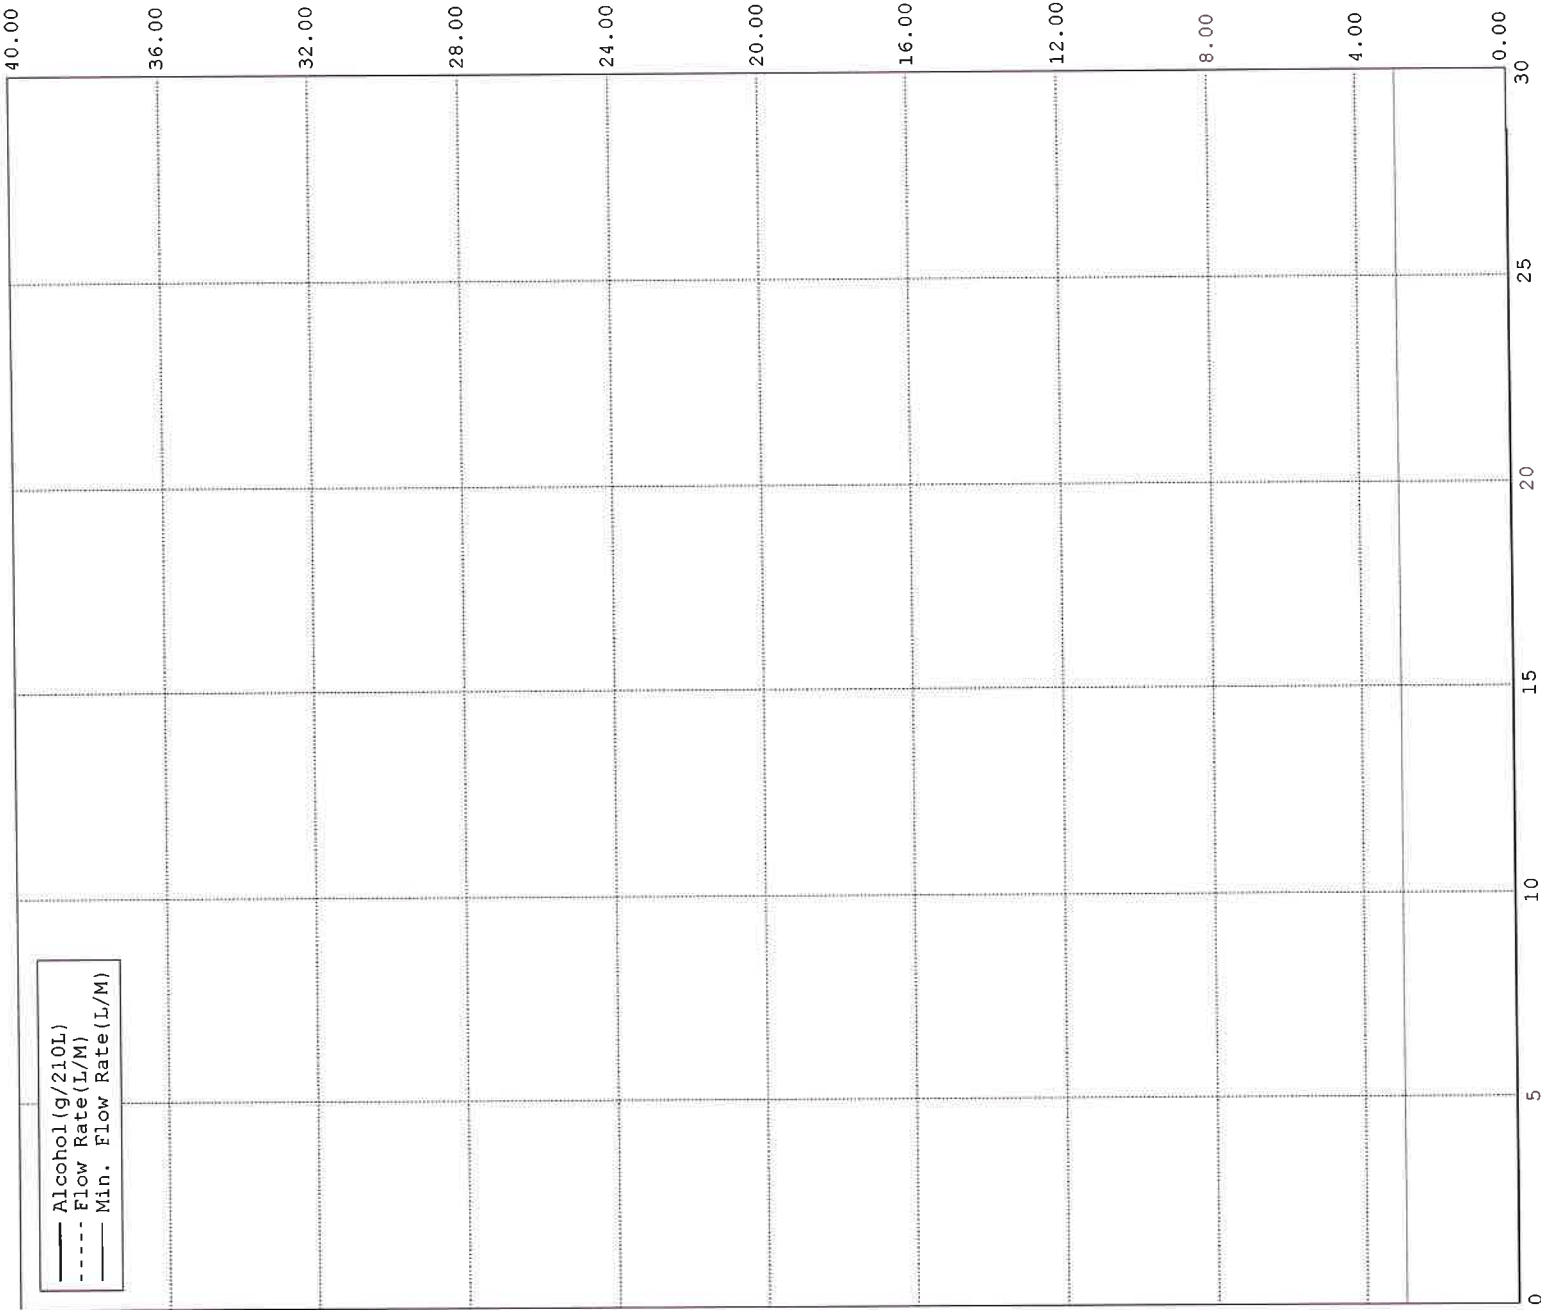

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100699

Date: 06/11/2025
 Time: 14:39:14

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:
 INTERFERENCE - ACETONE
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.95: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:40
BLANK TEST	0.000	14:40
INTERNAL STANDARD	VERIFIED	14:40
Xq = 0.079 (0.11%)		
EXTERNAL STANDARD	0.081	14:41
X[1] = 0.0806 (0.0023) (0.0014)		
BLANK TEST	0.000	14:42
SUBJECT SAMPLE	XXX	14:42
X[1] = 0.1107 (-0.0141) (0.0003)		


Interference Detected

Filter 2 Average: 0.0013

Filter 3 Average: 0.0008

MNC 6/12/25

MNC

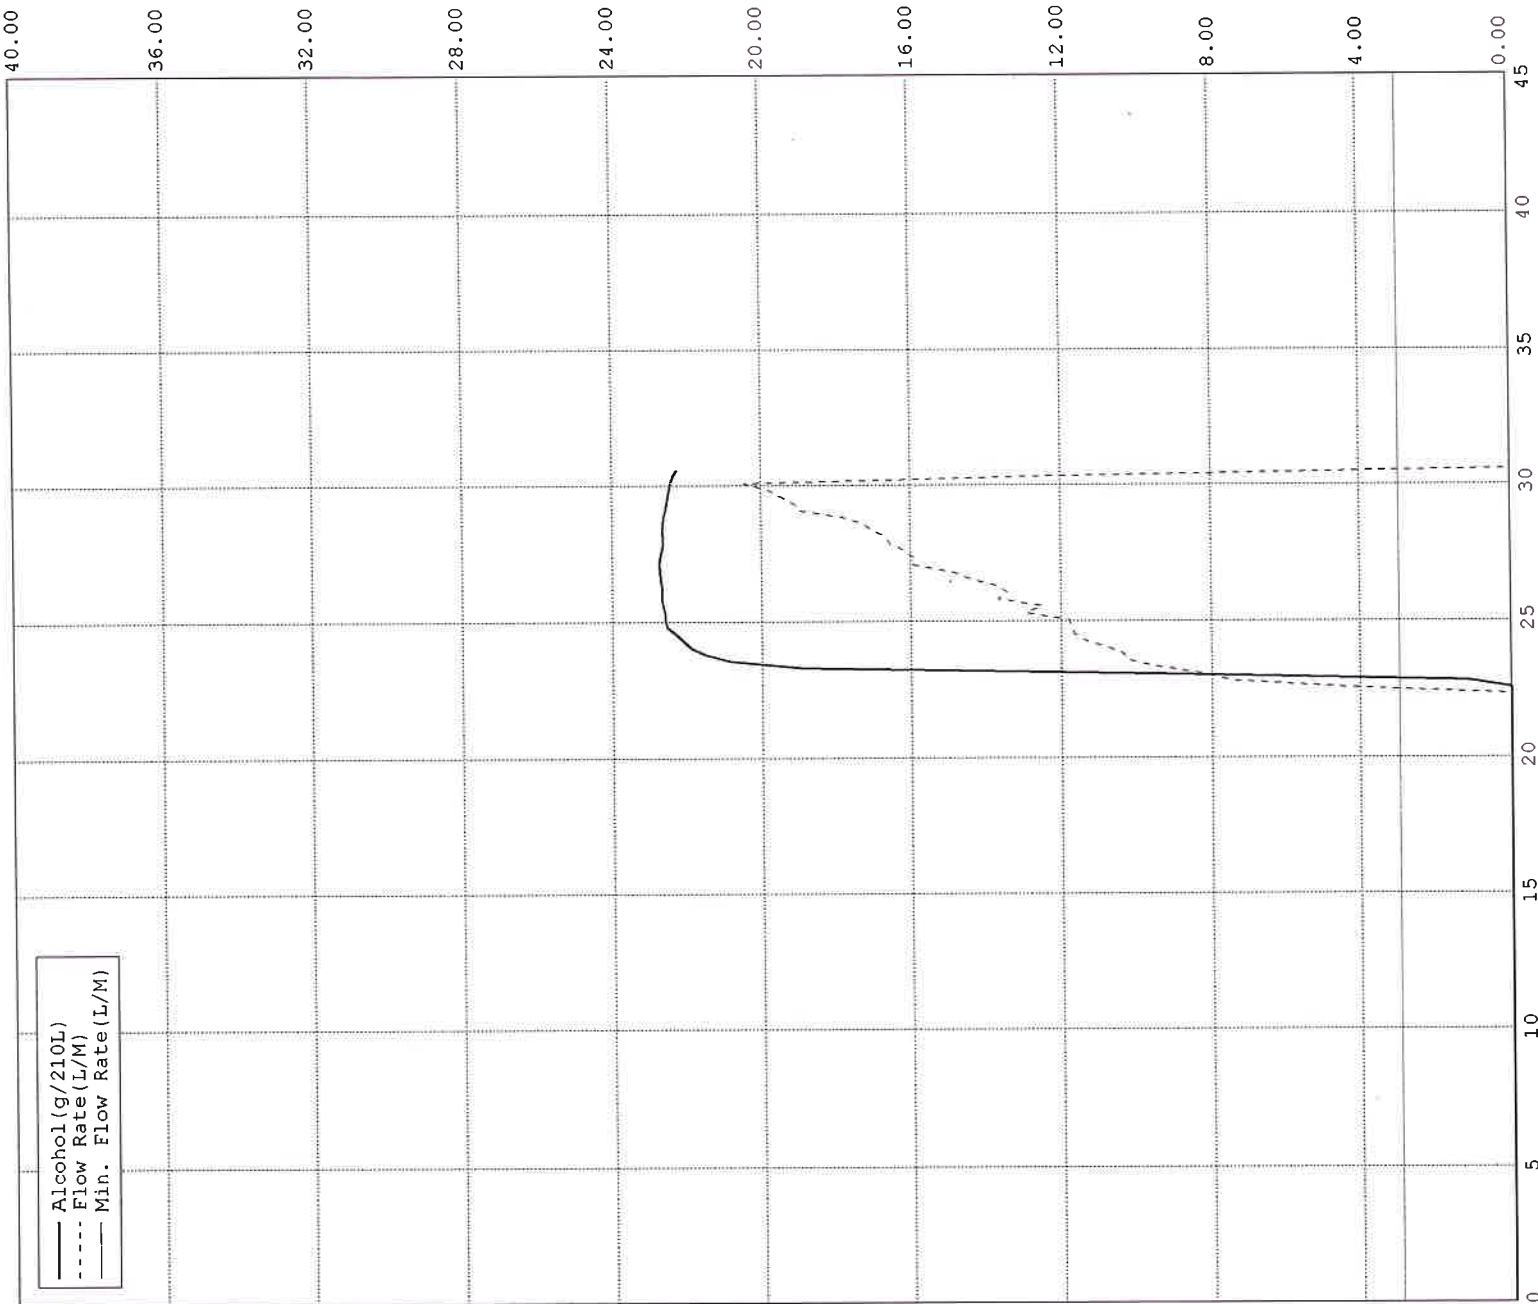

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100699

Date: 06/11/2025

Time: 14:44:48

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - IPA

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.95: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK PASSED 14:45

BLANK TEST 0.000 14:45

INTERNAL STANDARD VERIFIED 14:46

Xq = 0.079 (0.44%)

EXTERNAL STANDARD 0.082 14:46

X[1] = 0.0816 (0.0016) (0.0003)


BLANK TEST 0.000 14:47

SUBJECT SAMPLE XXX 14:48

X[1] = 0.1192 (-0.0237) (0.0012)

Interference Detected

MNC

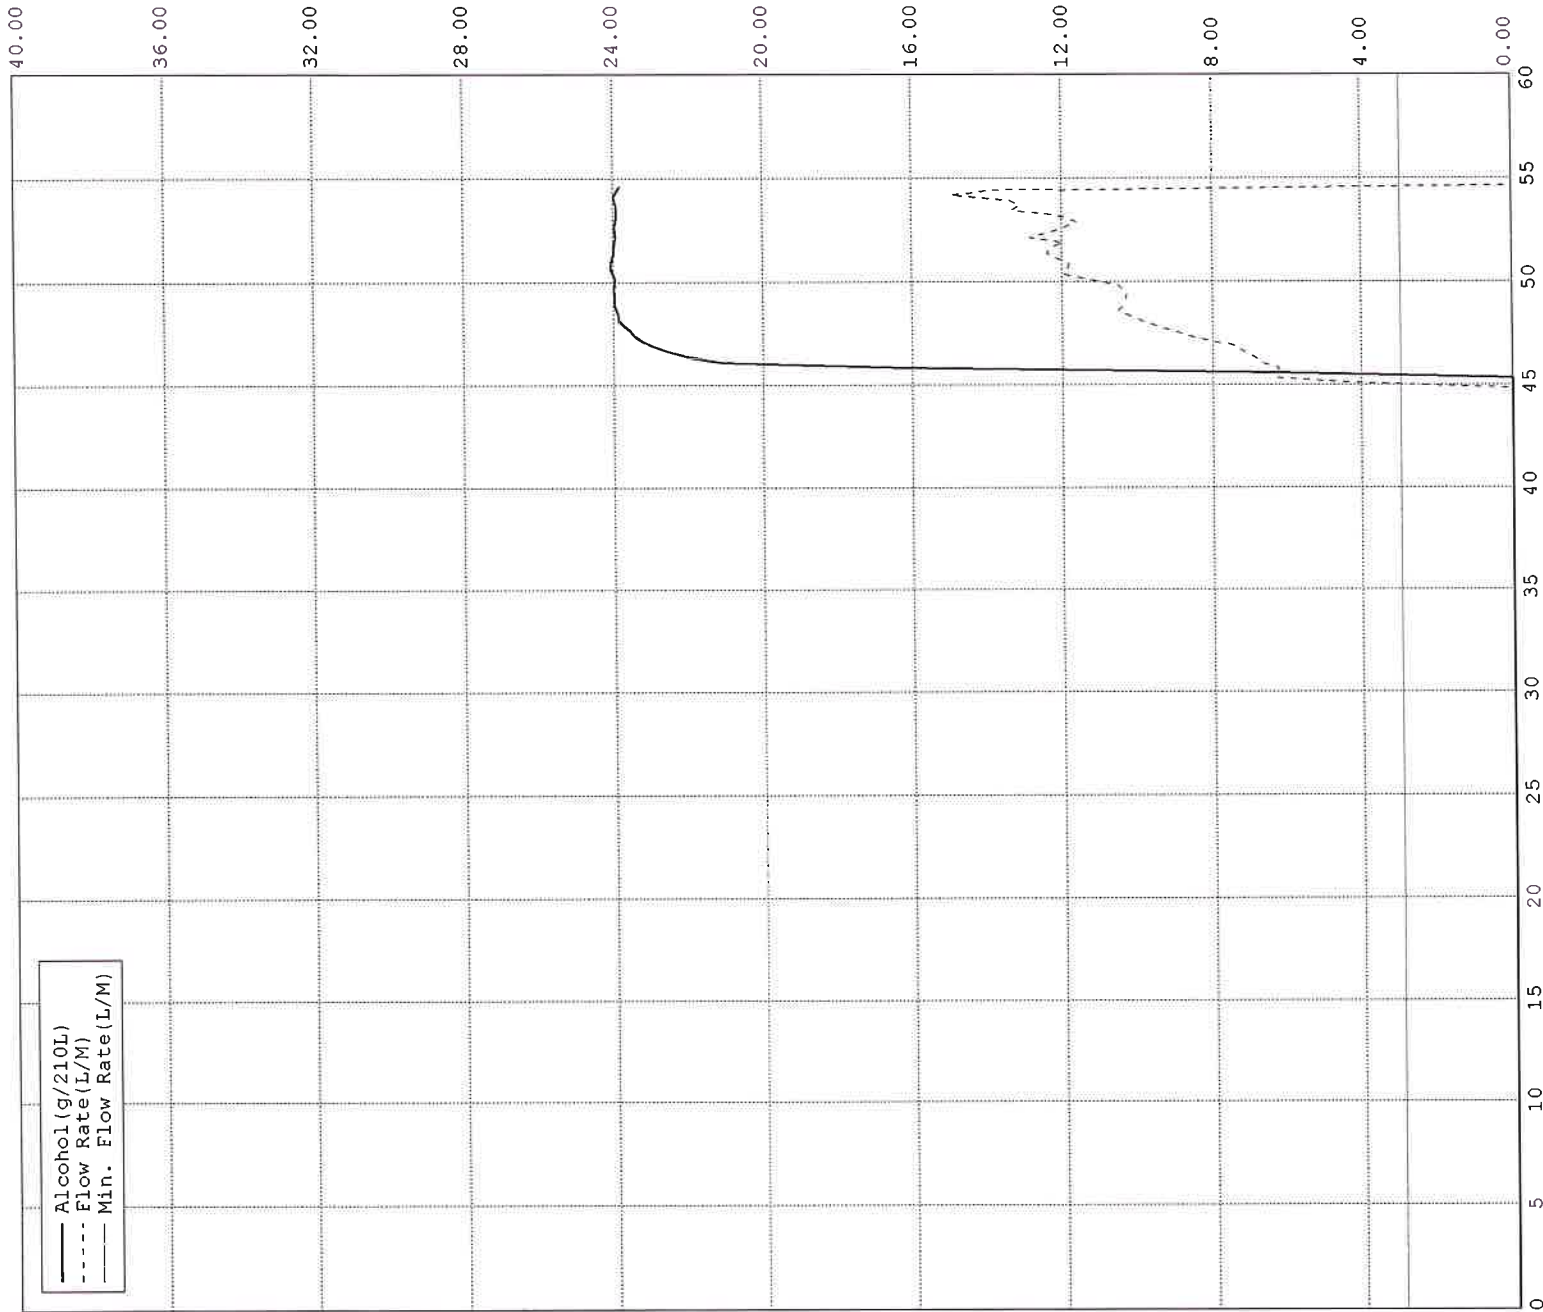

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100699

Date: 06/11/2025
Time: 14:27:41

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INTERFERENCE - BLANK
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.95: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:28
BLANK TEST	0.000	14:28
INTERNAL STANDARD	VERIFIED	14:28
$X_q = 0.077$ (1.54%)		
EXTERNAL STANDARD	0.080	14:29
$X[1] = 0.0796$ (0.0005)	(0.0004)	
BLANK TEST	0.000	14:30
SUBJECT SAMPLE (Vol=2.07L)	0.094	14:30
$X[1] = 0.0948$ (0.0015)	(-0.0009)	
BLANK TEST	0.000	14:31
EXTERNAL STANDARD	0.079	14:31
$X[1] = 0.0791$ (0.0006)	(0.0011)	
BLANK TEST	0.000	14:32

MNC

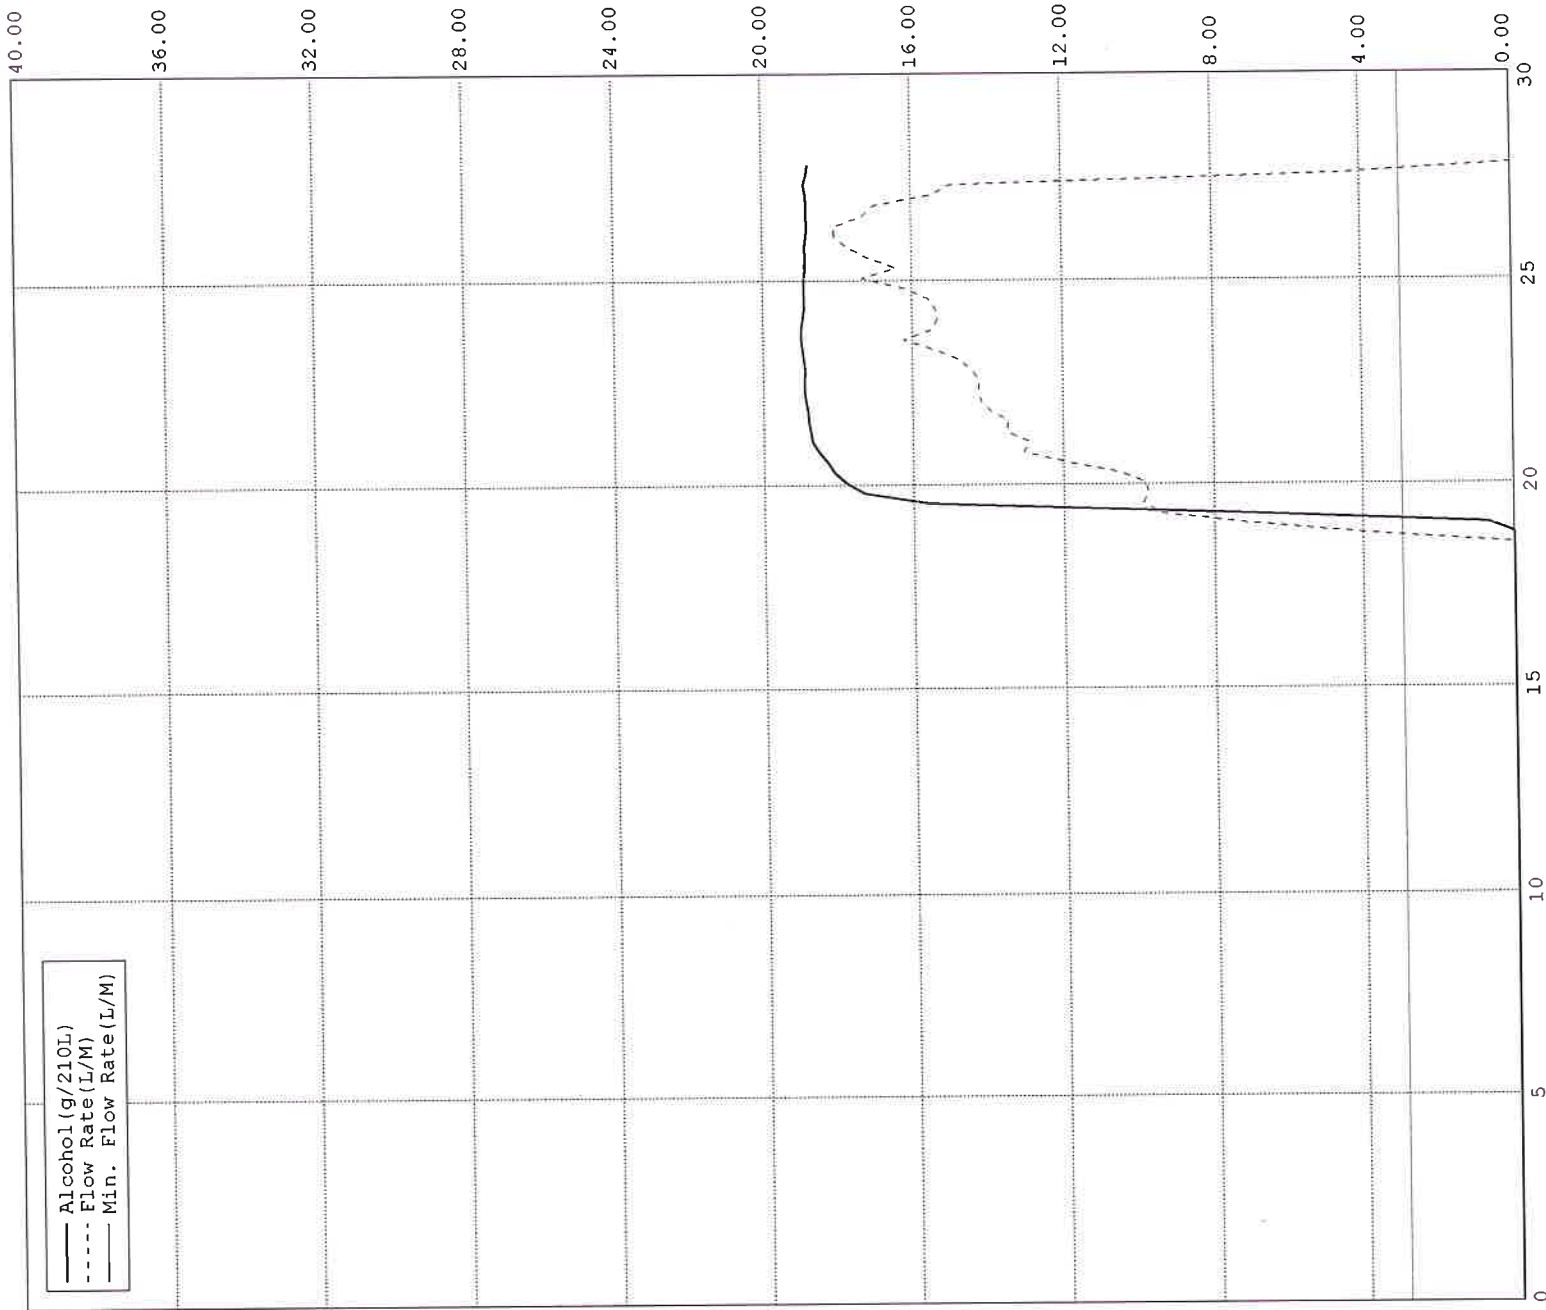

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100699

Date: 06/11/2025

Time: 15:05:22

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.93: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	15:06
BLANK TEST	0.000	15:06
INTERNAL STANDARD	VERIFIED	15:06
EXTERNAL STANDARD	0.078	15:06
BLANK TEST	0.000	15:07
SUBJECT SAMPLE (Vol=2.25L)	0.000	15:08
BLANK TEST	0.000	15:09
EXTERNAL STANDARD	0.080	15:09
BLANK TEST	0.000	15:10

MNC

