



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory
4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100695

Report Issue Date: 06/23/2025
Date Received: 2025-05-19
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.079	AG335202	0.079	0.078	0.078	0.078	0.078	0.078
0.300	0.297	AG427706	0.297	0.297	0.297	0.297	0.297	0.297

As Found - Evaluation Analyst: Carlie Glaister

As Found Conditions - Barometric Pressure (inHg): 29.74 Barometer Used: VWR S/N 240680771 Temperature (C): 22.8 Relative Humidity (%): 20

As-Found Lab Activity Date Range: 05/22/2025 - 05/22/2025

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.021	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.040	0.039	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.079	AG335202	0.077	0.077	0.077	0.077	0.077	0.077	+/- 0.004
0.100	0.098	AG333401	0.099	0.099	0.099	0.099	0.099	0.099	+/- 0.004
0.150	0.148	AG332004	0.146	0.145	0.146	0.145	0.146	0.146	+/- 0.006
0.300	0.295	AG427706	0.293	0.293	0.293	0.293	0.293	0.293	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.53 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 29

As-Left Lab Activity Date Range: 06/04/2025 - 06/05/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 06/23/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 06/23/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100695 Analyst or Technician Name: Kaija Swisher
DataMaster DMT Calibration Start Date: 6/4/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 290680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.53 Temperature(C) 22.3 Relative Humidity(%) 29
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)
- ☒ Interference (Volatiles) - *Print with View Details*

- 1. Acetone Reagent Lot Number: 70250603KS Expiration Date: 7/27/25
Simulator S/N: SD1200 Thermometer Verification Performed? ☒
- 2. Isopropanol Reagent Lot Number: 70250603KS Expiration Date: 9/3/25
Simulator S/N: SD1198 Thermometer Verification Performed? ☒
- 3. Negative (Ethanol Only) Lot Number: 231PY1233 Expiration Date: 9/3/25
Simulator S/N: SD199 Thermometer Verification Performed? ☒

0.100 solution exp: 9/20/2025
KS 06/05/2025

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/4/25
Data Interpretation Date (Technician): N/A (if applicable)
Data Interpretation Date (Analyst): 6/5/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100695

Date: 06/04/2025
 Time: 08:06:02

VERSIONS
 DMT: 3.02
 PIC: 3.03
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 48.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.73 V	PASSED
(1.07 V - 2.51 V)	
Cooler Voltage = 1.87 V	PASSED
(1.07 V - 2.51 V)	
Bias Voltage = 79 V	PASSED
(48 V - 112 V)	
Chopper Freq = 566 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.5 in	

PUMP INFO

Flow Rate = 4.270 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.001 V <= 0.010 V)	
PUMP OFF	PASSED
(0.001 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

	PASSED
Xq = 0.114 0.78% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100695

Date: 06/04/2025

Time: 8:18 AM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 47.2°C

Current Barometer 29.5 in

Volume (Ltr) 1.52

Settings

Lamp: 1.82 V

Bias: 79 V

Cooler: 1.87 V

Chopper: 565 Hz

Voltages (V)

Flow: 1.04 V

Detector: -0.058 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 11/07/2023
Time: 08:48:24

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.980197 0.800 <= CAL < 1.200
b1 = 0.0006 0.0000 <= b1 < 0.0040
b2 = 0.0057 0.0010 <= b2 < 0.0100
b3 = 0.0004 0.0000 <= b3 < 0.0040
Xq = 0.1136 0.0500 <= Xq < 0.2000
a21 = 1.137430 1.050 <= a21 < 1.300
a31 = 0.528219 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100695

Date: 06/04/2025
 Time: 08:46:47

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX


OPERATOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

DEPT/AGENCY:
 MINIMUM VOLUME TEST
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.51: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:47
BLANK TEST	0.000	08:47
INTERNAL STANDARD	VERIFIED	08:48
EXTERNAL STANDARD	0.077	08:48
BLANK TEST	0.000	08:49
SUBJECT SAMPLE (Vol=1.56L)	0.000	08:49
BLANK TEST	0.000	08:50
EXTERNAL STANDARD	0.078	08:51
BLANK TEST	0.000	08:51

KS

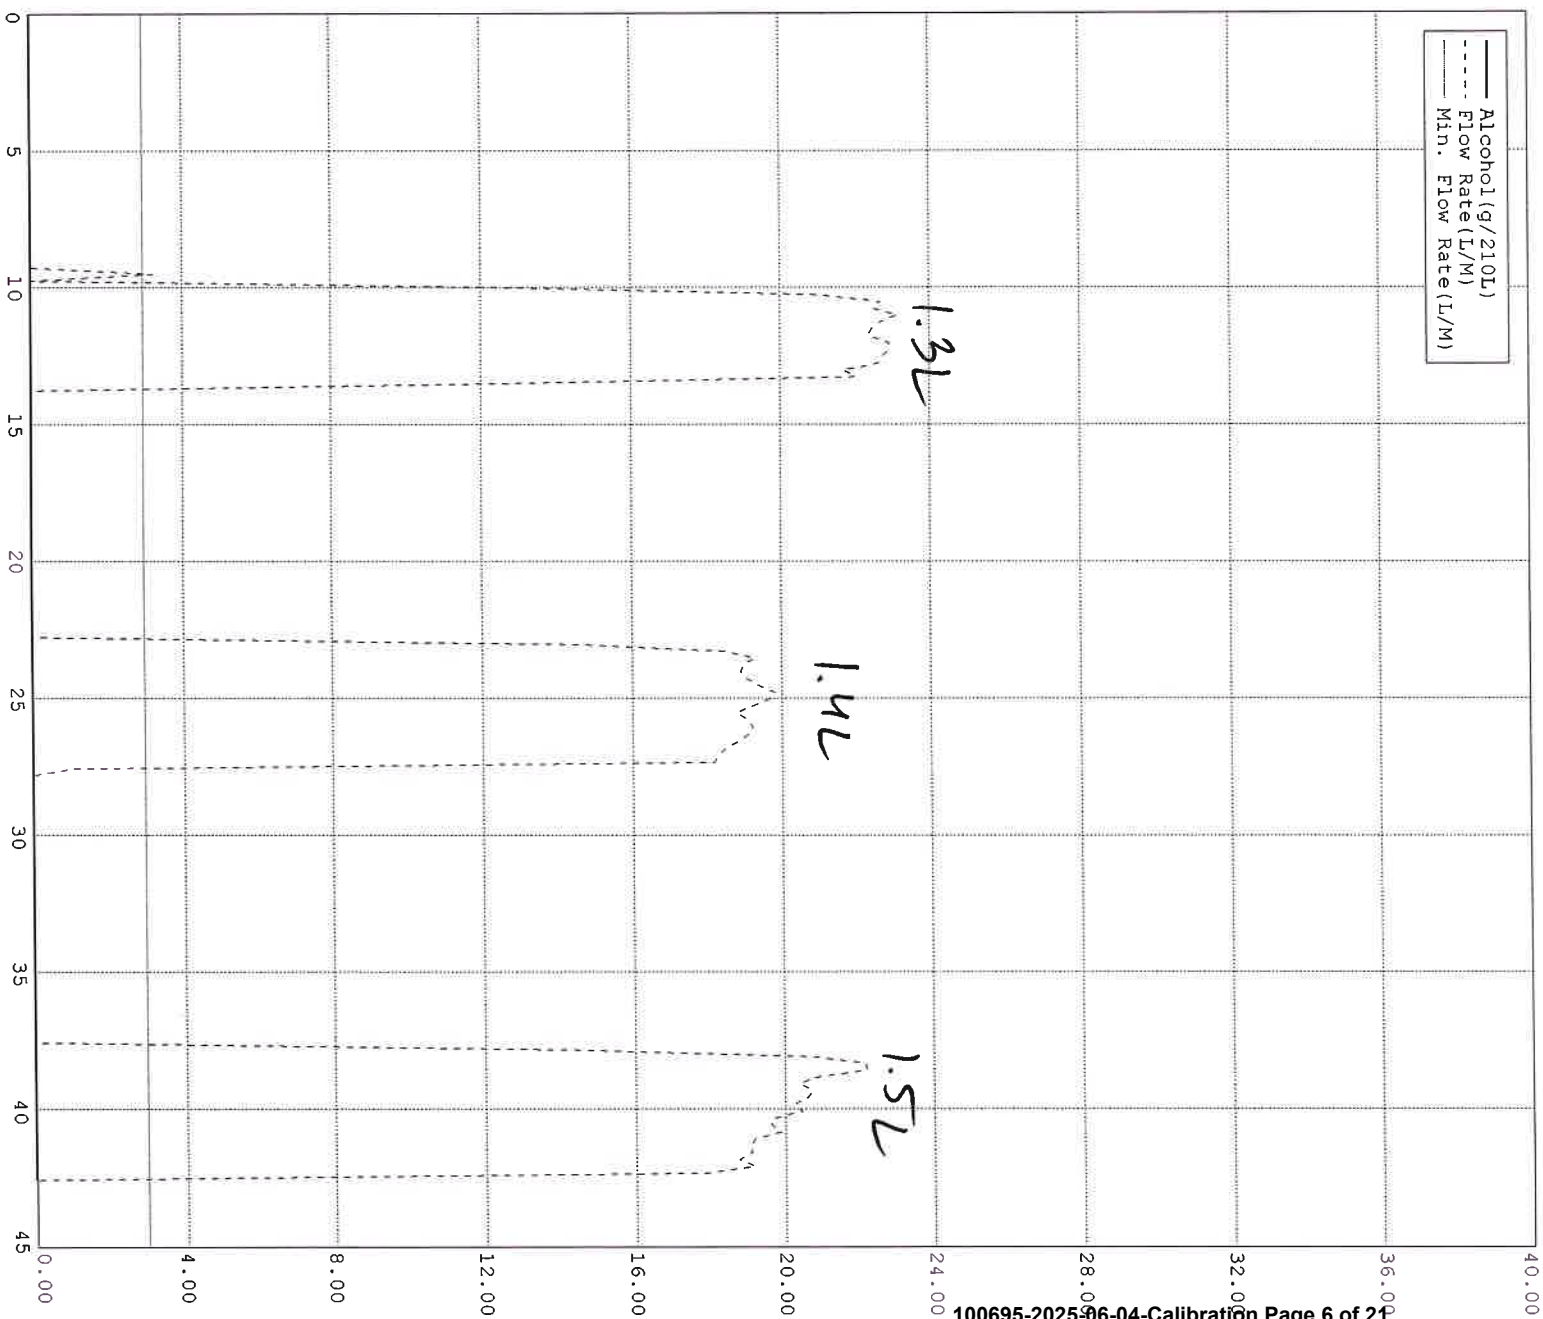

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100695

Date: 06/04/2025
 Time: 10:50:30

SUPERVISOR NAME:
 KAIJA SWISHER
 OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.039	0.0398	0.0004
0.079	0.0770	0.0000
0.098	0.0990	0.0000
0.148	0.1456	0.0005
0.295	0.2930	0.0000

SLOPE = 0.990531
 R^2 = 0.999842

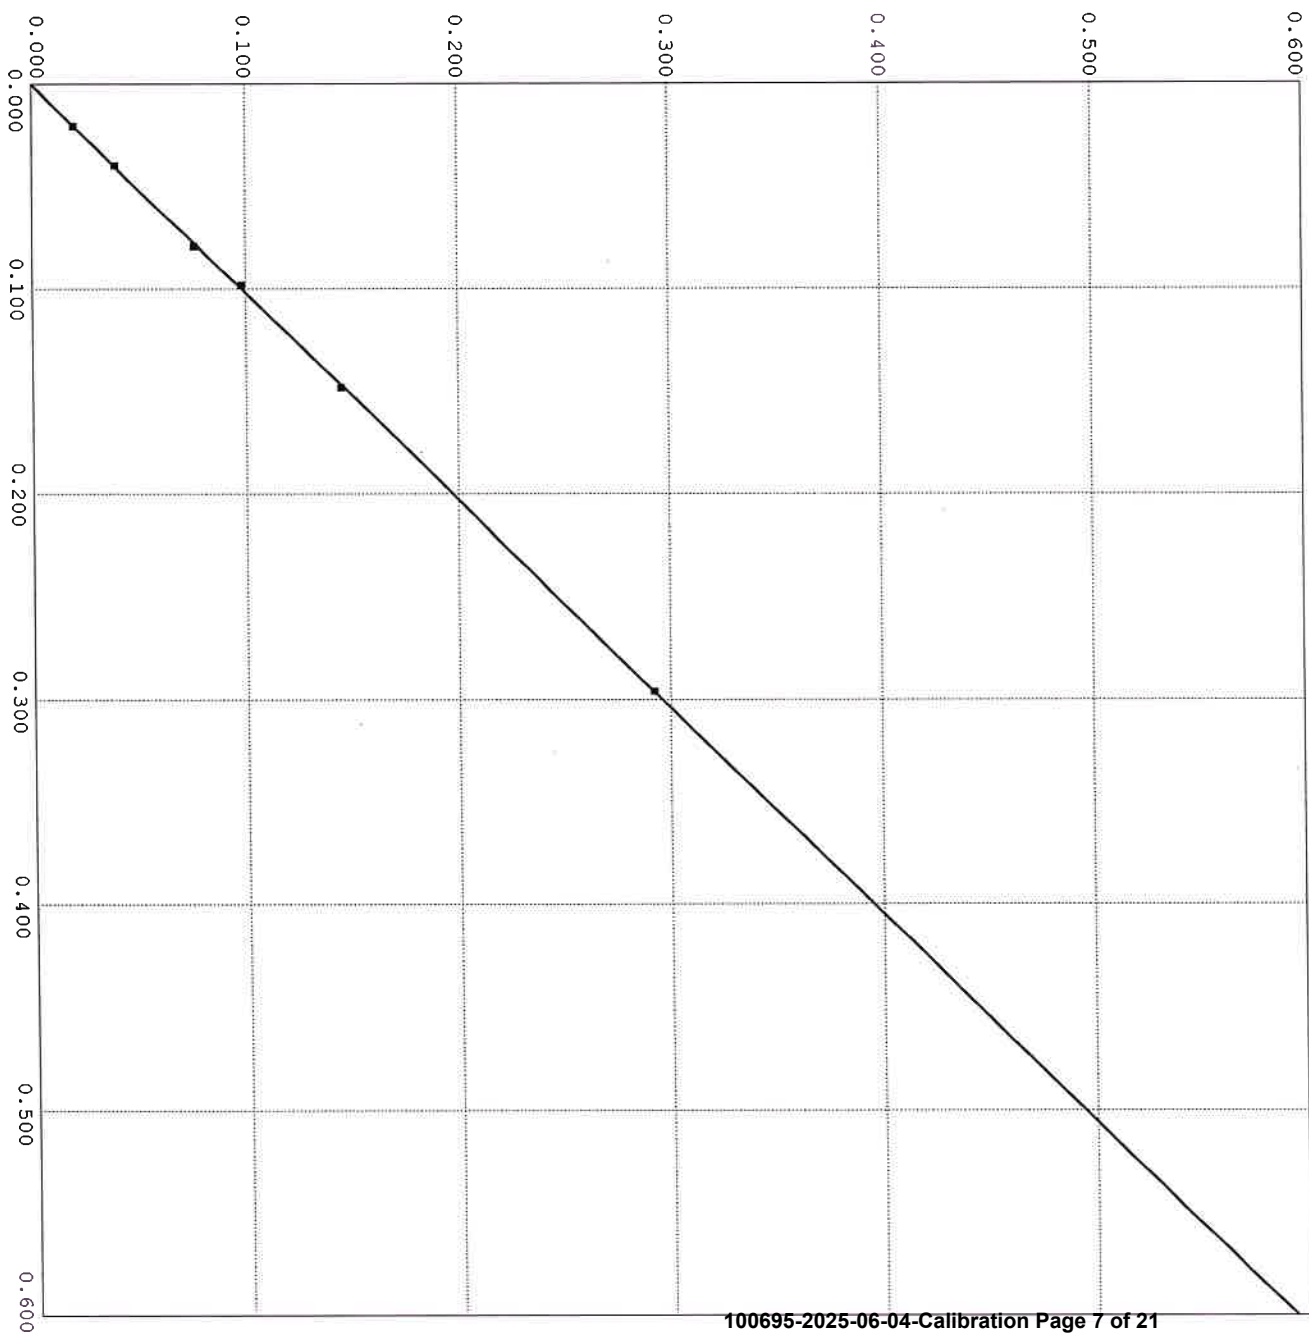

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 06/04/2025
Time: 10:50:32

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.47: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 168 psi

BLANK TEST	0.000	10:51
INTERNAL STANDARD	VERIFIED	10:51
EXTERNAL STANDARD	0.020	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.020	10:53
BLANK TEST	0.000	10:54
EXTERNAL STANDARD	0.021	10:54
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.020	10:55
BLANK TEST	0.000	10:56
EXTERNAL STANDARD	0.020	10:56
BLANK TEST	0.000	10:57

Average = 0.0202
Std Dev = 0.0004

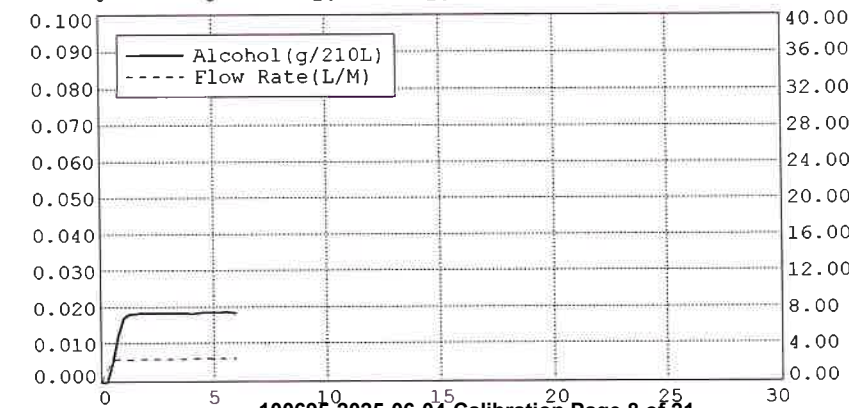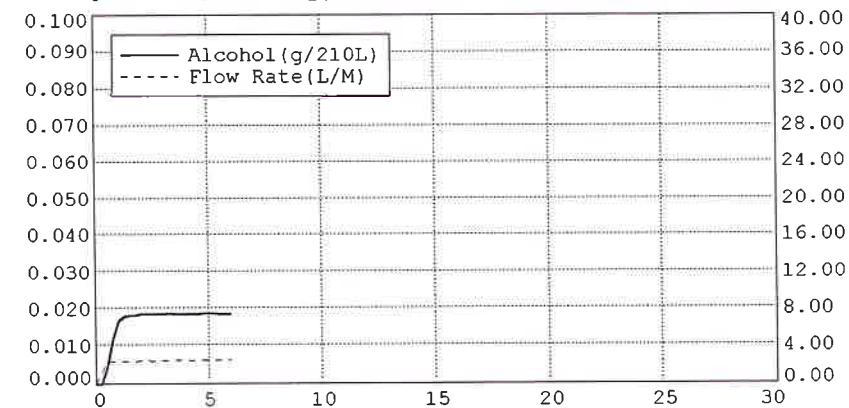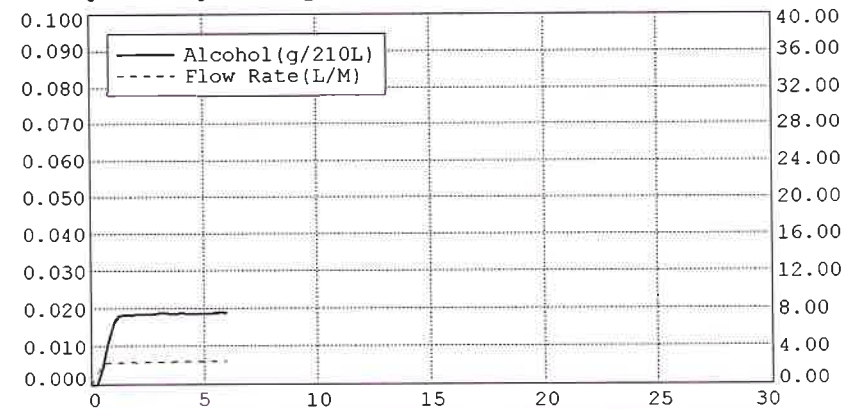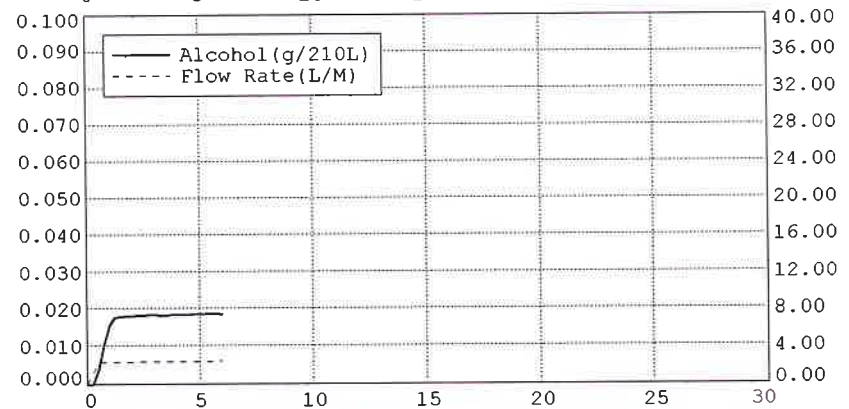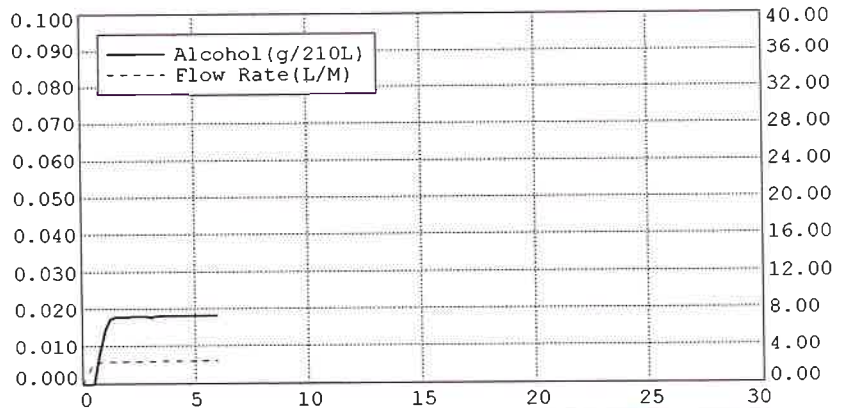

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 06/04/2025
Time: 11:00:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.46: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 901 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	11:01
INTERNAL STANDARD	VERIFIED	11:01
EXTERNAL STANDARD	0.040	11:01
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.039	11:03
BLANK TEST	0.000	11:03
EXTERNAL STANDARD	0.040	11:04
BLANK TEST	0.000	11:05
EXTERNAL STANDARD	0.040	11:05
BLANK TEST	0.000	11:06
EXTERNAL STANDARD	0.040	11:06
BLANK TEST	0.000	11:07

Average = 0.0398
Std Dev = 0.0004

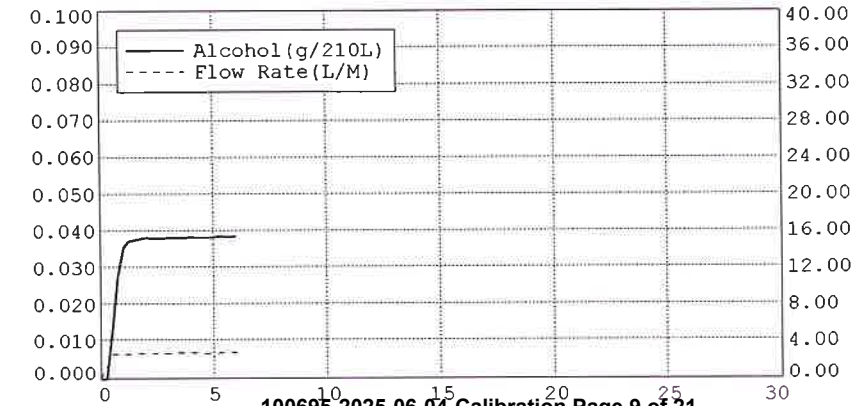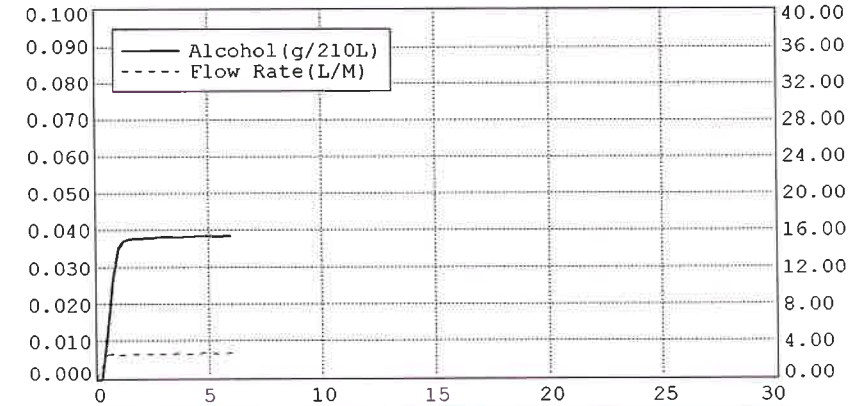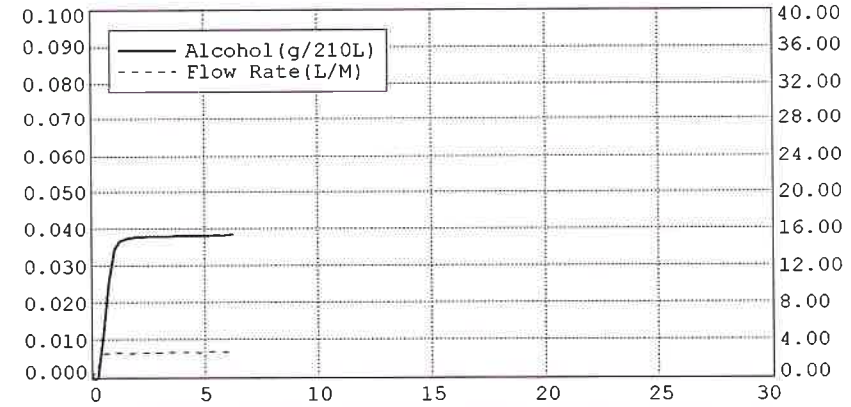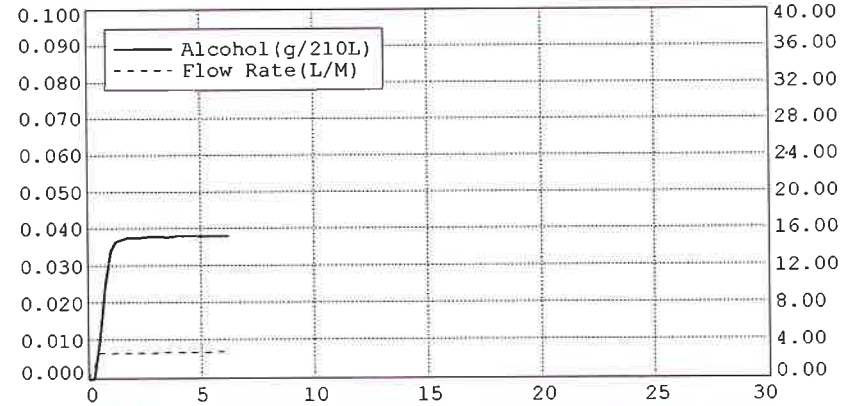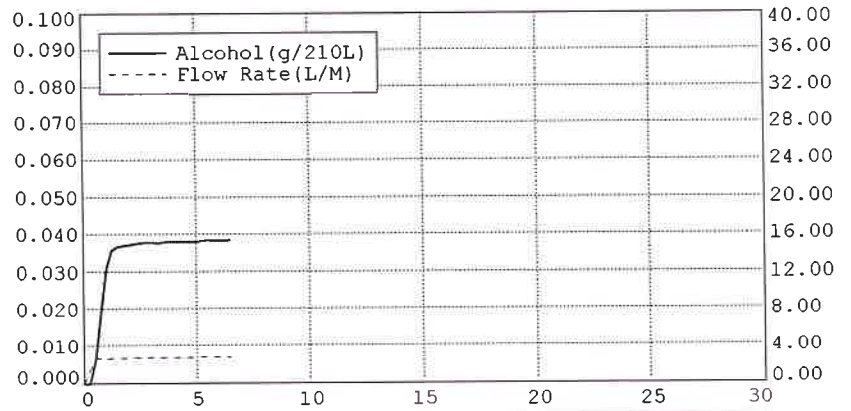

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 06/04/2025
Time: 11:07:55

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.46: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 216 psi

BLANK TEST	0.000	11:09
INTERNAL STANDARD	VERIFIED	11:09
EXTERNAL STANDARD	0.077	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.077	11:10
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.077	11:11
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.077	11:12
BLANK TEST	0.000	11:13
EXTERNAL STANDARD	0.077	11:14
BLANK TEST	0.000	11:14

Average = 0.0770
Std Dev = 0.0000

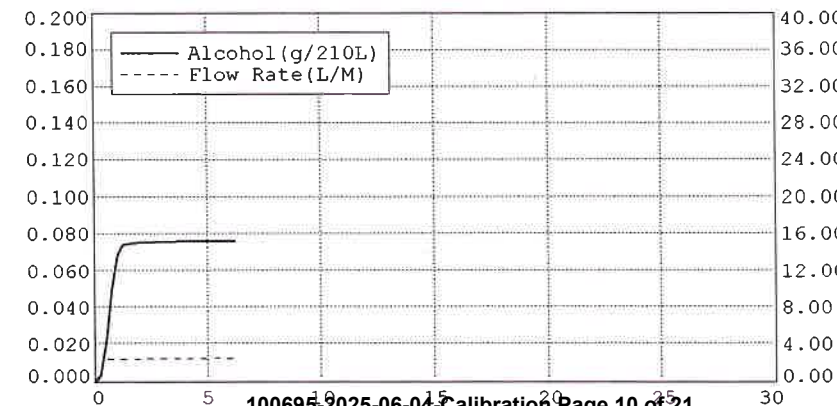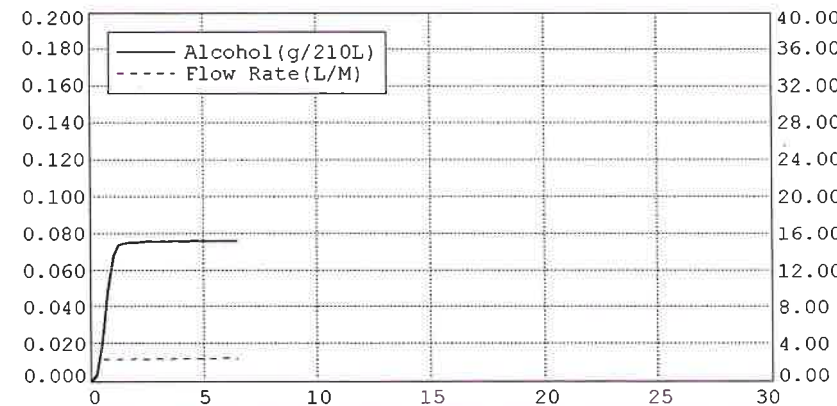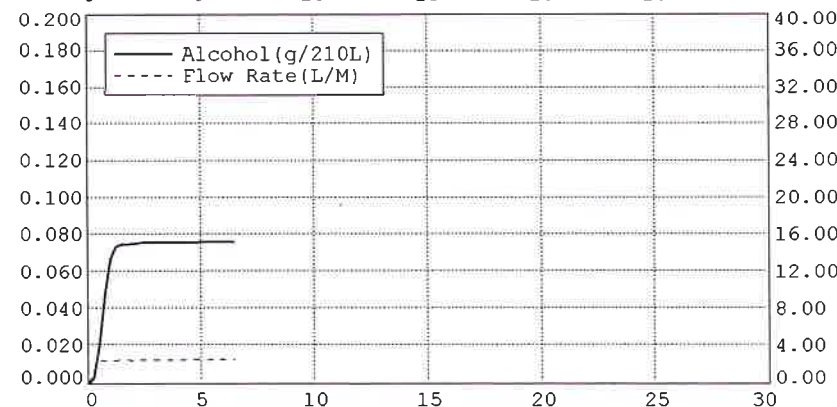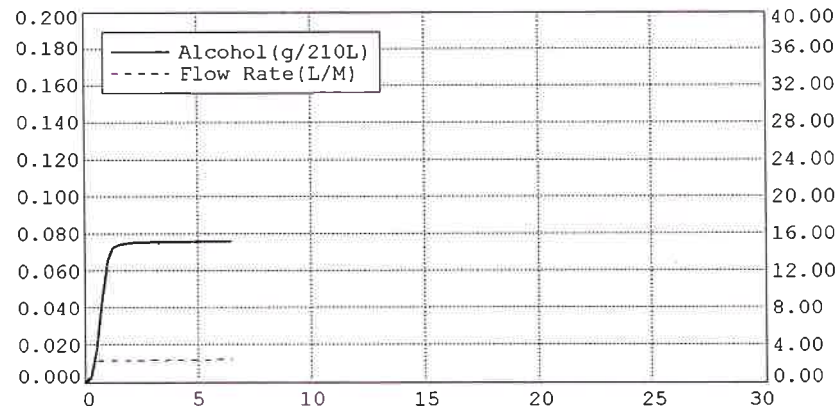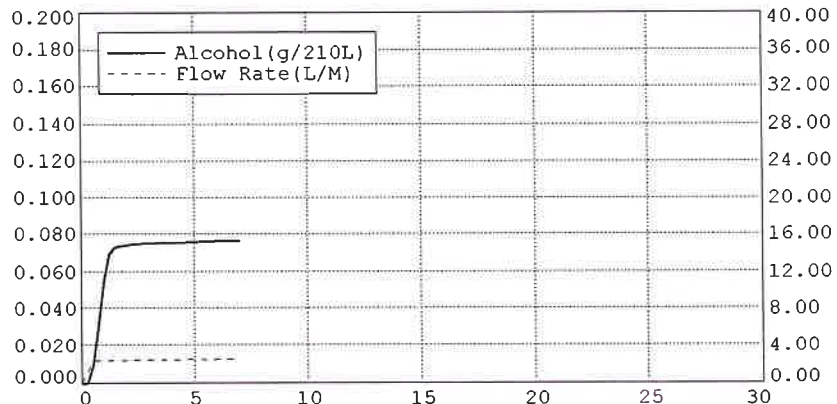

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 06/04/2025
Time: 11:15:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.46: 0.098
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 1046 psi

BLANK TEST	0.000	11:16
INTERNAL STANDARD	VERIFIED	11:16
EXTERNAL STANDARD	0.099	11:17
BLANK TEST	0.000	11:18
EXTERNAL STANDARD	0.099	11:18
BLANK TEST	0.000	11:19
EXTERNAL STANDARD	0.099	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.099	11:20
BLANK TEST	0.000	11:21
EXTERNAL STANDARD	0.099	11:21
BLANK TEST	0.000	11:22

Average = 0.0990
Std Dev = 0.0000

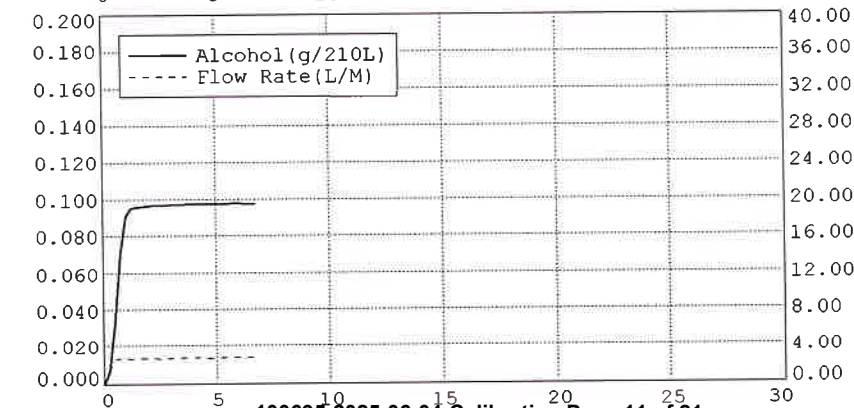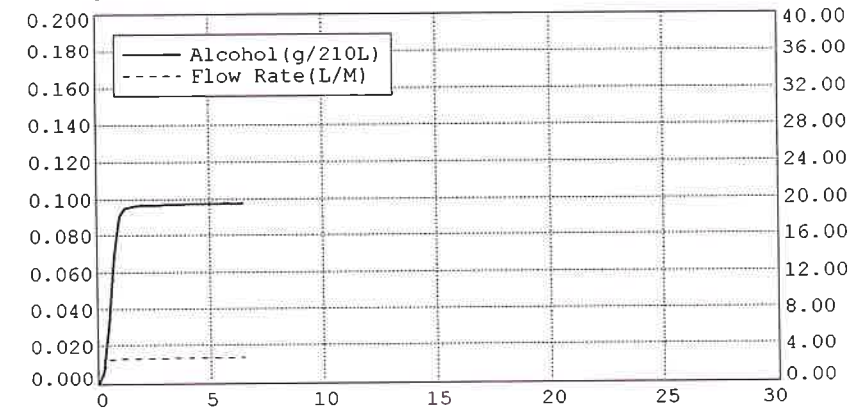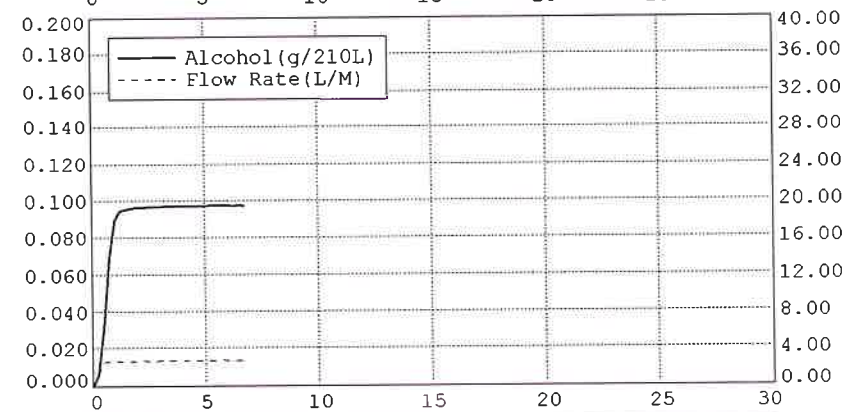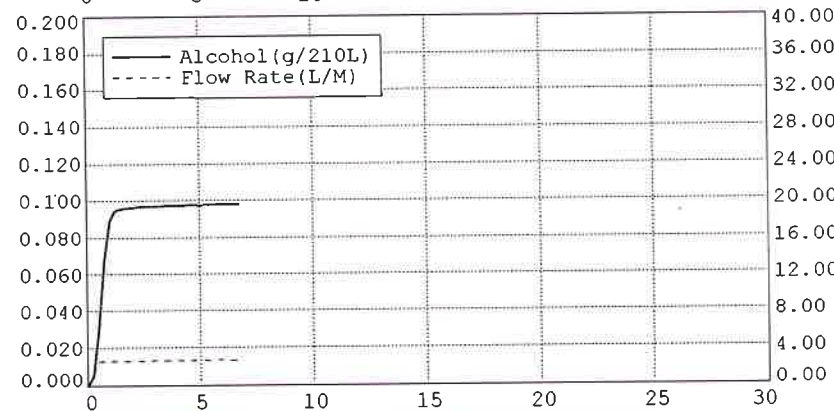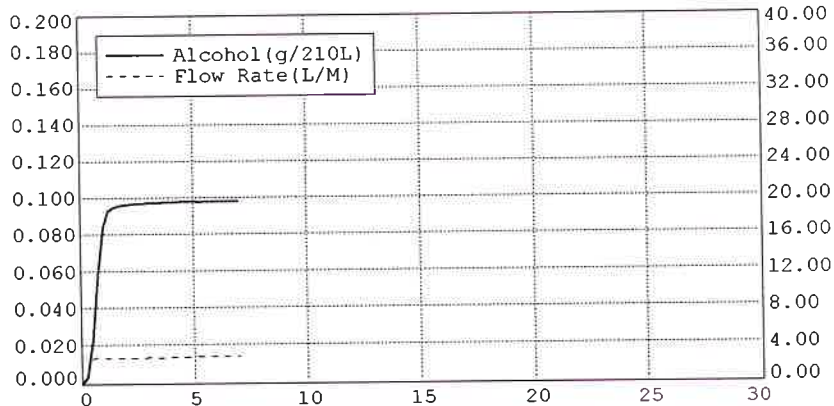

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 06/04/2025
Time: 11:23:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.45: 0.148
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 343 psi

BLANK TEST	0.000	11:24
INTERNAL STANDARD	VERIFIED	11:25
EXTERNAL STANDARD	0.146	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.145	11:26
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.146	11:27
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.145	11:28
BLANK TEST	0.000	11:29
EXTERNAL STANDARD	0.146	11:29
BLANK TEST	0.000	11:30

Average = 0.1456
Std Dev = 0.0005

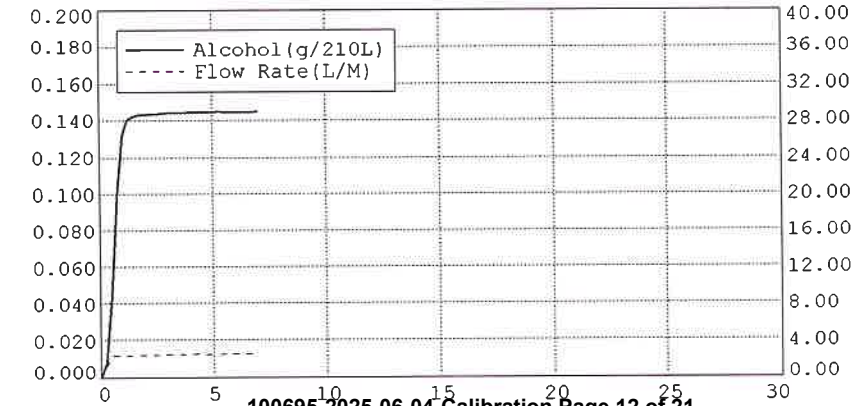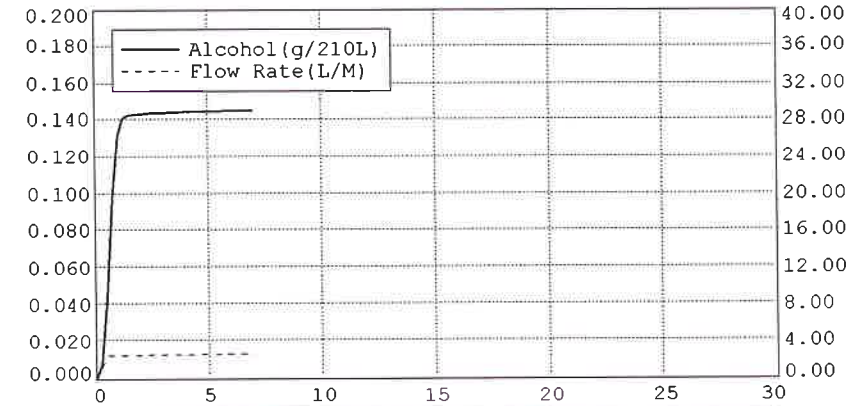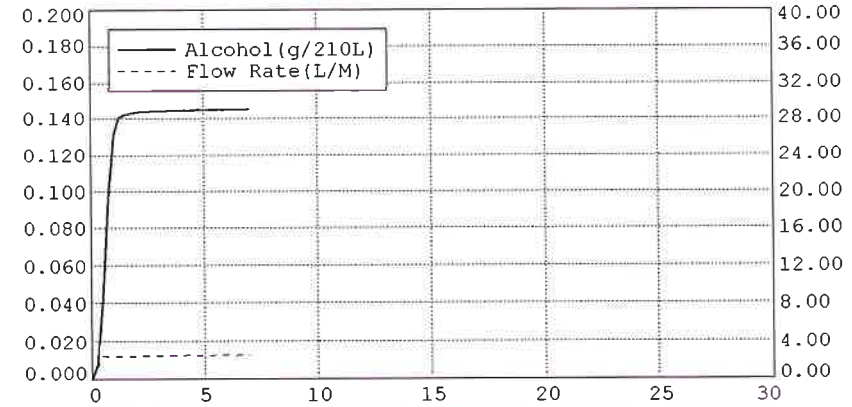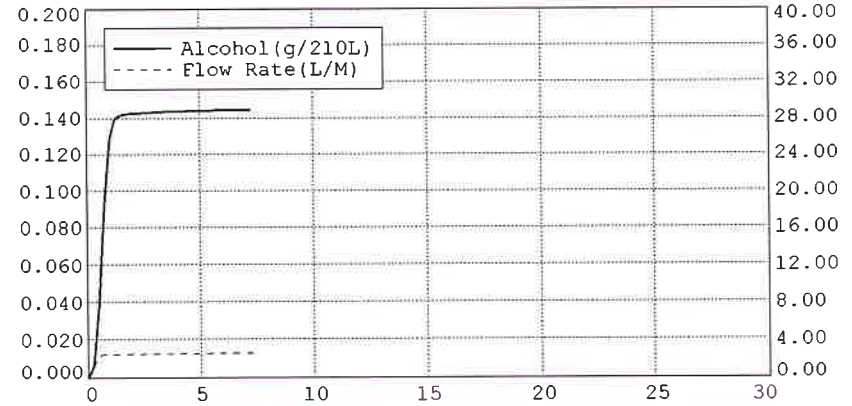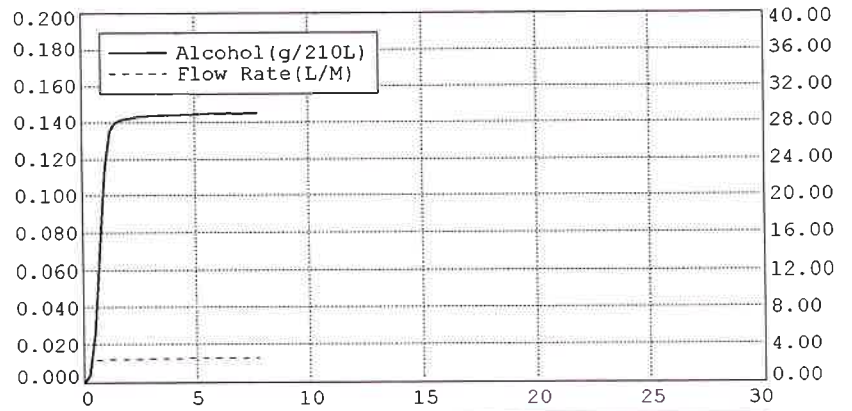

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100695






Date: 06/04/2025
Time: 11:32:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.45: 0.295
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 379 psi

BLANK TEST	0.000	11:33
INTERNAL STANDARD	VERIFIED	11:33
EXTERNAL STANDARD	0.293	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.293	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.293	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.293	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.293	11:38
BLANK TEST	0.000	11:39

Average = 0.2930
Std Dev = 0.0000

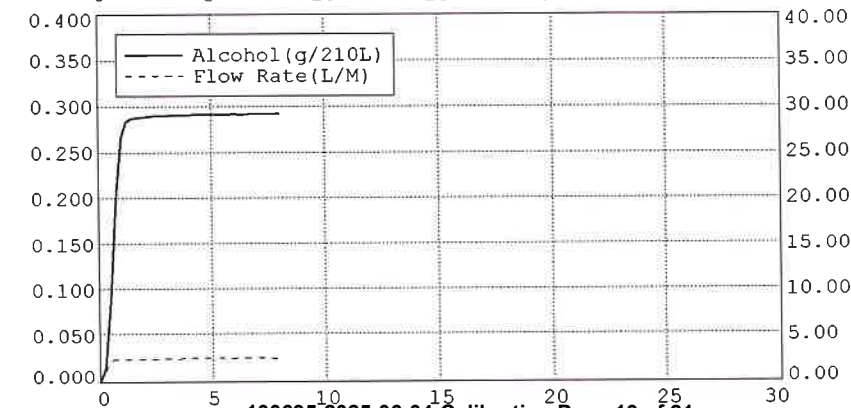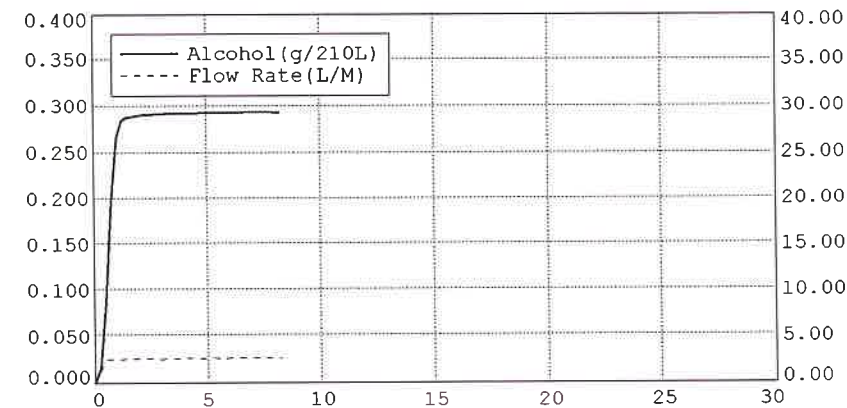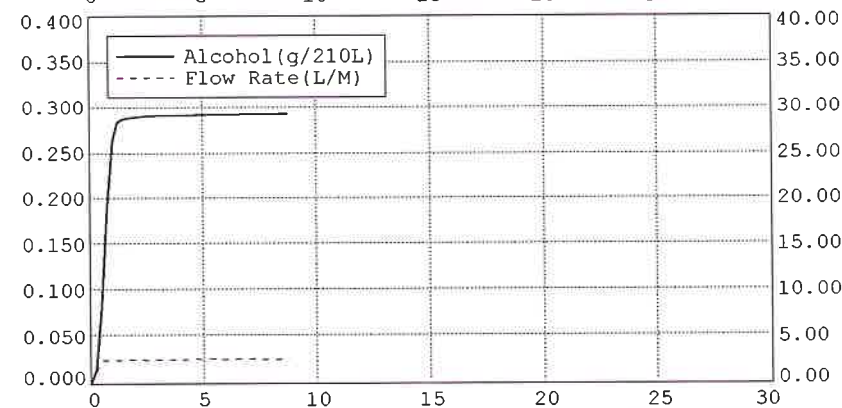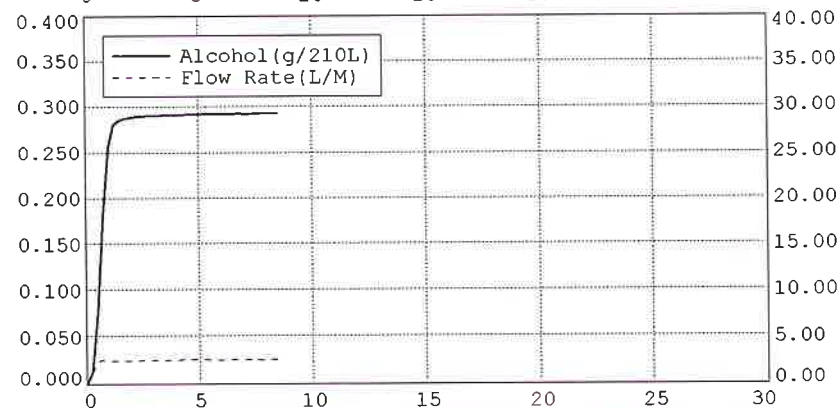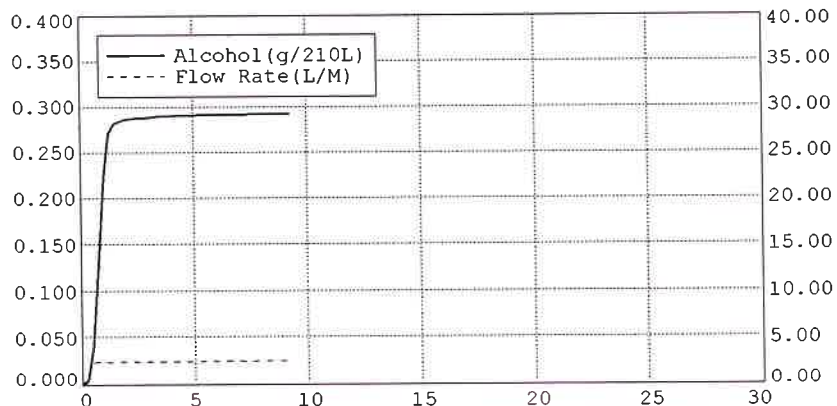

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100695

Date: 06/04/2025
Time: 12:05:40

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.43: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:06
BLANK TEST	0.000	12:07
INTERNAL STANDARD	VERIFIED	12:07
EXTERNAL STANDARD	0.078	12:07
BLANK TEST	0.000	12:08
SUBJECT SAMPLE	INCOMPLETE	12:10

KS

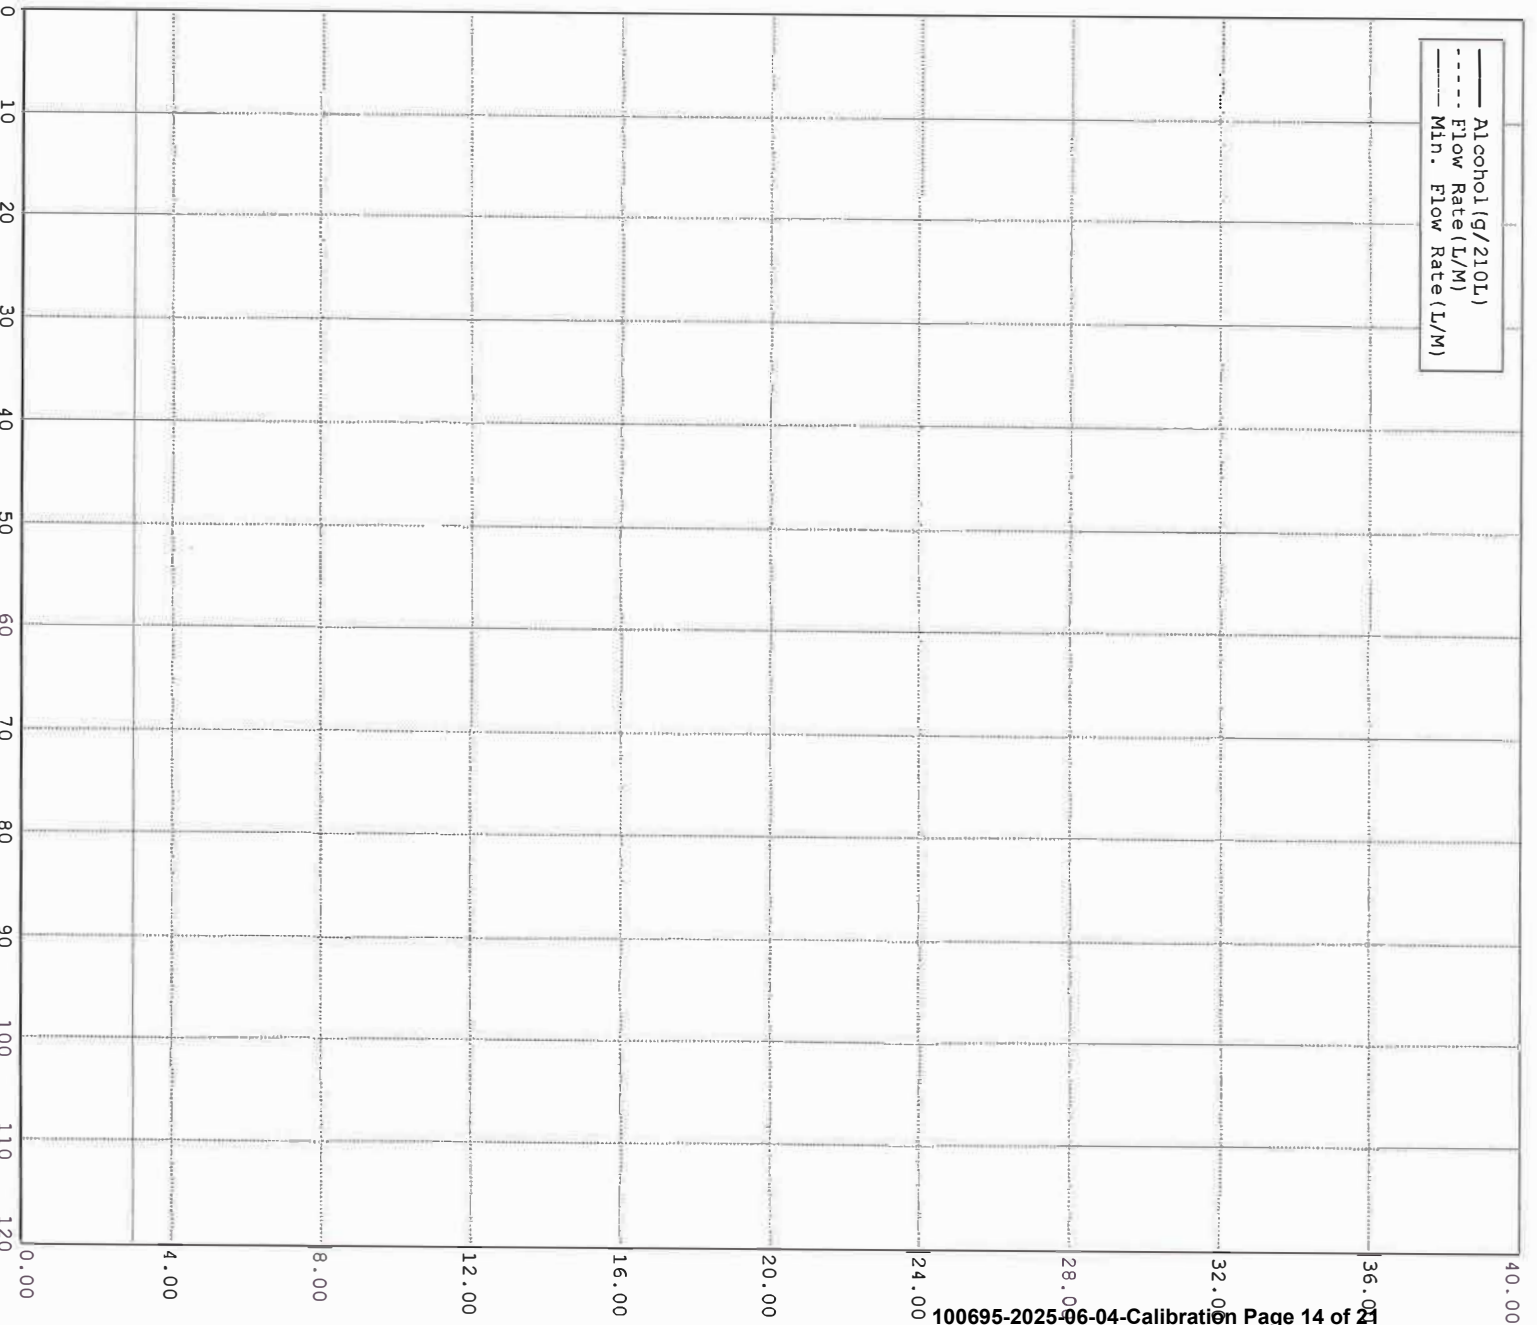

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100695

Date: 06/04/2025
Time: 12:14:54

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	
BLANK TEST	PASSED 12:16
INTERNAL STANDARD	0.000 12:16
EXTERNAL STANDARD	VERIFIED 12:16
BLANK TEST	0.078 12:16
BLANK TEST	0.000 12:17
SUBJECT SAMPLE	XXX 12:18

Maximum Attempts Exceeded

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

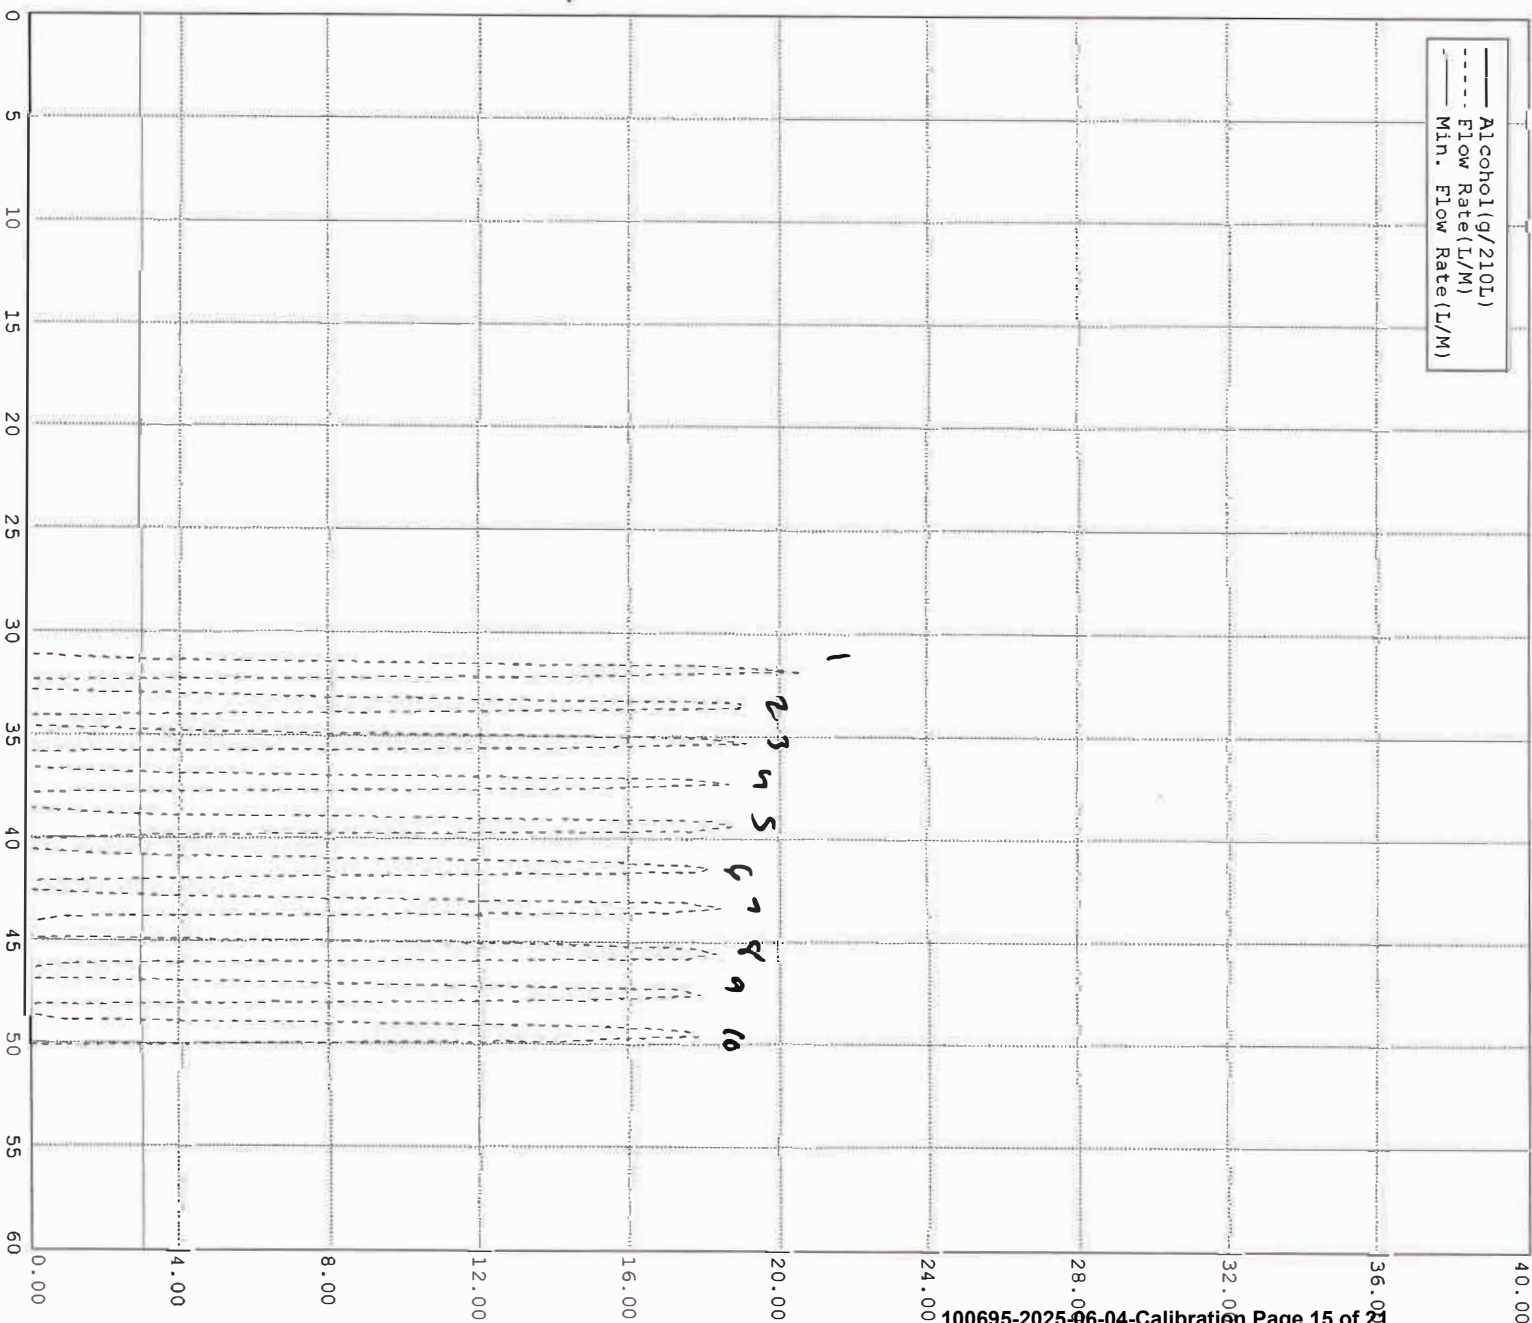

KS

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 06/04/2025
Time: 12:21:51

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:22
BLANK TEST	0.000	12:23
INTERNAL STANDARD	VERIFIED	12:23
EXTERNAL STANDARD	0.078	12:23
BLANK TEST	0.000	12:24
SUBJECT SAMPLE	INVALID	12:25

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

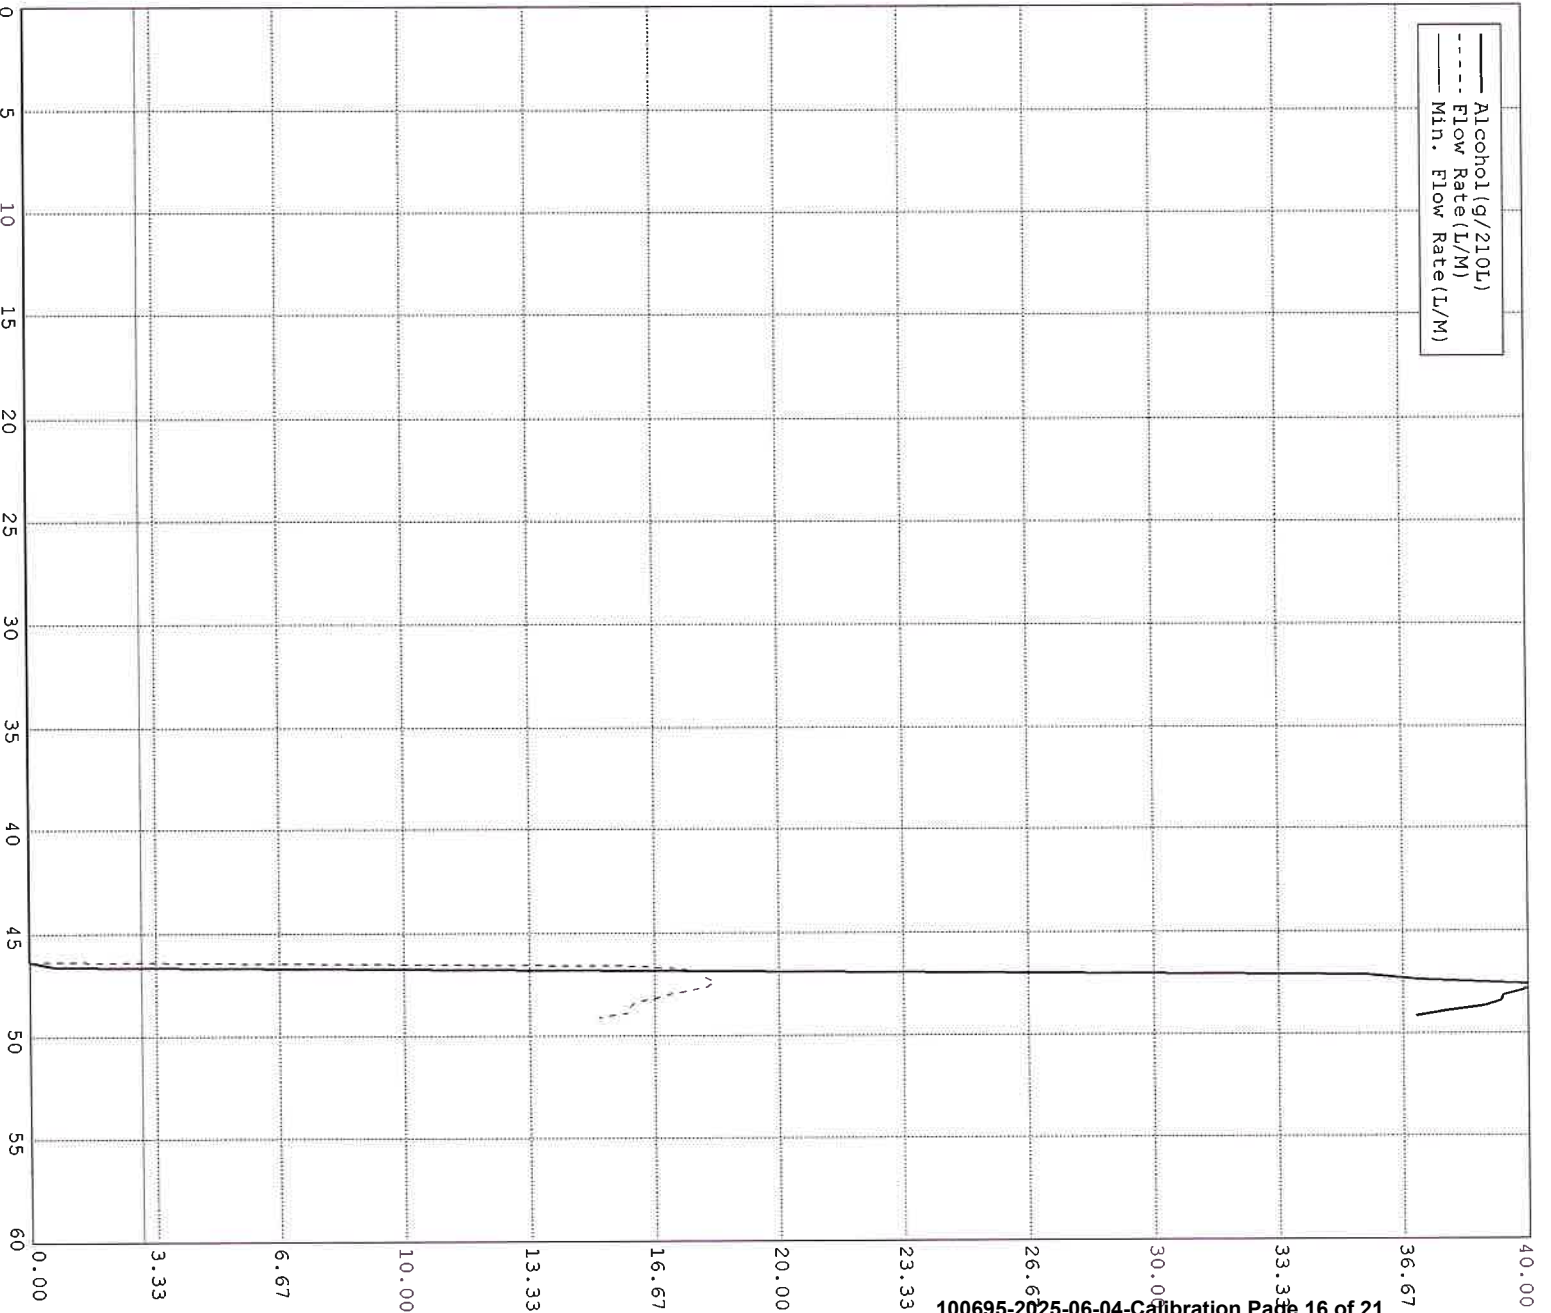

KS

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 06/04/2025
Time: 14:17:52

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:21
BLANK TEST	0.000	14:21
INTERNAL STANDARD	VERIFIED	14:21
EXTERNAL STANDARD	0.078	14:21
BLANK TEST	0.000	14:22

RFI DETECTED

KS

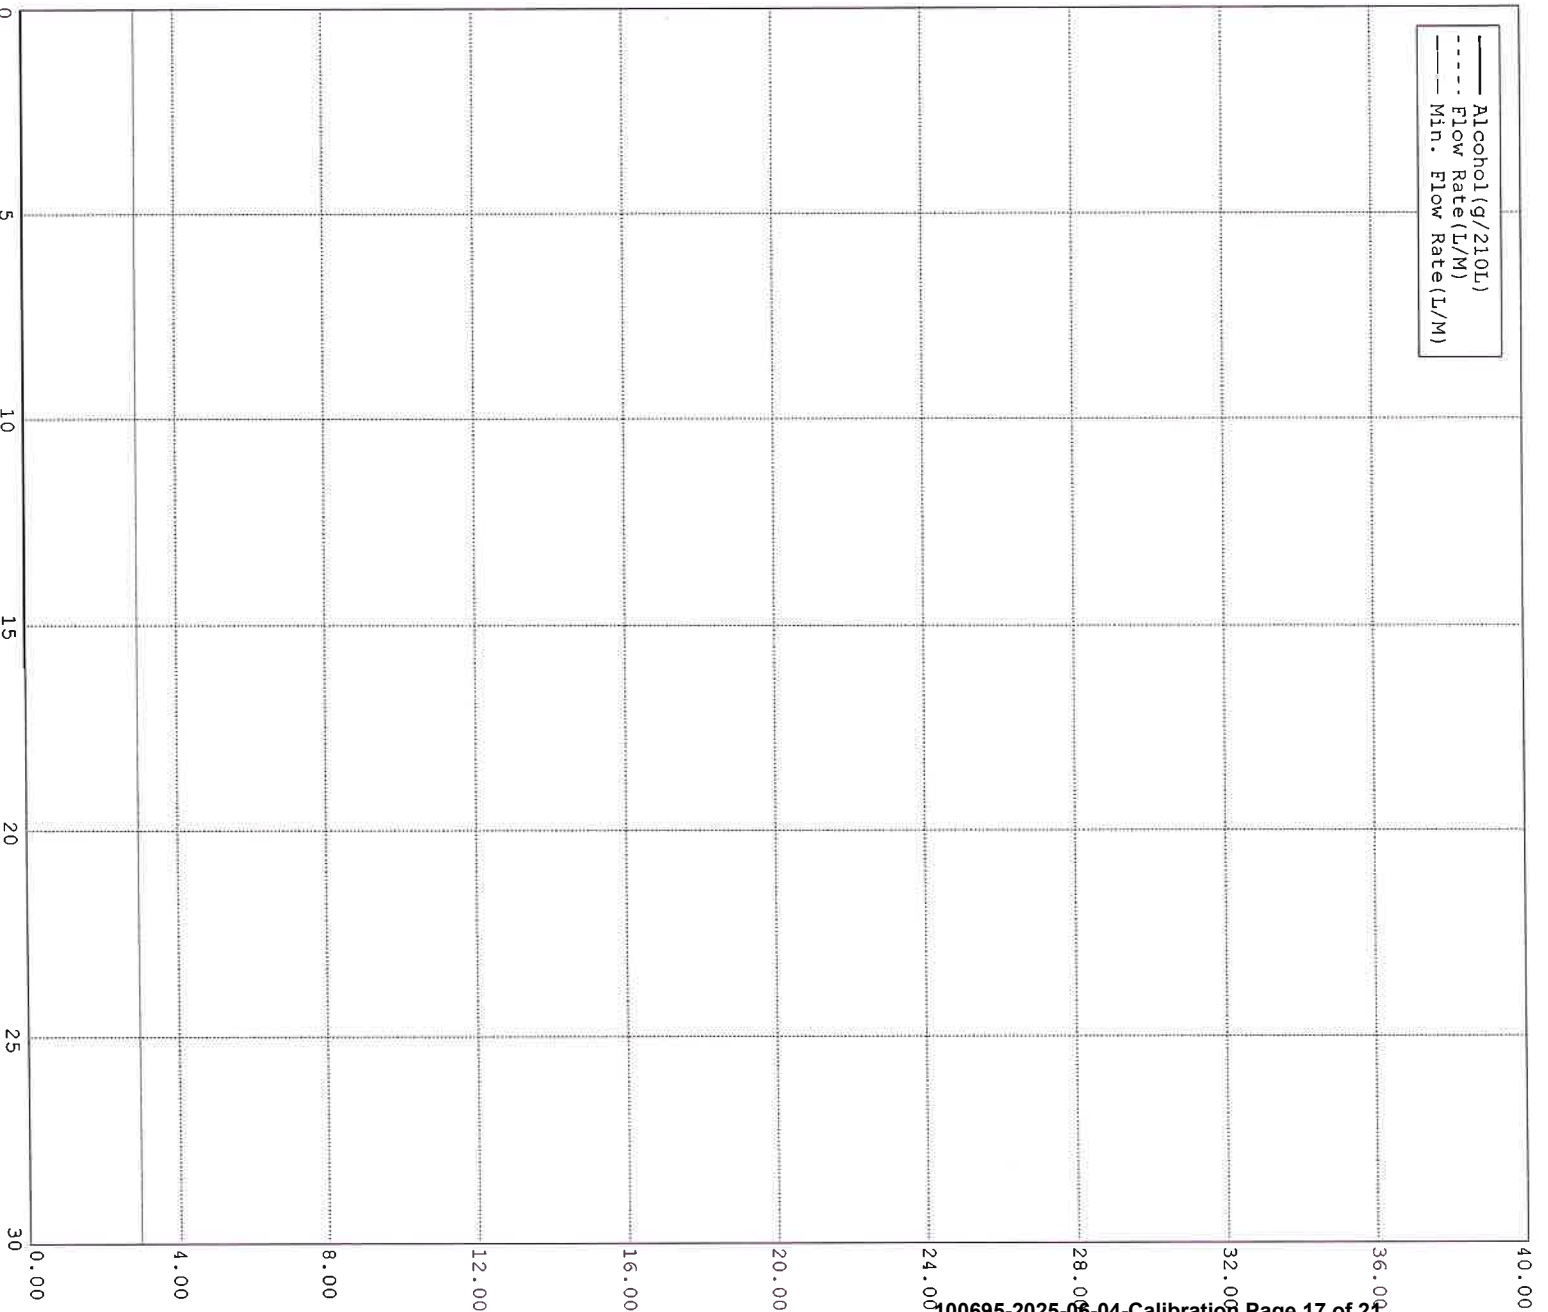

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100695

Date: 06/04/2025
Time: 12:41:40

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:42
BLANK TEST	0.000	12:42
INTERNAL STANDARD	VERIFIED	12:43
Xq = 0.115 (1.32%)	0.077	12:43
EXTERNAL STANDARD	X[1] = 0.0772 (-0.0013)	(0.0029)
BLANK TEST	0.000	12:44
SUBJECT SAMPLE	XXX	12:45
X[1] = 0.1107 (-0.0198)	(0.0022)	


Interference Detected

F2 average: -0.0009

F3 average: ~~0.0029~~
0.0030 KS 6/23/25

KS 6/5/25

KS

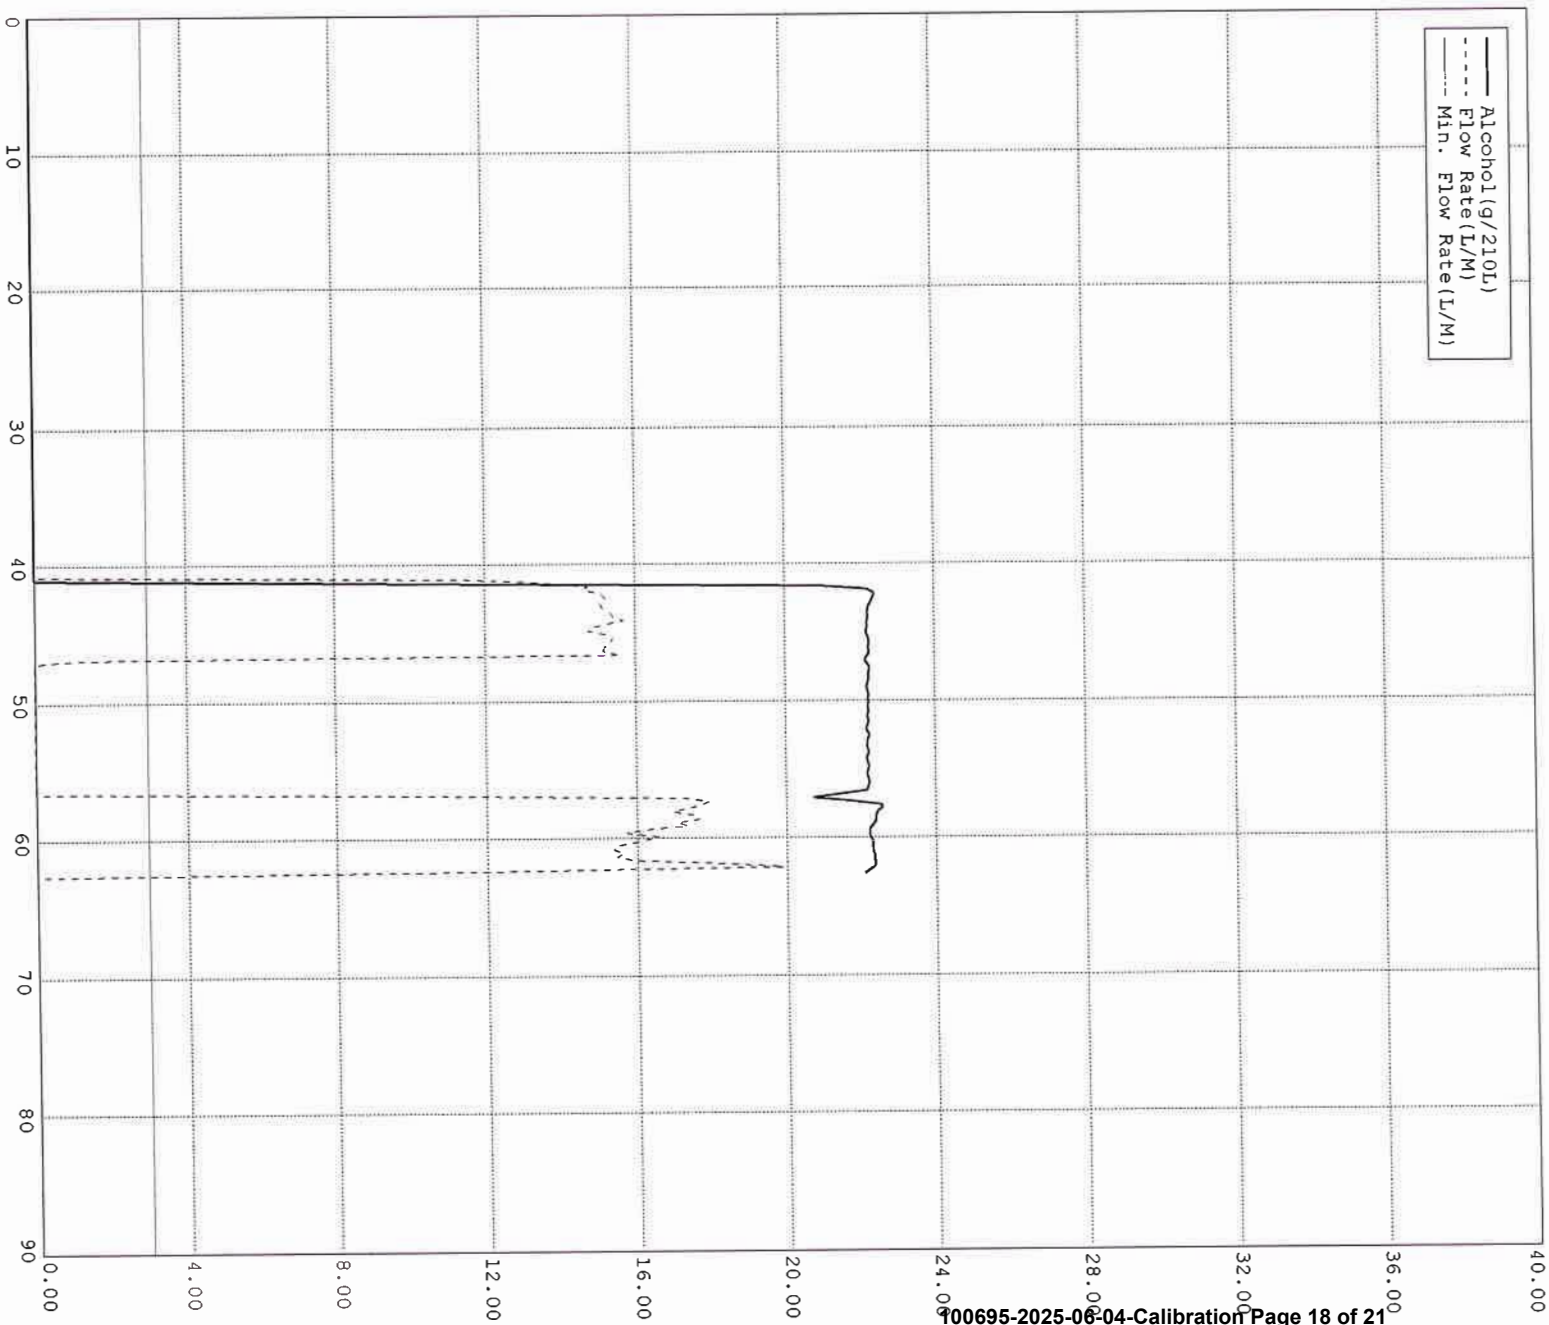

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100695

Date: 06/04/2025
Time: 12:35:02

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST	PASSED	12:36
INTERNAL STANDARD	0.000	12:36
Xq = 0.115 (0.93%)	VERIFIED	12:36
EXTERNAL STANDARD	0.077	12:36
X[1] = 0.0772 (-0.0004)	(0.0032)	
BLANK TEST	0.000	12:37
SUBJECT SAMPLE	XXX	12:38
X[1] = 0.1211 (-0.0214)	(0.0028)	

Interference Detected

KS

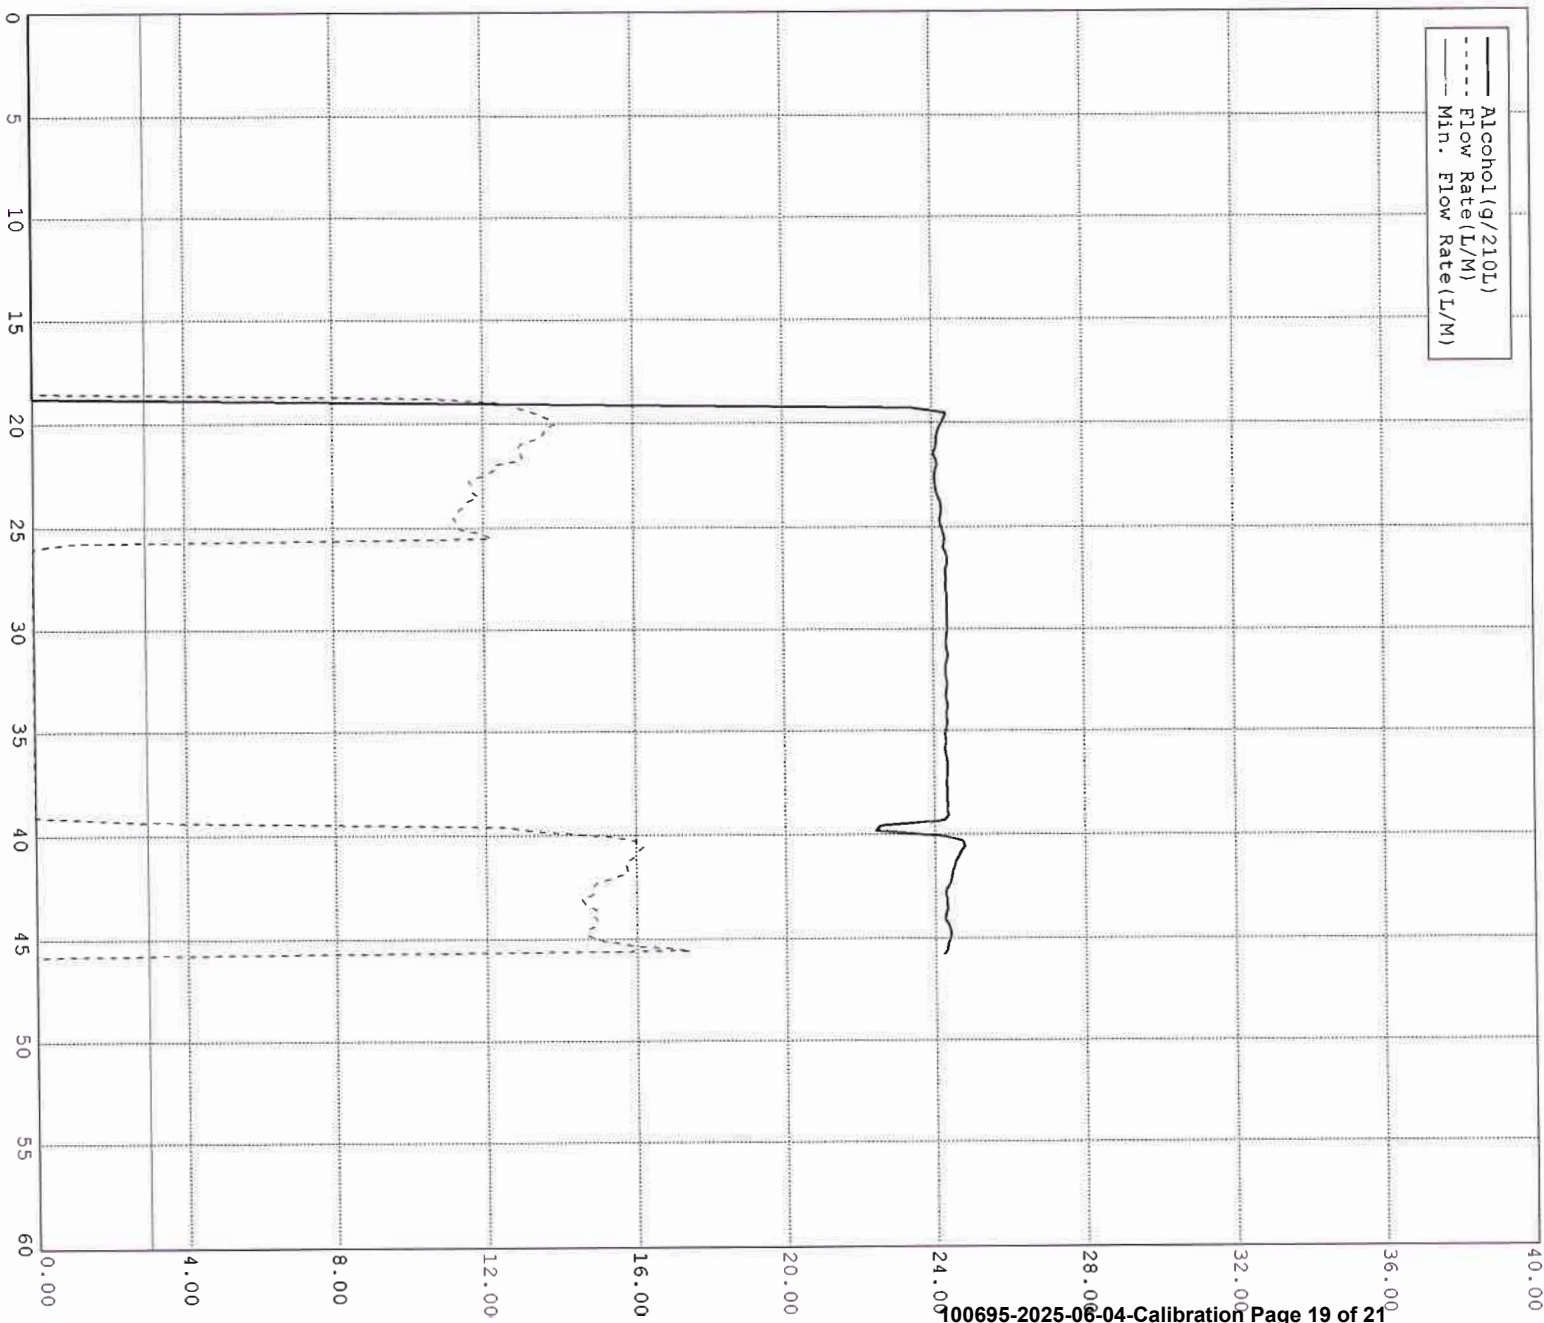

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 06/04/2025
Time: 12:52:31

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:54
BLANK TEST	0.000	12:54
INTERNAL STANDARD	VERIFIED	12:54
Xq = 0.114 (0.70%)		
EXTERNAL STANDARD	0.077	12:54
X[1] = 0.0768 (-0.0014)	(0.0033)	
BLANK TEST	0.000	12:55
SUBJECT SAMPLE (Vol=1.64L)	0.095	12:55
X[1] = 0.0950 (0.0007)	(0.0016)	
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.077	12:57
X[1] = 0.0772 (-0.0004)	(0.0026)	
BLANK TEST	0.000	12:58

Alcohol(g/210L)
---- Flow Rate(L/M)
---- Min. Flow Rate(L/M)

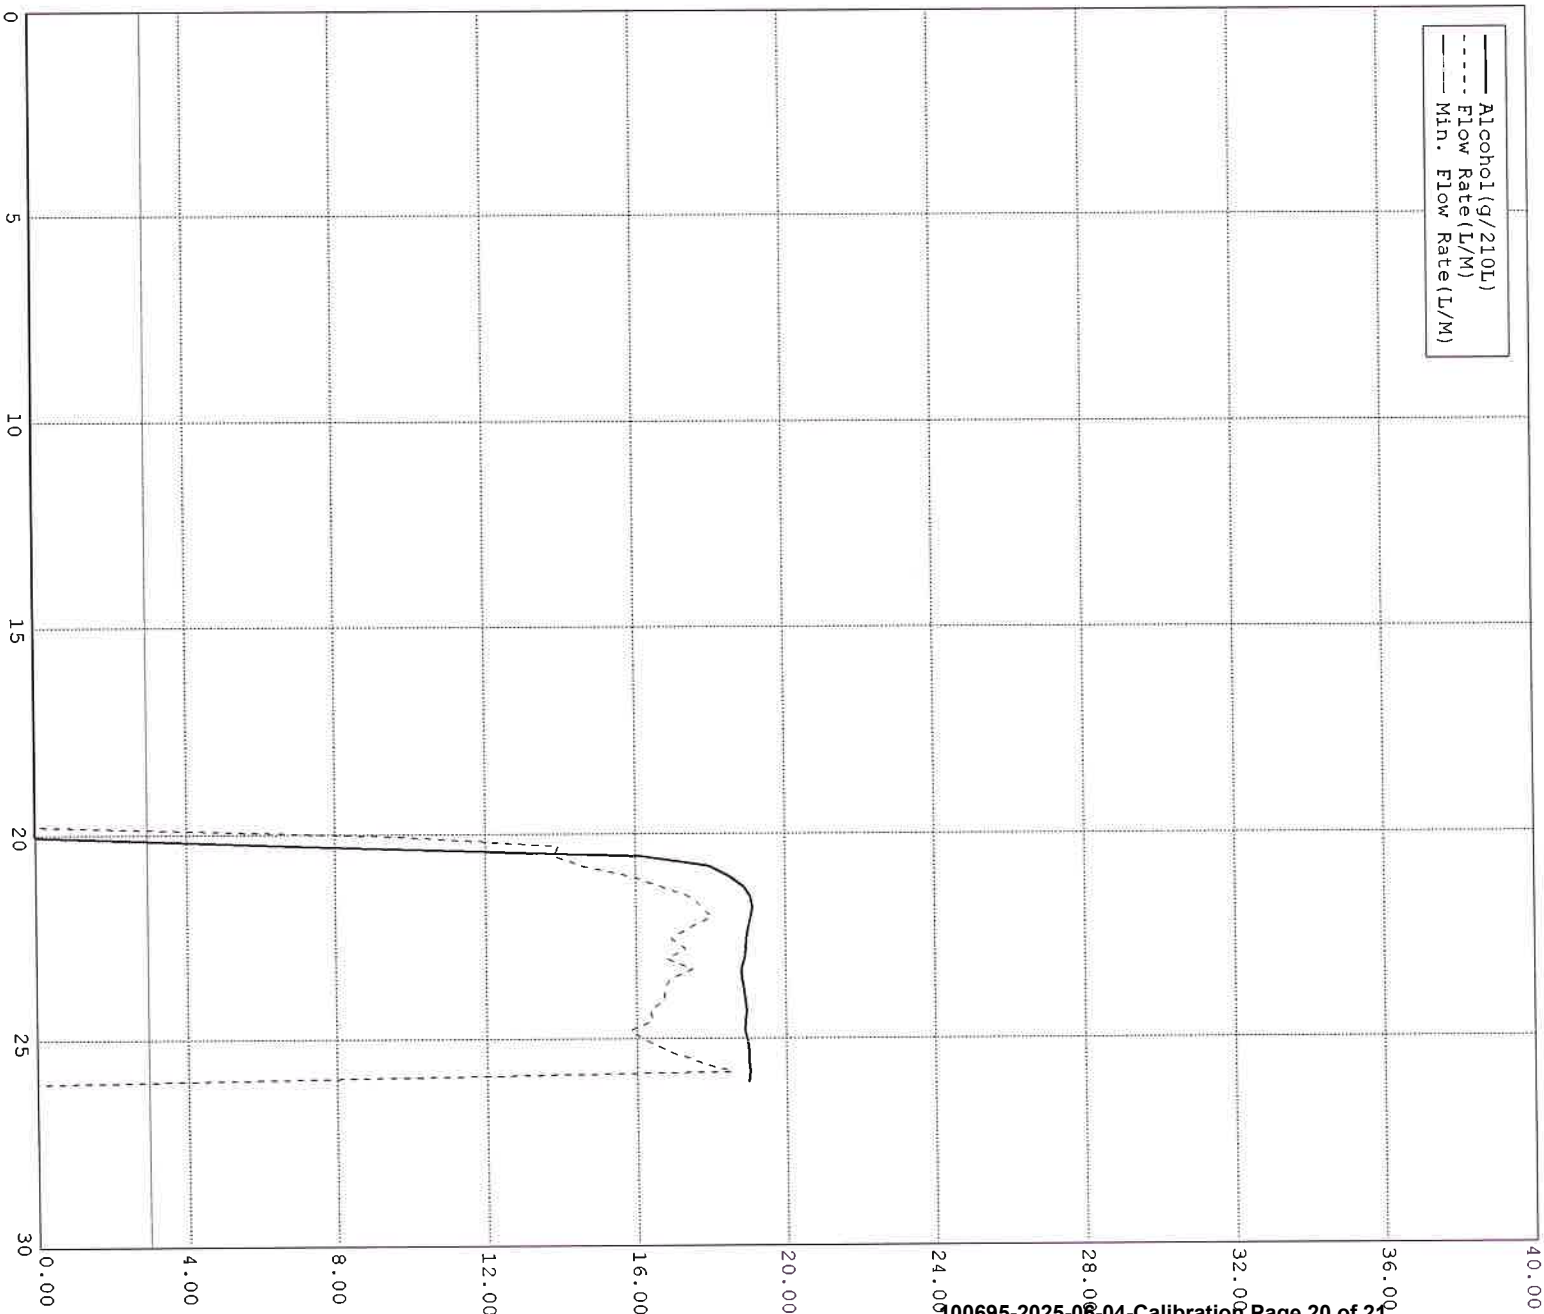

KS

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100695

Date: 06/04/2025
Time: 14:43:12

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON-DRINKING TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:45
BLANK TEST	0.000	14:45
INTERNAL STANDARD	VERIFIED	14:45
EXTERNAL STANDARD	0.078	14:45
BLANK TEST	0.000	14:46
SUBJECT SAMPLE (Vol=1.55L)	0.000	14:47
BLANK TEST	0.000	14:48
EXTERNAL STANDARD	0.078	14:48
BLANK TEST	0.000	14:49

KS

