




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100354

Report Issue Date: 06/26/2025
Date Received: 2025-03-25
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.021	0.021	0.019	0.020	0.020	0.020
0.080	0.080	AG335202	0.078	0.079	0.079	0.078	0.079	0.079
0.300	0.299	AG427706	0.294	0.294	0.294	0.294	0.294	0.294

As Found - Evaluation Analyst: Megan Carlock

As Found Conditions - Barometric Pressure (inHg): 29.79 Barometer Used: VWR S/N 240680771 Temperature (C): 22.7 Relative Humidity (%): 12

As-Found Lab Activity Date Range: 03/25/2025 - 03/25/2025

Replaced the O-ring. Instrument is recommended for repair because the PDF files for 4 tests are available on the physical instrument, but when the raw files are pulled the PDF files are not present.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.019	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG407908	0.039	0.039	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.079	AG335202	0.077	0.077	0.077	0.077	0.076	0.077	+/- 0.004
0.100	0.099	AG333401	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.149	AG332004	0.144	0.144	0.144	0.144	0.144	0.144	+/- 0.006
0.300	0.297	AG427706	0.291	0.292	0.291	0.292	0.292	0.292	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.64 Barometer Used: VWR S/N 240680771 Temperature (C): 22.0 Relative Humidity (%): 41

As-Left Lab Activity Date Range: 06/23/2025 - 06/24/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 06/26/2025

colleen.obryant@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 06/26/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100354 Analyst or Technician Name: C.O. Bryant
DataMaster DMT Calibration Start Date: 6/23/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 2406807#1
Calibration Due Date: 10 Sep 2026
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.64 Temperature(C) 22.0 Relative Humidity(%) 41
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)
- ☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20250603KS Expiration Date: 7/27/25
Simulator S/N: 501200 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250603KS Expiration Date: 9/13/25 COB 6/24/25
Simulator S/N: 501198 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 9/6/25 COB 2025.06.26
Simulator S/N: 501199 Thermometer Verification Performed? ☒ 2025.09.20

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 19 Sep 25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/24/25
Data Interpretation Date (Technician): NA (if applicable)
Data Interpretation Date (Analyst): 6/24/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100354

Date: 06/23/2025
Time: 14:04:03

VERSIONS

DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 48.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.80 V	PASSED
(0.95 V - 2.23 V)	
Cooler Voltage = 1.43 V	PASSED
(0.95 V - 2.21 V)	
Bias Voltage = 79 V	PASSED
(47 V - 111 V)	
Chopper Freq = 523 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.8 in	

PUMP INFO

Flow Rate = 4.612 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.002 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.097 1.93%	PASSED
(0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100354

Date: 06/23/2025

Time: 2:22 PM

Temperatures (°C)

Sample Cell: 48.9°C

Breath Tube: 47.7°C

Current Barometer 29.8 in

Volume (Ltr) 1.45

Settings

Lamp: 1.80 V

Bias: 79 V

Cooler: 1.48 V

Chopper: 523 Hz

Voltages (V)

Flow: 1.05 V

Detector: -0.052 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100354

Date: 09/27/2011
Time: 13:04:23

OPERATOR NAME:
COLLEEN S OBRYANT
CERTIFICATE #: 6237

LOT #: GUTH100
BOTTLE #: 11050
EXPIRATION: 04/06/2013

Ca	=	0.1000		
CAL	=	0.969216	0.800 <=	CAL < 1.200
b1	=	0.0001	0.0000 <=	b1 < 0.0040
b2	=	0.0049	0.0010 <=	b2 < 0.0100
b3	=	0.0001	0.0000 <=	b3 < 0.0040
Xq	=	0.0953	0.0500 <=	Xq < 0.2000
a21	=	1.175978	1.050 <=	a21 < 1.300
a31	=	0.450287	0.300 <=	a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100354

Date: 06/24/2025
Time: 08:45:25


SUBJECT NAME:
TEST TEST
LICENSE #: VOLUME TEST

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:46
BLANK TEST	0.000	08:46
INTERNAL STANDARD	VERIFIED	08:46
EXTERNAL STANDARD	0.076	08:46
BLANK TEST	0.000	08:47
SUBJECT SAMPLE (Vol=1.59L)	0.000	08:48
BLANK TEST	0.000	08:49
EXTERNAL STANDARD	0.077	08:50
BLANK TEST	0.000	08:50

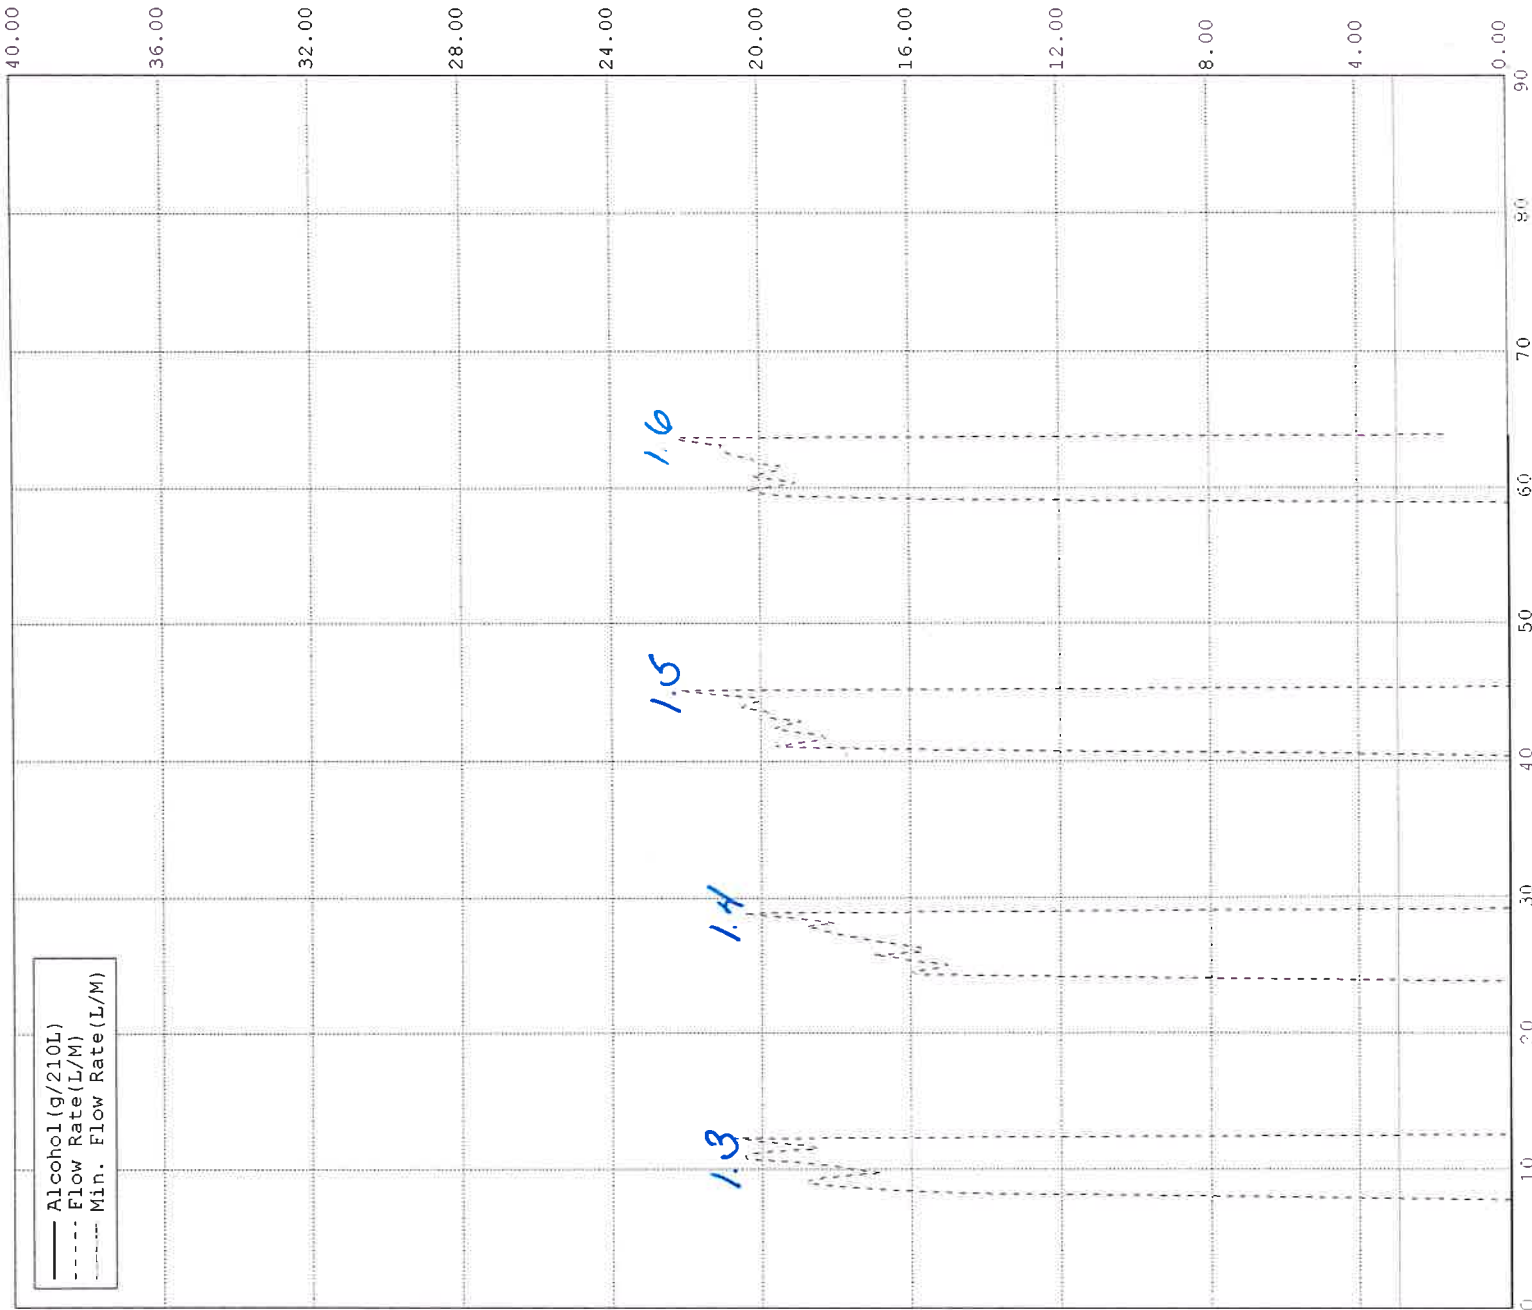

LINEARITY CHECK


Alaska Department of Public Safety
 DATA MASTER dmt: 100354

Date: 06/24/2025
 Time: 08:52:42

SUPERVISOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0198	0.0004
0.040	0.0390	0.0000
0.079	0.0768	0.0004
0.099	0.0980	0.0000
0.149	0.1440	0.0000
0.297	0.2916	0.0005
SLOPE	= 0.980617	
R ²	= 0.999885	

CC

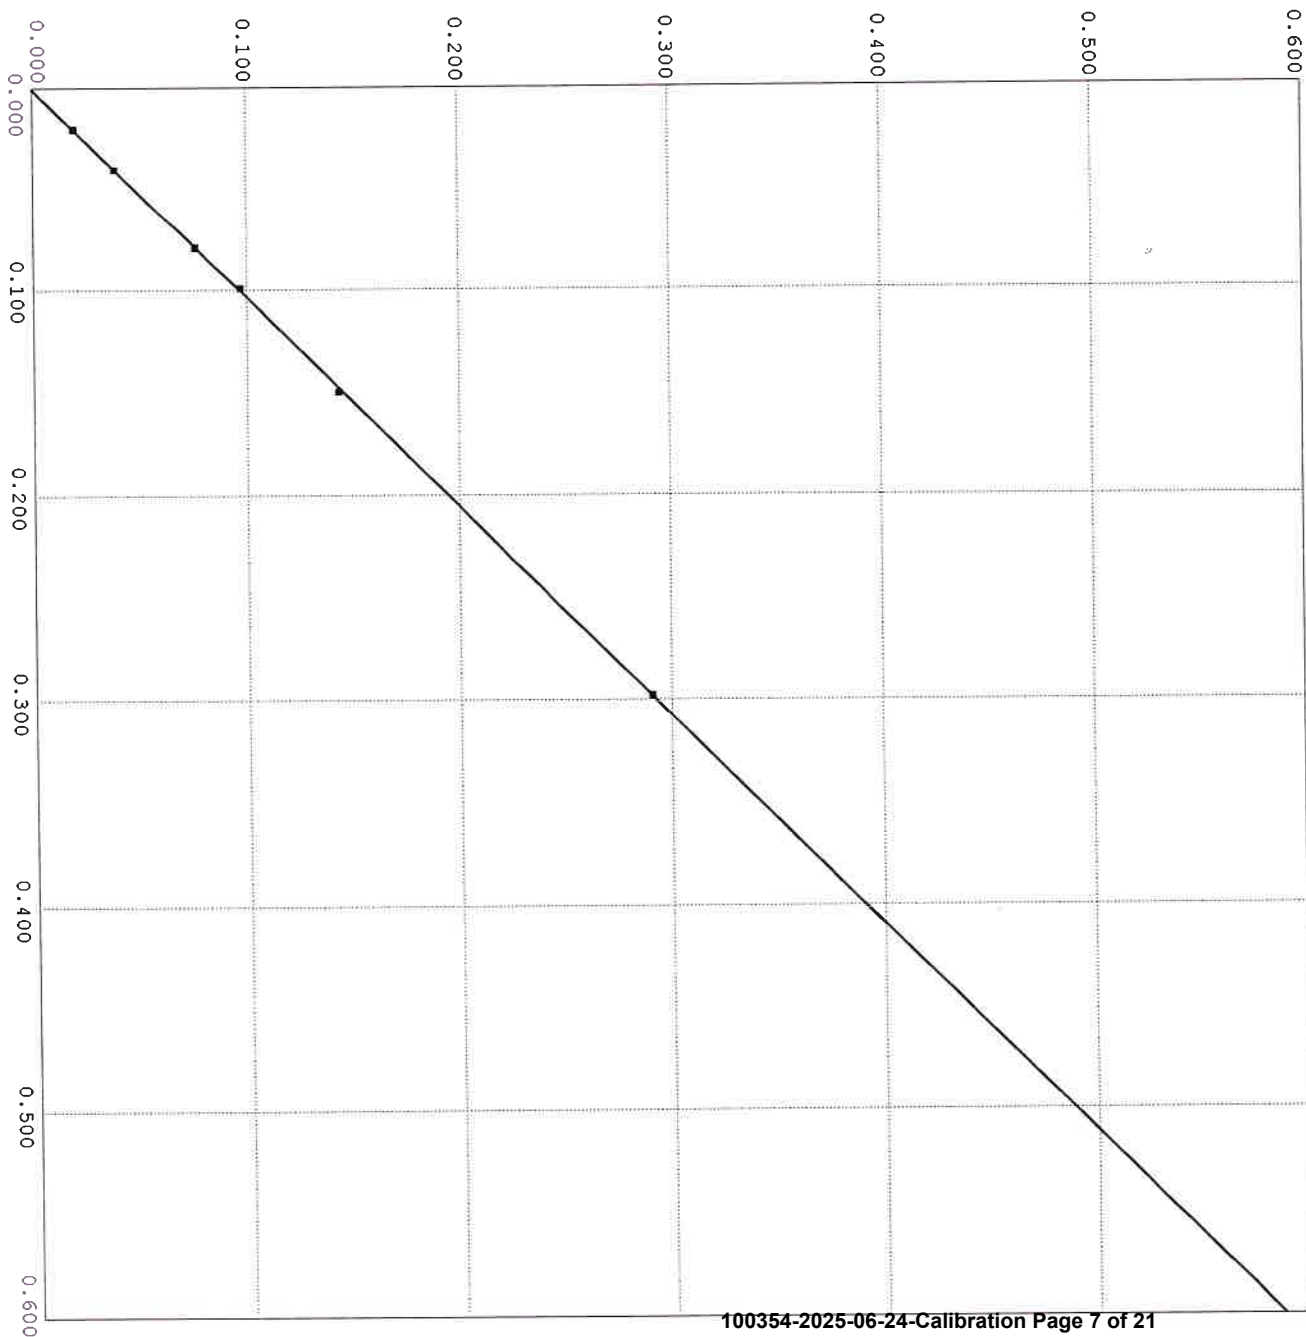

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100354






Date: 06/24/2025
Time: 08:52:44

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.64: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 723 psi

BLANK TEST	0.000	08:53
INTERNAL STANDARD	VERIFIED	08:54
EXTERNAL STANDARD	0.020	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.019	08:55
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.020	08:56
BLANK TEST	0.000	08:57
EXTERNAL STANDARD	0.020	08:57
BLANK TEST	0.000	08:58
EXTERNAL STANDARD	0.020	08:58
BLANK TEST	0.000	08:59

Average = 0.0198
Std Dev = 0.0004

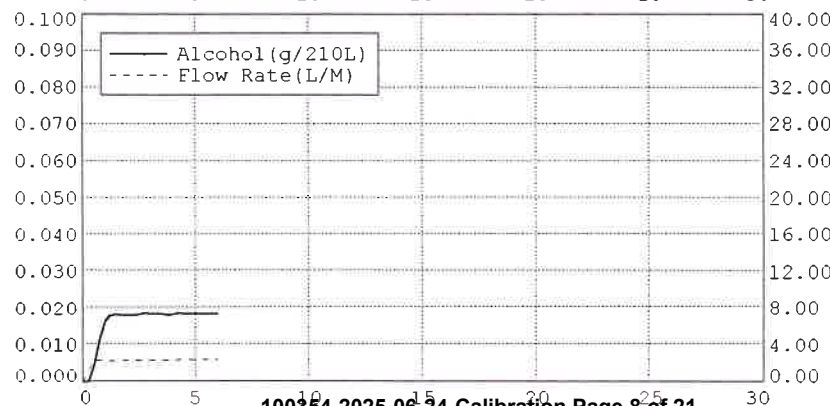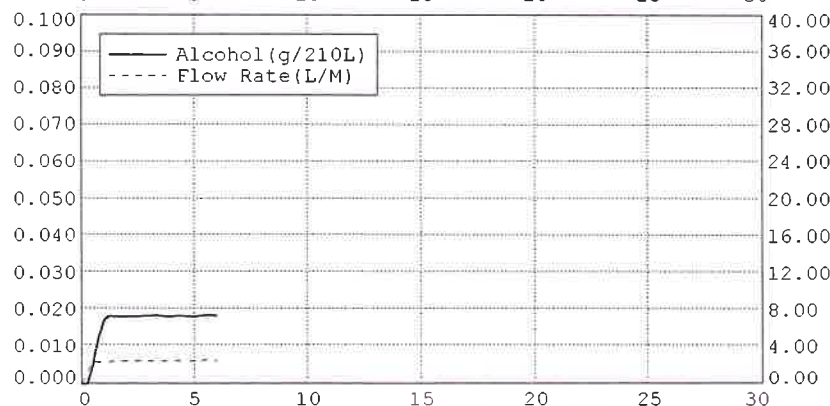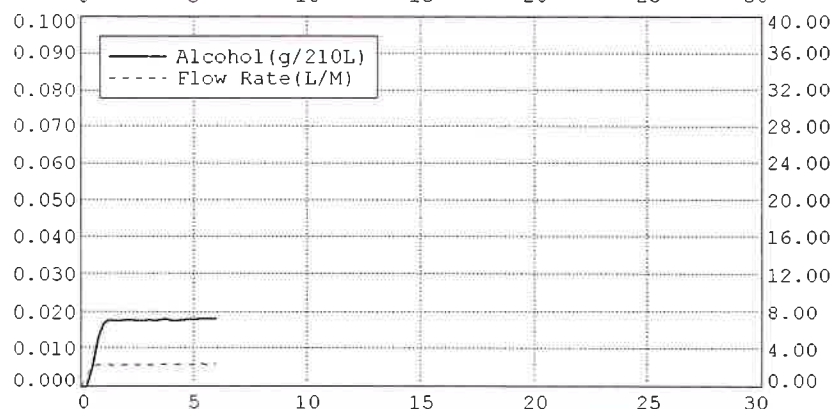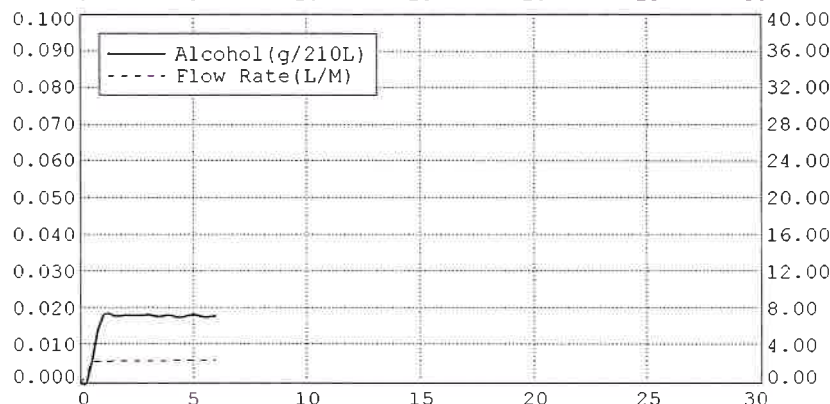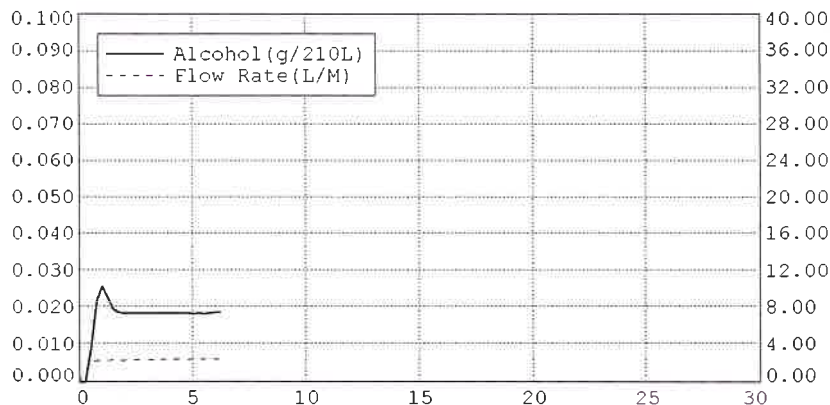

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100354






Date: 06/24/2025
Time: 09:00:02

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.64: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 1027 psi

BLANK TEST	0.000	09:01
INTERNAL STANDARD	VERIFIED	09:01
EXTERNAL STANDARD	0.039	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.039	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.039	09:03
BLANK TEST	0.000	09:04
EXTERNAL STANDARD	0.039	09:05
BLANK TEST	0.000	09:05
EXTERNAL STANDARD	0.039	09:06
BLANK TEST	0.000	09:07

Average = 0.0390
Std Dev = 0.0000

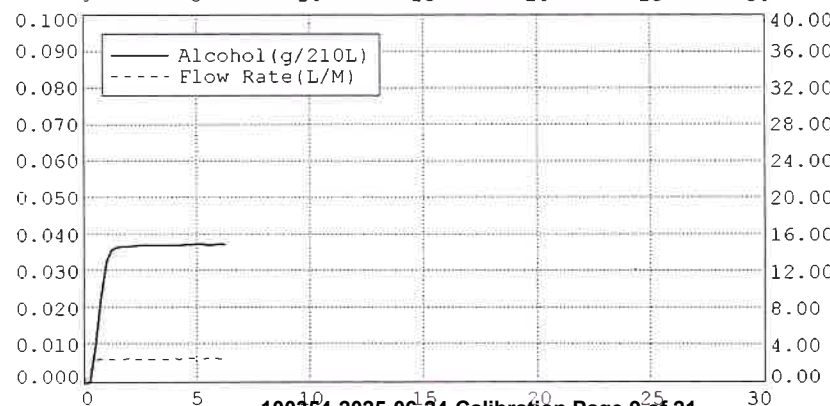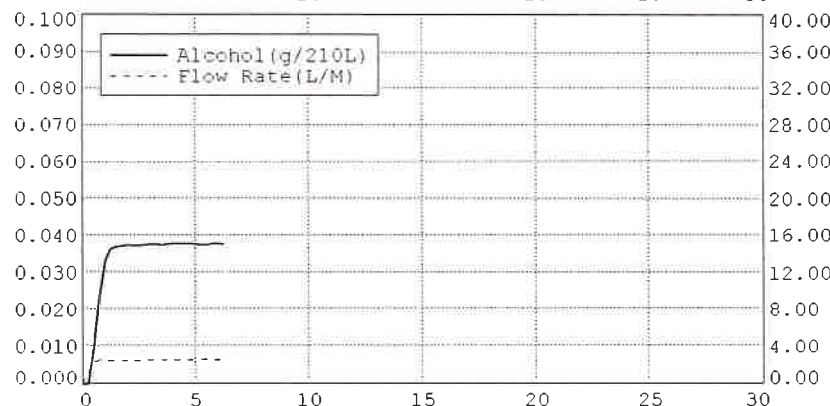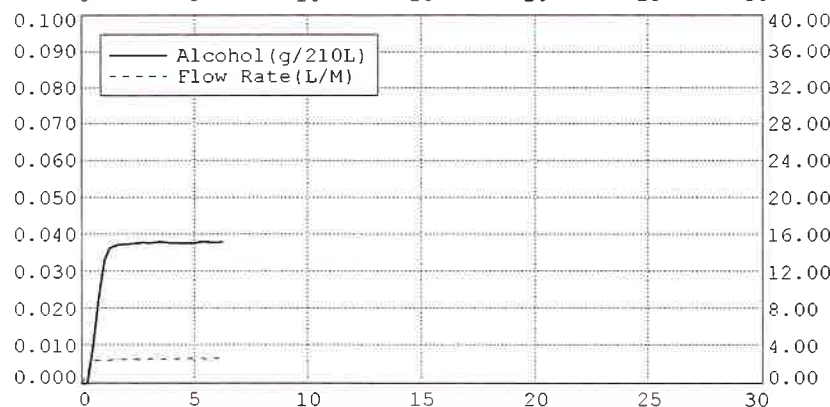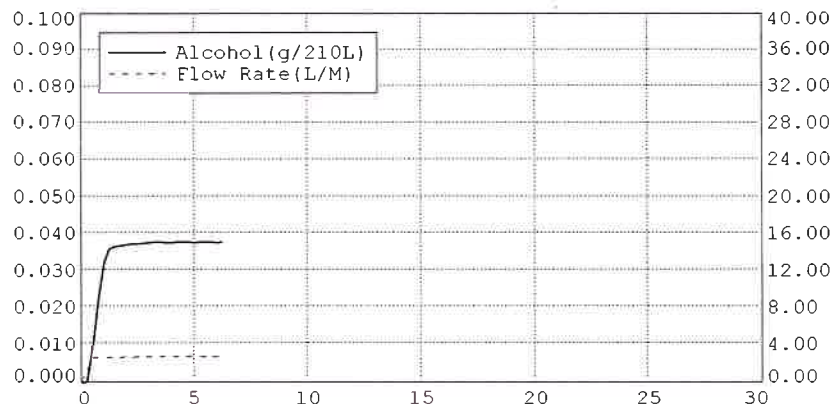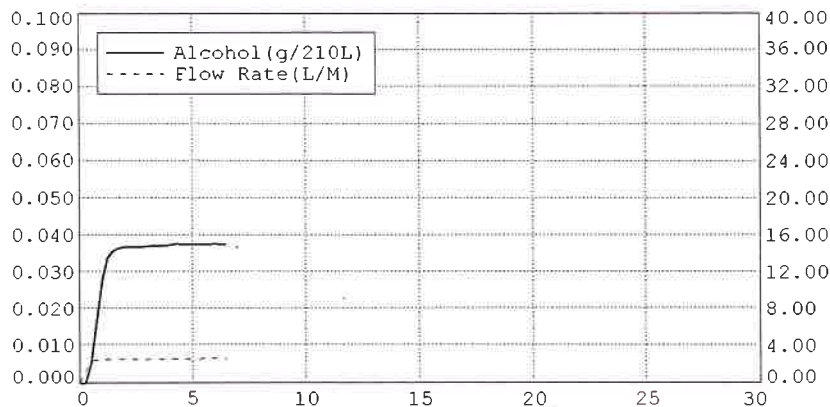

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100354






Date: 06/24/2025
Time: 09:07:48

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 498 psi

BLANK TEST	0.000	09:09
INTERNAL STANDARD	VERIFIED	09:09
EXTERNAL STANDARD	0.077	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.077	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.077	09:11
BLANK TEST	0.000	09:12
EXTERNAL STANDARD	0.077	09:12
BLANK TEST	0.000	09:13
EXTERNAL STANDARD	0.076	09:13
BLANK TEST	0.000	09:14

Average = 0.0768
Std Dev = 0.0004

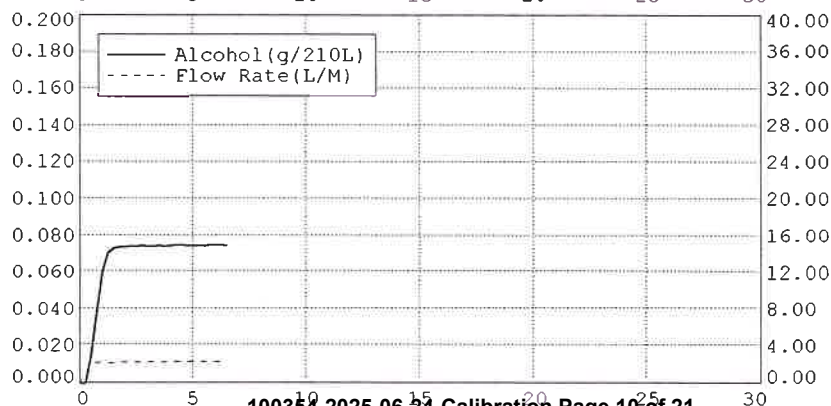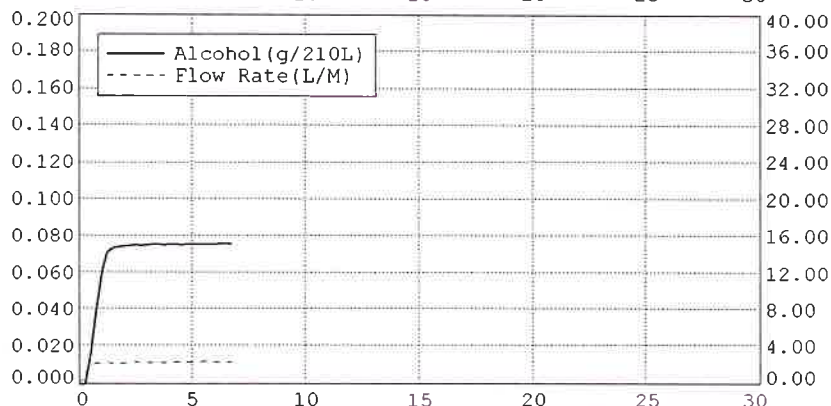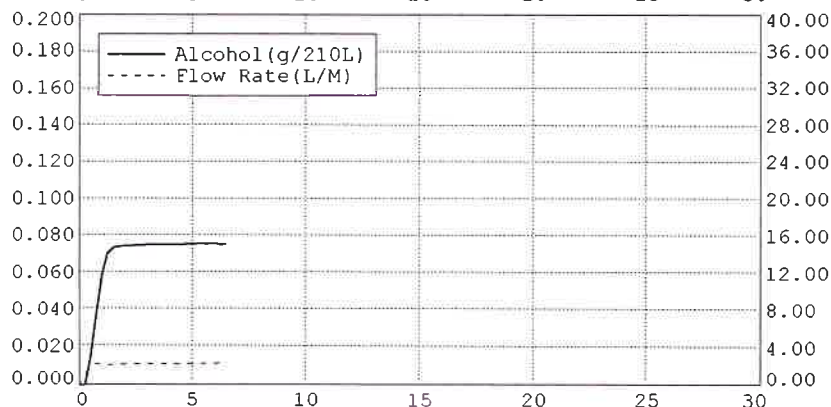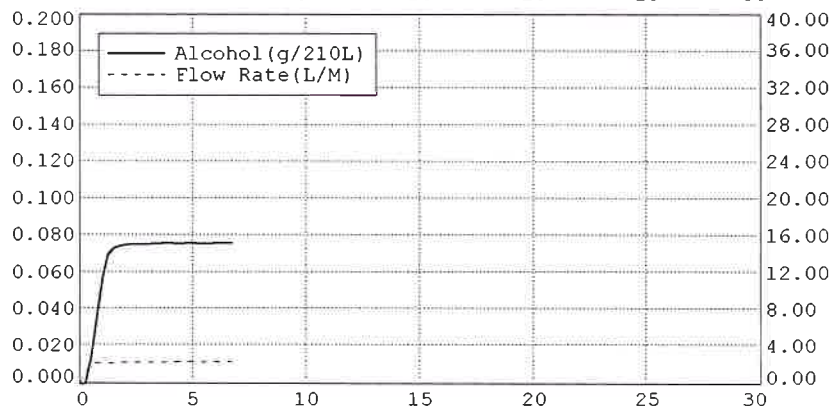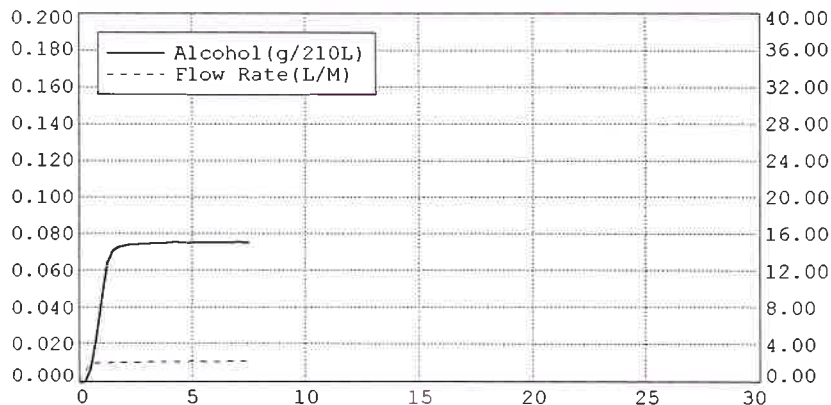

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100354






Date: 06/24/2025
Time: 09:22:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.64: 0.099
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 963 psi

BLANK TEST	0.000	09:23
INTERNAL STANDARD	VERIFIED	09:23
EXTERNAL STANDARD	0.098	09:23
BLANK TEST	0.000	09:24
EXTERNAL STANDARD	0.098	09:24
BLANK TEST	0.000	09:25
EXTERNAL STANDARD	0.098	09:25
BLANK TEST	0.000	09:26
EXTERNAL STANDARD	0.098	09:27
BLANK TEST	0.000	09:27
EXTERNAL STANDARD	0.098	09:28
BLANK TEST	0.000	09:29

Average = 0.0980
Std Dev = 0.0000

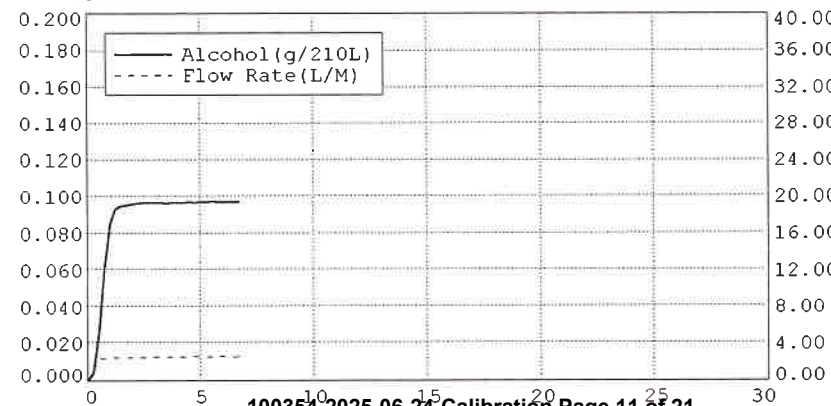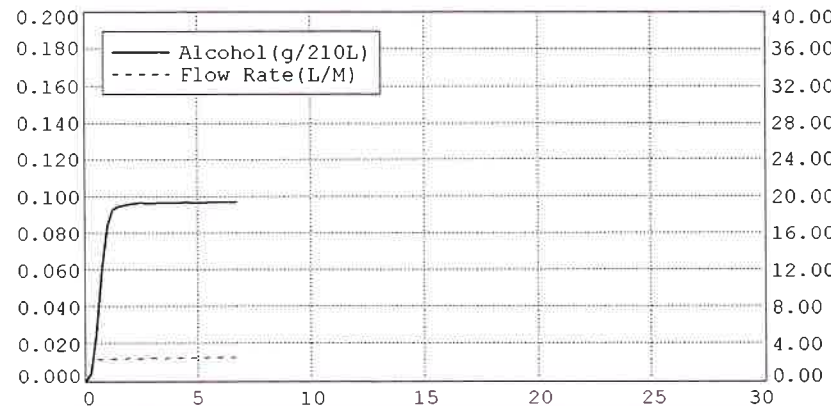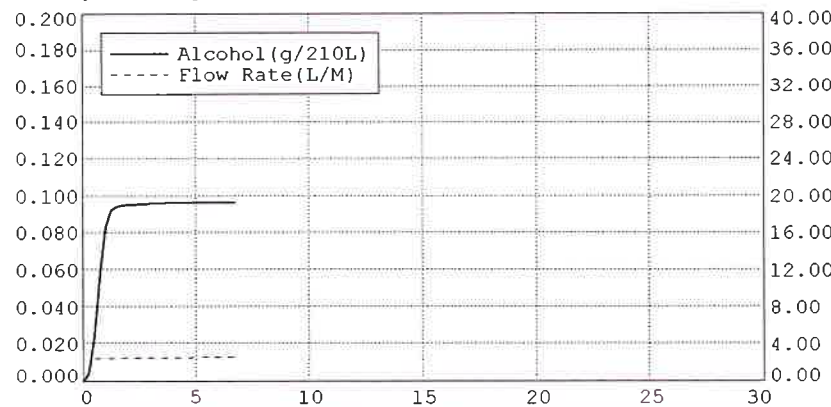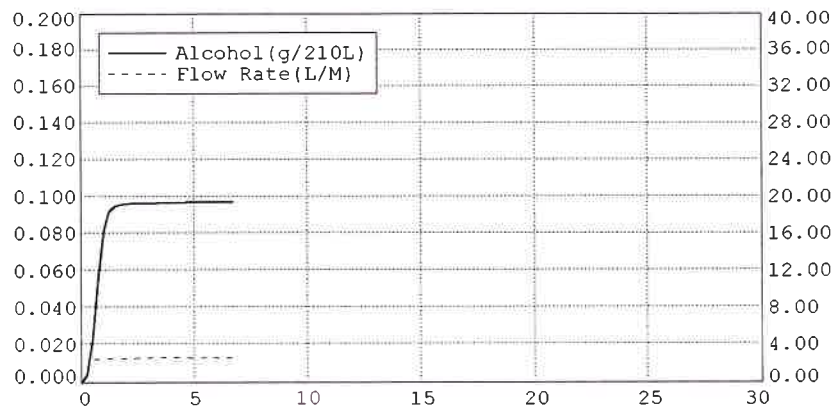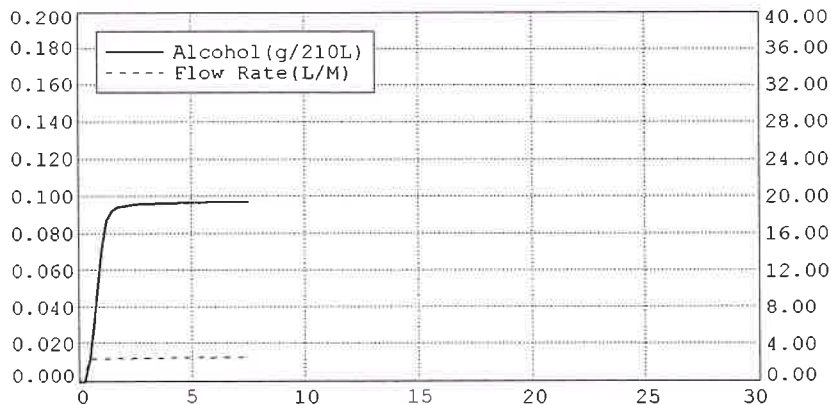

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100354






Date: 06/24/2025
Time: 09:30:25

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.64: 0.149
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 202 psi

BLANK TEST	0.000	09:32
INTERNAL STANDARD	VERIFIED	09:32
EXTERNAL STANDARD	0.144	09:32
BLANK TEST	0.000	09:33
EXTERNAL STANDARD	0.144	09:33
BLANK TEST	0.000	09:34
EXTERNAL STANDARD	0.144	09:34
BLANK TEST	0.000	09:35
EXTERNAL STANDARD	0.144	09:36
BLANK TEST	0.000	09:36
EXTERNAL STANDARD	0.144	09:37
BLANK TEST	0.000	09:38

Average = 0.1440
Std Dev = 0.0000

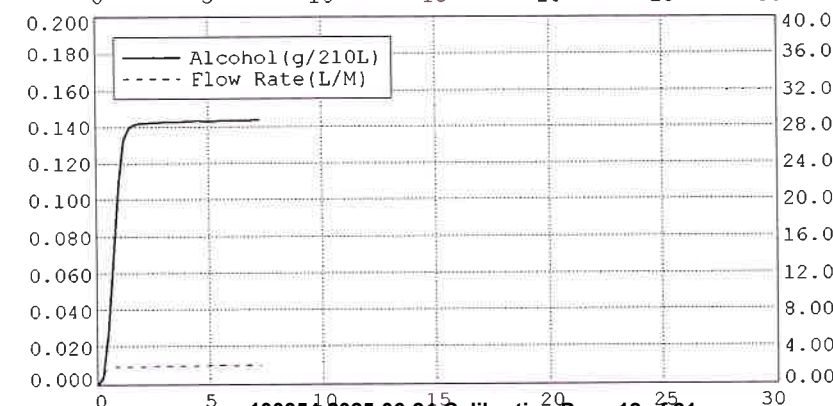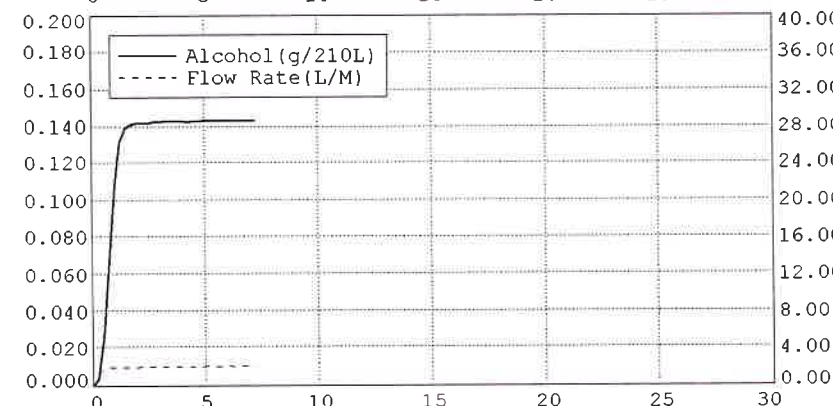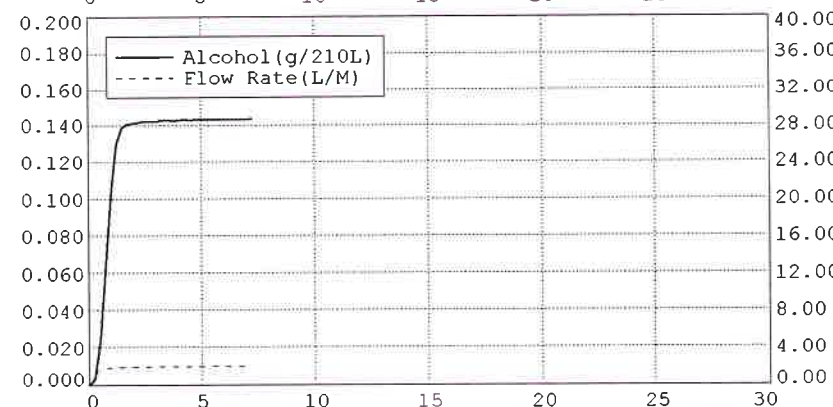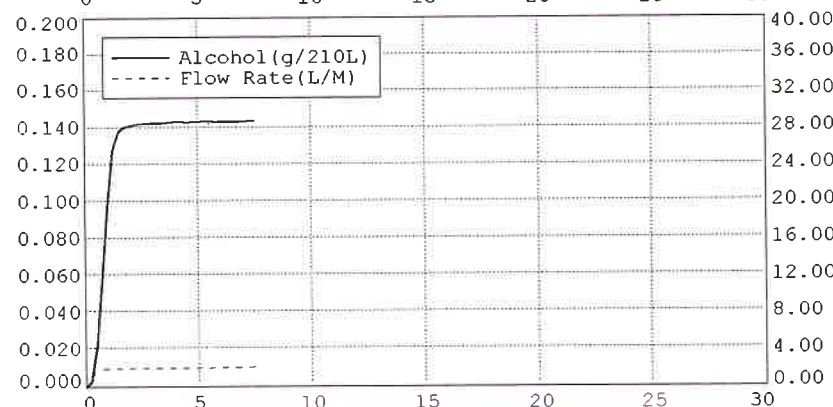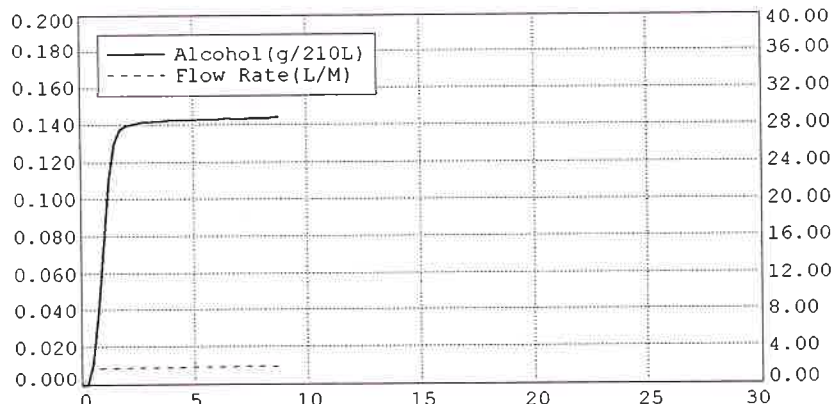

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100354






Date: 06/24/2025
Time: 09:53:19

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.64: 0.297
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 276 psi

BLANK TEST	0.000	09:54
INTERNAL STANDARD	VERIFIED	09:54
EXTERNAL STANDARD	0.291	09:55
BLANK TEST	0.000	09:55
EXTERNAL STANDARD	0.292	09:56
BLANK TEST	0.000	09:57
EXTERNAL STANDARD	0.291	09:57
BLANK TEST	0.000	09:58
EXTERNAL STANDARD	0.292	09:58
BLANK TEST	0.000	09:59
EXTERNAL STANDARD	0.292	09:59
BLANK TEST	0.000	10:00

Average = 0.2916
Std Dev = 0.0005

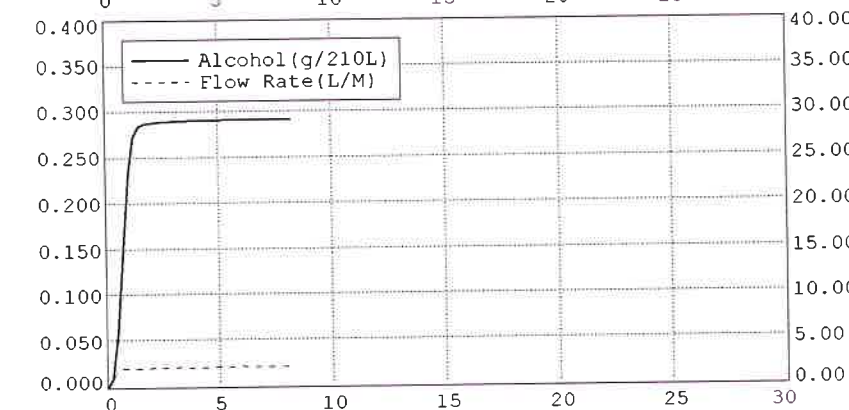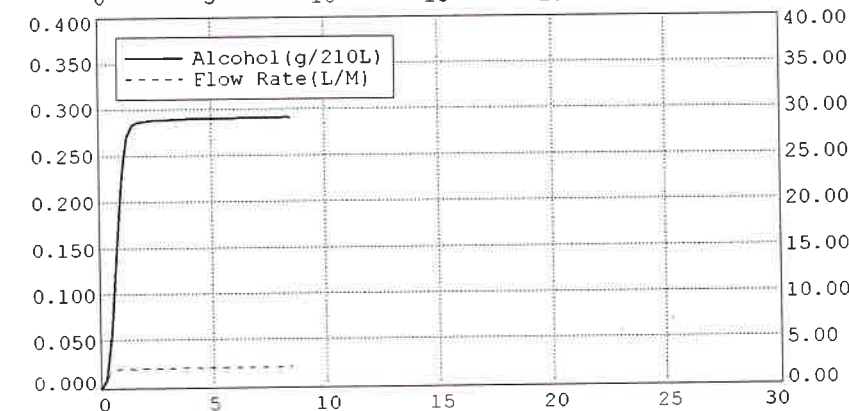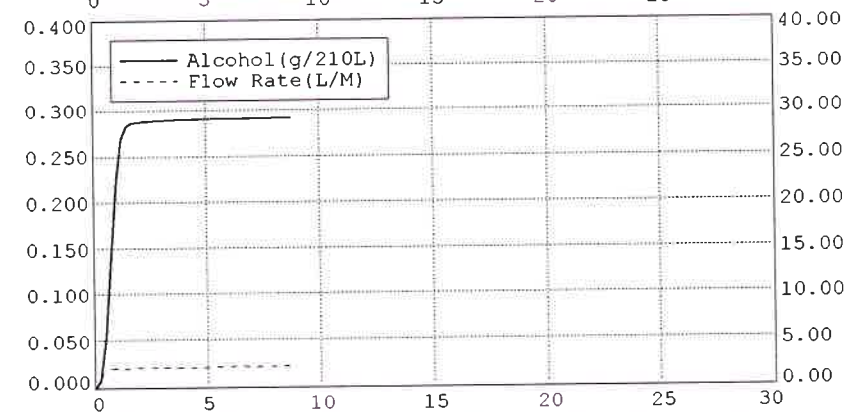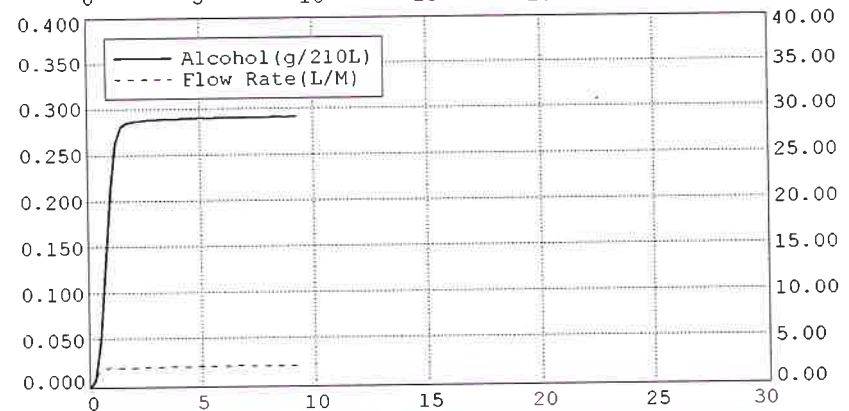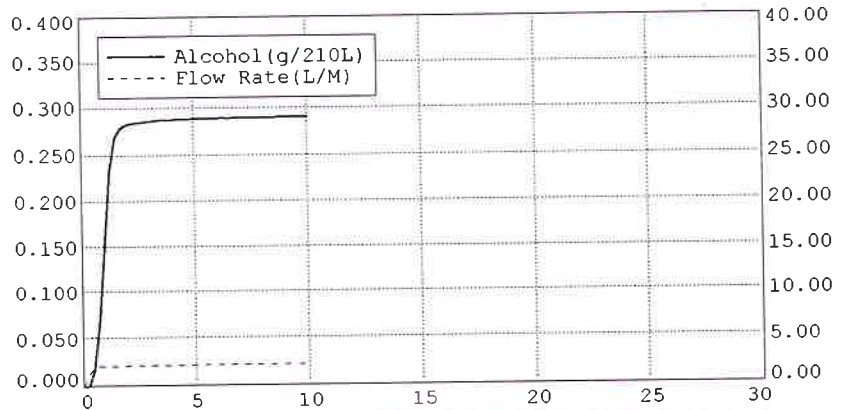

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100354

Date: 06/24/2025
Time: 12:04:18

SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE


OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:05
BLANK TEST	0.000	12:05
INTERNAL STANDARD	VERIFIED	12:05
EXTERNAL STANDARD	0.076	12:05
BLANK TEST	0.000	12:06
SUBJECT SAMPLE	INCOMPLETE	12:08

CS

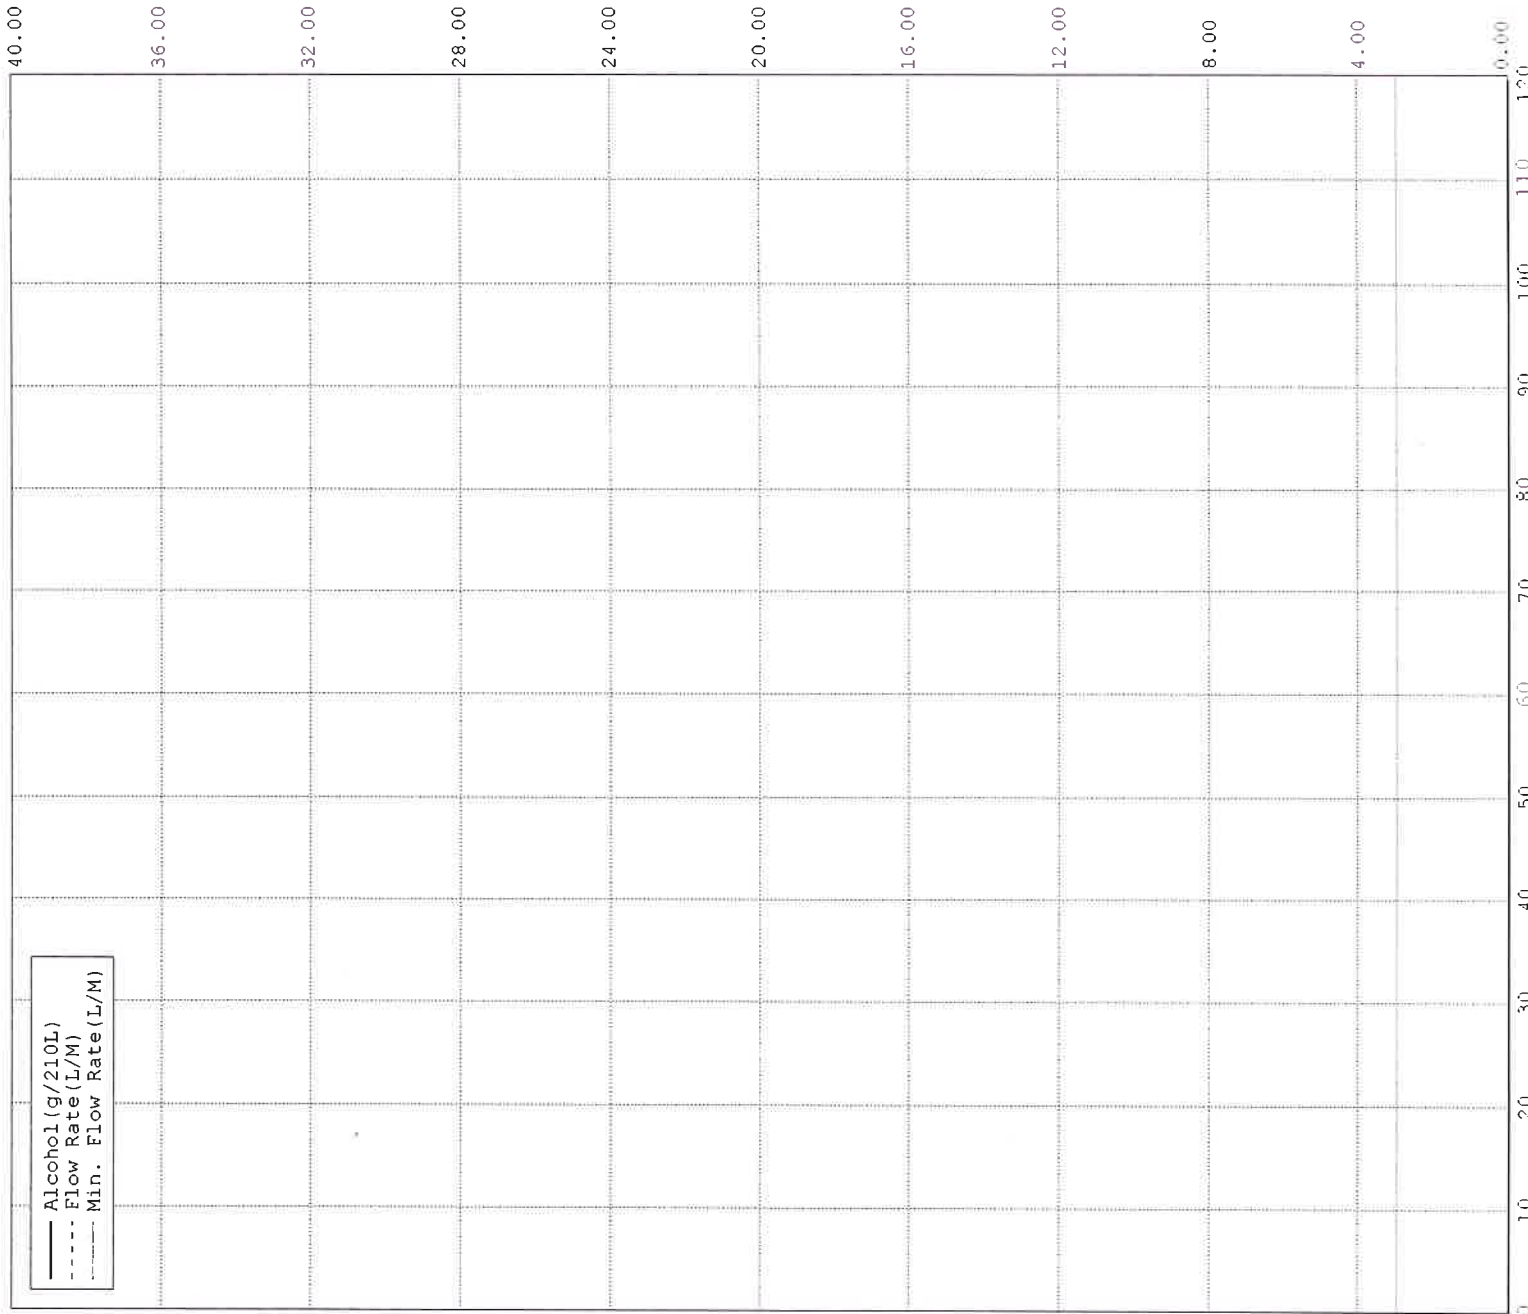

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100354

Date: 06/24/2025

Time: 12:11:22

SUBJECT NAME:

TEST TEST

LICENSE #: MAX ATTEMPTS

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 25-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.64: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD


BLANK TEST

SUBJECT SAMPLE

PASSED 12:12
0.000 12:12
VERIFIED 12:12
0.077 12:12
0.000 12:13
XXX 12:14

Maximum Attempts Exceeded

OK

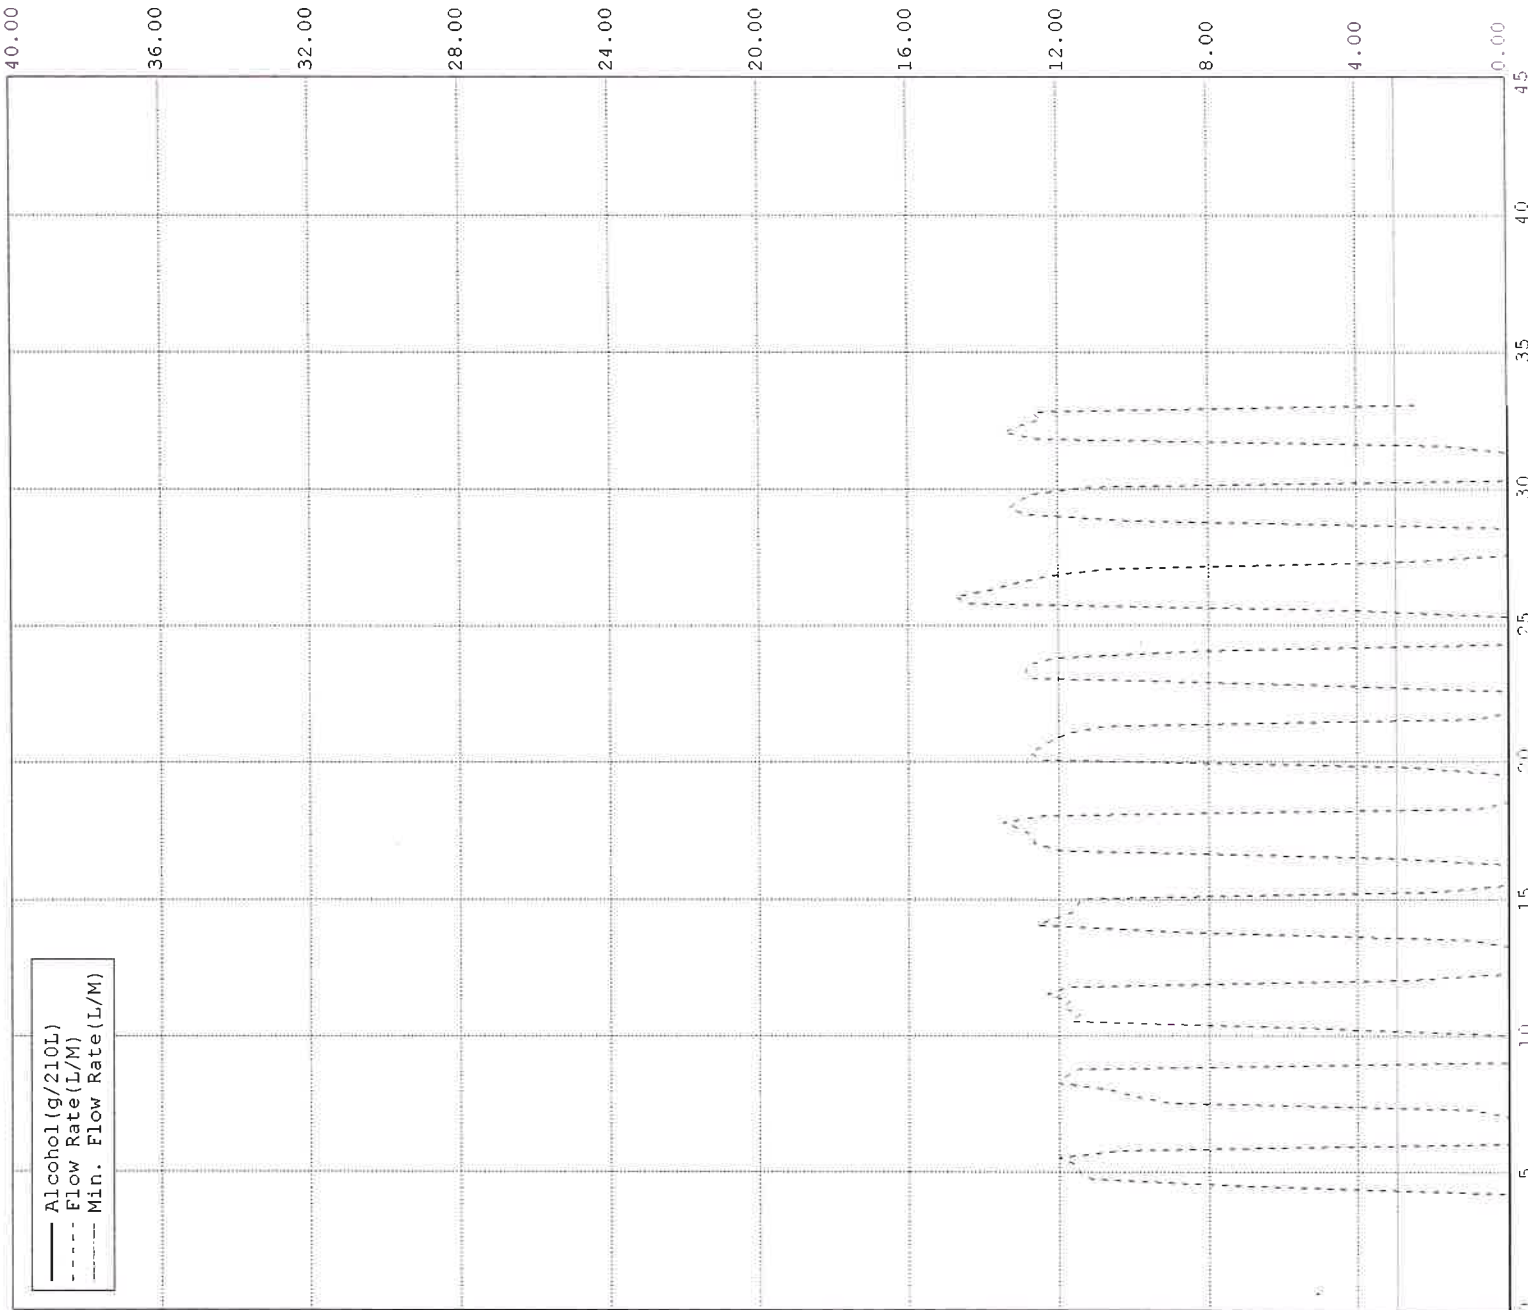

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100354

Date: 06/24/2025

Time: 12:16:12

SUBJECT NAME:

TEST TEST

LICENSE #: INVALID

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 25-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.63: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD


EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 12:17
0.000 12:17
VERIFIED 12:17
0.076 12:17
0.000 12:18
INVALID 12:18

2025

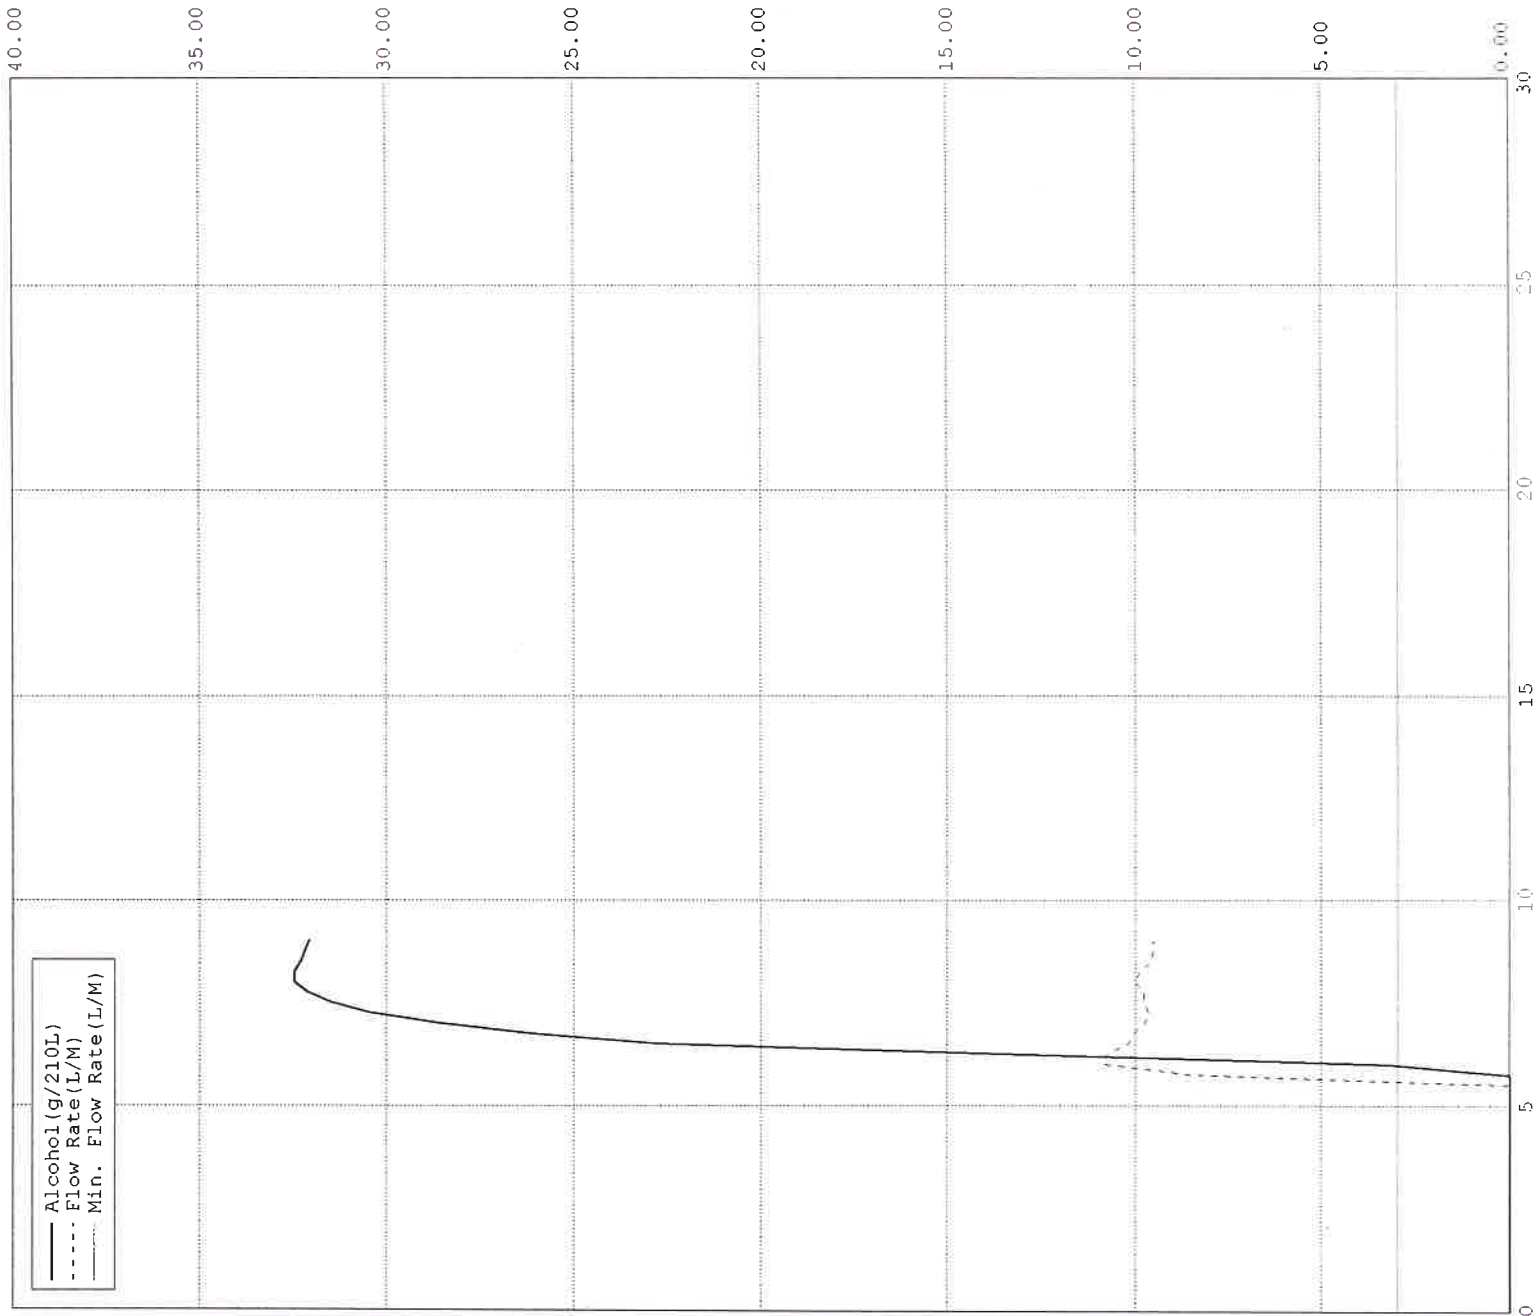

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100354

Date: 06/24/2025
Time: 12:20:42

SUBJECT NAME:
TEST TEST
LICENSE #: RFI

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.62: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 12:22
INTERNAL STANDARD VERIFIED 12:22
EXTERNAL STANDARD 0.076 12:23
BLANK TEST 0.000 12:24

RFI DETECTED

CAL

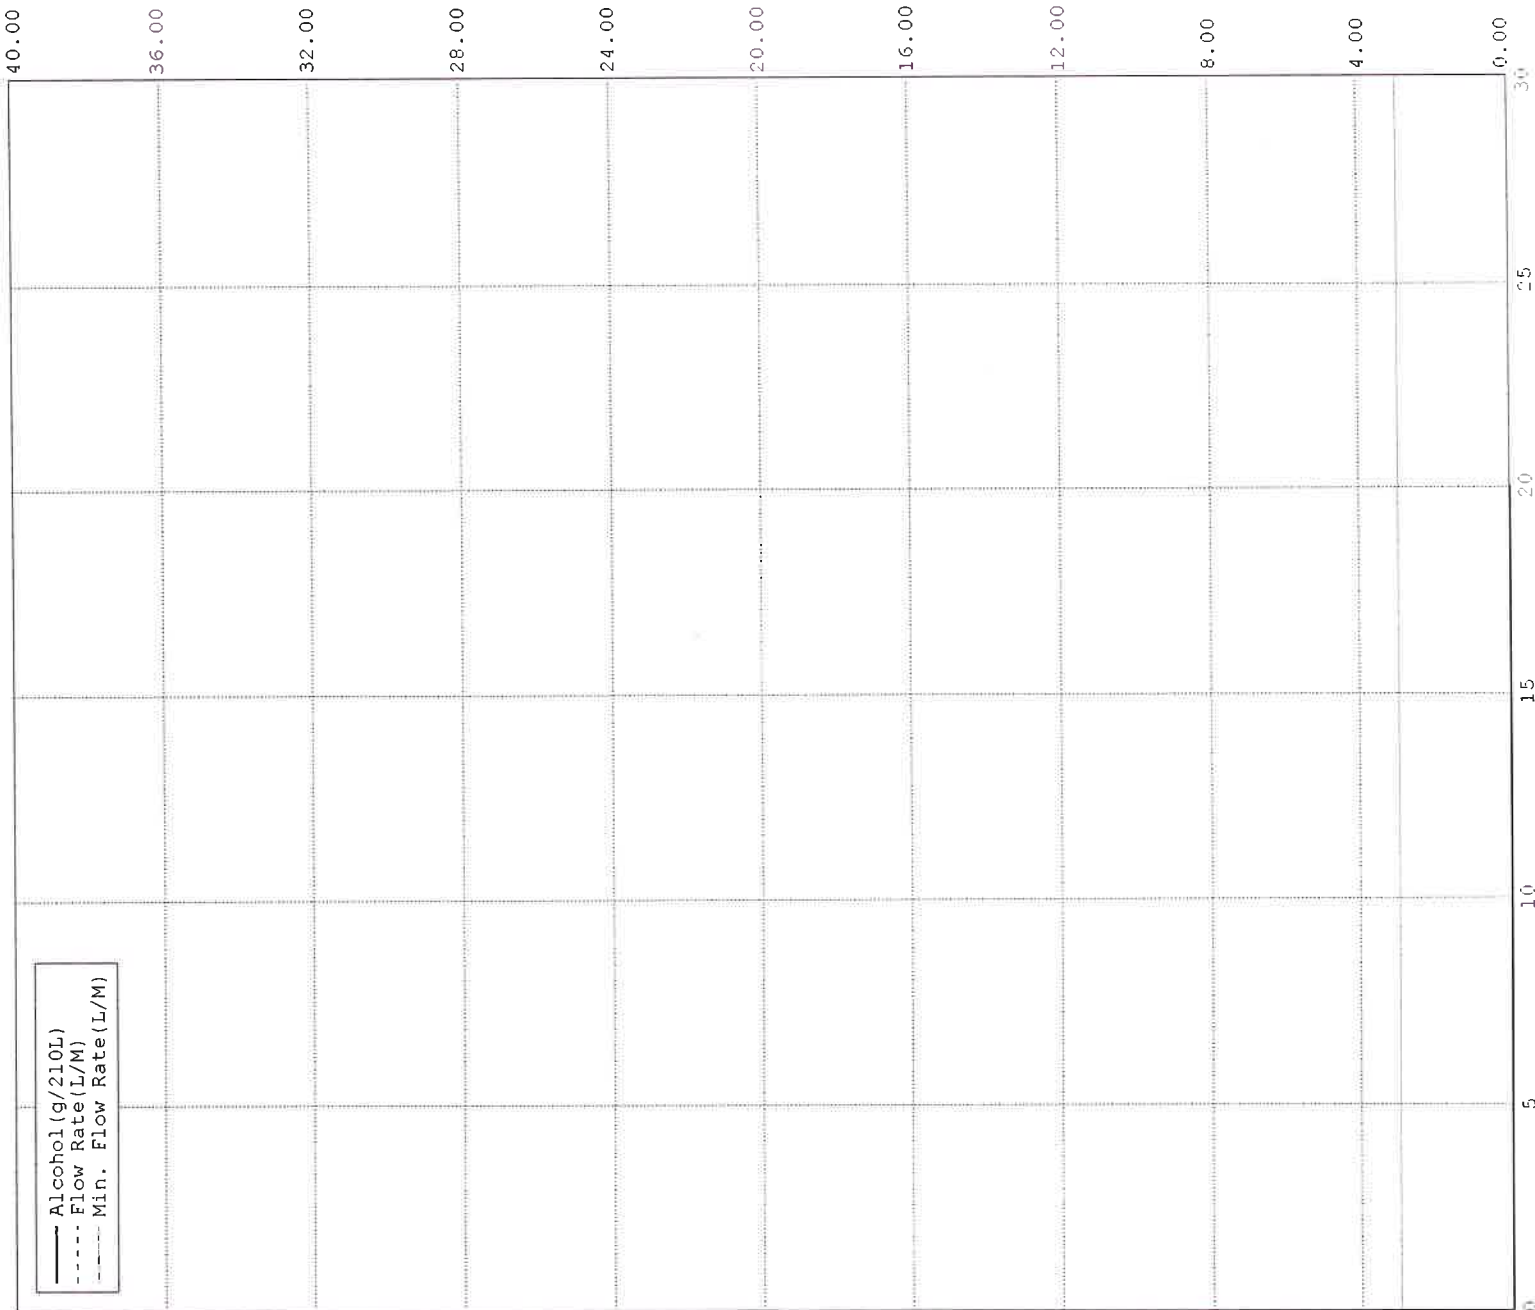

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100354

Date: 06/24/2025
 Time: 12:27:10

SUBJECT NAME:
 TEST TEST
 LICENSE #: INT-ACETONE


OPERATOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 25-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.63: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:30
BLANK TEST	0.000	12:30
INTERNAL STANDARD	VERIFIED	12:30
Xg = 0.097 (1.84%)		
EXTERNAL STANDARD	0.076	12:30
X[1] = 0.0764 (-0.0007)	(0.0026)	
BLANK TEST	0.000	12:31
SUBJECT SAMPLE	xxx	12:32
X[1] = 0.1094 (-0.0181)	(0.0010)	

Interference Detected

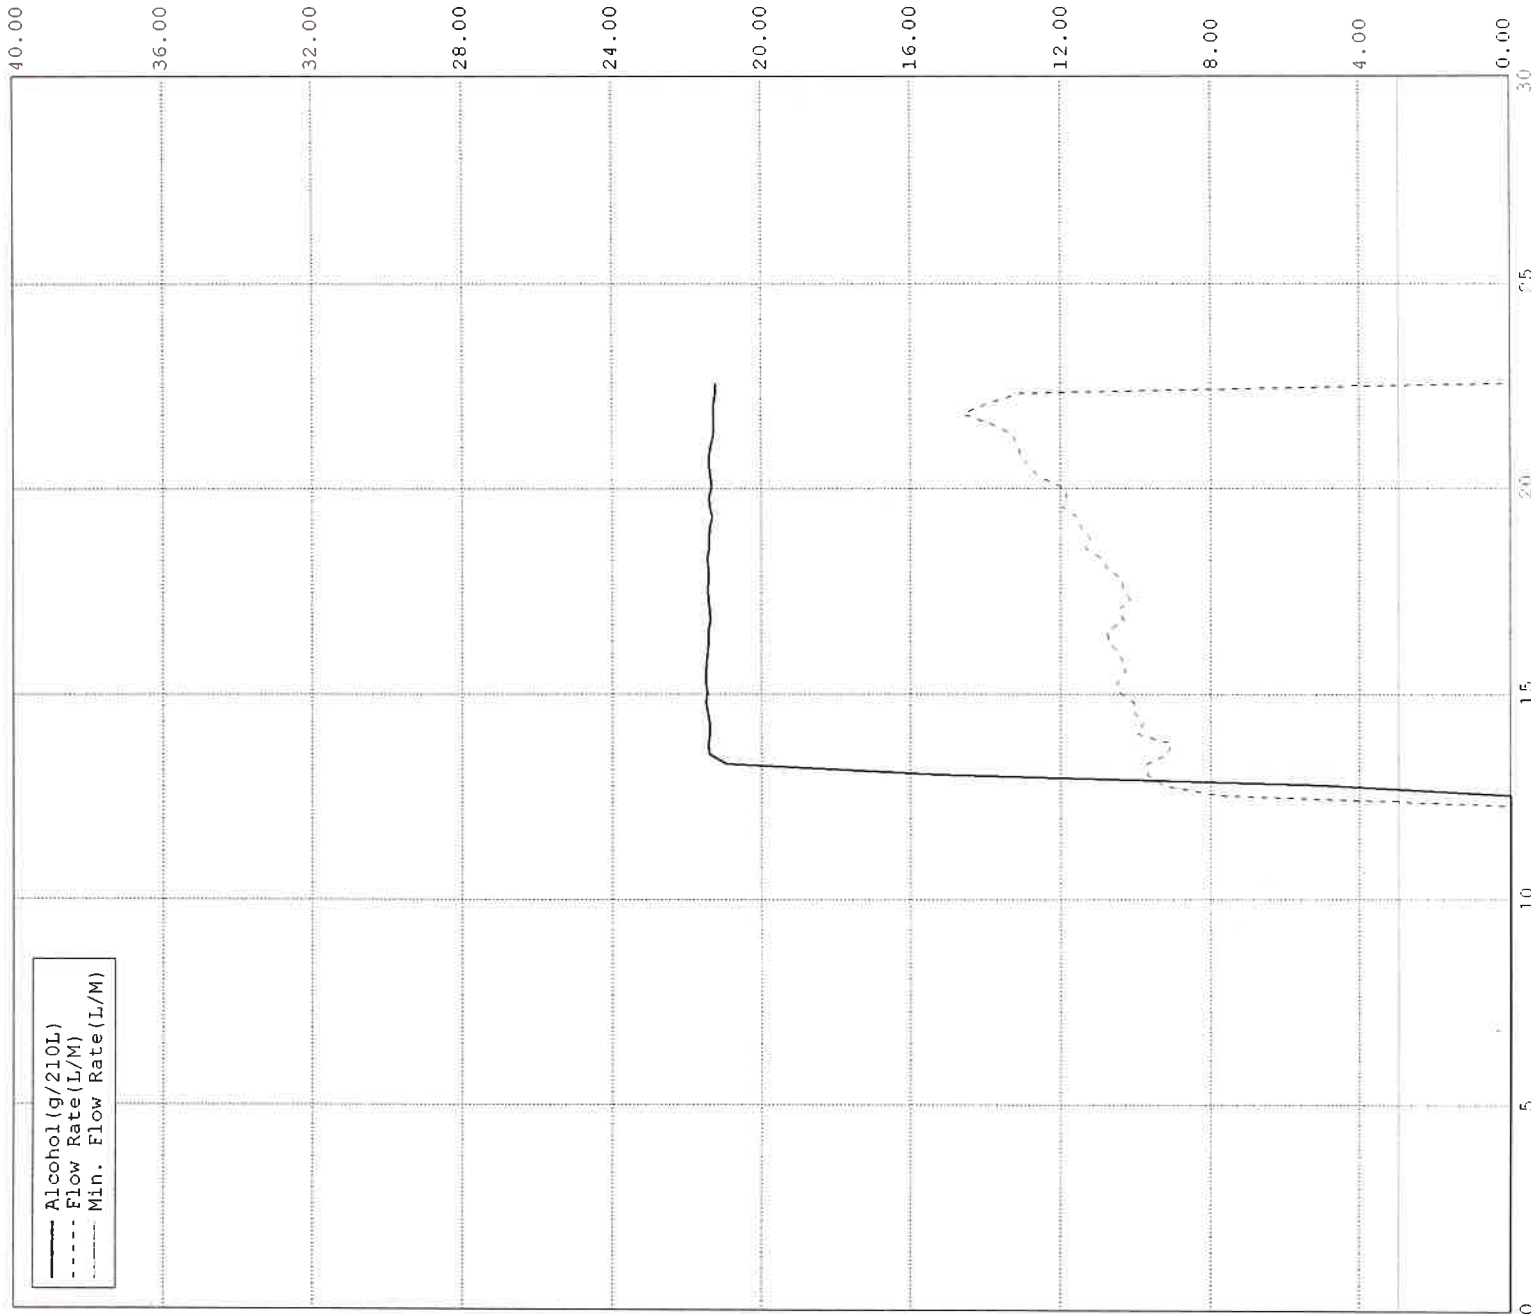

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100354

Date: 06/24/2025
Time: 12:35:57

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.64: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:37
BLANK TEST	0.000	12:37
INTERNAL STANDARD	VERIFIED	12:37
$x_q = 0.097$ (2.02%)	0.077	12:38
EXTERNAL STANDARD	$x[1] = 0.0766$ (0.0001)	(0.0030)
BLANK TEST	0.000	12:39
SUBJECT SAMPLE	XXX	12:39
	$x[1] = 0.1182$ (-0.0260)	(0.0023)

Interference Detected

OK

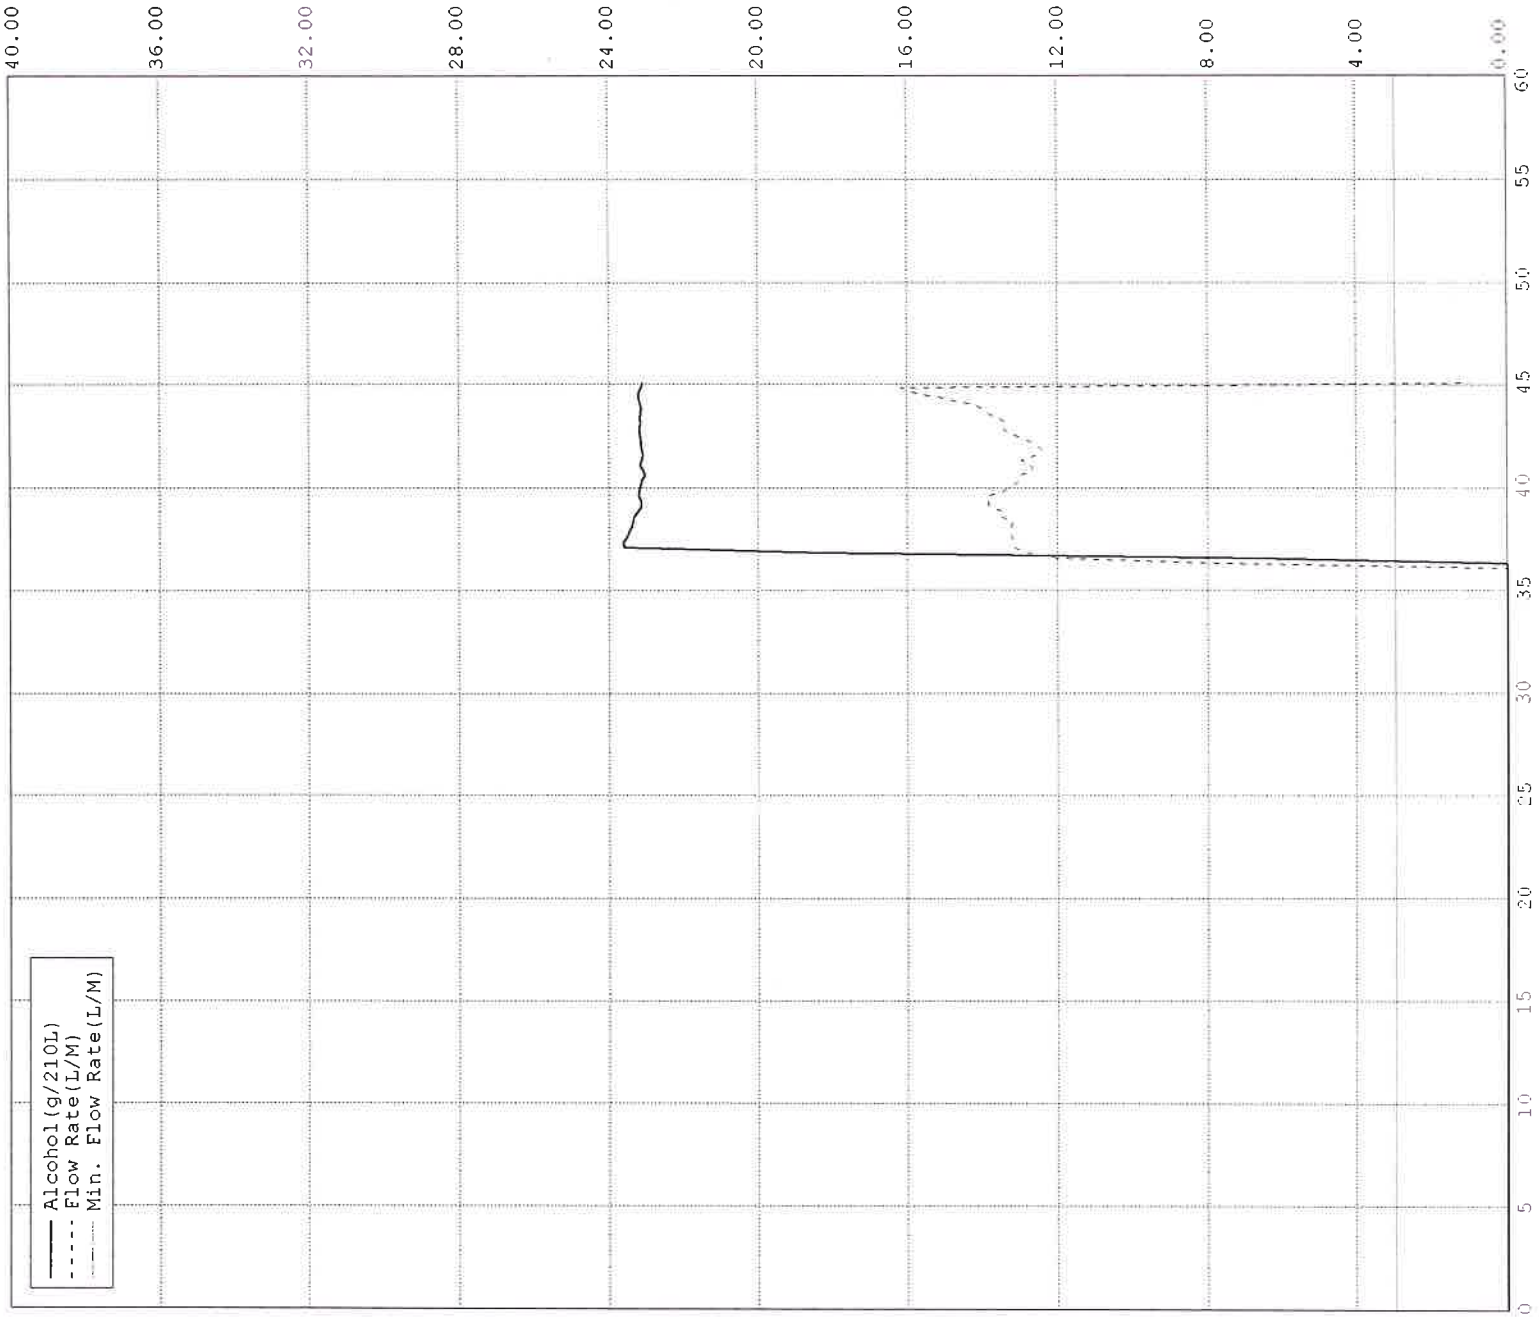

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100354

Date: 06/24/2025
 Time: 12:45:00

SUBJECT NAME:
 TEST TEST
 LICENSE #: INT-NEGATIVE

OPERATOR NAME:
 COLLEEN S OBRYANT
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 25-1234
 TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.62: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:46
BLANK TEST	0.000	12:46
INTERNAL STANDARD	VERIFIED	12:46
$X_q = 0.097$ (2.11%)		
EXTERNAL STANDARD	0.076	12:46
$X[1] = 0.0763$ (-0.0007)	(0.0028)	
BLANK TEST	0.000	12:47
SUBJECT SAMPLE (Vol=1.93L)	0.091	12:48
$X[1] = 0.0913$ (-0.0006)	(0.0016)	
BLANK TEST	0.000	12:49
EXTERNAL STANDARD	0.076	12:49
$X[1] = 0.0763$ (-0.0004)	(0.0028)	
BLANK TEST	0.000	12:50

Filter Avg = -0.0004

Filter 3 avg = 0.0028

(Signature)

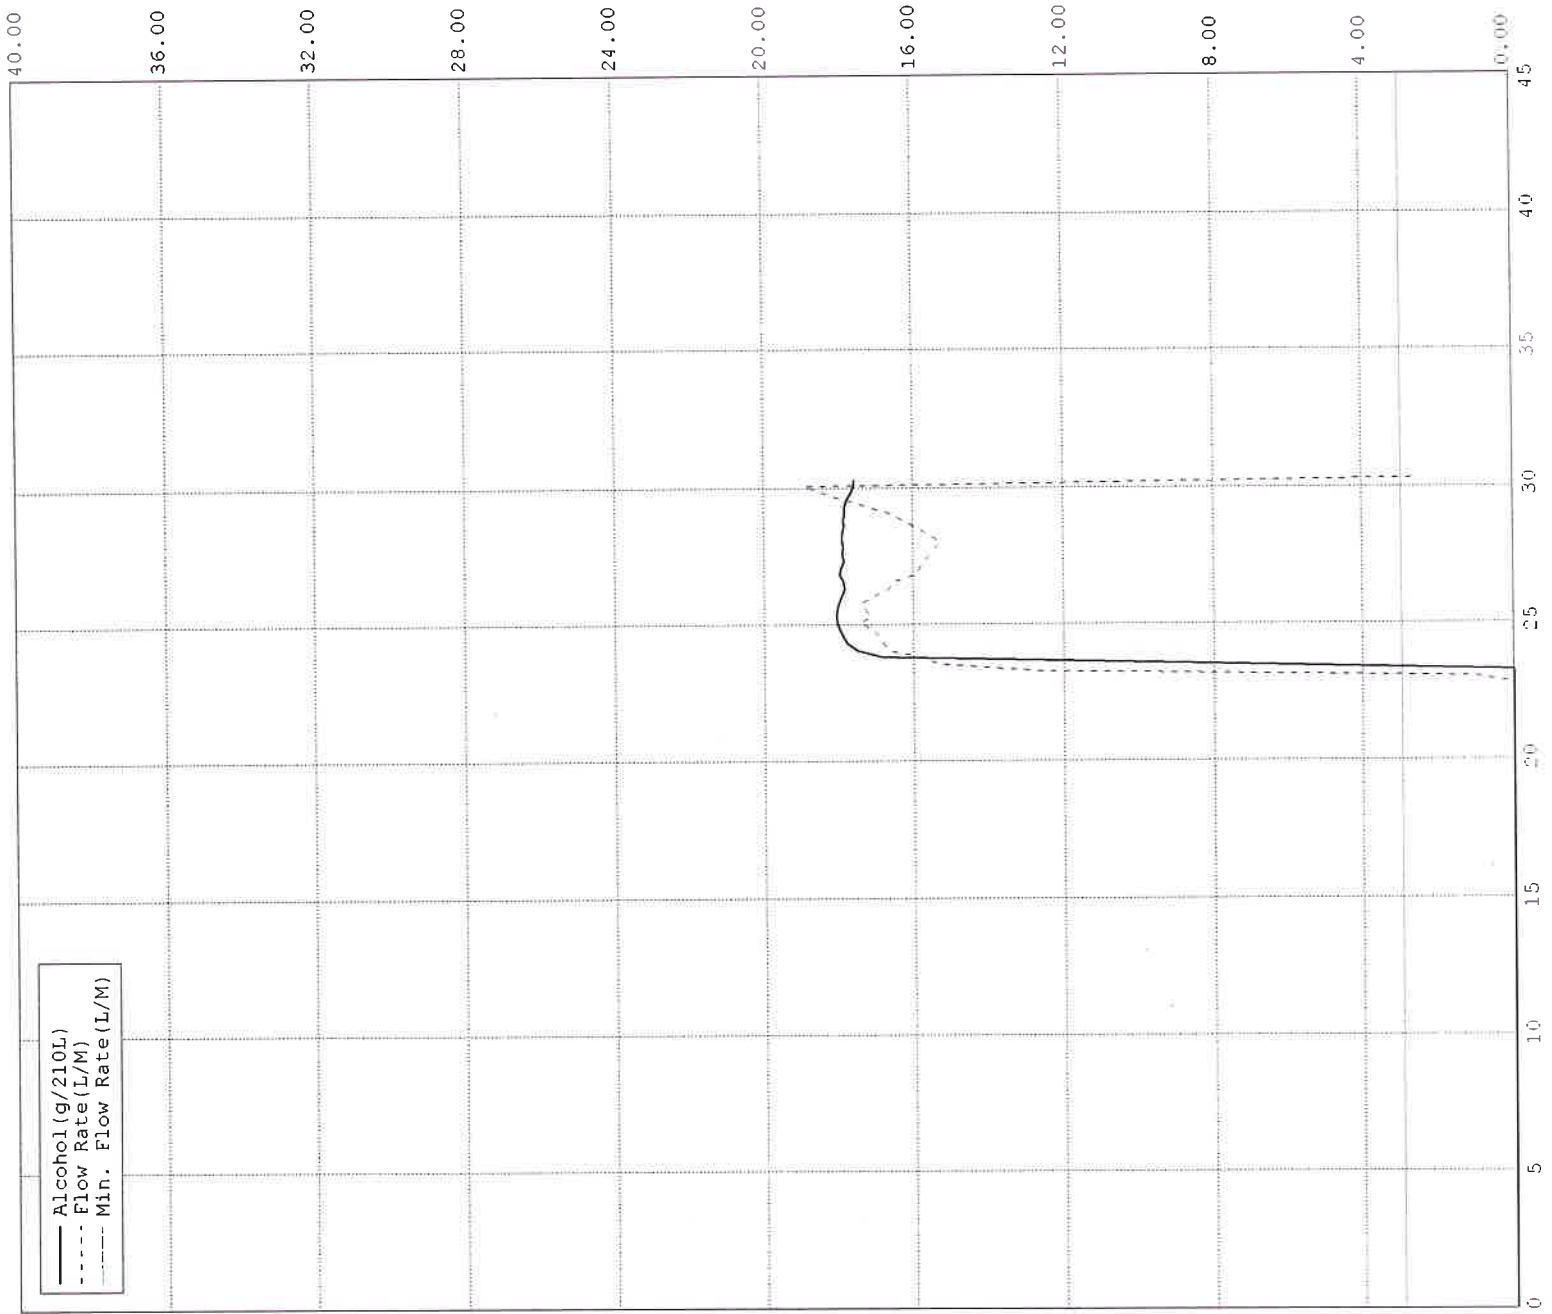

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100354

Date: 06/24/2025
Time: 13:06:50

SUBJECT NAME:
TEST TEST
LICENSE #: NONDRINKING

OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.63: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:08
BLANK TEST	0.000	13:08
INTERNAL STANDARD	VERIFIED	13:08
EXTERNAL STANDARD	0.077	13:08
BLANK TEST	0.000	13:09
SUBJECT SAMPLE (Vol=1.95L)	0.000	13:10
BLANK TEST	0.000	13:10
EXTERNAL STANDARD	0.077	13:11
BLANK TEST	0.000	13:12

COB

