




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100398

Report Issue Date: 04/23/2025
Date Received: 2025-03-20
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.019	AG408002	0.020	0.020	0.020	0.019	0.019	0.020
0.080	0.077	AG335202	0.076	0.077	0.077	0.077	0.076	0.077
0.300	0.290	AG427706	0.288	0.287	0.288	0.288	0.288	0.288

As Found - Evaluation Analyst: Kaija Swisher

As Found Conditions - Barometric Pressure (inHg): 29.04 Barometer Used: VWR S/N 240680771 Temperature (C): 22.6 Relative Humidity (%): 15

As-Found Lab Activity Date Range: 03/20/2025 - 03/20/2025

Replaced O-Ring. Due to internal standard errors out in the field, see infield instrument review 2024.10.25-2024.12.12, and a high internal standard (2.51%) on VOC, instrument marked as ready for adjustment.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.021	0.021	0.020	0.021	0.021	+/- 0.002
0.040	0.040	AG407908	0.040	0.040	0.040	0.039	0.040	0.040	+/- 0.003
0.080	0.079	AG335202	0.079	0.079	0.079	0.079	0.079	0.079	+/- 0.004
0.100	0.099	AG333401	0.100	0.100	0.100	0.099	0.100	0.100	+/- 0.004
0.150	0.148	AG332004	0.146	0.146	0.146	0.147	0.146	0.146	+/- 0.006
0.300	0.296	AG427706	0.296	0.296	0.296	0.297	0.296	0.296	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.57 Barometer Used: VWR S/N 240680771 Temperature (C): 22.4 Relative Humidity (%): 19

As-Left Lab Activity Date Range: 04/16/2025 - 04/16/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Colleen O'Bryant on 04/16/2025

colleen.obryant@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 04/23/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100398 Analyst or Technician Name: C. O. Bryant

DataMaster DMT Calibration Start Date: 4/16/25

Diagnostic Test

☒ Perform Diagnostic Test (View Details)

☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

☒ Adjust Voltages (if needed)

- Lamp (2.60 V Maximum)
- Bias
- Cooler (2.00 V Maximum)
- Chopper Frequency
- Detector Voltage (-0.100V to 0.100V)

☒ Set RFI Sensitivity

☒ Adjust internal barometer reading to match NIST-traceable barometer

Barometer/Thermometer/Hygrometer S/N: 240680771

Calibration Due Date: 10 Sep 26

☒ Verify Volume Setting (1.50 L $\pm$ 0.10 L), adjust if needed

☒ Print Technician Screen

☒ Print "Cal Factors"

Minimum Volume Test

☒ Perform Minimum Volume (Subject) Test: 1.7 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.57 Temperature(C) 20.4 Relative Humidity(%) 19

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

☒ Incomplete

☒ Maximum Attempts Exceeded

☒ Invalid

☒ Radio Frequency Interference (RFI)

☒ Interference (Volatiles) - Print with View Details

1. Acetone Reagent Lot Number: 20250219KS Expiration Date: 5/19/25

Simulator S/N: 501200 Thermometer Verification Performed? ☒

2. Isopropanol Reagent Lot Number: 20250219KS Expiration Date: 5/19/25

Simulator S/N: 501198 Thermometer Verification Performed? ☒

3. Negative (Ethanol Only) Lot Number: 234P41233 Expiration Date: 5/19/25

Simulator S/N: 501199 Thermometer Verification Performed? ☒ 9/20/25

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 19 Sep 25

Administrative

☒ Verify Stylus Calibration

☒ Reset Options

☒ Clear Memory

☒ Verification of Calibration (VOC)

☒ Perform Non-Drinking Subject Test

☒ Upload Instrument

☒ Remove Dry Gas Tank Before Shutdown

☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 4/16/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 4/16/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100398

Date: 04/16/2025
Time: 07:34:41

VERSIONS

DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 49.0°C (44.0°C - 52.0°C)	PASSED
Breath Tube = 48.1°C (38.0°C - 50.0°C)	PASSED

SETTINGS

Lamp Voltage = 1.85 V (1.11 V - 2.59 V)	PASSED
Cooler Voltage = 1.66 V (1.00 V - 2.32 V)	PASSED
Bias Voltage = 80 V (48 V - 112 V)	PASSED
Chopper Freq = 536 Hz (475 Hz - 575 Hz)	PASSED
Barometer = 29.5 in	

PUMP INFO

Flow Rate = 4.216 L/M (3.500 L/M - 6.500 L/M)	PASSED
--	--------

DETECTOR INFO

PUMP ON (0.002 V <= 0.010 V)	PASSED
PUMP OFF (0.002 V <= 0.010 V)	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.083 0.63% (0.00% - 4.00%)	PASSED
----------------------------------	--------

Technician Screen

DATAMASTER dmt: 100398

Date: 04/16/2025

Time: 7:58 AM

Temperatures (°C)

Sample Cell: 48.9°C

Breath Tube: 48.0°C

Current Barometer 29.6 in

Volume (Ltr) 1.45

Settings

Lamp: 1.82 V

Bias: 80 V

Cooler: 1.66 V

Chopper: 535 Hz

Voltages (V)

Flow: 1.03 V

Detector: 0.065 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100398

Date: 04/08/2025
Time: 11:07:27

OPERATOR NAME:
CARLIE GLAISTER
CERTIFICATE #: 10436

Ca = 0.1000
CAL = 0.997676 0.800 <= CAL < 1.200
b1 = 0.0004 0.0000 <= b1 < 0.0040
b2 = 0.0065 0.0010 <= b2 < 0.0100
b3 = 0.0008 0.0000 <= b3 < 0.0040
Xq = 0.0822 0.0500 <= Xq < 0.2000
a21 = 1.234982 1.050 <= a21 < 1.300
a31 = 0.485940 0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100398

Date: 04/16/2025
 Time: 08:03:01

SUBJECT NAME:
 TEST TEST
 LICENSE #: VOLUME TEST


OPERATOR NAME:
 COLLEEN S OBRVANT
 OPERATOR'S #: 6237

DEPT/AGENCY:
 AAA1
 CASE/REPORT: 25-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.58: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:04
BLANK TEST	0.000	08:04
INTERNAL STANDARD	VERIFIED	08:04
EXTERNAL STANDARD	0.079	08:05
BLANK TEST	0.000	08:05
SUBJECT SAMPLE (Vol=1.57L)	0.000	08:07
BLANK TEST	0.000	08:08
EXTERNAL STANDARD	0.080	08:08
BLANK TEST	0.000	08:09

CB

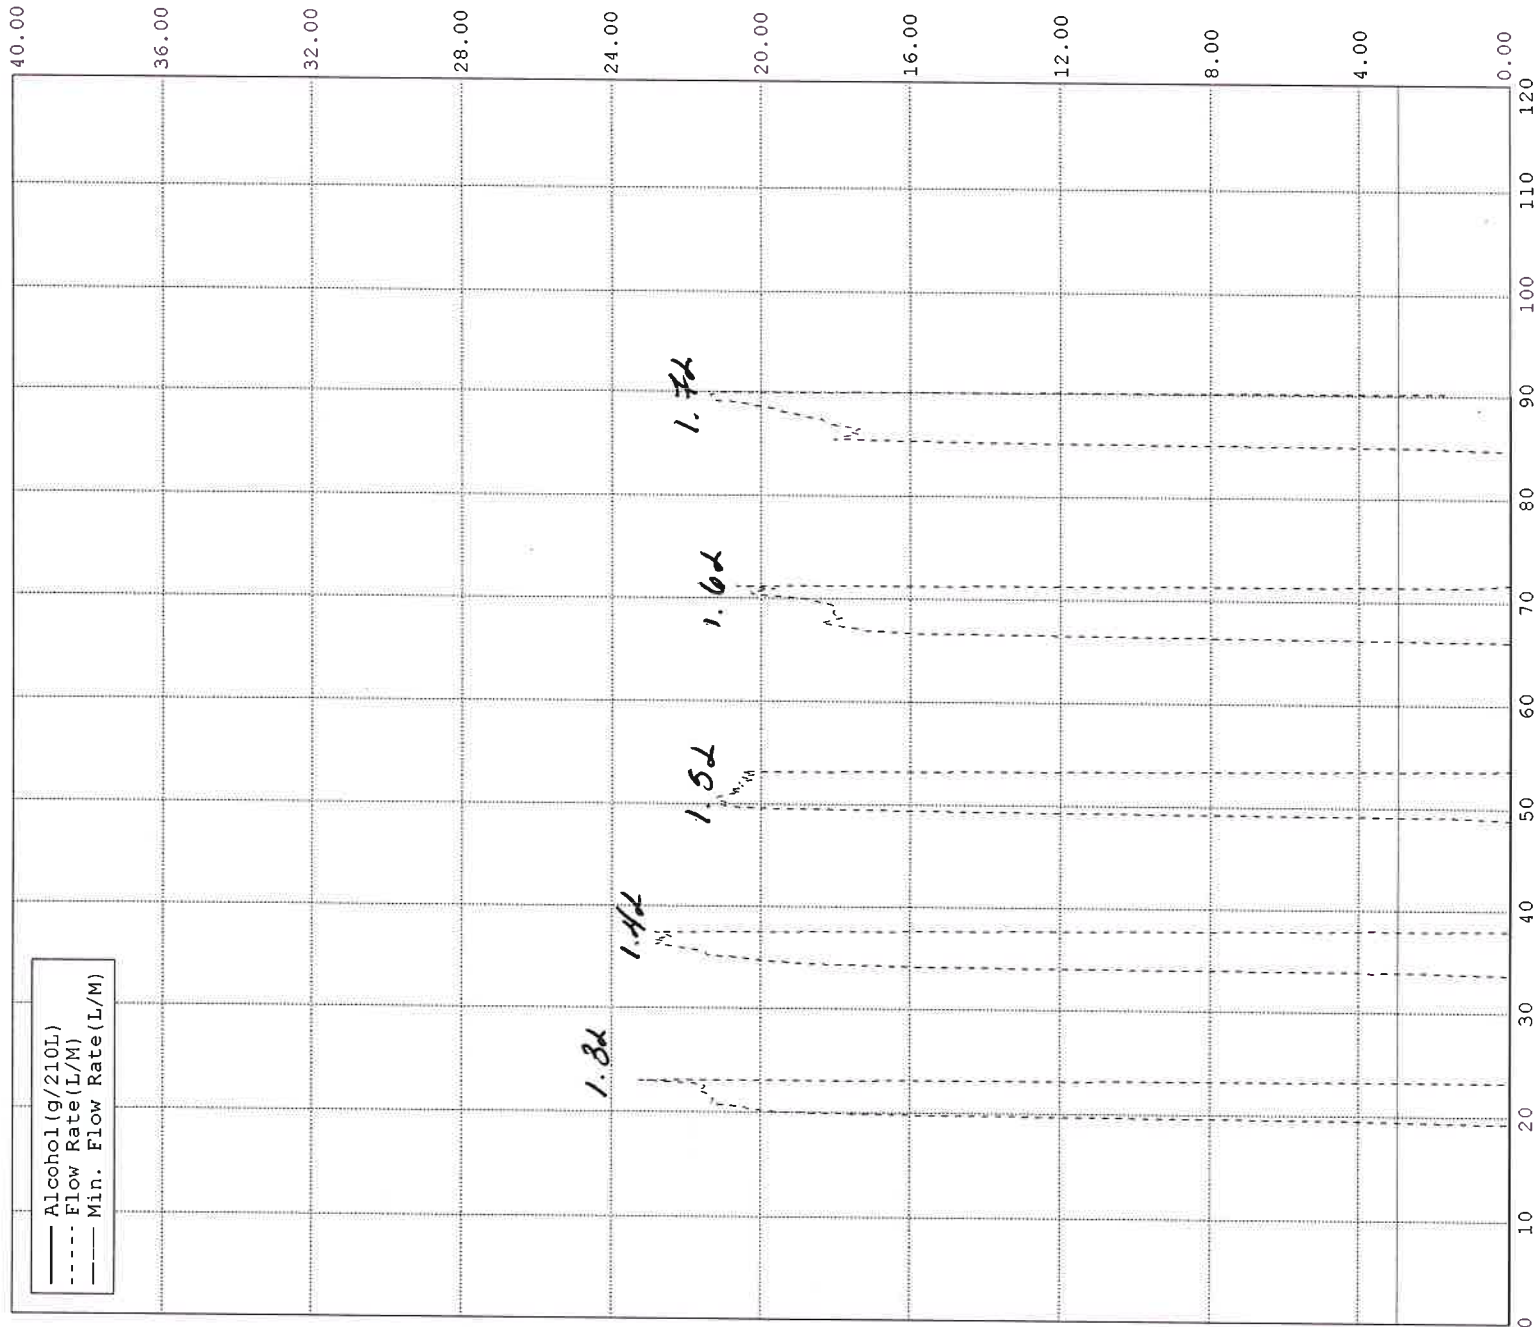

LINEARITY CHECK

Alaska Department of Public Safety
 DATAMASTER dmt: 100398


Date: 04/16/2025
 Time: 08:22:18

SUPERVISOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0206	0.0005
0.040	0.0398	0.0004
0.079	0.0790	0.0000
0.099	0.0998	0.0004
0.148	0.1462	0.0004
0.296	0.2962	0.0004

SLOPE = 0.998431
 R² = 0.999916

CS

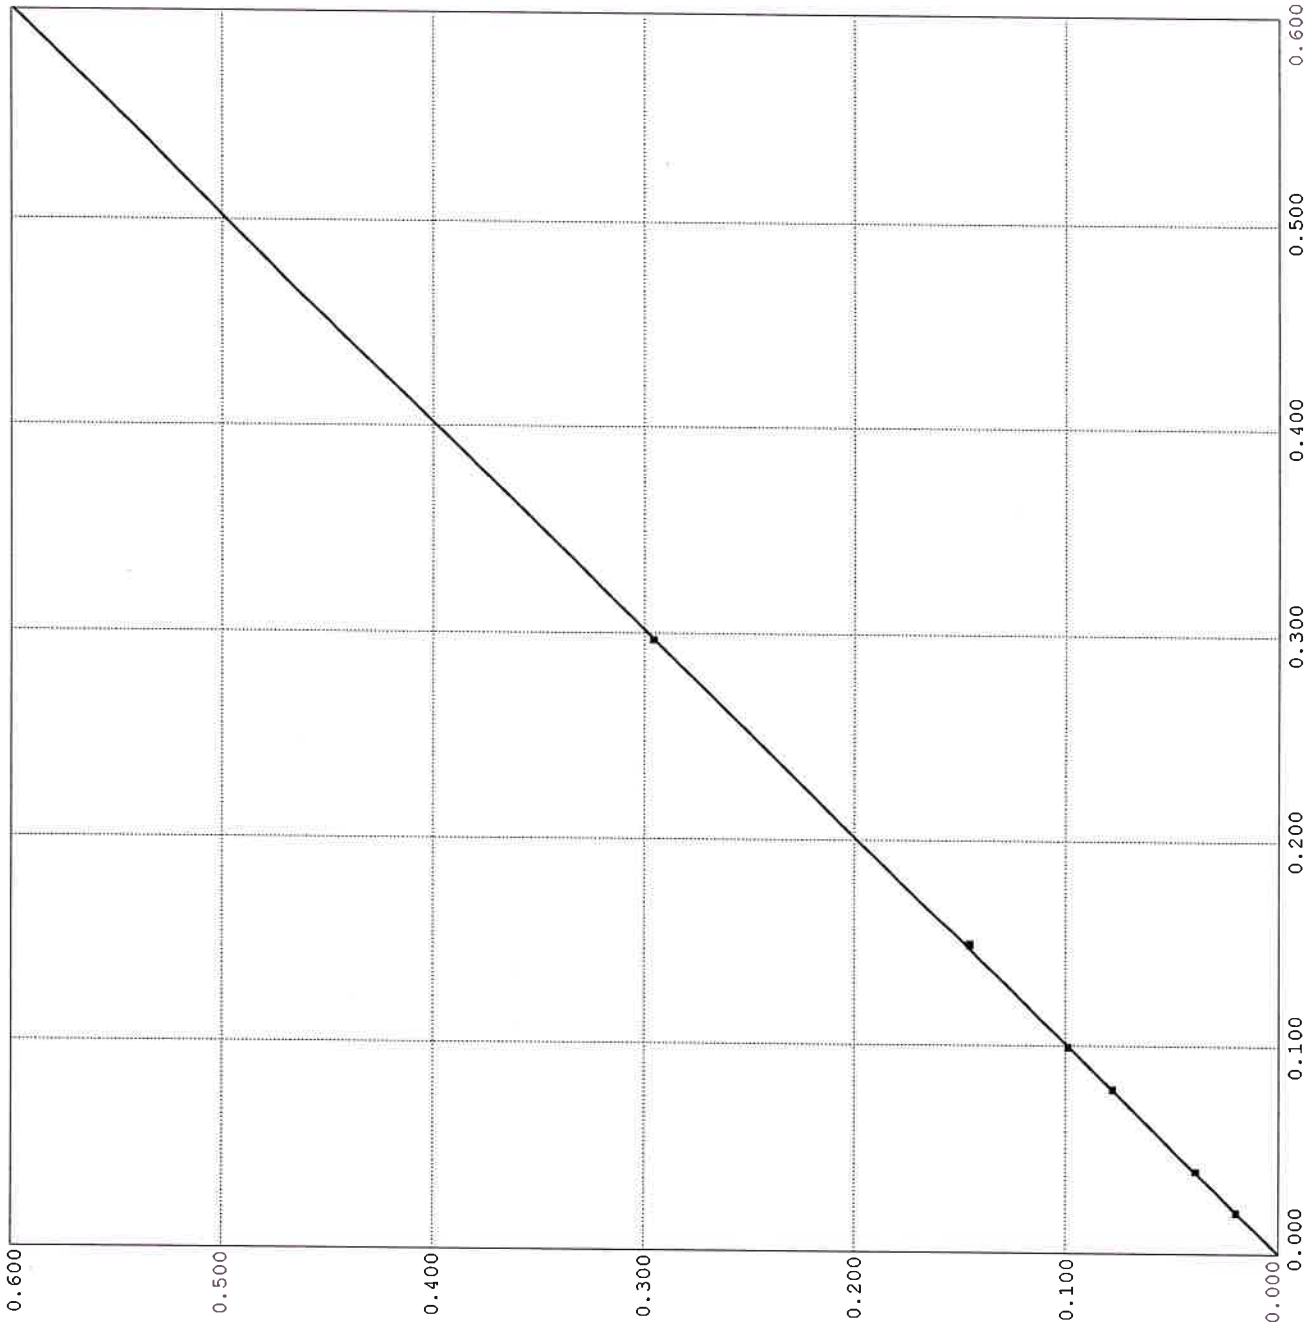

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100398






Date: 04/16/2025
Time: 08:22:20

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.58: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 229 psi

BLANK TEST	0.000	08:27
INTERNAL STANDARD	VERIFIED	08:28
EXTERNAL STANDARD	0.020	08:28
BLANK TEST	0.000	08:29
EXTERNAL STANDARD	0.021	08:29
BLANK TEST	0.000	08:30
EXTERNAL STANDARD	0.021	08:30
BLANK TEST	0.000	08:31
EXTERNAL STANDARD	0.020	08:31
BLANK TEST	0.000	08:32
EXTERNAL STANDARD	0.021	08:32
BLANK TEST	0.000	08:33

Average = 0.0206
Std Dev = 0.0005

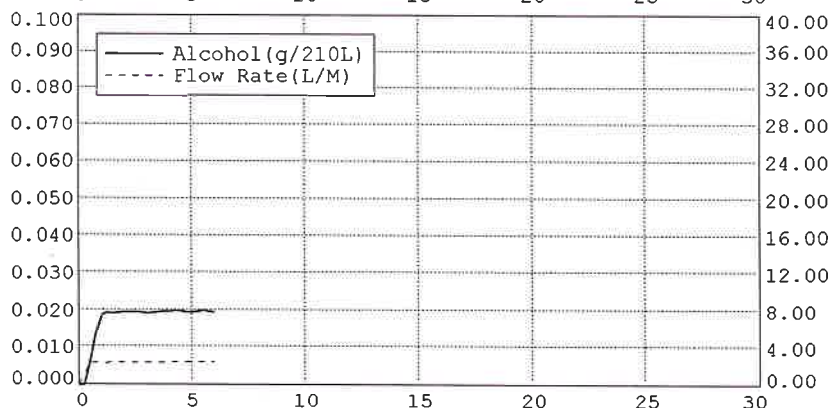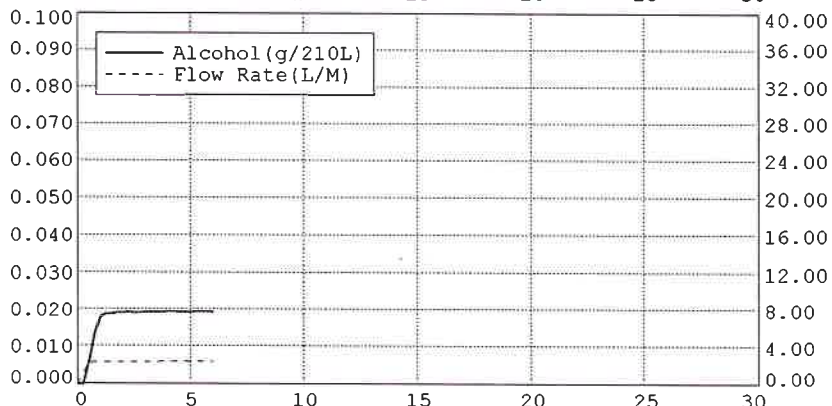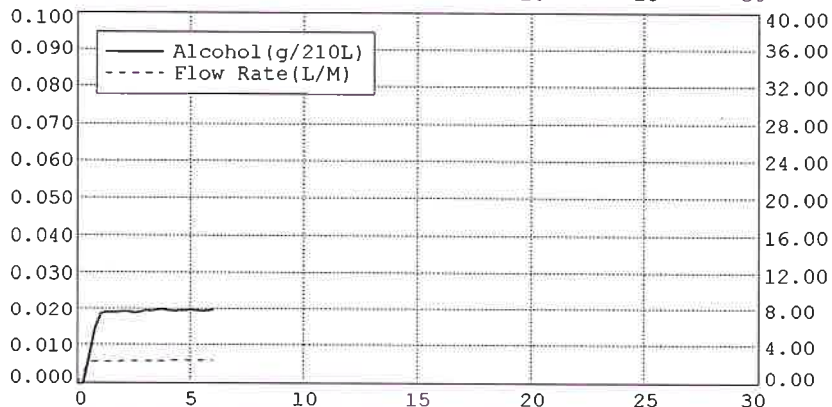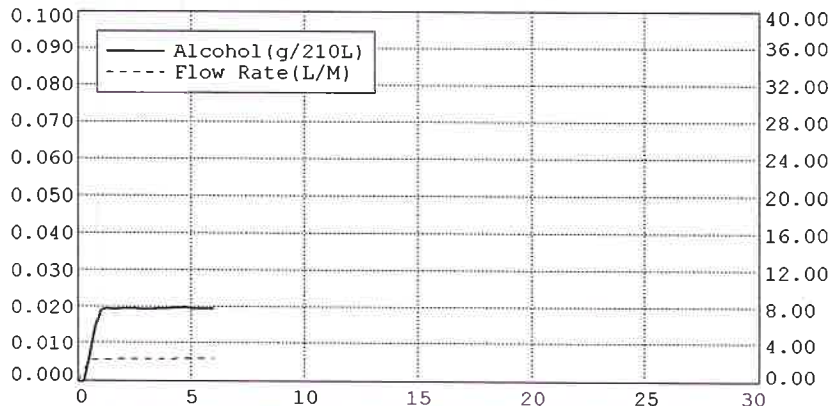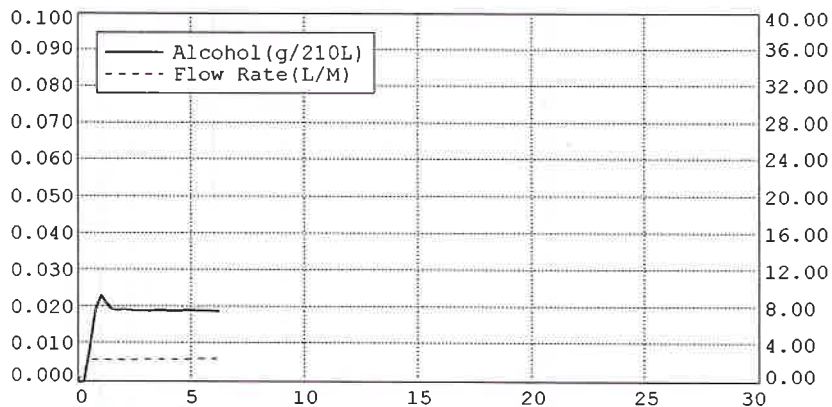

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100398






Date: 04/16/2025
Time: 08:37:38

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.58: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 782 psi

BLANK TEST	0.000	08:43
INTERNAL STANDARD	VERIFIED	08:43
EXTERNAL STANDARD	0.040	08:43
BLANK TEST	0.000	08:44
EXTERNAL STANDARD	0.040	08:44
BLANK TEST	0.000	08:45
EXTERNAL STANDARD	0.040	08:45
BLANK TEST	0.000	08:46
EXTERNAL STANDARD	0.039	08:46
BLANK TEST	0.000	08:47
EXTERNAL STANDARD	0.040	08:47
BLANK TEST	0.000	08:48

Average = 0.0398
Std Dev = 0.0004

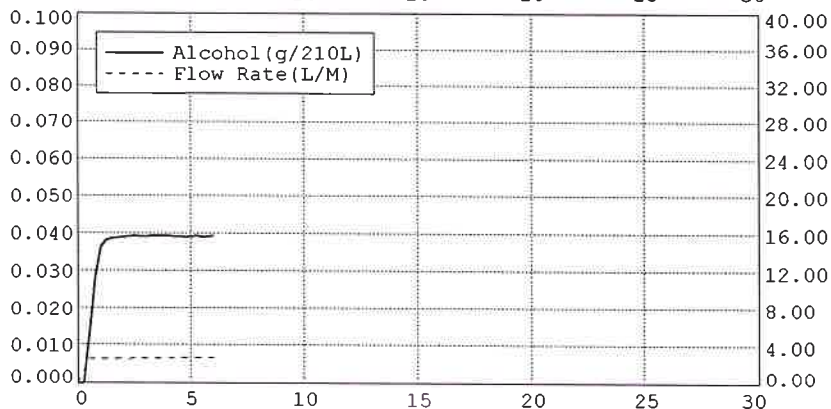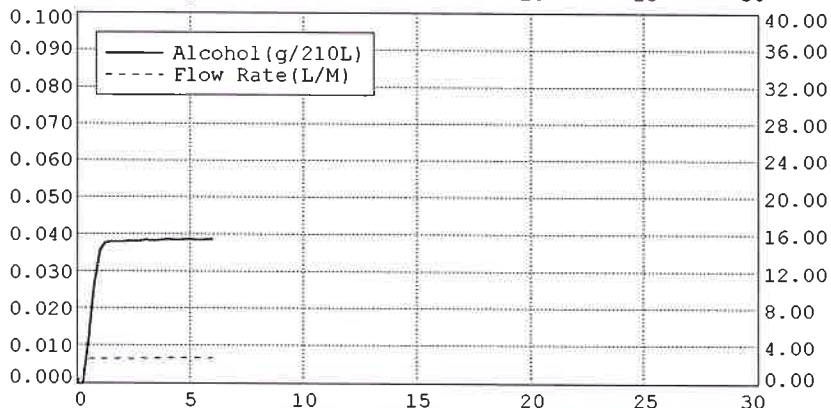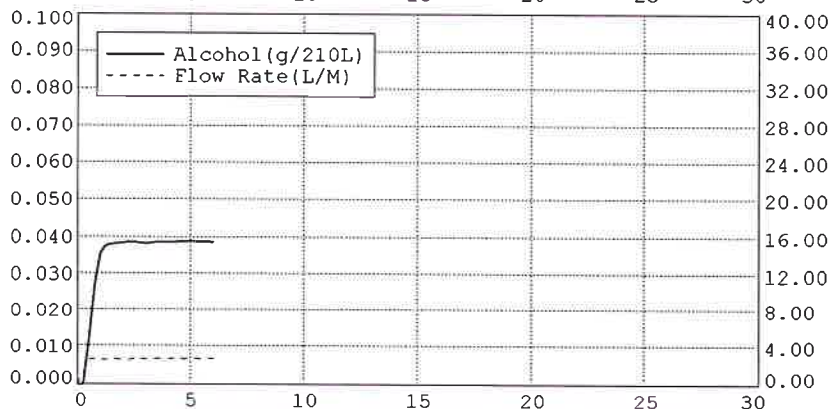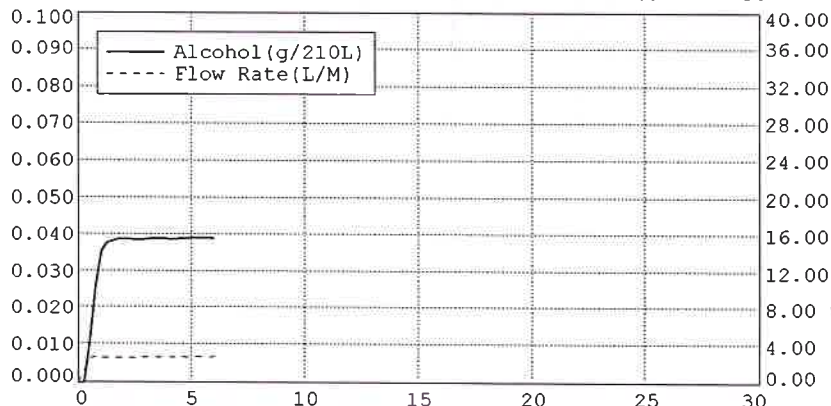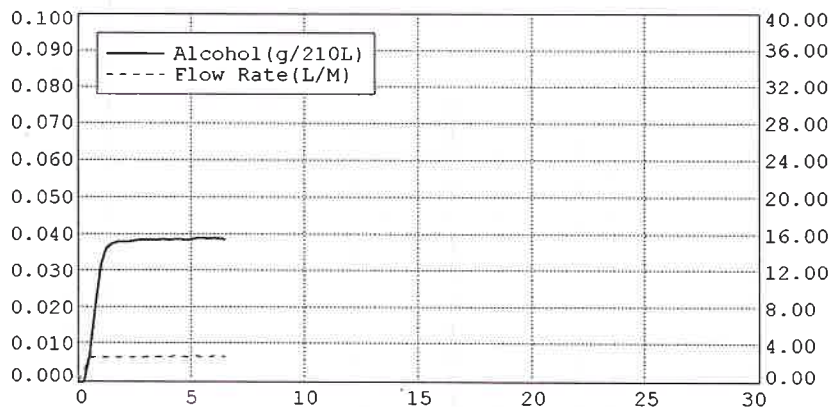

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100398






Date: 04/16/2025
Time: 08:49:24

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.57: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 522 psi

BLANK TEST	0.000	08:50
INTERNAL STANDARD	VERIFIED	08:50
EXTERNAL STANDARD	0.079	08:50
BLANK TEST	0.000	08:51
EXTERNAL STANDARD	0.079	08:51
BLANK TEST	0.000	08:52
EXTERNAL STANDARD	0.079	08:53
BLANK TEST	0.000	08:53
EXTERNAL STANDARD	0.079	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.079	08:55
BLANK TEST	0.000	08:56

Average = 0.0790
Std Dev = 0.0000

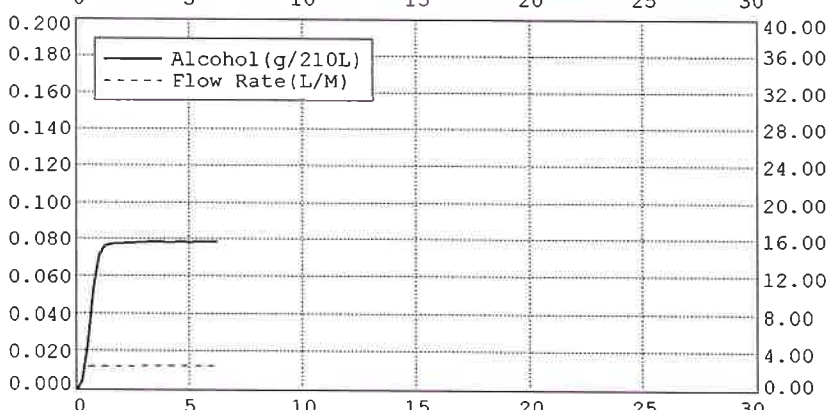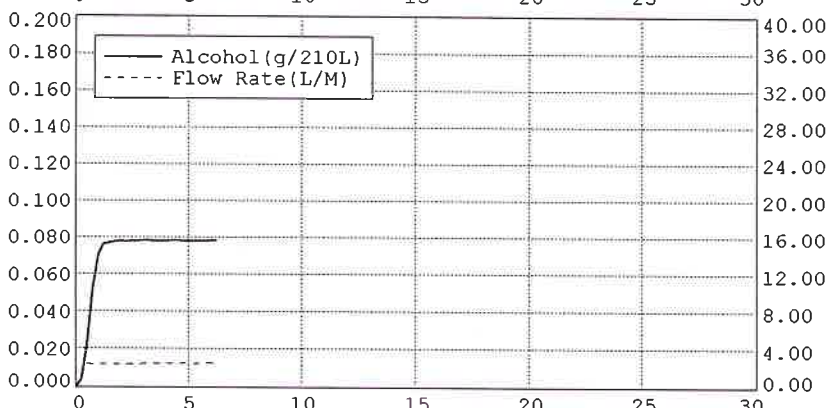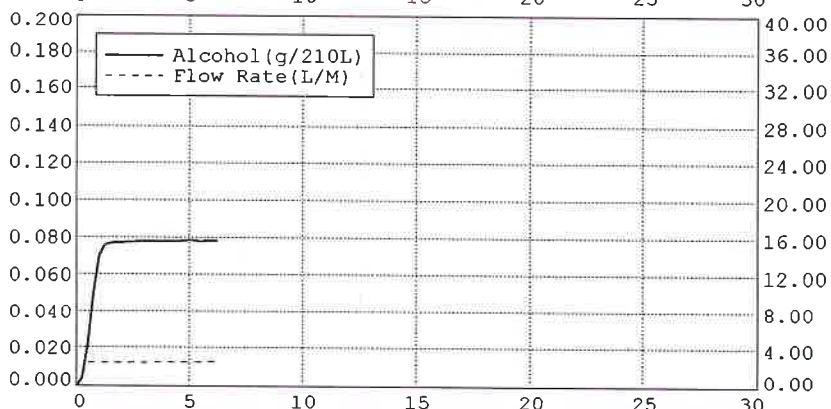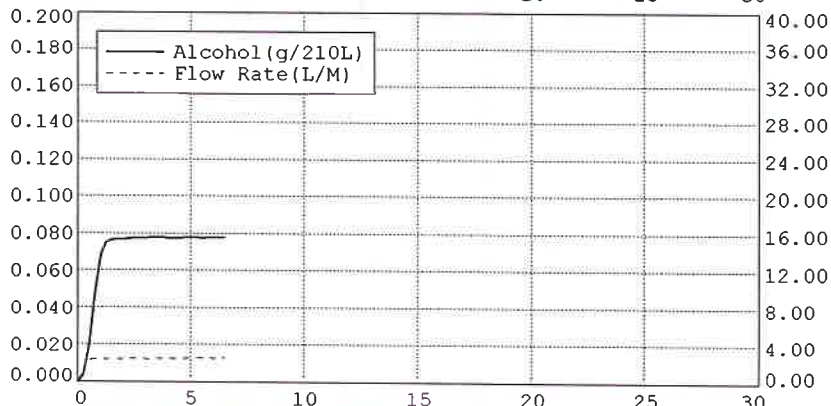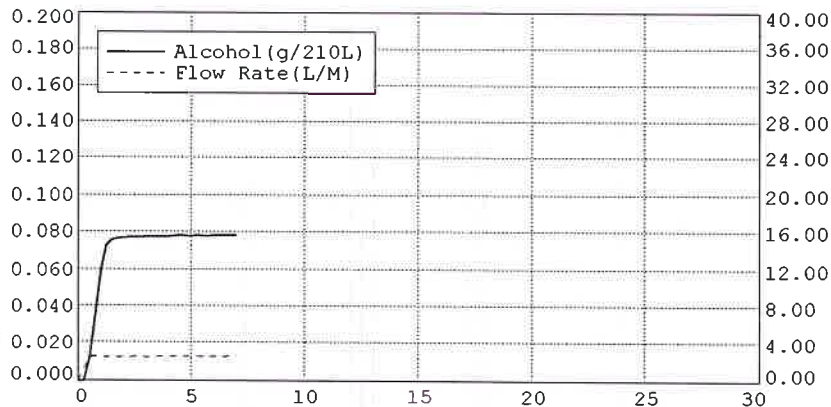

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100398






Date: 04/16/2025
Time: 08:57:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.56: 0.099
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 551 psi

BLANK TEST	0.000	08:58
INTERNAL STANDARD	VERIFIED	08:59
EXTERNAL STANDARD	0.100	08:59
BLANK TEST	0.000	09:00
EXTERNAL STANDARD	0.100	09:00
BLANK TEST	0.000	09:01
EXTERNAL STANDARD	0.100	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.099	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.100	09:03
BLANK TEST	0.000	09:04

Average = 0.0998
Std Dev = 0.0004

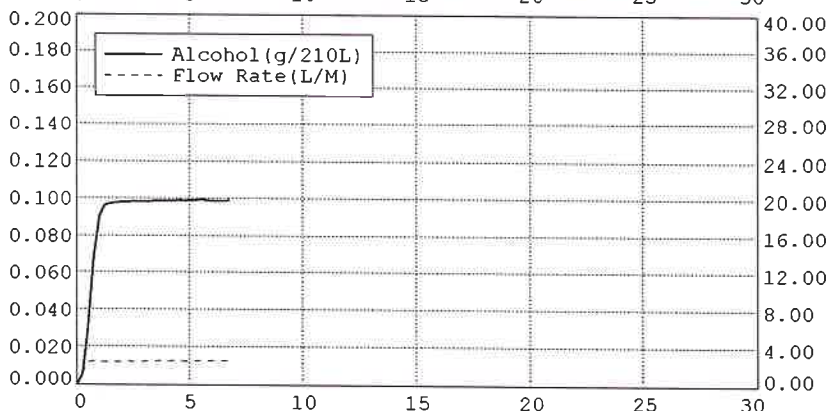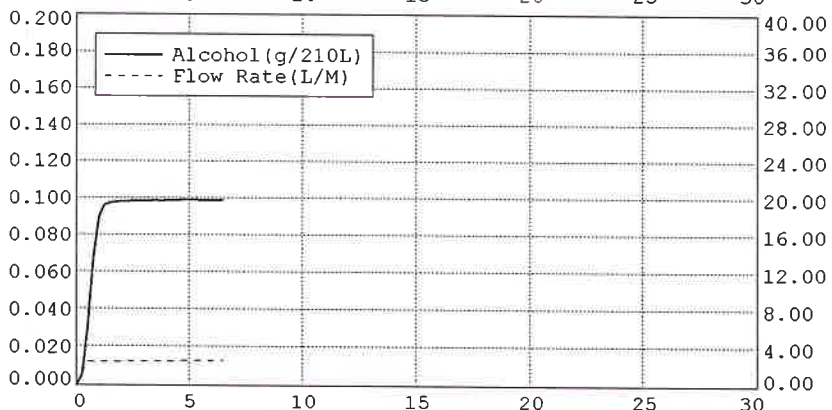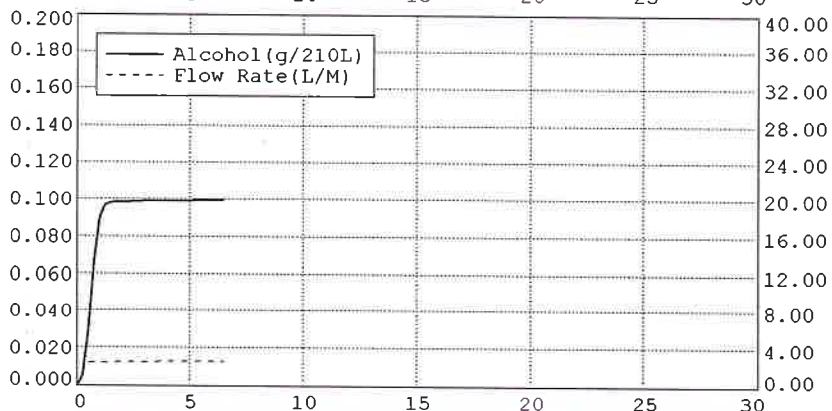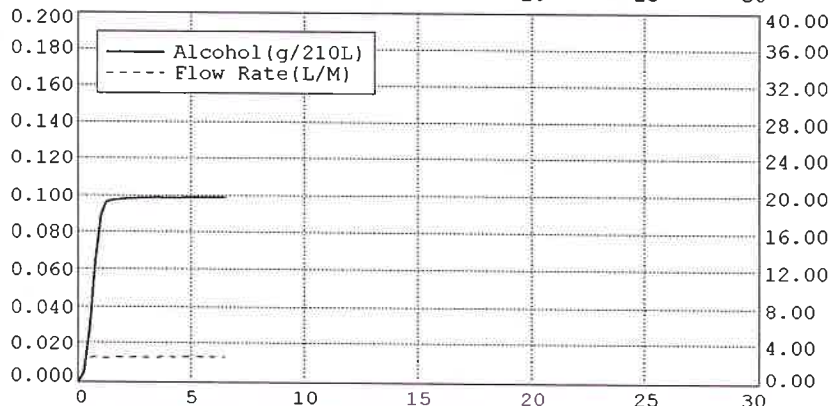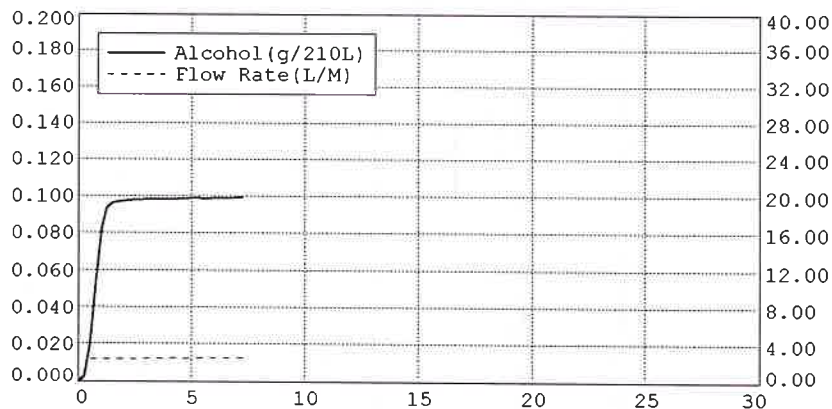

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100398






Date: 04/16/2025
Time: 09:06:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.56: 0.148
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 537 psi

BLANK TEST	0.000	09:07
INTERNAL STANDARD	VERIFIED	09:07
EXTERNAL STANDARD	0.146	09:08
BLANK TEST	0.000	09:08
EXTERNAL STANDARD	0.146	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.146	09:10
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.147	09:11
BLANK TEST	0.000	09:12
EXTERNAL STANDARD	0.146	09:12
BLANK TEST	0.000	09:13

Average = 0.1462
Std Dev = 0.0004

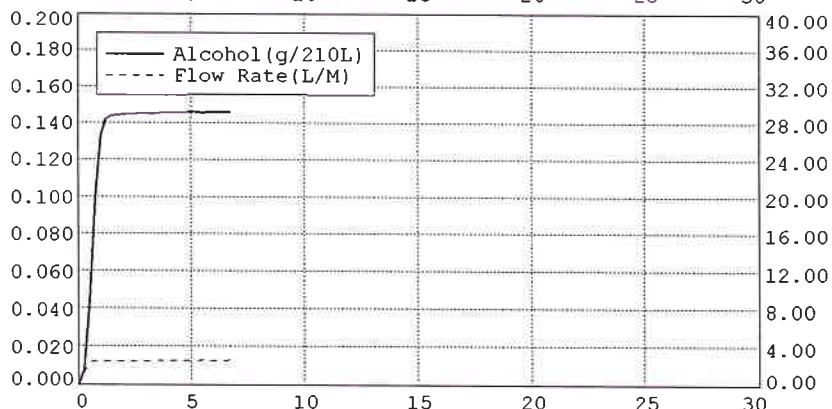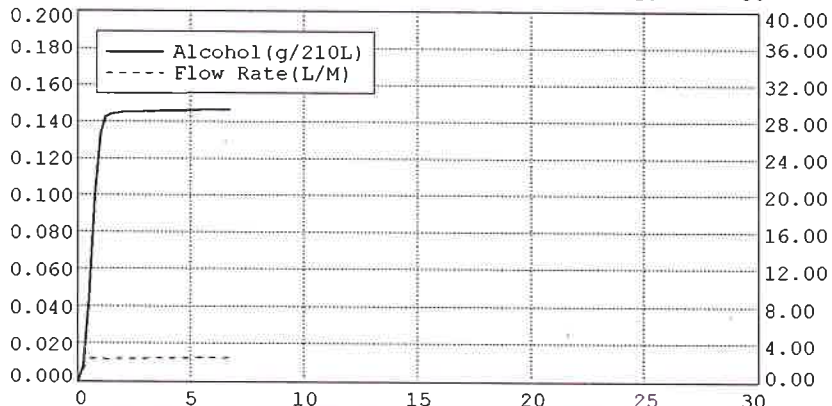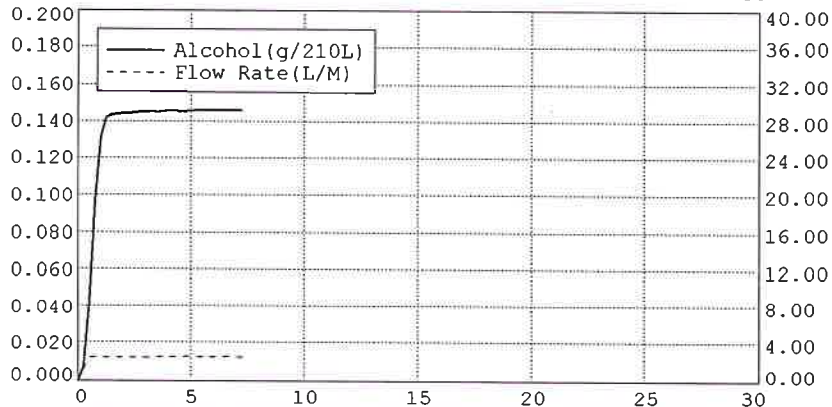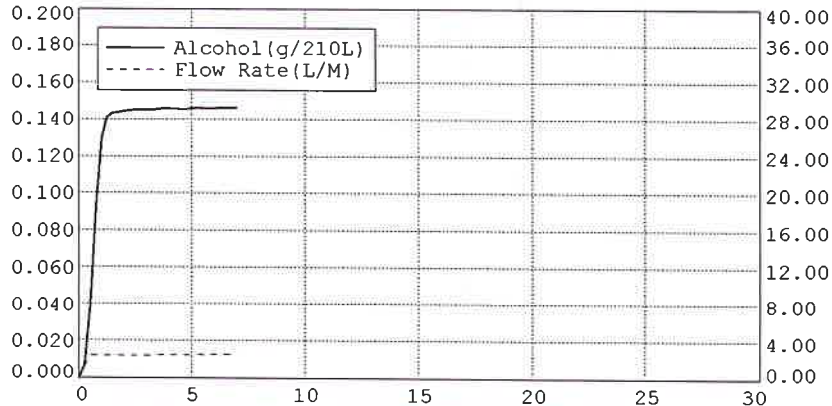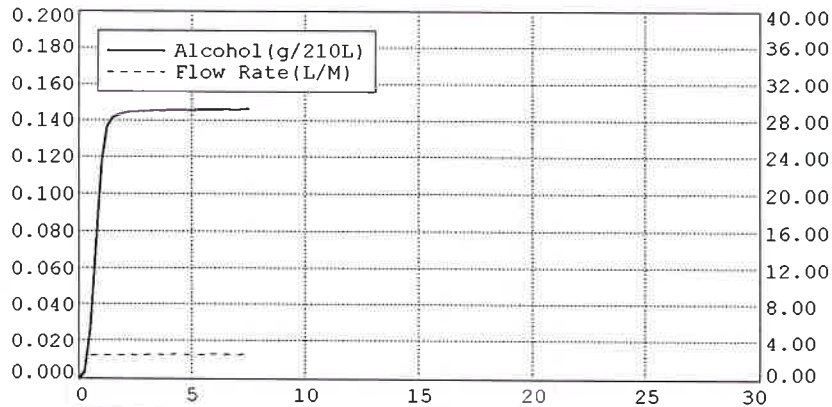

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100398






Date: 04/16/2025
Time: 09:14:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.57: 0.296
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 183 psi

BLANK TEST	0.000	09:16
INTERNAL STANDARD	VERIFIED	09:16
EXTERNAL STANDARD	0.296	09:16
BLANK TEST	0.000	09:17
EXTERNAL STANDARD	0.296	09:17
BLANK TEST	0.000	09:18
EXTERNAL STANDARD	0.296	09:18
BLANK TEST	0.000	09:19
EXTERNAL STANDARD	0.297	09:19
BLANK TEST	0.000	09:20
EXTERNAL STANDARD	0.296	09:21
BLANK TEST	0.000	09:22

Average = 0.2962
Std Dev = 0.0004

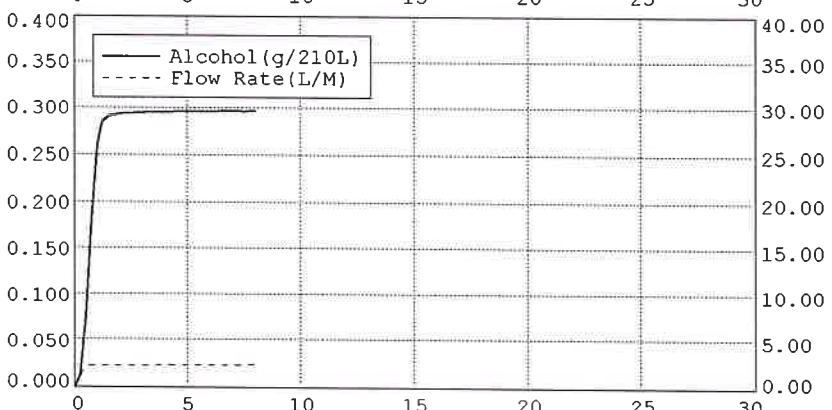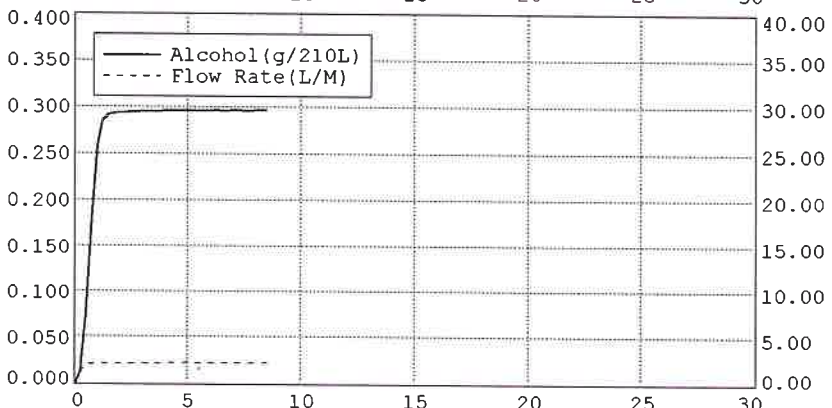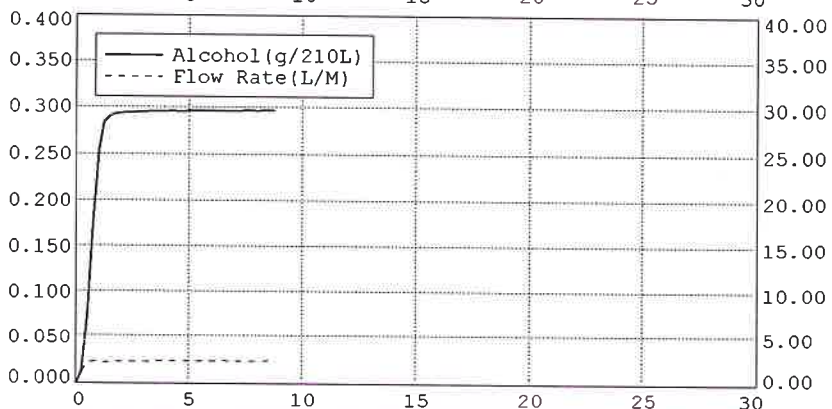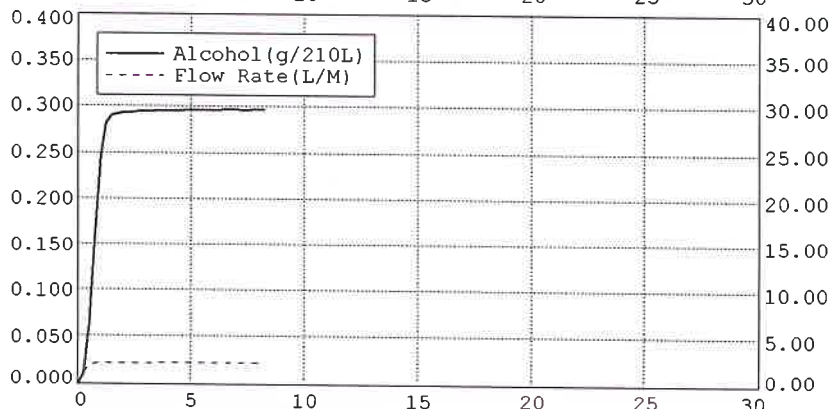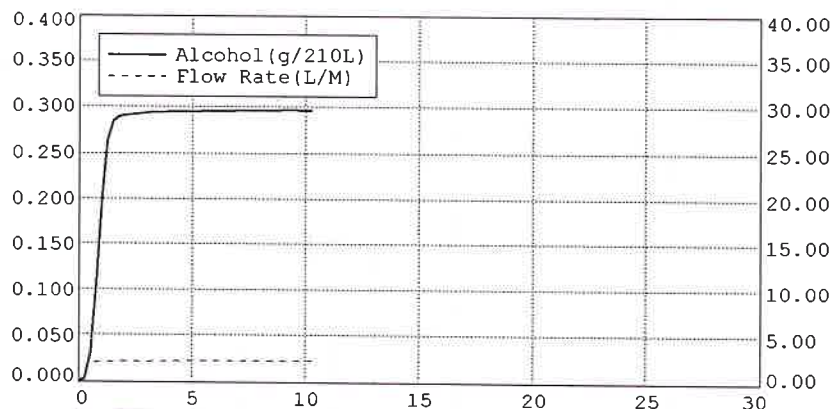

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100398

Date: 04/16/2025
Time: 11:08:30

SUBJECT NAME:
TEST TEST
LICENSE #: INCOMPLETE


OPERATOR NAME:
COLLEEN S OBRYANT
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.52: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:09
BLANK TEST	0.000	11:10
INTERNAL STANDARD	VERIFIED	11:10
EXTERNAL STANDARD	0.079	11:10
BLANK TEST	0.000	11:11
SUBJECT SAMPLE	INCOMPLETE	11:13

AS

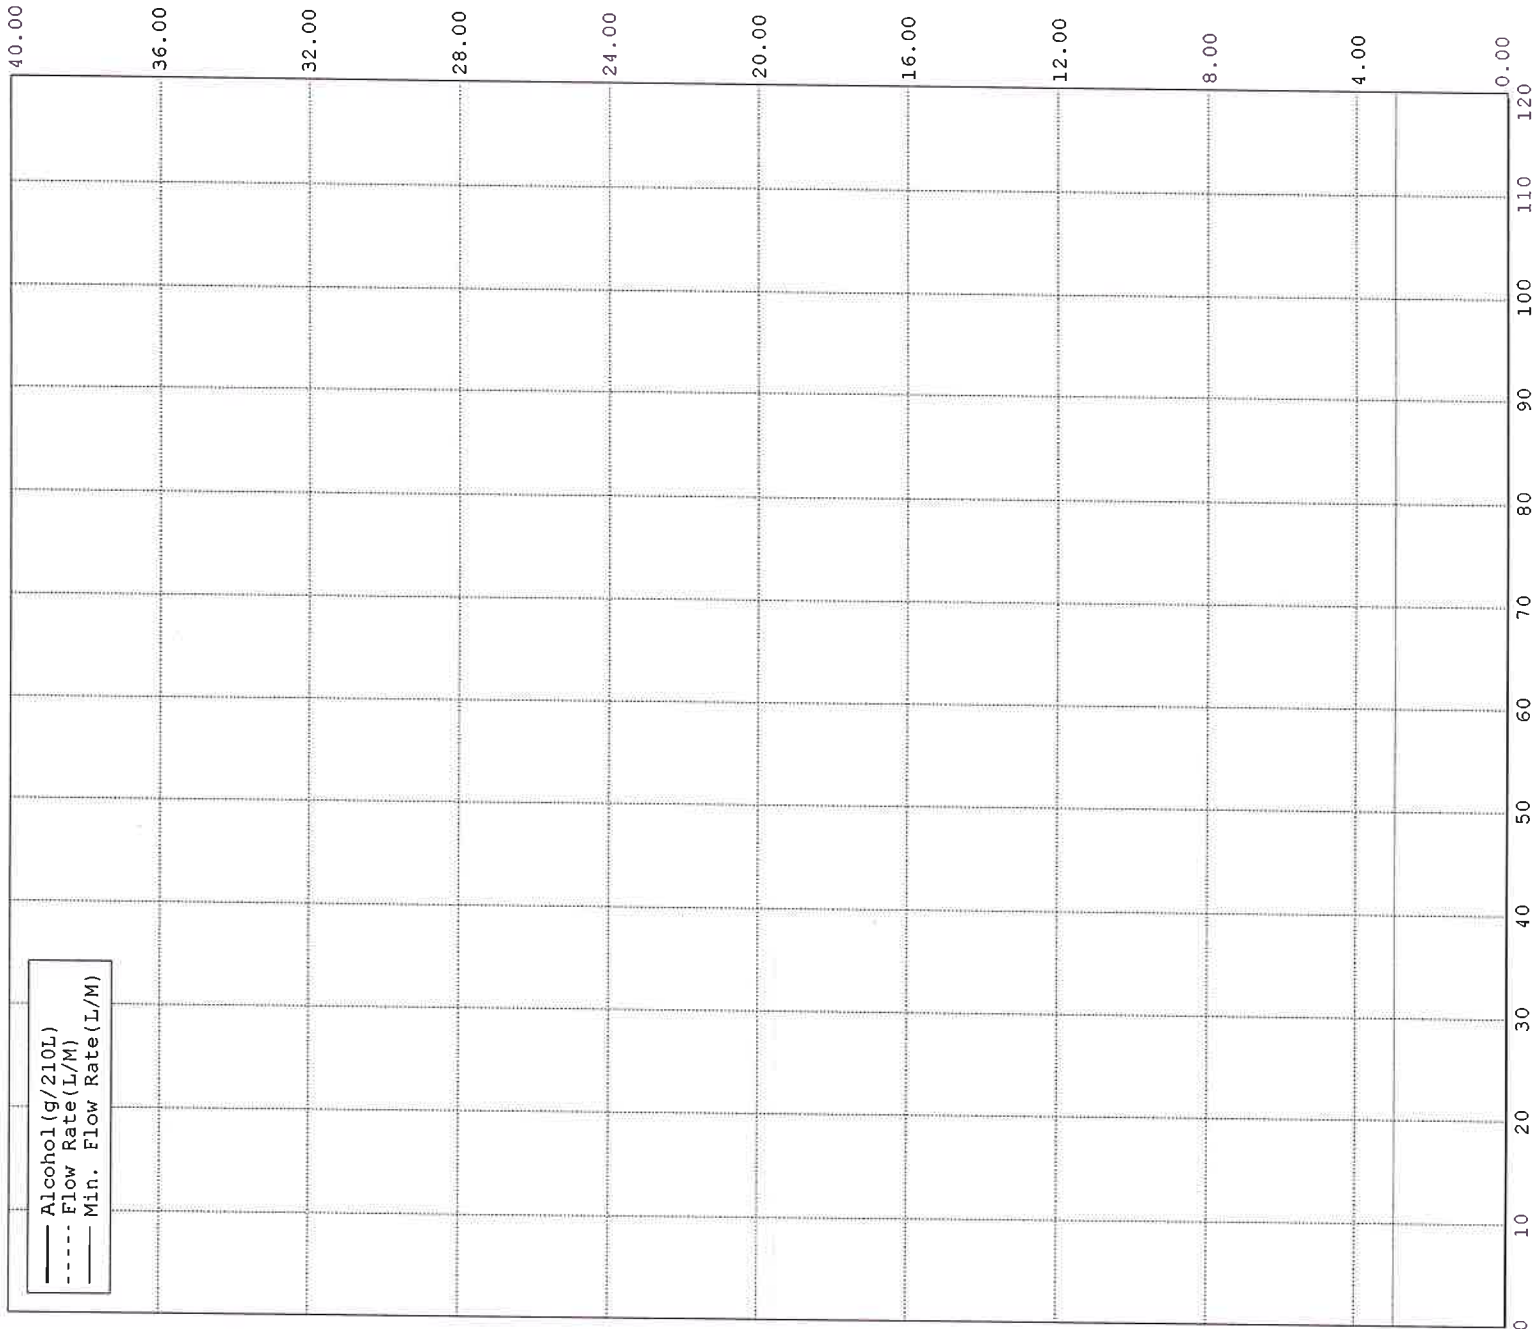

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100398

Date: 04/16/2025
 Time: 11:15:51

SUBJECT NAME:
 TEST TEST
 LICENSE #: MAX ATTEMPTS

OPERATOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237


DEPT/AGENCY:
 AAA1
 CASE/REPORT: 25-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.51: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:16
BLANK TEST	0.000	11:16
INTERNAL STANDARD	VERIFIED	11:17
EXTERNAL STANDARD	0.079	11:17
BLANK TEST	0.000	11:18
SUBJECT SAMPLE	XXX	11:19

Maximum Attempts Exceeded

CS

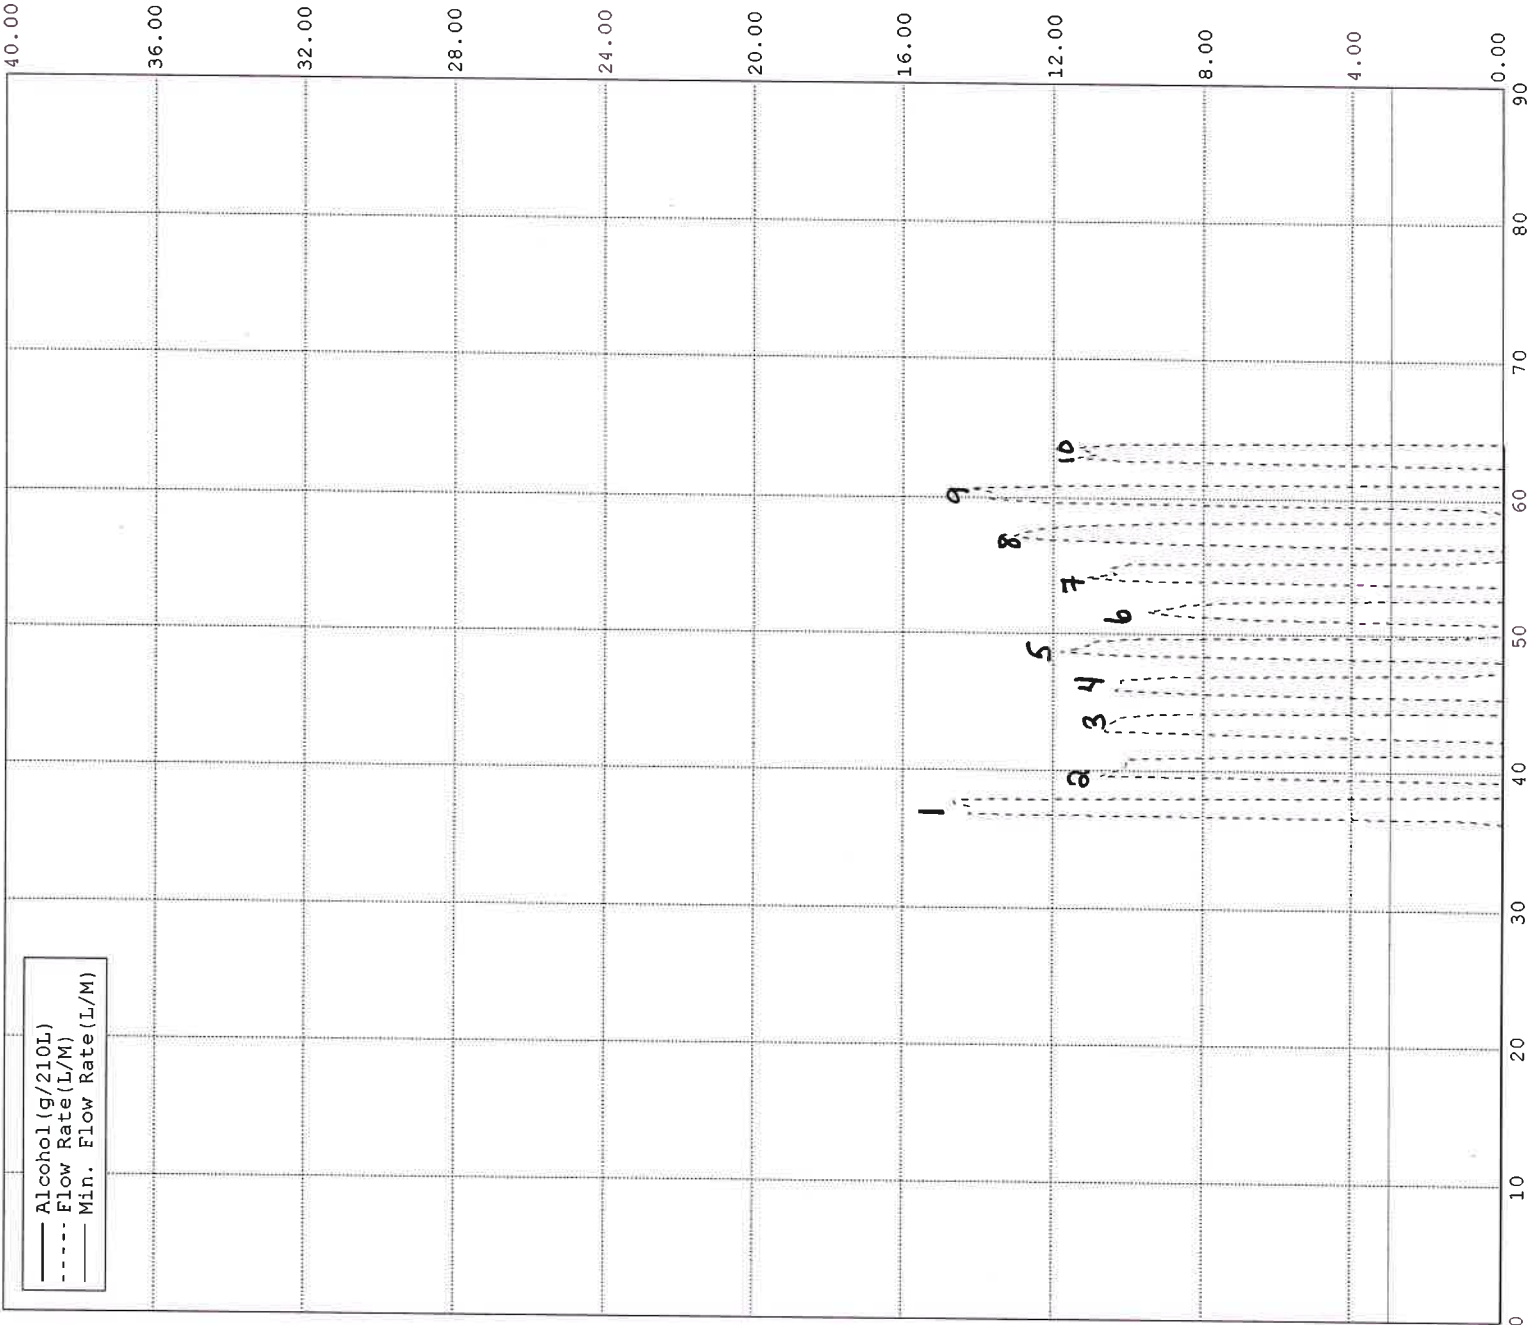

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 04/16/2025

Time: 11:21:39

SUBJECT NAME:

TEST TEST

LICENSE #: INVALID

OPERATOR NAME:

COLLEEN S OBRYANT

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 25-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.52: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED

0.000

VERIFIED

0.079

0.000

INVALID

11:22

11:22

11:22

11:23

11:24

11:24

OB



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100398

Date: 04/16/2025

Time: 11:26:07

SUBJECT NAME:

TEST TEST

LICENSE #: RFI

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 25-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.52: 0.079

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

PASSED

0.000

VERIFIED

0.079

0.000

11:27

11:27


11:27

11:27

11:28

RFI DETECTED

003

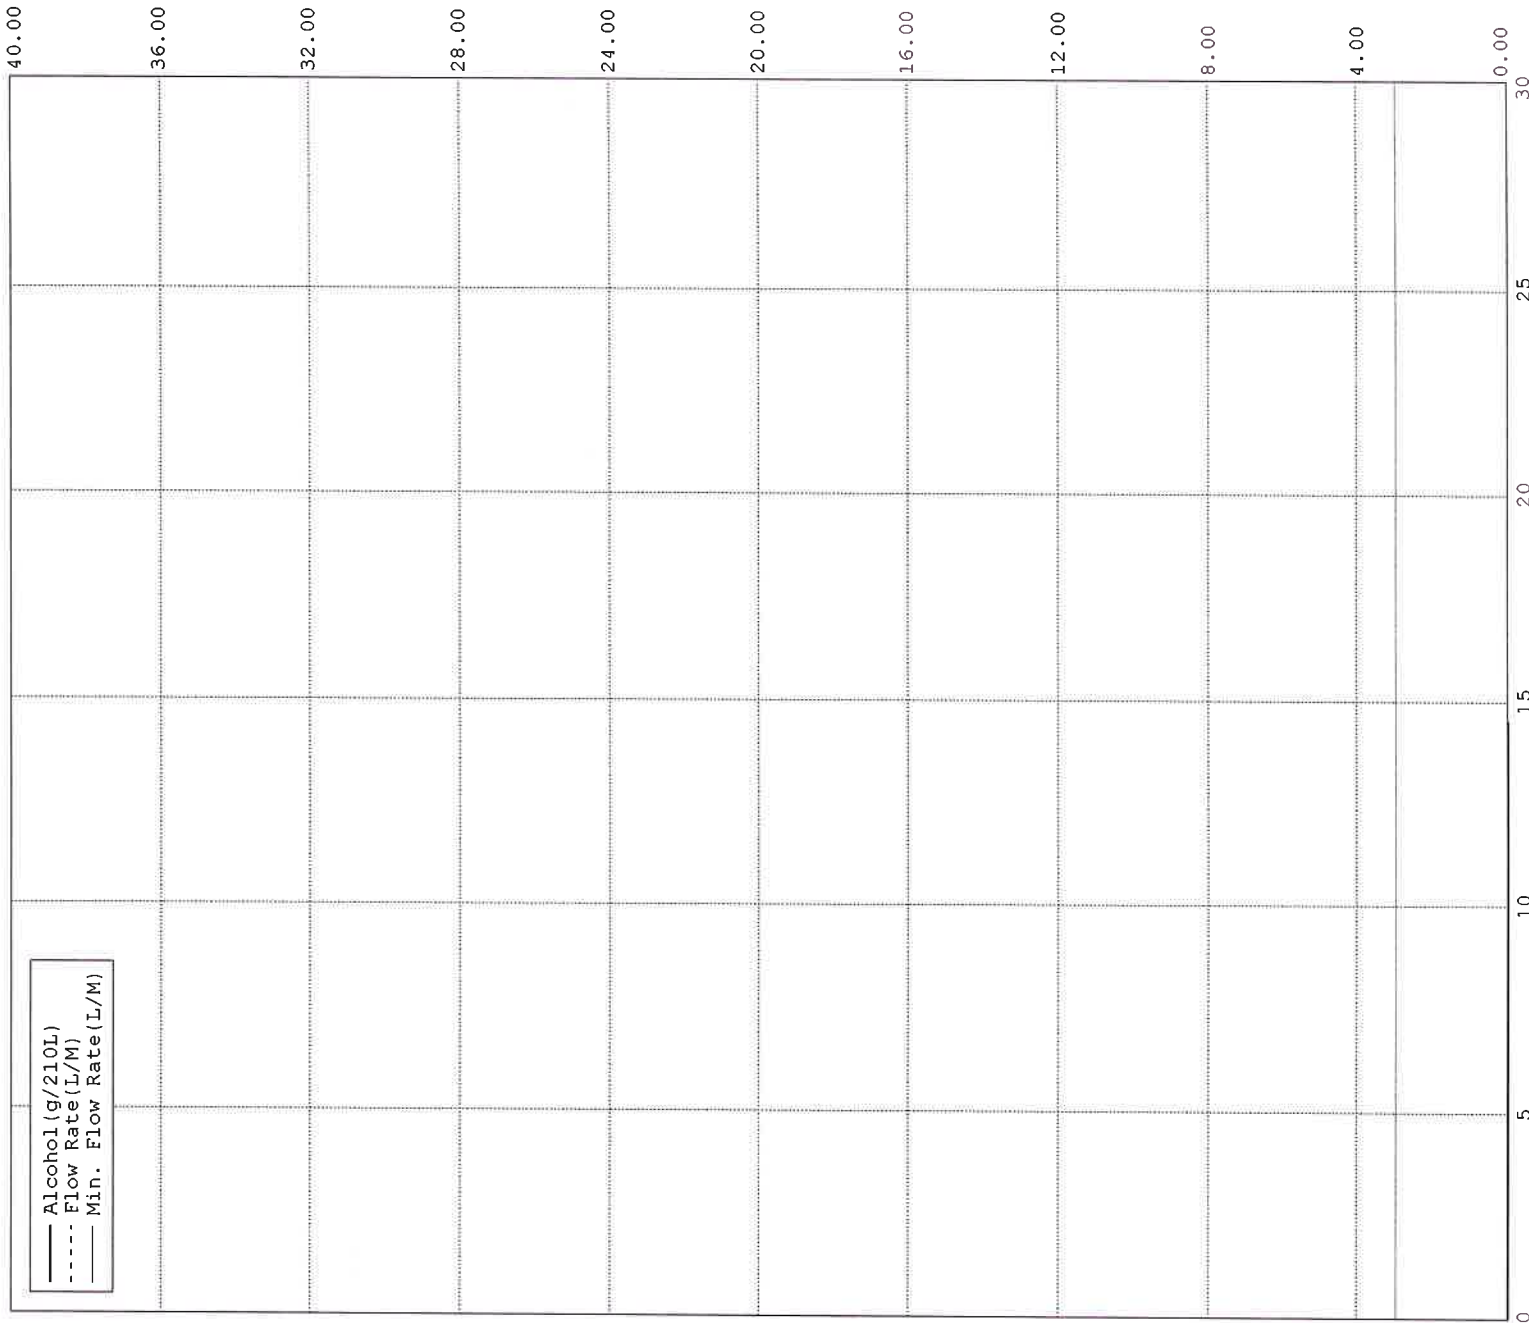

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100398

Date: 04/16/2025
 Time: 11:35:29

SUBJECT NAME:
 TEST TEST
 LICENSE #: INT-ACETONE

OPERATOR NAME:
 COLLEEN S O'BRYAN
 OPERATOR'S #: 6237


DEPT/AGENCY:
 AAA1
 CASE/REPORT: 25-1234
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.52: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:36
BLANK TEST	0.000	11:36
INTERNAL STANDARD	VERIFIED	11:36
Xq = 0.083 (0.53%)		
EXTERNAL STANDARD	0.079	11:37
X[1] = 0.0790 (-0.0017)	(0.0031)	
BLANK TEST	0.000	11:38
SUBJECT SAMPLE	XXX	11:38
X[1] = 0.1072 (-0.0223)	(0.0021)	

Interference Detected

OB

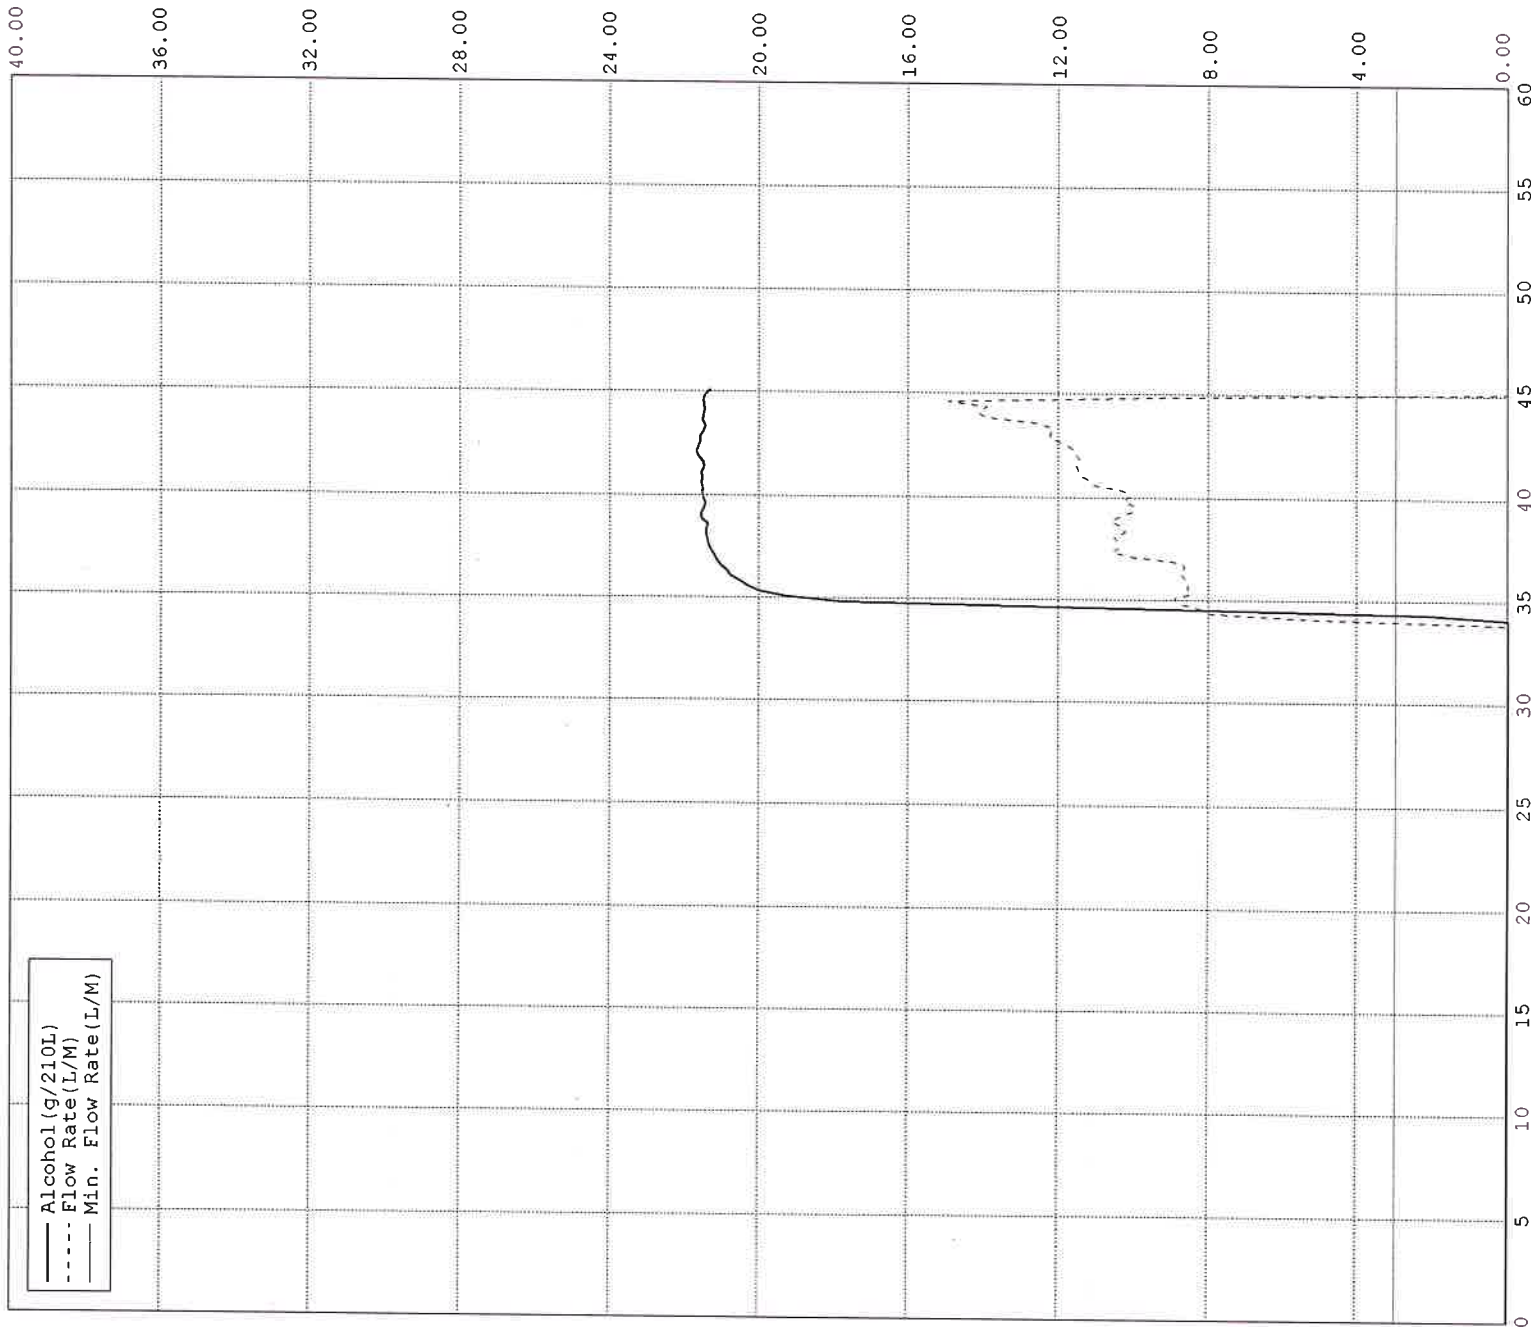

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100398

Date: 04/16/2025
Time: 11:44:04

SUBJECT NAME:
TEST TEST
LICENSE #: INT-IPA

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237


DEPT/AGENCY:
AAA1
CASE/REPORT: 25-1234
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.50: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:45
BLANK TEST	0.000	11:45
INTERNAL STANDARD	VERIFIED	11:45
$X_q = 0.082$ (0.11%)	0.079	11:45
EXTERNAL STANDARD	(0.0030)	
$X[1] = 0.0789$ (-0.0010)	0.000	11:46
BLANK TEST	XXX	11:47
SUBJECT SAMPLE	(0.0043)	
$X[1] = 0.1183$ (-0.0314)		

Interference Detected

Handwritten signature

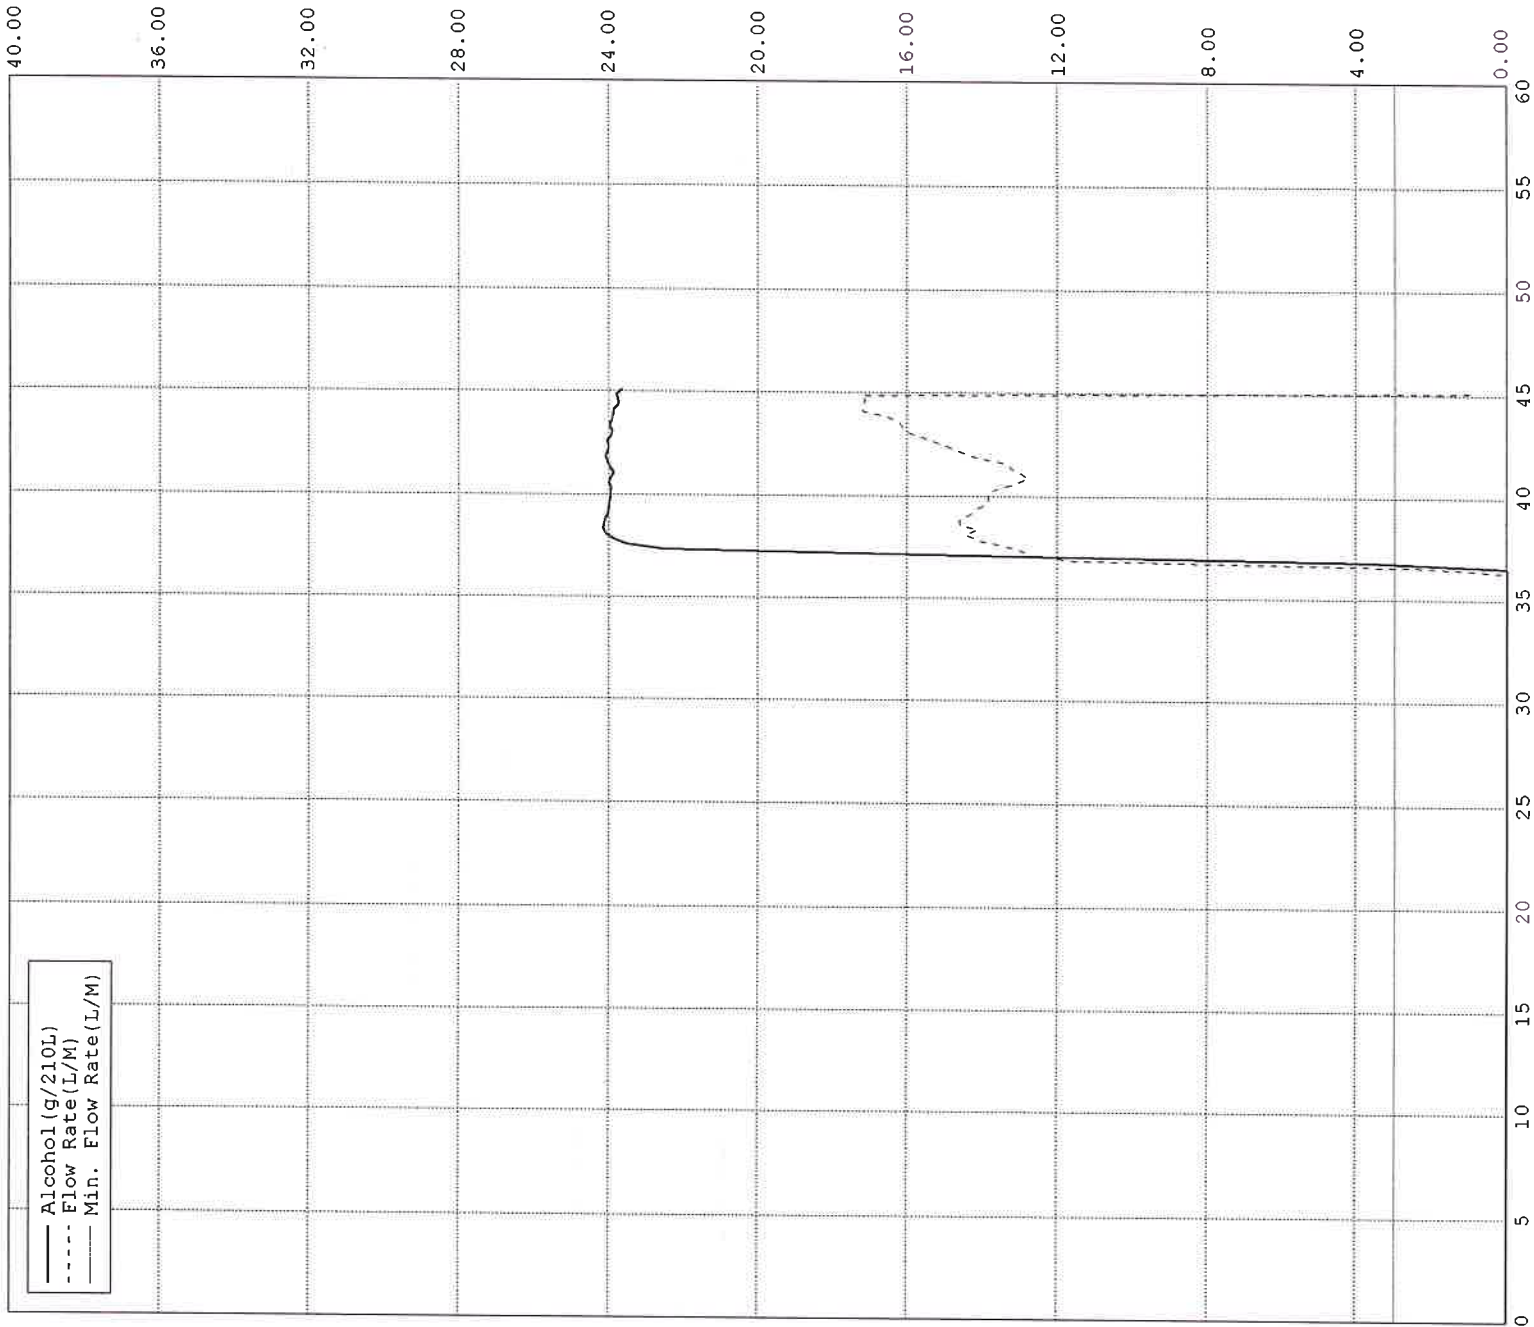

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100398

Date: 04/16/2025
Time: 11:58:56

SUBJECT NAME:
TEST TEST
LICENSE #: INT-NEGATIVE

OPERATOR NAME:
COLLEEN S O'BRYAN
OPERATOR'S #: 6237

DEPT/AGENCY:
AAA1

CASE/REPORT: 25-1234
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION


NOMINAL: 0.080
TARGET AT 29.50: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:00
BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
Xq = 0.083 (0.85%)		
EXTERNAL STANDARD	0.079	12:01
X[1] = 0.0793 (-0.0007)	(0.0032)	
BLANK TEST	0.000	12:02
SUBJECT SAMPLE (Vol=1.93L)	0.093	12:03
X[1] = 0.0933 (-0.0021)	(0.0023)	
BLANK TEST	0.000	12:04
EXTERNAL STANDARD	0.079	12:04
X[1] = 0.0785 (-0.0009)	(0.0025)	
BLANK TEST	0.000	12:05

Filter 2 avg - -0.0011
Filter 3 avg - 0.0030

COB 2025.04.16

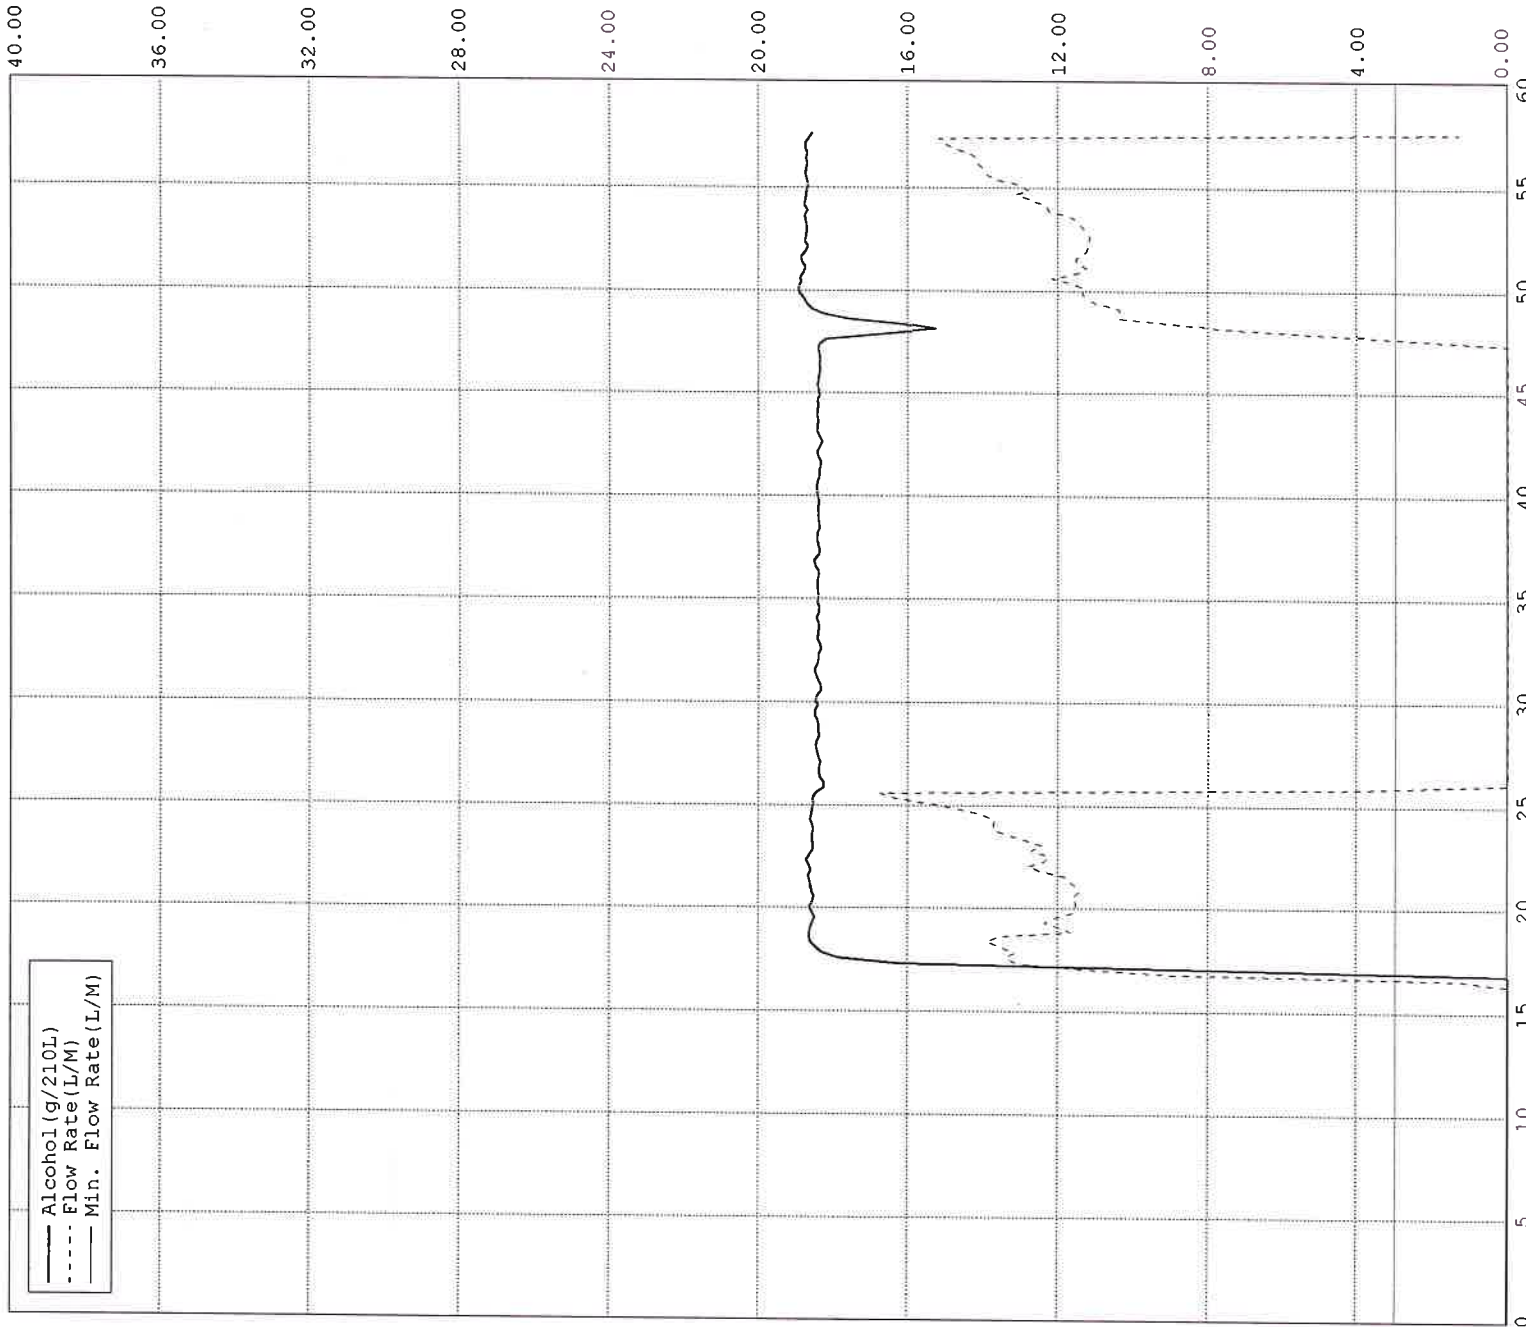

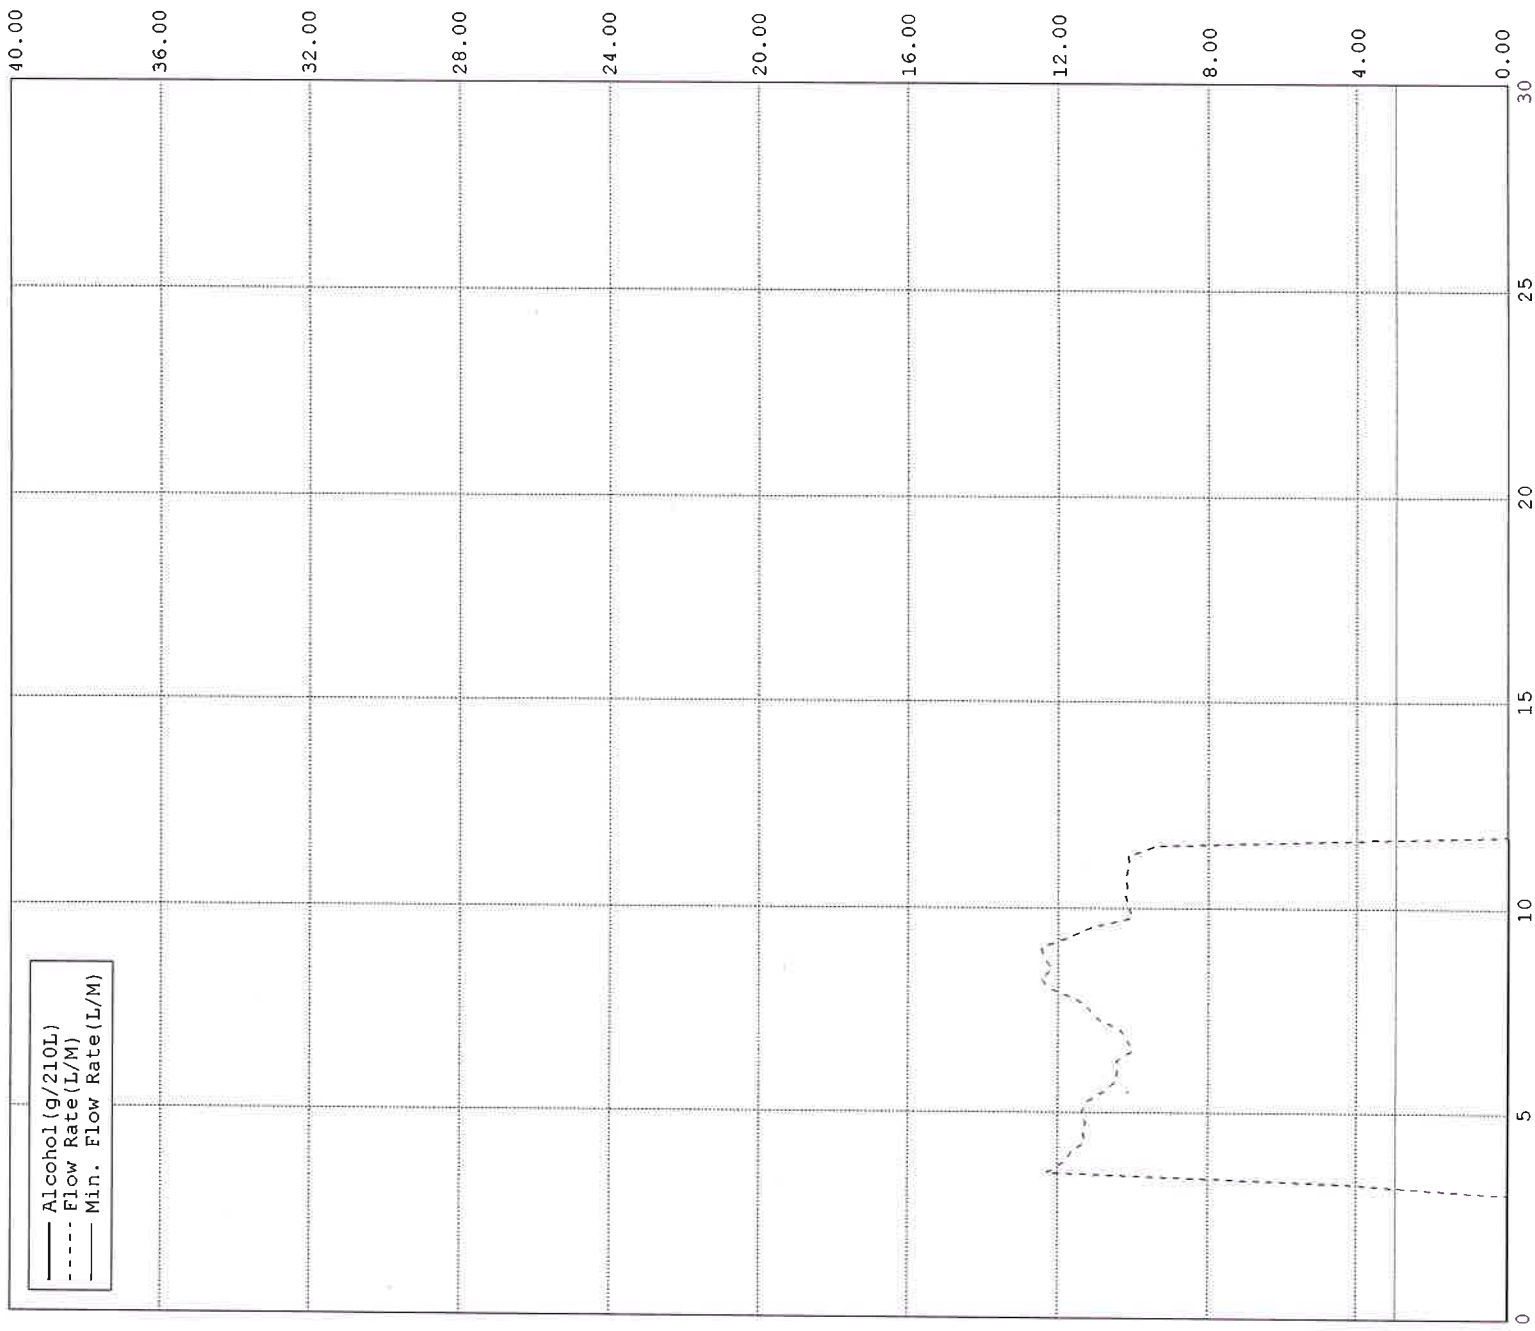

SUBJECT TEST	
Alaska Department of Public Safety DATAMASTER dmt: 100398	
Date: 04/16/2025 Time: 12:28:51	
SUBJECT NAME: TEST TEST LICENSE #: NDST	
OPERATOR NAME: COLLEEN S OBRYANT OPERATOR'S #: 6237	
DEPT/AGENCY: AAA1	
CASE/REPORT: 25-1234 TEST TYPE: TEST	
EXTERNAL STANDARD INFORMATION NOMINAL: 0.080 TARGET AT 29.49: 0.079 LOT #: AG335202 EXPIRATION: 12/18/2025	
DIAGNOSTIC CHECK	PASSED 12:29
BLANK TEST	0.000 12:29
INTERNAL STANDARD	VERIFIED 12:30
EXTERNAL STANDARD	0.079 12:30
BLANK TEST	0.000 12:31
SUBJECT SAMPLE (Vol=1.54L)	0.000 12:31
BLANK TEST	0.000 12:32
EXTERNAL STANDARD	0.079 12:32
BLANK TEST	0.000 12:33

