




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100399

Report Issue Date: 06/17/2025
Date Received: Not Recorded
Condition of Item: Not Recorded

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

No As-Found Data Collected

As-Left Data

Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.021	0.022	0.019	0.022	0.021	+/- 0.002
0.040	0.040	AG407908	0.040	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG335202	0.079	0.079	0.078	0.079	0.079	0.079	+/- 0.004
0.100	0.100	AG333401	0.101	0.101	0.101	0.101	0.101	0.101	+/- 0.004
0.150	0.150	AG332004	0.149	0.148	0.148	0.148	0.148	0.148	+/- 0.006
0.300	0.301	AG427706	0.301	0.301	0.300	0.300	0.300	0.300	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 30.00 Barometer Used: VWR S/N 240680771 Temperature (C): 24.4 Relative Humidity (%): 23

As-Left Lab Activity Date Range: 06/11/2025 - 06/12/2025

Instrument does not upload, and the tank was not removed because the instrument is currently used in-house.

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock

Results authorized by Megan Carlock on 06/17/2025

megan.crouse@alaska.gov

Technically and administratively reviewed by Colleen O'Bryant on 06/17/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100399 (Morse) Analyst or Technician Name: Megan Corlock

DataMaster DMT Calibration Start Date: 6/11/25

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/26
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 30.00 Temperature(C) 24.4 Relative Humidity(%) 23

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) - Print with View Details
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20250603KS Expiration Date: 9/3/25 ^{NMC 6/17/25} Acetone - 7/27/25
Simulator S/N: SD1200 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20250603KS Expiration Date: 9/3/25
Simulator S/N: SD1198 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 23IP41233 Expiration Date: 9/20/25
Simulator S/N: SD1199 Thermometer Verification Performed? ☒ ^{sim exp: 9/10/25}

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/2025

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

* Instrument does not upload, kept in-house

** Tank was not removed because this instrument is used internally currently
NMC 6/11/25

Completion

Lab Work End Date: 6/11/25

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 6/12/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100399

Date: 06/11/2025
 Time: 08:33:30

VERSIONS
 DMT: 3.02
 PIC: 3.03
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 48.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.82 V	PASSED
(1.00 V - 2.32 V)	
Cooler Voltage = 1.58 V	PASSED
(0.99 V - 2.31 V)	
Bias Voltage = 81 V	PASSED
(49 V - 113 V)	
Chopper Freq = 524 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 30.0 in	

PUMP INFO

Flow Rate = 4.551 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.003 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

	PASSED
Xq = 0.085 0.72% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100399

Date: 06/11/2025

Time: 8:48 AM

Temperatures (°C)

Sample Cell: 48.8°C

Breath Tube: 46.3°C

Current Barometer 30.0 in

Volume (Ltr) 1.56

Settings

Lamp: 1.79 V

Bias: 81 V

Cooler: 1.65 V

Chopper: 524 Hz

Voltages (V)

Flow: 1.06 V

Detector: -0.004 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 07/26/2021
Time: 14:45:57

OPERATOR NAME:
BRANDI BARNETT
CERTIFICATE #: 7038

Ca	=	0.1000		
CAL	=	0.997064	0.800	<= CAL < 1.200
b1	=	0.0003	0.0000	<= b1 < 0.0040
b2	=	0.0053	0.0010	<= b2 < 0.0100
b3	=	0.0003	0.0000	<= b3 < 0.0040
Xq	=	0.0844	0.0500	<= Xq < 0.2000
a21	=	1.216343	1.050	<= a21 < 1.300
a31	=	0.426899	0.300	<= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 06/11/2025
Time: 10:29:08

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.01: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:30
BLANK TEST	0.000	10:30
INTERNAL STANDARD	VERIFIED	10:30
EXTERNAL STANDARD	0.079	10:30
BLANK TEST	0.000	10:31
SUBJECT SAMPLE (Vol=1.61L)	0.000	10:32
BLANK TEST	0.000	10:33
EXTERNAL STANDARD	0.080	10:33
BLANK TEST	0.000	10:34

MNC

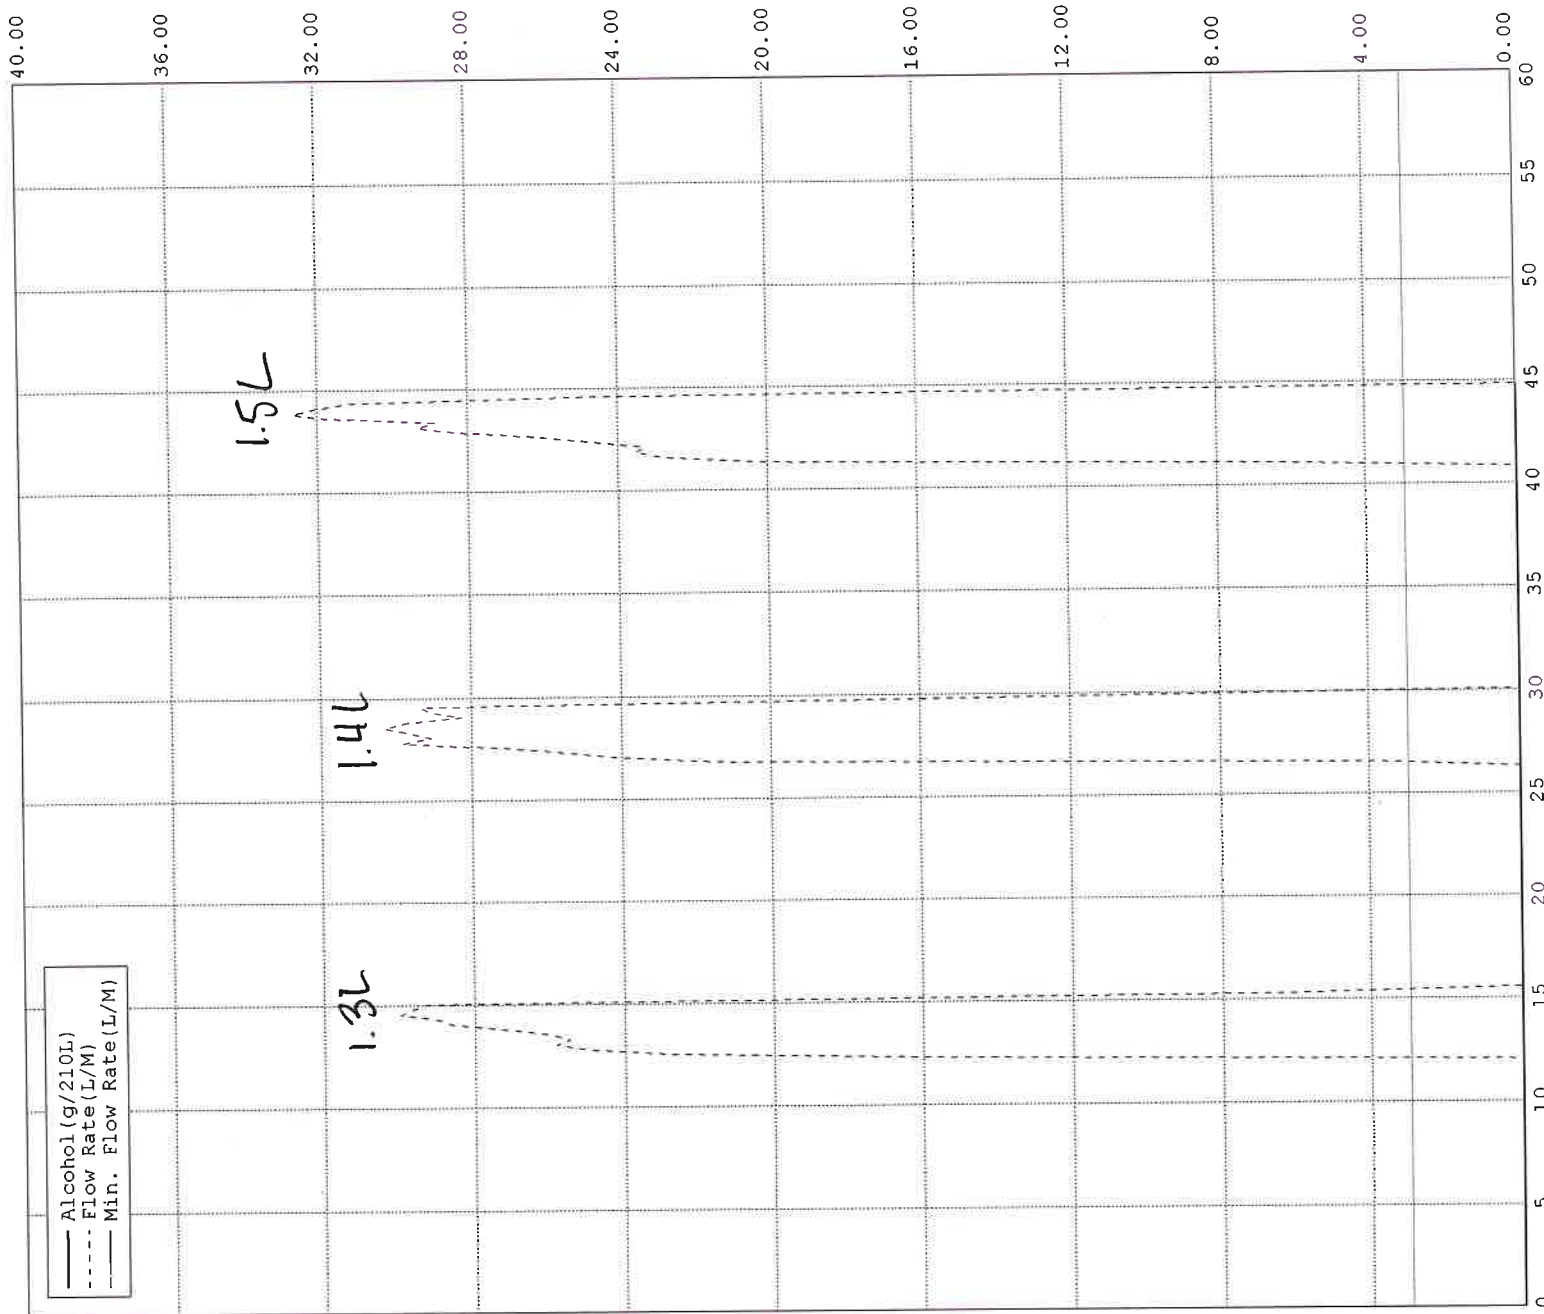

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100399

Date: 06/11/2025
 Time: 10:36:20

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0210	0.0012
0.040	0.0400	0.0000
0.080	0.0788	0.0004
0.100	0.1010	0.0000
0.150	0.1482	0.0004
0.301	0.3004	0.0005

SLOPE = 0.995333
 R^2 = 0.999893

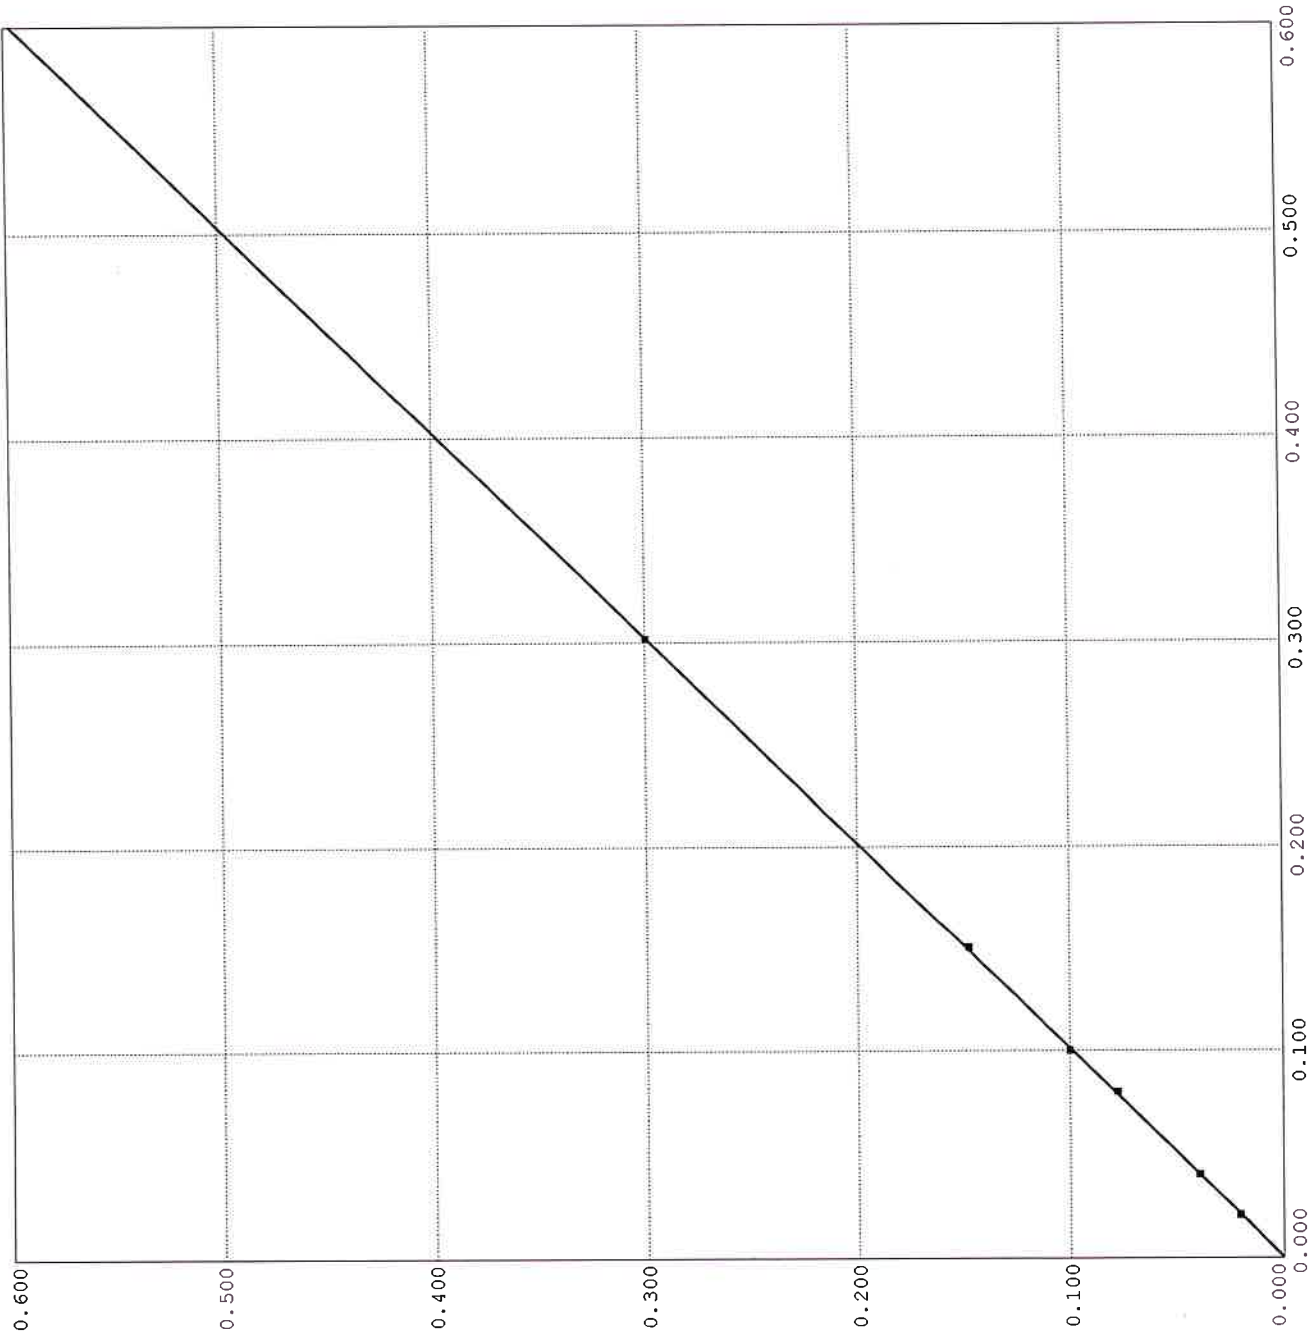

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 06/11/2025
Time: 10:39:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 30.01: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 1160 psi

BLANK TEST	0.000	10:40
INTERNAL STANDARD	VERIFIED	10:41
EXTERNAL STANDARD	0.021	10:41
BLANK TEST	0.000	10:42
EXTERNAL STANDARD	0.021	10:42
BLANK TEST	0.000	10:43
EXTERNAL STANDARD	0.022	10:43
BLANK TEST	0.000	10:44
EXTERNAL STANDARD	0.019	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.022	10:45
BLANK TEST	0.000	10:46

Average = 0.0210
Std Dev = 0.0012

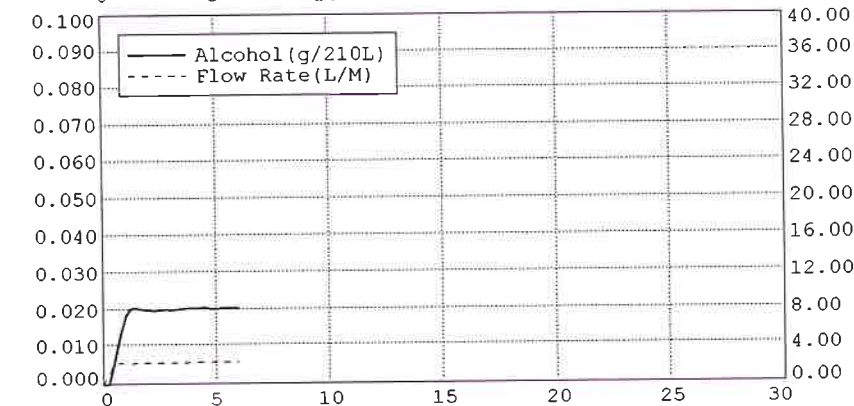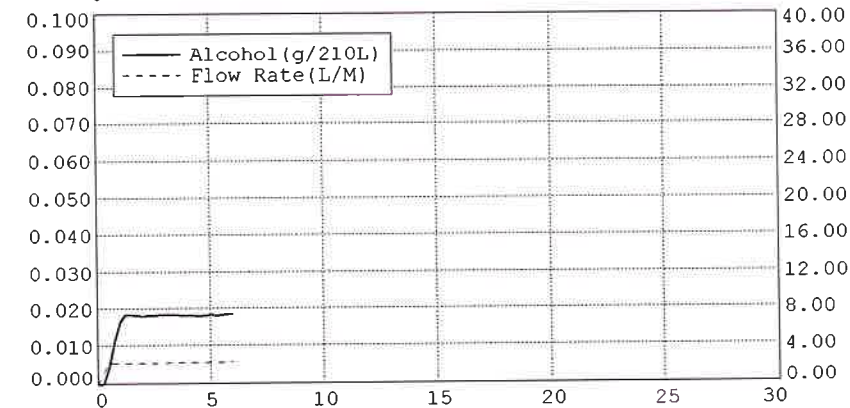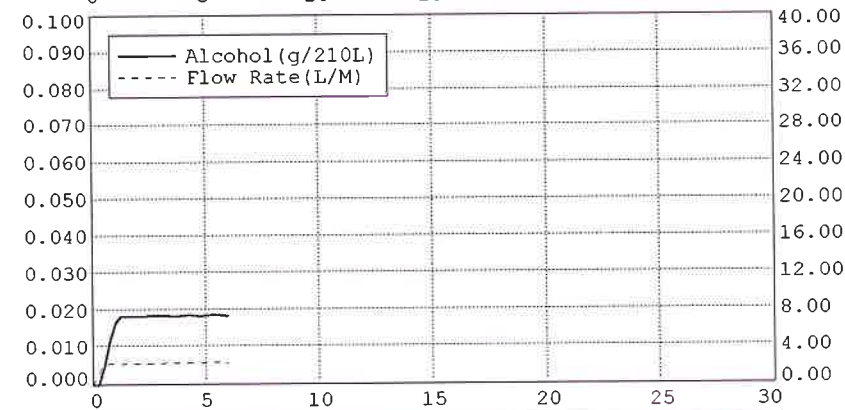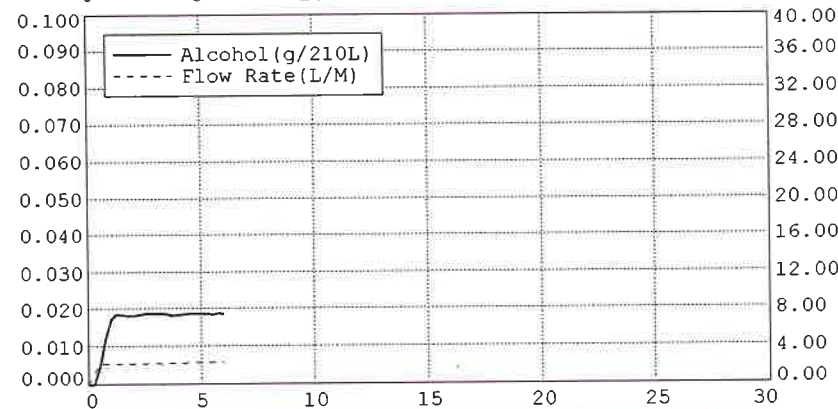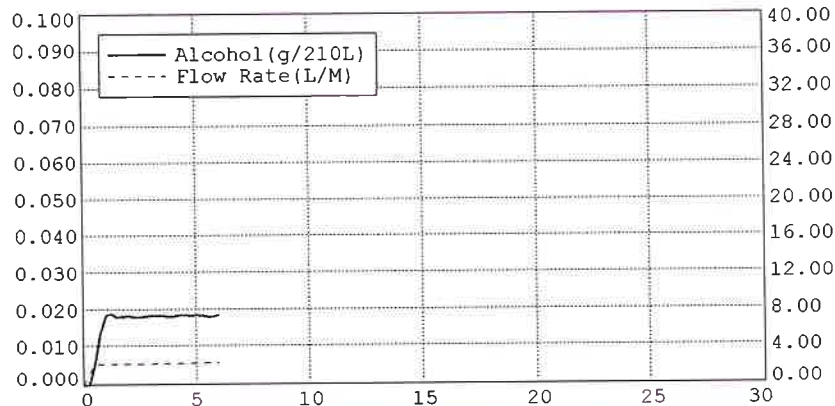

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 06/11/2025
Time: 10:47:52

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 30.01: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 1080 psi

BLANK TEST	0.000	10:49
INTERNAL STANDARD	VERIFIED	10:49
EXTERNAL STANDARD	0.040	10:50
BLANK TEST	0.000	10:50
EXTERNAL STANDARD	0.040	10:51
BLANK TEST	0.000	10:52
EXTERNAL STANDARD	0.040	10:52
BLANK TEST	0.000	10:53
EXTERNAL STANDARD	0.040	10:53
BLANK TEST	0.000	10:54
EXTERNAL STANDARD	0.040	10:54
BLANK TEST	0.000	10:55

Average = 0.0400
Std Dev = 0.0000

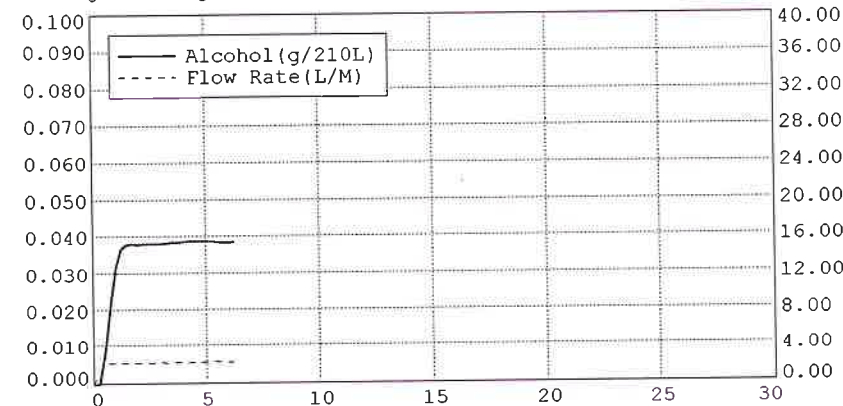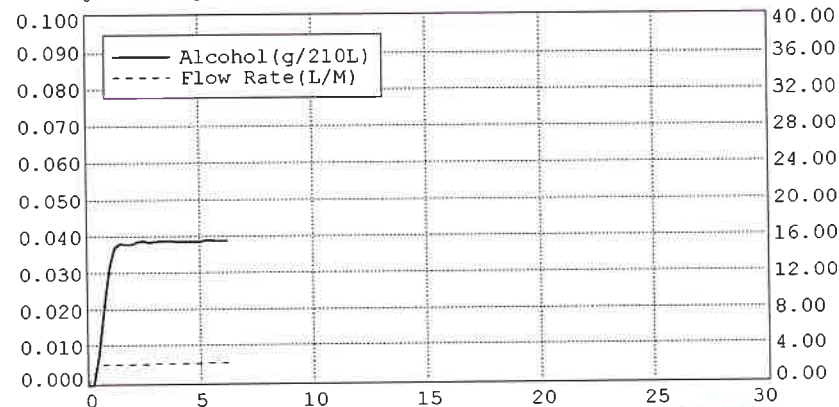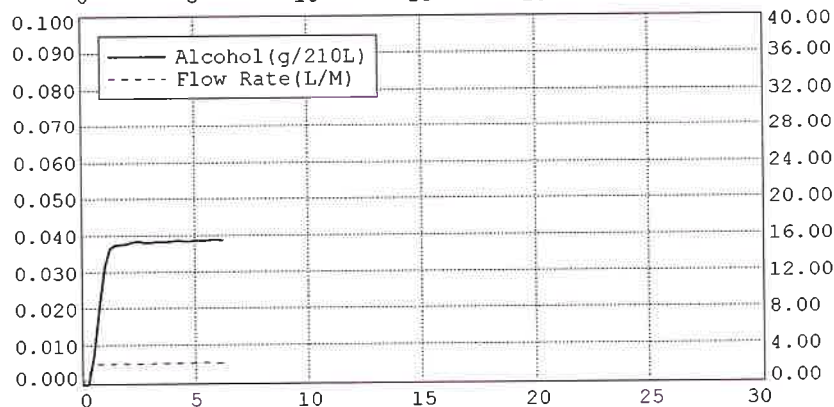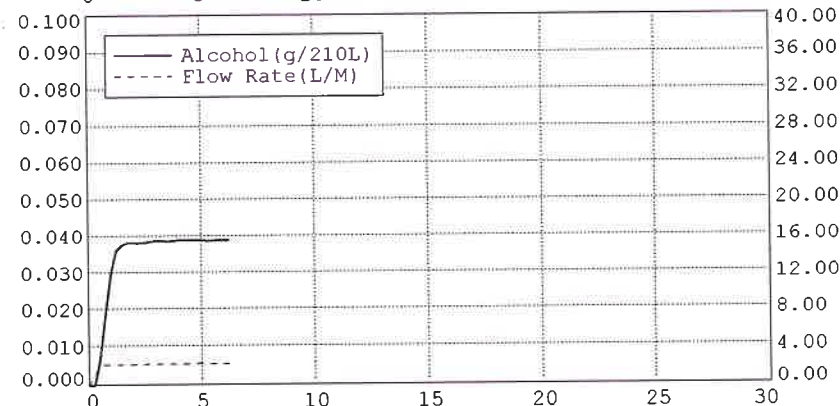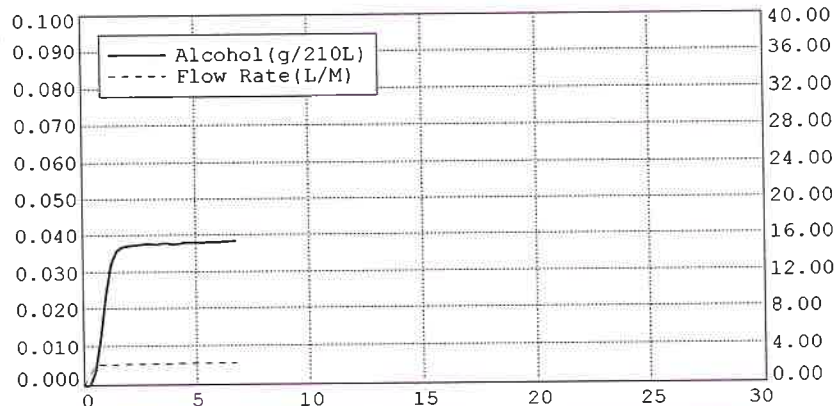

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 06/11/2025
Time: 10:55:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.01: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 191 psi

BLANK TEST	0.000	10:57
INTERNAL STANDARD	VERIFIED	10:57
EXTERNAL STANDARD	0.079	10:57
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.079	10:59
BLANK TEST	0.000	10:59
EXTERNAL STANDARD	0.078	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.079	11:01
BLANK TEST	0.000	11:02
EXTERNAL STANDARD	0.079	11:02
BLANK TEST	0.000	11:03

Average = 0.0788
Std Dev = 0.0004

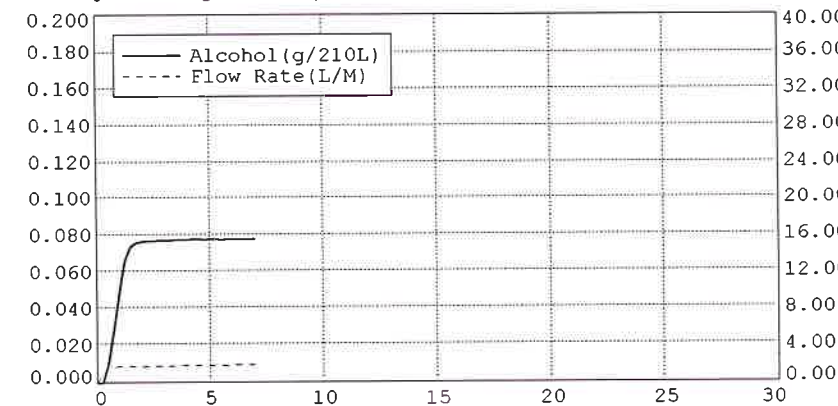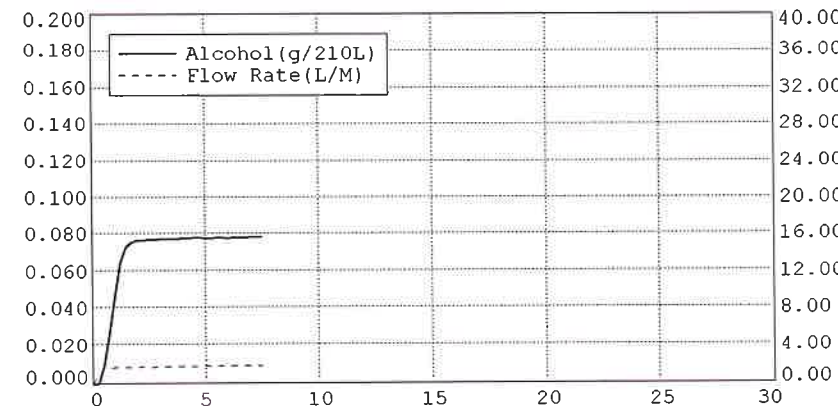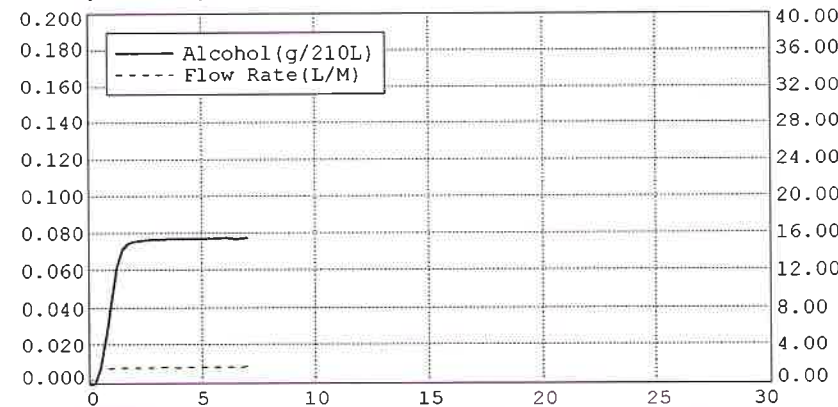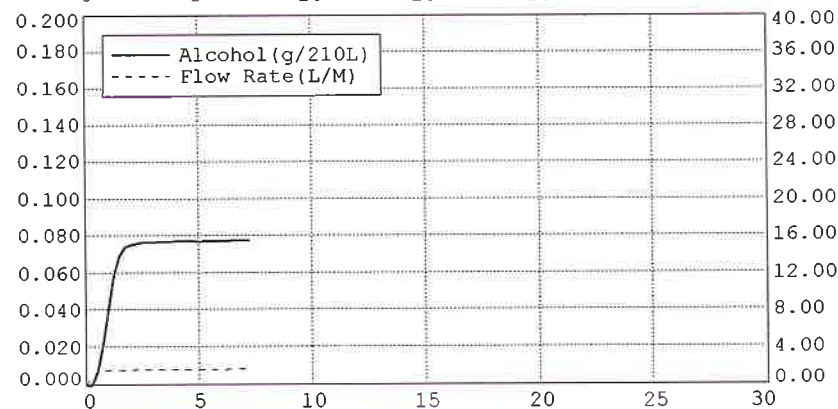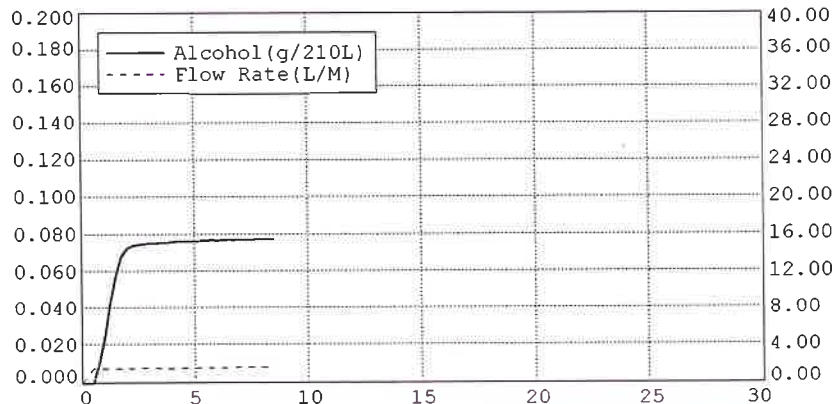

LINEARITY CHECK: Control Test 4






Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 06/11/2025
Time: 11:06:38

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.100
TARGET AT 30.00: 0.100
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 1012 psi

BLANK TEST	0.000	11:08
INTERNAL STANDARD	VERIFIED	11:08
EXTERNAL STANDARD	0.101	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.101	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.101	11:11
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.101	11:12
BLANK TEST	0.000	11:13
EXTERNAL STANDARD	0.101	11:13
BLANK TEST	0.000	11:14

Average = 0.1010
Std Dev = 0.0000

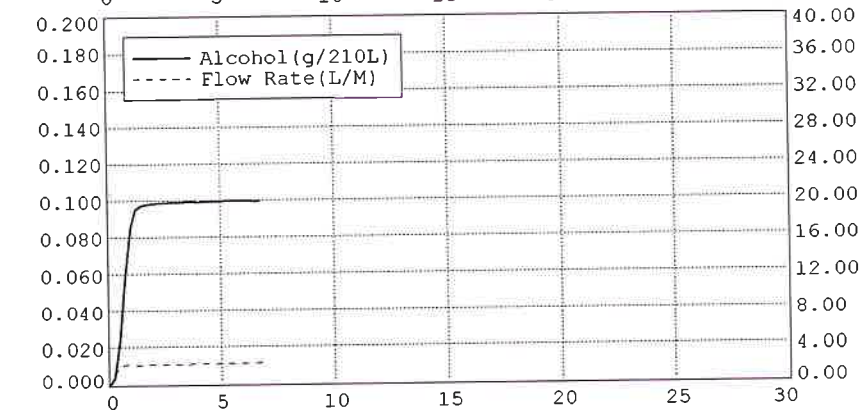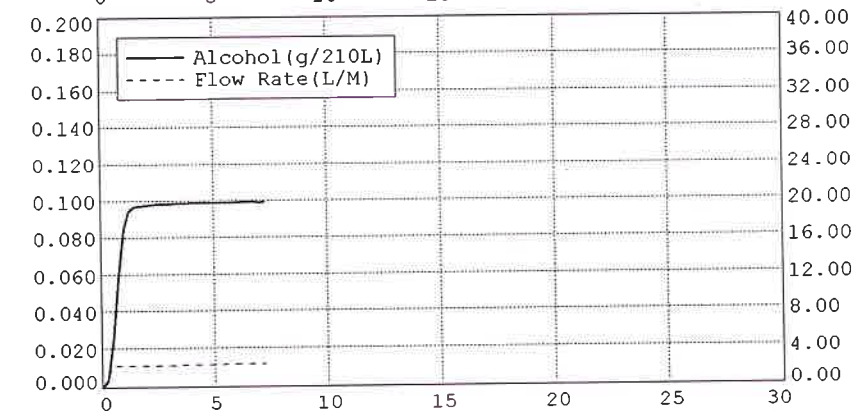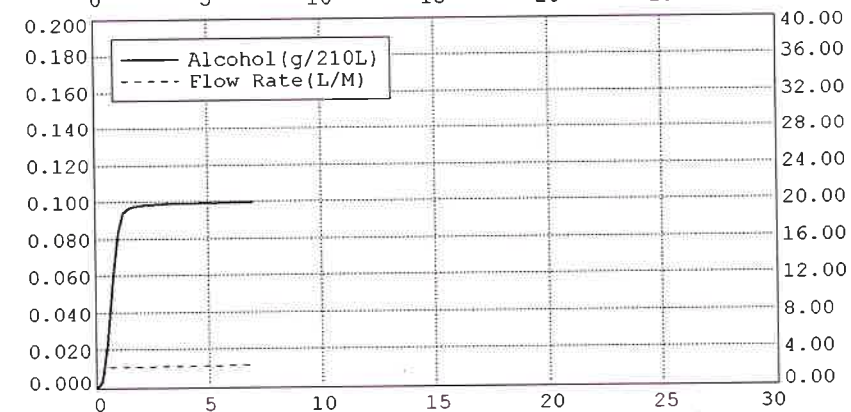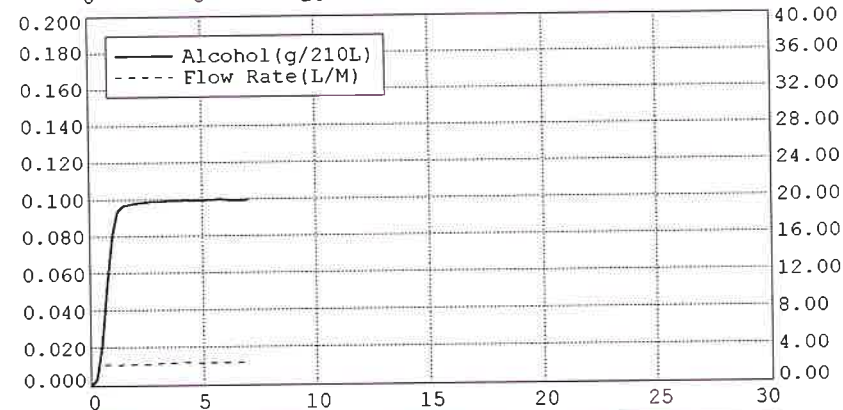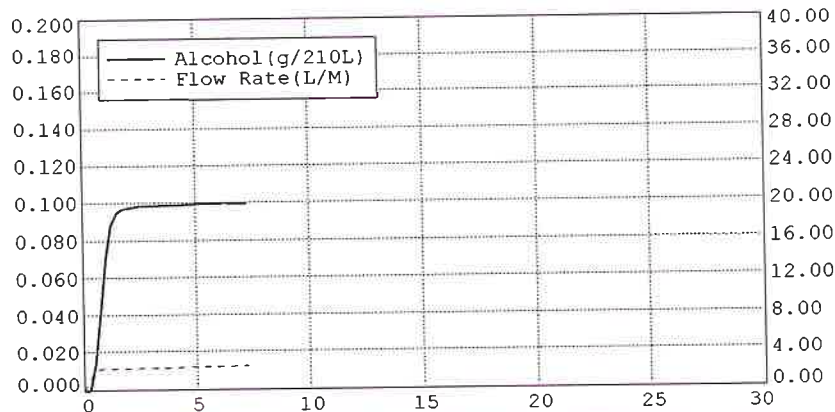

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 06/11/2025
Time: 11:18:39

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 30.00: 0.150
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 239 psi

BLANK TEST	0.000	11:20
INTERNAL STANDARD	VERIFIED	11:20
EXTERNAL STANDARD	0.149	11:21
BLANK TEST	0.000	11:21
EXTERNAL STANDARD	0.148	11:22
BLANK TEST	0.000	11:23
EXTERNAL STANDARD	0.148	11:23
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.148	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.148	11:25
BLANK TEST	0.000	11:26

Average = 0.1482
Std Dev = 0.0004

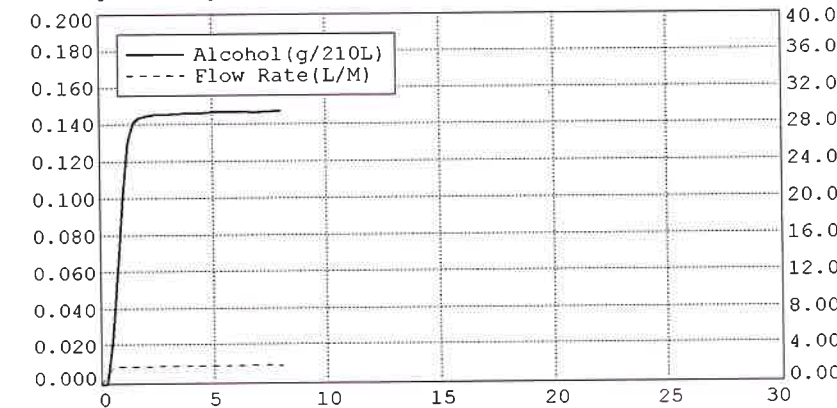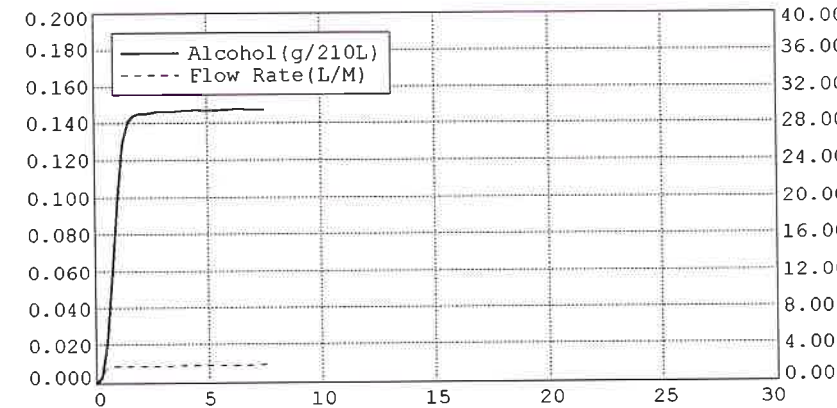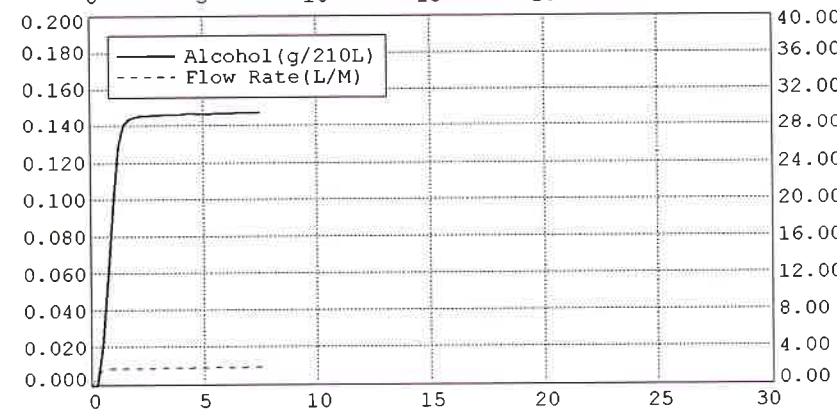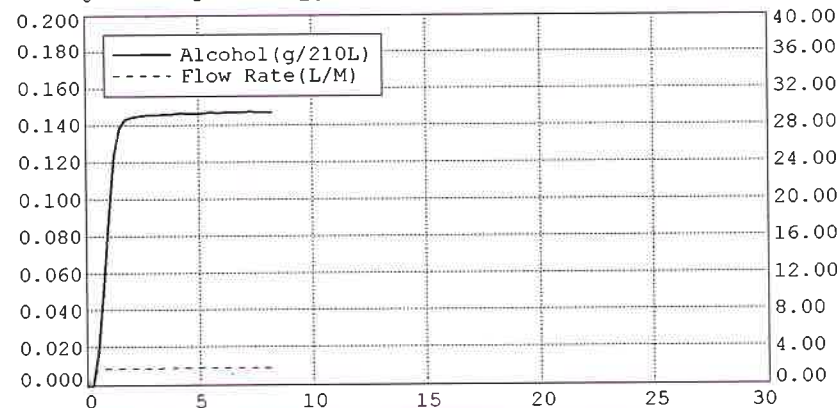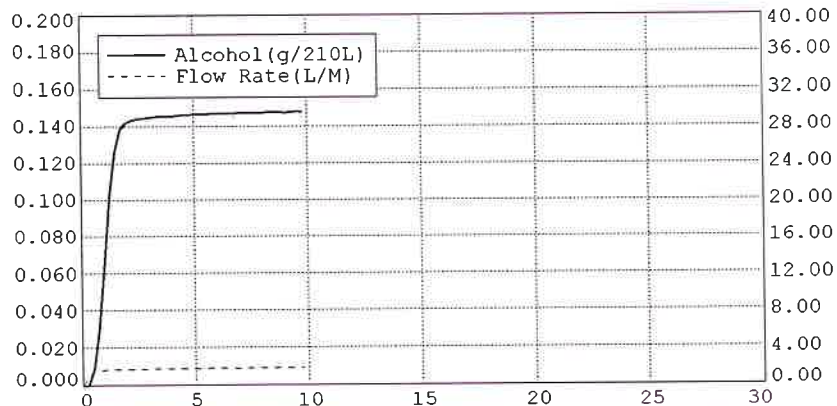

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100399






Date: 06/11/2025
Time: 11:27:35

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 30.00: 0.301
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 348 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	11:29
INTERNAL STANDARD	VERIFIED	11:29
EXTERNAL STANDARD	0.301	11:29
BLANK TEST	0.000	11:30
EXTERNAL STANDARD	0.301	11:31
BLANK TEST	0.000	11:32
EXTERNAL STANDARD	0.300	11:32
BLANK TEST	0.000	11:33
EXTERNAL STANDARD	0.300	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.300	11:34
BLANK TEST	0.000	11:35

Average = 0.3004
Std Dev = 0.0005

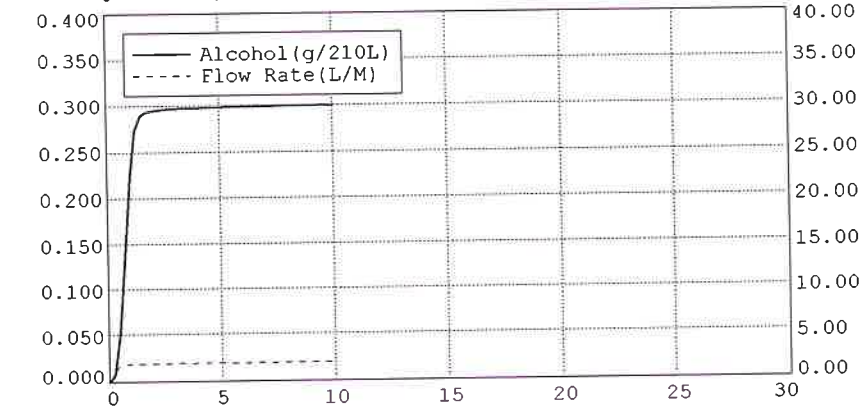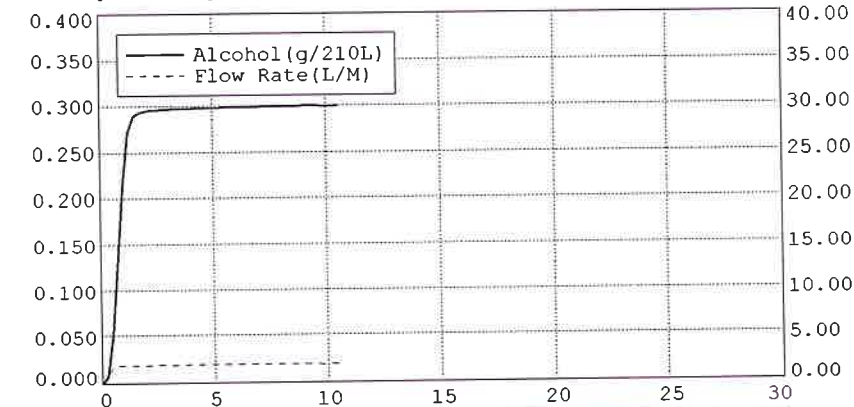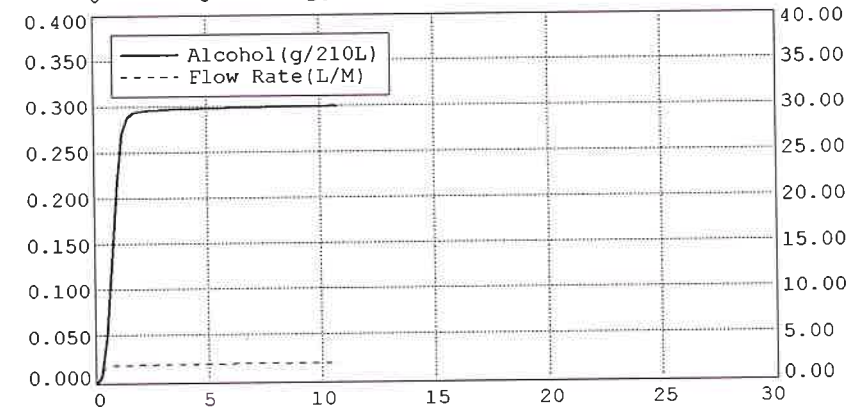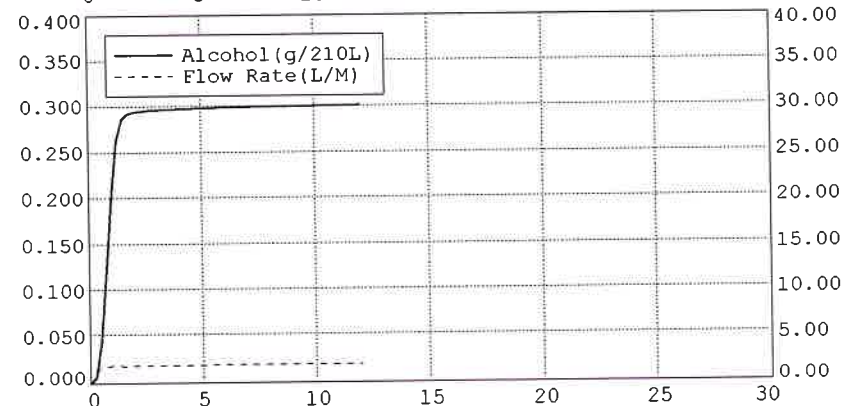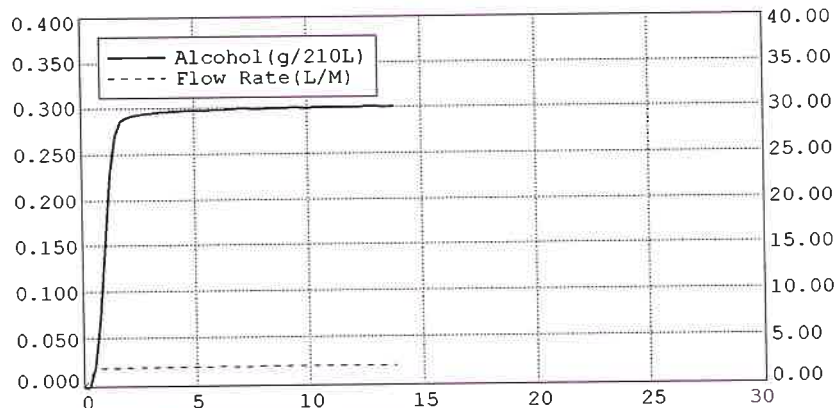

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 06/11/2025
Time: 11:40:15

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.99: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:41
BLANK TEST	0.000	11:41
INTERNAL STANDARD	VERIFIED	11:41
EXTERNAL STANDARD	0.081	11:41
BLANK TEST	0.000	11:42
SUBJECT SAMPLE	INCOMPLETE	11:44

MNC

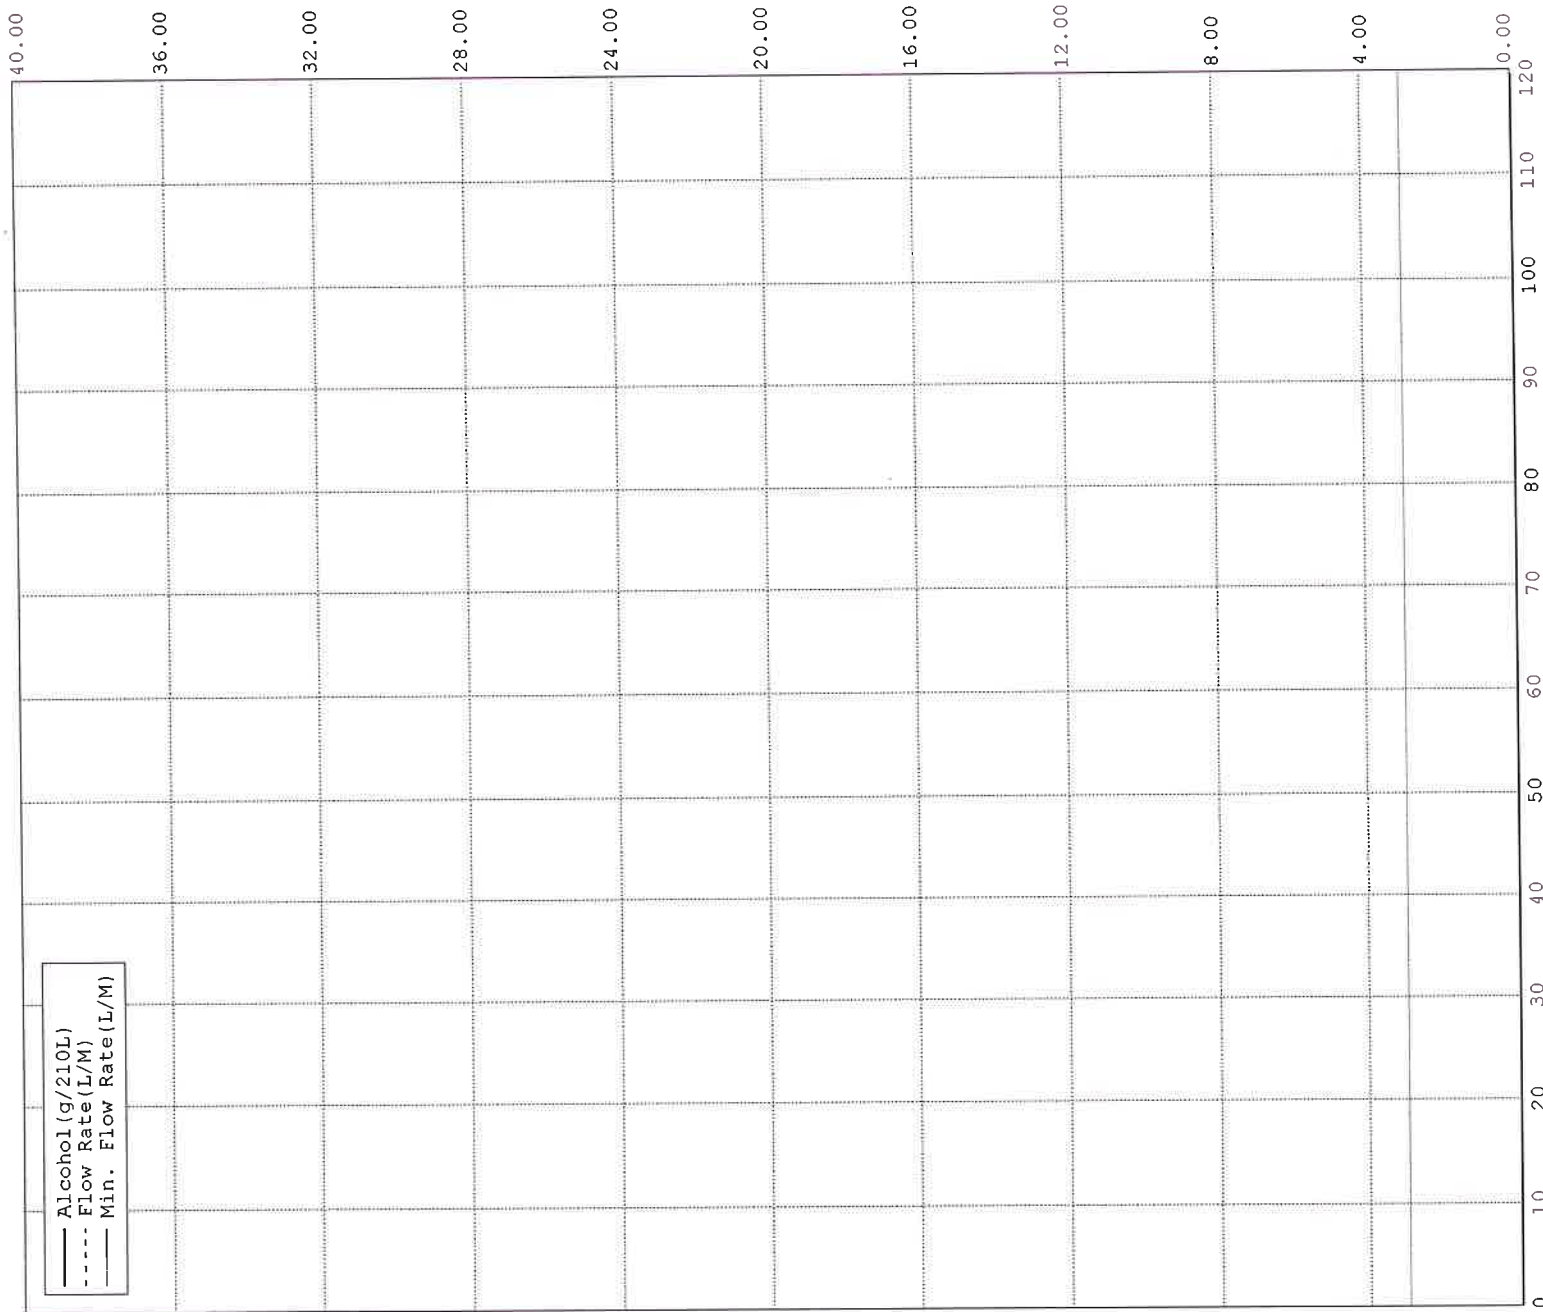

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 06/11/2025
Time: 11:47:57

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.99: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:48
BLANK TEST	0.000	11:49
INTERNAL STANDARD	VERIFIED	11:49
EXTERNAL STANDARD	0.080	11:49
BLANK TEST	0.000	11:50
SUBJECT SAMPLE	XXX	11:51

Maximum Attempts Exceeded

MNC

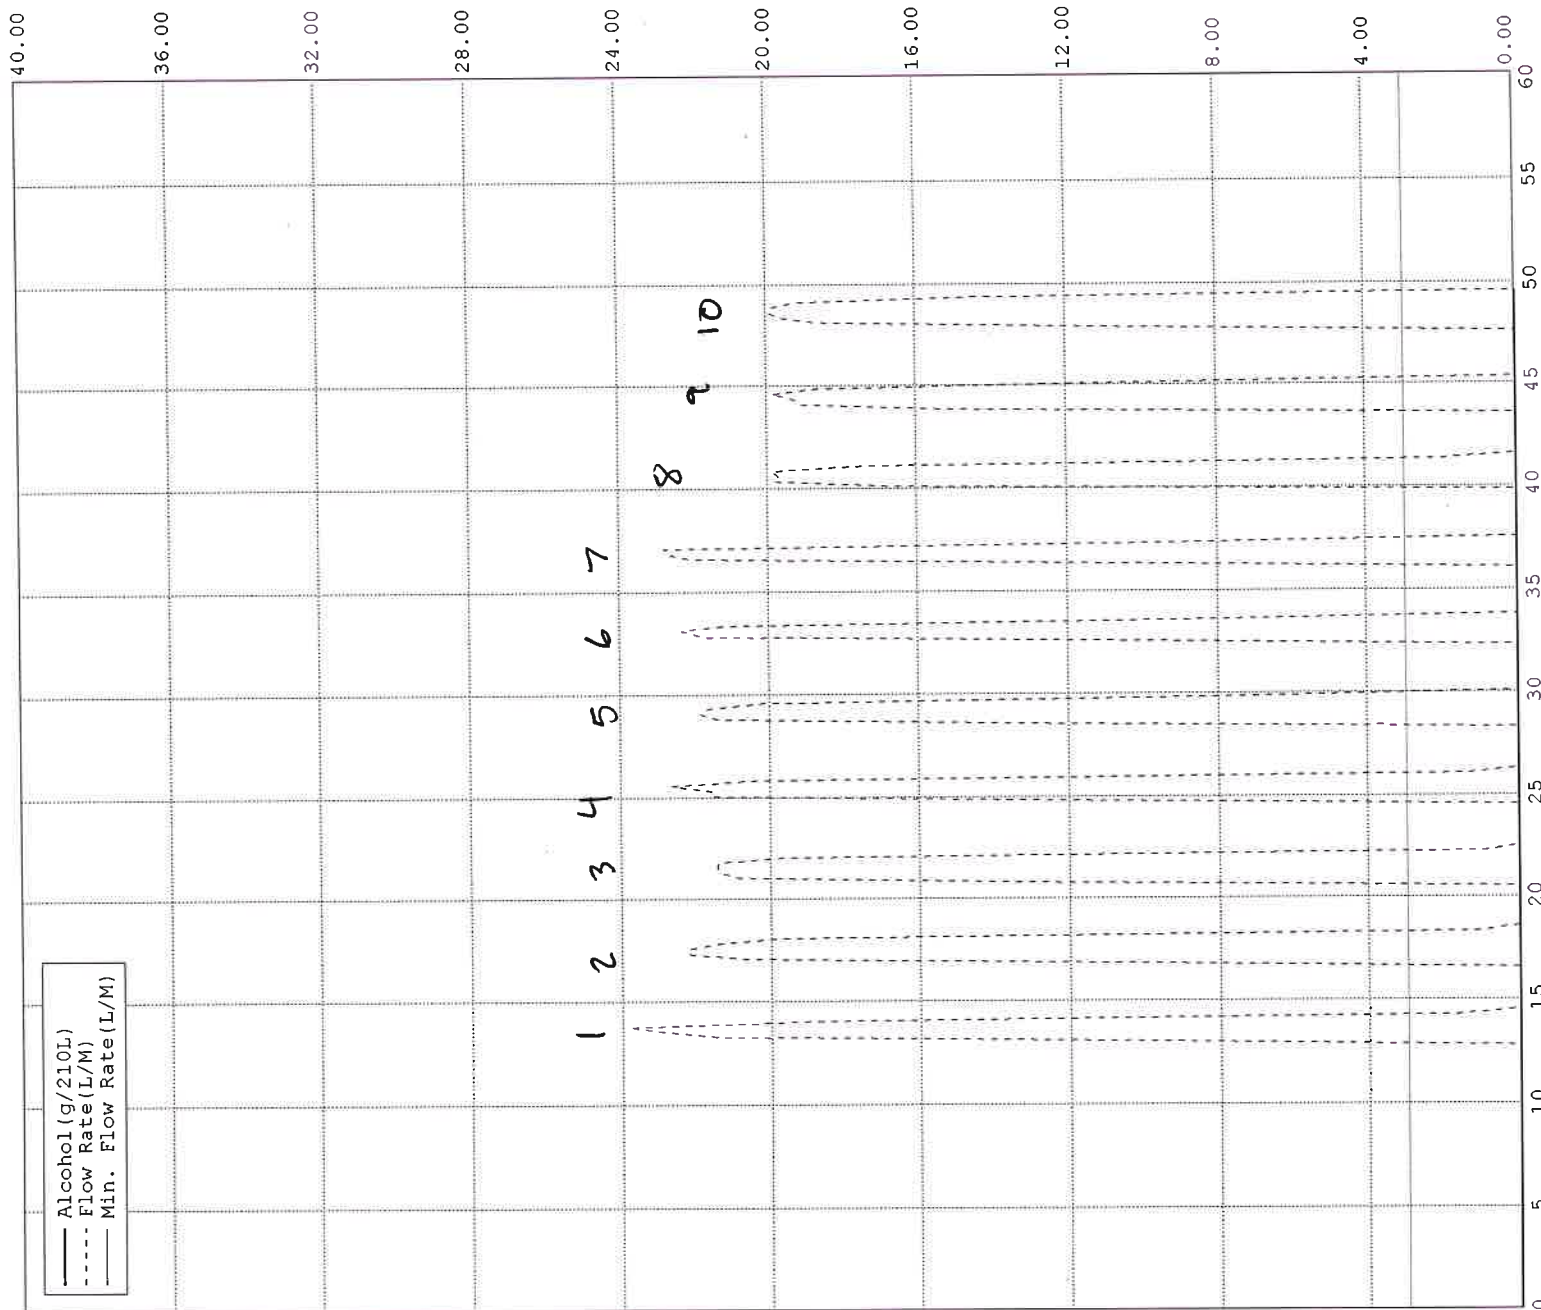

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100399

Date: 06/11/2025
Time: 11:57:42

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.98: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:58
BLANK TEST	0.000	11:58
INTERNAL STANDARD	VERIFIED	11:58
EXTERNAL STANDARD	0.080	11:59
BLANK TEST	0.000	12:00
SUBJECT SAMPLE	INVALID	12:00

MNC



SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100399

Date: 06/11/2025
Time: 12:10:24

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:

RFI
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.98: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:11
BLANK TEST	0.000	12:11
INTERNAL STANDARD	VERIFIED	12:11
EXTERNAL STANDARD	0.080	12:11
BLANK TEST	0.000	12:12

RFI DETECTED

MNC

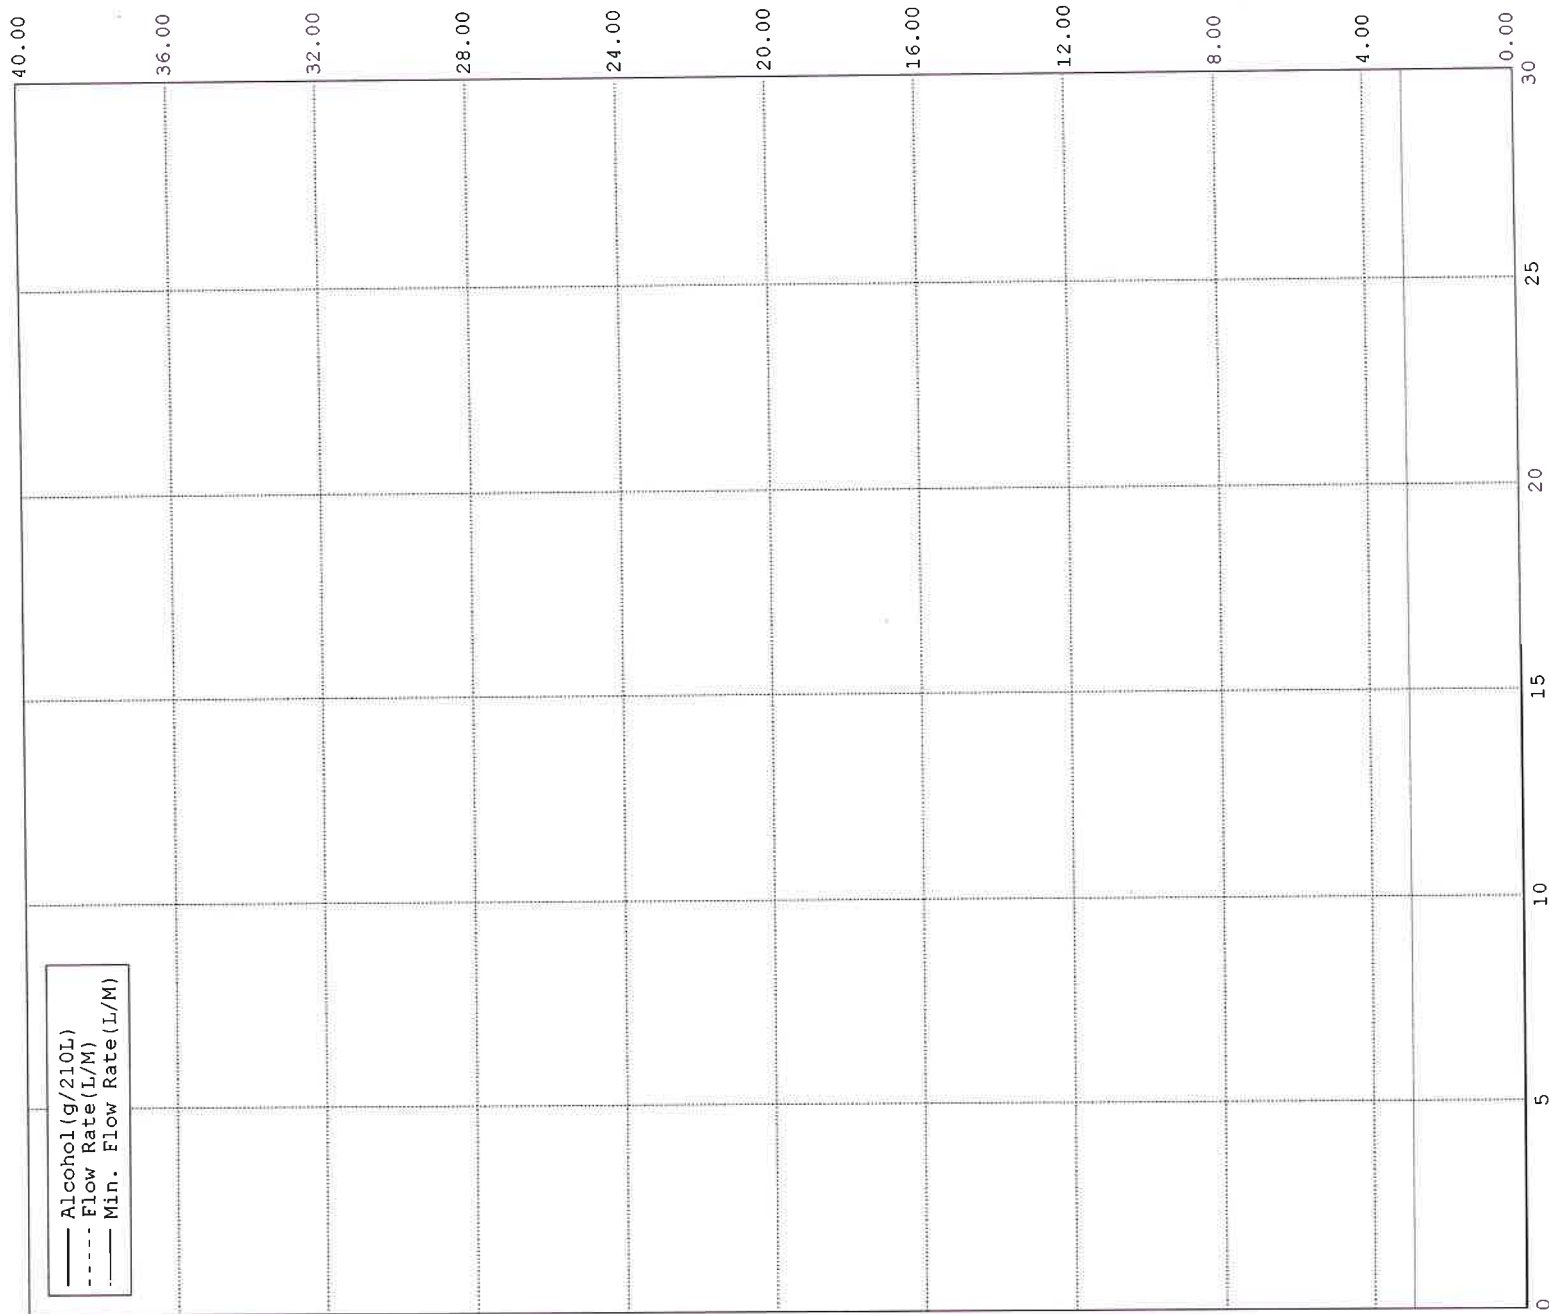

SUBJECT TEST

Alaska Department of Public Safety
 DATA MASTER dmt: 100399

Date: 06/11/2025
 Time: 14:16:43

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:
 INTERFERENCE - ACETONE
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.96: 0.080
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:17
BLANK TEST	0.000	14:17
INTERNAL STANDARD	VERIFIED	14:17
Xq = 0.085 (1.03%)	0.079	14:18
EXTERNAL STANDARD	(0.0022)	
X[1] = 0.0795 (-0.0010)	0.000	14:19
BLANK TEST	XXX	14:19
SUBJECT SAMPLE	(0.0002)	
X[1] = 0.1130 (-0.0228)		


Interference Detected

Filter 2 Average: -0.0008

Filter 3 Average: 0.0021

MNC 6/12/25

MNC

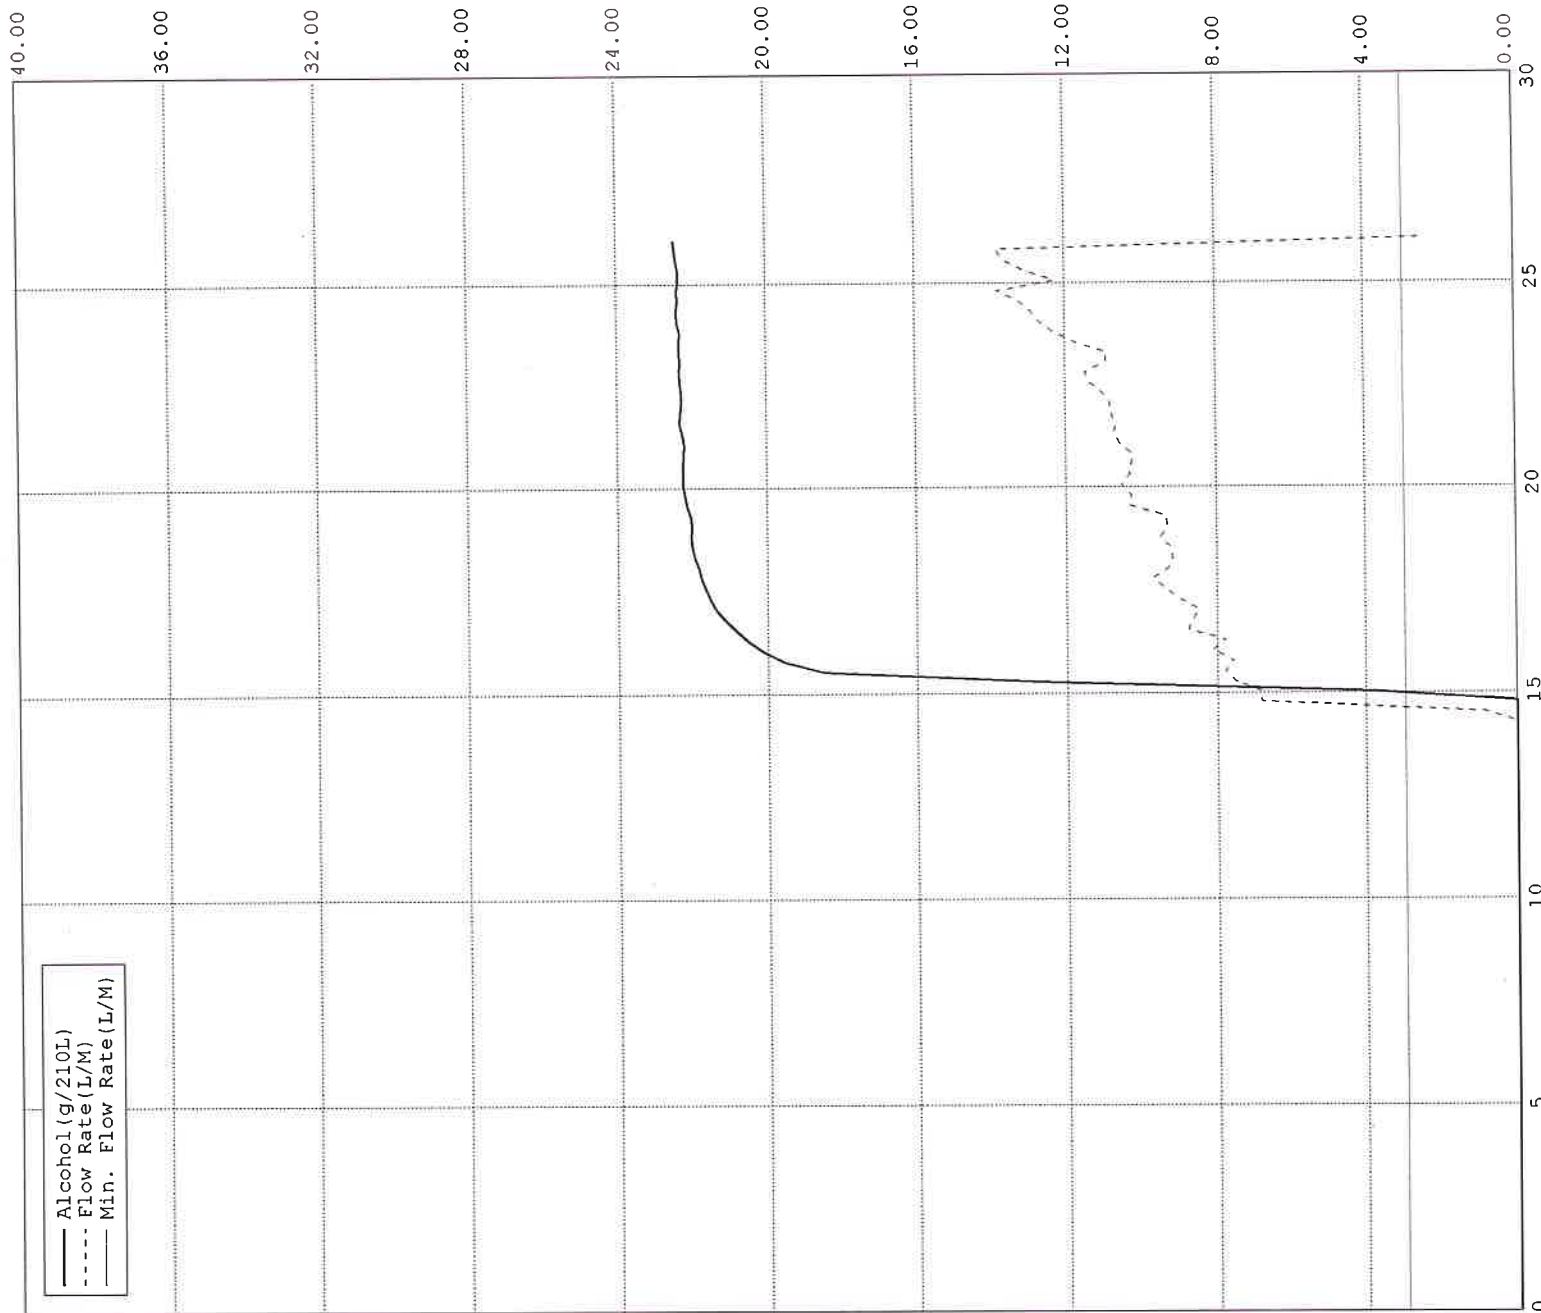

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100399

Date: 06/11/2025

Time: 12:49:26

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - IPA

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.97: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

PASSED

0.000

12:50

INTERNAL STANDARD

VERIFIED

0.080

12:50

$X_q = 0.085$ (0.83%)

EXTERNAL STANDARD

0.080

12:51

$X[1] = 0.0797$ (-0.0003)

(0.0027)

0.000

12:52

BLANK TEST

XXX

12:52

SUBJECT SAMPLE


$X[1] = 0.1216$ (-0.0329)

(0.0027)

Interference Detected

Interference Detected

MNC

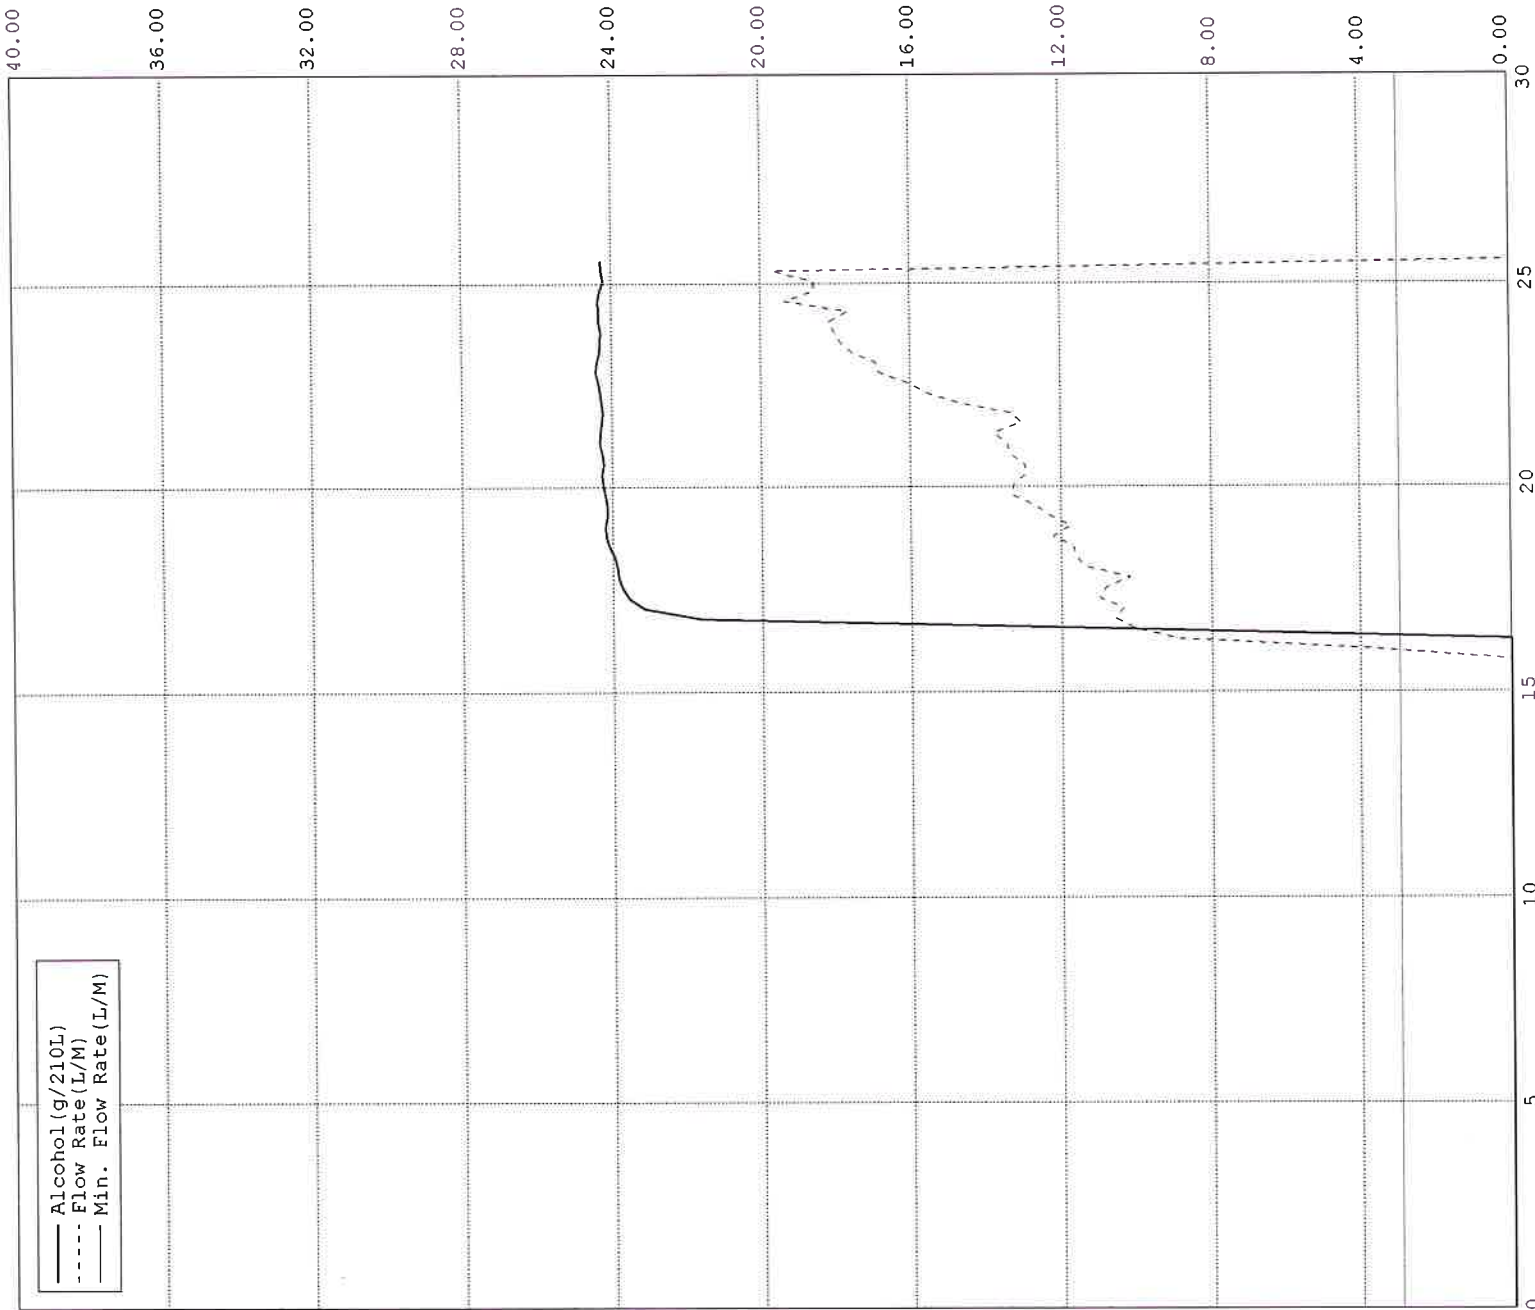

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100399

Date: 06/11/2025
Time: 12:24:32

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - BLANK
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.98: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:27
BLANK TEST	0.000	12:28
INTERNAL STANDARD	VERIFIED	12:28
$X_q = 0.085$ (0.83%)		
EXTERNAL STANDARD	0.080	12:28
$X[1] = 0.0797$ (-0.0010)	(0.0018)	
BLANK TEST	0.000	12:29
SUBJECT SAMPLE (Vol=1.82L)	0.097	12:29
$X[1] = 0.0970$ (-0.0018)	(0.0004)	
BLANK TEST	0.000	12:30
EXTERNAL STANDARD	0.080	12:31
$X[1] = 0.0795$ (-0.0009)	(0.0018)	
BLANK TEST	0.000	12:32

MNC



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100399

Date: 06/11/2025

Time: 15:01:01

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.95: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	15:01
BLANK TEST	0.000	15:02
INTERNAL STANDARD	VERIFIED	15:02
EXTERNAL STANDARD	0.080	15:02
BLANK TEST	0.000	15:03
SUBJECT SAMPLE (Vol=2.72L)	0.000	15:03
BLANK TEST	0.000	15:04
EXTERNAL STANDARD	0.080	15:04
BLANK TEST	0.000	15:05

MNC

