




State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100386

**Report Issue Date:** 03/10/2026  
**Date Received:** 2025-10-21  
**Condition of Item:** Damaged

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.019	0.019	0.019	0.019	0.020	0.019
0.080	0.078	AG335202	0.076	0.076	0.076	0.077	0.076	0.076
0.300	0.294	AG427706	0.287	0.287	0.288	0.288	0.287	0.287

As Found - Evaluation Analyst: Derek Walton  
 As Found Conditions - Barometric Pressure (inHg): 29.28 Barometer Used: VWR S/N 240680771 Temperature (C): 21.0 Relative Humidity (%): 21  
 As-Found Lab Activity Date Range: 10/21/2025 - 10/23/2025

Filter wheel solenoid wire coating is flaking. Attempted upload via modem again - unsuccessful.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.040	AG407908	0.039	0.040	0.040	0.040	0.040	0.040	+/- 0.003
0.080	0.080	AG436502	0.079	0.079	0.079	0.079	0.078	0.079	+/- 0.004
0.100	0.100	AG516101	0.099	0.099	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.150	AG515604	0.148	0.146	0.147	0.149	0.149	0.148	+/- 0.006
0.300	0.299	AG516110	0.295	0.294	0.293	0.294	0.294	0.294	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.87 Barometer Used: VWR S/N 240680771 Temperature (C): 19.9 Relative Humidity (%): 9  
 As-Left Lab Activity Date Range: 02/18/2026 - 02/19/2026

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Colleen O'Bryant on 03/10/2026

[colleen.obryant@alaska.gov](mailto:colleen.obryant@alaska.gov)

Technically and administratively reviewed by Derek Walton on 03/10/2026

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100386 Analyst or Technician Name: C.O. Bryant

DataMaster DMT Calibration Start Date: 2/18/26

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 240680771  
Calibration Due Date: 10 Sep 2026
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.87 Temperature(C) 19.9 Relative Humidity(%) 9

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
  - Invalid
  - Interference (Volatiles) - *Print with View Details*
  - Maximum Attempts Exceeded
  - Radio Frequency Interference (RFI)
- 5/18/26 COB 2026.03.10
1. Acetone Reagent Lot Number: 20260218COB Expiration Date: 8/19/27  
Simulator S/N: SD108P Thermometer Verification Performed?  5/18/26 COB 2026.03.10
  2. Isopropanol Reagent Lot Number: 20260218COB Expiration Date: 8/19/27  
Simulator S/N: SD1199 Thermometer Verification Performed?
  3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 8/19/27  
Simulator S/N: SD1144 Thermometer Verification Performed?

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 14 Mar 2027

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 2/19/26

Data Interpretation Date (Technician): \_\_\_\_\_ (if applicable)

Data Interpretation Date (Analyst): 2/19/26

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100386  
-----

Date: 02/18/2026  
Time: 12:27:26

VERSIONS  
DMT: 3.02  
PIC: 3.02  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C            PASSED  
(44.0°C - 52.0°C)  
Breath Tube       = 43.5°C        PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage     = 1.91 V           PASSED  
(1.15 V - 2.67 V)  
Cooler Voltage   = 1.66 V           PASSED  
(1.00 V - 2.32 V)  
Bias Voltage     = 79 V            PASSED  
(47 V - 111 V)  
Chopper Freq    = 517 Hz            PASSED  
(475 Hz - 575 Hz)  
Barometer        = 29.9 in

PUMP INFO

Flow Rate = 4.824 L/M            PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON                            PASSED  
(0.002 V <= 0.010 V)  
PUMP OFF                           PASSED  
(0.002 V <= 0.010 V)

FILTER INFO

Filter 1                           PASSED  
Filter 2                           PASSED  
Filter 3                           PASSED

INTERNAL STANDARD

Xq = 0.101 0.61% (0.00% - 4.00%)            PASSED

Technician Screen

-----  
DATAMASTER dmt: 100386  
-----

Date: 02/18/2026

Time: 12:58 PM

Temperatures (°C)

Sample Cell: 48.6°C

Breath Tube: 43.5°C

Current Barometer 29.9 in

Volume (Ltr) 1.45

Settings

Lamp: 1.96 V

Bias: 79 V

Cooler: 1.68 V

Chopper: 517 Hz

Voltages (V)

Flow: 1.06 V

Detector: 0.086 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100386  
-----

Date: 02/03/2026  
Time: 11:32:35

OPERATOR NAME:  
KAIJA SWISHER  
CERTIFICATE #: 10746

Ca = 0.1000  
CAL = 0.978675    0.800 <= CAL < 1.200  
b1 = 0.0009    0.0000 <= b1 < 0.0040  
b2 = 0.0063    0.0010 <= b2 < 0.0100  
b3 = 0.0007    0.0000 <= b3 < 0.0040  
Xq = 0.1001    0.0500 <= Xq < 0.2000  
a21 = 1.173040    1.050 <= a21 < 1.300  
a31 = 0.545697    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100386

Date: 02/18/2026  
Time: 12:59:28

SUBJECT NAME:  
TEST TEST  
LICENSE #: VOLUME TEST


OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 26-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.90: 0.080  
LOT #: AG436502  
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	13:00
INTERNAL STANDARD	0.000	13:00
EXTERNAL STANDARD	0.078	13:00
INTERNAL STANDARD	0.000	13:01
EXTERNAL STANDARD	0.000	13:03
INTERNAL STANDARD	0.000	13:04
EXTERNAL STANDARD	0.080	13:04
INTERNAL STANDARD	0.000	13:05
EXTERNAL STANDARD	0.000	13:05

*OKB*

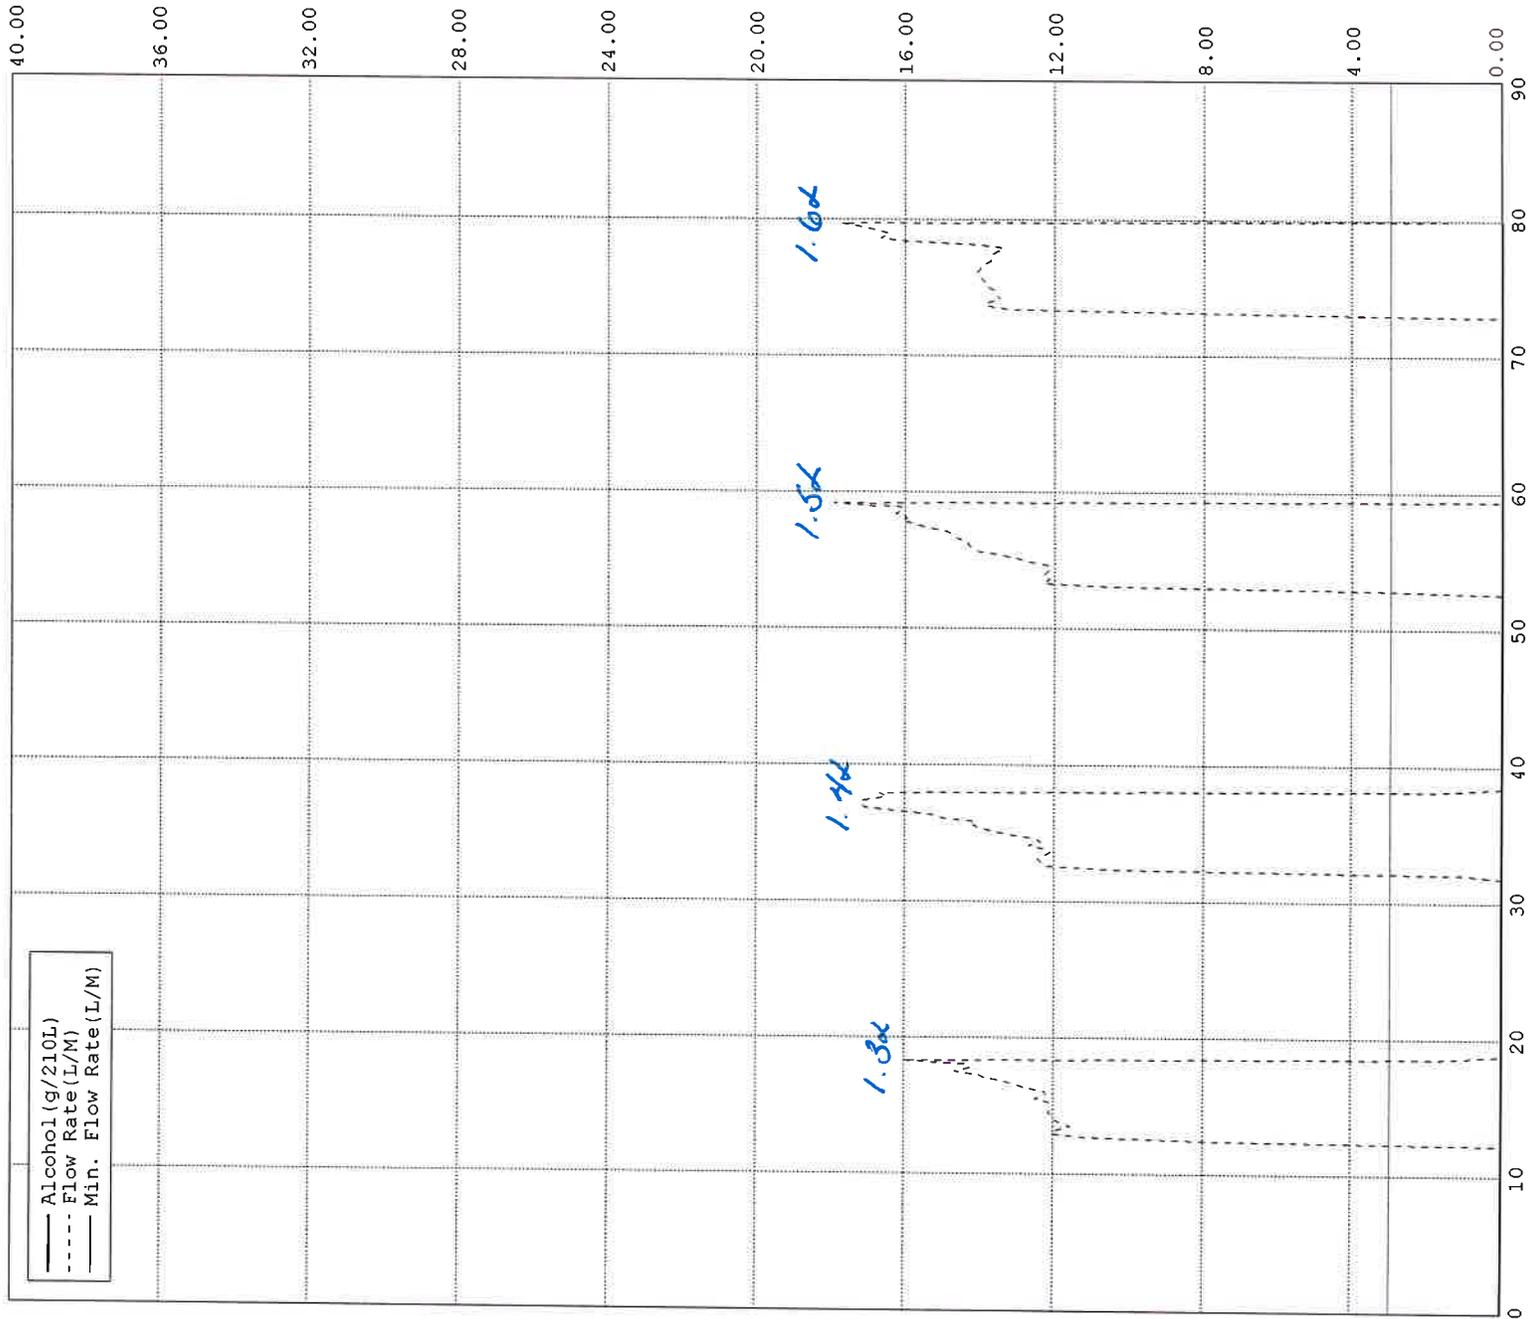

LINEARITY CHECK

Alaska Department of Public Safety  
DATAMASTER dmt: 100386


Date: 02/19/2026  
Time: 07:09:06

SUPERVISOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

TARGET	AVERAGE	STD. DEV.
0.020	0.0202	0.0004
0.040	0.0398	0.0004
0.080	0.0788	0.0004
0.100	0.0984	0.0005
0.150	0.1478	0.0013
0.299	0.2940	0.0007

SLOPE = 0.981699  
R<sup>2</sup> = 0.999998

CORB

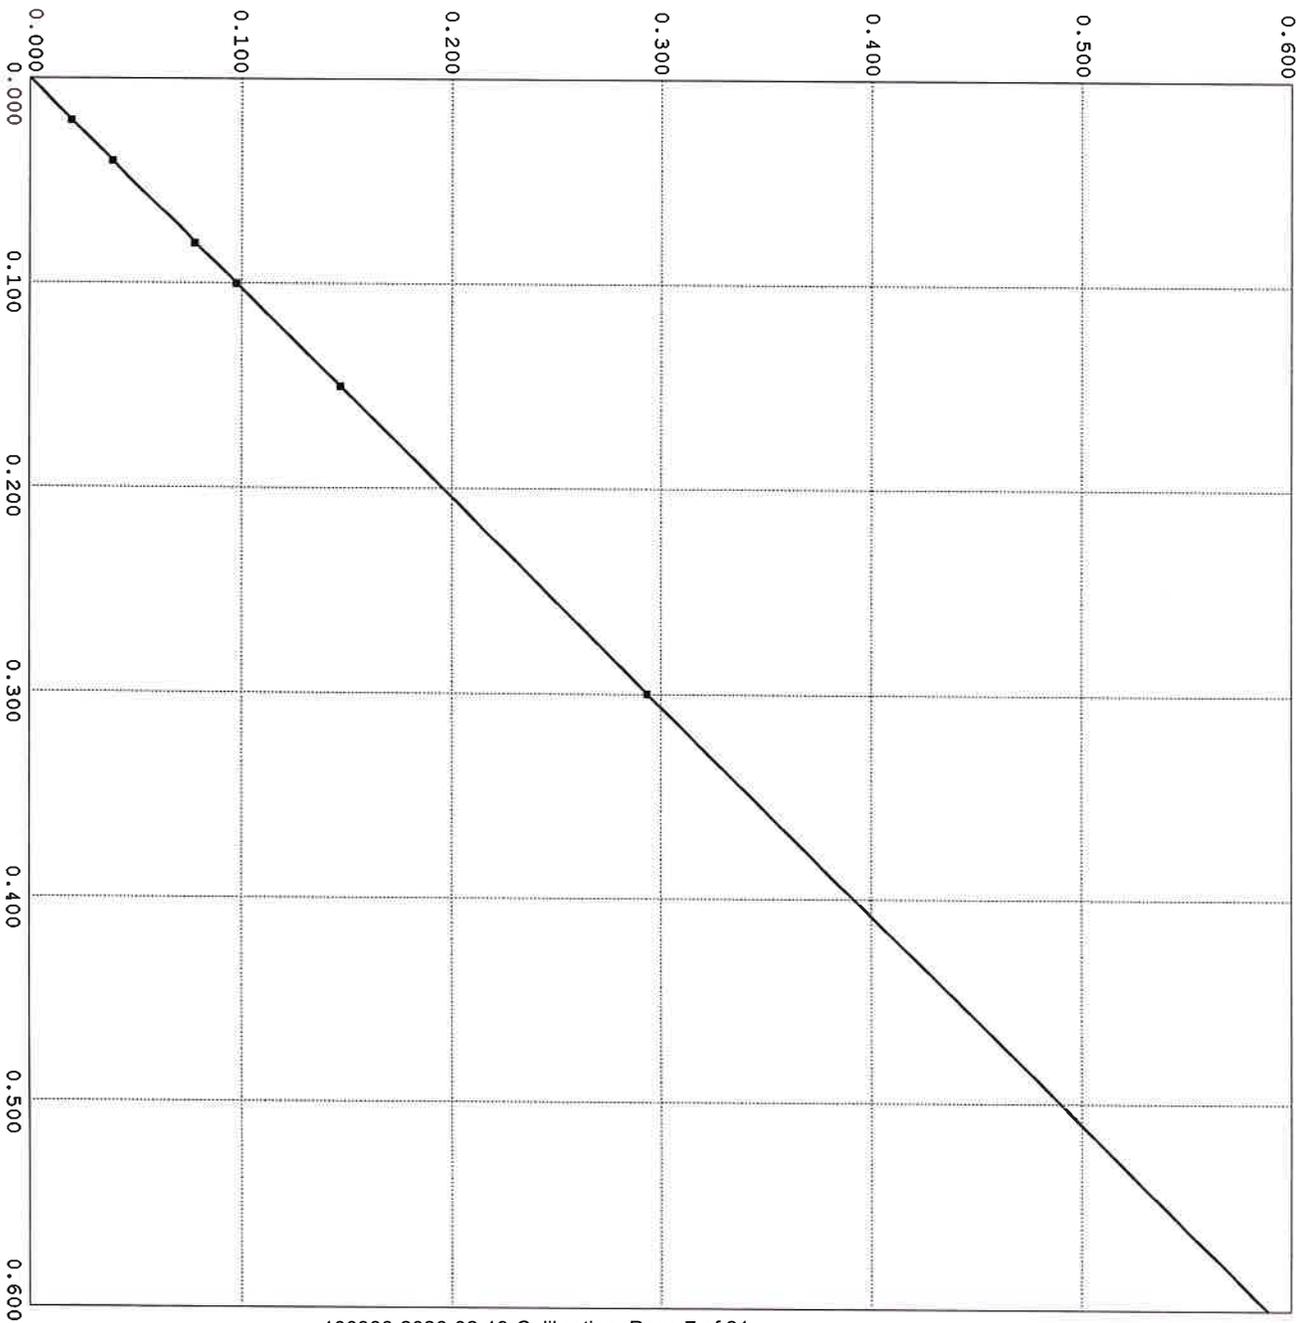

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
DATAMASTER dmt: 100386






Date: 02/19/2026  
Time: 07:09:08

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
TARGET AT 29.84: 0.020  
LOT #: AG402003 AG408002 *02/19/26*  
EXPIRATION: 03/20/2026  
TANK PRESSURE: 601 psi

BLANK TEST	0.000	07:49
INTERNAL STANDARD	VERIFIED	07:49
EXTERNAL STANDARD	0.021	07:49
BLANK TEST	0.000	07:50
EXTERNAL STANDARD	0.020	07:50
BLANK TEST	0.000	07:51
EXTERNAL STANDARD	0.020	07:51
BLANK TEST	0.000	07:52
EXTERNAL STANDARD	0.020	07:53
BLANK TEST	0.000	07:53
EXTERNAL STANDARD	0.020	07:54
BLANK TEST	0.000	07:55

Average = 0.0202  
Std Dev = 0.0004

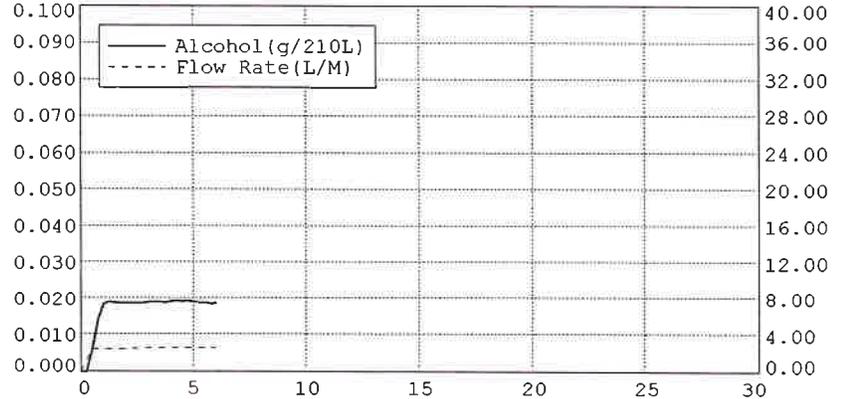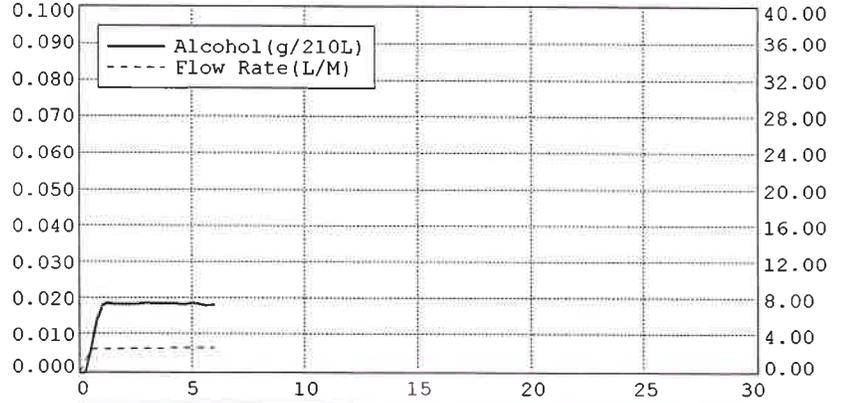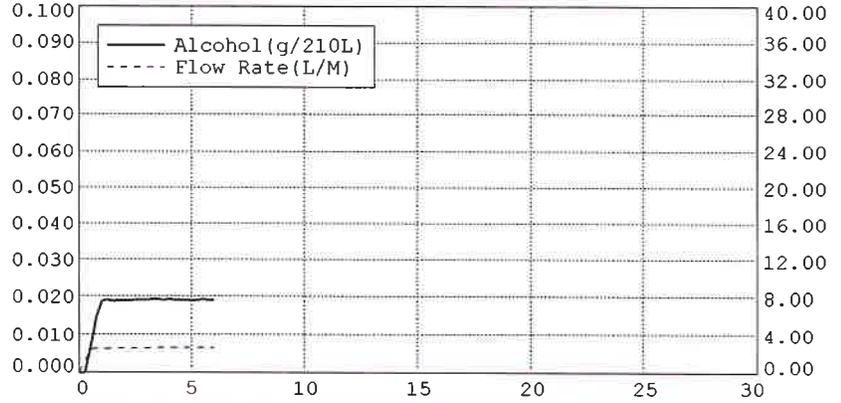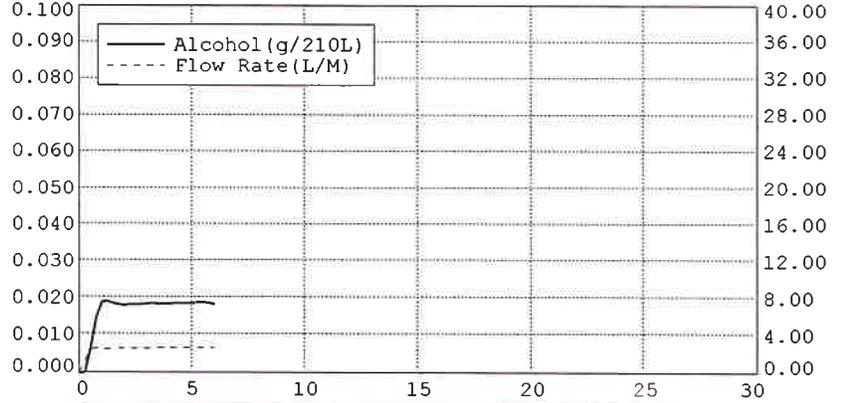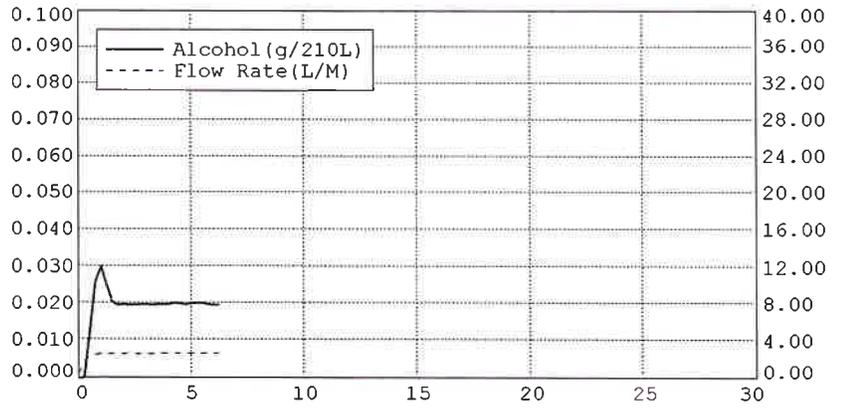

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100386






Date: 02/19/2026  
 Time: 07:58:24

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.84: 0.040  
 LOT #: AG407908  
 EXPIRATION: 03/19/2026  
 TANK PRESSURE: 606 psi

BLANK TEST	0.000	07:59
INTERNAL STANDARD	VERIFIED	07:59
EXTERNAL STANDARD	0.039	07:59
BLANK TEST	0.000	08:00
EXTERNAL STANDARD	0.040	08:01
BLANK TEST	0.000	08:01
EXTERNAL STANDARD	0.040	08:02
BLANK TEST	0.000	08:03
EXTERNAL STANDARD	0.040	08:03
BLANK TEST	0.000	08:04
EXTERNAL STANDARD	0.040	08:04
BLANK TEST	0.000	08:05

Average = 0.0398  
 Std Dev = 0.0004

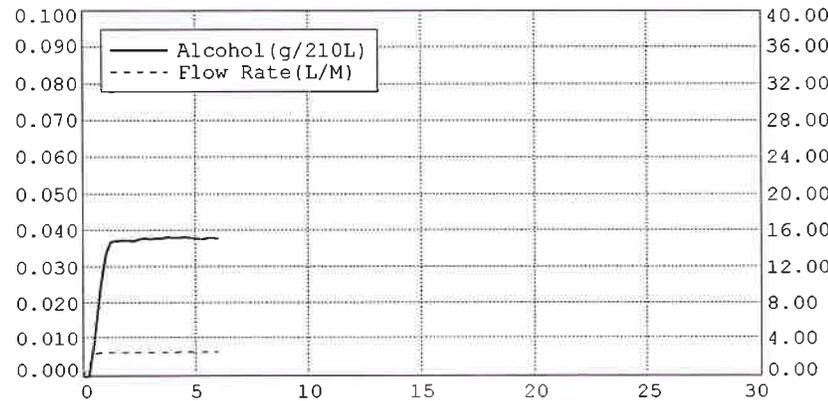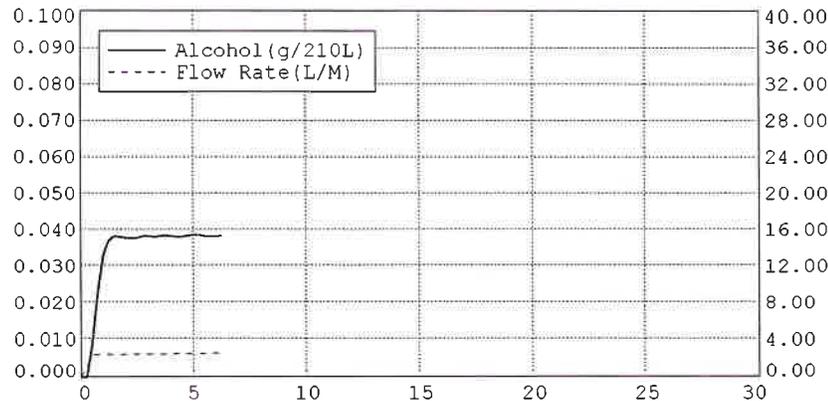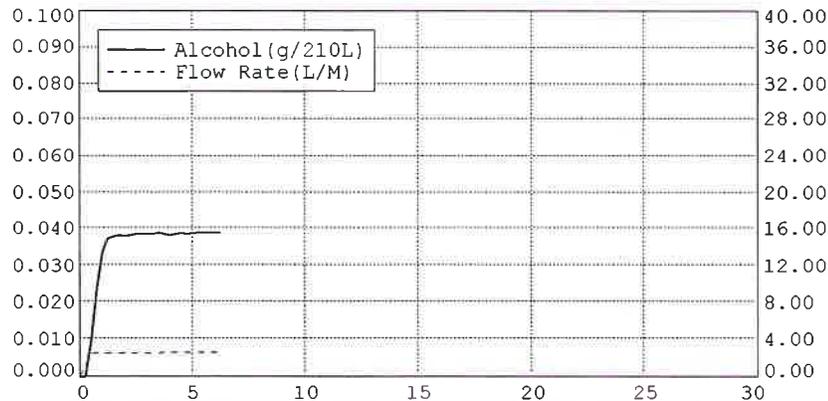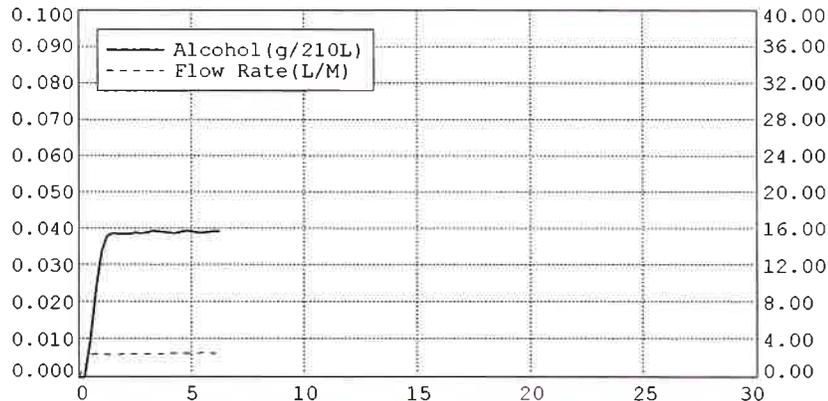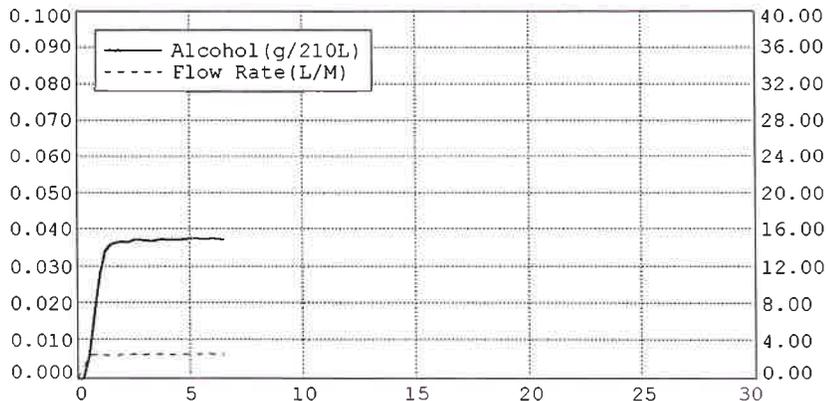

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100386






Date: 02/19/2026  
 Time: 08:44:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.85: 0.080  
 LOT #: AG436502  
 EXPIRATION: 12/30/2026  
 TANK PRESSURE: 933 psi

BLANK TEST	0.000	08:46
INTERNAL STANDARD	VERIFIED	08:46
EXTERNAL STANDARD	0.079	08:46
BLANK TEST	0.000	08:47
EXTERNAL STANDARD	0.079	08:47
BLANK TEST	0.000	08:48
EXTERNAL STANDARD	0.079	08:48
BLANK TEST	0.000	08:49
EXTERNAL STANDARD	0.079	08:49
BLANK TEST	0.000	08:50
EXTERNAL STANDARD	0.078	08:50
BLANK TEST	0.000	08:51

Average = 0.0788  
 Std Dev = 0.0004

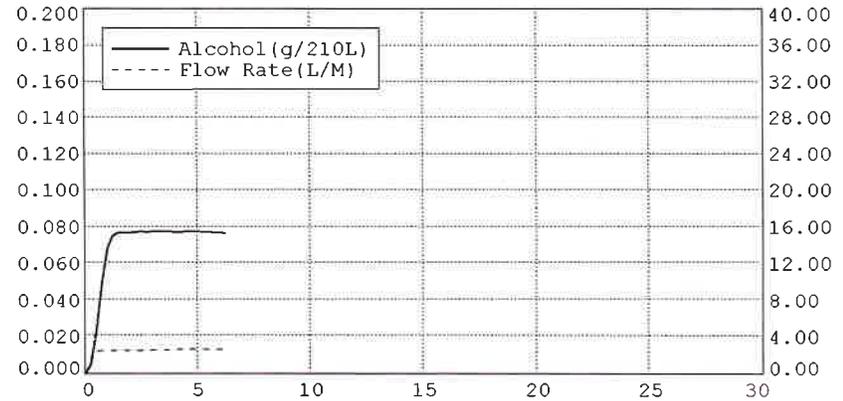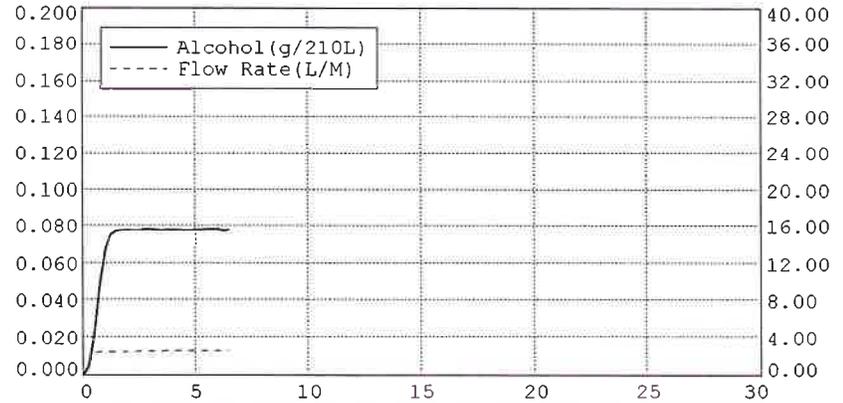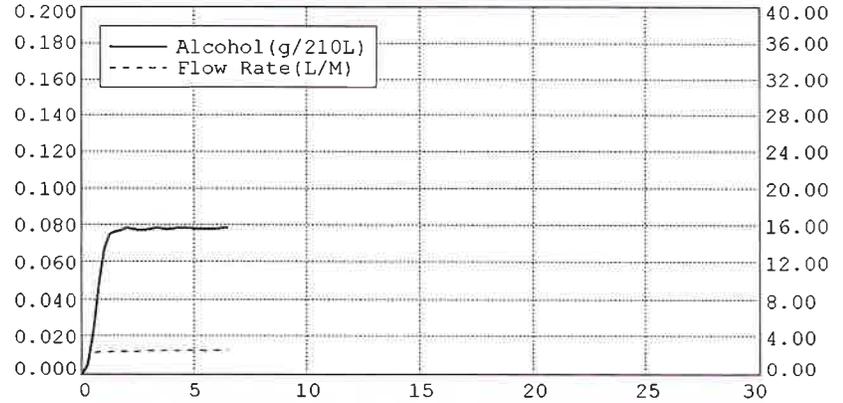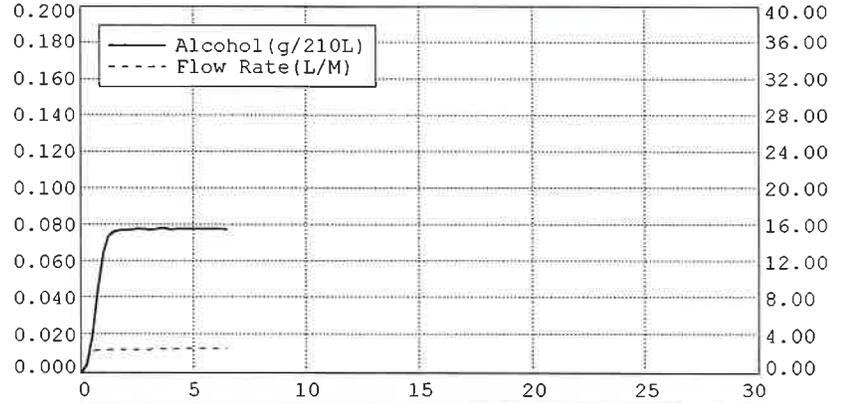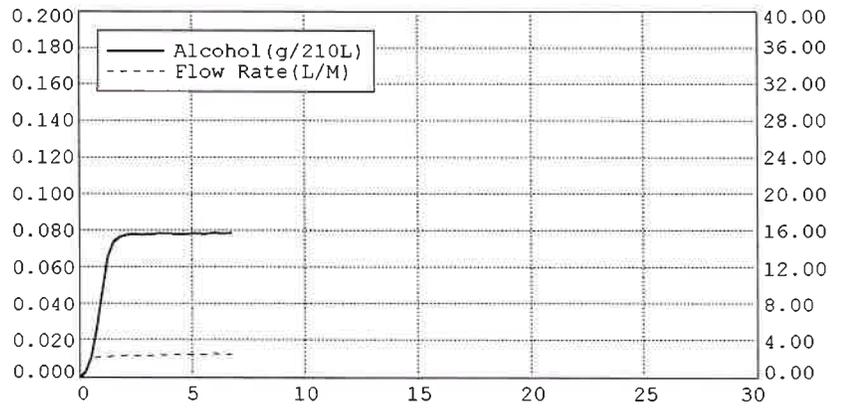

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100386






Date: 02/19/2026  
 Time: 08:52:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.84: 0.100  
 LOT #: AG516101  
 EXPIRATION: 06/10/2027  
 TANK PRESSURE: 989 psi

BLANK TEST	0.000	08:53
INTERNAL STANDARD	VERIFIED	08:53
EXTERNAL STANDARD	0.099	08:53
BLANK TEST	0.000	08:54
EXTERNAL STANDARD	0.099	08:54
BLANK TEST	0.000	08:55
EXTERNAL STANDARD	0.098	08:56
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.098	08:57
BLANK TEST	0.000	08:58
EXTERNAL STANDARD	0.098	08:58
BLANK TEST	0.000	08:59

Average = 0.0984  
 Std Dev = 0.0005

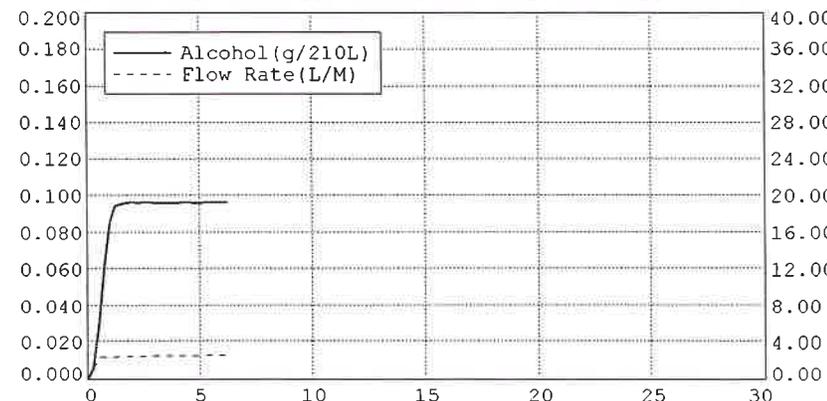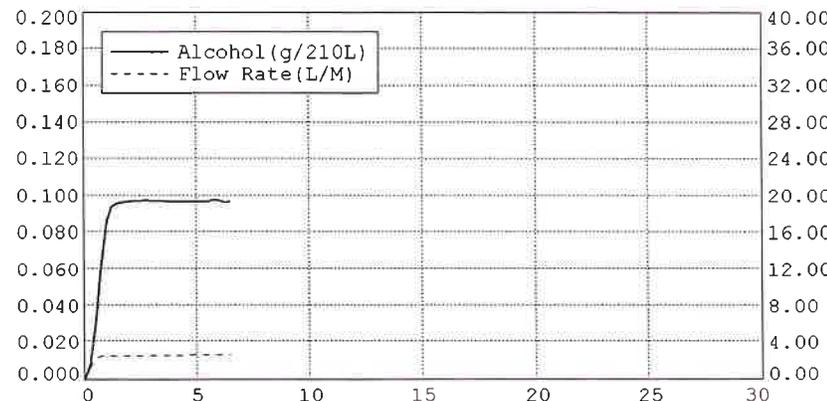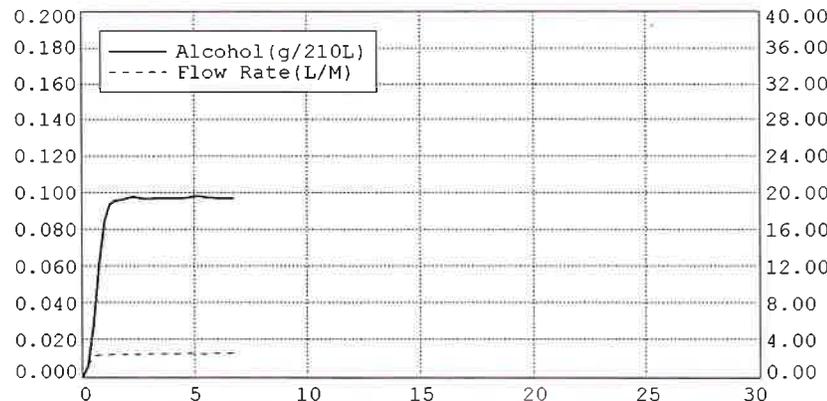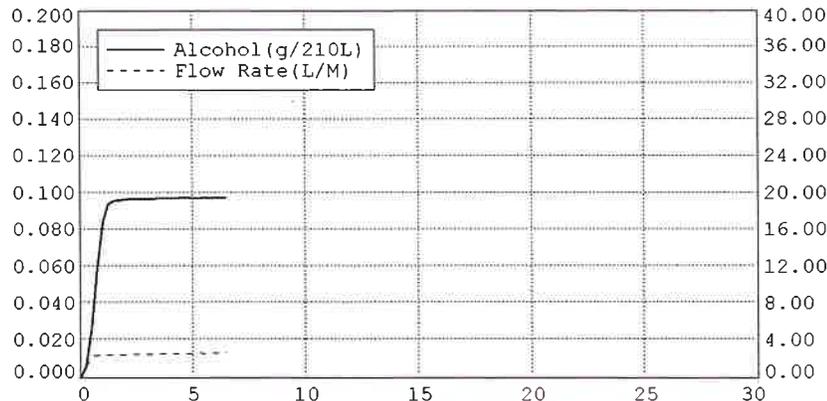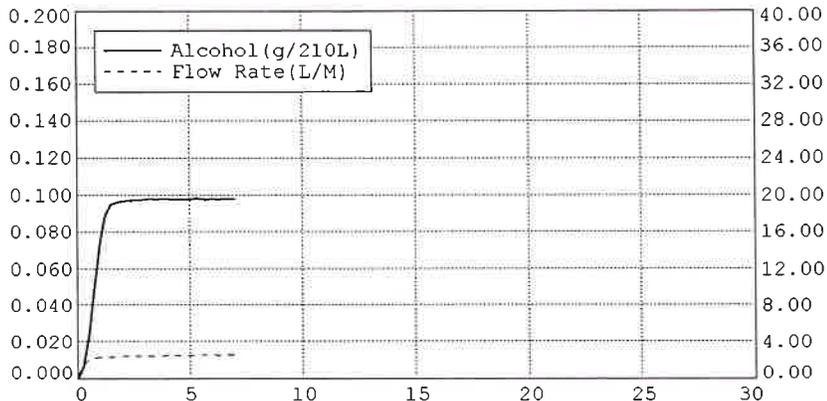

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
 DATAMASTER dmt: 100386






Date: 02/19/2026  
 Time: 09:00:14

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
 TARGET AT 29.84: 0.150  
 LOT #: AG515604  
 EXPIRATION: 06/05/2027  
 TANK PRESSURE: 614 psi

BLANK TEST	0.000	09:01
INTERNAL STANDARD	VERIFIED	09:01
EXTERNAL STANDARD	0.148	09:01
BLANK TEST	0.000	09:02
EXTERNAL STANDARD	0.146	09:02
BLANK TEST	0.000	09:03
EXTERNAL STANDARD	0.147	09:04
BLANK TEST	0.000	09:05
EXTERNAL STANDARD	0.149	09:05
BLANK TEST	0.000	09:06
EXTERNAL STANDARD	0.149	09:06
BLANK TEST	0.000	09:07

Average = 0.1478  
 Std Dev = 0.0013

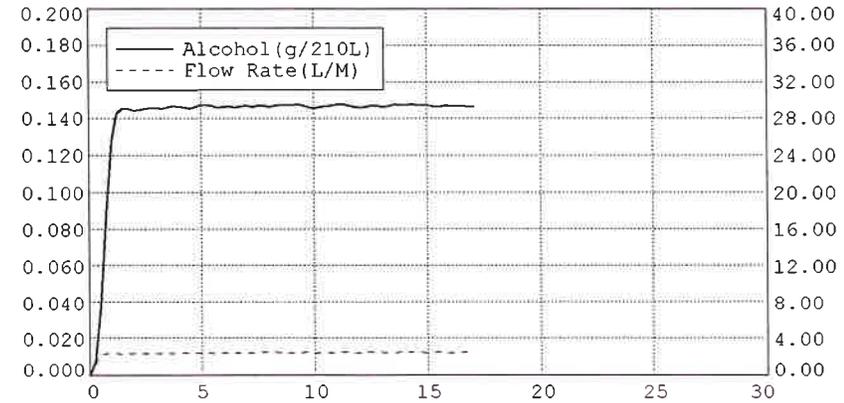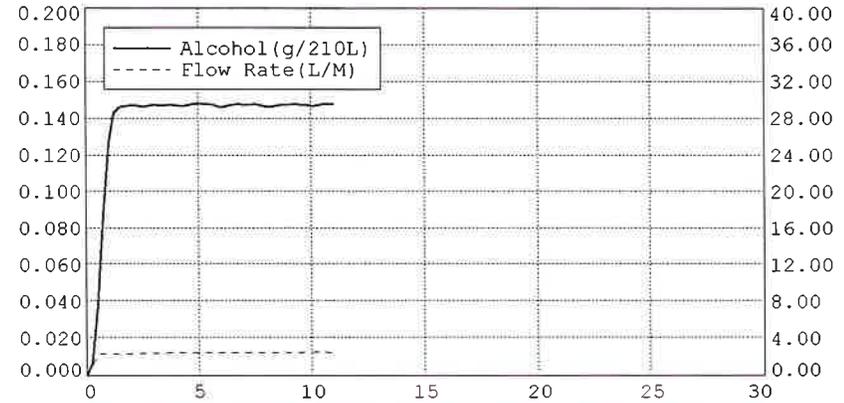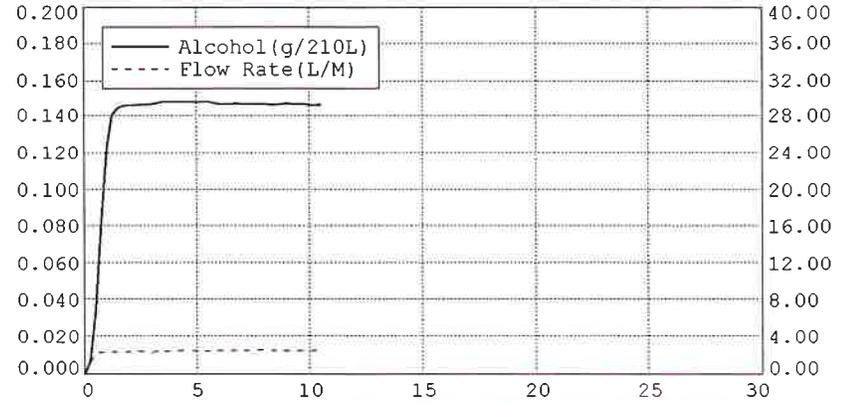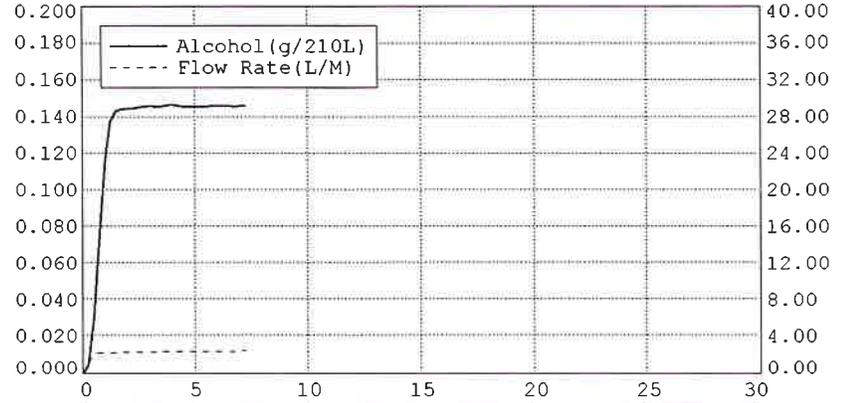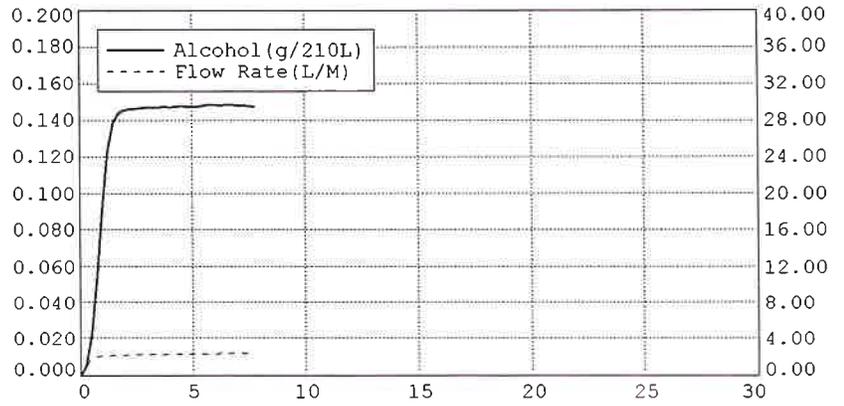

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100386






Date: 02/19/2026  
 Time: 09:08:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.84: 0.299  
 LOT #: AG516110  
 EXPIRATION: 06/10/2027  
 TANK PRESSURE: 389 psi

BLANK TEST	0.000	09:09
INTERNAL STANDARD	VERIFIED	09:09
EXTERNAL STANDARD	0.295	09:09
BLANK TEST	0.000	09:10
EXTERNAL STANDARD	0.294	09:11
BLANK TEST	0.000	09:11
EXTERNAL STANDARD	0.293	09:12
BLANK TEST	0.000	09:13
EXTERNAL STANDARD	0.294	09:13
BLANK TEST	0.000	09:14
EXTERNAL STANDARD	0.294	09:14
BLANK TEST	0.000	09:15

Average = 0.2940  
 Std Dev = 0.0007

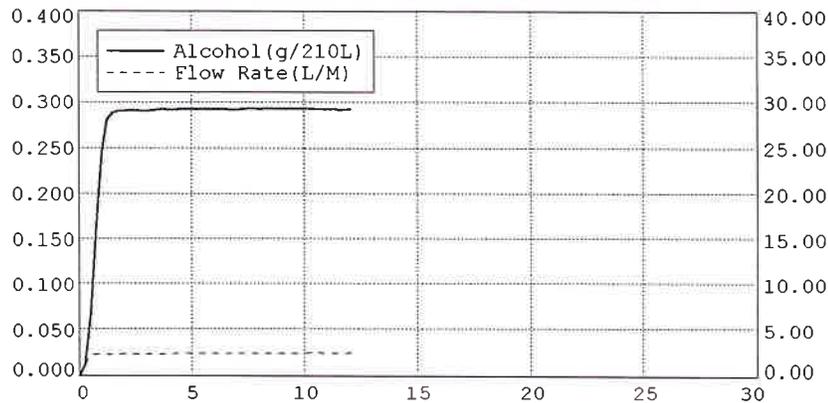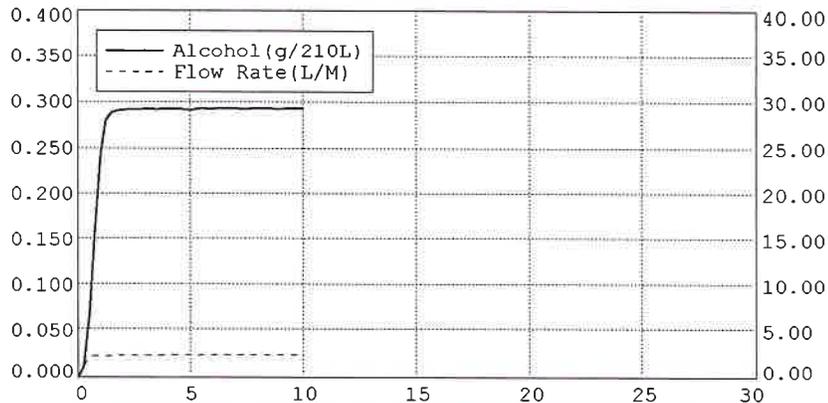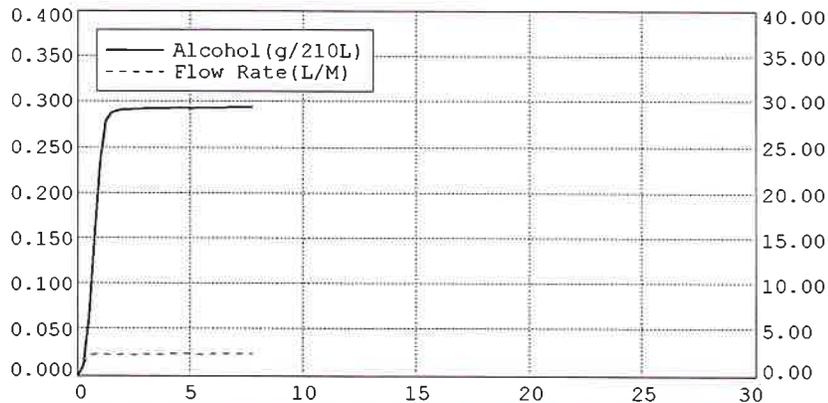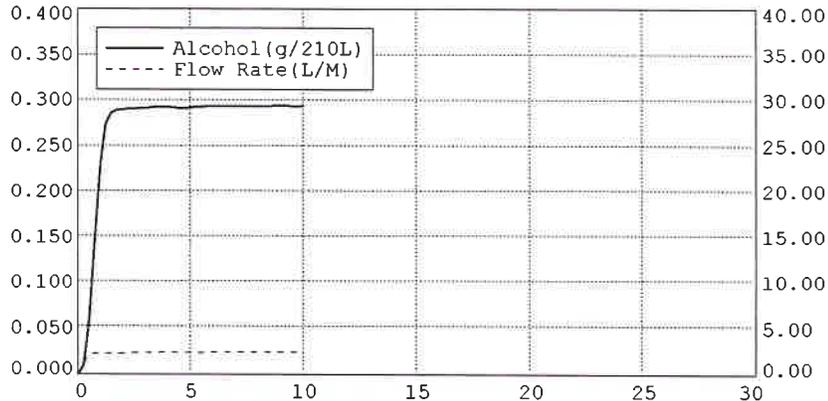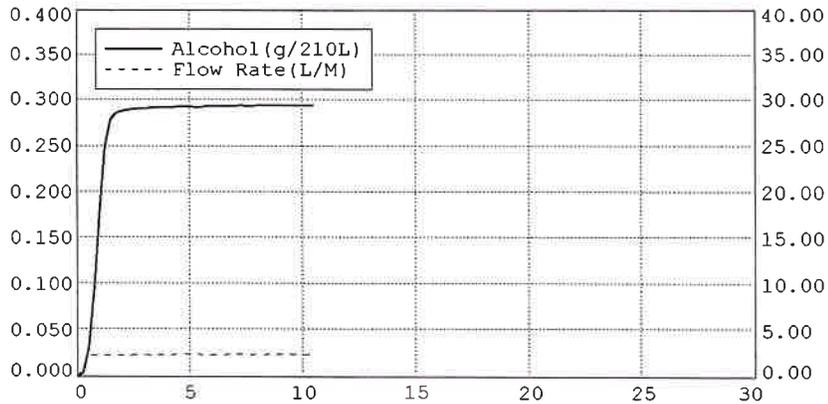

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100386

Date: 02/19/2026

Time: 09:56:36

SUBJECT NAME:

TEST TEST

LICENSE #: INCOMPLETE

OPERATOR NAME:

COLLEEN S OBRyant

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 26-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.82: 0.080

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE

PASSED 09:58


0.000 09:58

VERIFIED 09:58

0.078 09:58

0.000 09:59

INCOMPLETE 10:01

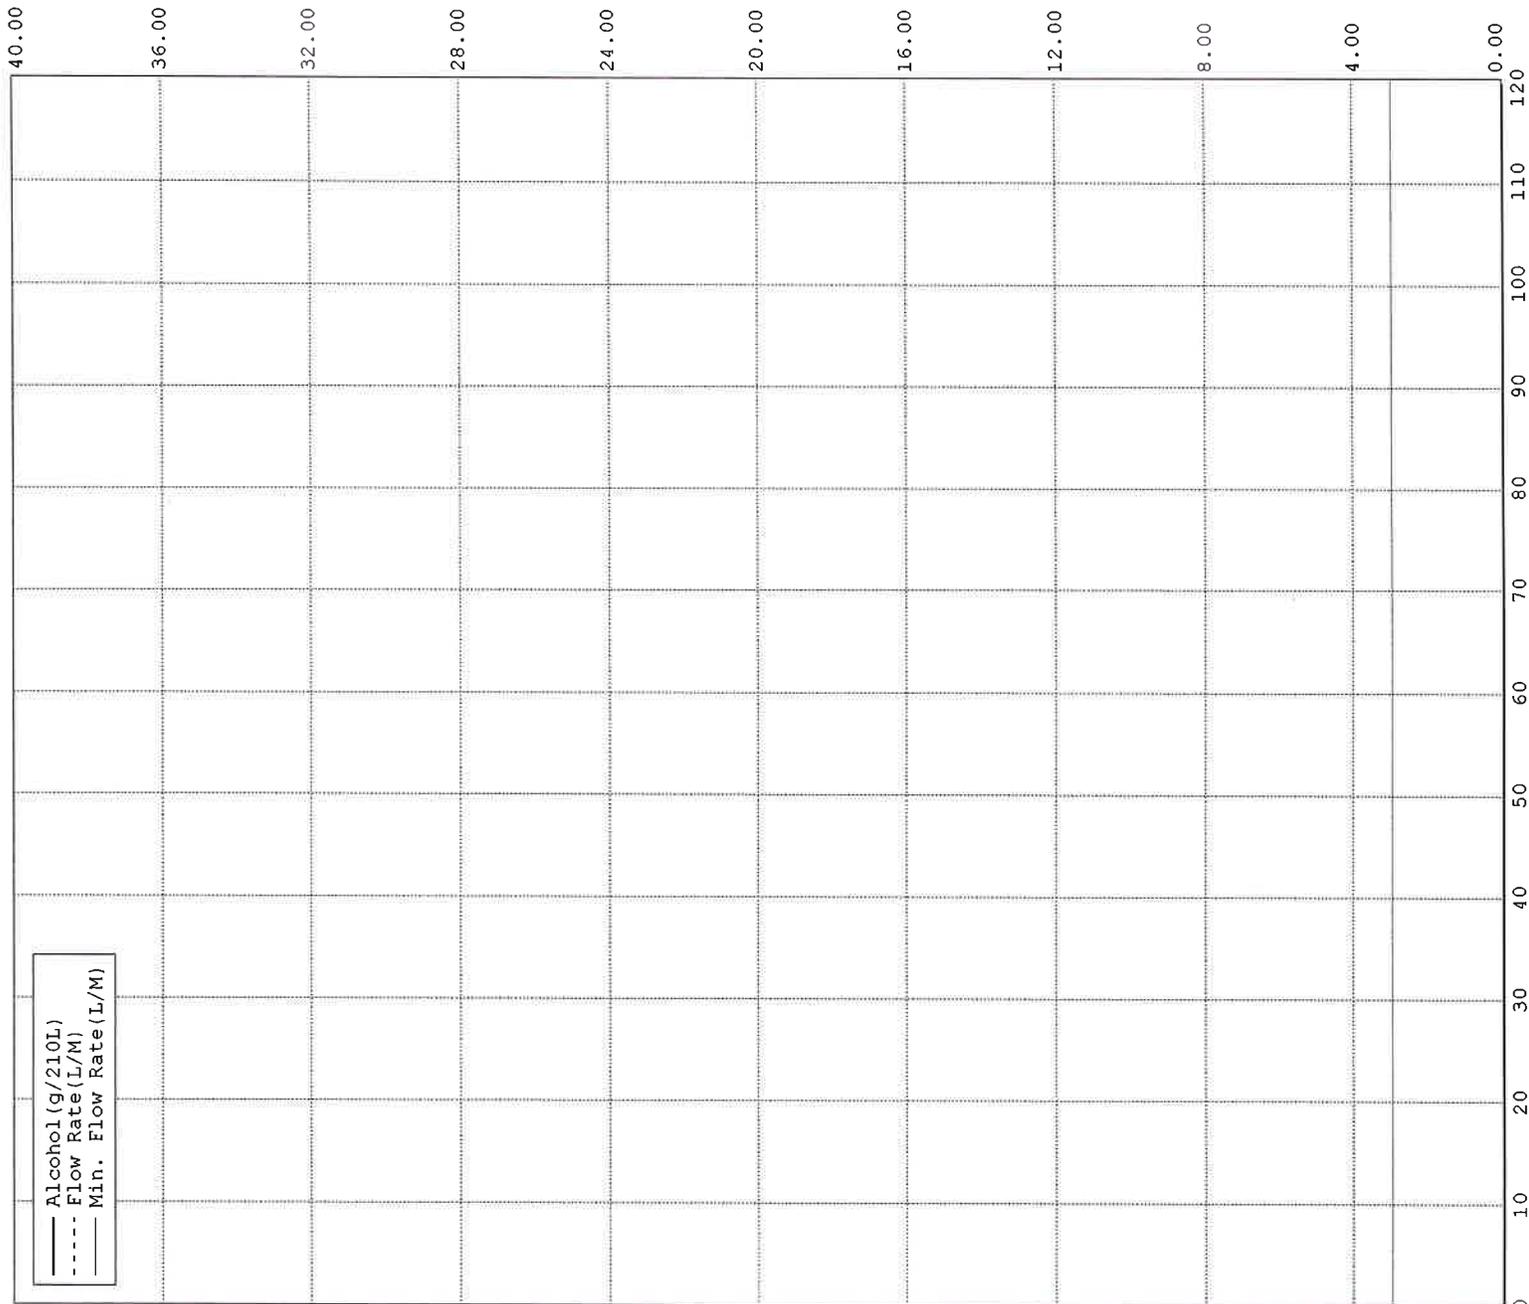

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100386

Date: 02/19/2026  
Time: 11:23:40

SUBJECT NAME:  
TEST TEST  
LICENSE #: MAX ATTEMPTS


OPERATOR NAME:  
COLLEEN S OBRYANT  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 26-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.80: 0.080  
LOT #: AG436502  
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 11:24  
BLANK TEST 0.000 11:24  
INTERNAL STANDARD VERIFIED 11:24  
EXTERNAL STANDARD 0.078 11:25  
BLANK TEST 0.000 11:26  
SUBJECT SAMPLE XXX 11:26

Maximum Attempts Exceeded

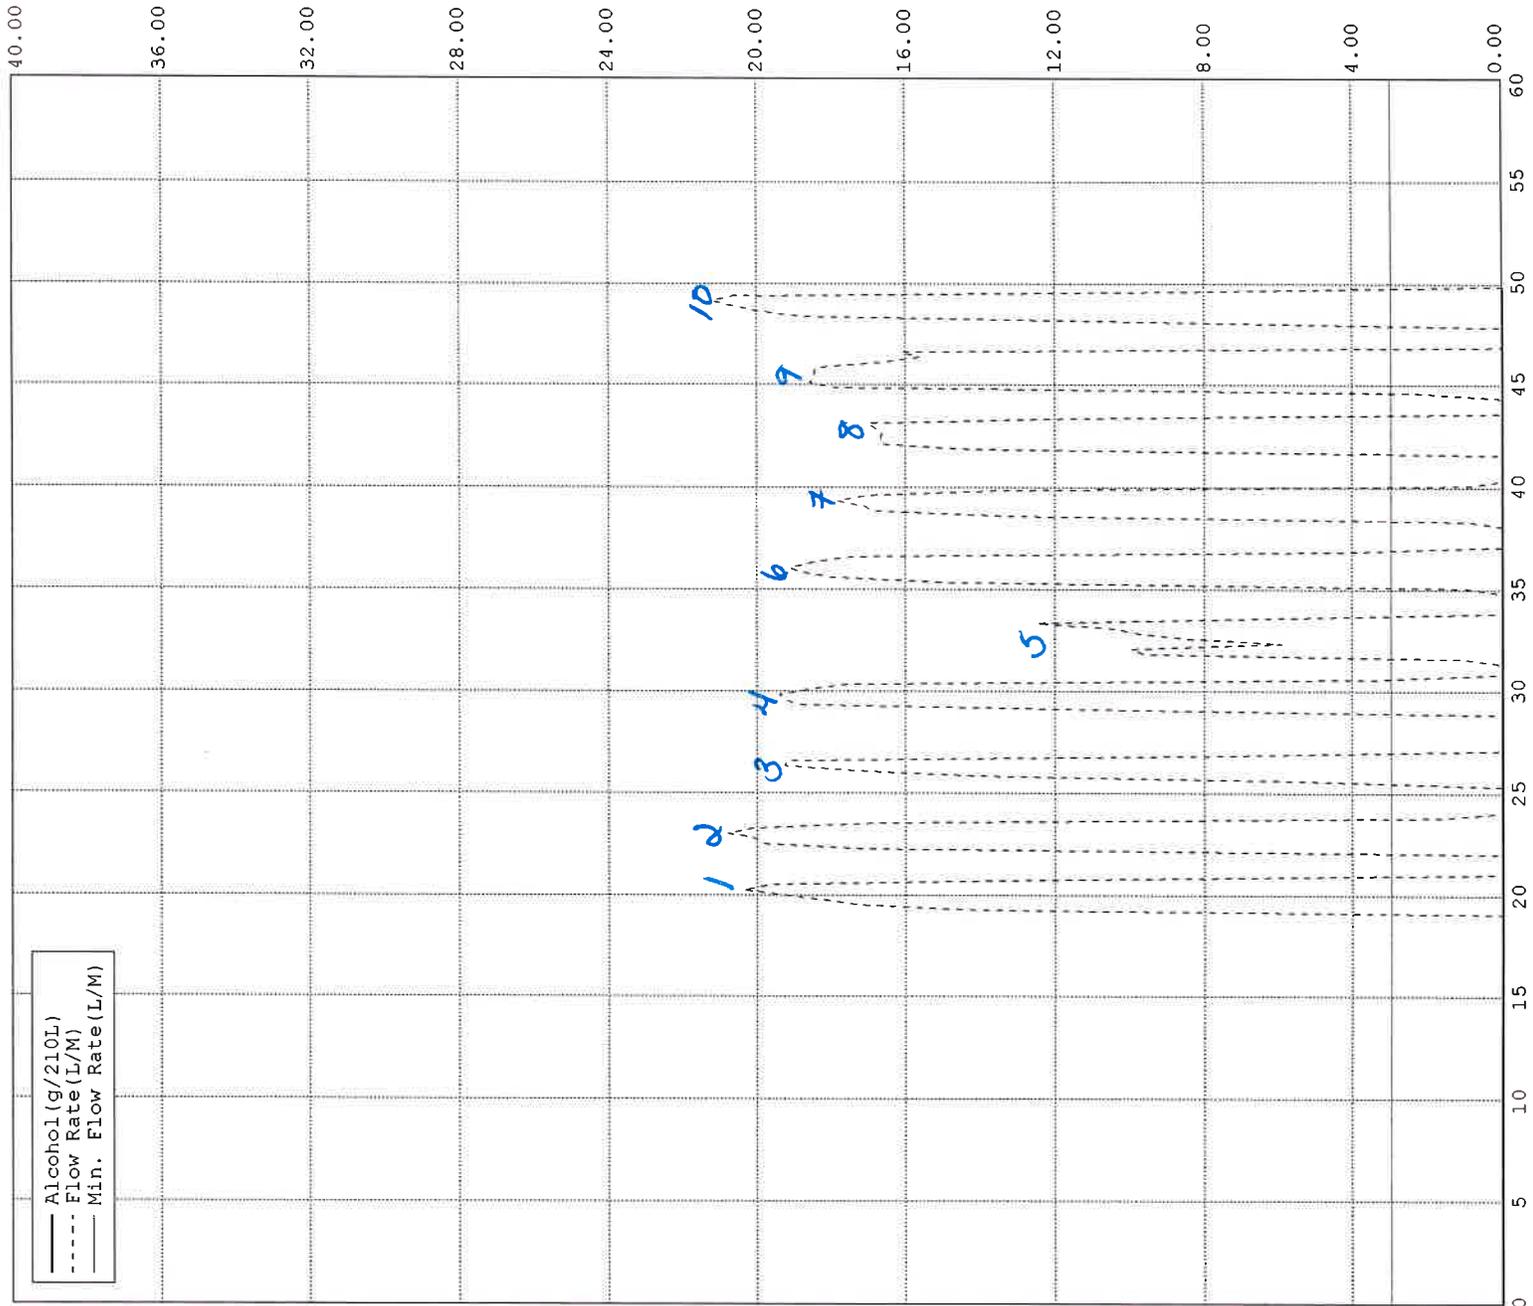

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100386

Date: 02/19/2026

Time: 11:09:25

SUBJECT NAME:

TEST TEST

LICENSE #: INVALID

OPERATOR NAME:

COLLEEN S OBRyant

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 26-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.80: 0.080

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

PASSED 11:10

BLANK TEST

0.000 11:10

INTERNAL STANDARD

VERIFIED 11:10


0.079 11:11

EXTERNAL STANDARD

0.000 11:12

INVALID 11:12

SUBJECT SAMPLE

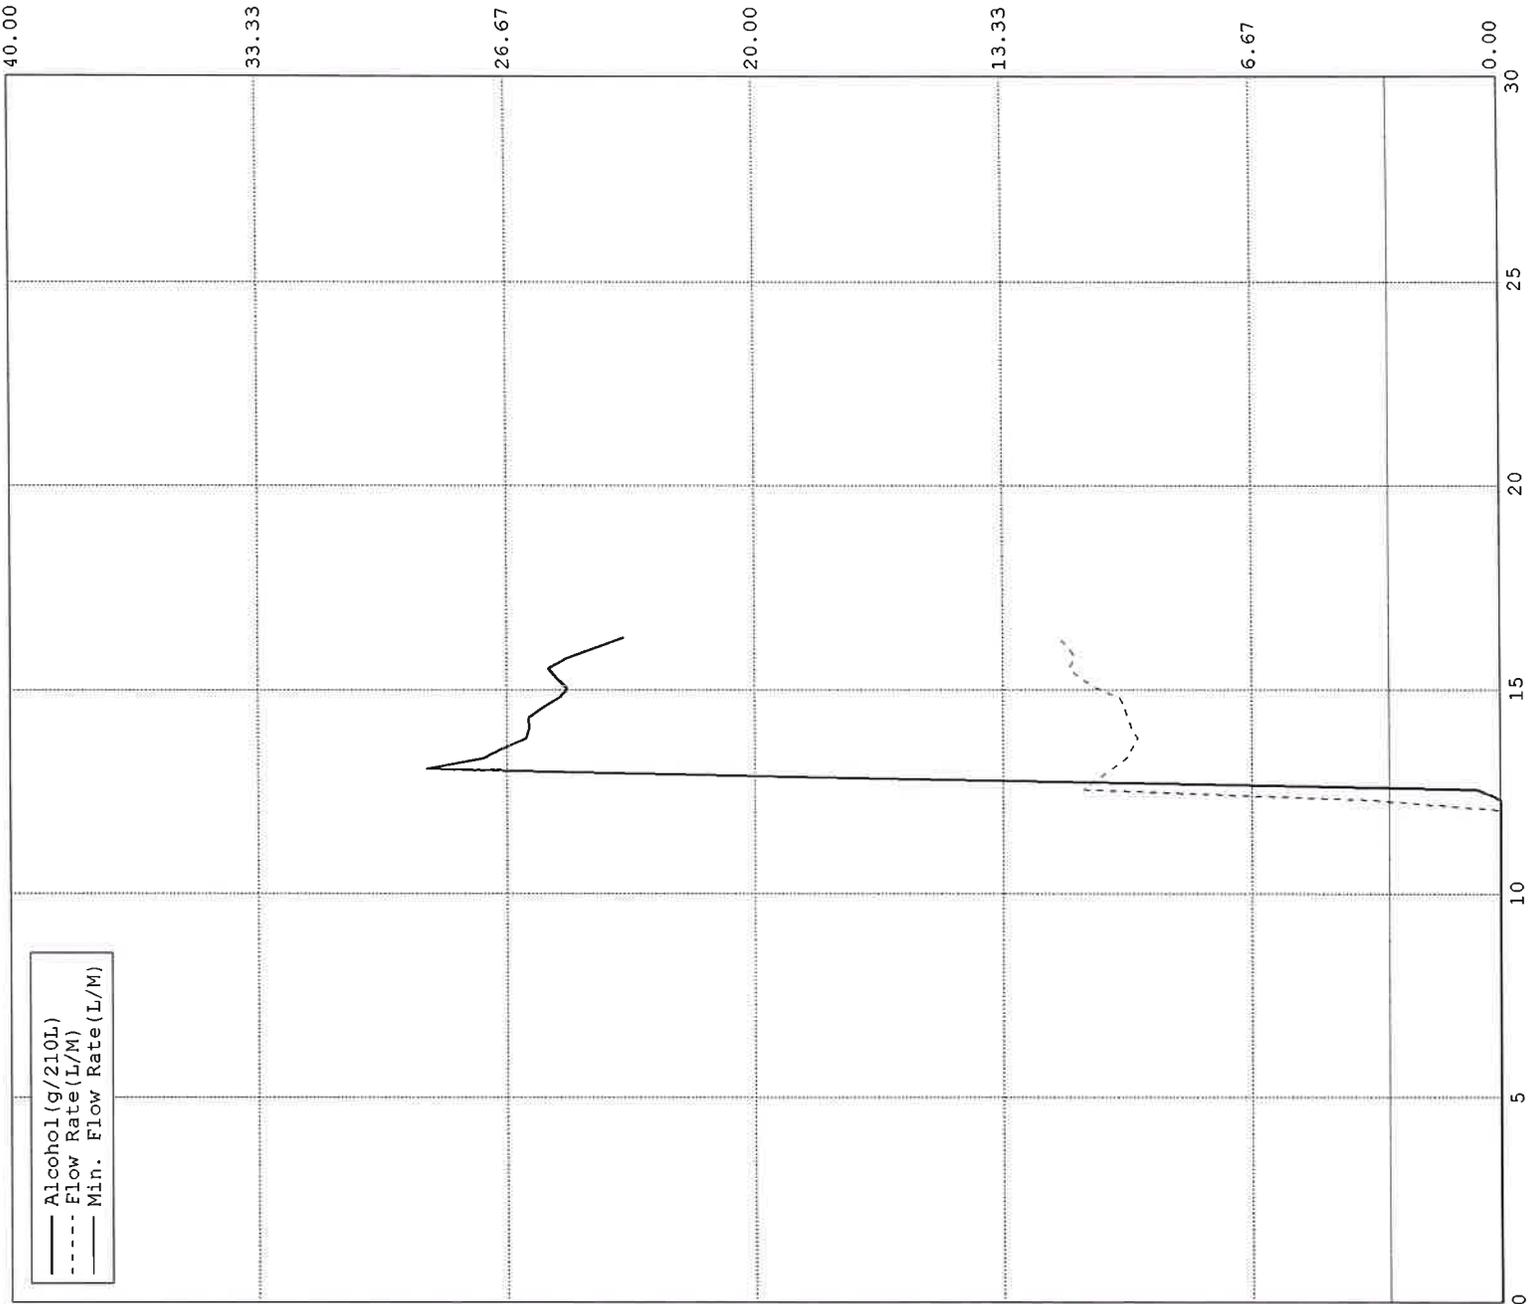

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100386

Date: 02/19/2026

Time: 11:02:38

SUBJECT NAME:

TEST TEST

LICENSE #: RFI

OPERATOR NAME:

COLLEEN S OBRyant

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 26-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.80: 0.080

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

PASSED 11:03


0.000 11:03

VERIFIED 11:03

0.078 11:04

0.000 11:05

RFI DETECTED

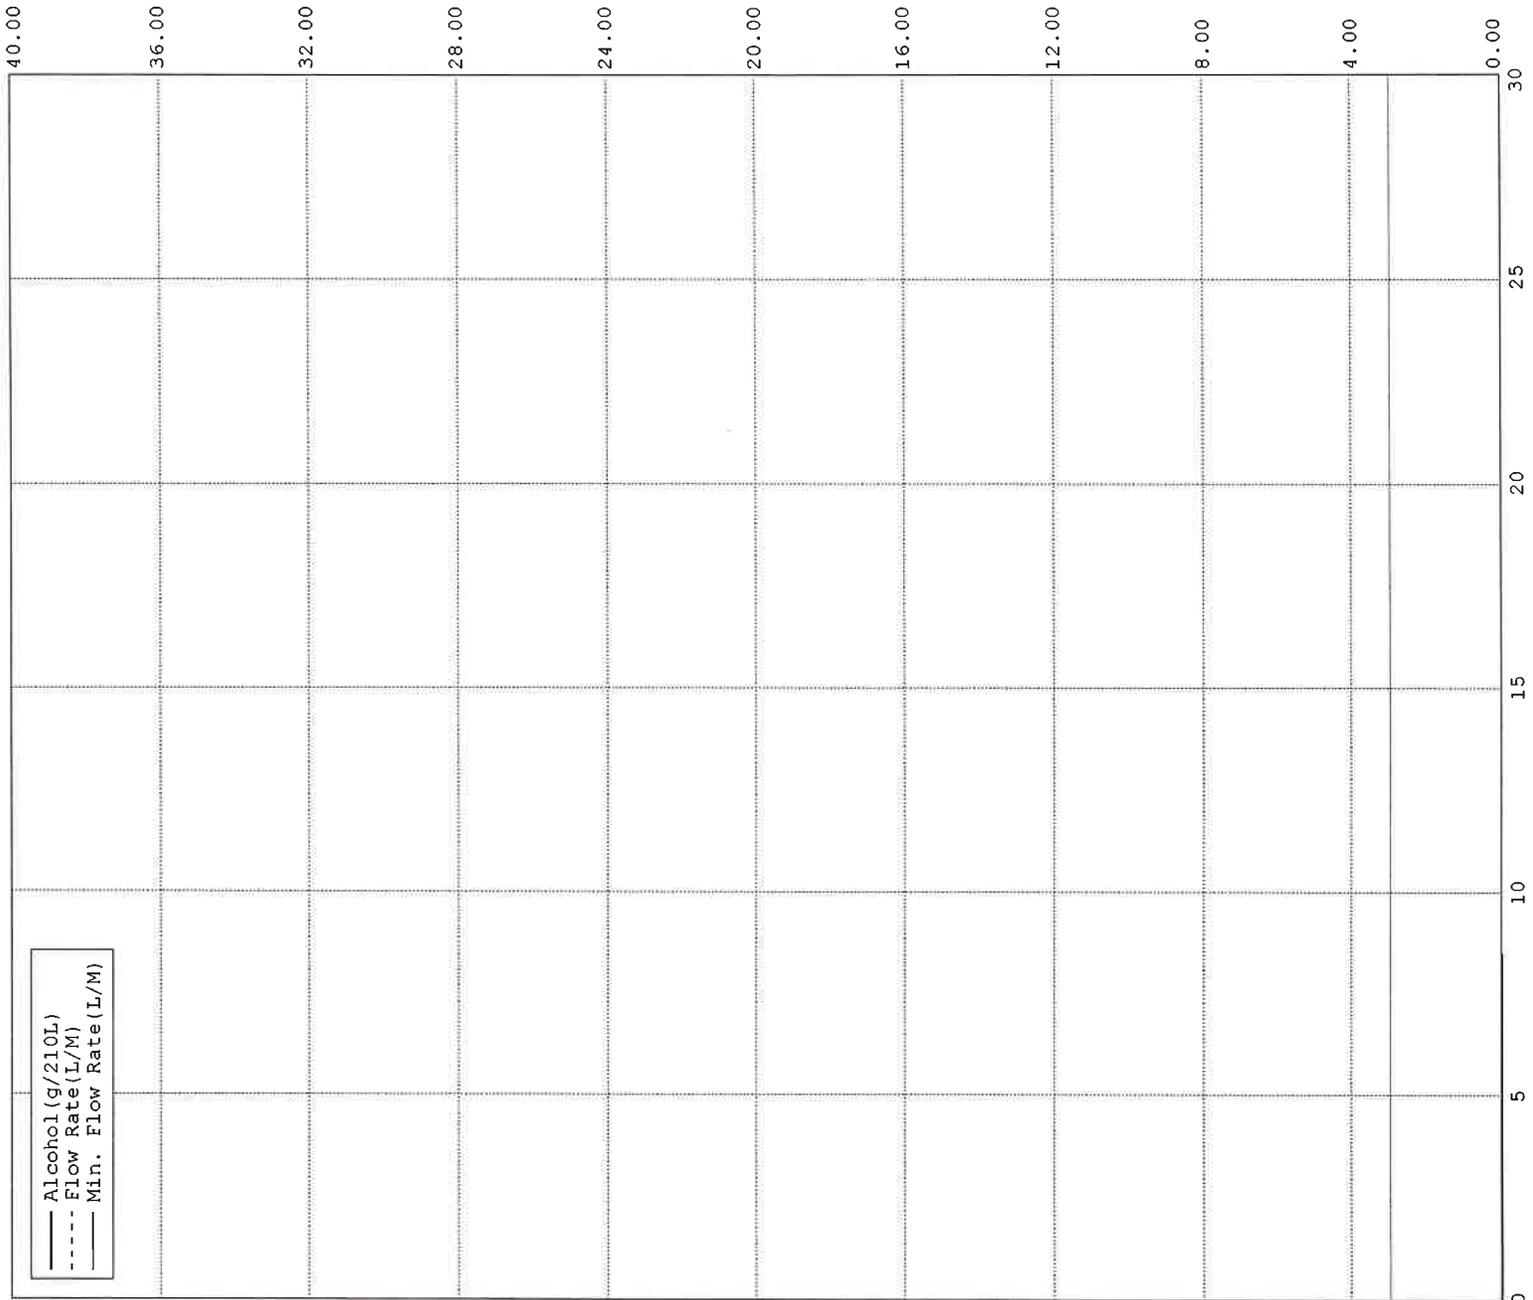

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100386

Date: 02/19/2026  
Time: 09:28:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-ACETONE

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 26-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.84: 0.080  
LOT #: AG436502  
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 09:30  
BLANK TEST 0.000 09:30  
INTERNAL STANDARD VERIFIED 09:30  
Xg = 0.099 (1.49%)  
EXTERNAL STANDARD 0.079 09:31  
X[1] = 0.0795 (-0.0013) (0.0009)  
BLANK TEST 0.000 09:31  
SUBJECT SAMPLE XXX 09:32  
X[1] = 0.1104 (-0.0151) (0.0024)

Interference Detected

*Filter Avg = -0.0007*

*Filter Avg = 0.0010*

*COB*



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100386

Date: 02/19/2026  
Time: 09:38:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: INT-IPA

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237


DEPT/AGENCY:  
AAA1  
CASE/REPORT: 26-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.83: 0.080  
LOT #: AG436502  
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	09:40
BLANK TEST	0.000	09:41
INTERNAL STANDARD	VERIFIED	09:41
Xq = 0.100 (0.26%)		
EXTERNAL STANDARD	0.079	09:41
X[1] = 0.0789 (-0.0008) (0.0014)		
BLANK TEST	0.000	09:42
SUBJECT SAMPLE	XXX	09:43
X[1] = 0.1166 (-0.0242) (-0.0004)		

Interference Detected

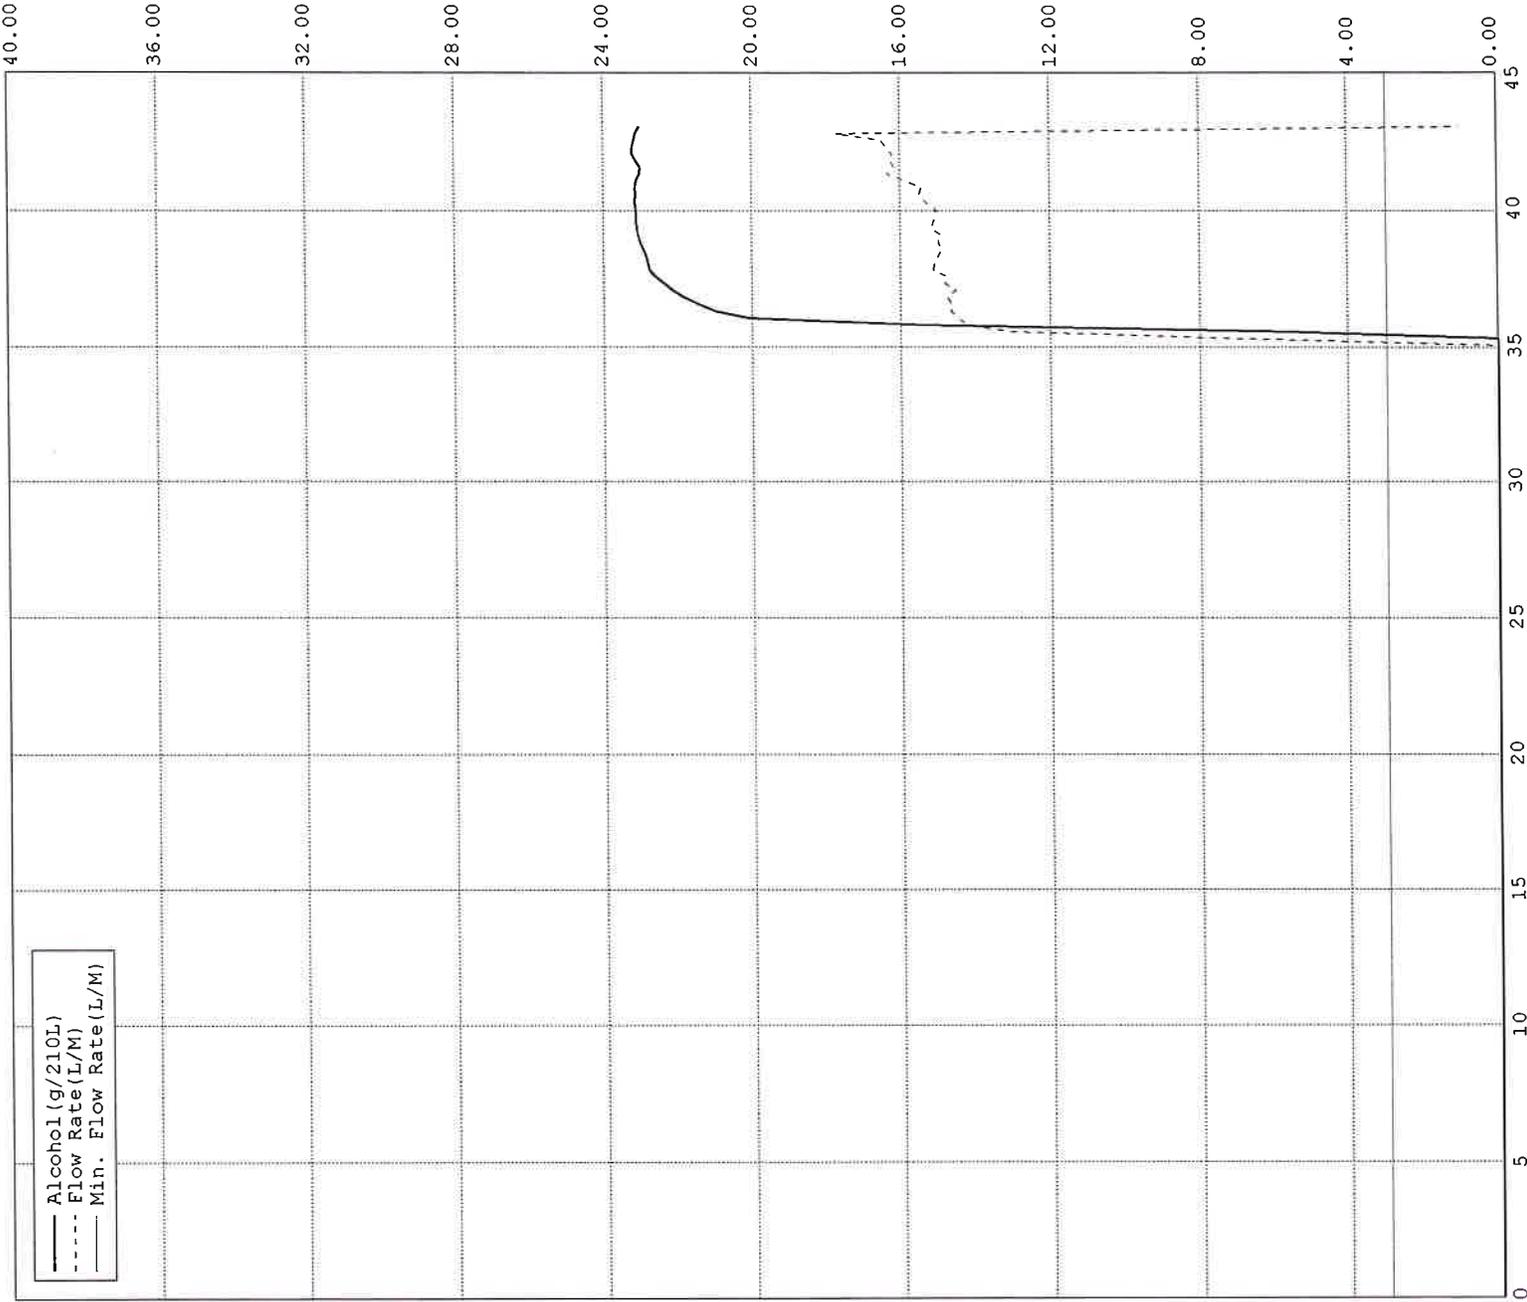

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100386

Date: 02/19/2026

Time: 09:47:42

SUBJECT NAME:

TEST TEST

LICENSE #: INT-NEGATIVE

OPERATOR NAME:

COLLEEN S O'BRYAN

OPERATOR'S #: 6237

DEPT/AGENCY:

AAA1

CASE/REPORT: 26-1234

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.83: 0.080

LOT #: AG436502

EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK PASSED 09:49

BLANK TEST 0.000 09:50

INTERNAL STANDARD VERIFIED 09:50

Xg = 0.100 (0.09%)

EXTERNAL STANDARD 0.079 09:50

X[1] = 0.0794 (-0.0001) (0.0019)

BLANK TEST 0.000 09:51

SUBJECT SAMPLE (Vol=1.91L) 0.095 09:51


X[1] = 0.0950 (0.0015) (-0.0004)

BLANK TEST 0.000 09:52

EXTERNAL STANDARD 0.080 09:53

X[1] = 0.0796 (-0.0007) (-0.0001)

BLANK TEST 0.000 09:54

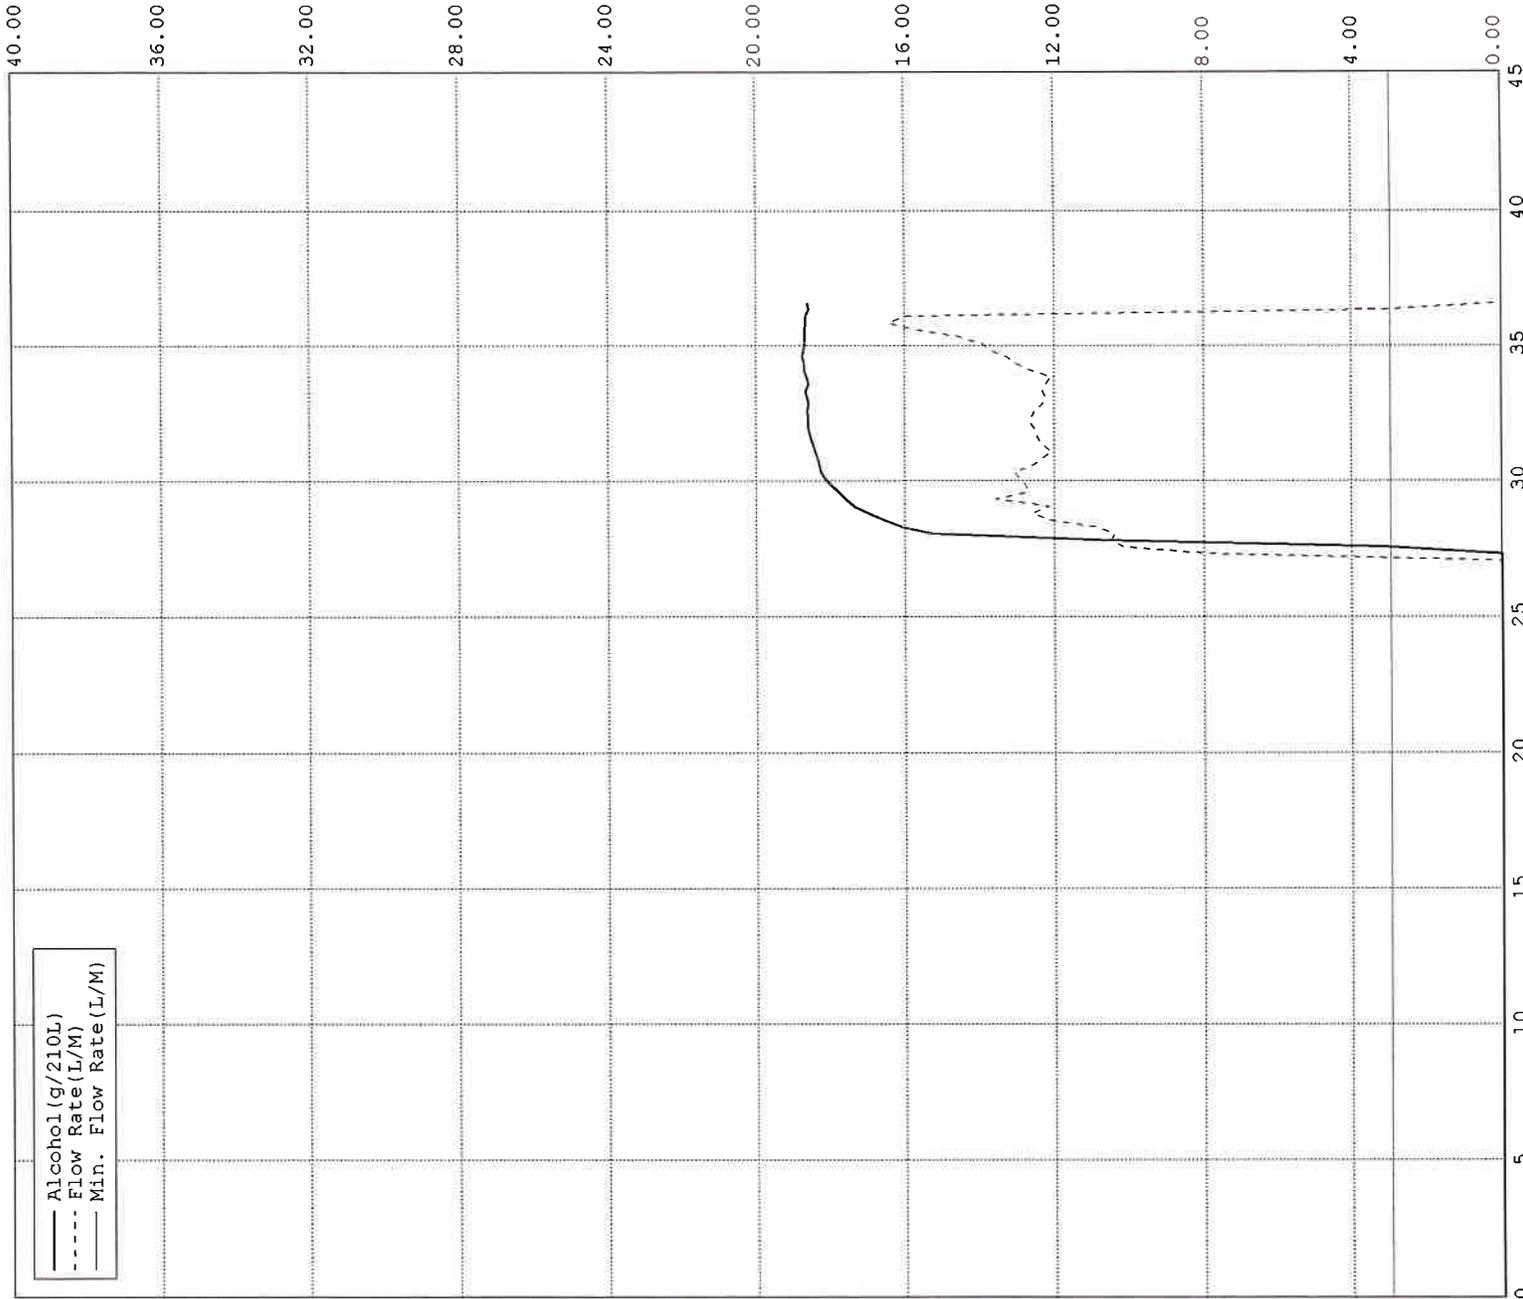

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100386

Date: 02/19/2026  
Time: 11:49:07

SUBJECT NAME:  
TEST TEST  
LICENSE #: NDST

OPERATOR NAME:  
COLLEEN S O'BRYAN  
OPERATOR'S #: 6237

DEPT/AGENCY:  
AAA1  
CASE/REPORT: 26-1234  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.79: 0.080  
LOT #: AG436502  
EXPIRATION: 12/30/2026

DIAGNOSTIC CHECK	PASSED	11:50
BLANK TEST	0.000	11:50
INTERNAL STANDARD	VERIFIED	11:50
EXTERNAL STANDARD	0.079	11:50
BLANK TEST	0.000	11:51
SUBJECT SAMPLE (Vol=1.63L)	0.000	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.080	11:53
BLANK TEST	0.000	11:54

