




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100676

Report Issue Date: 01/10/2025
Date Received: 2024-12-09
Condition of Item: Damaged

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.020	0.020
0.080	0.079	09523080A1	0.080	0.080	0.079	0.079	0.079	0.079
0.300	0.297	AG427706	0.295	0.295	0.295	0.295	0.294	0.295

As Found - Evaluation Analyst: Megan Carlock

As Found Conditions - Barometric Pressure (inHg): 29.57 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.6 Relative Humidity (%): 21

As-Found Lab Activity Date Range: 12/09/2024 - 12/10/2024

Resecured the double check valve to the wall and replaced the O-ring.

Linearity was performed since it is not influenced by the piece detached from the breath hose, however a non-drinking subject test could not be performed due to this issue.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.020	0.020	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.040	0.040	0.039	0.039	0.039	0.039	+/- 0.003
0.080	0.078	09523080A1	0.079	0.078	0.078	0.078	0.078	0.078	+/- 0.004
0.100	0.097	AG333401	0.098	0.098	0.098	0.097	0.098	0.098	+/- 0.004
0.150	0.146	AG332004	0.143	0.143	0.143	0.144	0.143	0.143	+/- 0.006
0.300	0.292	AG427706	0.290	0.290	0.290	0.290	0.290	0.290	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.11 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.3 Relative Humidity (%): 20

As-Left Lab Activity Date Range: 12/11/2024 - 12/11/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Serial Number: 100676

Results authorized by Megan Carlock on 12/11/2024

megan.crouse@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 01/10/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100676 Analyst or Technician Name: Megan Carlock
DataMaster DMT Calibration Start Date: 12/11/24

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230367229
Calibration Due Date: 5/2/2025
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.11 Temperature(C) 22.3 Relative Humidity(%) 20
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)
- ☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR4161 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR5298 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 9/20/25
Simulator S/N: DR4163 Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 12/11/24
Data Interpretation Date (Technician): N/A (if applicable)
Data Interpretation Date (Analyst): 12/11/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

 Alaska Department of Public Safety
 DATAMASTER dmt: 100676

Date: 12/11/2024
 Time: 08:16:47

VERSIONS
 DMT: 3.02
 PIC: 3.03
 Modem: 2.6
 Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 48.1°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.62 V	PASSED
(0.98 V - 2.30 V)	
Cooler Voltage = 1.74 V	PASSED
(1.02 V - 2.38 V)	
Bias Voltage = 78 V	PASSED
(47 V - 109 V)	
Chopper Freq = 536 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.2 in	

PUMP INFO

Flow Rate = 4.082 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.001 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.090 0.29% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100676

Date: 12/11/2024

Time: 8:41 AM

Temperatures (°C)

Sample Cell: 49.4°C

Breath Tube: 47.7°C

Current Barometer 29.1 in

Volume (Ltr) 1.48

Settings

Lamp: 1.67 V

Bias: 78 V

Cooler: 1.74 V

Chopper: 535 Hz

Voltages (V)

Flow: 1.06 V

Detector: -0.008 V


CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100676

Date: 06/18/2024
Time: 12:01:24

OPERATOR NAME:
MEGAN CARLOCK
CERTIFICATE #: 10747

Ca	=	0.1000		
CAL	=	1.007862	0.800	<= CAL < 1.200
b1	=	0.0008	0.0000	<= b1 < 0.0040
b2	=	0.0055	0.0010	<= b2 < 0.0100
b3	=	0.0006	0.0000	<= b3 < 0.0040
Xq	=	0.0907	0.0500	<= Xq < 0.2000
a21	=	1.234429	1.050	<= a21 < 1.300
a31	=	0.571716	0.300	<= a31 < 0.800

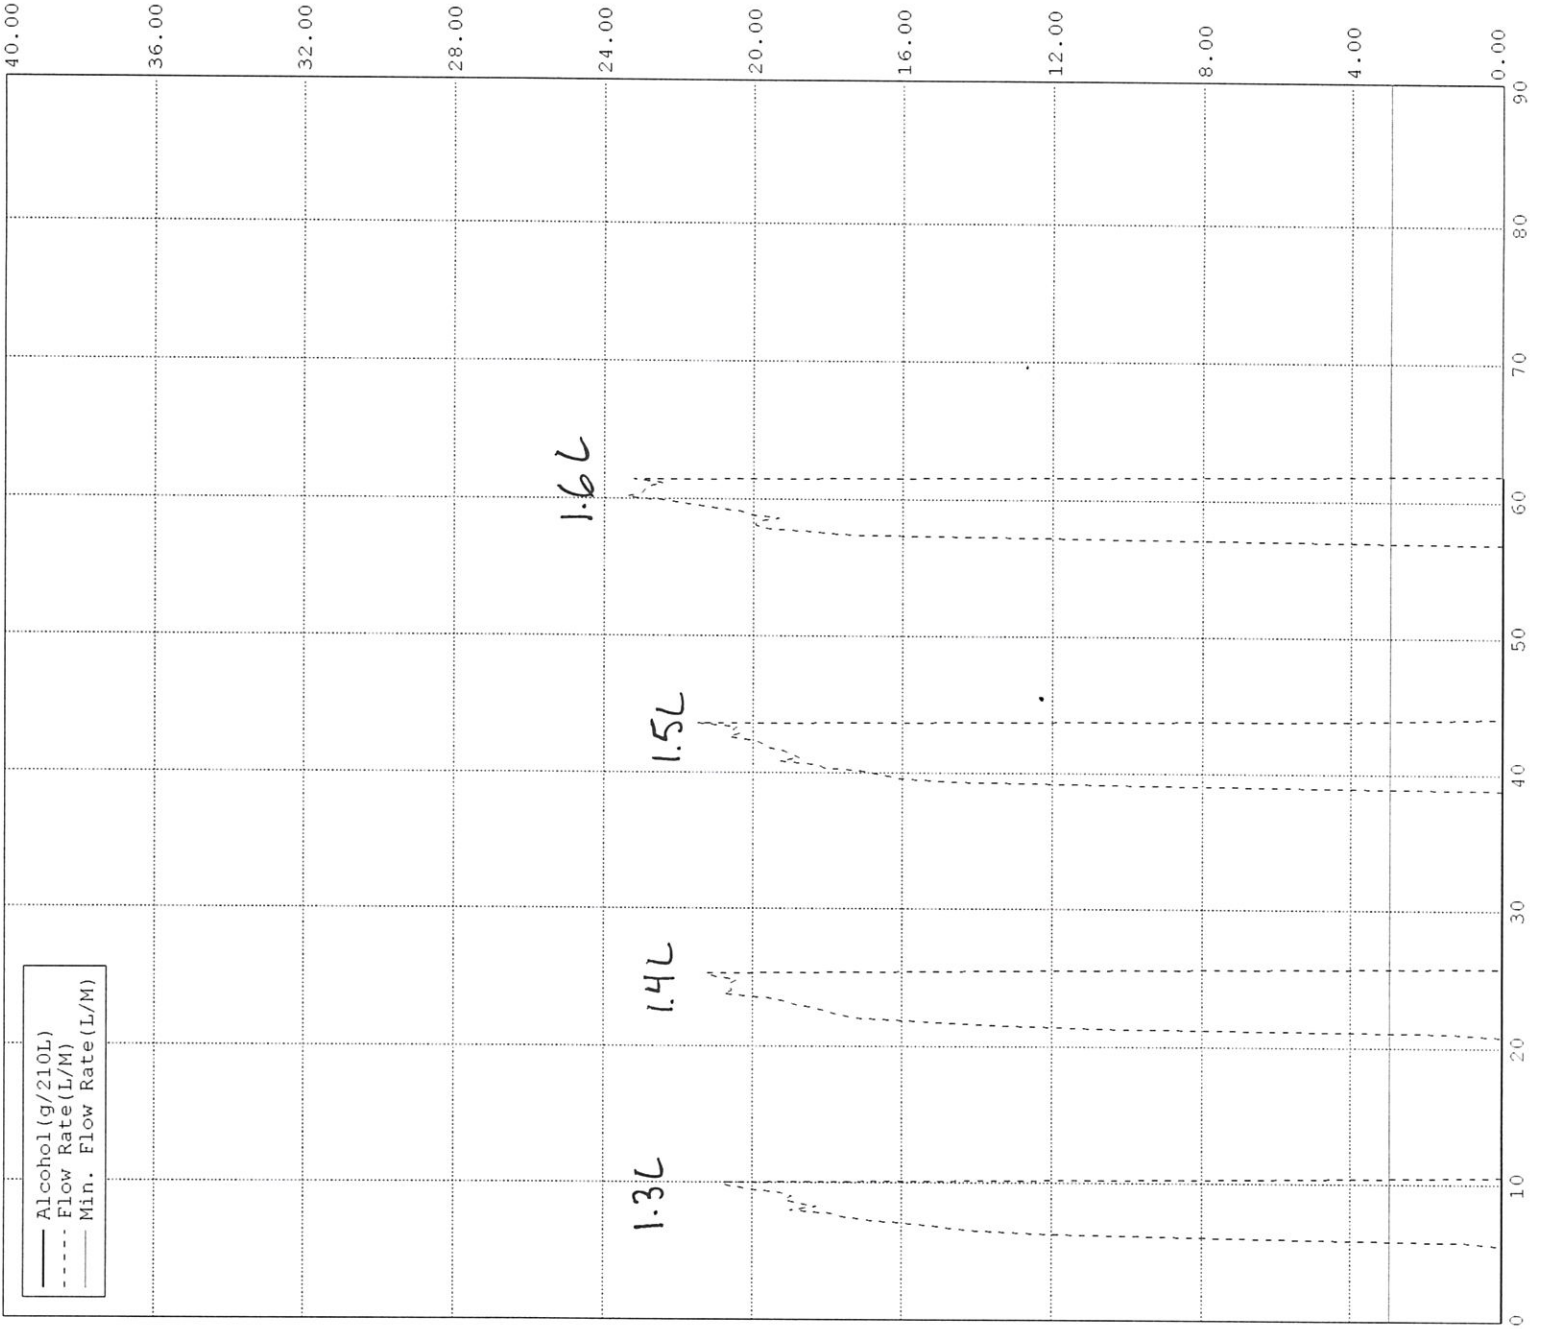

SUBJECT TEST	

Alaska Department of Public Safety	
DATAMASTER dmt: 100676	

Date: 12/11/2024	
Time: 08:44:26	
SUBJECT NAME:	
TEST TEST	
LICENSE #: XXX	
OPERATOR NAME:	
MEGAN CARLOCK	
OPERATOR'S #: 10747	
DEPT/AGENCY:	
MINIMUM VOLUME TEST	
CASE/REPORT: XXX	
TEST TYPE: TEST	
EXTERNAL STANDARD INFORMATION	
NOMINAL: 0.080	
TARGET AT 29.12: 0.078	
LOT #: 09523080A1	
EXPIRATION: 05/05/2025	
DIAGNOSTIC CHECK	PASSED 08:45
BLANK TEST	0.000 08:45
INTERNAL STANDARD	VERIFIED 08:45
EXTERNAL STANDARD	0.078 08:45
BLANK TEST	0.000 08:46
SUBJECT SAMPLE (Vol=1.57L)	0.000 08:47
BLANK TEST	0.000 08:48
EXTERNAL STANDARD	0.079 08:49
BLANK TEST	0.000 08:49

MNC

100676 2024.12.11 Calibration Page 7 of 22

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100676

Date: 12/11/2024
 Time: 10:09:08

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.019	0.0200	0.0000
0.039	0.0394	0.0005
0.078	0.0782	0.0004
0.097	0.0978	0.0004
0.146	0.1432	0.0004
0.292	0.2900	0.0000

SLOPE = 0.987803
 R^2 = 0.999886

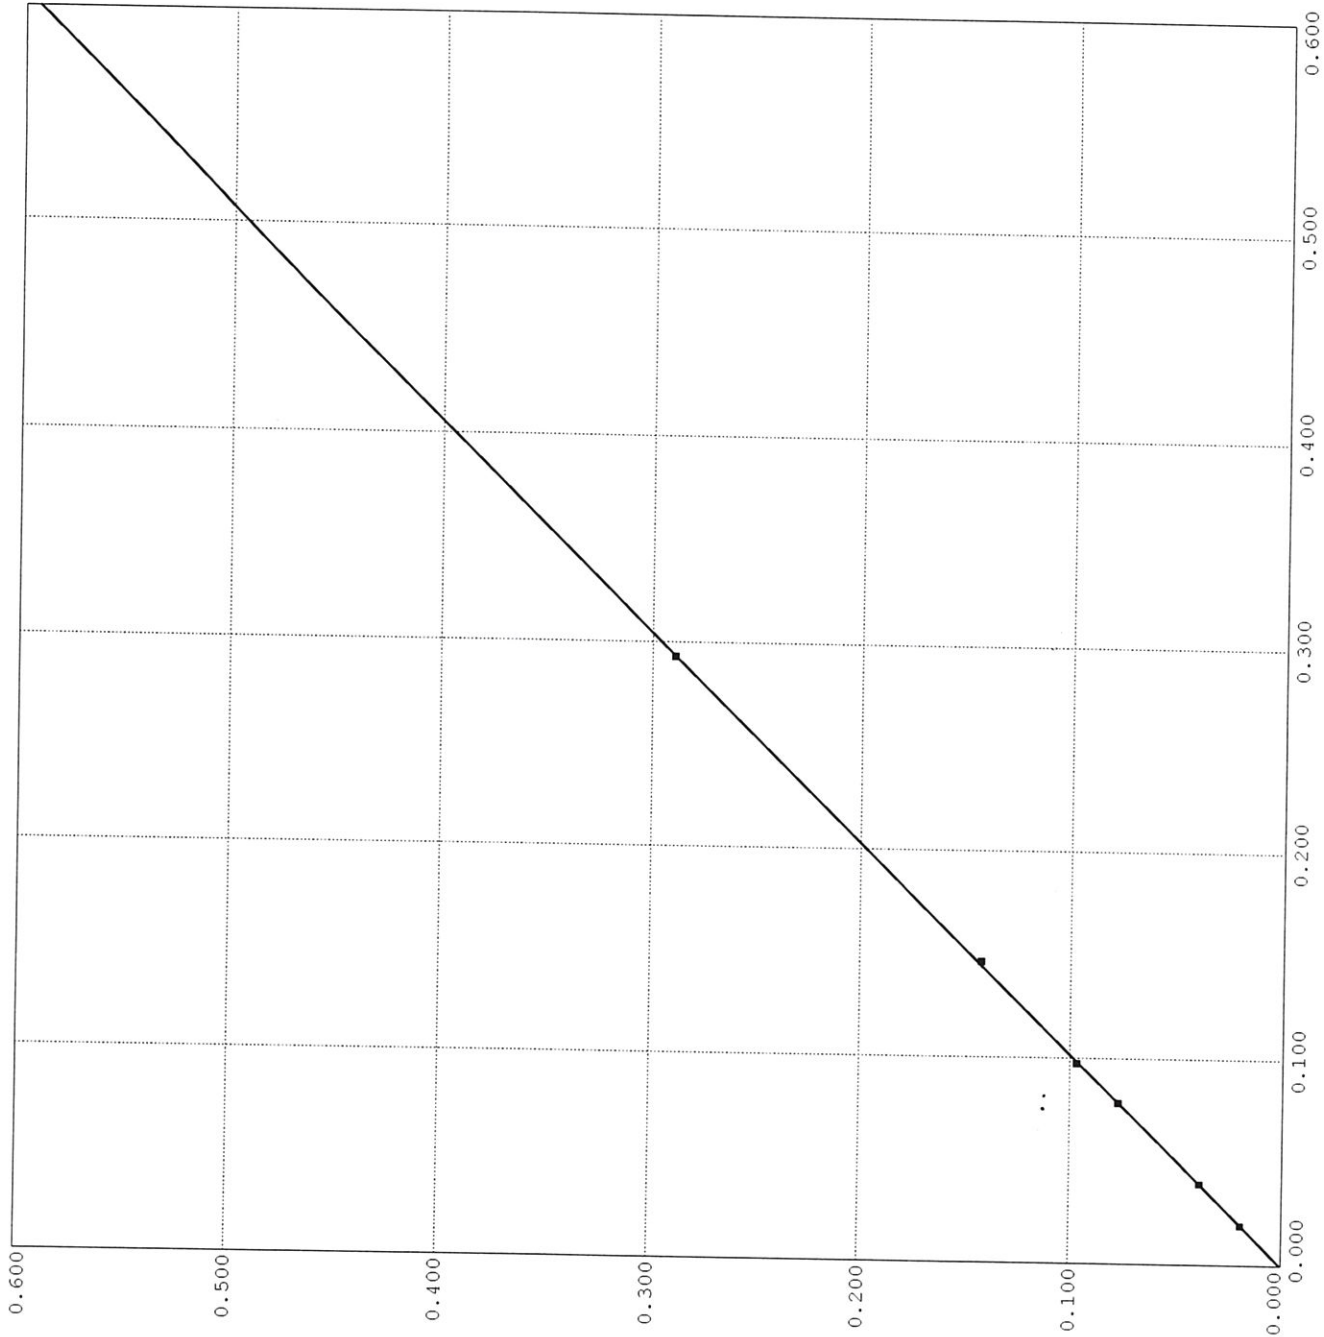

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100676






Date: 12/11/2024
Time: 10:09:10

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.10: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 274 psi

BLANK TEST	0.000	10:10
INTERNAL STANDARD	VERIFIED	10:10
EXTERNAL STANDARD	0.020	10:11
BLANK TEST	0.000	10:11
EXTERNAL STANDARD	0.020	10:12
BLANK TEST	0.000	10:12
EXTERNAL STANDARD	0.020	10:13
BLANK TEST	0.000	10:14
EXTERNAL STANDARD	0.020	10:14
BLANK TEST	0.000	10:15
EXTERNAL STANDARD	0.020	10:15
BLANK TEST	0.000	10:16

Average = 0.0200
Std Dev = 0.0000

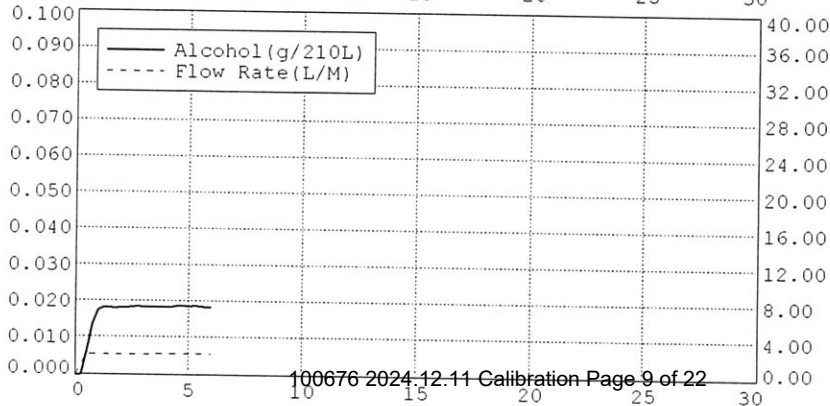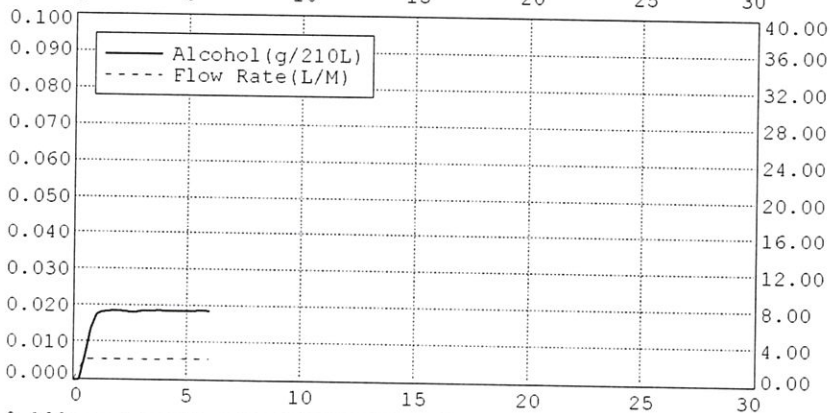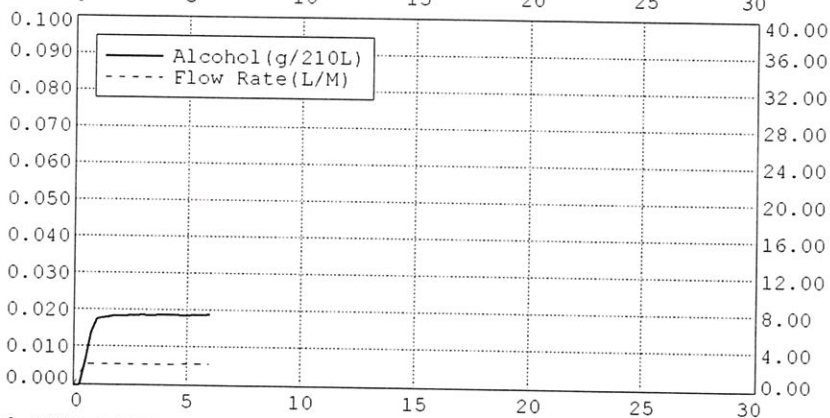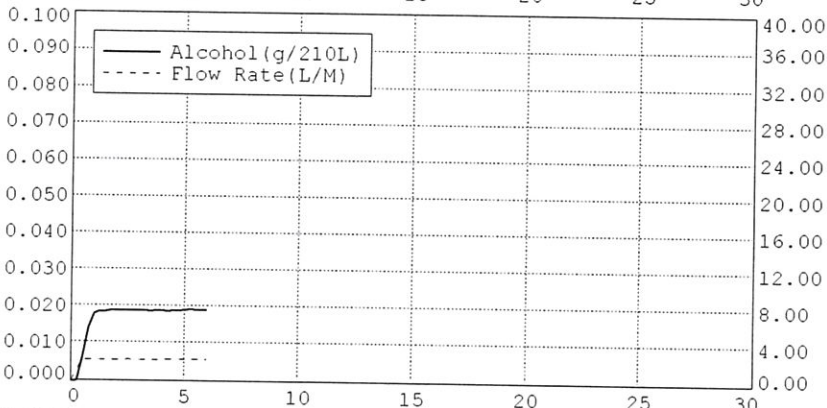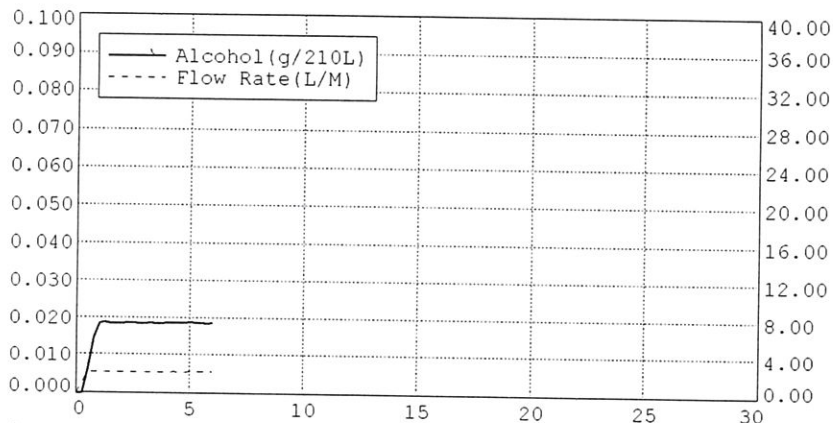

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100676






Date: 12/11/2024
Time: 10:16:59

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.10: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 933 psi

BLANK TEST	0.000	10:18
INTERNAL STANDARD	VERIFIED	10:18
EXTERNAL STANDARD	0.040	10:18
BLANK TEST	0.000	10:19
EXTERNAL STANDARD	0.040	10:19
BLANK TEST	0.000	10:20
EXTERNAL STANDARD	0.039	10:20
BLANK TEST	0.000	10:21
EXTERNAL STANDARD	0.039	10:22
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.039	10:23
BLANK TEST	0.000	10:24

Average = 0.0394
Std Dev = 0.0005

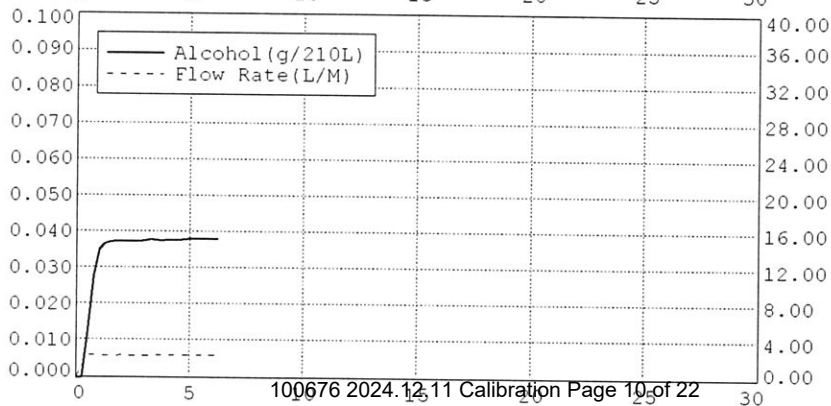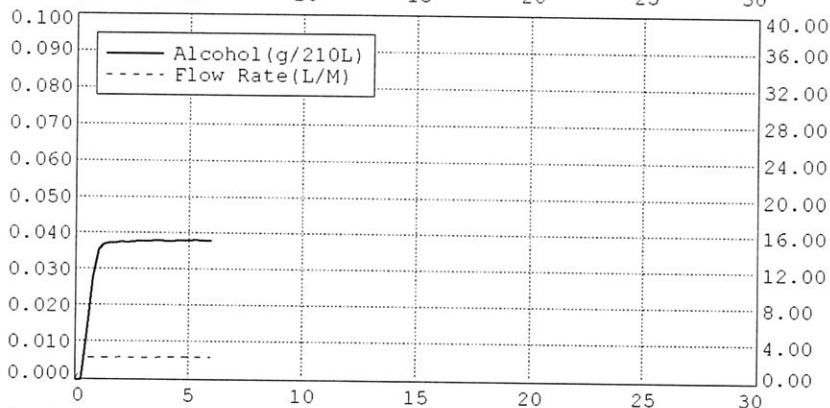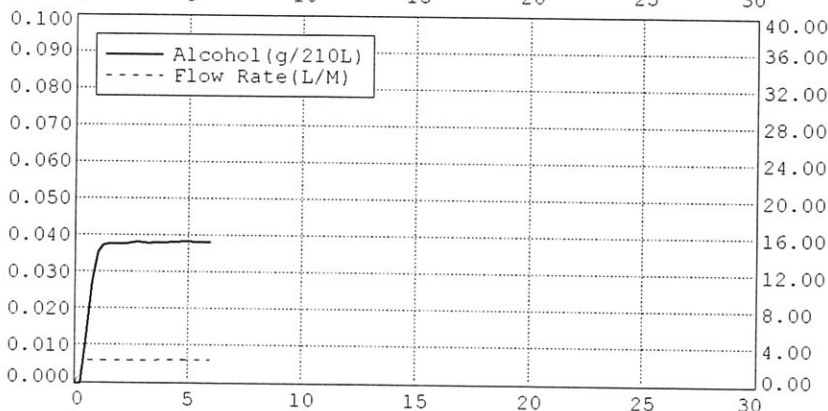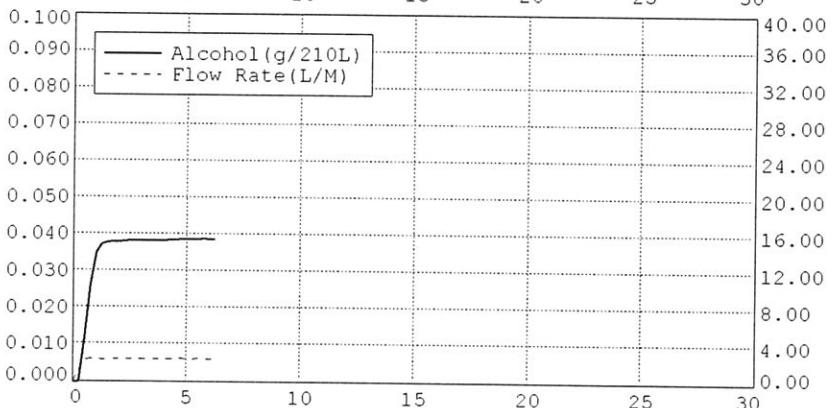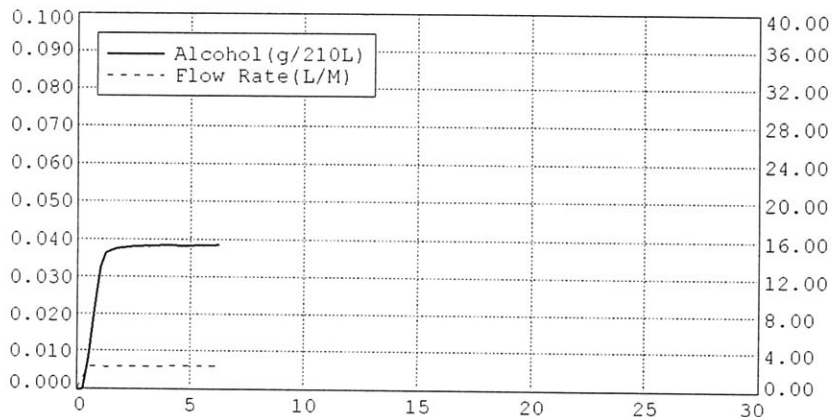

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100676






Date: 12/11/2024
Time: 10:25:04

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: 09523080A1
EXPIRATION: 05/05/2025
TANK PRESSURE: 210 psi

BLANK TEST	0.000	10:26
INTERNAL STANDARD	VERIFIED	10:26
EXTERNAL STANDARD	0.079	10:26
BLANK TEST	0.000	10:27
EXTERNAL STANDARD	0.078	10:27
BLANK TEST	0.000	10:28
EXTERNAL STANDARD	0.078	10:29
BLANK TEST	0.000	10:29
EXTERNAL STANDARD	0.078	10:30
BLANK TEST	0.000	10:31
EXTERNAL STANDARD	0.078	10:31
BLANK TEST	0.000	10:32

Average = 0.0782
Std Dev = 0.0004

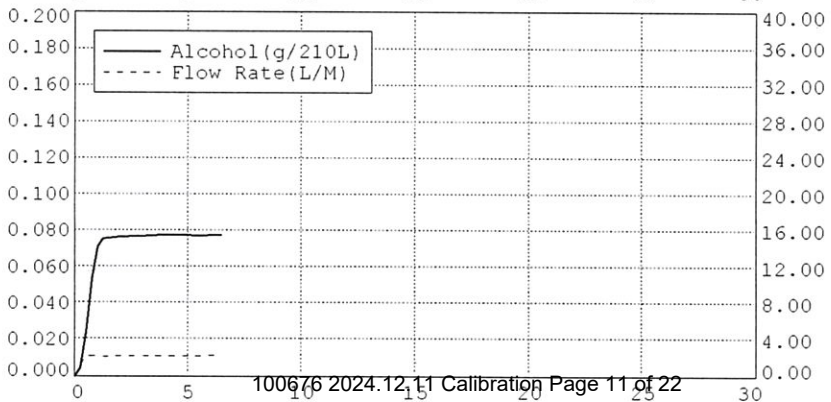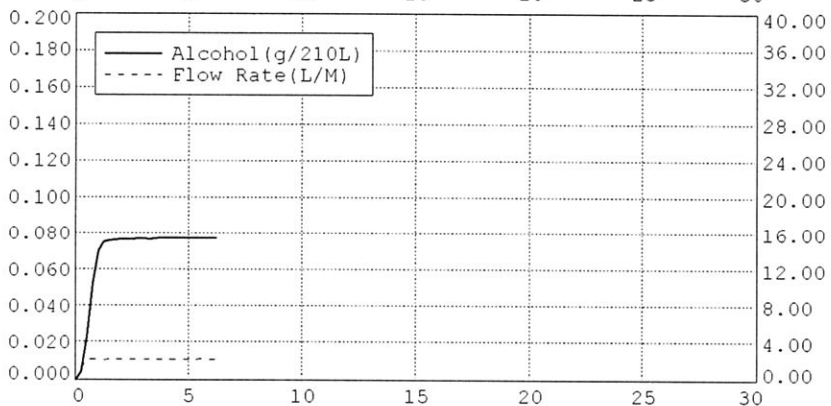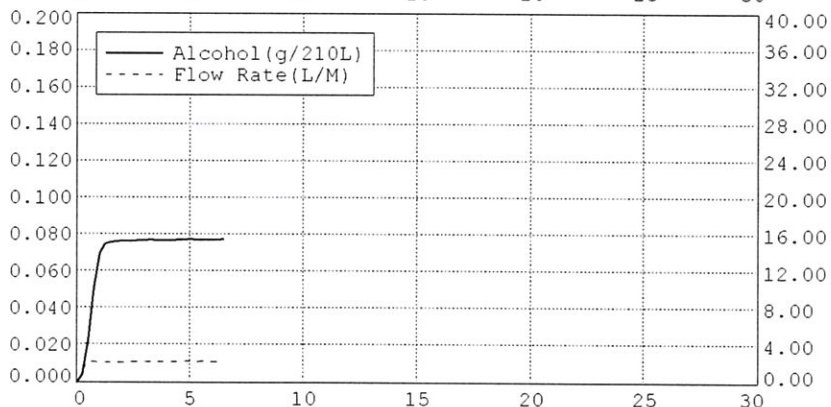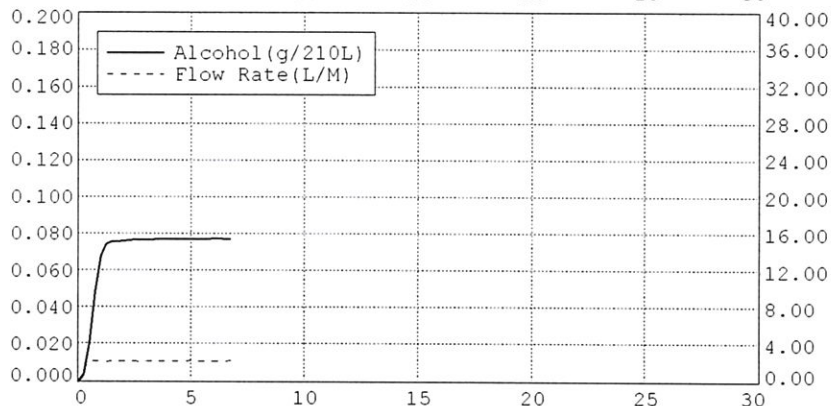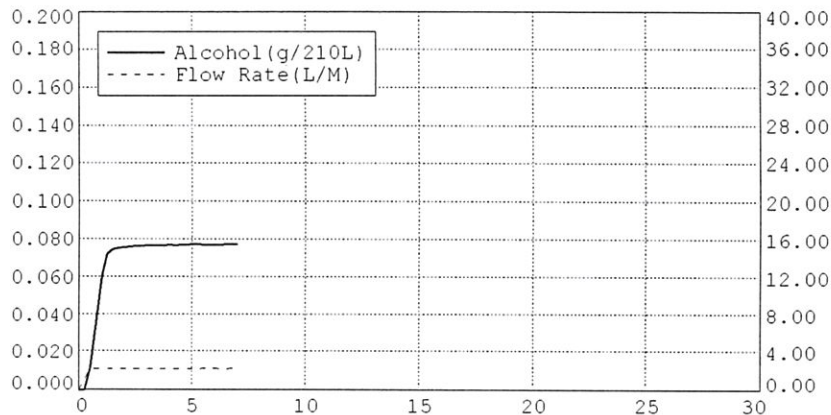

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100676






Date: 12/11/2024
Time: 10:33:22

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.10: 0.097
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 925 psi

TEST TYPE	Result	Time
BLANK TEST	0.000	10:35
INTERNAL STANDARD	VERIFIED	10:35
EXTERNAL STANDARD	0.098	10:35
BLANK TEST	0.000	10:36
EXTERNAL STANDARD	0.098	10:36
BLANK TEST	0.000	10:37
EXTERNAL STANDARD	0.098	10:37
BLANK TEST	0.000	10:38
EXTERNAL STANDARD	0.097	10:38
BLANK TEST	0.000	10:39
EXTERNAL STANDARD	0.098	10:40
BLANK TEST	0.000	10:40

Average = 0.0978
Std Dev = 0.0004

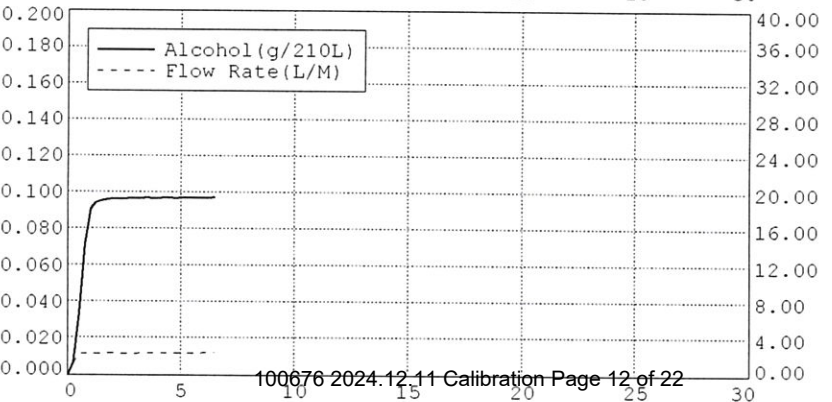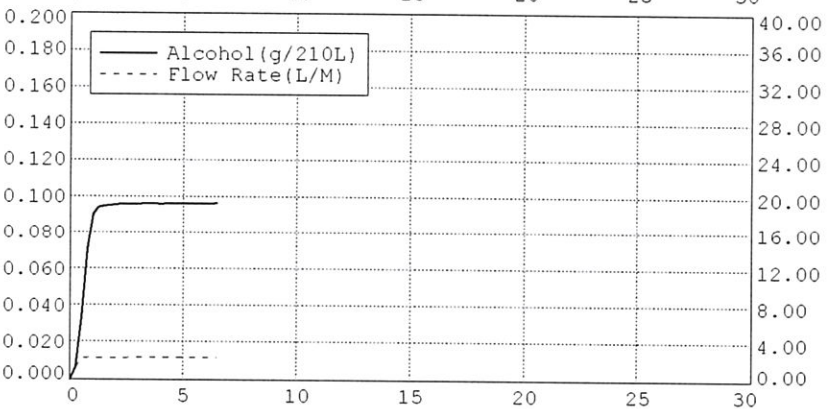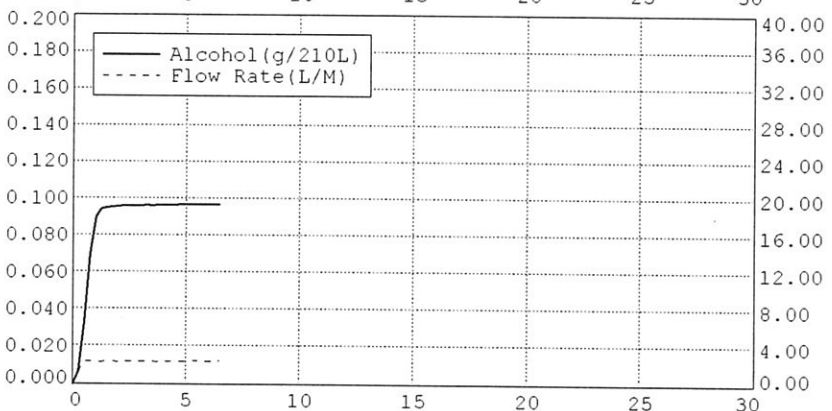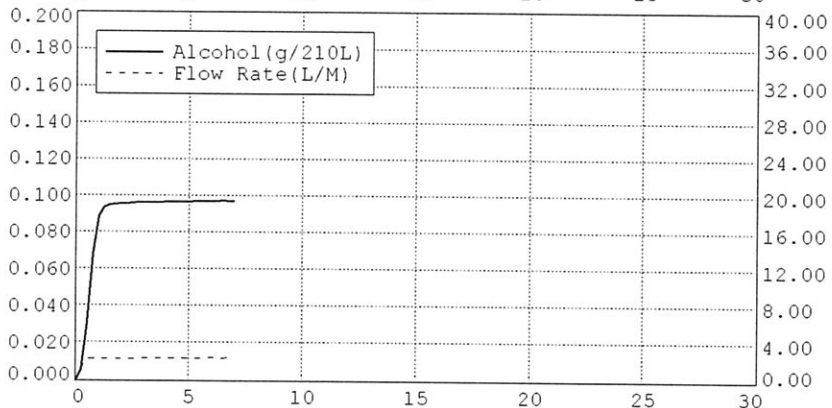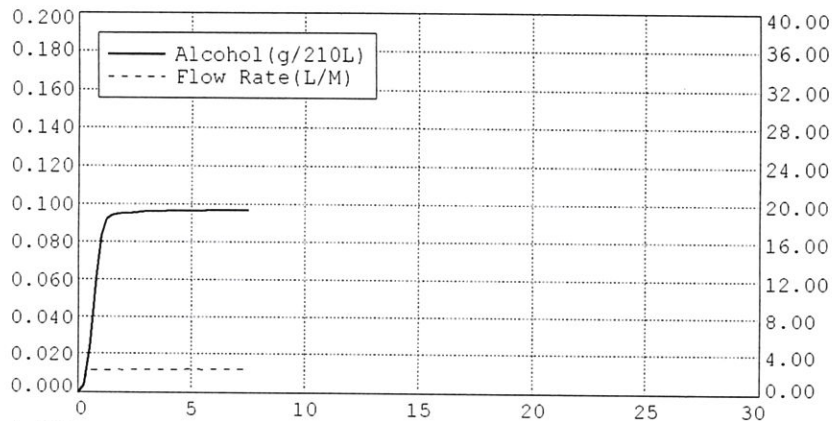

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100676






Date: 12/11/2024
Time: 10:42:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.10: 0.146
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 395 psi

BLANK TEST	0.000	10:43
INTERNAL STANDARD	VERIFIED	10:43
EXTERNAL STANDARD	0.143	10:44
BLANK TEST	0.000	10:45
EXTERNAL STANDARD	0.143	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.143	10:46
BLANK TEST	0.000	10:47
EXTERNAL STANDARD	0.144	10:47
BLANK TEST	0.000	10:48
EXTERNAL STANDARD	0.143	10:48
BLANK TEST	0.000	10:49

Average = 0.1432
Std Dev = 0.0004

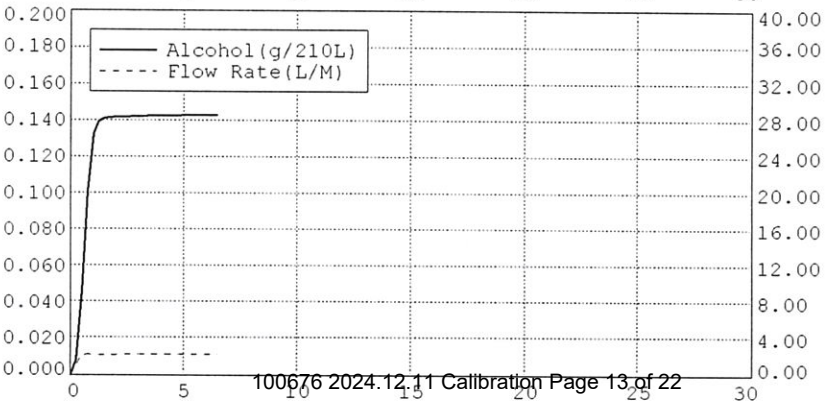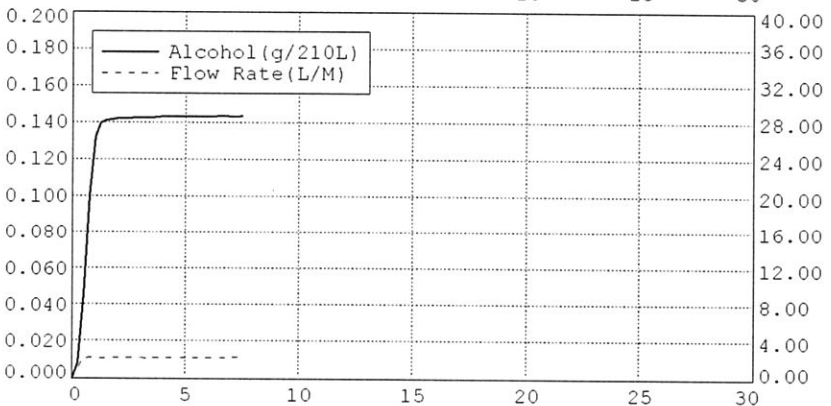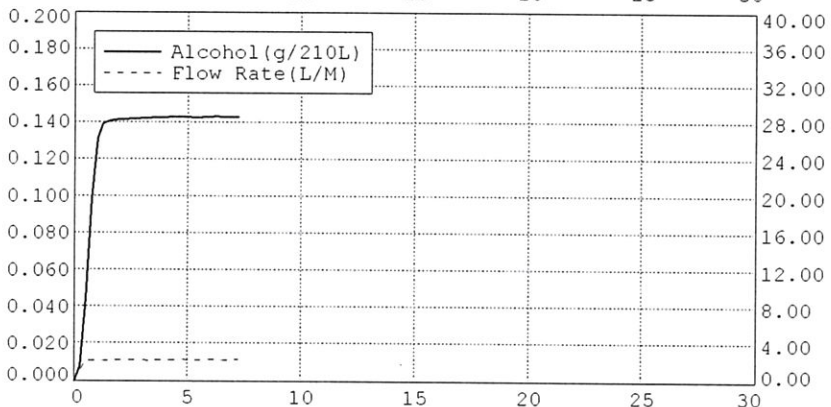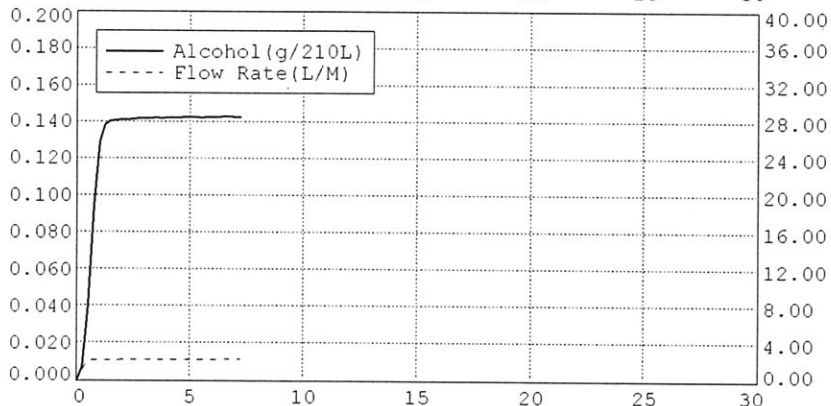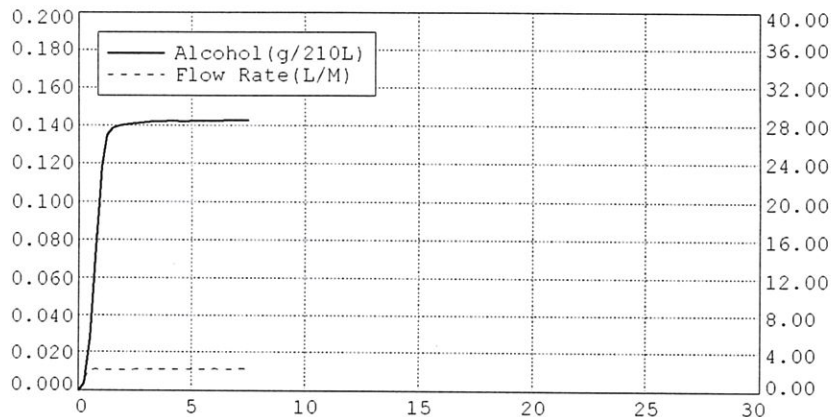

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100676






Date: 12/11/2024
Time: 10:52:43


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.10: 0.292
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 228 psi

BLANK TEST	0.000	10:54
INTERNAL STANDARD	VERIFIED	10:54
EXTERNAL STANDARD	0.290	10:54
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.290	10:55
BLANK TEST	0.000	10:56
EXTERNAL STANDARD	0.290	10:56
BLANK TEST	0.000	10:57
EXTERNAL STANDARD	0.290	10:57
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.290	10:59
BLANK TEST	0.000	10:59

Average = 0.2900
Std Dev = 0.0000

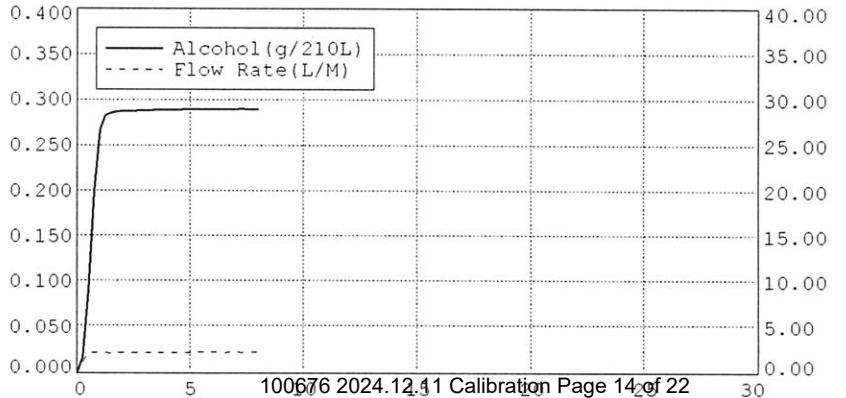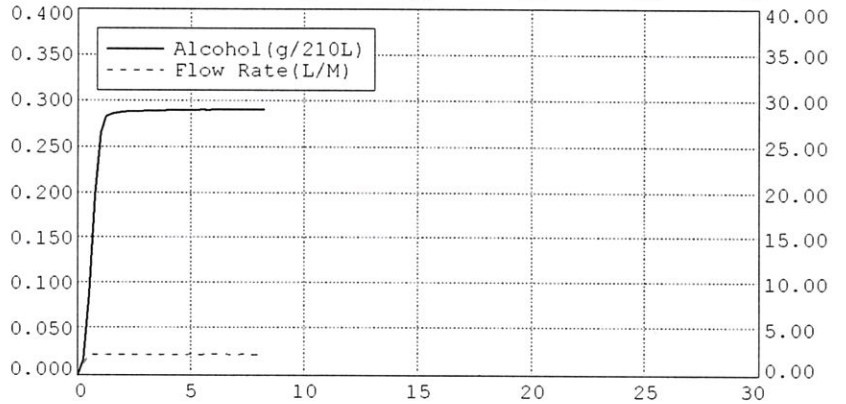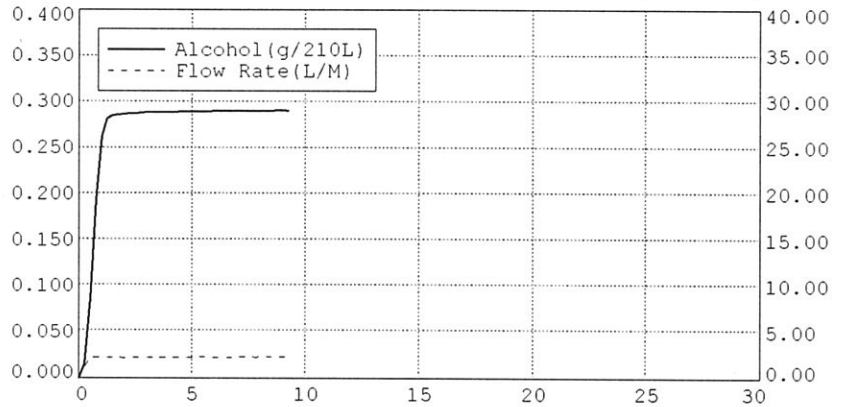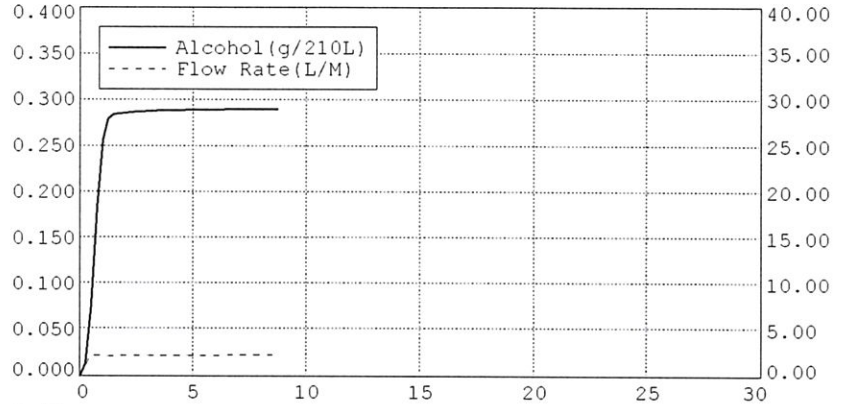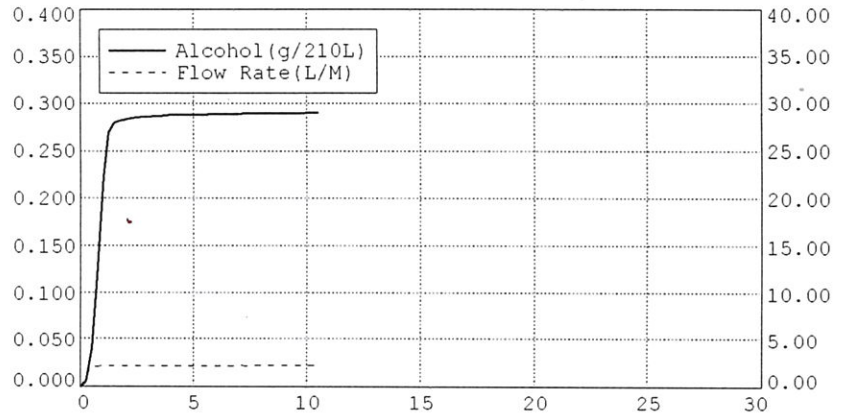

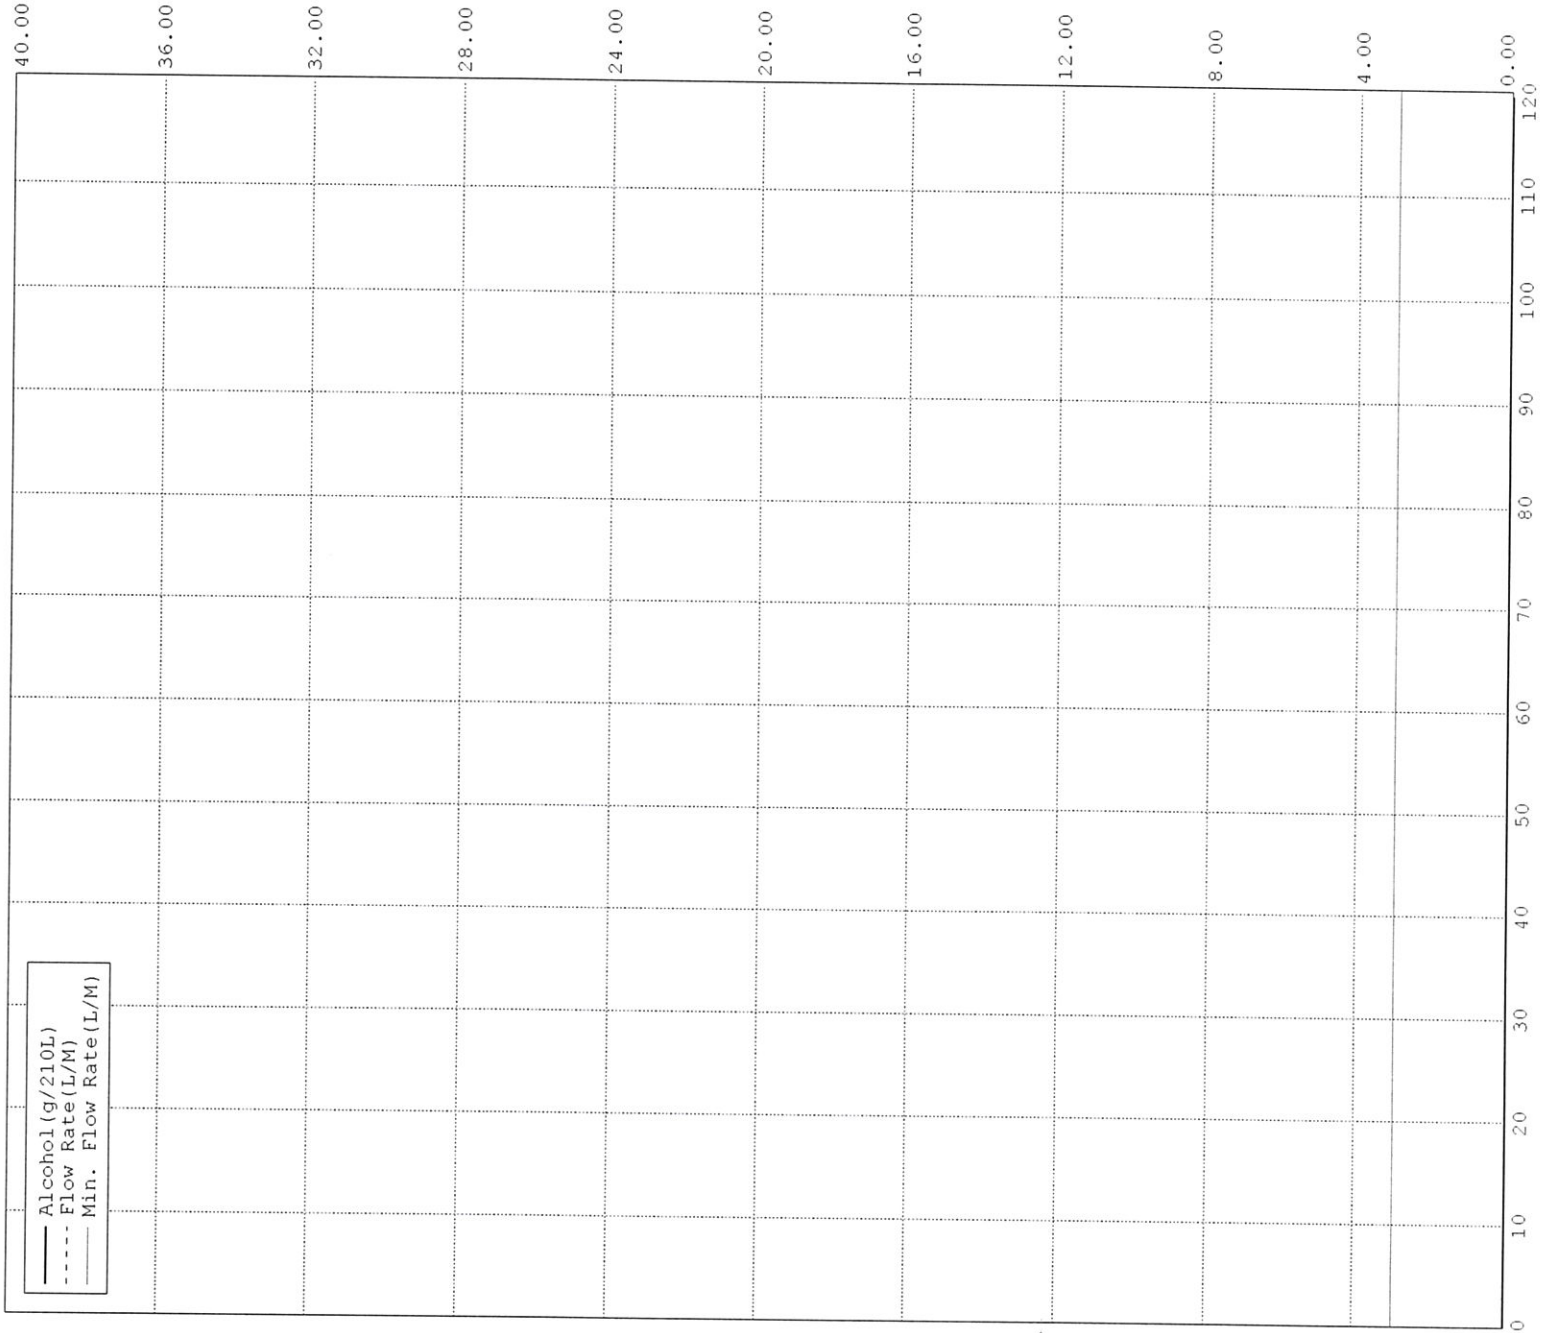

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100676

Date: 12/11/2024
Time: 11:03:45

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	11:04
BLANK TEST	0.000	11:04
INTERNAL STANDARD	VERIFIED	11:04
EXTERNAL STANDARD	0.079	11:05
BLANK TEST	0.000	11:06
SUBJECT SAMPLE	INCOMPLETE	11:08

MNC

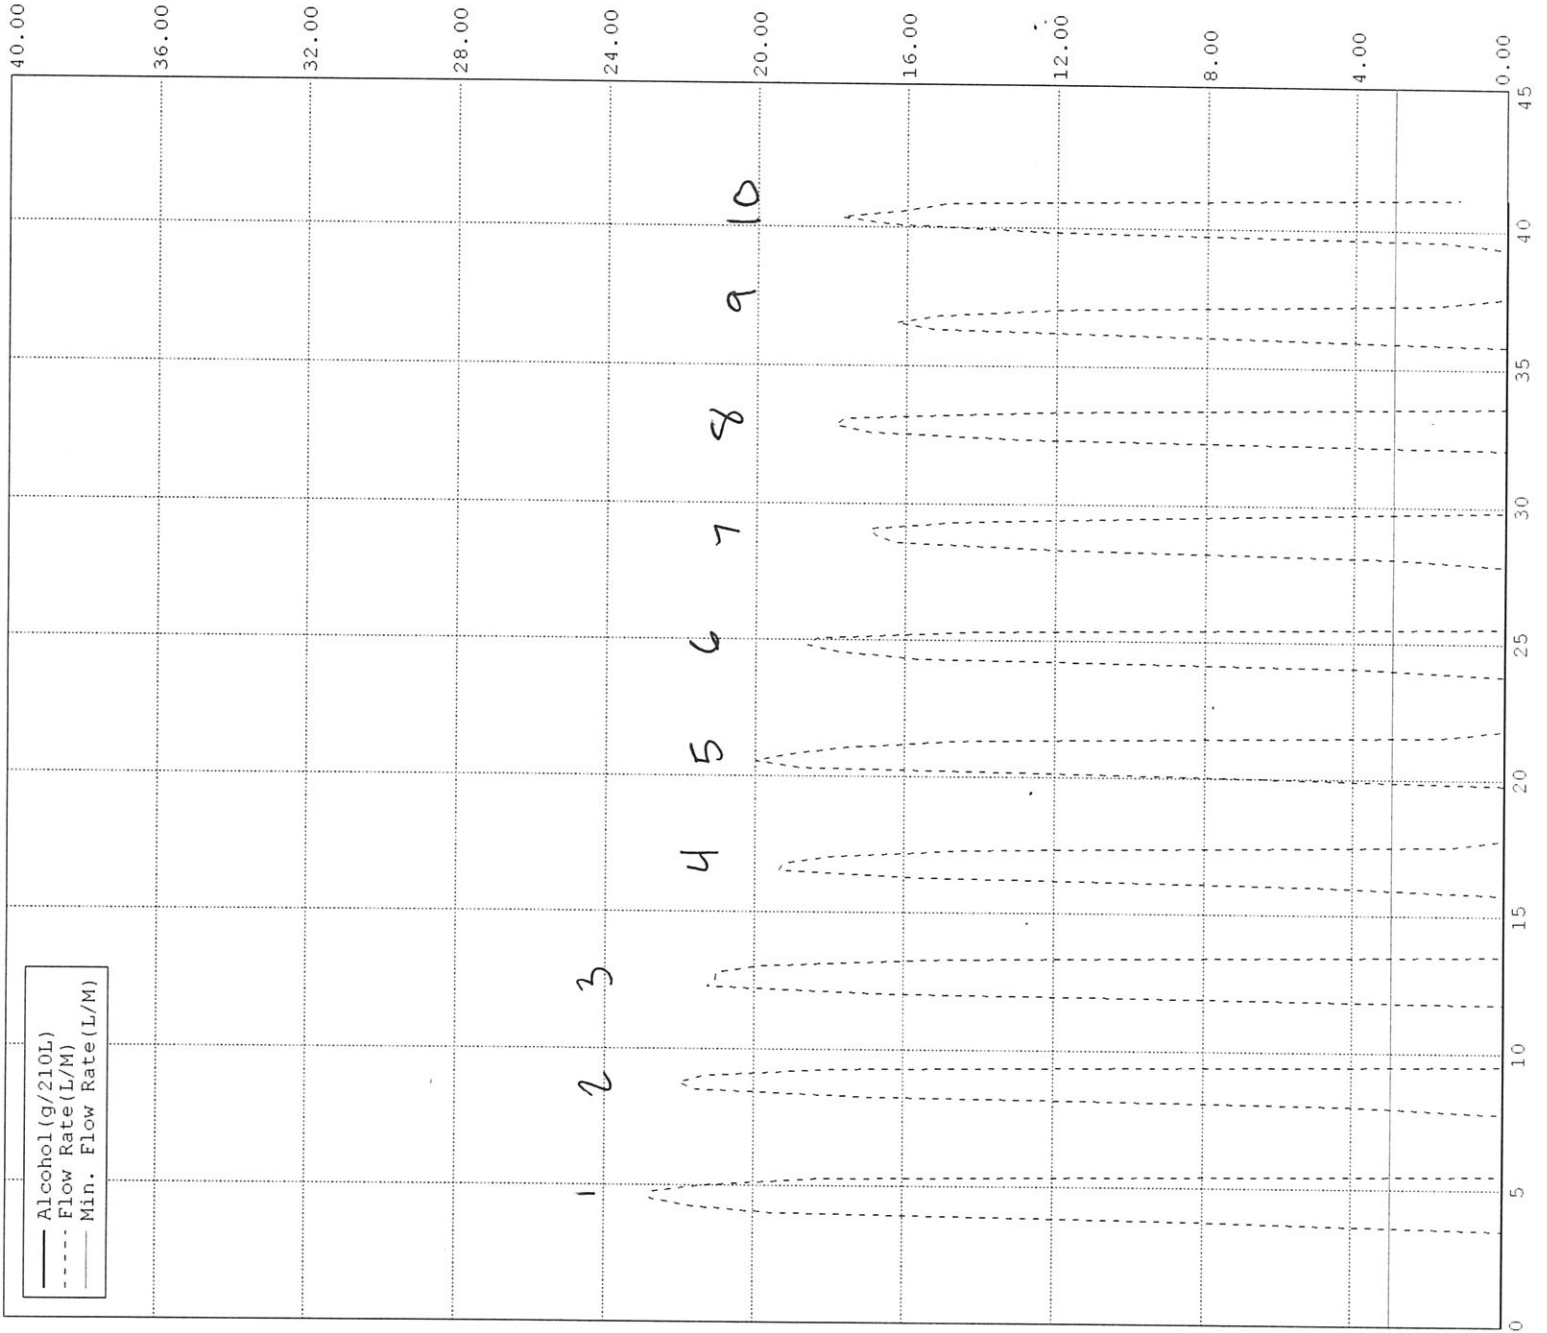

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100676

Date: 12/11/2024
Time: 11:09:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 11:11
INTERNAL STANDARD VERIFIED 11:11
EXTERNAL STANDARD 0.079 11:11
BLANK TEST 0.000 11:12
SUBJECT SAMPLE XXX 11:13

Maximum Attempts Exceeded

MNC

100676 2024.12.11 Calibration Page 16 of 22

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100676

Date: 12/11/2024
 Time: 11:15:21

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX


OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:
 INVALID
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.10: 0.078
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	11:17
BLANK TEST	0.000	11:17
INTERNAL STANDARD	VERIFIED	11:18
EXTERNAL STANDARD	0.079	11:18
BLANK TEST	0.000	11:19
SUBJECT SAMPLE	INVALID	11:19

MNC

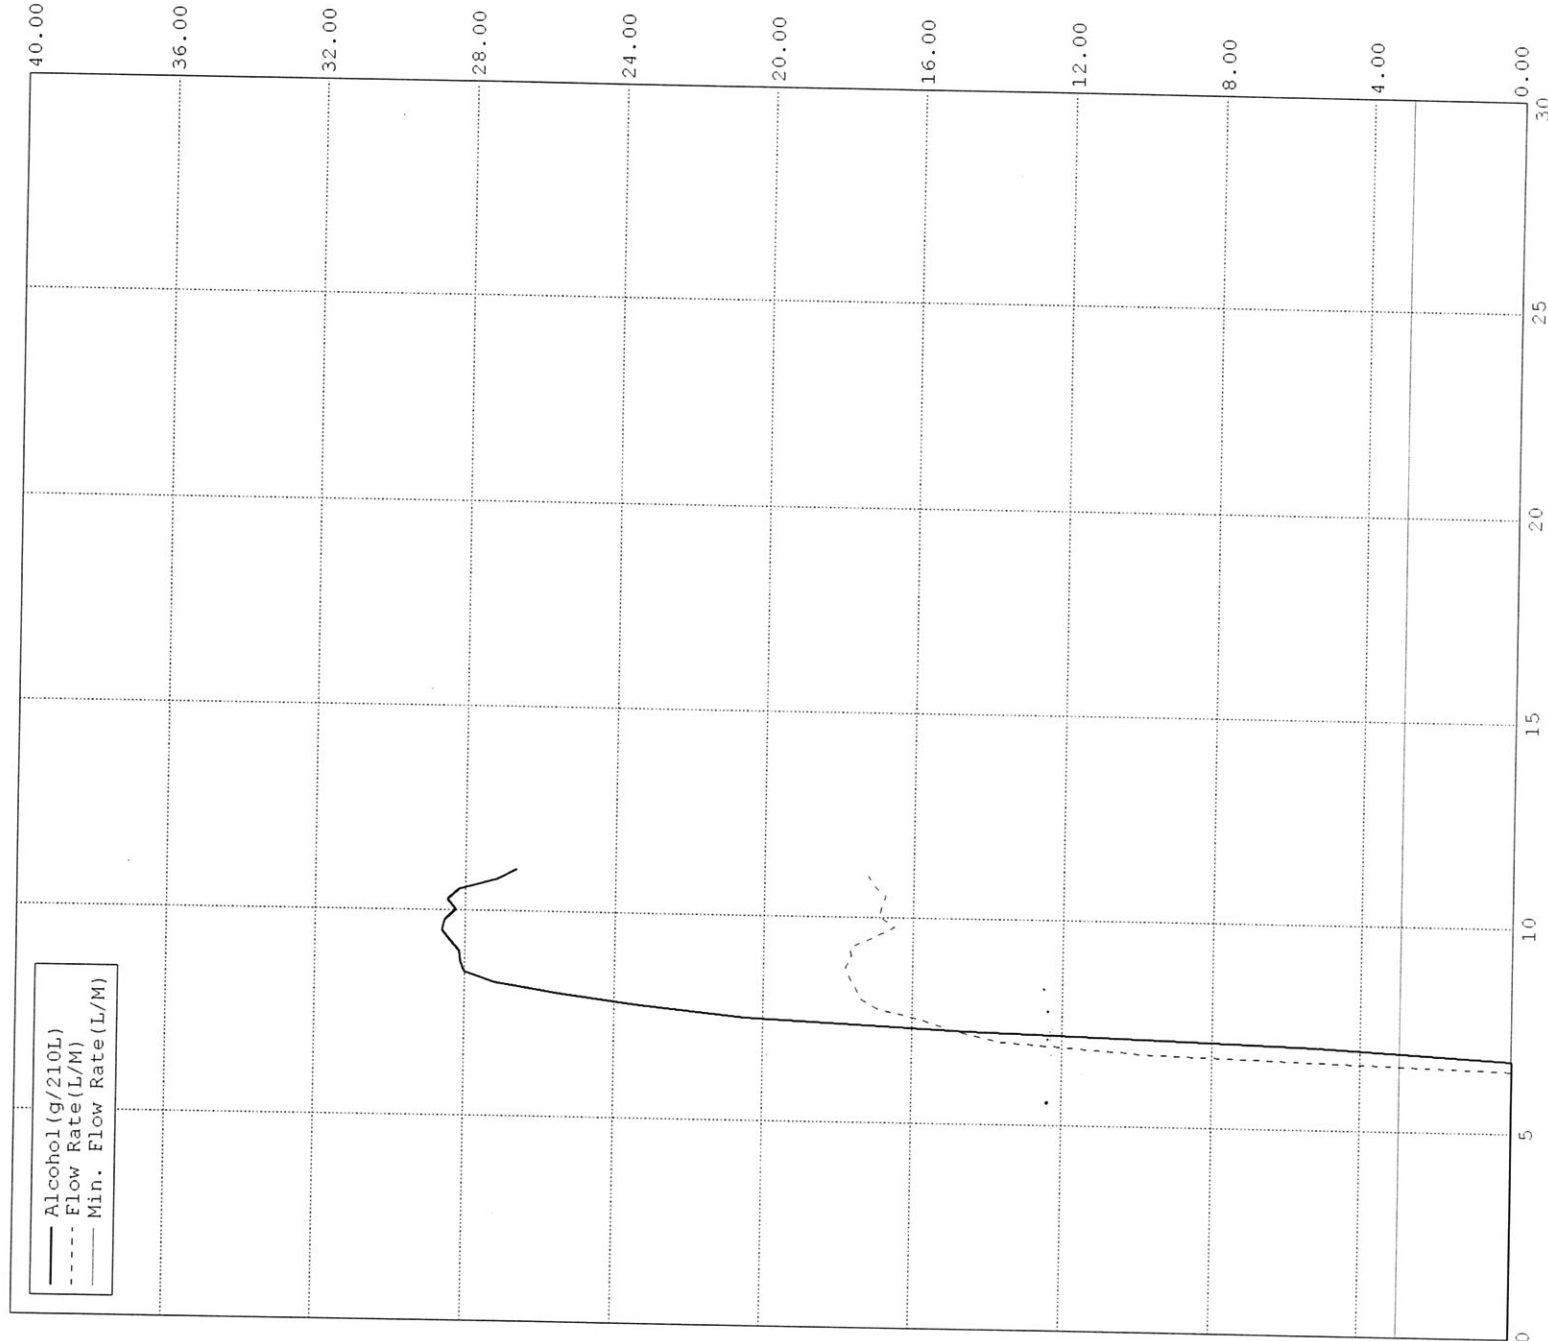

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100676

Date: 12/11/2024
Time: 11:26:00

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:

RFI
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 11:27
INTERNAL STANDARD 0.000 11:27
EXTERNAL STANDARD VERIFIED 11:27
BLANK TEST 0.079 11:27
0.000 11:28

RFI DETECTED

MNC

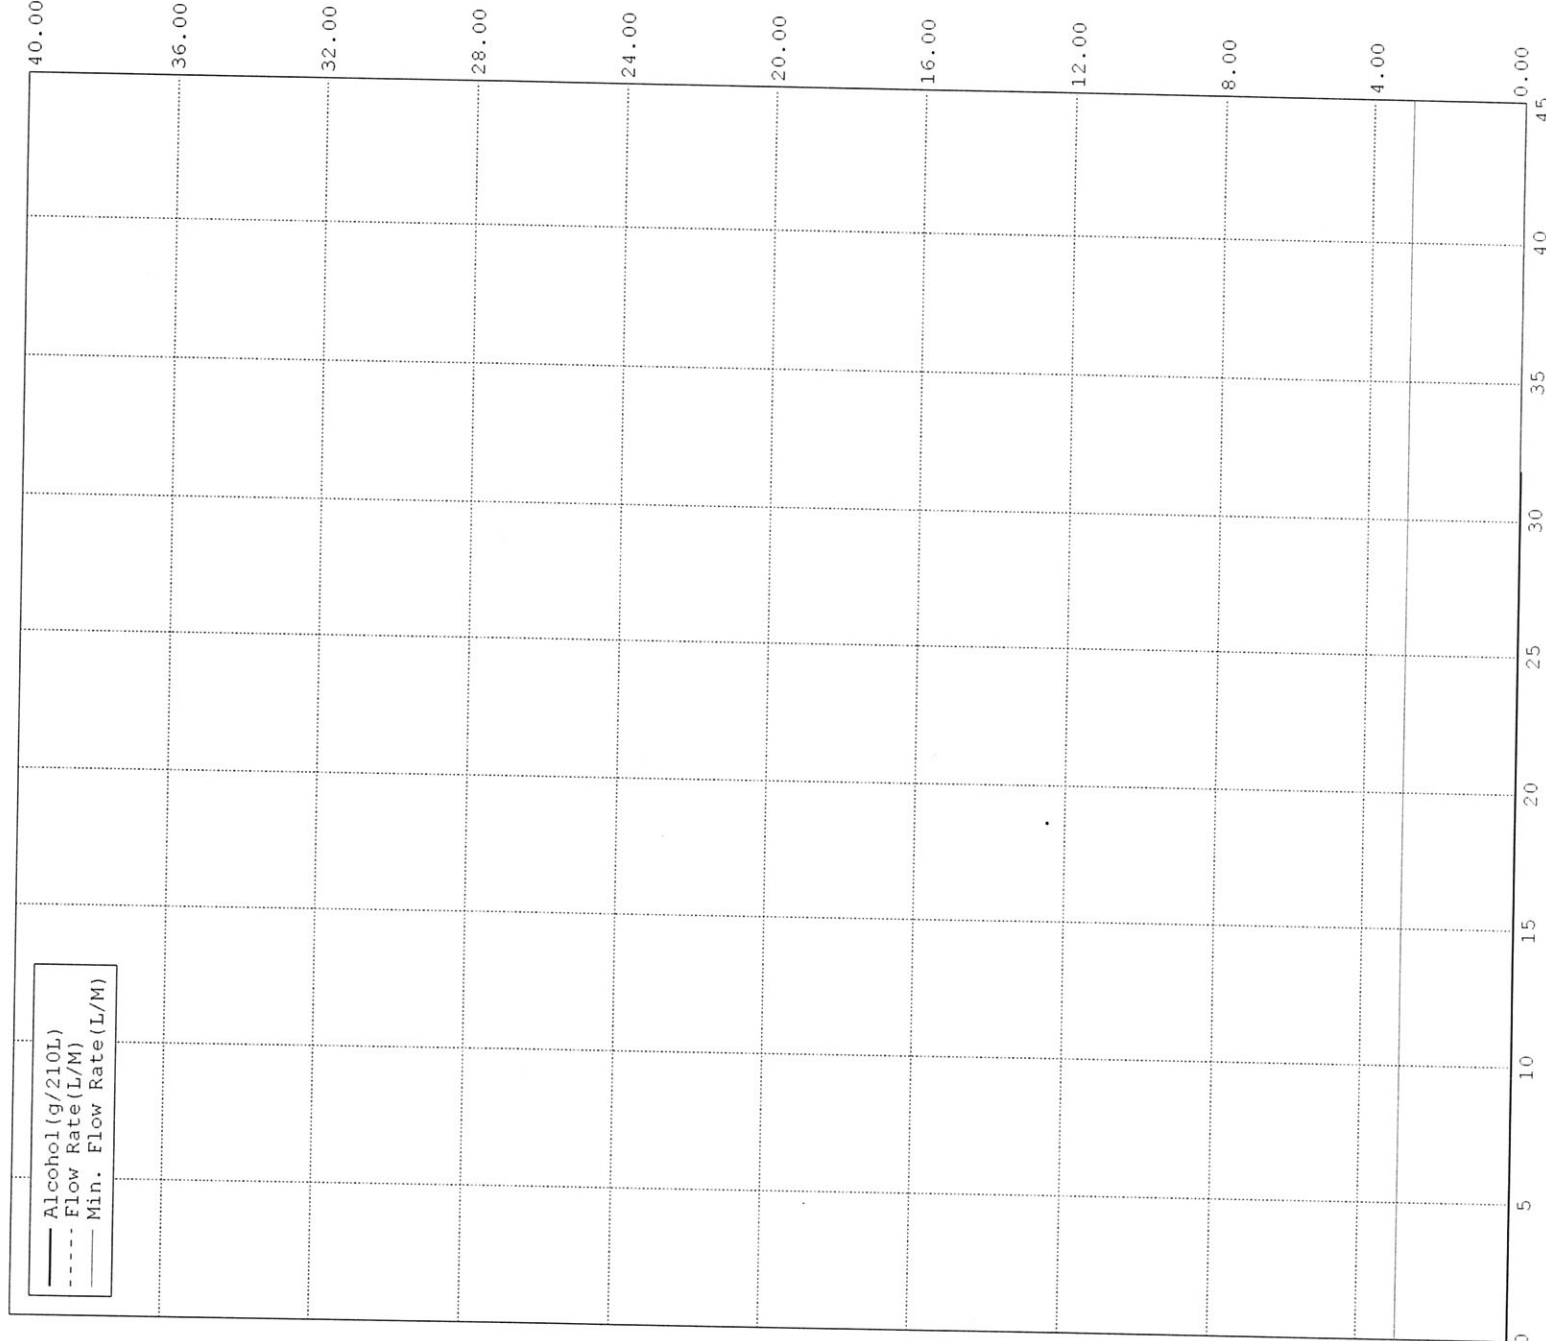

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100676

Date: 12/11/2024
 Time: 11:58:29

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:
 INTERFERENCE - ACETONE
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.09: 0.078
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025


DIAGNOSTIC CHECK	PASSED	11:59
BLANK TEST	0.000	11:59
INTERNAL STANDARD	VERIFIED	11:59
Xq = 0.091 (0.19%)		
EXTERNAL STANDARD	0.078	12:00
X[1] = 0.0785 (0.0005) (0.0028)		
BLANK TEST	0.000	12:00
SUBJECT SAMPLE	XXX	12:01
X[1] = 0.1053 (-0.0254) (0.0000)		

Interference Detected

Filter 2 Average: 0.0002

Filter 3 Average: 0.0025
 MNC 12/11/24

MNC

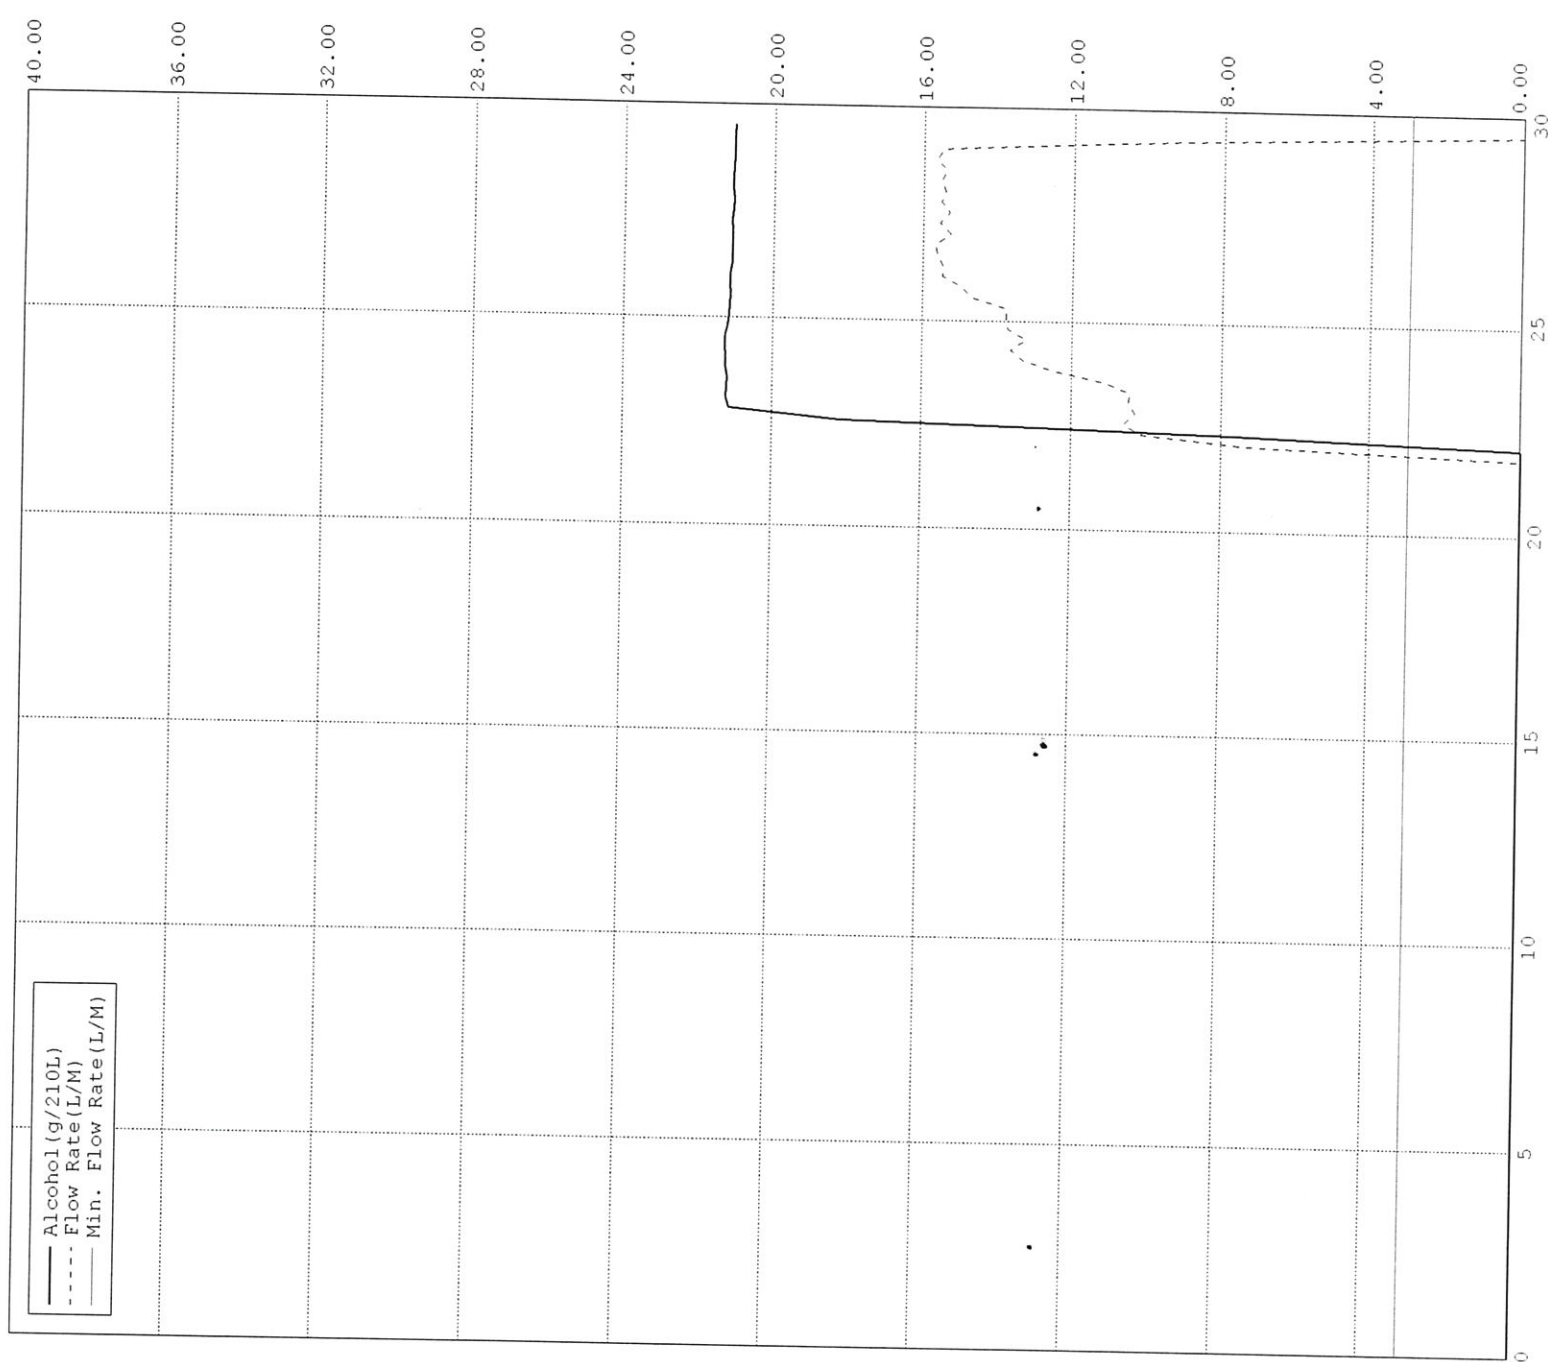

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100676

Date: 12/11/2024
Time: 11:53:08

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.09: 0.078
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	11:54
BLANK TEST	0.000	11:54
INTERNAL STANDARD	VERIFIED	11:54
$X_q = 0.091$ (0.10%)		
EXTERNAL STANDARD	0.078	11:54
$X[1] = 0.0783$ (0.0003) (0.0024)		
BLANK TEST	0.000	11:55
SUBJECT SAMPLE	XXX	11:55
$X[1] = 0.1196$ (-0.0294) (0.0013)		

Interference Detected

MNC

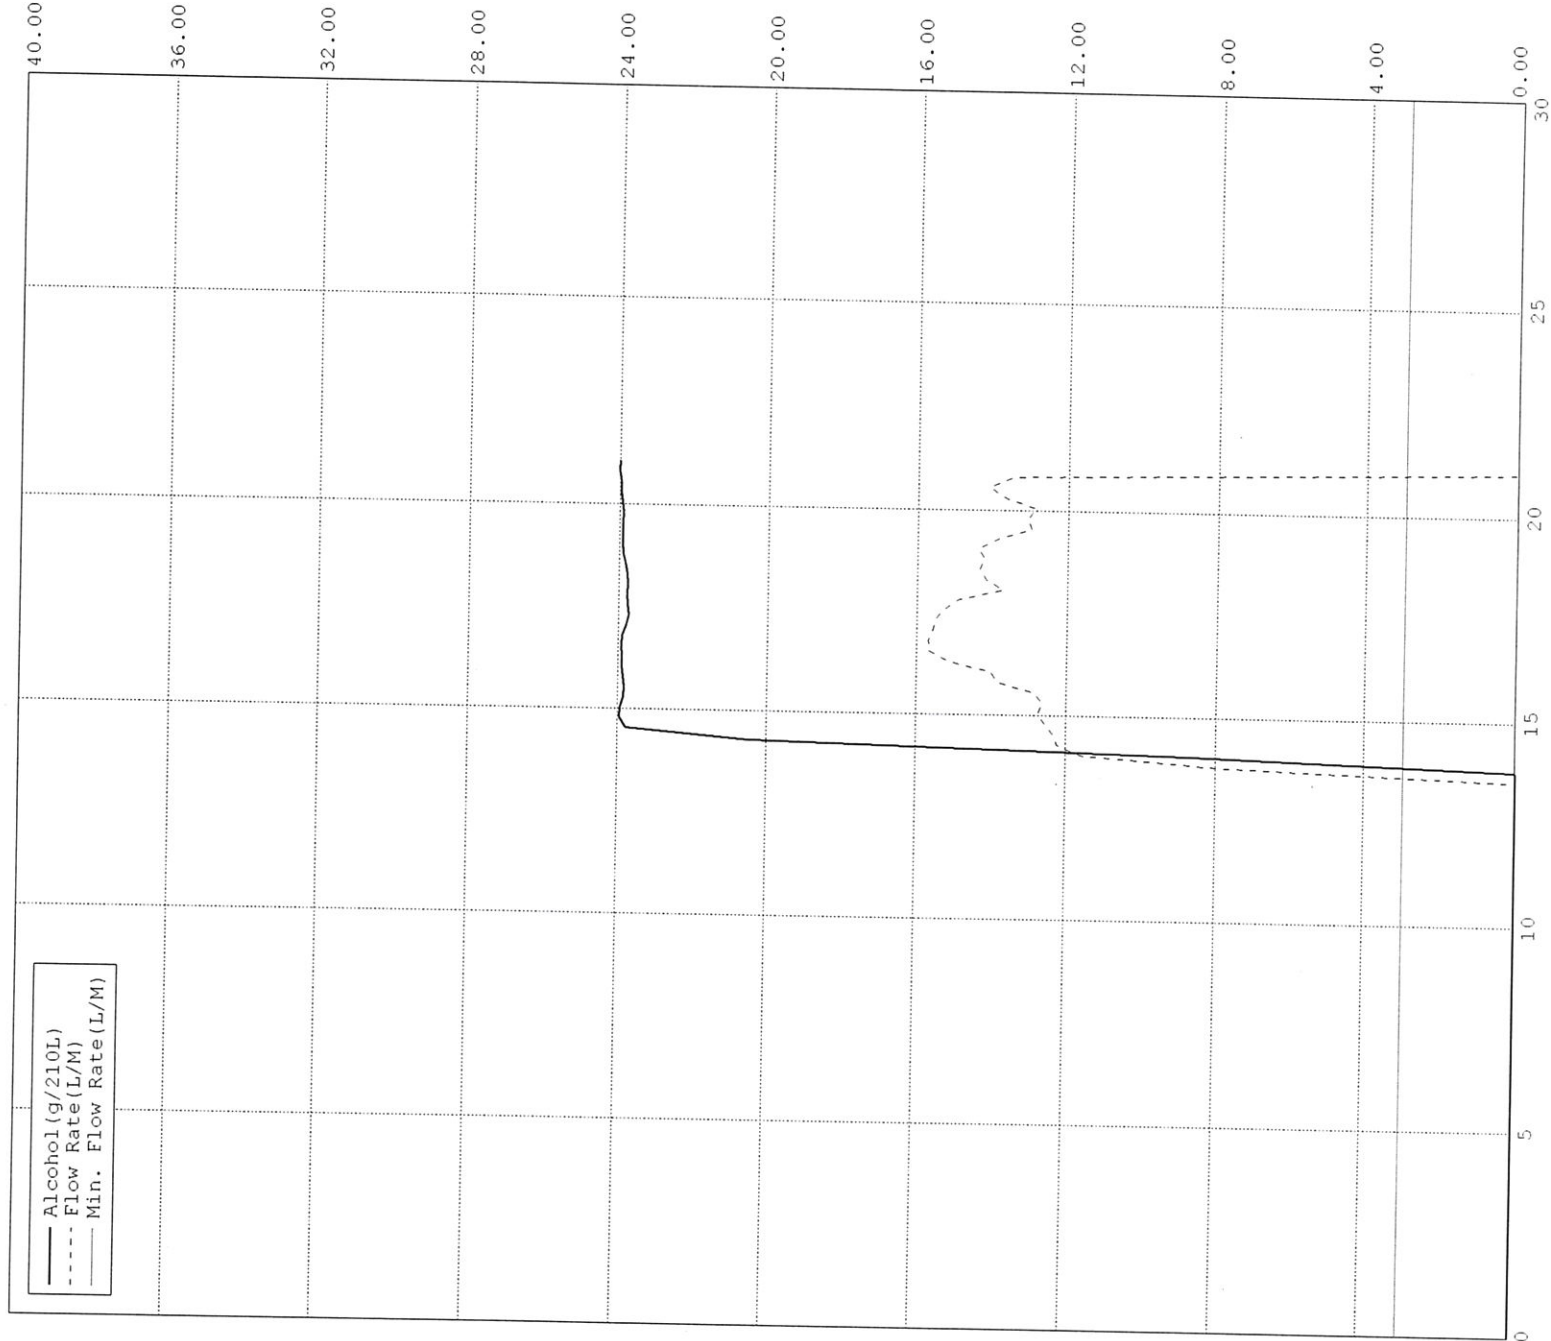

SUBJECT TEST

 Alaska Department of Public Safety
 DATAMASTER dmt: 100676

Date: 12/11/2024
 Time: 11:46:50

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX


OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

DEPT/AGENCY:
 INTERFERENCE - NEGATIVE
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.08: 0.078
 LOT #: 09523080A1
 EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	11:47
BLANK TEST	0.000	11:47
INTERNAL STANDARD	VERIFIED	11:48
Xq = 0.091 (0.29%)		
EXTERNAL STANDARD	0.078	11:48
X[1] = 0.0784 (0.0004) (0.0030)		
BLANK TEST	0.000	11:49
SUBJECT SAMPLE (Vol=1.57L)	0.095	11:49
X[1] = 0.0955 (-0.0018) (0.0004)		
BLANK TEST	0.000	11:50
EXTERNAL STANDARD	0.078	11:50
X[1] = 0.0776 (-0.0004) (0.0019)		
BLANK TEST	0.000	11:51

MNC

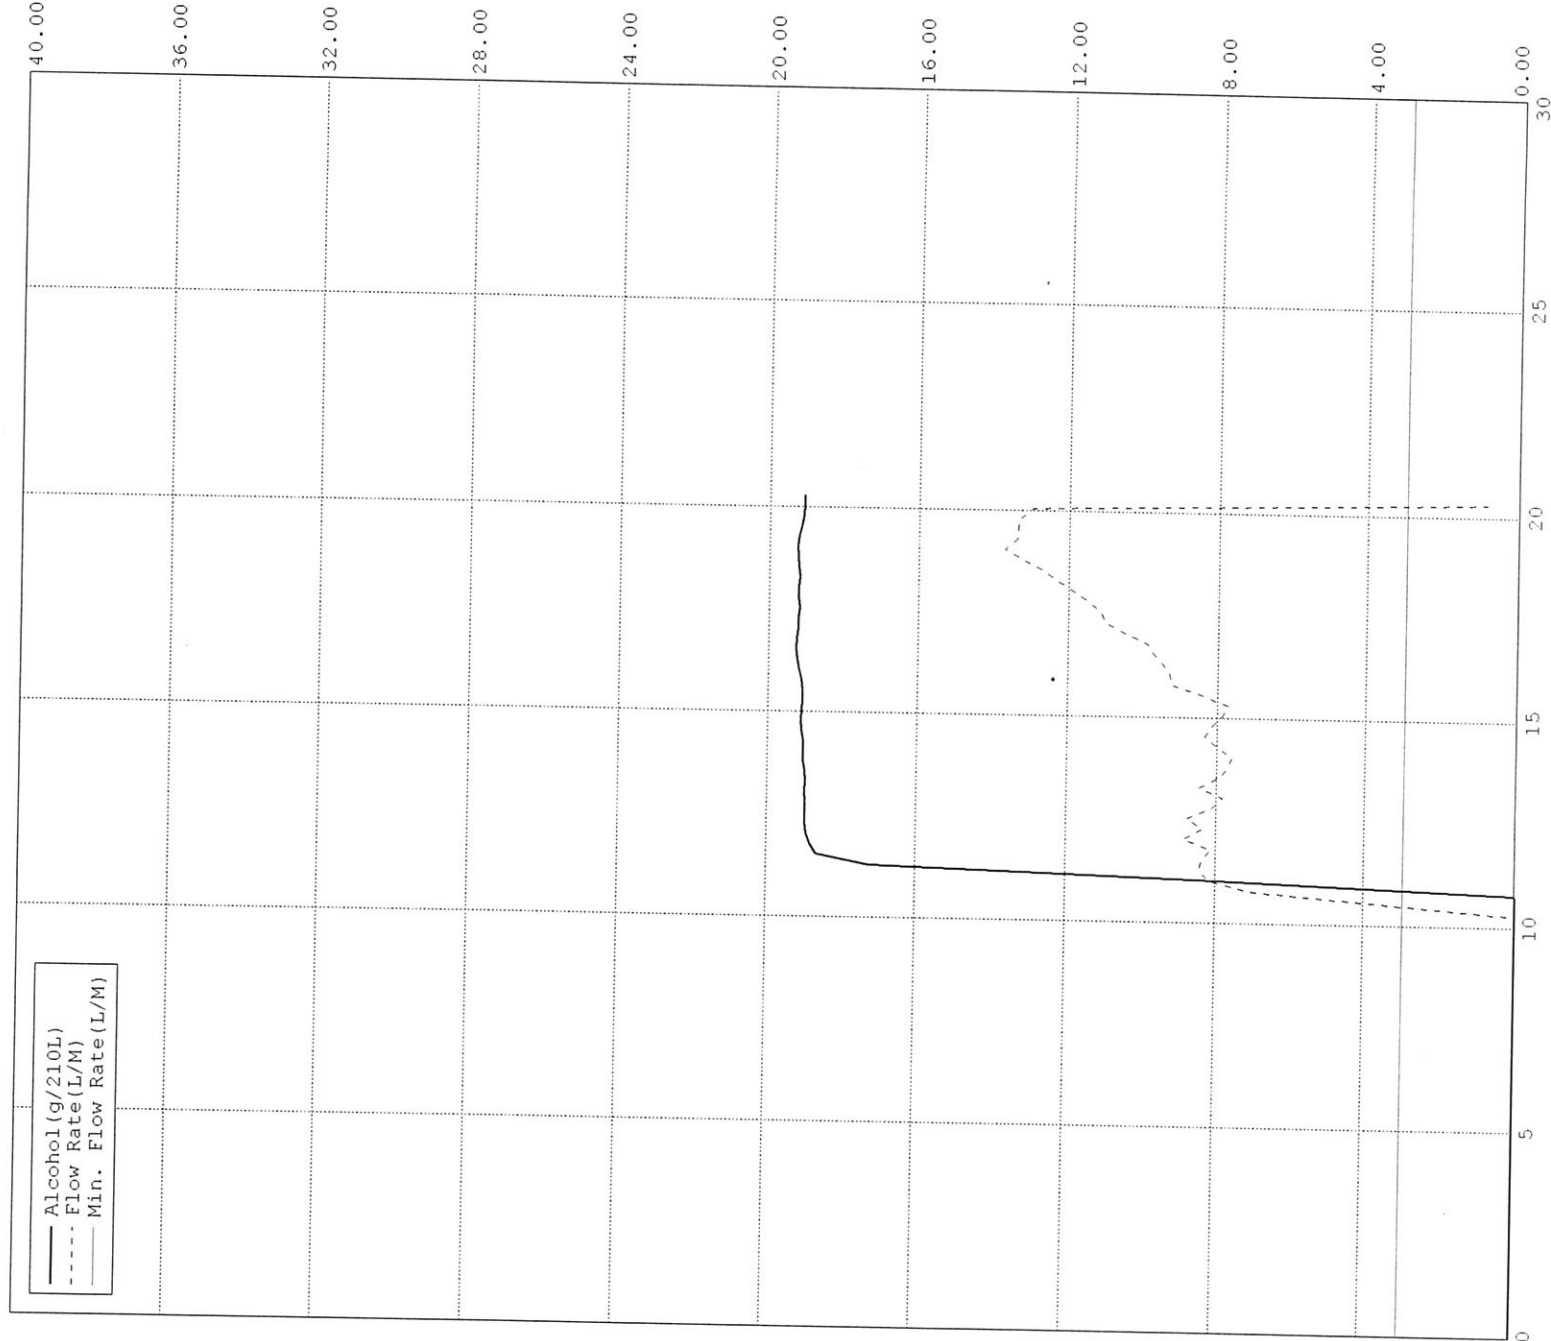

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100676

Date: 12/11/2024
Time: 12:24:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.07: 0.078
LOT #: 09523080A1
EXPIRATION: 05/05/2025

DIAGNOSTIC CHECK	PASSED	12:25
BLANK TEST	0.000	12:25
INTERNAL STANDARD	VERIFIED	12:26
EXTERNAL STANDARD	0.079	12:26
BLANK TEST	0.000	12:27
SUBJECT SAMPLE (Vol=2.00L)	0.000	12:27
BLANK TEST	0.000	12:28
EXTERNAL STANDARD	0.079	12:28
BLANK TEST	0.000	12:29

MNC

