




State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100670

Report Issue Date: 01/10/2025
Date Received: 2024-08-06
Condition of Item: No apparent damage

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.021	0.021	0.020	0.020	0.020
0.080	0.080	AG335202	0.080	0.080	0.080	0.080	0.081	0.080
0.300	0.298	AG327804	0.302	0.302	0.302	0.302	0.302	0.302

As Found - Evaluation Analyst: Colleen O'Bryant

As Found Conditions - Barometric Pressure (inHg): 29.76 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.4 Relative Humidity (%): 59

As-Found Lab Activity Date Range: 08/06/2024 - 08/07/2024

Modem still isn't functional, will need to be repaired.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.020	0.019	0.020	0.020	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.039	0.040	0.039	0.039	+/- 0.003
0.080	0.078	AG335202	0.078	0.078	0.078	0.078	0.079	0.078	+/- 0.004
0.100	0.097	AG333401	0.099	0.099	0.099	0.098	0.099	0.099	+/- 0.004
0.150	0.146	AG332004	0.146	0.146	0.146	0.146	0.146	0.146	+/- 0.006
0.300	0.292	AG427706	0.293	0.293	0.293	0.294	0.294	0.293	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.11 Barometer Used: Fisher S/N 230307229 Temperature (C): 22.3 Relative Humidity (%): 20

As-Left Lab Activity Date Range: 12/11/2024 - 12/11/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock

Results authorized by Megan Carlock on 01/10/2025

megan.crouse@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 01/10/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100670 Analyst or Technician Name: Megan Carlock

DataMaster DMT Calibration Start Date: 12/10/24 12/11/24

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

MNC
1/10/25

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
Calibration Due Date: 5/2/2025
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.6 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.11 Temperature(C) 22.3 Relative Humidity(%) 20
Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Interference (Volatiles) – Print with View Details
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR4161 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR5298 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 23TP41233 Expiration Date: 9/20/25
Simulator S/N: DR4163 Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 230631106
Calibration Due Date: 9/19/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 12/11/24
Data Interpretation Date (Technician): N/A (if applicable)
Data Interpretation Date (Analyst): 12/11/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 08:35:45

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C	PASSED
(44.0°C - 52.0°C)	
Breath Tube = 47.7°C	PASSED
(38.0°C - 50.0°C)	

SETTINGS

Lamp Voltage = 1.75 V	PASSED
(1.05 V - 2.45 V)	
Cooler Voltage = 1.68 V	PASSED
(1.01 V - 2.35 V)	
Bias Voltage = 79 V	PASSED
(47 V - 111 V)	
Chopper Freq = 523 Hz	PASSED
(475 Hz - 575 Hz)	
Barometer = 29.1 in	

PUMP INFO

Flow Rate = 4.775 L/M	PASSED
(3.500 L/M - 6.500 L/M)	

DETECTOR INFO

PUMP ON	PASSED
(0.001 V <= 0.010 V)	
PUMP OFF	PASSED
(0.002 V <= 0.010 V)	

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD	PASSED
Xq = 0.088 0.79% (0.00% - 4.00%)	

Technician Screen

DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 8:42 AM

Temperatures (°C)
Sample Cell: 49.5°C
Breath Tube: 46.8°C

Current Barometer 29.1 in
Volume (Ltr) 1.50

Settings
Lamp: 1.83 V
Bias: 79 V
Cooler: 1.61 V
Chopper: 522 Hz


Voltages (V)
Flow: 1.04 V
Detector: 0.010 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 09/21/2011
Time: 14:17:27

Ca	=	0.1500		
CAL	=	0.983698	0.800	<= CAL < 1.200
b1	=	0.0002	0.0000	<= b1 < 0.0040
b2	=	0.0023	0.0010	<= b2 < 0.0100
b3	=	0.0000	0.0000	<= b3 < 0.0040
Xq	=	0.0886	0.0500	<= Xq < 0.2000
a21	=	1.179698	1.050	<= a21 < 1.300
a31	=	0.439665	0.300	<= a31 < 0.800

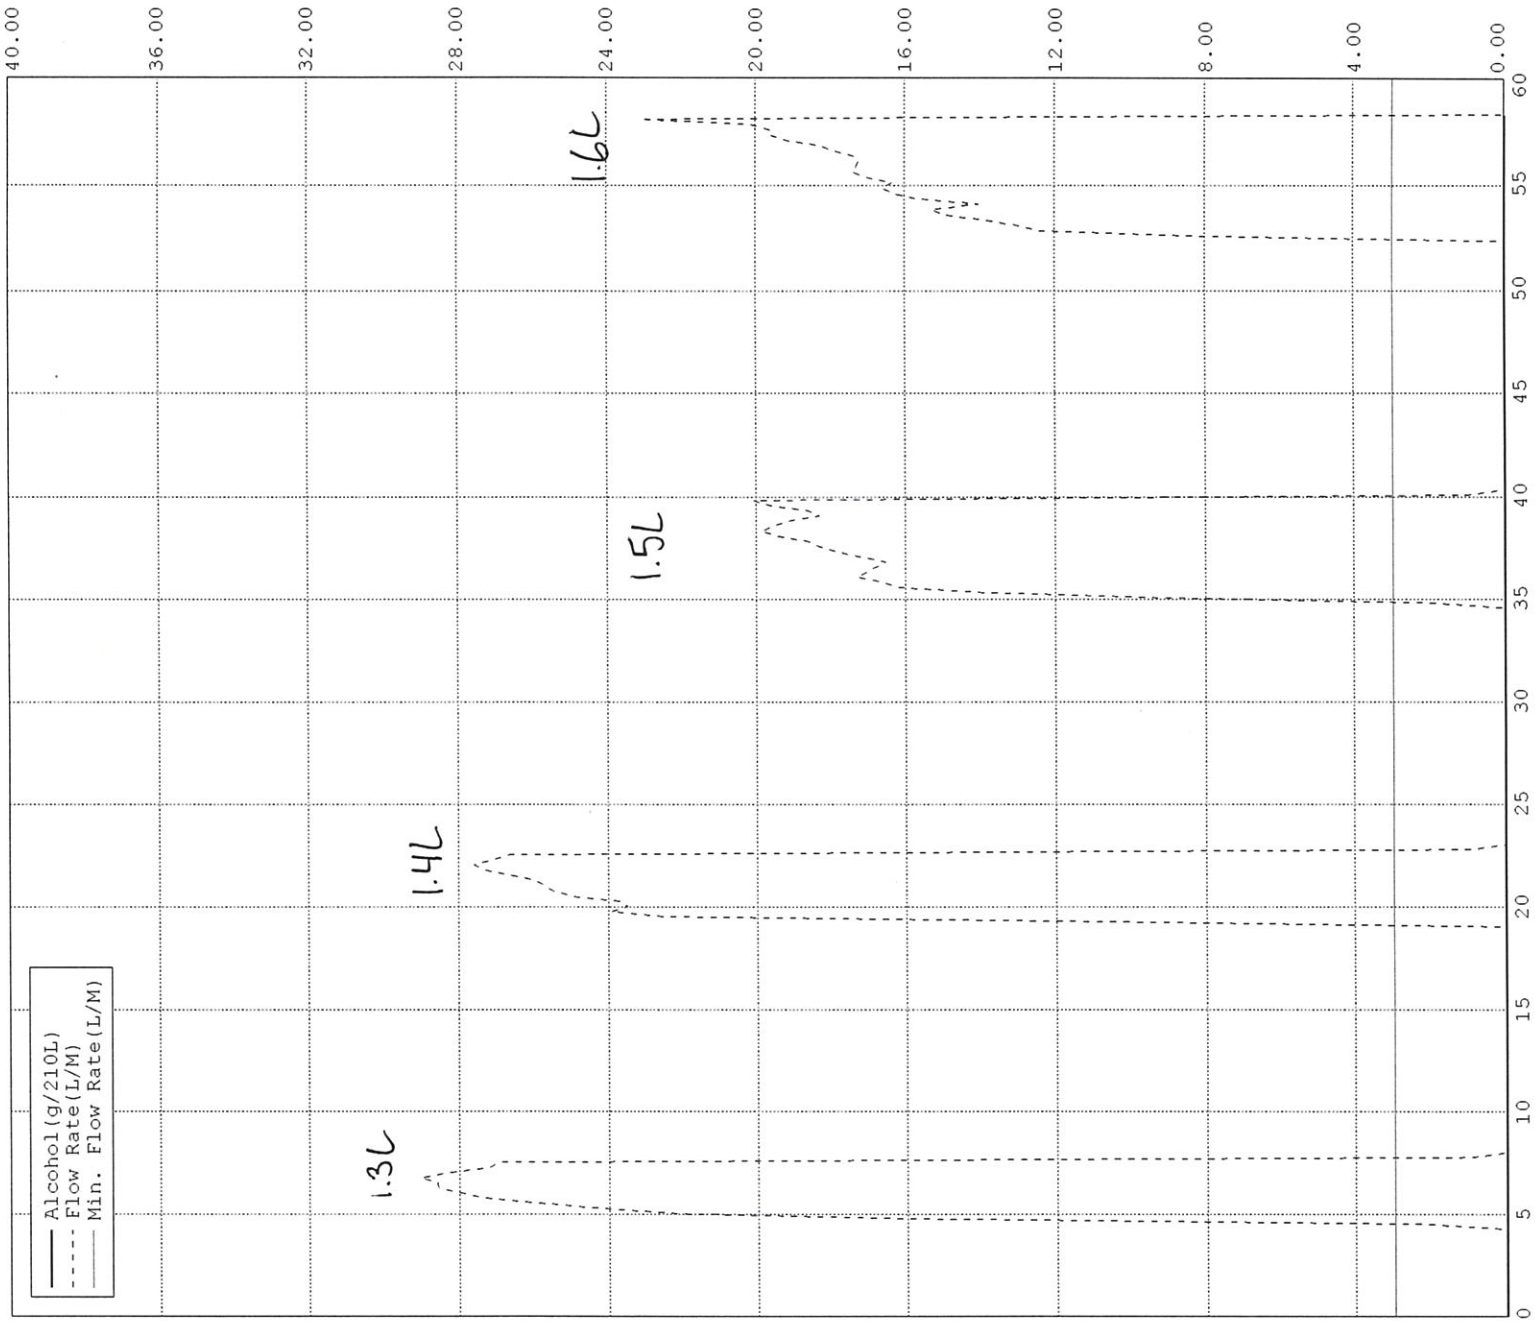

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 08:52:15

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.12: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:53
BLANK TEST	0.000	08:53
INTERNAL STANDARD	VERIFIED	08:53
EXTERNAL STANDARD	0.078	08:53
BLANK TEST	0.000	08:54
SUBJECT SAMPLE (Vol=1.59L)	0.000	08:55
BLANK TEST	0.000	08:56
EXTERNAL STANDARD	0.078	08:56
BLANK TEST	0.000	08:57

MNC

LINEARITY CHECK


 Alaska Department of Public Safety
 DATAMASTER dmt: 100670

Date: 12/11/2024
 Time: 10:19:28

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.019	0.0198	0.0004
0.039	0.0392	0.0004
0.078	0.0782	0.0004
0.097	0.0988	0.0004
0.146	0.1460	0.0000
0.292	0.2934	0.0005

SLOPE = 1.002656
 R² = 0.999952

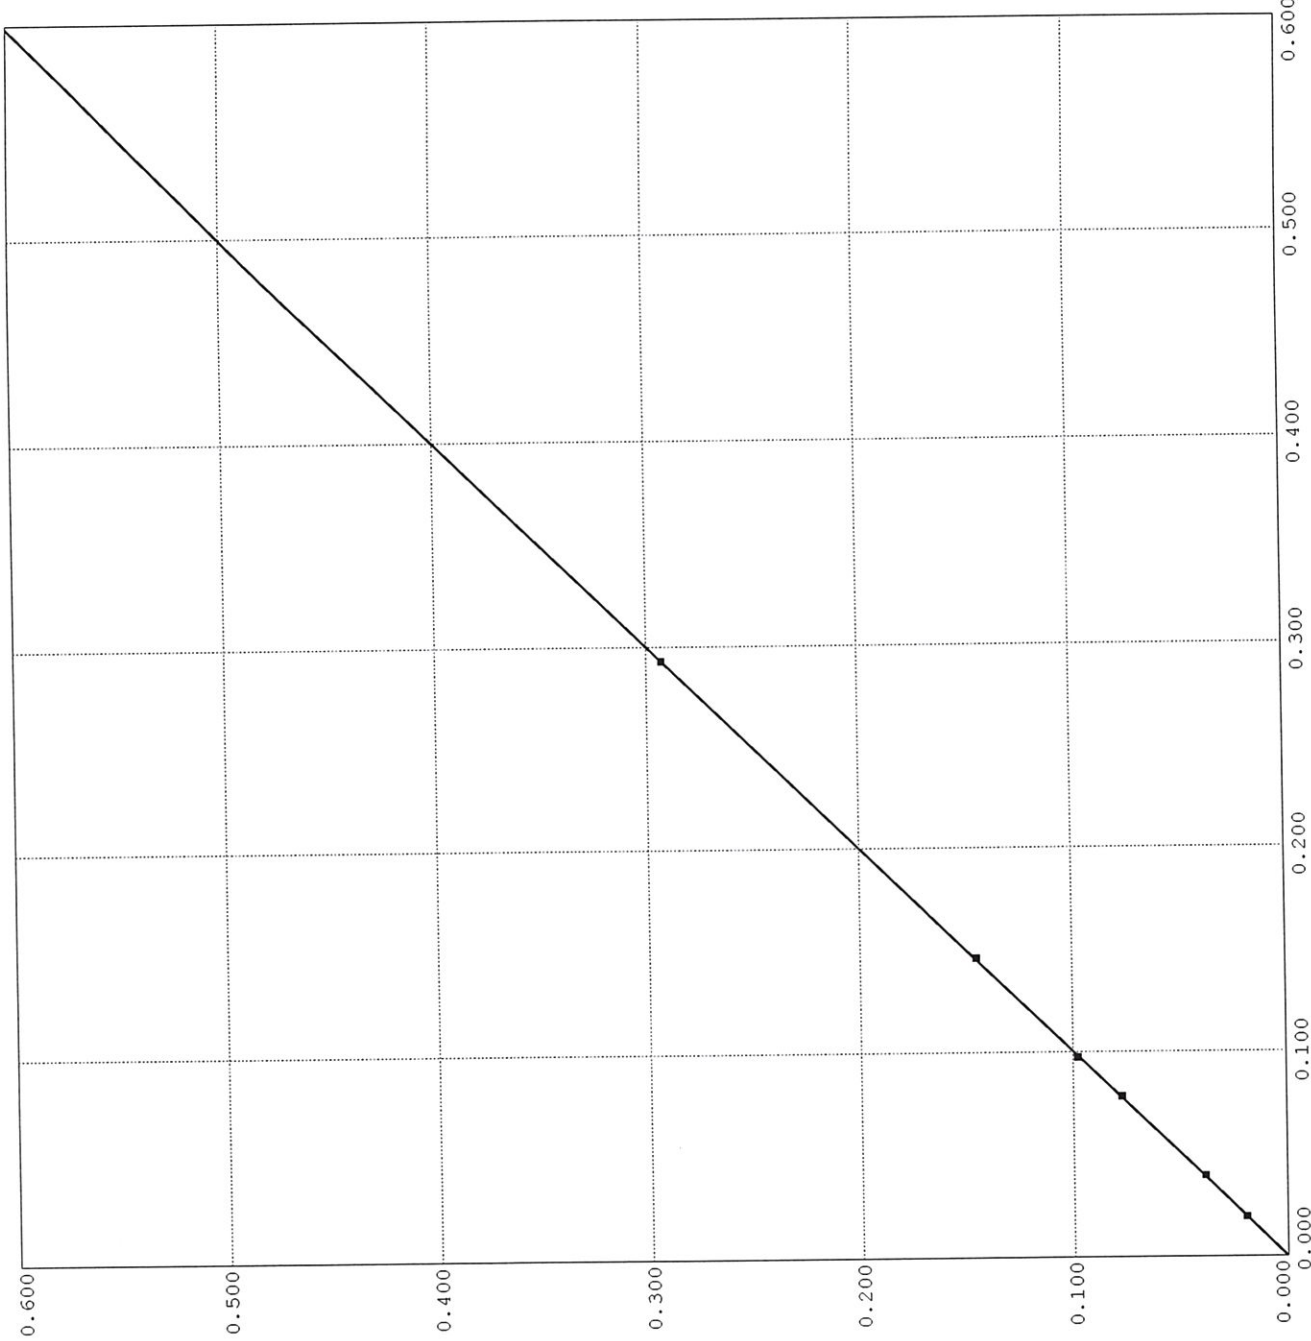

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100670






Date: 12/11/2024
Time: 10:19:29

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 29.10: 0.019
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 681 psi

BLANK TEST	0.000	10:20
INTERNAL STANDARD	VERIFIED	10:20
EXTERNAL STANDARD	0.020	10:21
BLANK TEST	0.000	10:22
EXTERNAL STANDARD	0.019	10:22
BLANK TEST	0.000	10:23
EXTERNAL STANDARD	0.020	10:23
BLANK TEST	0.000	10:24
EXTERNAL STANDARD	0.020	10:24
BLANK TEST	0.000	10:25
EXTERNAL STANDARD	0.020	10:25
BLANK TEST	0.000	10:26

Average = 0.0198
Std Dev = 0.0004

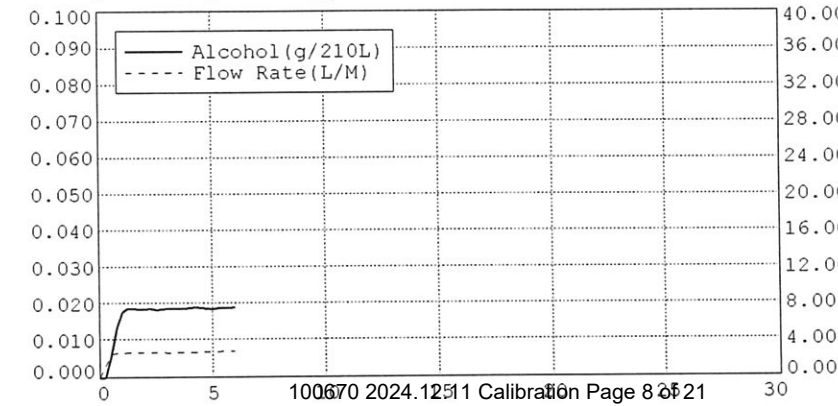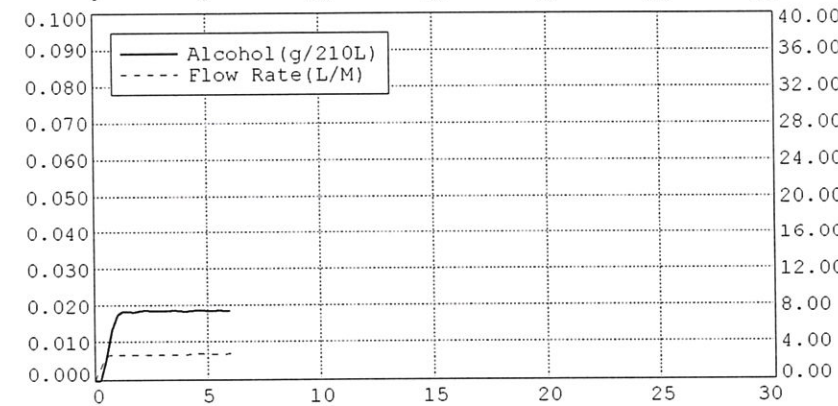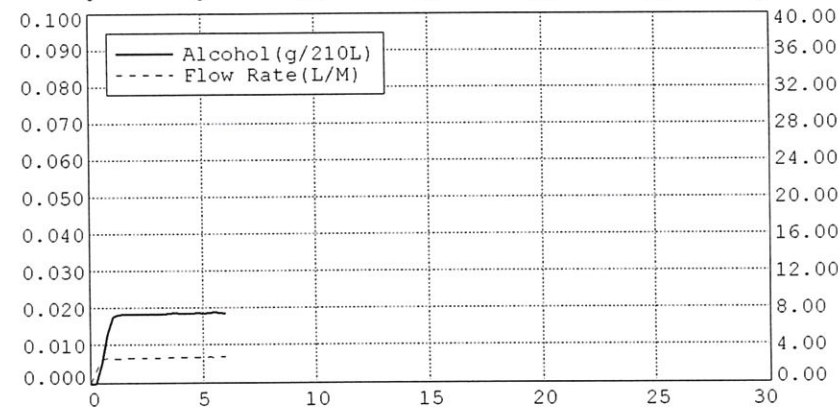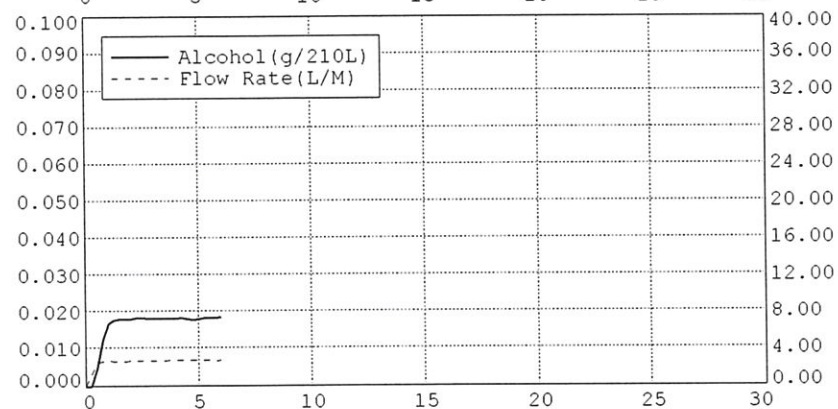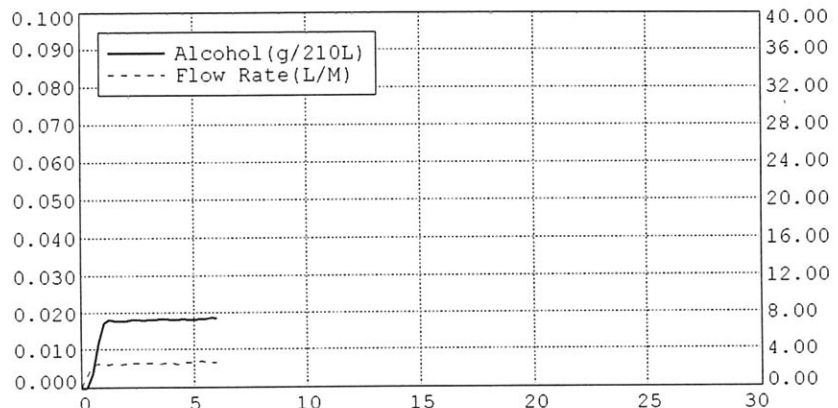

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100670






Date: 12/11/2024
Time: 10:27:13

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.10: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 1023 psi

BLANK TEST	0.000	10:28
INTERNAL STANDARD	VERIFIED	10:28
EXTERNAL STANDARD	0.039	10:28
BLANK TEST	0.000	10:29
EXTERNAL STANDARD	0.039	10:29
BLANK TEST	0.000	10:30
EXTERNAL STANDARD	0.039	10:31
BLANK TEST	0.000	10:31
EXTERNAL STANDARD	0.040	10:32
BLANK TEST	0.000	10:32
EXTERNAL STANDARD	0.039	10:33
BLANK TEST	0.000	10:34

Average = 0.0392
Std Dev = 0.0004

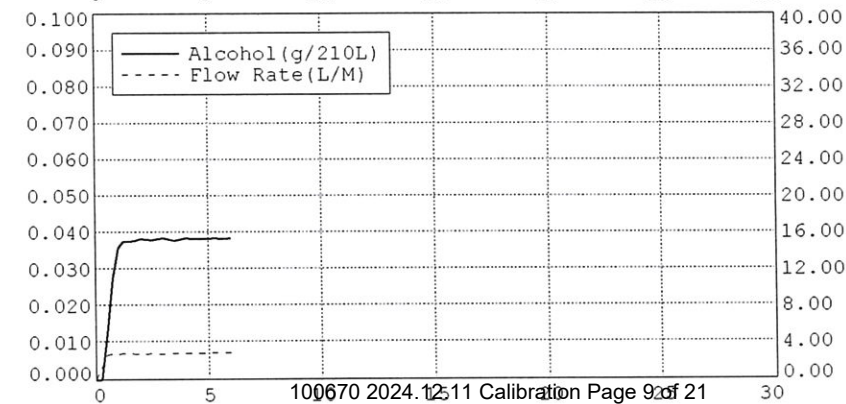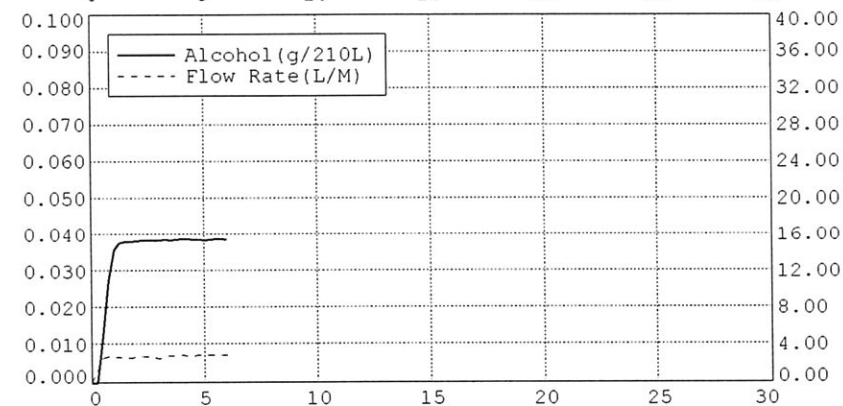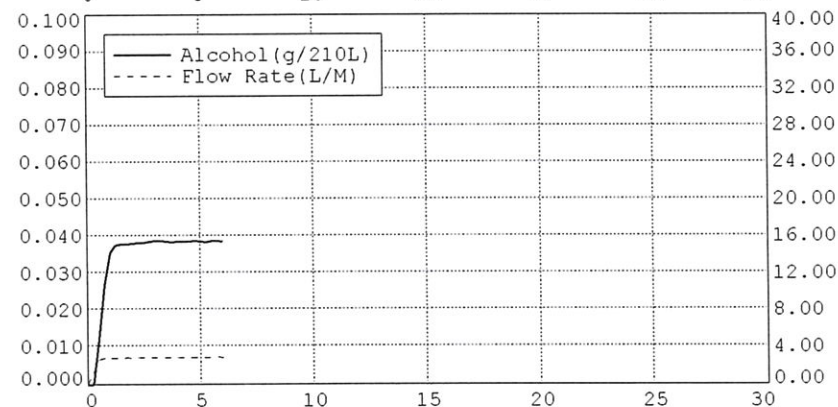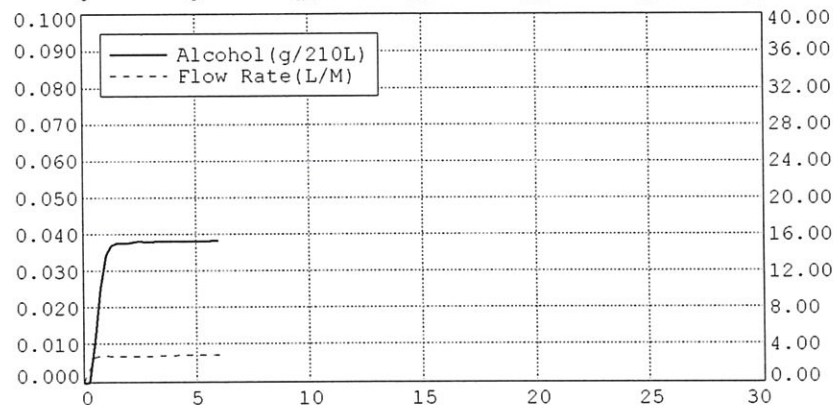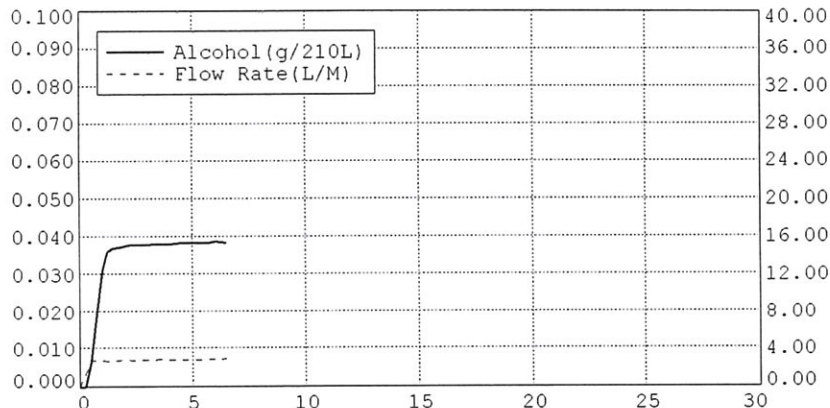

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100670






Date: 12/11/2024
Time: 10:35:21

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.11: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 607 psi

BLANK TEST	0.000	10:36
INTERNAL STANDARD	VERIFIED	10:36
EXTERNAL STANDARD	0.078	10:36
BLANK TEST	0.000	10:37
EXTERNAL STANDARD	0.078	10:38
BLANK TEST	0.000	10:38
EXTERNAL STANDARD	0.078	10:39
BLANK TEST	0.000	10:40
EXTERNAL STANDARD	0.078	10:40
BLANK TEST	0.000	10:41
EXTERNAL STANDARD	0.079	10:41
BLANK TEST	0.000	10:42

Average = 0.0782
Std Dev = 0.0004

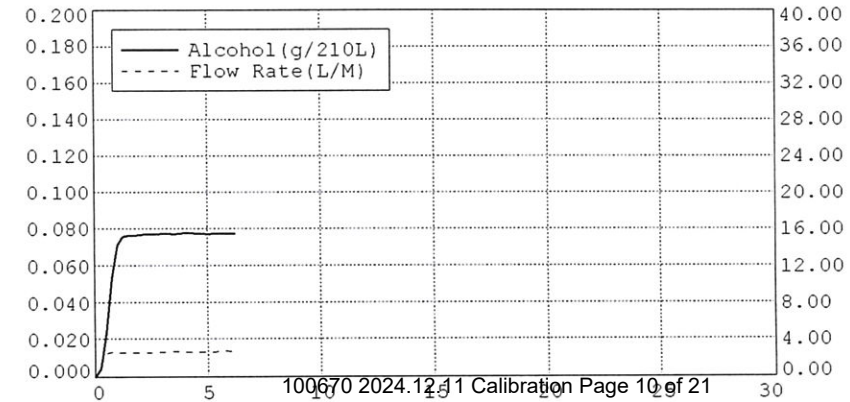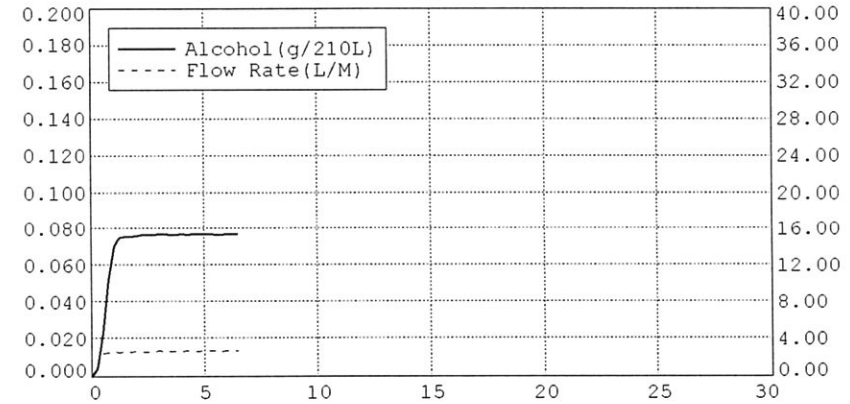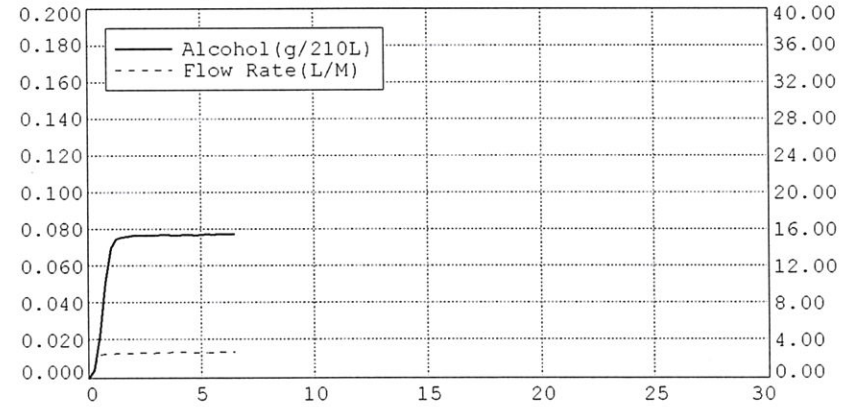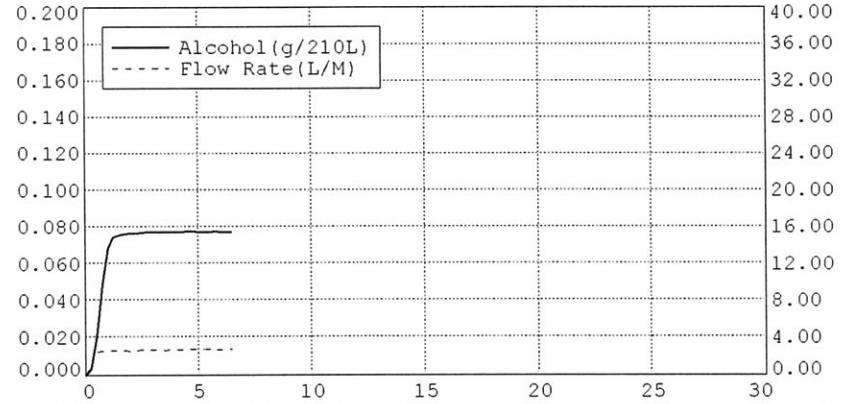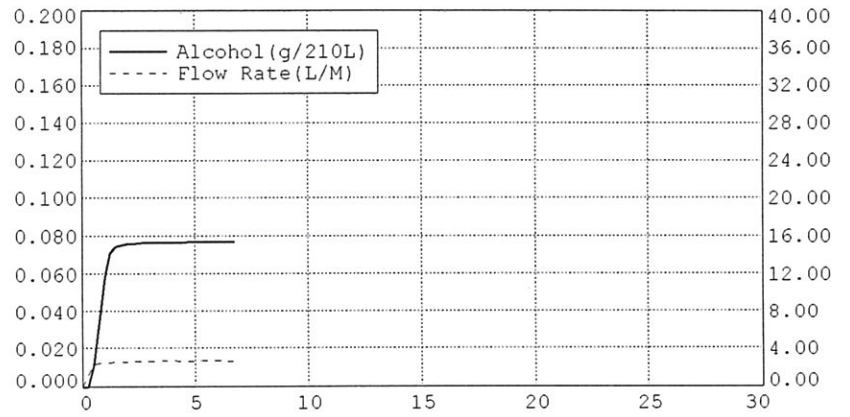

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100670






Date: 12/11/2024
Time: 10:44:01

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 29.10: 0.097
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 666 psi

BLANK TEST	0.000	10:45
INTERNAL STANDARD	VERIFIED	10:45
EXTERNAL STANDARD	0.099	10:45
BLANK TEST	0.000	10:46
EXTERNAL STANDARD	0.099	10:46
BLANK TEST	0.000	10:47
EXTERNAL STANDARD	0.099	10:47
BLANK TEST	0.000	10:48
EXTERNAL STANDARD	0.098	10:49
BLANK TEST	0.000	10:49
EXTERNAL STANDARD	0.099	10:50
BLANK TEST	0.000	10:51

Average = 0.0988
Std Dev = 0.0004

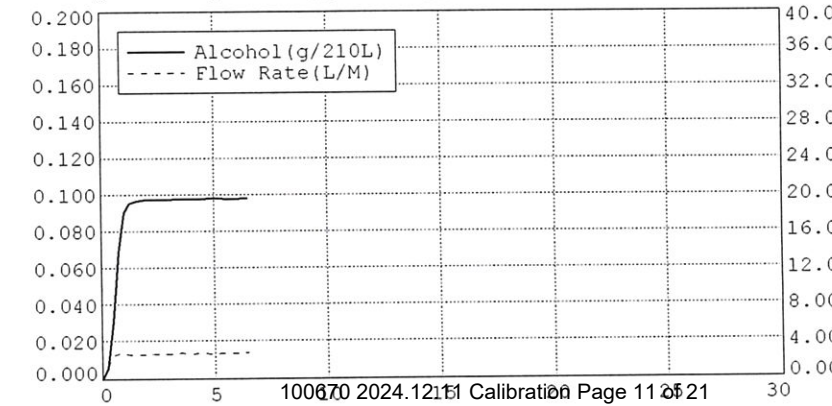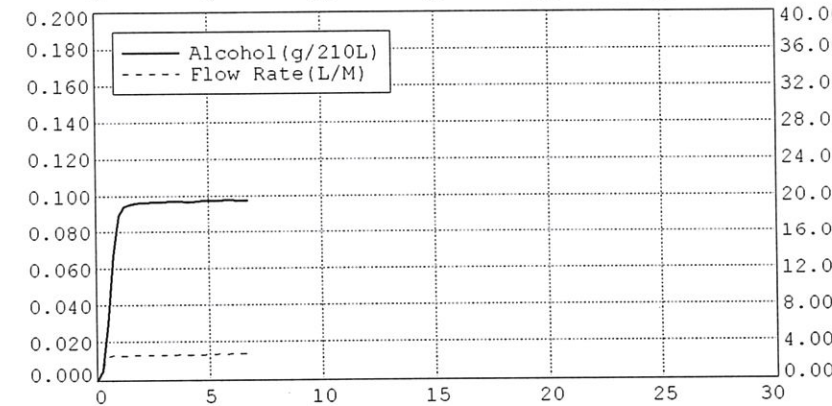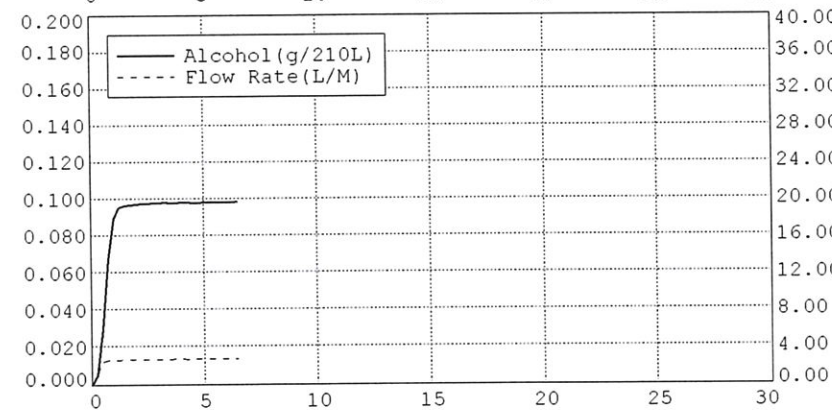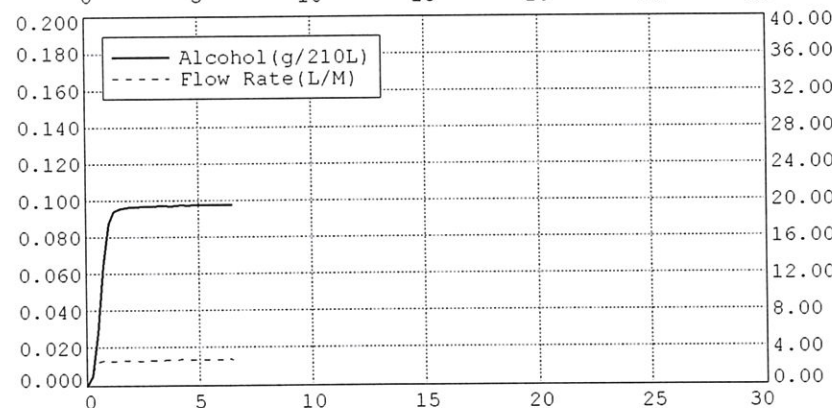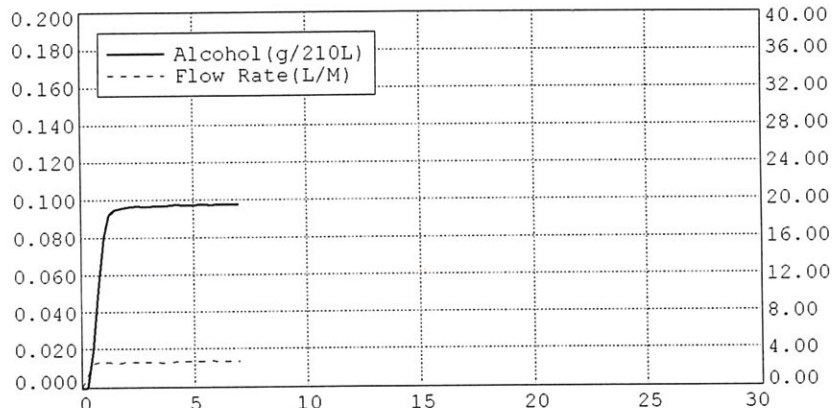

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100670


Date: 12/11/2024
Time: 10:53:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 29.11: 0.146
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 269 psi

BLANK TEST	0.000	10:54
INTERNAL STANDARD	VERIFIED	10:54
EXTERNAL STANDARD	0.146	10:54
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.146	10:55
BLANK TEST	0.000	10:56
EXTERNAL STANDARD	0.146	10:56
BLANK TEST	0.000	10:57
EXTERNAL STANDARD	0.146	10:57
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.146	10:59
BLANK TEST	0.000	10:59

Average = 0.1460
Std Dev = 0.0000

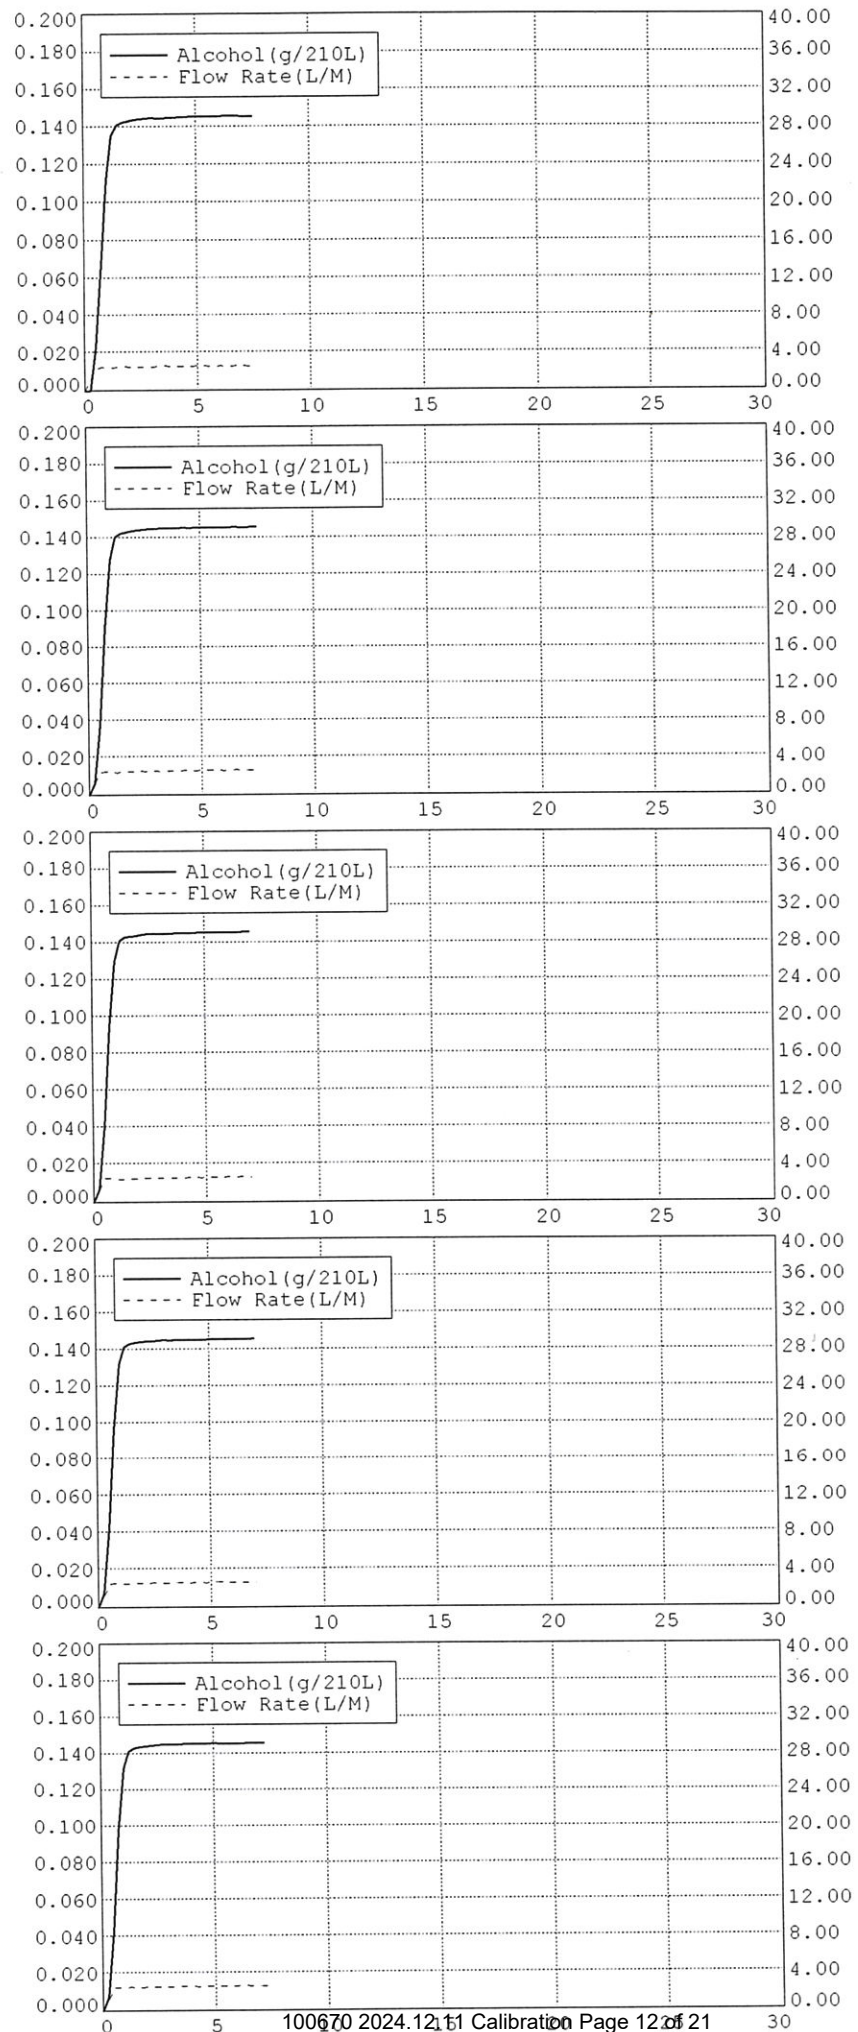

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100670






Date: 12/11/2024
Time: 11:03:51

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.10: 0.292
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 294 psi

BLANK TEST	0.000	11:04
INTERNAL STANDARD	VERIFIED	11:05
EXTERNAL STANDARD	0.293	11:05
BLANK TEST	0.000	11:06
EXTERNAL STANDARD	0.293	11:06
BLANK TEST	0.000	11:07
EXTERNAL STANDARD	0.293	11:07
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.294	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.294	11:09
BLANK TEST	0.000	11:10

Average = 0.2934
Std Dev = 0.0005

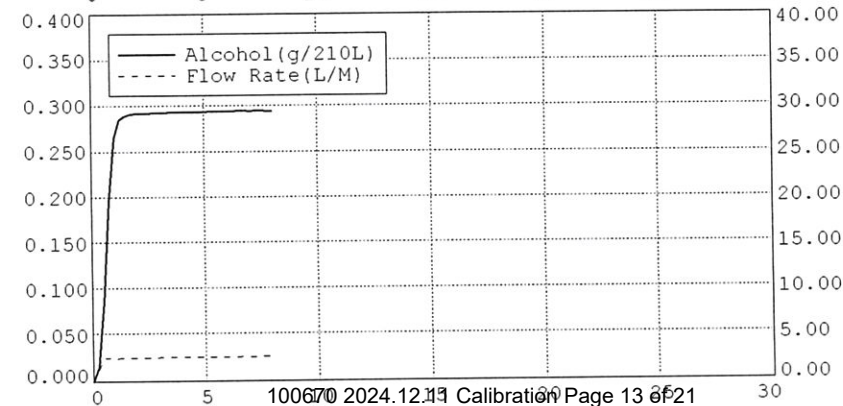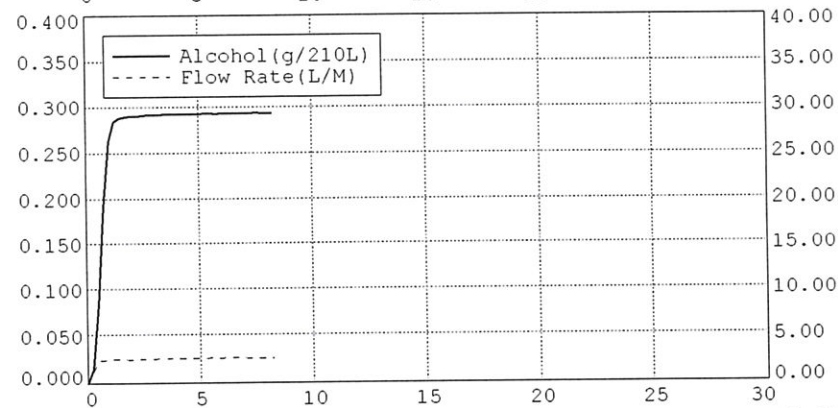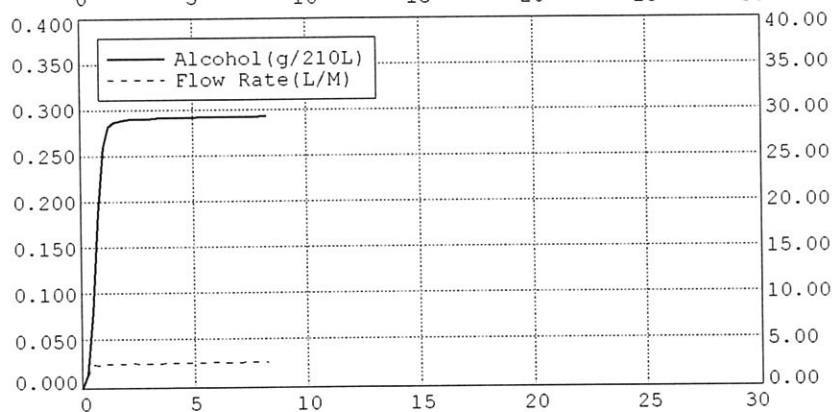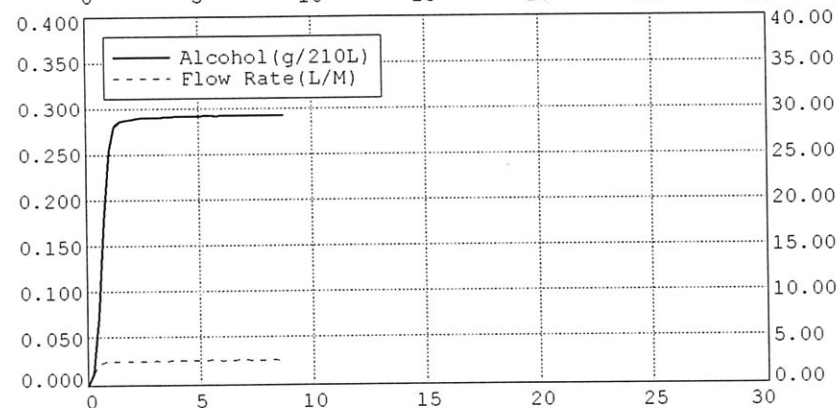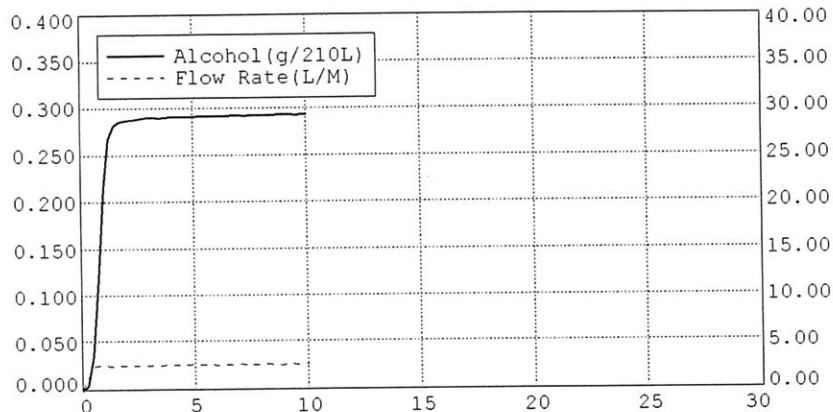

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 11:14:32

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:15
BLANK TEST	0.000	11:15
INTERNAL STANDARD	VERIFIED	11:15
EXTERNAL STANDARD	0.079	11:15
BLANK TEST	0.000	11:16
SUBJECT SAMPLE	INCOMPLETE	11:18

MNC

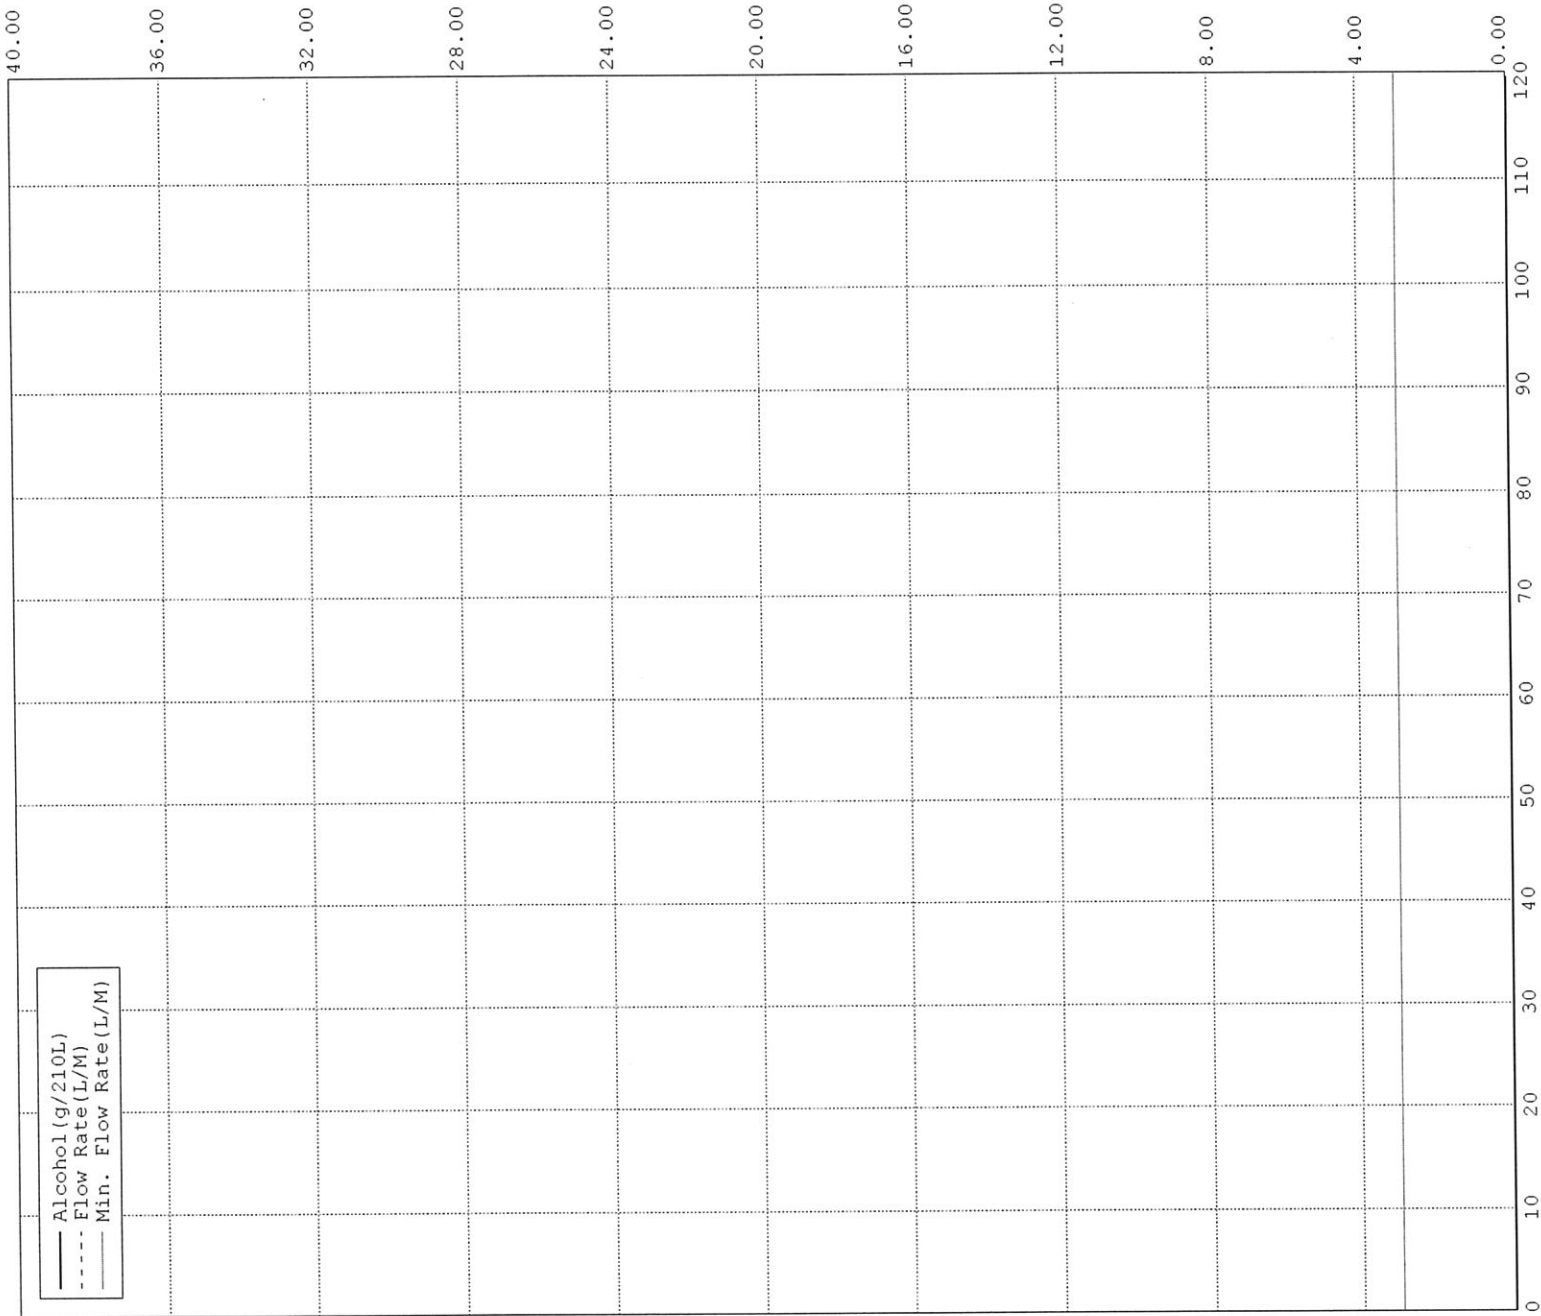

SUBJECT TEST

Alaska Department of Public Safety
 DATAMASTER dmt: 100670

Date: 12/11/2024
 Time: 11:20:29

SUBJECT NAME:
 TEST TEST
 LICENSE #: XXX

OPERATOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747


DEPT/AGENCY:
 MAXIMUM ATTEMPTS EXCEEDED
 CASE/REPORT: XXX
 TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
 NOMINAL: 0.080
 TARGET AT 29.10: 0.078
 LOT #: AG335202
 EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:21
BLANK TEST	0.000	11:21
INTERNAL STANDARD	VERIFIED	11:21
EXTERNAL STANDARD	0.079	11:21
BLANK TEST	0.000	11:22
SUBJECT SAMPLE	XXX	11:23

Maximum Attempts Exceeded

MNC

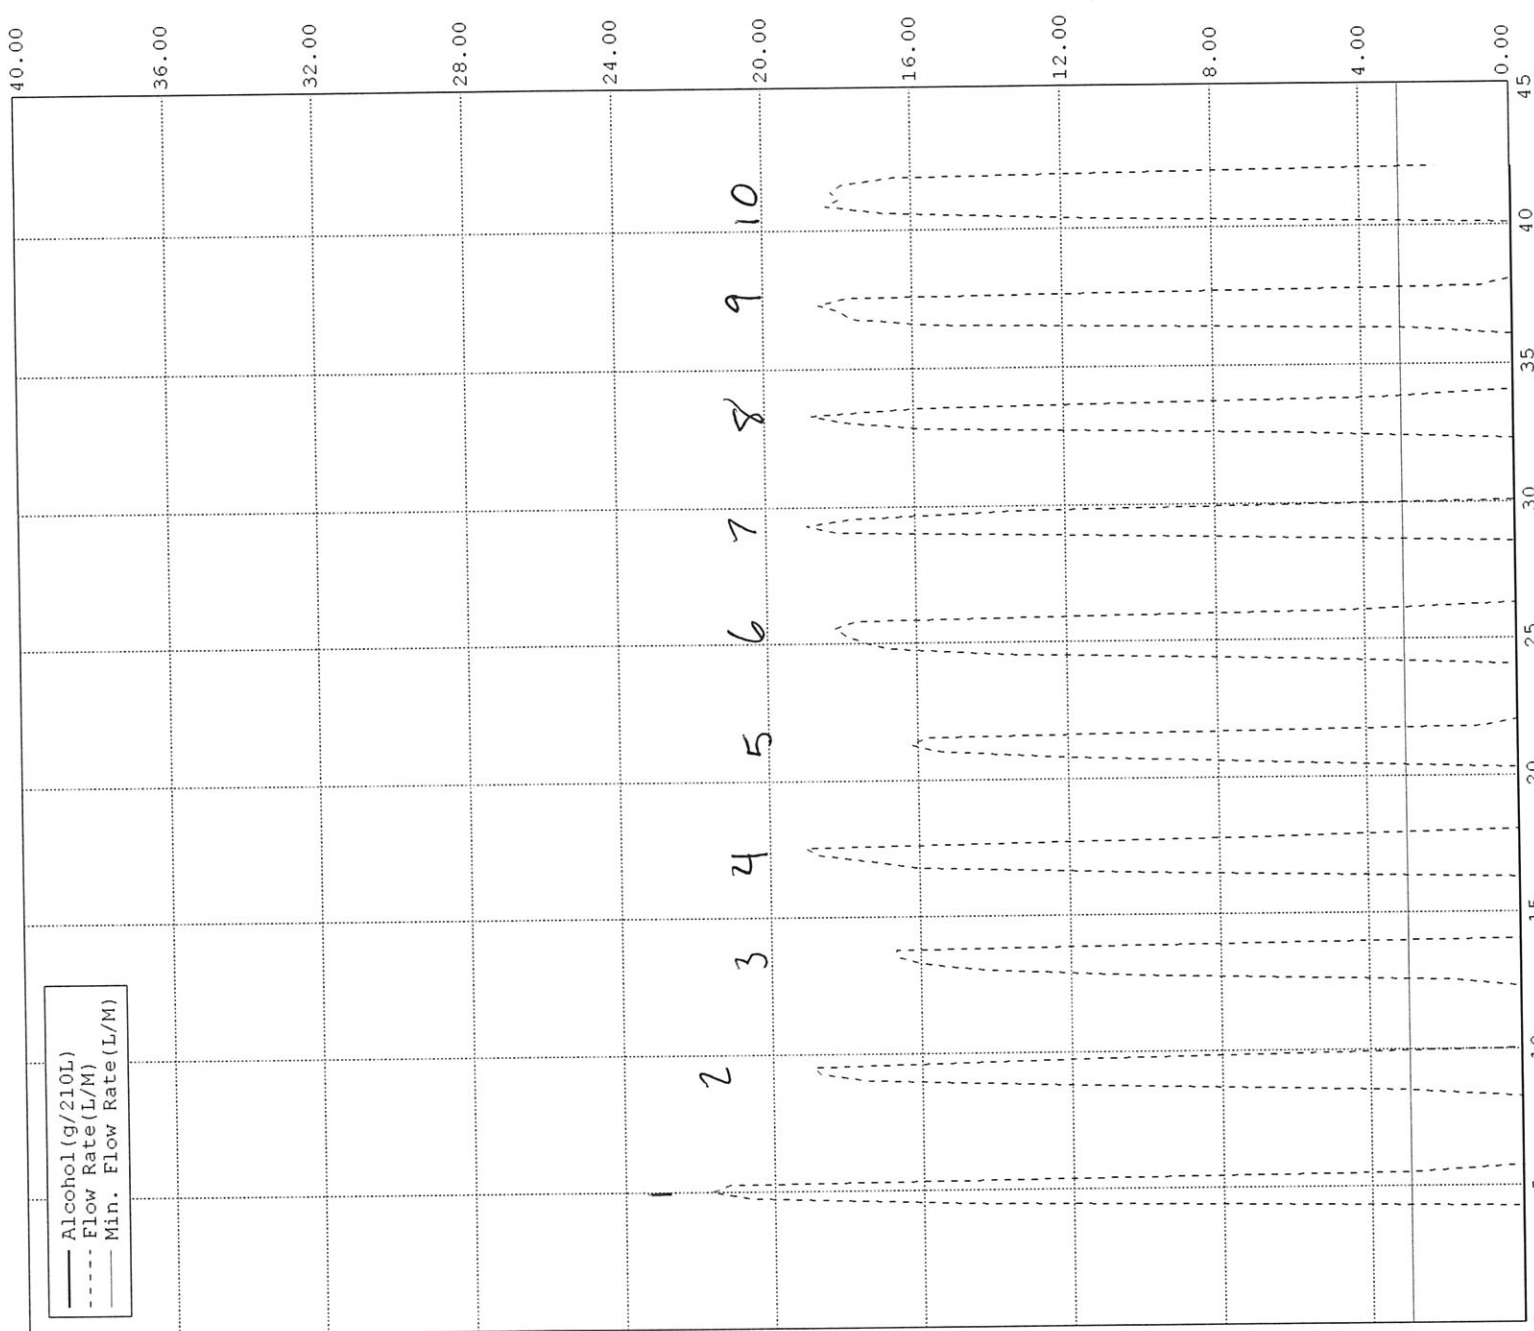

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 11:25:55

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:27
BLANK TEST	0.000	11:27
INTERNAL STANDARD	VERIFIED	11:27
EXTERNAL STANDARD	0.079	11:27
BLANK TEST	0.000	11:28
SUBJECT SAMPLE	INVALID	11:28

MNC

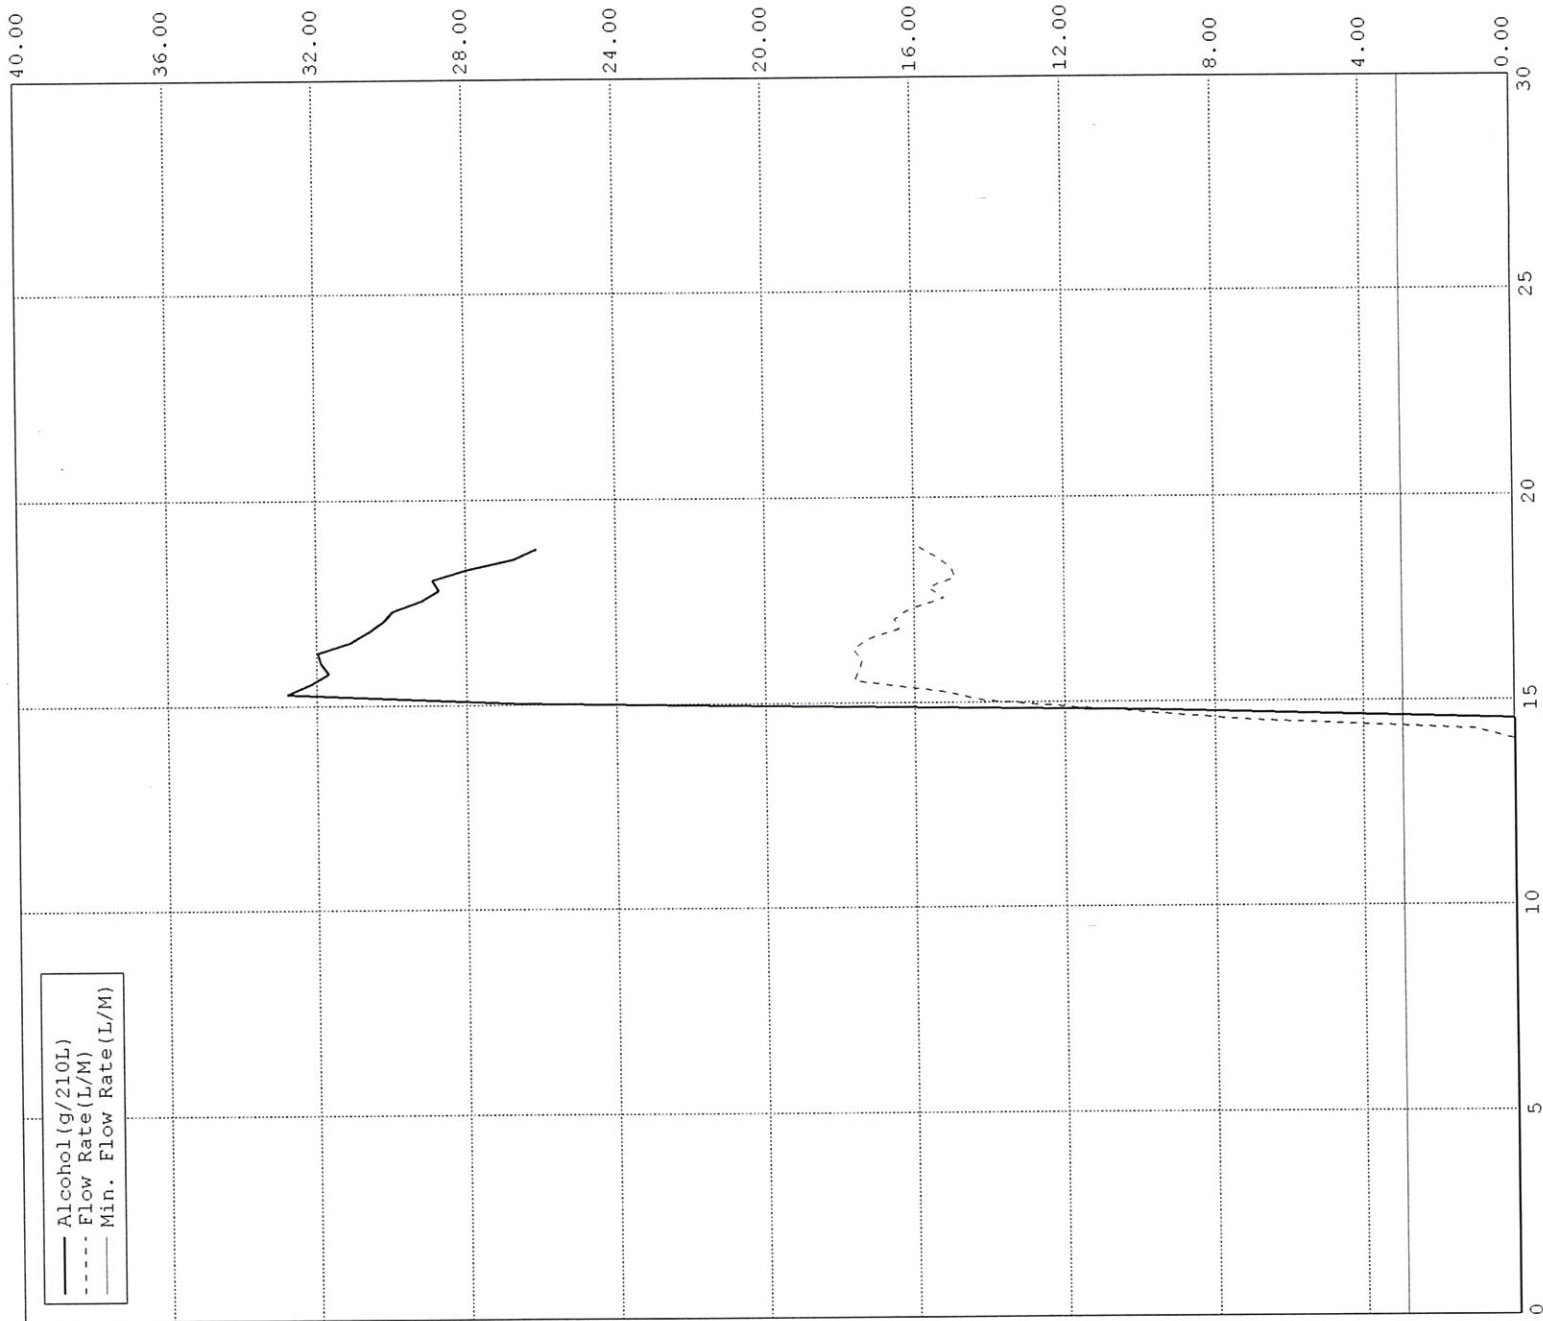

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 11:31:42

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:

RFI
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 29.10: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:36
BLANK TEST	0.000	11:36
INTERNAL STANDARD	VERIFIED	11:36
EXTERNAL STANDARD	0.078	11:36
BLANK TEST	0.000	11:37

RFI DETECTED

MNC

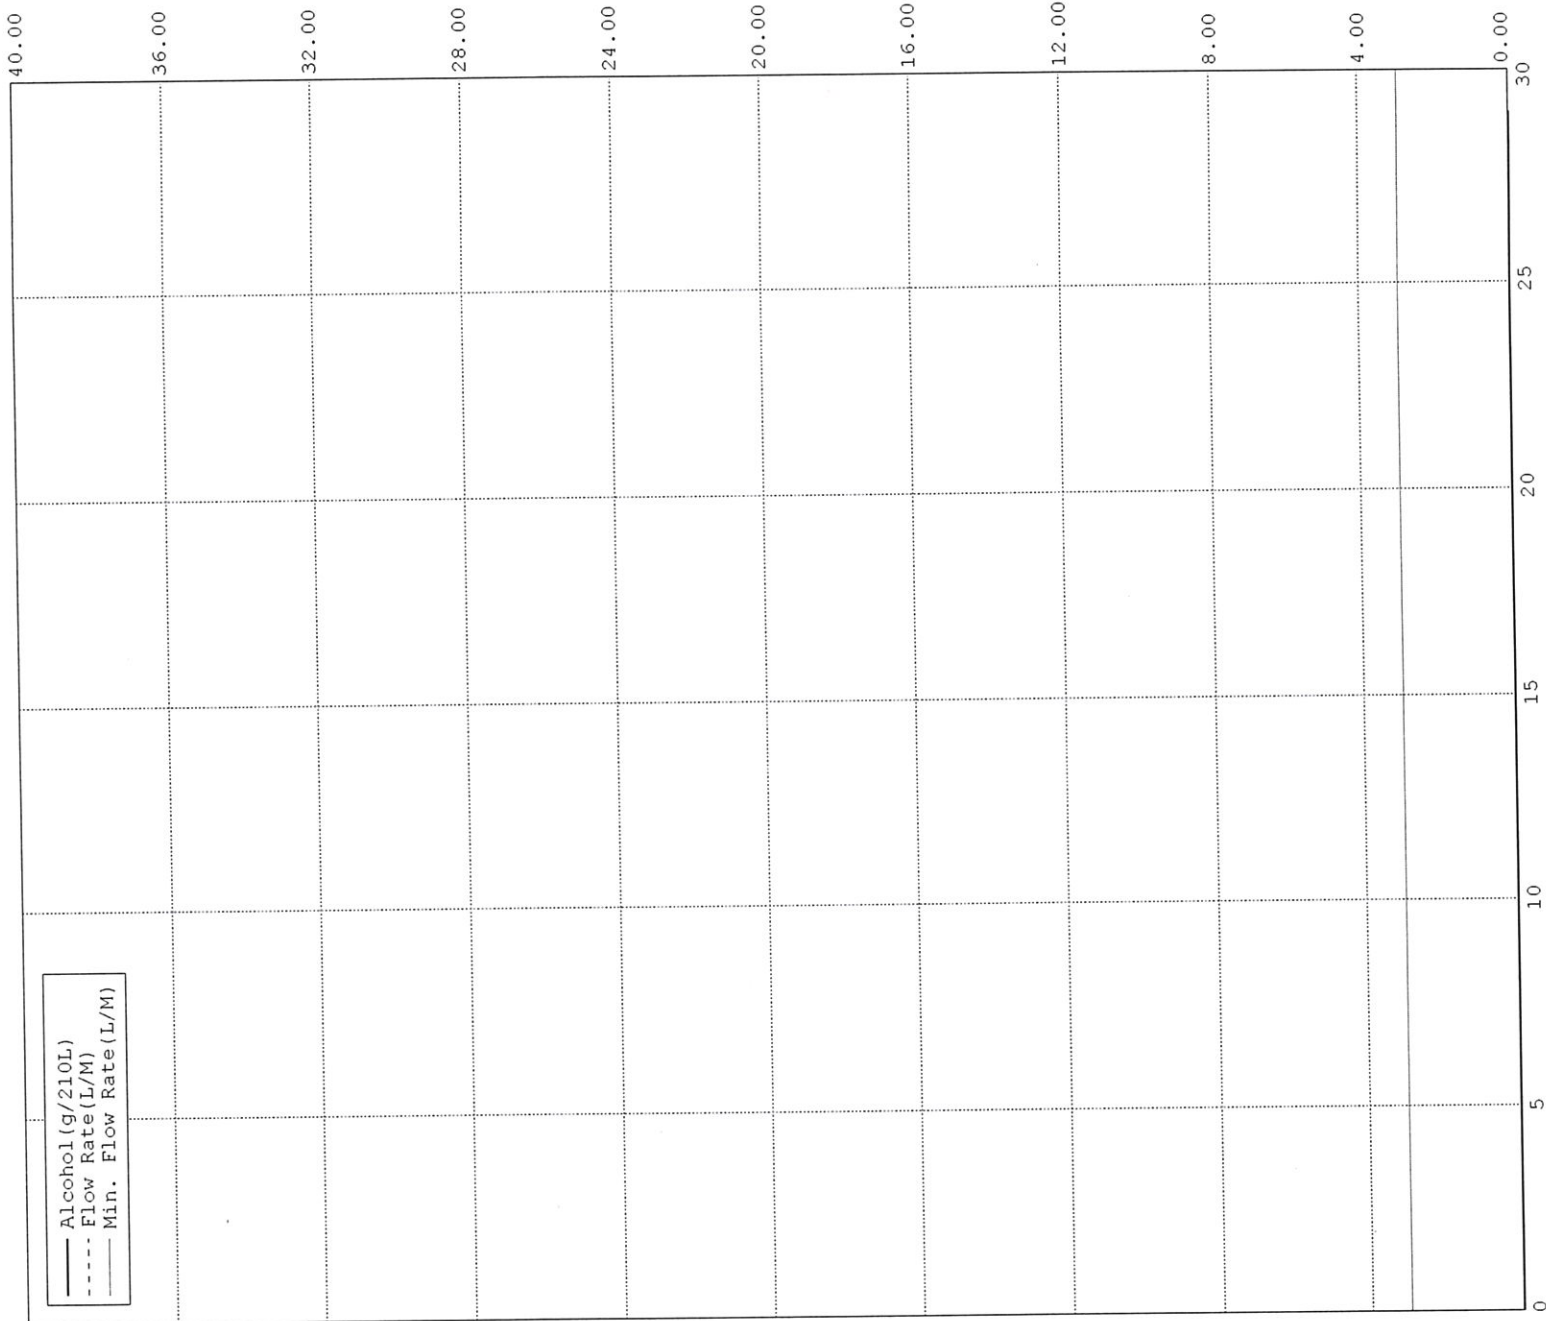

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 12:11:00

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.08: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:11
BLANK TEST	0.000	12:12
INTERNAL STANDARD	VERIFIED	12:12
Xg = 0.089 (0.39%)		
EXTERNAL STANDARD	0.079	12:12
X[1] = 0.0786 (0.0014) (0.0017)		
BLANK TEST	0.000	12:13
SUBJECT SAMPLE	XXX	12:13
X[1] = 0.1098 (-0.0227) (0.0000)		


Interference Detected

Filter 2 Average: 0.0011

Filter 3 Average: 0.0019

MNC 12/11/24

MNC

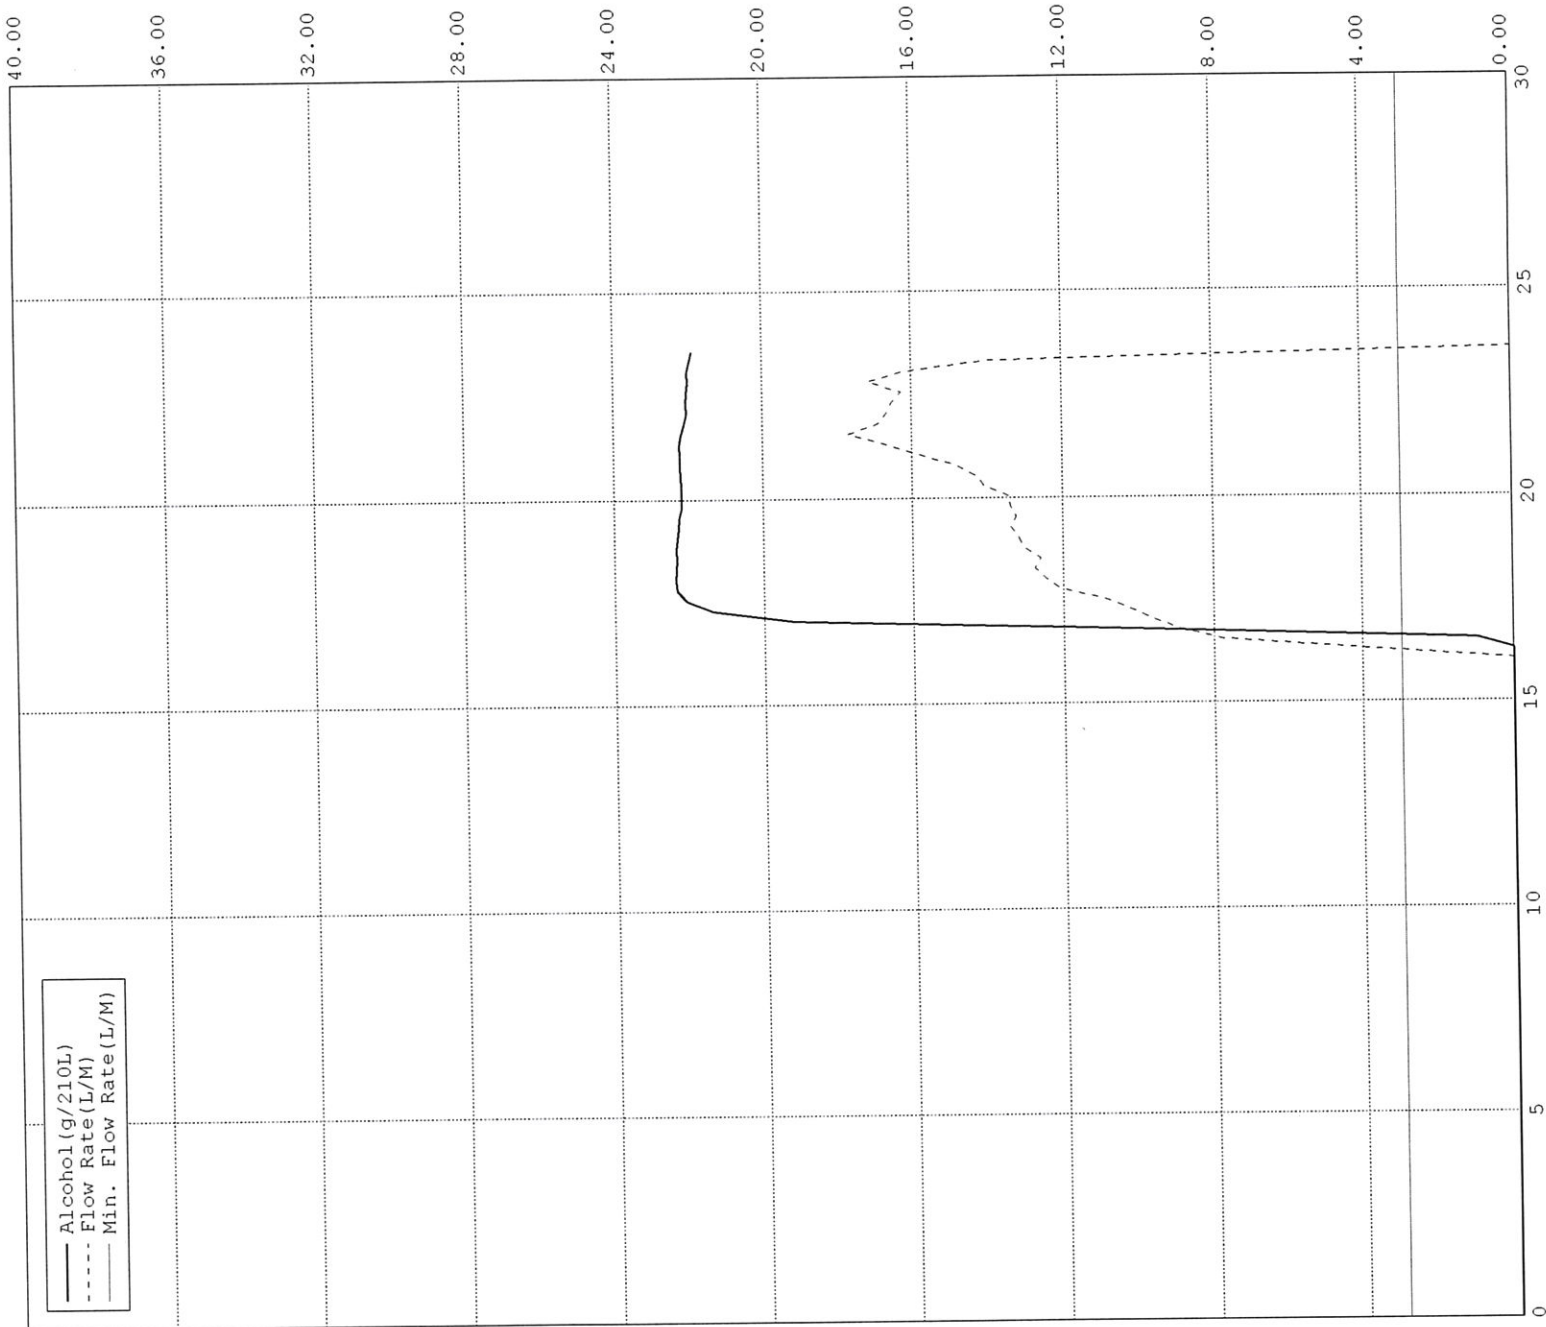

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100670

Date: 12/11/2024

Time: 12:05:46

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - IPA

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.08: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

PASSED 12:06

BLANK TEST

0.000 12:06

INTERNAL STANDARD

VERIFIED 12:07

Xg = 0.089 (0.10%)

EXTERNAL STANDARD

0.078 12:07

X[l] = 0.0784 (0.0008) (0.0019)

BLANK TEST

0.000 12:08

SUBJECT SAMPLE

XXX 12:08

X[l] = 0.1207 (-0.0288) (0.0007)

Interference Detected



MNC

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100670

Date: 12/11/2024
Time: 11:56:17

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.08: 0.078
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	11:59
BLANK TEST	0.000	11:59
INTERNAL STANDARD	VERIFIED	11:59
$X_q = 0.089$ (0.20%)		
EXTERNAL STANDARD	0.079	12:00
$X[1] = 0.0785$ (0.0011)	(0.0018)	
BLANK TEST	0.000	12:01
SUBJECT SAMPLE (Vol=1.75L)	0.096	12:01
$X[1] = 0.0967$ (-0.0029)	(-0.0004)	
BLANK TEST	0.000	12:02
EXTERNAL STANDARD	0.078	12:02
$X[1] = 0.0781$ (0.0010)	(0.0021)	
BLANK TEST	0.000	12:03

MNC



SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100670

Date: 12/11/2024

Time: 12:34:58

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

NON-DRINKING SUBJECT TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 29.07: 0.078

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

EXTERNAL STANDARD

BLANK TEST

SUBJECT SAMPLE (Vol=2.52L)

BLANK TEST

EXTERNAL STANDARD

BLANK TEST

PASSED 12:35
0.000 12:36
VERIFIED 12:36
0.079 12:36
0.000 12:37
0.000 12:37
0.000 12:38
0.079 12:38
0.000 12:39

MNC

