



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory
4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100406

Report Issue Date: 01/13/2025
Date Received: 2024-06-13
Condition of Item: Damaged

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG217902	0.019	0.019	0.019	0.020	0.020	0.019
0.080	0.080	AG335202	0.079	0.079	0.079	0.079	0.079	0.079
0.300	0.299	AG327804	0.300	0.299	0.299	0.299	0.299	0.299

As Found - Evaluation Analyst: Kaija Swisher

As Found Conditions - Barometric Pressure (inHg): 29.85 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.0 Relative Humidity (%): 45

As-Found Lab Activity Date Range: 06/13/2024 - 06/18/2024

Double check valve not securely attached even after adhesive was used. Exposed wire (bottom right side of board). VOC and linearity was able to be completed after securing breath tube connection. Replaced O-Ring. Linearity performed 6/18/24, status message "breath tube temp too low" occurred multiple times before testing could begin. Supervised casework with Derek Walton.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.021	0.021	0.020	0.021	0.020	0.021	+/- 0.002
0.040	0.040	AG407908	0.041	0.041	0.041	0.040	0.041	0.041	+/- 0.003
0.080	0.080	AG335202	0.080	0.080	0.080	0.080	0.080	0.080	+/- 0.004
0.100	0.101	AG333401	0.102	0.102	0.101	0.102	0.102	0.102	+/- 0.004
0.150	0.151	AG332004	0.149	0.149	0.149	0.149	0.149	0.149	+/- 0.006
0.300	0.302	AG427706	0.301	0.300	0.300	0.300	0.301	0.300	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 30.11 Barometer Used: Fisher S/N 230307229 Temperature (C): 21.4 Relative Humidity (%): 3

As-Left Lab Activity Date Range: 11/21/2024 - 11/21/2024

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Megan Carlock



State of Alaska
Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
Anchorage, Alaska 99507
David Kanaris, Chief, Forensic Laboratories



Serial Number: 100406

Results authorized by Megan Carlock on 01/10/2025

megan.crouse@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 01/13/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100406

Analyst or Technician Name: Megan Carlock

DataMaster DMT Calibration Start Date: 11/21/24

Diagnostic Test

- ☒ Perform Diagnostic Test (View Details)
- ☒ Internal Standard Value $\leq 3.00\%$

Technician Screen and Calibration Factors

- ☒ Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- ☒ Set RFI Sensitivity
- ☒ Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 230307229
- Calibration Due Date: 5/2/25
- ☒ Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- ☒ Print Technician Screen
- ☒ Print "Cal Factors"

Minimum Volume Test

- ☒ Perform Minimum Volume (Subject) Test: 1.5 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 30.11 Temperature(C) 21.4 Relative Humidity(%) 3

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- ☒ Incomplete
- ☒ Invalid
- ☒ Maximum Attempts Exceeded
- ☒ Radio Frequency Interference (RFI)
- ☒ Interference (Volatiles) - *Print with View Details*

1. Acetone Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR4161 Thermometer Verification Performed? ☒
2. Isopropanol Reagent Lot Number: 20241107KS Expiration Date: 2/7/25
Simulator S/N: DR5298 Thermometer Verification Performed? ☒
3. Negative (Ethanol Only) Lot Number: 231P41233 Expiration Date: 9/20/25
Simulator S/N: DR4163 Thermometer Verification Performed? ☒

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 10/19/25 9/19/25
MNC 1/10/25

Administrative

- ☒ Verify Stylus Calibration
- ☒ Reset Options
- ☒ Clear Memory
- ☒ Verification of Calibration (VOC)
- ☒ Perform Non-Drinking Subject Test
- ☒ Upload Instrument
- ☒ Remove Dry Gas Tank Before Shutdown
- ☒ Add Ready for Tech Review Note

Completion

Lab Work End Date: 11/21/24

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 11/21/24

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 11/21/2024
Time: 10:36:30

VERSIONS
DMT: 3.02
PIC: 3.02
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.7°C (44.0°C - 52.0°C)	PASSED
Breath Tube = 43.5°C (38.0°C - 50.0°C)	PASSED

SETTINGS

Lamp Voltage = 1.76 V (1.07 V - 2.51 V)	PASSED
Cooler Voltage = 1.71 V (1.07 V - 2.51 V)	PASSED
Bias Voltage = 80 V (48 V - 112 V)	PASSED
Chopper Freq = 532 Hz (475 Hz - 575 Hz)	PASSED
Barometer = 30.1 in	

PUMP INFO

Flow Rate = 5.080 L/M (3.500 L/M - 6.500 L/M)	PASSED
--	--------

DETECTOR INFO

PUMP ON (0.002 V <= 0.010 V)	PASSED
PUMP OFF (0.002 V <= 0.010 V)	PASSED

FILTER INFO

Filter 1	PASSED
Filter 2	PASSED
Filter 3	PASSED

INTERNAL STANDARD

Xq = 0.085 0.51% (0.00% - 4.00%)	PASSED
----------------------------------	--------

Technician Screen

DATAMASTER dmt: 100406

Date: 11/21/2024

Time: 10:53 AM

Temperatures (°C)

Sample Cell: 48.7°C

Breath Tube: 44.5°C

Current Barometer 30.1 in

Volume (Ltr) 1.55

Settings

Lamp: 1.68 V

Bias: 80 V

Cooler: 1.94 V

Chopper: 534 Hz

Voltages (V)

Flow: 1.07 V

Detector: -0.024 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 06/14/2021
Time: 06:49:18

OPERATOR NAME:
INTOX I METERS
CERTIFICATE #: TEST

Ca	=	0.1000		
CAL	=	0.983721	0.800 <=	CAL < 1.200
b1	=	0.0005	0.0000 <=	b1 < 0.0040
b2	=	0.0062	0.0010 <=	b2 < 0.0100
b3	=	0.0009	0.0000 <=	b3 < 0.0040
Xq	=	0.0850	0.0500 <=	Xq < 0.2000
a21	=	1.190258	1.050 <=	a21 < 1.300
a31	=	0.460872	0.300 <=	a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100406

Date: 11/21/2024

Time: 10:57:29

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

MINIMUM VOLUME TEST

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080


TARGET AT 30.11: 0.081

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:58
BLANK TEST	0.000	10:58
INTERNAL STANDARD	VERIFIED	10:58
EXTERNAL STANDARD	0.080	10:59
BLANK TEST	0.000	10:59
SUBJECT SAMPLE (Vol=1.55L)	0.000	11:00
BLANK TEST	0.000	11:01
EXTERNAL STANDARD	0.081	11:01
BLANK TEST	0.000	11:02

MNC

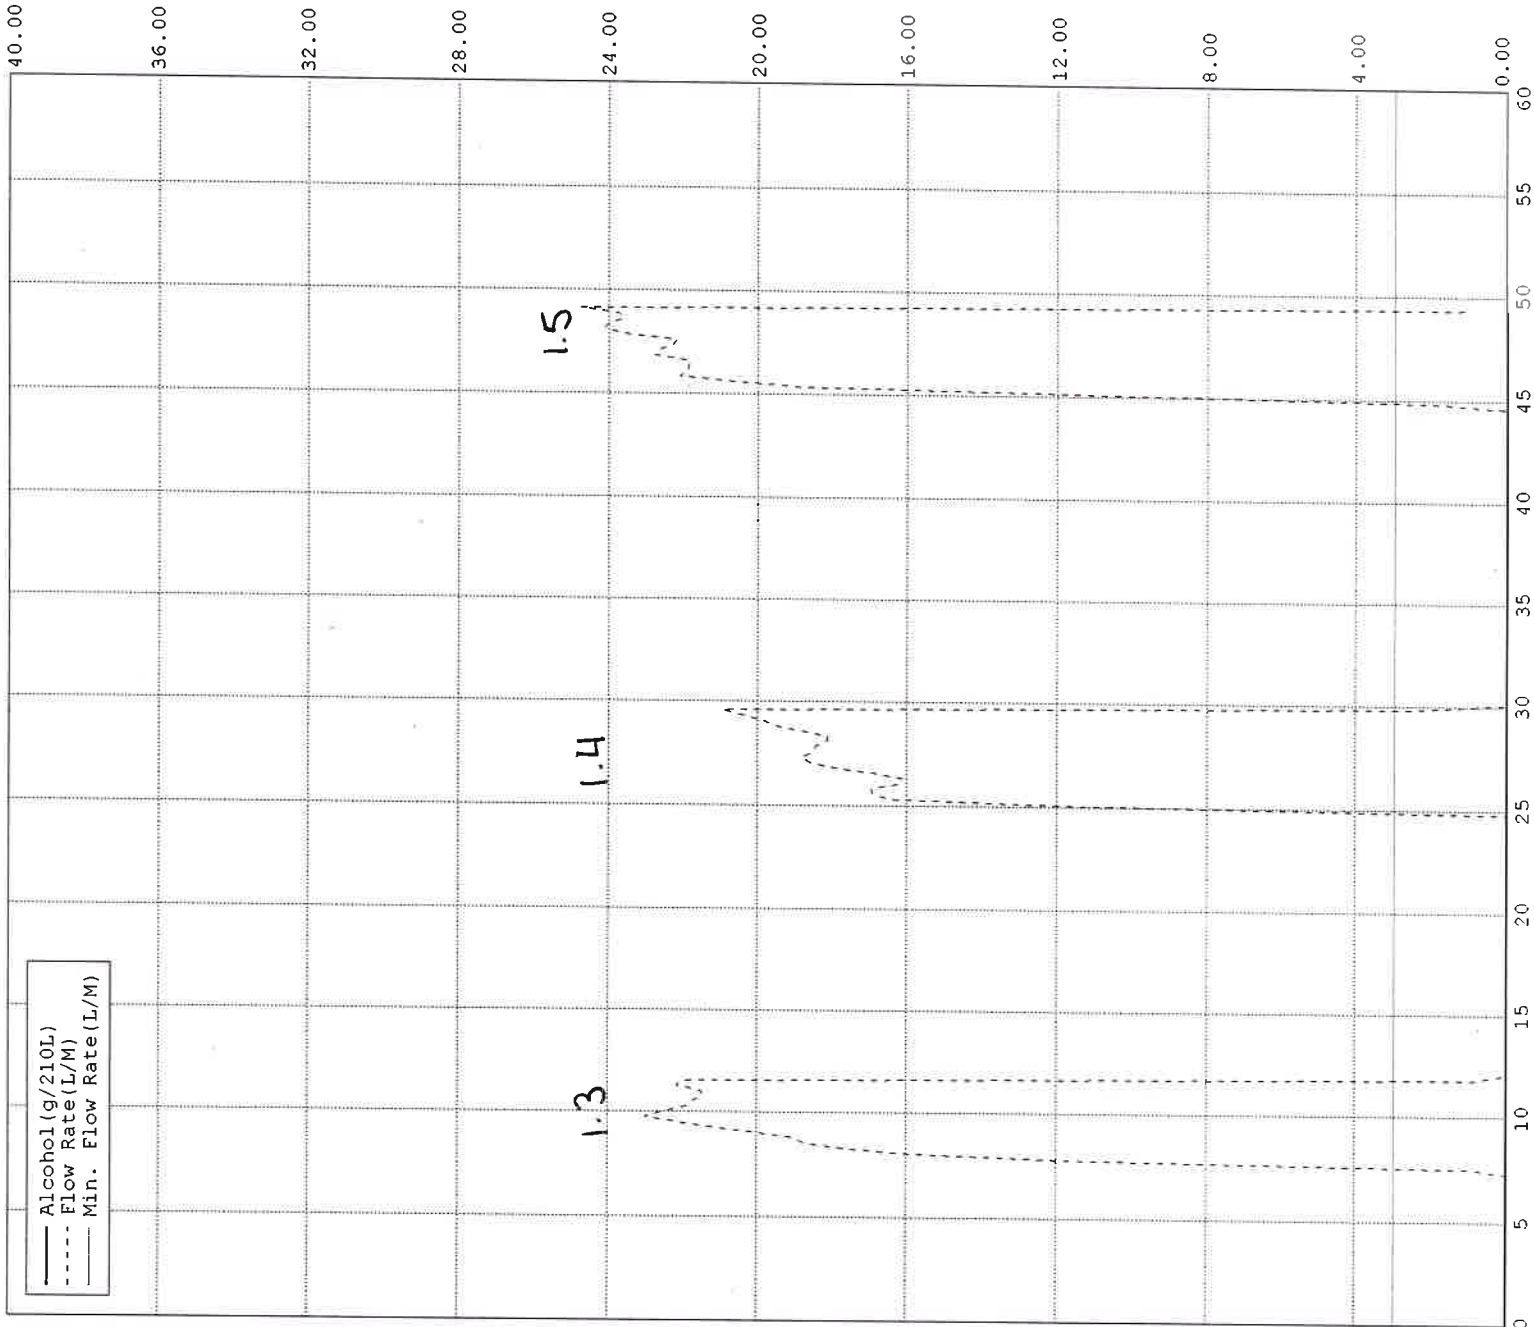

LINEARITY CHECK


Alaska Department of Public Safety
 DATAMASTER dmt: 100406

Date: 11/21/2024
 Time: 11:04:35

SUPERVISOR NAME:
 MEGAN CARLOCK
 OPERATOR'S #: 10747

TARGET	AVERAGE	STD. DEV.
0.020	0.0206	0.0005
0.040	0.0408	0.0004
0.080	0.0800	0.0000
0.101	0.1018	0.0004
0.151	0.1490	0.0000
0.302	0.3004	0.0005

SLOPE = 0.990475
 R² = 0.999939

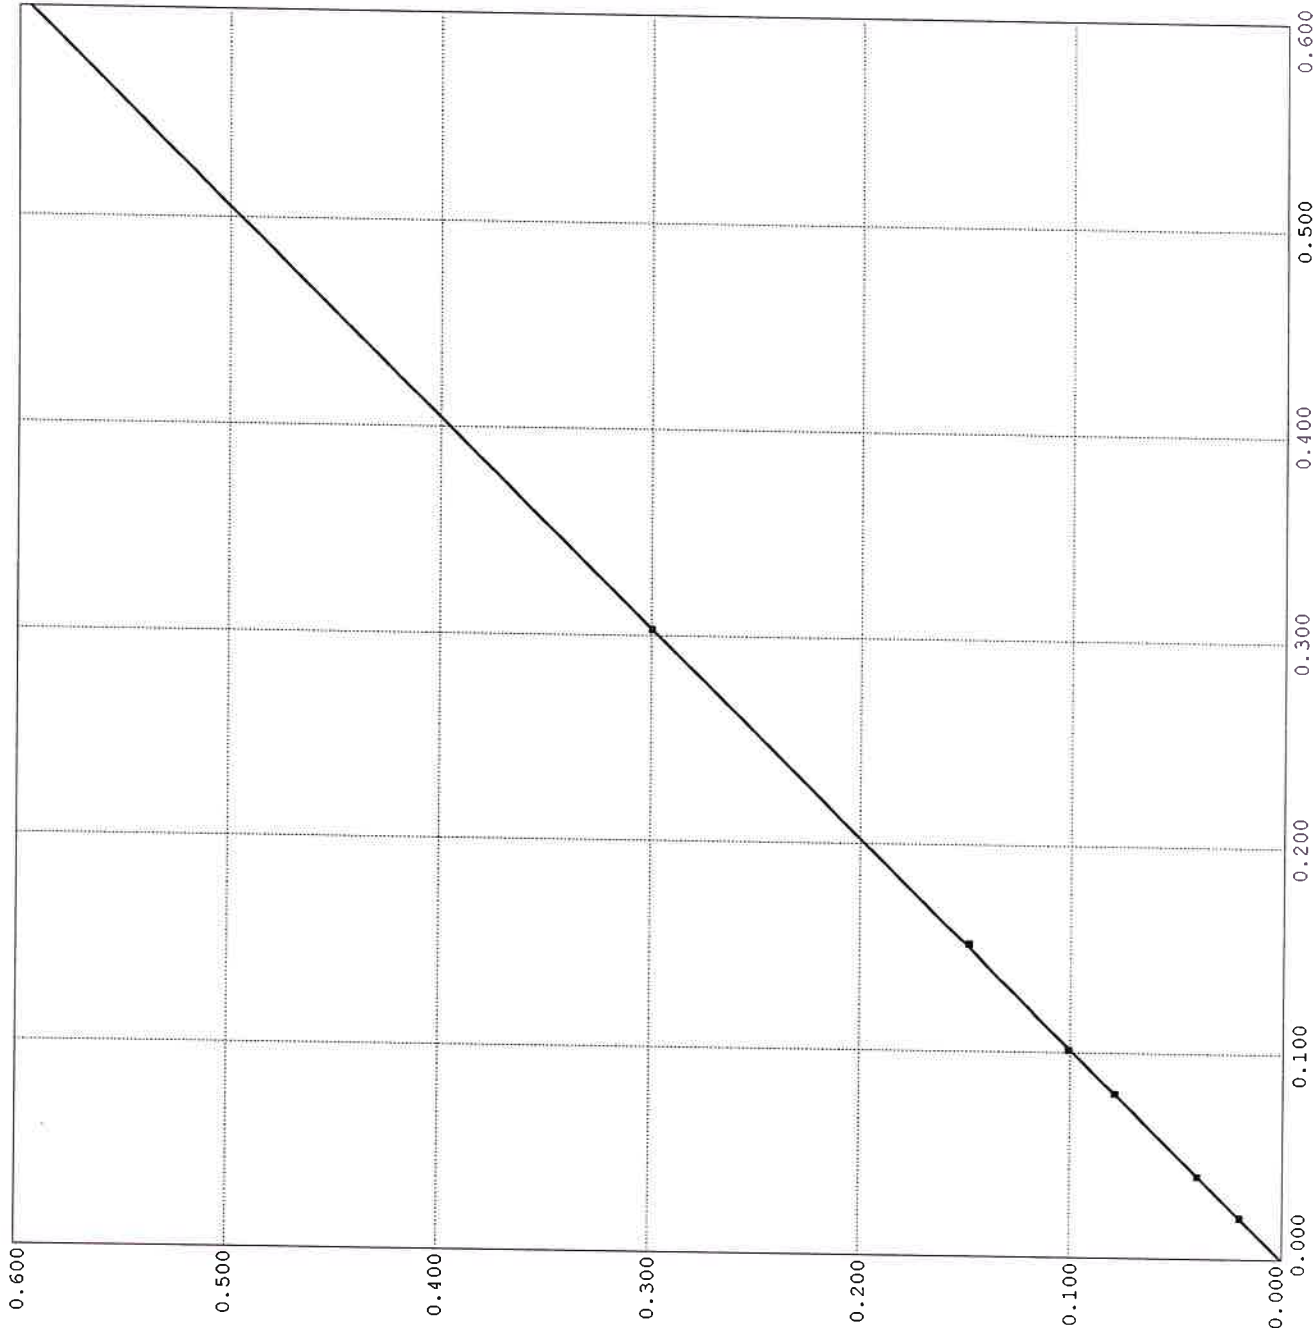

MNC

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
DATAMASTER dmt: 100406






Date: 11/21/2024
Time: 11:04:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
TARGET AT 30.10: 0.020
LOT #: AG408002
EXPIRATION: 03/20/2026
TANK PRESSURE: 335 psi

TEST TYPE	CONC	TIME
BLANK TEST	0.000	11:06
INTERNAL STANDARD	VERIFIED	11:06
EXTERNAL STANDARD	0.021	11:06
BLANK TEST	0.000	11:07
EXTERNAL STANDARD	0.021	11:07
BLANK TEST	0.000	11:08
EXTERNAL STANDARD	0.020	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.021	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.020	11:10
BLANK TEST	0.000	11:11

Average = 0.0206
Std Dev = 0.0005

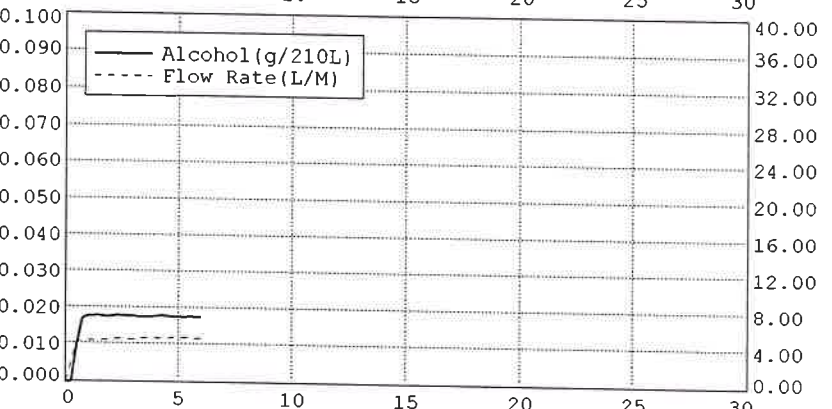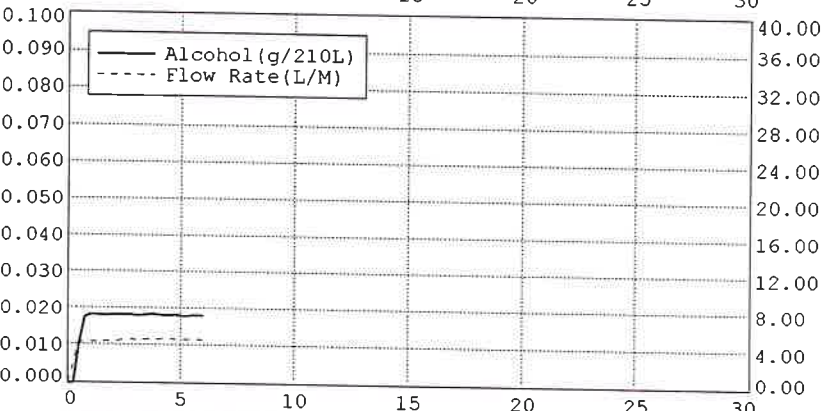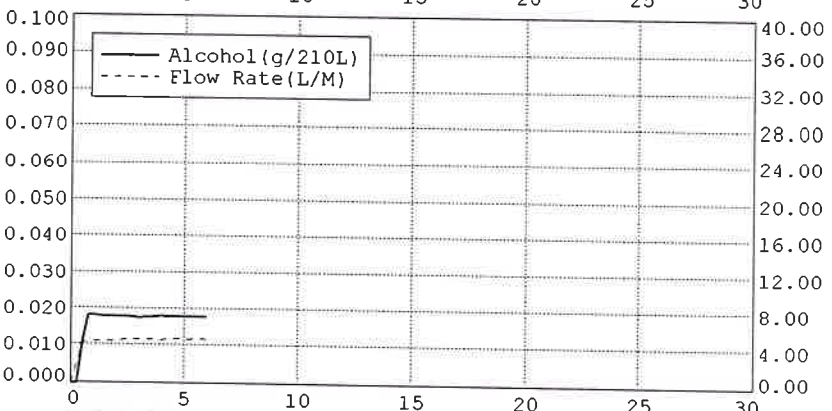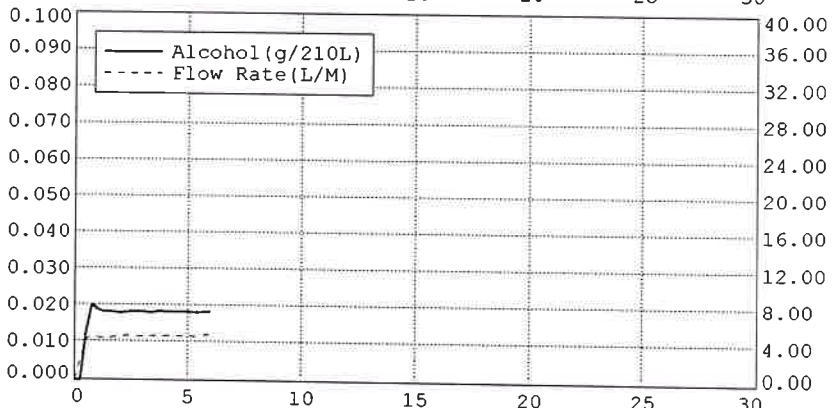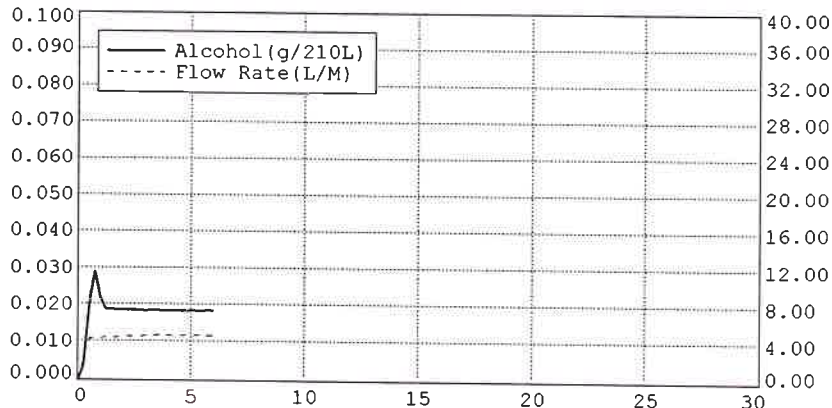

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100406






Date: 11/21/2024
Time: 11:12:11

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 30.10: 0.040
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 982 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	11:13
INTERNAL STANDARD	VERIFIED	11:13
EXTERNAL STANDARD	0.041	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.041	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.041	11:16
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.040	11:17
BLANK TEST	0.000	11:18
EXTERNAL STANDARD	0.041	11:18
BLANK TEST	0.000	11:19

Average = 0.0408
Std Dev = 0.0004

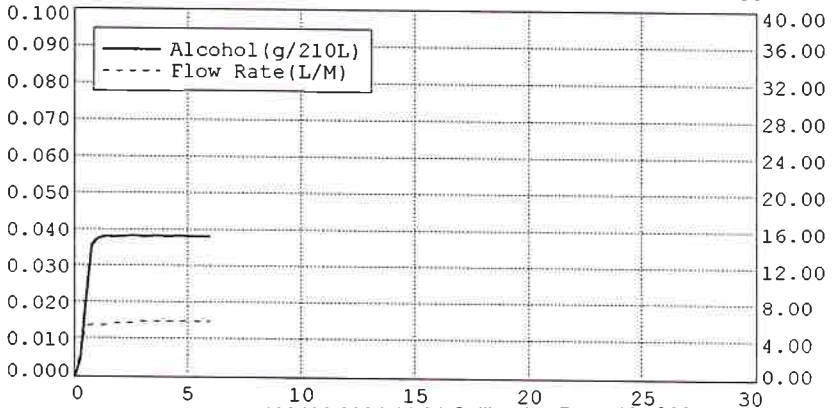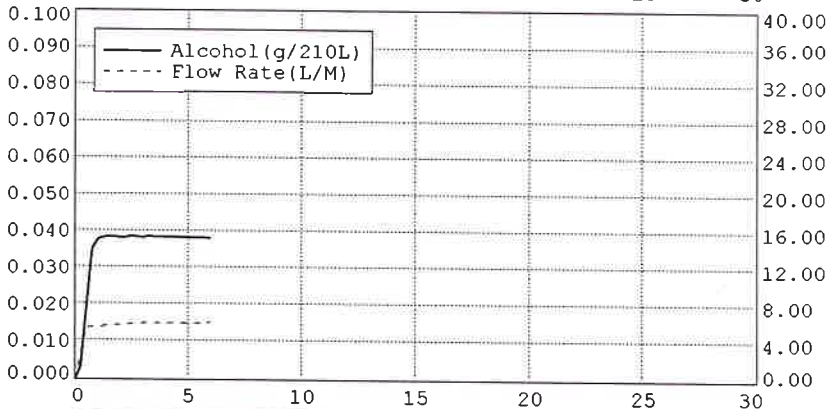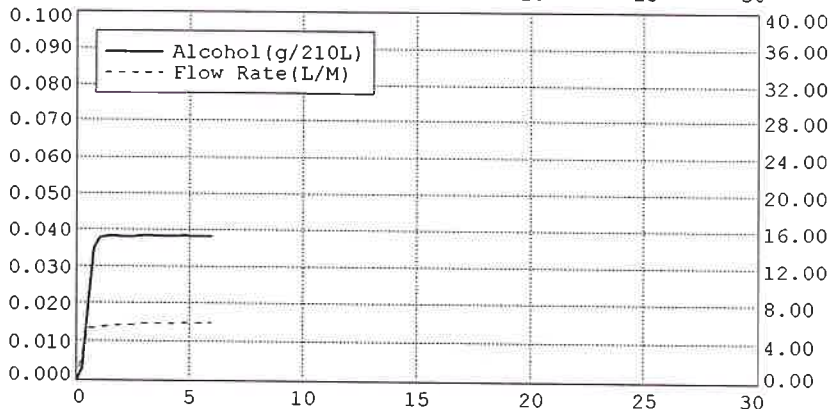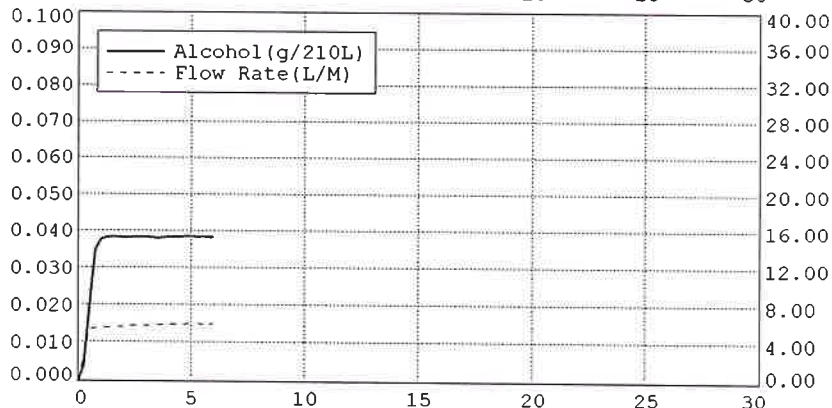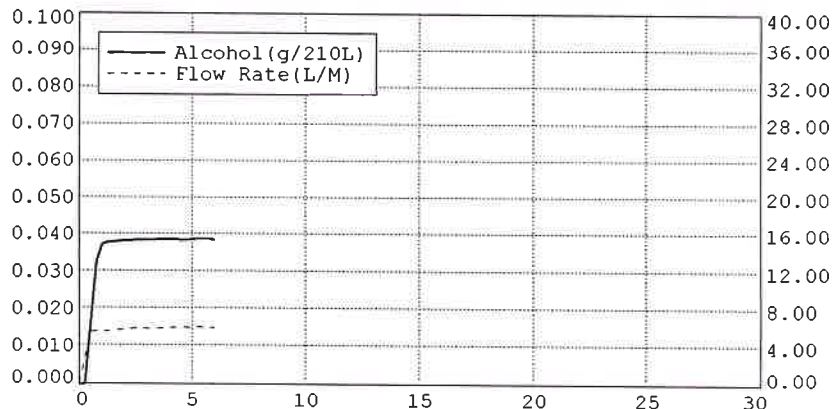

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
DATAMASTER dmt: 100406






Date: 11/21/2024
Time: 11:22:47

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.10: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025
TANK PRESSURE: 389 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	11:24
INTERNAL STANDARD	VERIFIED	11:24
EXTERNAL STANDARD	0.080	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.080	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.080	11:26
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.080	11:27
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.080	11:28
BLANK TEST	0.000	11:29

Average = 0.0800
Std Dev = 0.0000

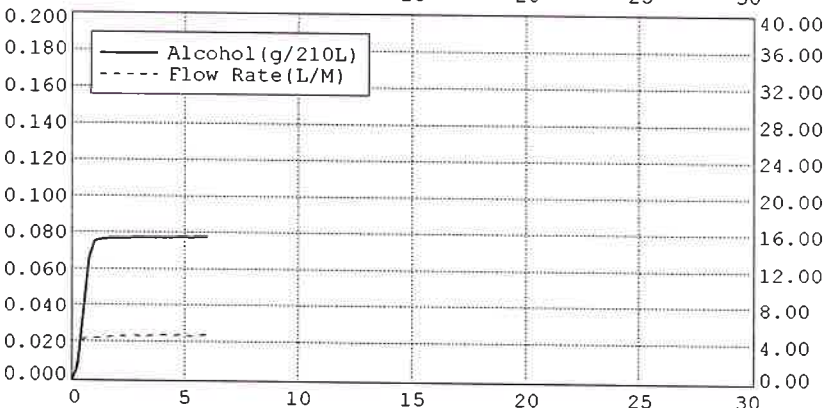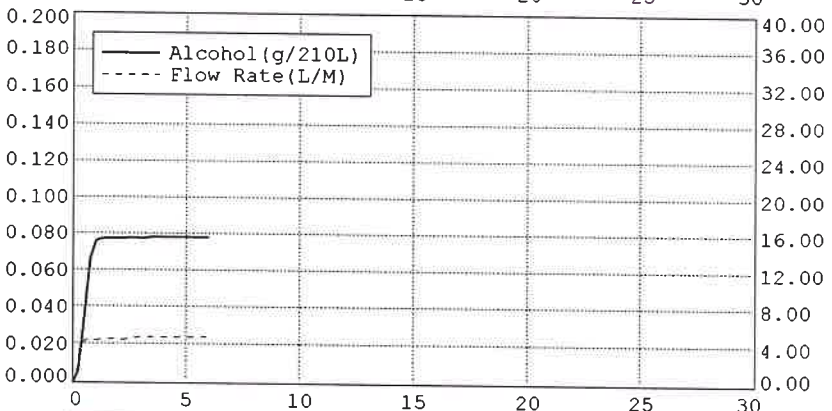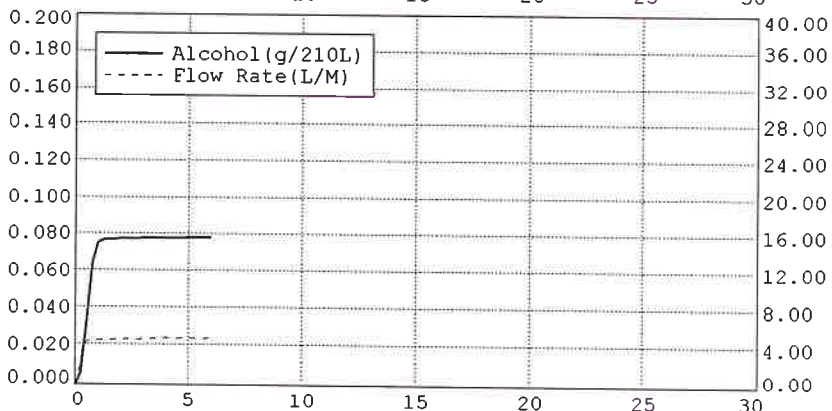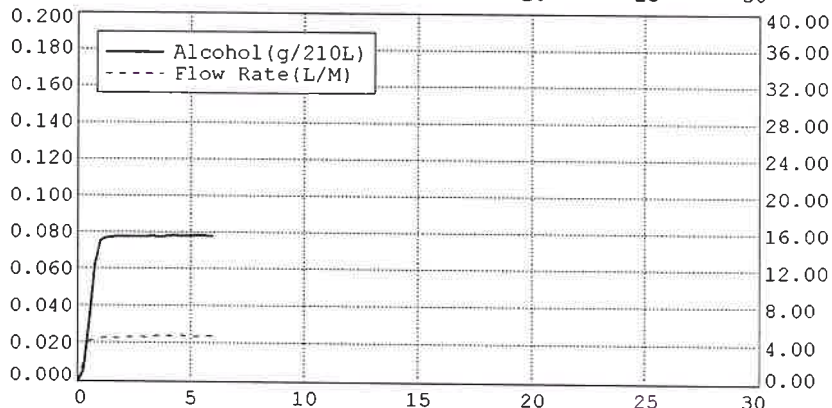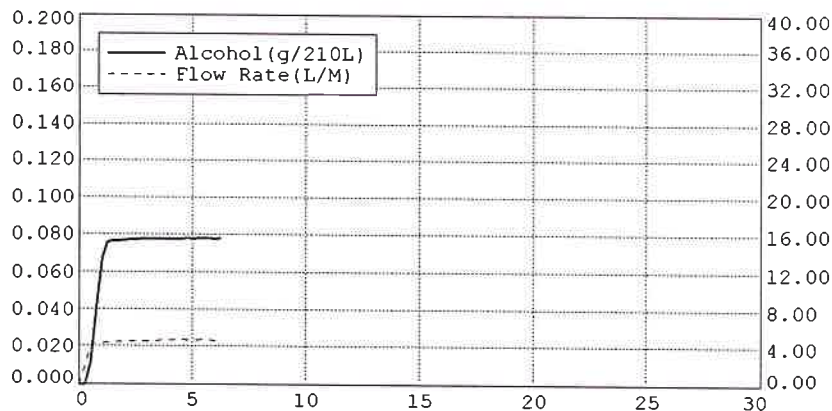

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
DATAMASTER dmt: 100406






Date: 11/21/2024
Time: 11:33:53

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
TARGET AT 30.10: 0.101
LOT #: AG333401
EXPIRATION: 11/30/2025
TANK PRESSURE: 1109 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	11:35
INTERNAL STANDARD	VERIFIED	11:35
EXTERNAL STANDARD	0.102	11:35
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	0.102	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.101	11:37
BLANK TEST	0.000	11:38
EXTERNAL STANDARD	0.102	11:38
BLANK TEST	0.000	11:39
EXTERNAL STANDARD	0.102	11:39
BLANK TEST	0.000	11:40

Average = 0.1018
Std Dev = 0.0004

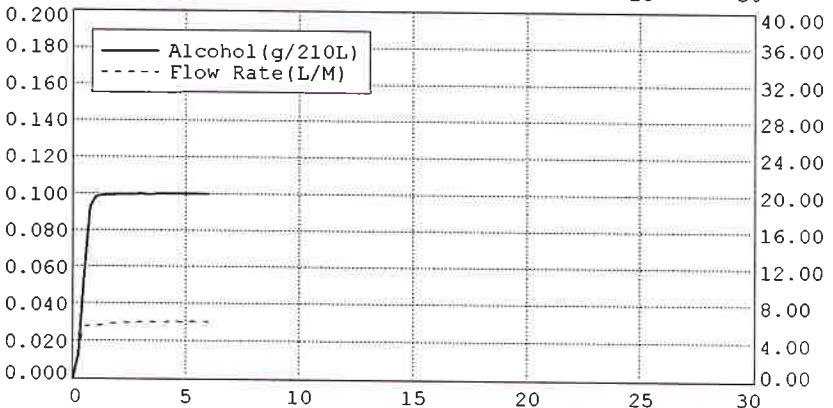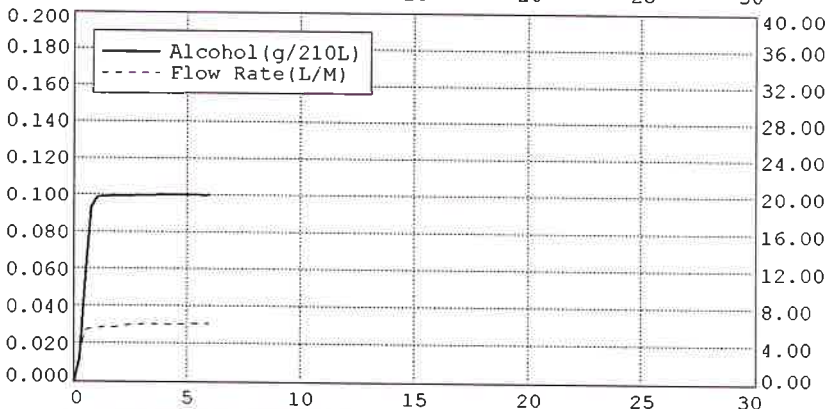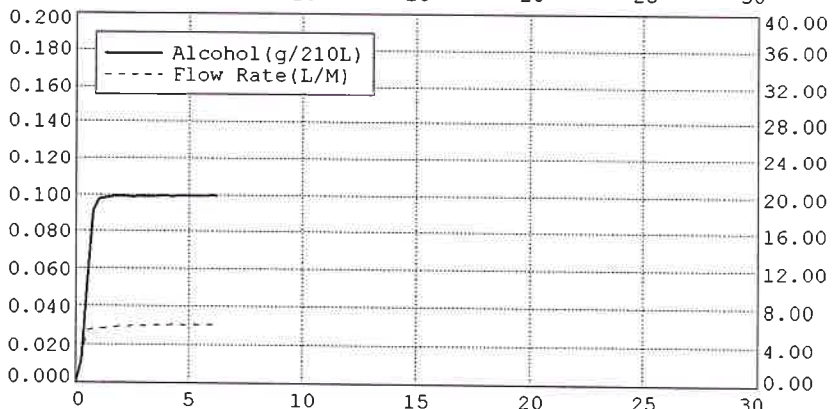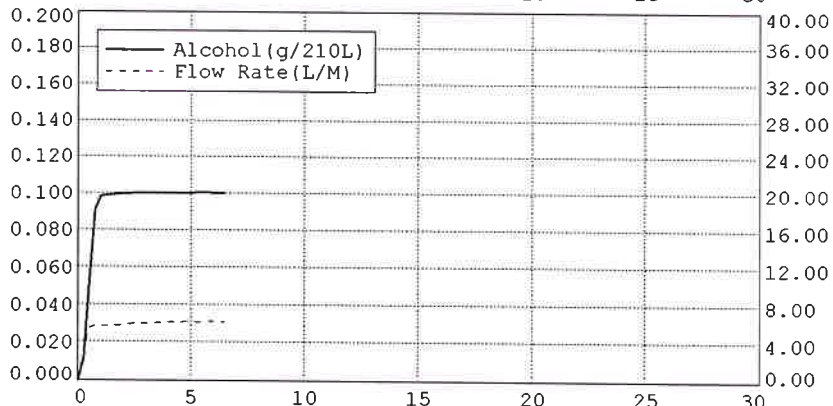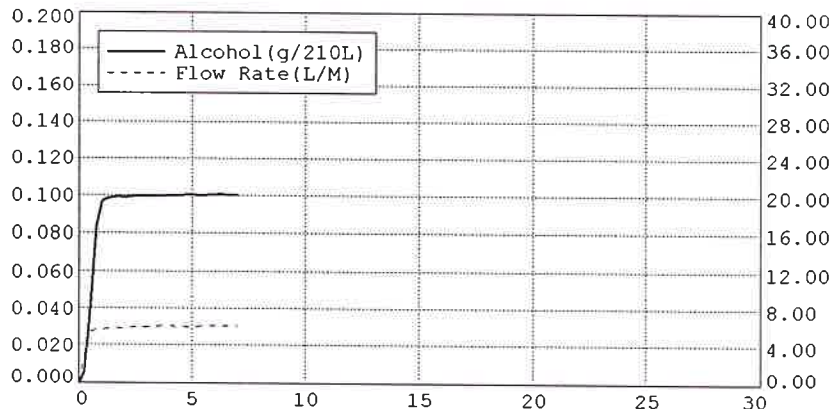

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
DATAMASTER dmt: 100406






Date: 11/21/2024
Time: 11:43:18

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
TARGET AT 30.10: 0.151
LOT #: AG332004
EXPIRATION: 11/16/2025
TANK PRESSURE: 436 psi

TEST TYPE	CONCENTRATION	TIME
BLANK TEST	0.000	11:44
INTERNAL STANDARD	VERIFIED	11:44
EXTERNAL STANDARD	0.149	11:44
BLANK TEST	0.000	11:45
EXTERNAL STANDARD	0.149	11:46
BLANK TEST	0.000	11:47
EXTERNAL STANDARD	0.149	11:47
BLANK TEST	0.000	11:48
EXTERNAL STANDARD	0.149	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.149	11:49
BLANK TEST	0.000	11:50

Average = 0.1490
Std Dev = 0.0000

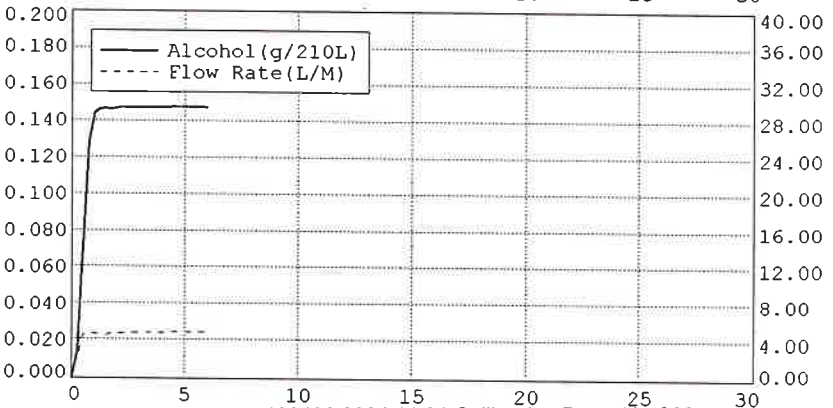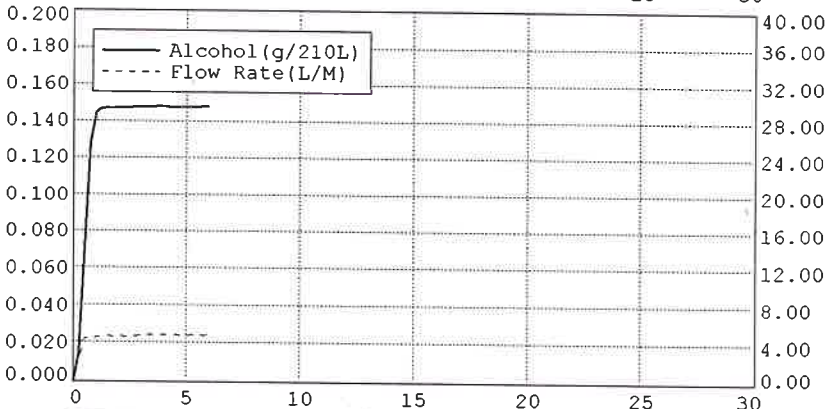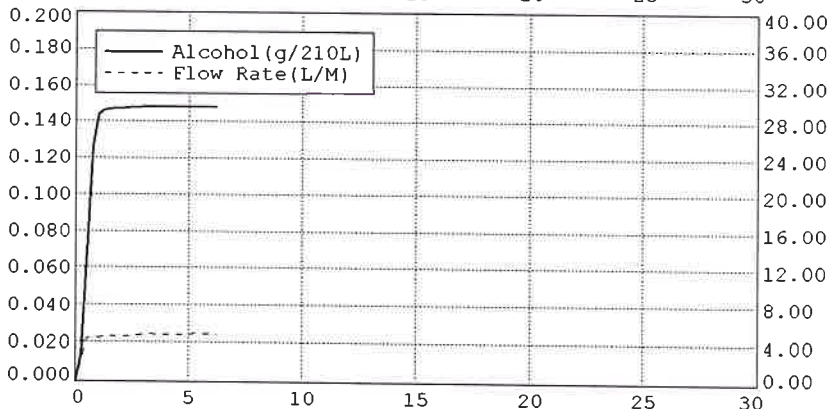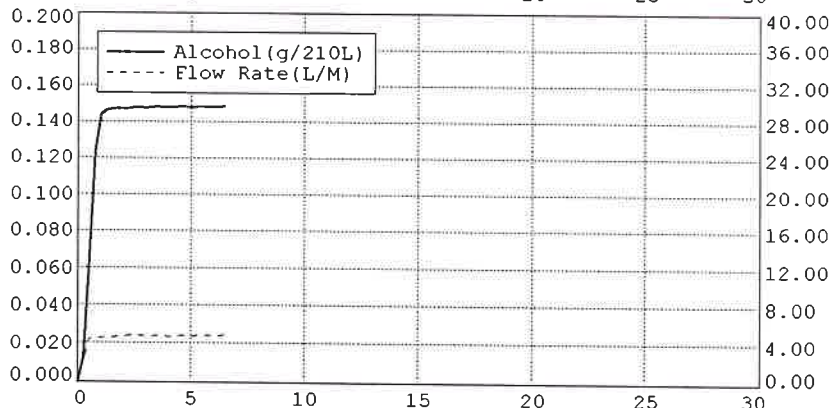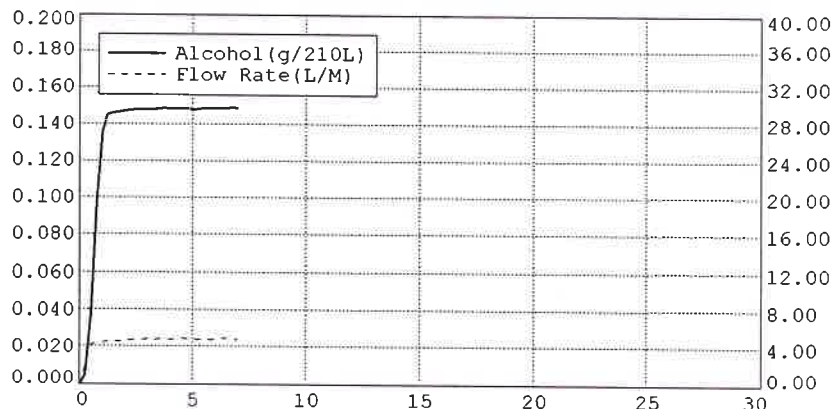

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100406






Date: 11/21/2024
Time: 11:51:06

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 30.10: 0.302
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 343 psi

TEST TYPE	Value	Time
BLANK TEST	0.000	11:52
INTERNAL STANDARD	VERIFIED	11:52
EXTERNAL STANDARD	0.301	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.300	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.300	11:55
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.300	11:56
BLANK TEST	0.000	11:57
EXTERNAL STANDARD	0.301	11:57
BLANK TEST	0.000	11:58

Average = 0.3004
Std Dev = 0.0005

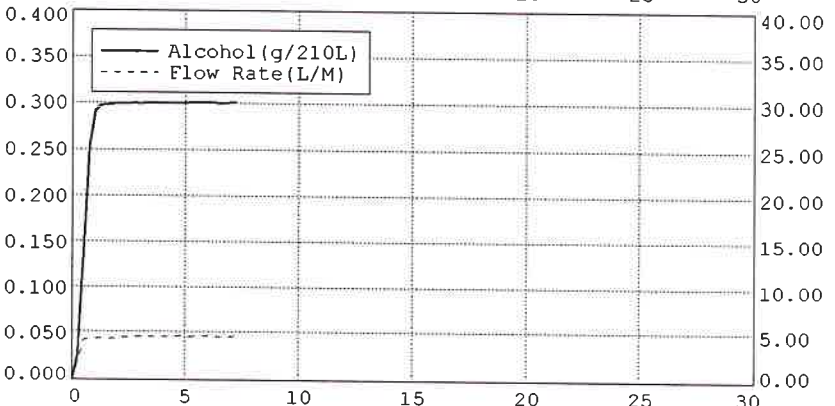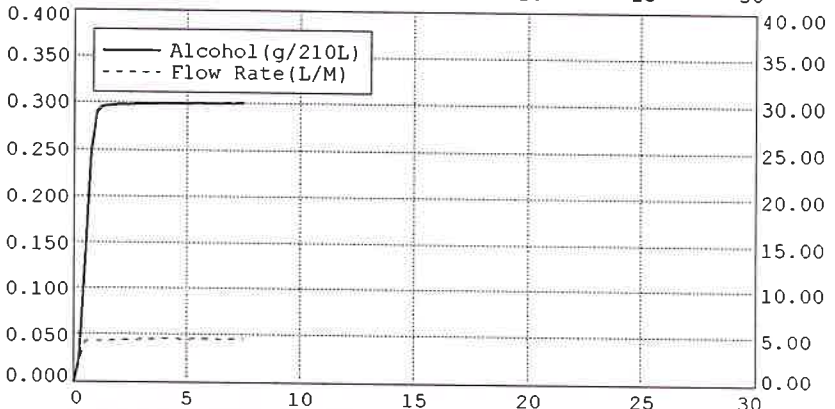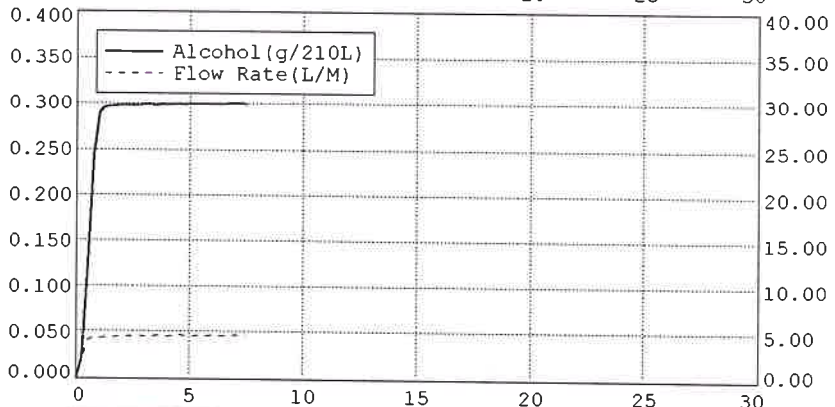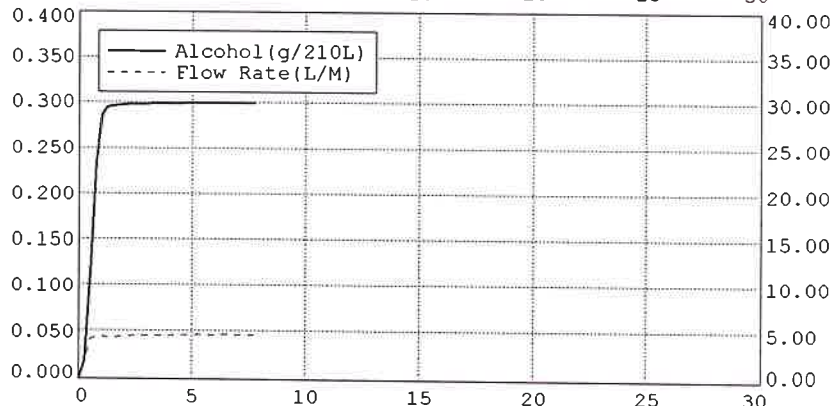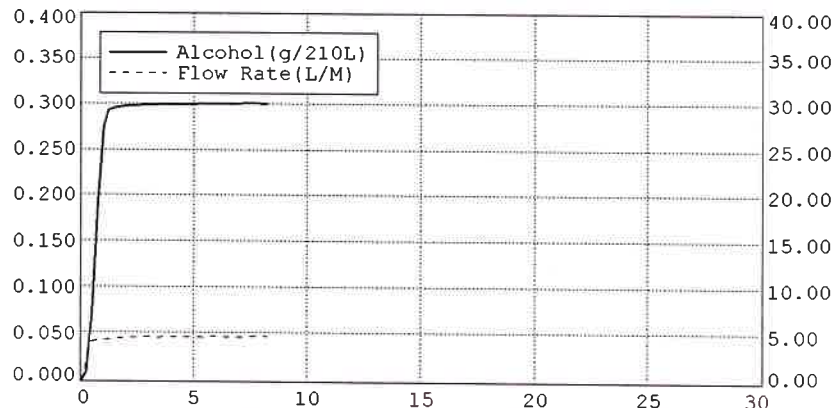

SUBJECT TEST

Alaska Department of Public Safety

DATA MASTER dmt: 100406

Date: 11/21/2024
Time: 12:03:42

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
TARGET AT 30.10: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:04
BLANK TEST	0.000	12:05
INTERNAL STANDARD	VERIFIED	12:05
EXTERNAL STANDARD	0.081	12:05
BLANK TEST	0.000	12:06
SUBJECT SAMPLE	INCOMPLETE	12:08

MNC

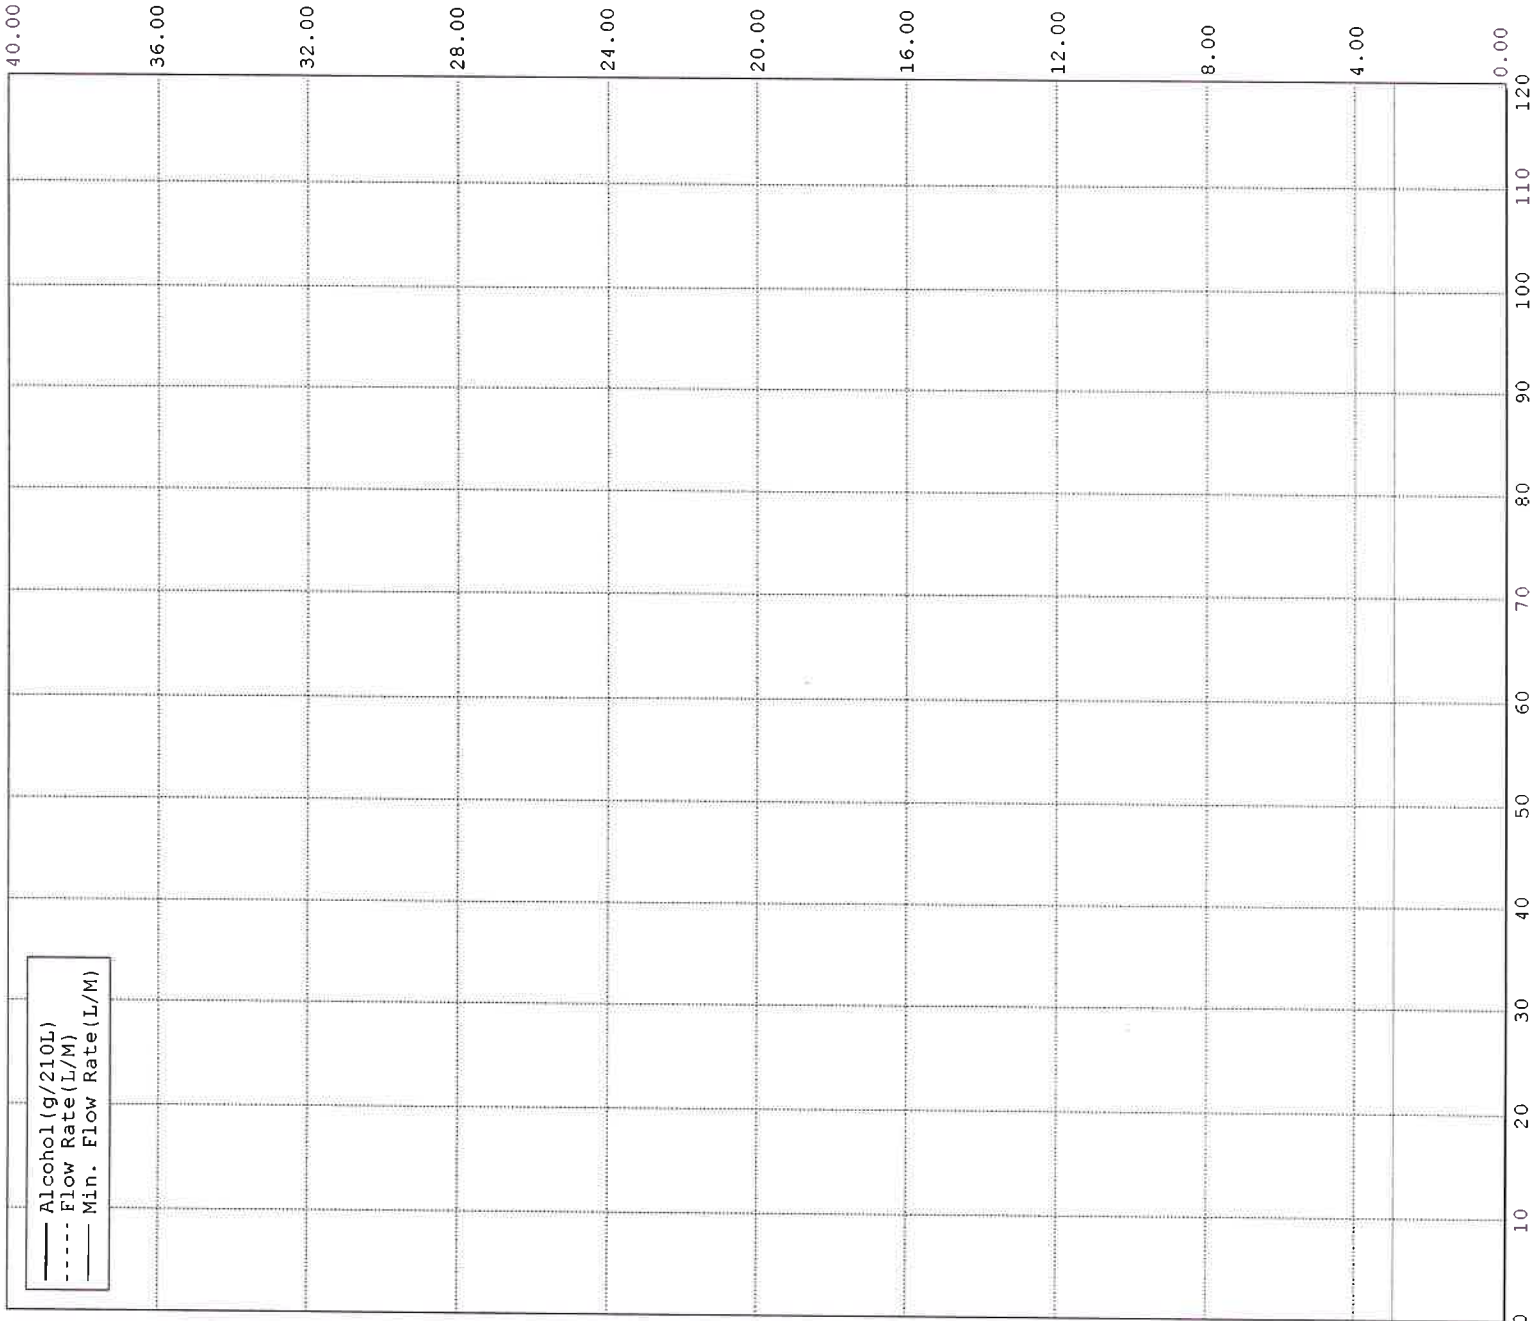

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 11/21/2024
Time: 12:10:28

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
MAXIMUM ATTEMPTS EXCEEDED
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.10: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:11
BLANK TEST	0.000	12:11
INTERNAL STANDARD	VERIFIED	12:11
EXTERNAL STANDARD	0.081	12:11
BLANK TEST	0.000	12:12
SUBJECT SAMPLE	XXX	12:13

Maximum Attempts Exceeded

MWC

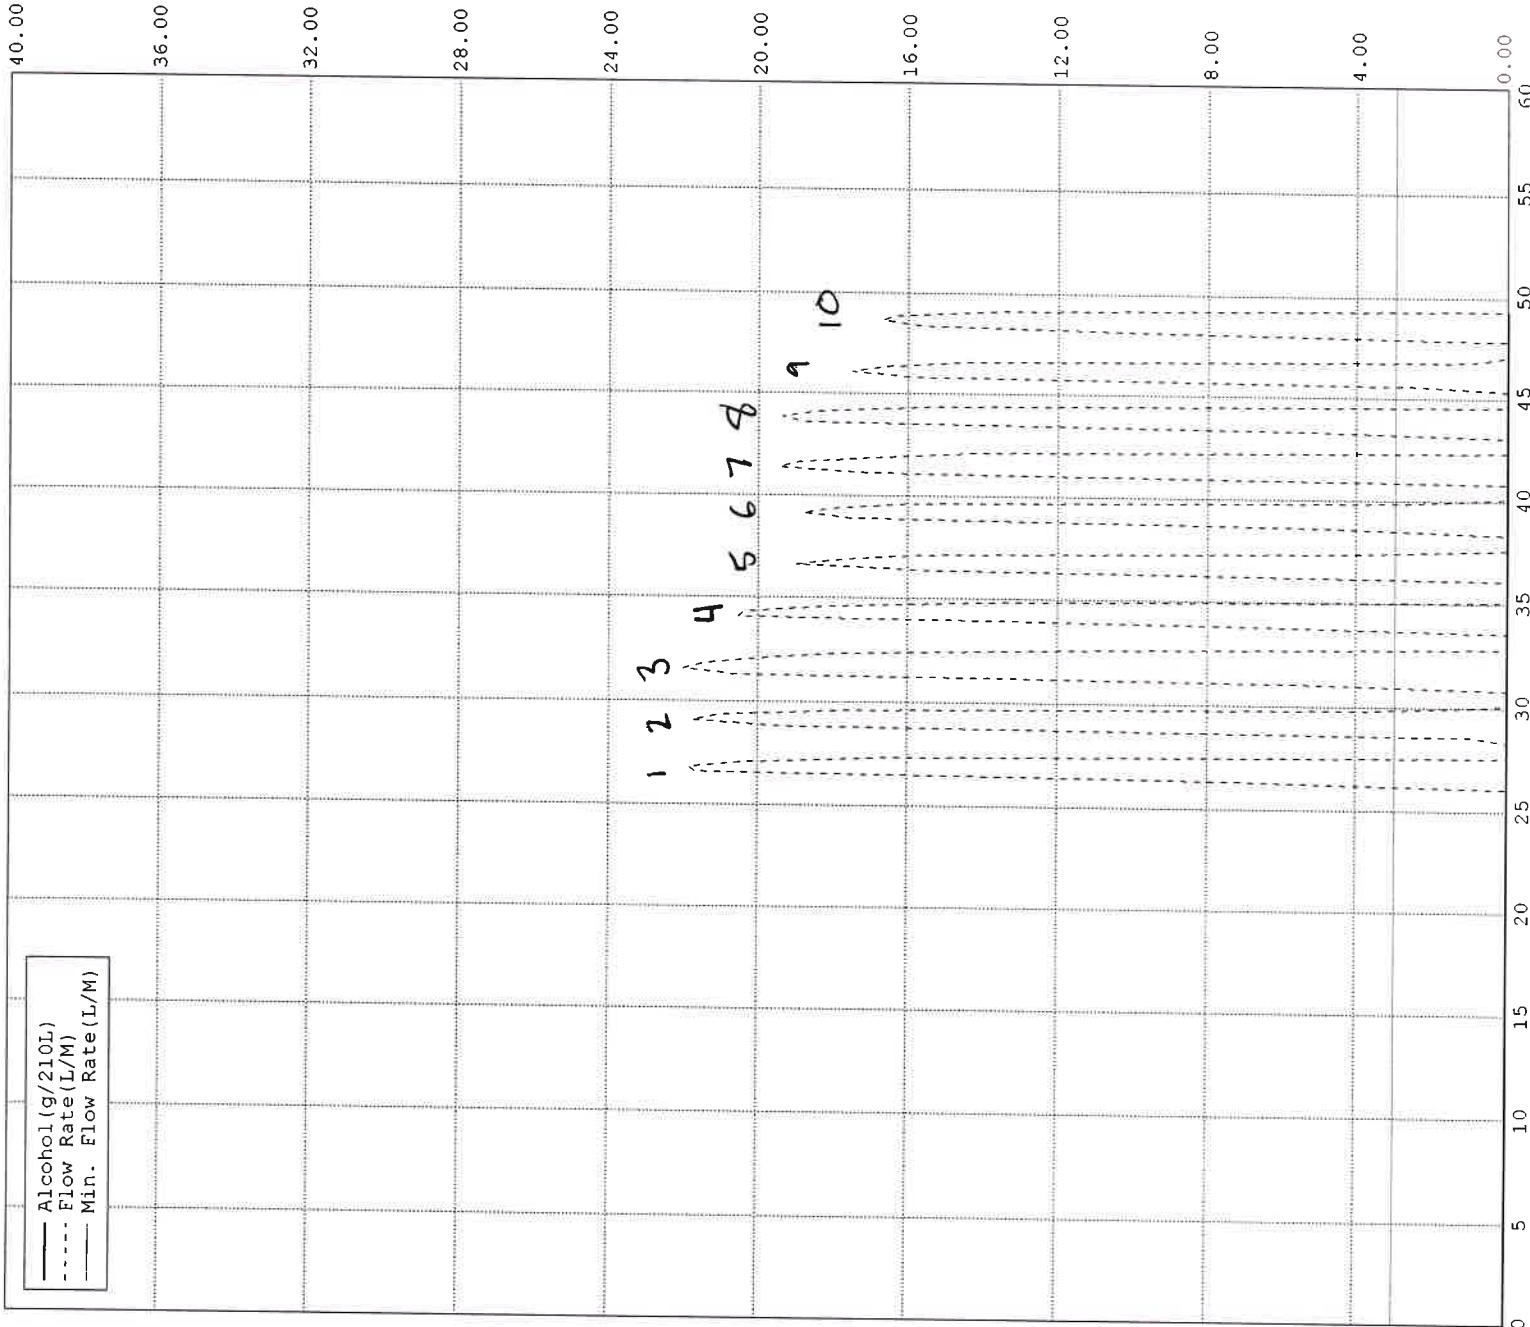

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 11/21/2024
Time: 12:15:17

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747


DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.11: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:16
BLANK TEST	0.000	12:16
INTERNAL STANDARD	VERIFIED	12:16
EXTERNAL STANDARD	0.081	12:16
BLANK TEST	0.000	12:17
SUBJECT SAMPLE	INVALID	12:18

MNC

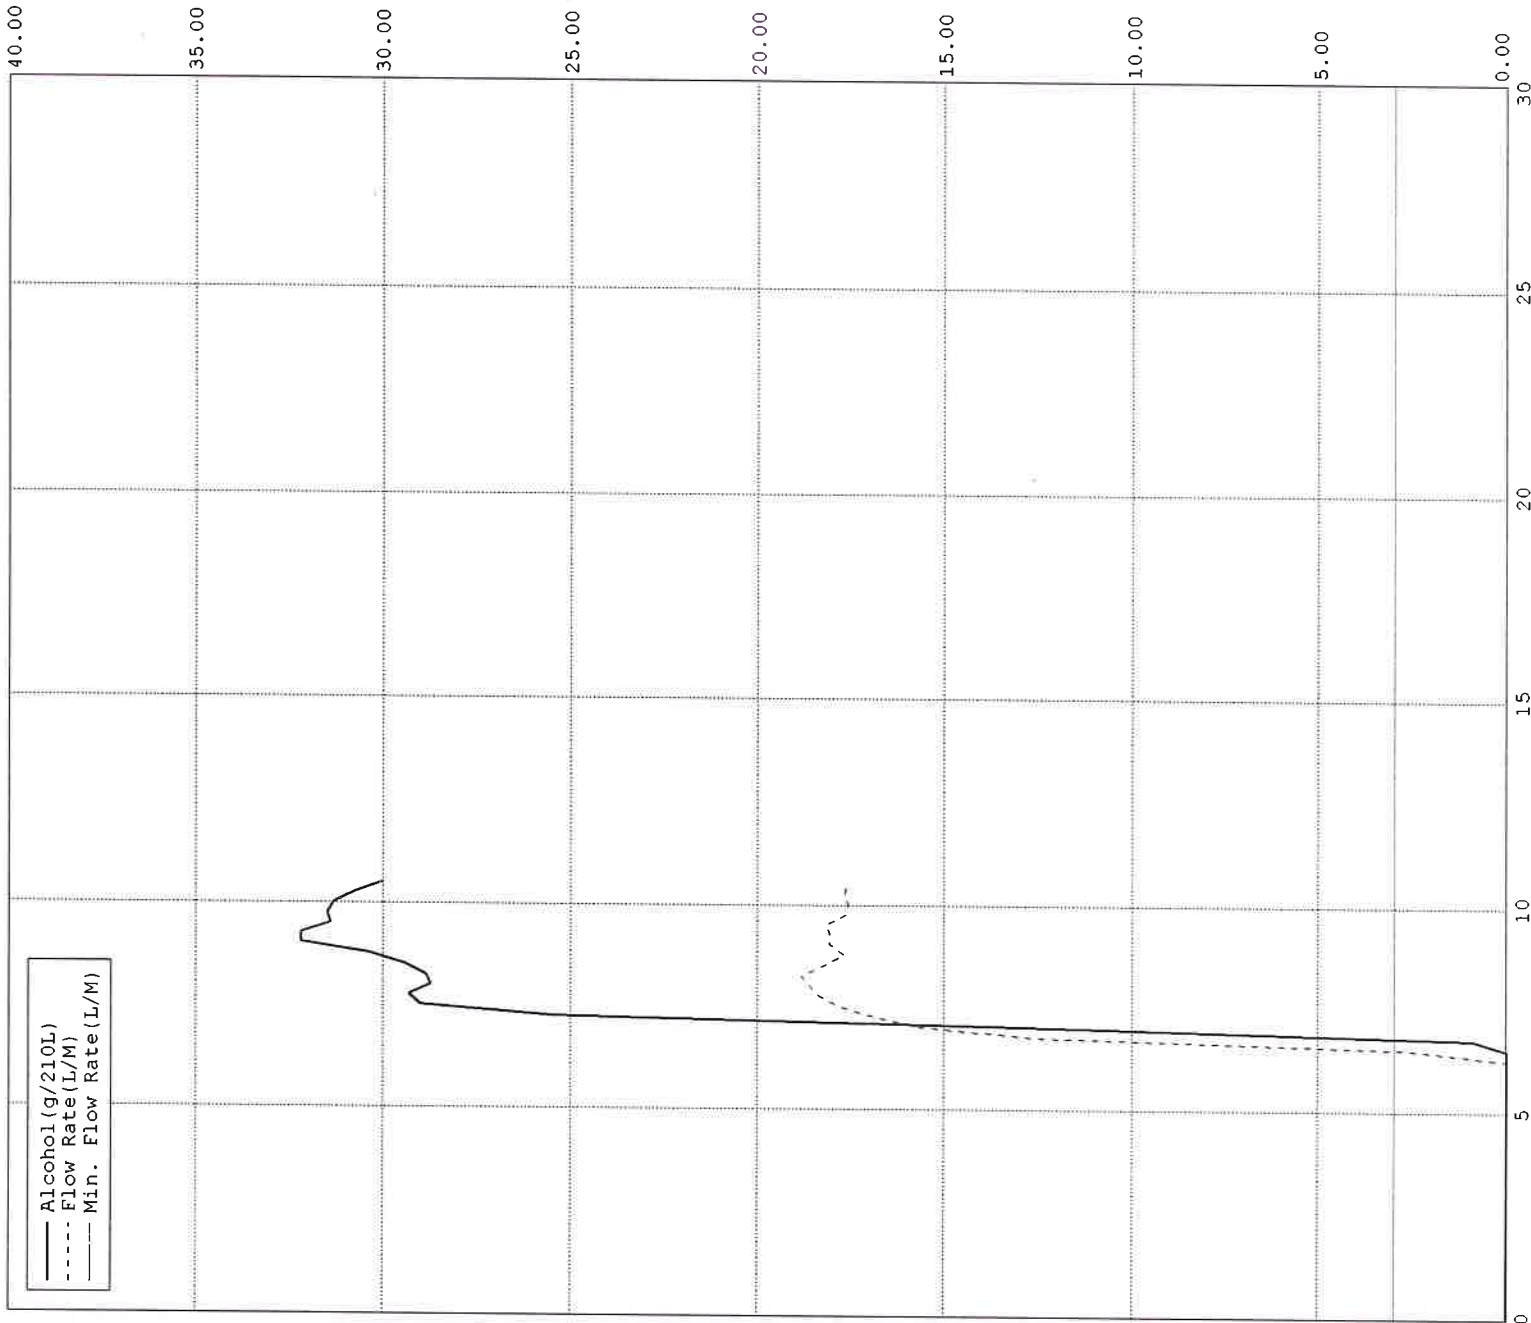

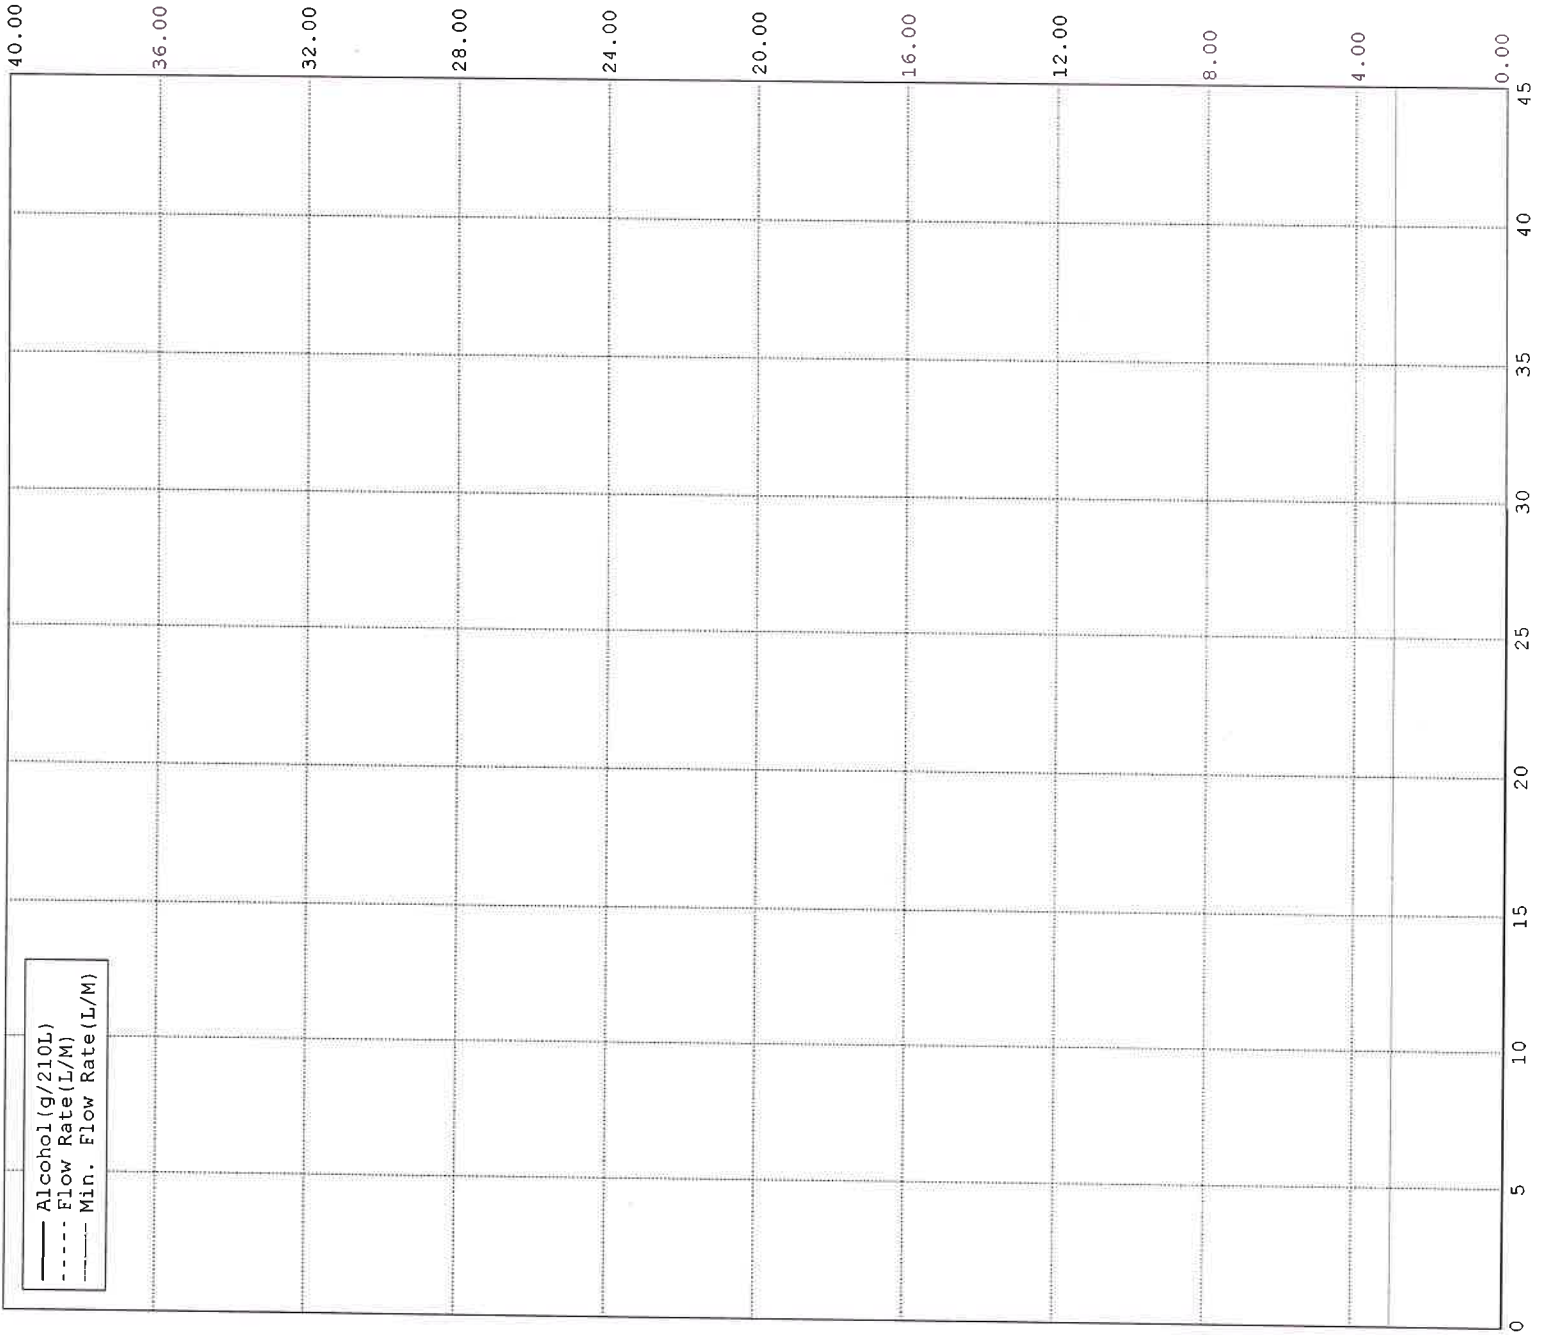

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 11/21/2024
Time: 12:19:59

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
RFI

CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.10: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
PASSED 12:21
0.000 12:21
VERIFIED 12:21
0.080 12:21
0.000 12:22

RFI DETECTED

MNC

SUBJECT TEST

Alaska Department of Public Safety

DATAMASTER dmt: 100406

Date: 11/21/2024

Time: 13:16:49

SUBJECT NAME:

TEST TEST

LICENSE #: XXX

OPERATOR NAME:

MEGAN CARLOCK

OPERATOR'S #: 10747

DEPT/AGENCY:

INTERFERENCE - ACETONE

CASE/REPORT: XXX

TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080

TARGET AT 30.10: 0.080

LOT #: AG335202

EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK

BLANK TEST

INTERNAL STANDARD

Xq = 0.085 (0.20%)

EXTERNAL STANDARD

X[1] = 0.0801 (-0.0016) (0.0015)

BLANK TEST

SUBJECT SAMPLE

X[1] = 0.1110 (-0.0214) (0.0002)

Interference Detected


Filter 2 Average: -0.0018

Filter 3 Average: 0.0014

MNC 11/21/24

MNC

Alcohol (g/210L)
Flow Rate (L/M)
Min. Flow Rate (L/M)

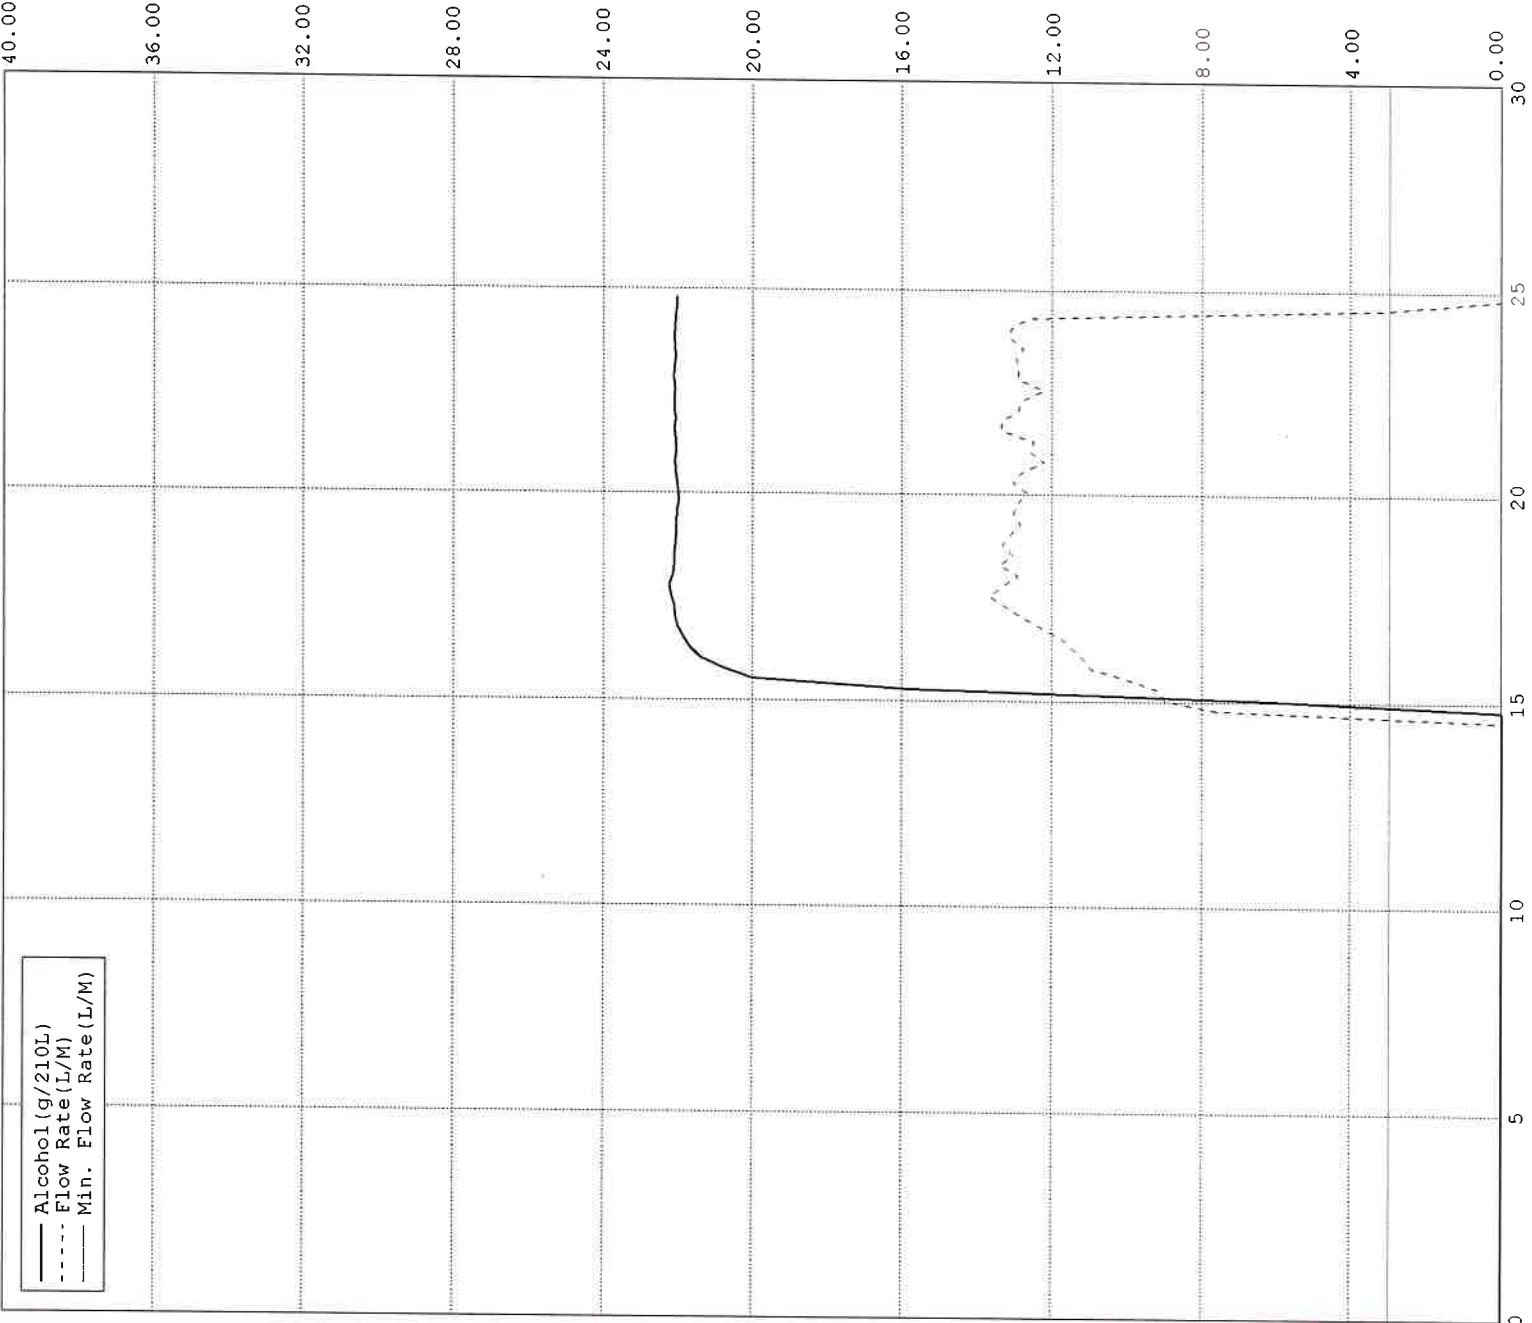



SUBJECT TEST	
Alaska Department of Public Safety DATAMASTER dmt: 100406	
Date: 11/21/2024 Time: 13:10:36	
SUBJECT NAME: TEST TEST LICENSE #: XXX	
OPERATOR NAME: MEGAN CARLOCK OPERATOR'S #: 10747	
DEPT/AGENCY: INTERFERENCE - IPA CASE/REPORT: XXX TEST TYPE: TEST	
EXTERNAL STANDARD INFORMATION NOMINAL: 0.080 TARGET AT 30.10: 0.080 LOT #: AG335202 EXPIRATION: 12/18/2025	
DIAGNOSTIC CHECK BLANK TEST INTERNAL STANDARD Xq = 0.086 (0.72%) EXTERNAL STANDARD X[1] = 0.0805 (-0.0022) BLANK TEST SUBJECT SAMPLE X[1] = 0.1196 (-0.0295)	PASSED 13:11 0.000 13:11 VERIFIED 13:11 0.080 13:12 (0.0011) 0.000 13:13 XXX 13:13 (0.0011)
Interference Detected	

MNC

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 11/21/2024
Time: 13:03:30

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.10: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:04
BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:05
Xq = 0.085 (0.51%)	0.080	13:05
EXTERNAL STANDARD	X[1] = 0.0800 (-0.0016)	(0.0020)
BLANK TEST	0.000	13:06
SUBJECT SAMPLE (Vol=1.81L)	0.096	13:06
X[1] = 0.0968 (-0.0017)	(0.0003)	
BLANK TEST	0.000	13:07
EXTERNAL STANDARD	0.080	13:07
X[1] = 0.0799 (-0.0019)	(0.0009)	
BLANK TEST	0.000	13:08

MNC

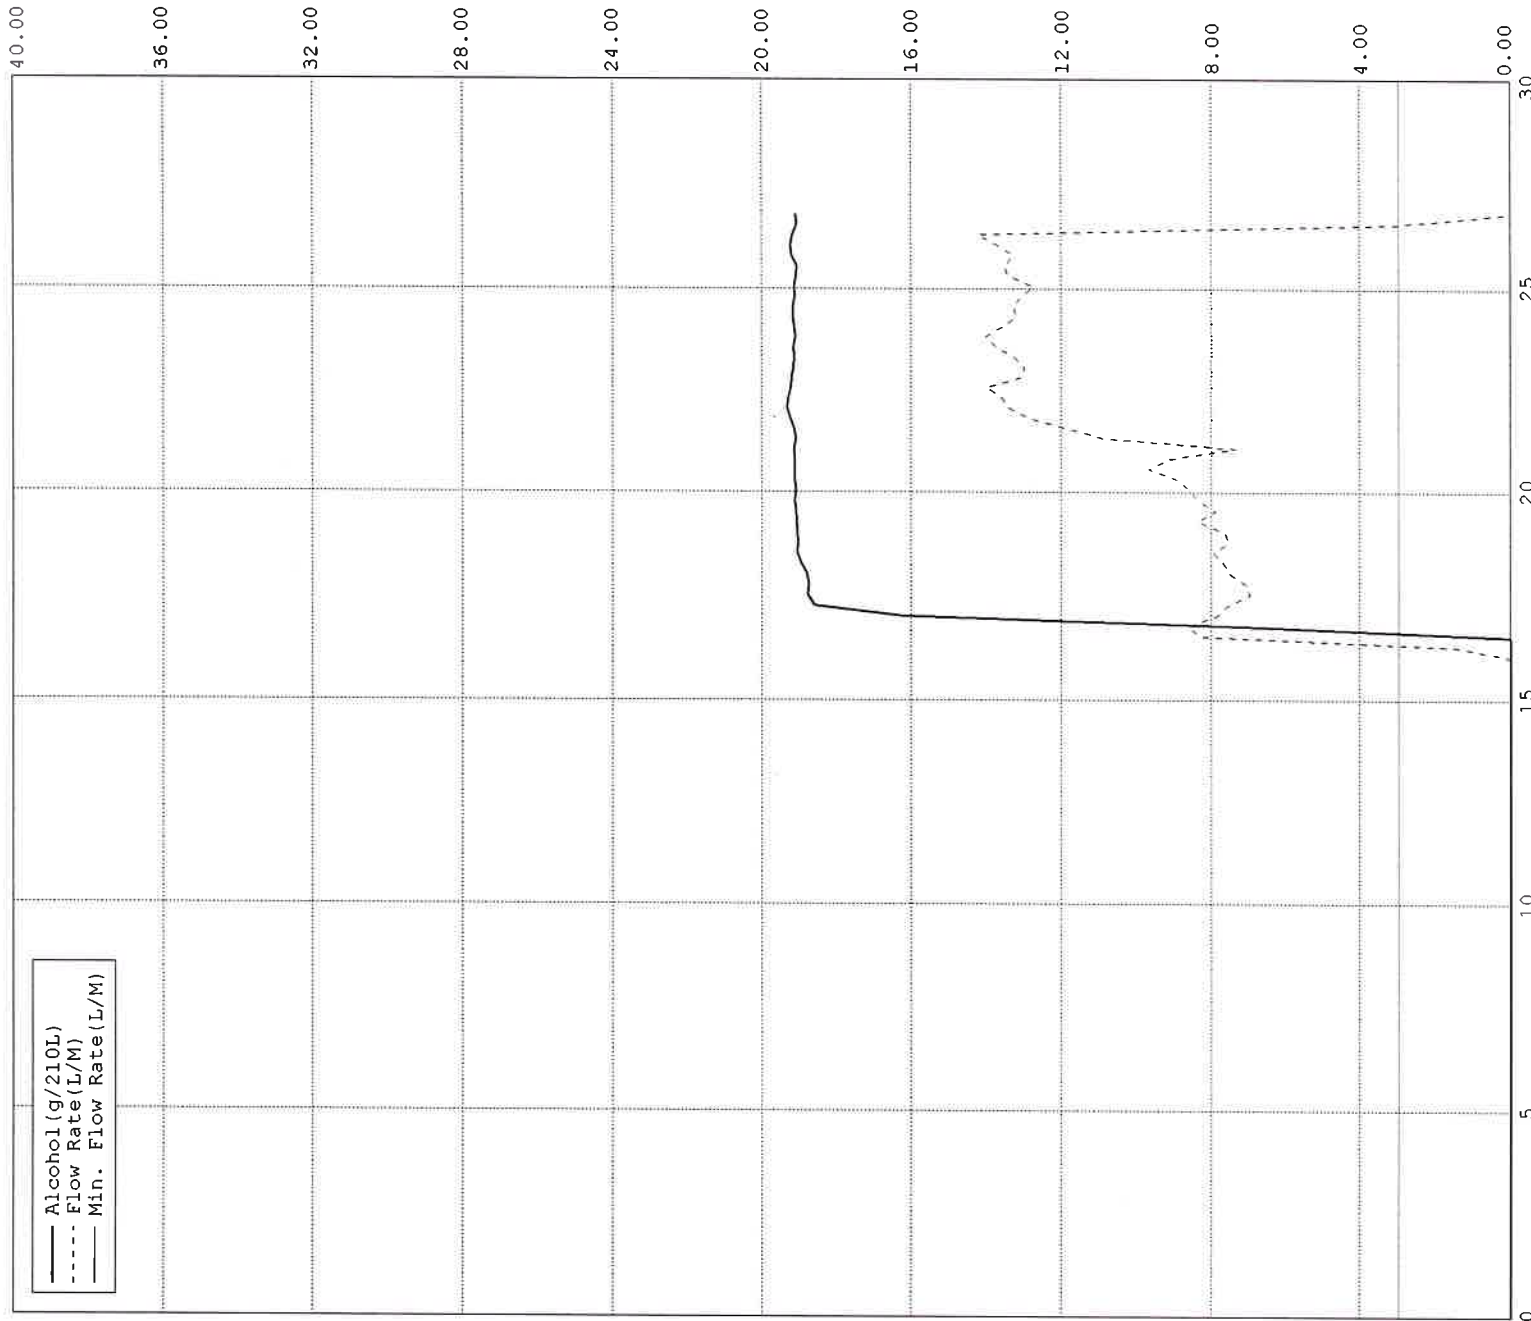

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100406

Date: 11/21/2024
Time: 13:48:11

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
MEGAN CARLOCK
OPERATOR'S #: 10747

DEPT/AGENCY:
NON-DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 30.08: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:49
BLANK TEST	0.000	13:49
INTERNAL STANDARD	VERIFIED	13:49
EXTERNAL STANDARD	0.081	13:49
BLANK TEST	0.000	13:50
SUBJECT SAMPLE (Vol=2.74L)	0.000	13:51
BLANK TEST	0.000	13:52
EXTERNAL STANDARD	0.081	13:52
BLANK TEST	0.000	13:53

MNC

