



State of Alaska  
 Department of Public Safety  
**Scientific Crime Detection Laboratory**

4805 Dr. Martin Luther King Jr. Ave.  
 Anchorage, Alaska 99507  
 David Kanaris, Chief, Forensic Laboratories



**Breath Alcohol Calibration Report**  
**Calibration Item:** DataMaster DMT  
**Serial Number:** 100697

**Report Issue Date:** 10/02/2025  
**Date Received:** 2025-05-15  
**Condition of Item:** No apparent damage

**Method Used:** DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual  
**Calibration Range:** 0.020 g/210L - 0.300 g/210L

As-Found Data								
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.021	0.020	0.020	0.020
0.080	0.079	AG335202	0.078	0.078	0.078	0.079	0.078	0.078
0.300	0.298	AG427706	0.295	0.293	0.294	0.294	0.294	0.294

As Found - Evaluation Analyst: Carlie Glaister

As Found Conditions - Barometric Pressure (inHg): 29.74 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 21

As-Found Lab Activity Date Range: 05/22/2025 - 05/22/2025

Adjustment is being recommended due to previous internal standard errors while in the field. During evaluation no internal standard errors were experienced. Reset options due to duplicate subject test printing.

As-Left Data									
Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.019	AG408002	0.020	0.020	0.020	0.019	0.020	0.020	+/- 0.002
0.040	0.039	AG407908	0.039	0.039	0.038	0.039	0.040	0.039	+/- 0.003
0.080	0.078	AG335202	0.078	0.078	0.077	0.078	0.078	0.078	+/- 0.004
0.100	0.097	AG333401	0.098	0.098	0.098	0.098	0.098	0.098	+/- 0.004
0.150	0.146	AG332004	0.144	0.144	0.144	0.144	0.144	0.144	+/- 0.006
0.300	0.292	AG427706	0.290	0.290	0.290	0.290	0.290	0.290	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.14 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 40

As-Left Lab Activity Date Range: 09/22/2025 - 09/23/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

**This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.**

Results authorized by Kaija Swisher on 09/23/2025

[kaija.swisher@alaska.gov](mailto:kaija.swisher@alaska.gov)

Technically and administratively reviewed by Derek Walton on 10/02/2025

# Alaska Scientific Crime Detection Laboratory

## DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 160697 Analyst or Technician Name: Kaija Swisher

DataMaster DMT Calibration Start Date: 9/22/25

### Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value  $\leq$  3.00%

### Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
  - Lamp (2.60 V Maximum)
  - Bias
  - Cooler (2.00 V Maximum)
  - Chopper Frequency
  - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer  
Barometer/Thermometer/Hygrometer S/N: 240680771  
Calibration Due Date: 9/10/26
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

### Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.4L liters (1.3 L to 1.7 L)

### As Left Linearity Testing

Barometric Pressure (in Hg) 29.14 Temperature(C) 22.3 Relative Humidity(%) 40

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

### Functional Tests

- Incomplete
- Invalid
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)
- Interference (Volatiles) – *Print with View Details*

1. Acetone Reagent Lot Number: 20250922KS Expiration Date: 12/22/25  
Simulator S/N: DR4178 Thermometer Verification Performed?
2. Isopropanol Reagent Lot Number: 20250922KS Expiration Date: 12/22/25  
Simulator S/N: DR4177 Thermometer Verification Performed?
3. Negative (Ethanol Only) Lot Number: 25CP41280 Expiration Date: 12/22/25/3/19/27  
Simulator S/N: DR4163 Thermometer Verification Performed?  (Solvent)

Calibrated External Thermometer S/N: 250159297

Calibration Due Date: 3/14/27

### Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

### Completion

Lab Work End Date: 9/22/25

Data Interpretation Date (Technician): NA (if applicable)

Data Interpretation Date (Analyst): 9/23/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 09:36:30

VERSIONS

DMT: 3.02  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.8°C PASSED  
(44.0°C - 52.0°C)  
Breath Tube = 46.2°C PASSED  
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.70 V PASSED  
(1.02 V - 2.38 V)  
Cooler Voltage = 1.69 V PASSED  
(1.01 V - 2.37 V)  
Bias Voltage = 80 V PASSED  
(48 V - 112 V)  
Chopper Freq = 512 Hz PASSED  
(475 Hz - 575 Hz)  
Barometer = 29.1 in

PUMP INFO

Flow Rate = 4.073 L/M PASSED  
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED  
(0.002 v <= 0.010 v)  
PUMP OFF PASSED  
(0.002 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD

Xq = 0.081 1.06% (0.00% - 4.00%) PASSED

Technician Screen

-----  
DATAMASTER dmt: 100697  
-----

Date: 09/22/2025

Time: 10:34 AM

Temperatures (°C)

Sample Cell: 48.8°C

Breath Tube: 46.8°C

Current Barometer 29.1 in

Volume (Ltr) 1.54

Settings

Lamp: 1.76 V

Bias: 80 V

Cooler: 1.58 V

Chopper: 517 Hz

Voltages (V)

Flow: 1.05 V

Detector: -0.018 V

CALIBRATION FACTORS

-----  
Alaska Department of Public Safety  
DATAMASTER dmt: 100697  
-----

Date: 06/16/2025  
Time: 12:51:09

OPERATOR NAME:  
DEREK WALTON  
CERTIFICATE #: 9508

Ca = 0.1000  
CAL = 1.015351    0.800 <= CAL < 1.200  
b1 = 0.0007    0.0000 <= b1 < 0.0040  
b2 = 0.0042    0.0010 <= b2 < 0.0100  
b3 = 0.0007    0.0000 <= b3 < 0.0040  
Xq = 0.0820    0.0500 <= Xq < 0.2000  
a21 = 1.130606    1.050 <= a21 < 1.300  
a31 = 0.483977    0.300 <= a31 < 0.800

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 10:55:55

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
MINIMUM VOLUME TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.14: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	10:57
BLANK TEST	0.000	10:57
INTERNAL STANDARD	VERIFIED	10:57
EXTERNAL STANDARD	0.078	10:57
BLANK TEST	0.000	10:58
SUBJECT SAMPLE (Vol=1.52L)	0.000	10:59
BLANK TEST	0.000	11:00
EXTERNAL STANDARD	0.078	11:00
BLANK TEST	0.000	11:01

KS

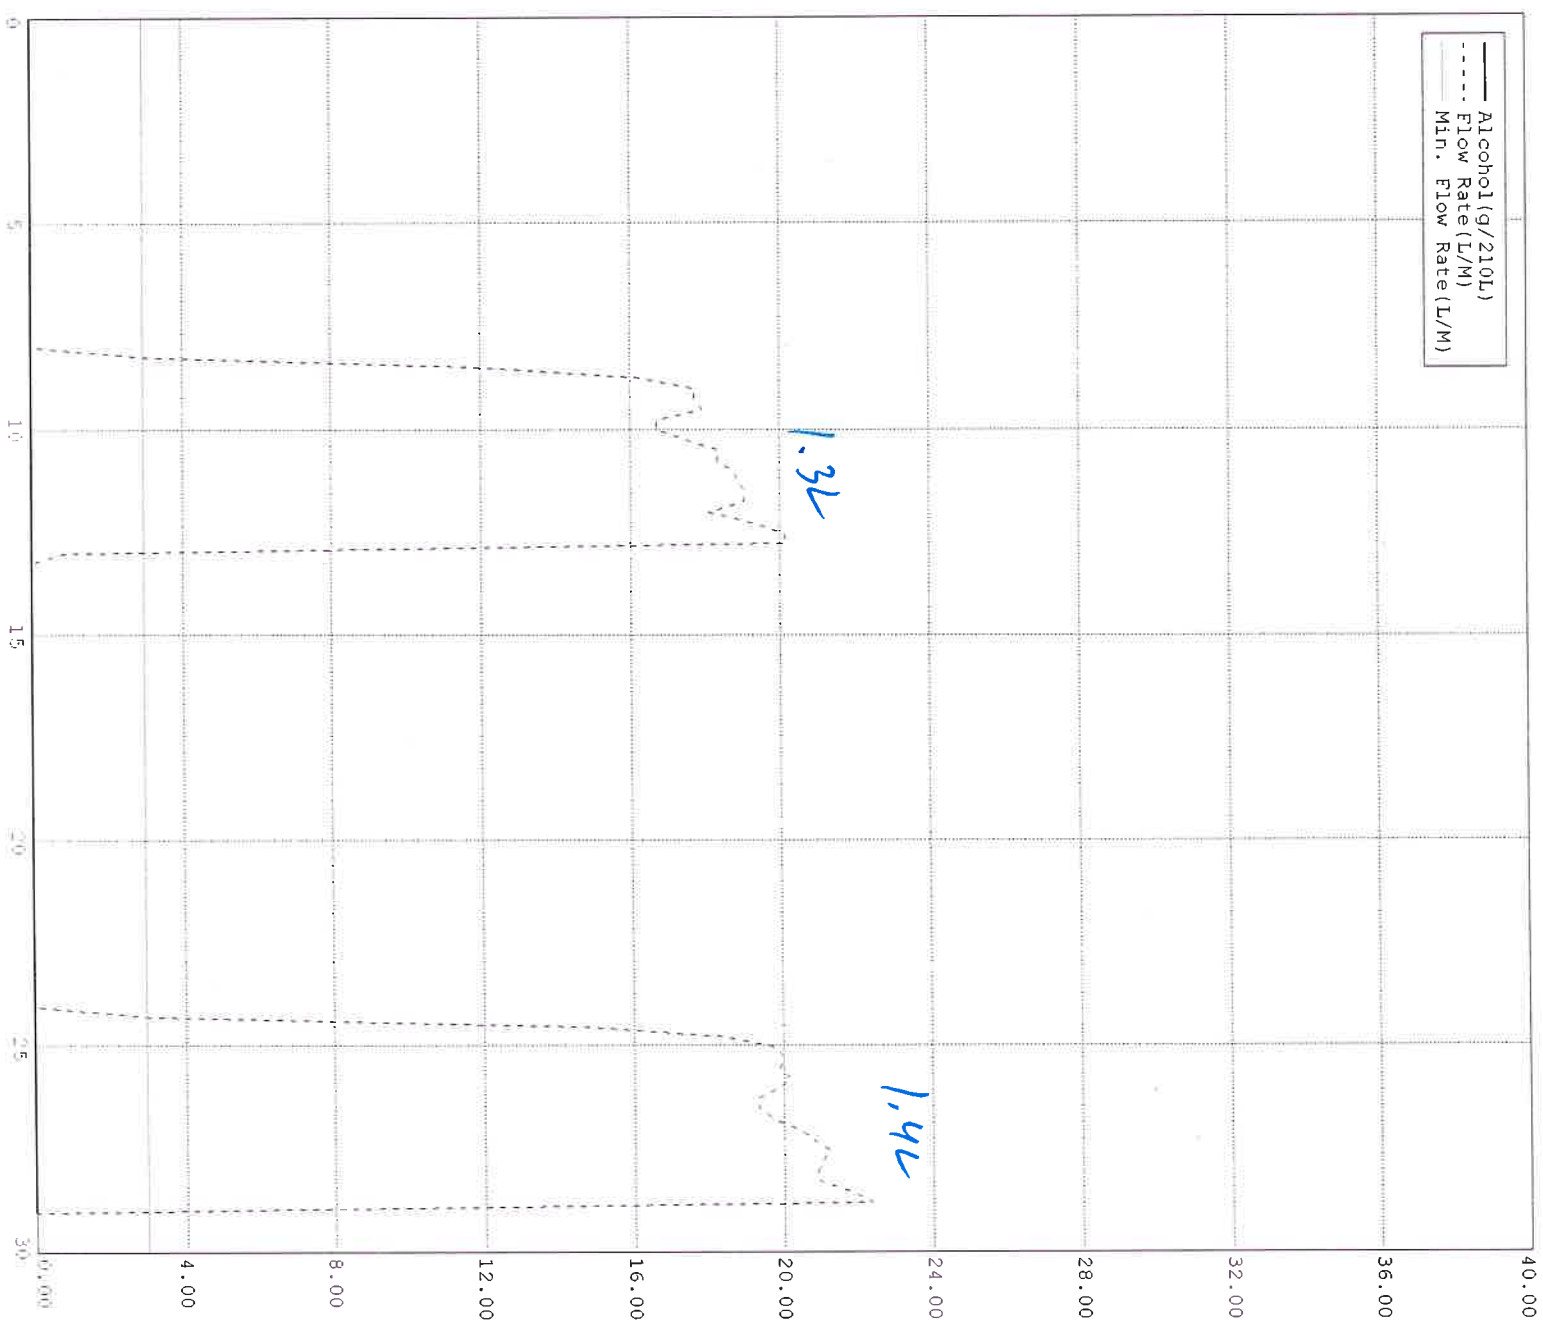

LINEARITY CHECK


Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 11:06:39

SUPERVISOR NAME:  
KAITA SWISHER  
OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.019	0.0198	0.0004
0.039	0.0390	0.0007
0.078	0.0778	0.0004
0.097	0.0980	0.0000
0.146	0.1440	0.0000
0.292	0.2900	0.0000

SLOPE = 0.989553  
R<sup>2</sup> = 0.999929

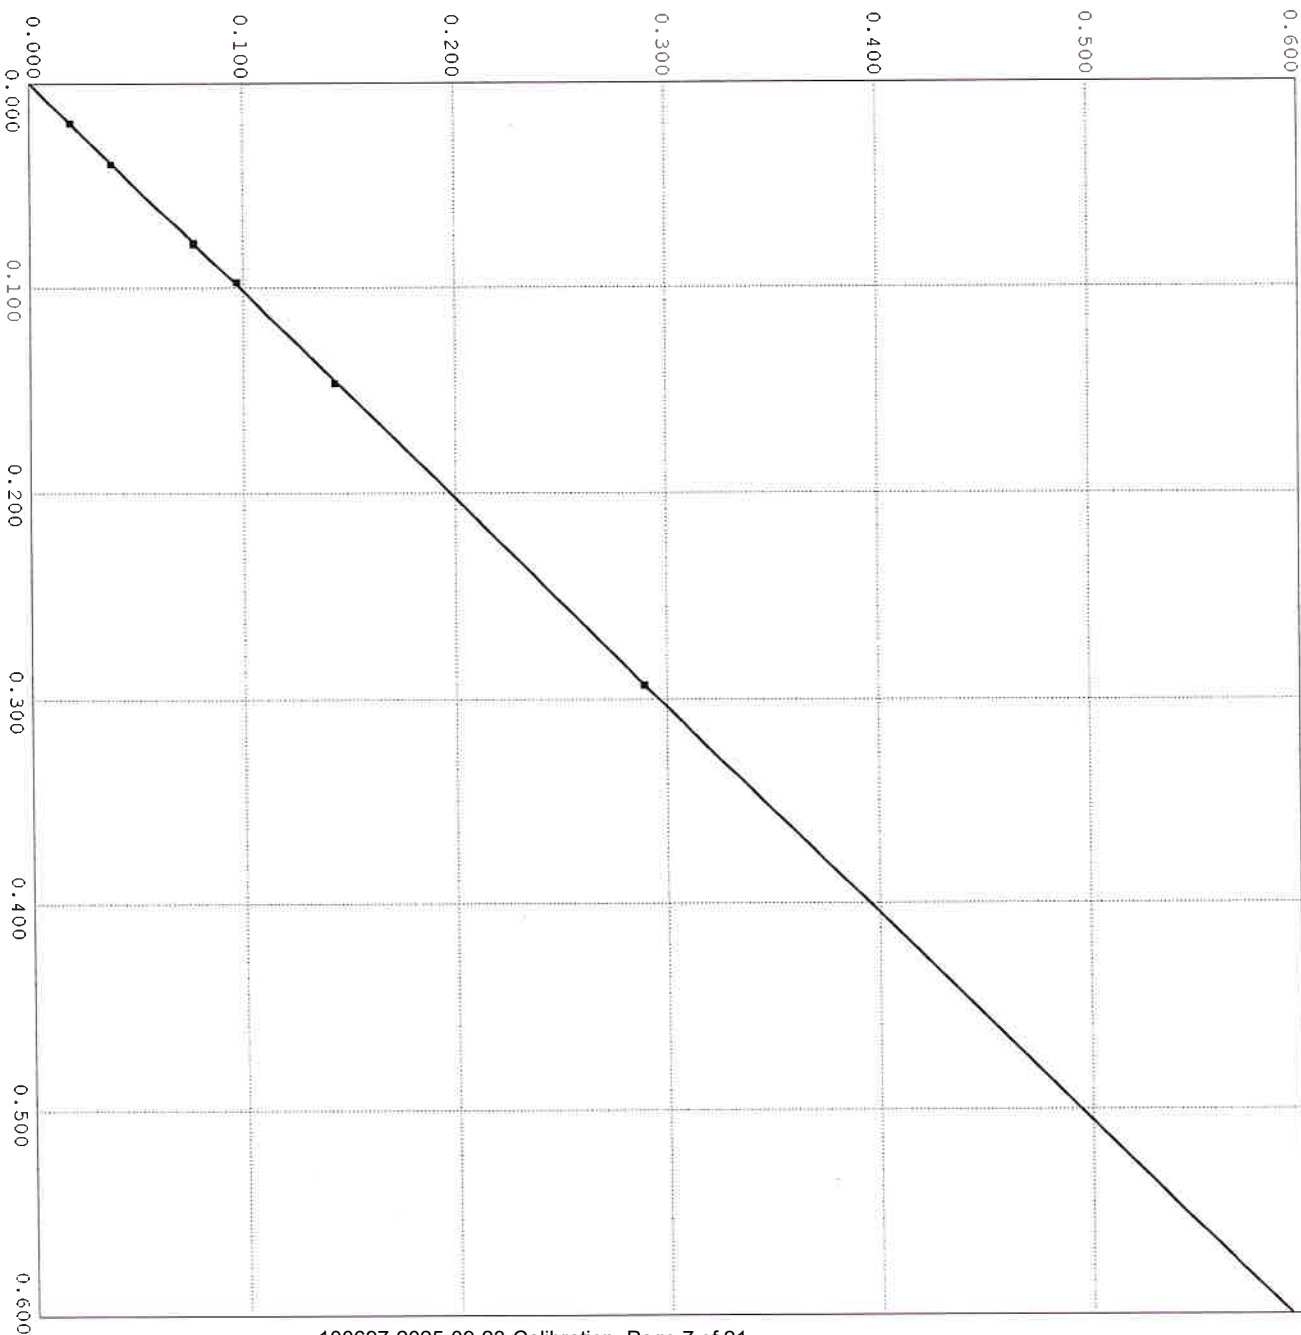

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety  
 DATAMASTER dmt: 100697






Date: 09/22/2025  
 Time: 11:06:42

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020  
 TARGET AT 29.15: 0.019  
 LOT #: AG408002  
 EXPIRATION: 03/20/2026  
 TANK PRESSURE: 455 psi

BLANK TEST	0.000	11:08
INTERNAL STANDARD	VERIFIED	11:08
EXTERNAL STANDARD	0.020	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.020	11:09
BLANK TEST	0.000	11:10
EXTERNAL STANDARD	0.020	11:10
BLANK TEST	0.000	11:11
EXTERNAL STANDARD	0.019	11:11
BLANK TEST	0.000	11:12
EXTERNAL STANDARD	0.020	11:13
BLANK TEST	0.000	11:13

Average = 0.0198  
 Std Dev = 0.0004

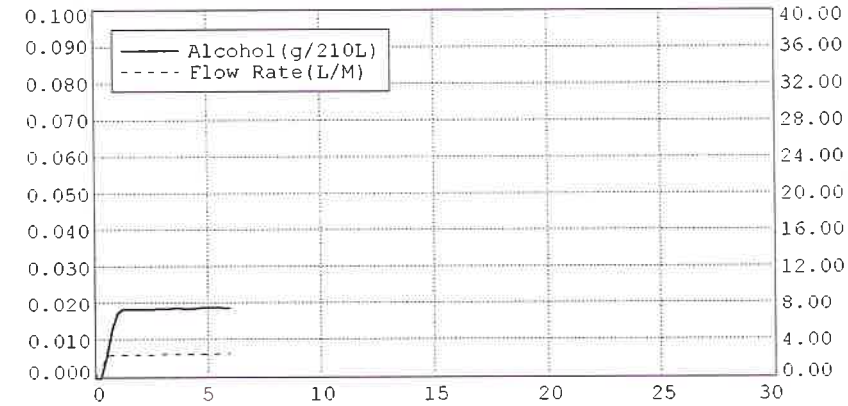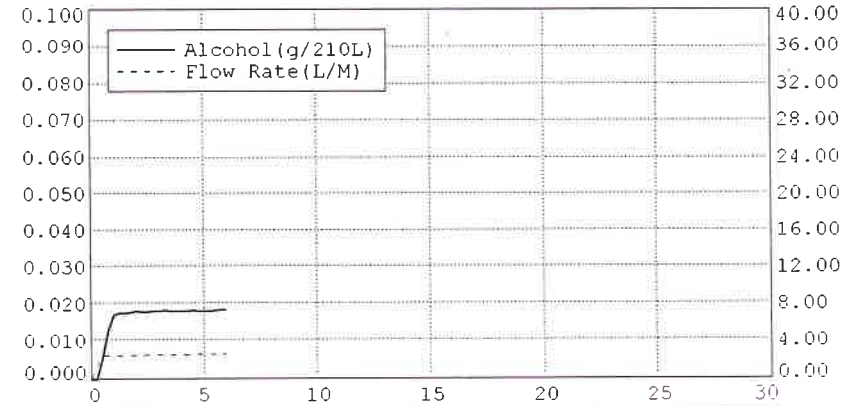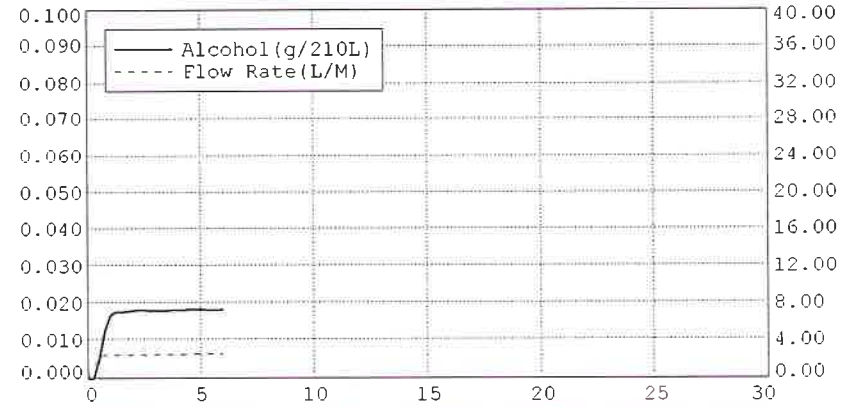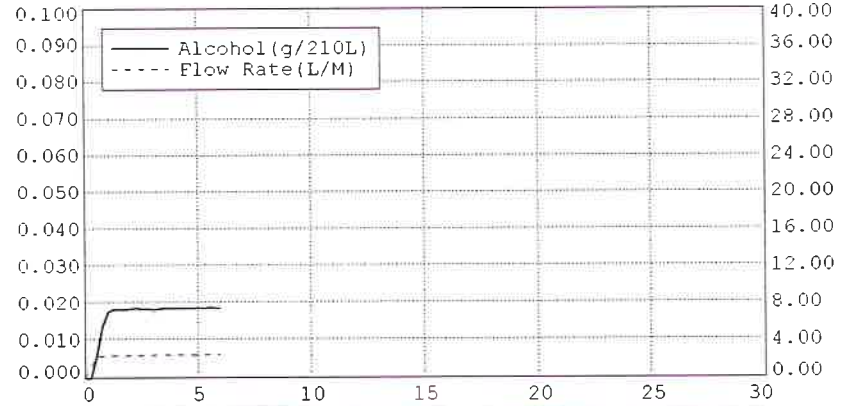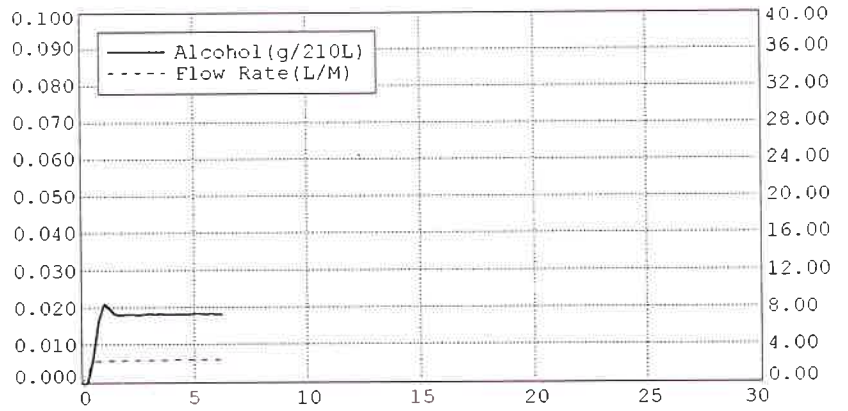



LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety  
 DATAMASTER dmt: 100697






Date: 09/22/2025  
 Time: 11:14:27

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040  
 TARGET AT 29.15: 0.039  
 LOT #: AG407908  
 EXPIRATION: 03/19/2026  
 TANK PRESSURE: 895 psi

BLANK TEST	0.000	11:17
INTERNAL STANDARD	VERIFIED	11:18
EXTERNAL STANDARD	0.039	11:18
BLANK TEST	0.000	11:19
EXTERNAL STANDARD	0.039	11:19
BLANK TEST	0.000	11:20
EXTERNAL STANDARD	0.038	11:20
BLANK TEST	0.000	11:21
EXTERNAL STANDARD	0.039	11:21
BLANK TEST	0.000	11:22
EXTERNAL STANDARD	0.040	11:22
BLANK TEST	0.000	11:23

Average = 0.0390  
 Std Dev = 0.0007

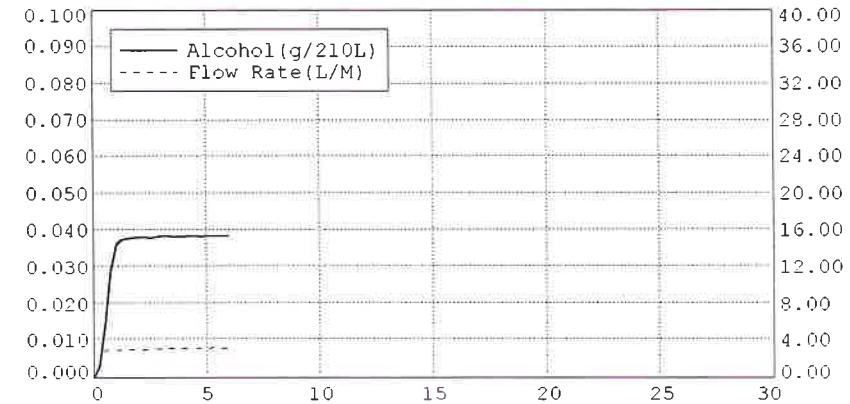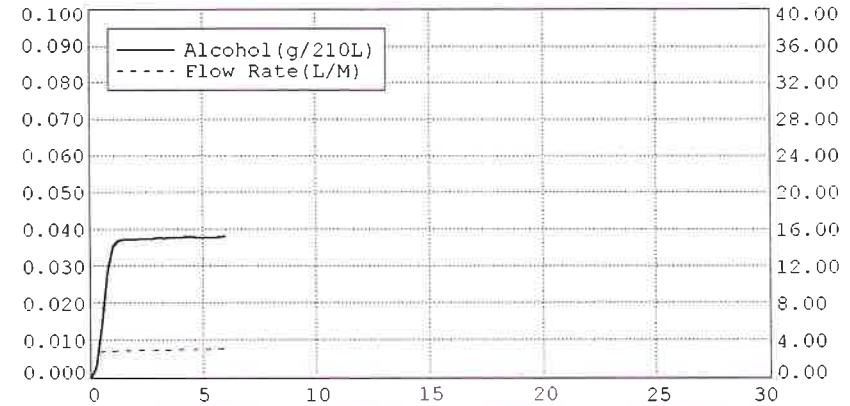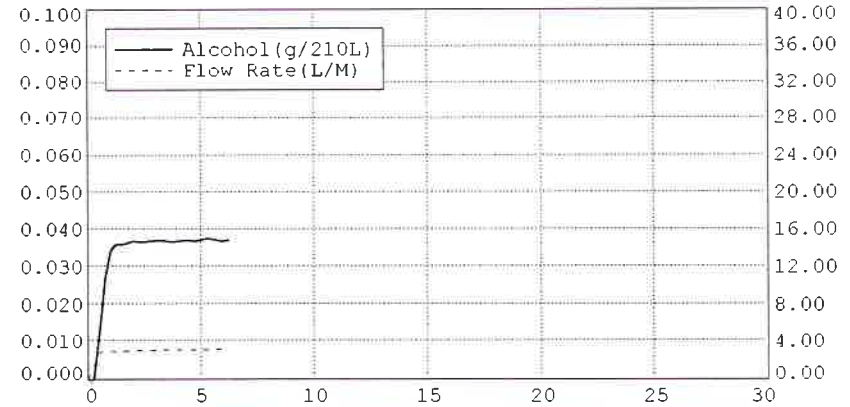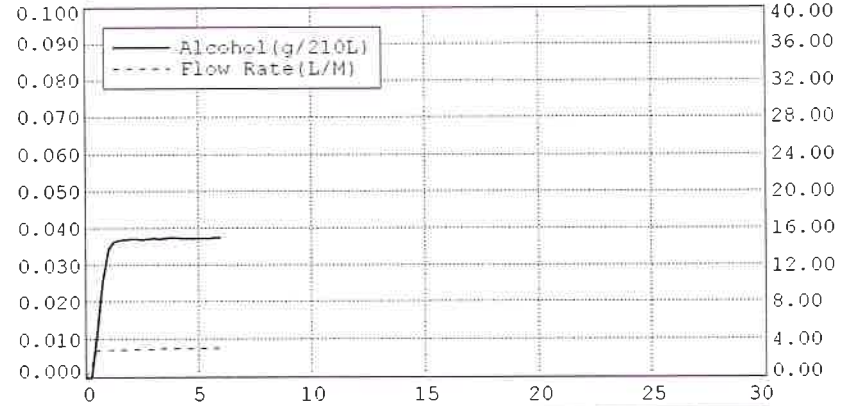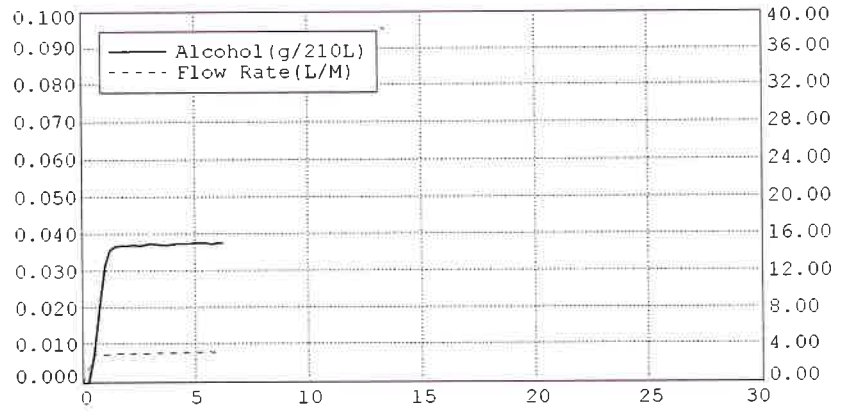

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety  
 DATAMASTER dmt: 100697






Date: 09/22/2025  
 Time: 11:24:12

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
 TARGET AT 29.15: 0.078  
 LOT #: AG335202  
 EXPIRATION: 12/18/2025  
 TANK PRESSURE: 1112 psi

BLANK TEST	0.000	11:25
INTERNAL STANDARD	VERIFIED	11:25
EXTERNAL STANDARD	0.078	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.078	11:26
BLANK TEST	0.000	11:27
EXTERNAL STANDARD	0.077	11:28
BLANK TEST	0.000	11:28
EXTERNAL STANDARD	0.078	11:29
BLANK TEST	0.000	11:30
EXTERNAL STANDARD	0.078	11:30
BLANK TEST	0.000	11:31

Average = 0.0778  
 Std Dev = 0.0004

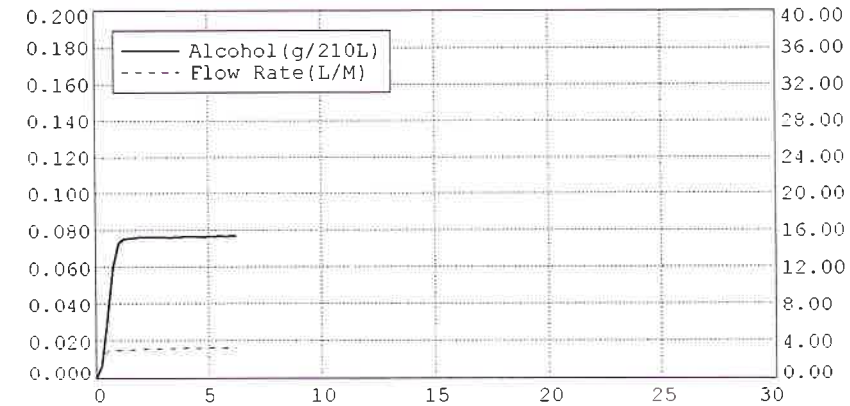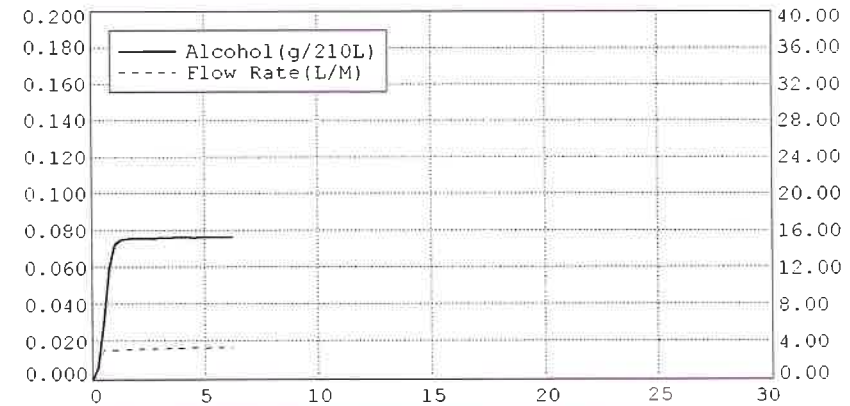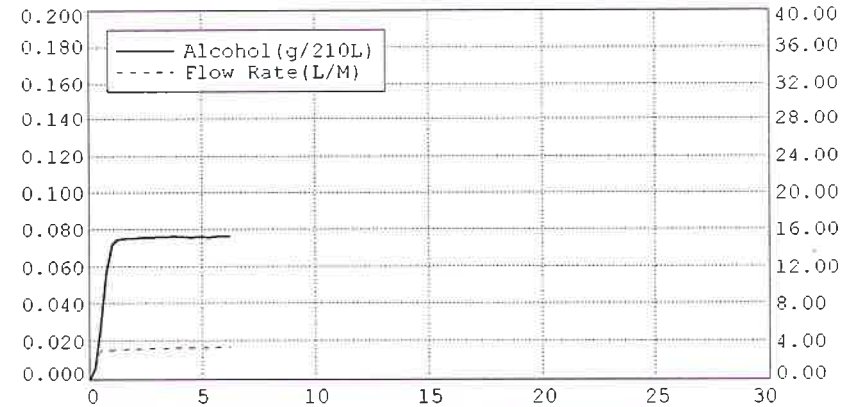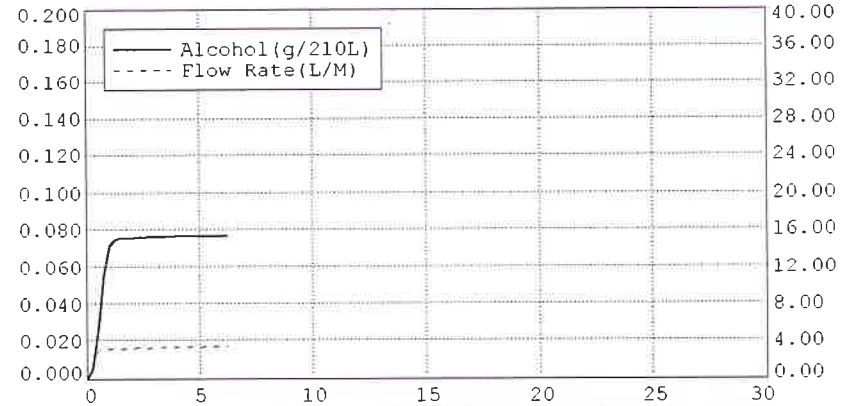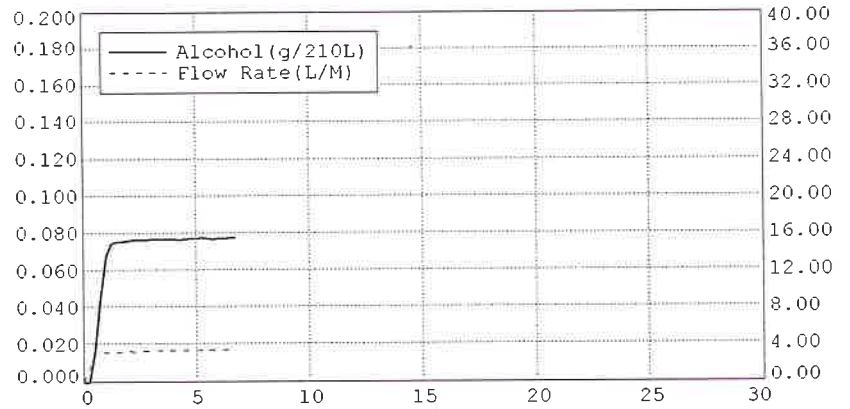

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety  
 DATAMASTER dmt: 100697






Date: 09/22/2025  
 Time: 11:31:56

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100  
 TARGET AT 29.15: 0.097  
 LOT #: AG333401  
 EXPIRATION: 11/30/2025  
 TANK PRESSURE: 900 psi

BLANK TEST	0.000	11:33
INTERNAL STANDARD	VERIFIED	11:33
EXTERNAL STANDARD	0.098	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.098	11:34
BLANK TEST	0.000	11:35
EXTERNAL STANDARD	0.098	11:35
BLANK TEST	0.000	11:36
EXTERNAL STANDARD	0.098	11:36
BLANK TEST	0.000	11:37
EXTERNAL STANDARD	0.098	11:37
BLANK TEST	0.000	11:38

Average = 0.0980  
 Std Dev = 0.0000

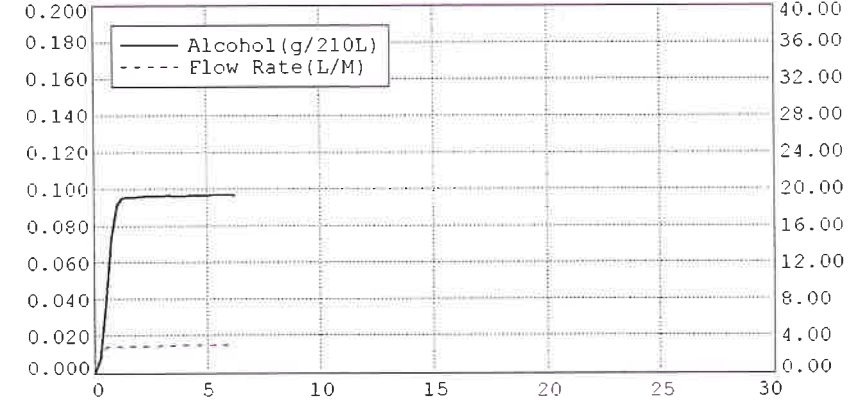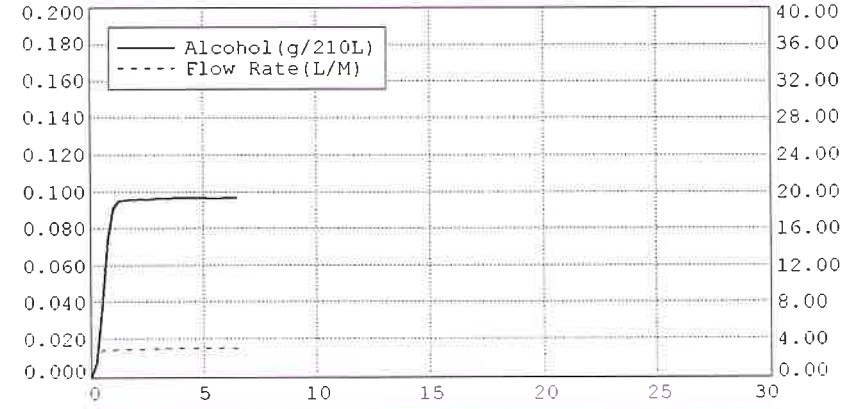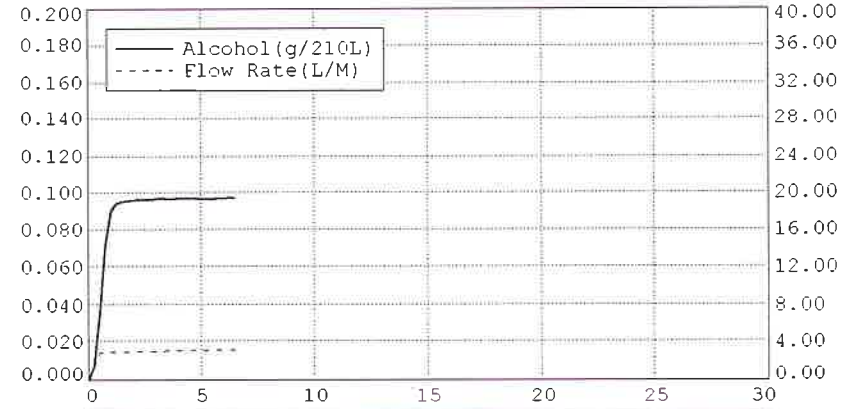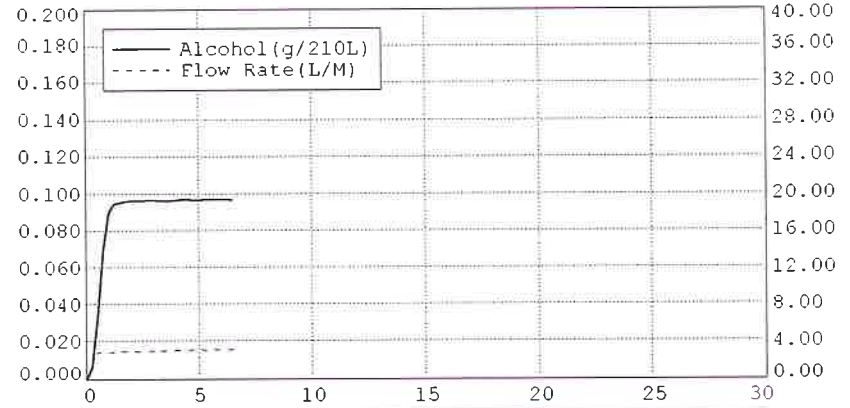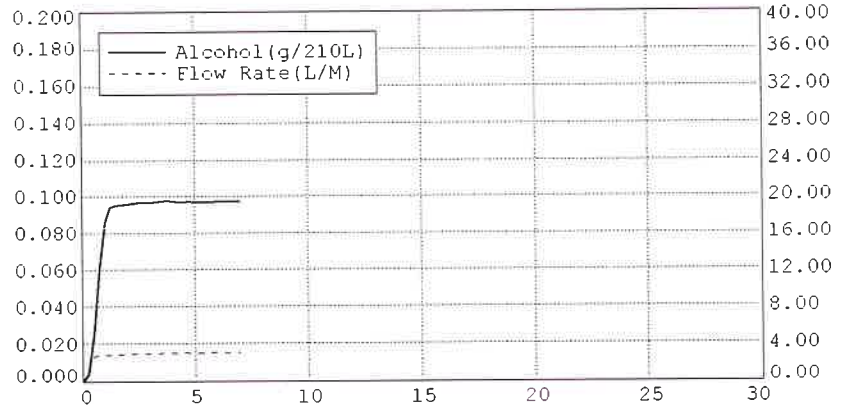

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety  
DATAMASTER dmt: 100697






Date: 09/22/2025  
Time: 11:39:37

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150  
TARGET AT 29.15: 0.146  
LOT #: AG332004  
EXPIRATION: 11/16/2025  
TANK PRESSURE: 408 psi

BLANK TEST	0.000	11:40
INTERNAL STANDARD	VERIFIED	11:41
EXTERNAL STANDARD	0.144	11:41
BLANK TEST	0.000	11:42
EXTERNAL STANDARD	0.144	11:42
BLANK TEST	0.000	11:43
EXTERNAL STANDARD	0.144	11:43
BLANK TEST	0.000	11:44
EXTERNAL STANDARD	0.144	11:44
BLANK TEST	0.000	11:45
EXTERNAL STANDARD	0.144	11:45
BLANK TEST	0.000	11:46

Average = 0.1440  
Std Dev = 0.0000

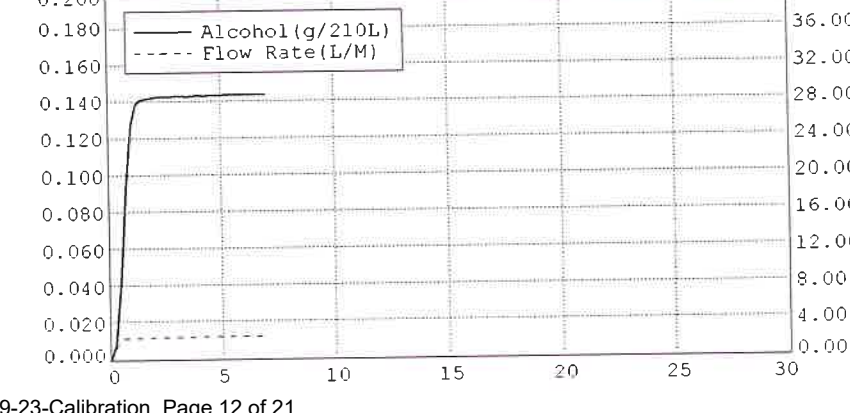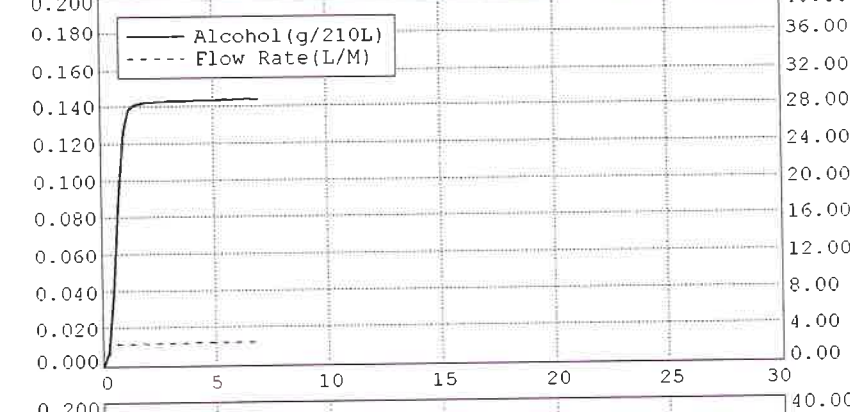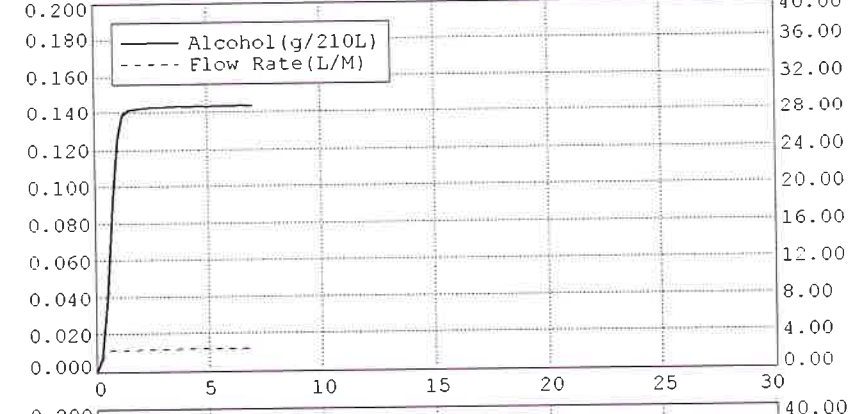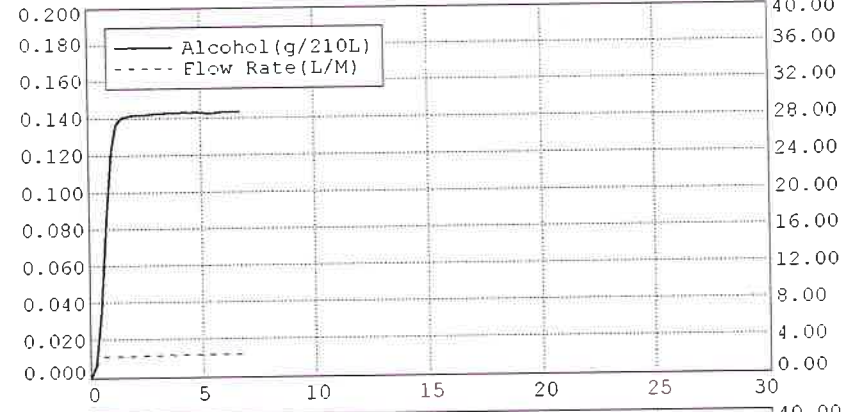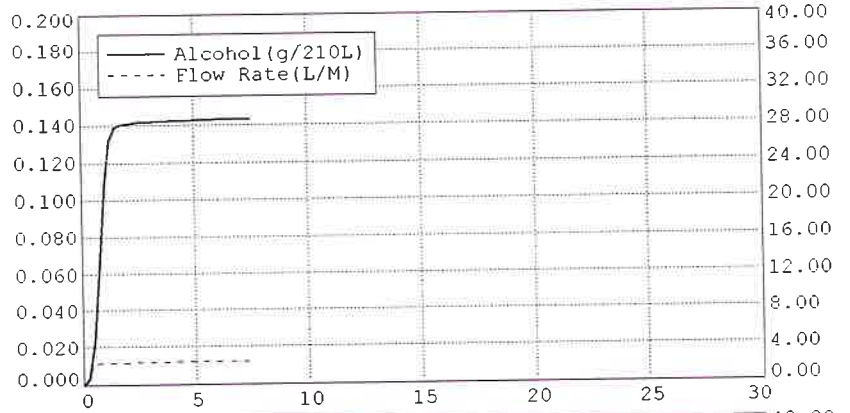

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety  
 DATAMASTER dmt: 100697






Date: 09/22/2025  
 Time: 11:49:31

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300  
 TARGET AT 29.15: 0.292  
 LOT #: AG427706  
 EXPIRATION: 10/03/2026  
 TANK PRESSURE: 341 psi

BLANK TEST	0.000	11:50
INTERNAL STANDARD	VERIFIED	11:51
EXTERNAL STANDARD	0.290	11:51
BLANK TEST	0.000	11:52
EXTERNAL STANDARD	0.290	11:52
BLANK TEST	0.000	11:53
EXTERNAL STANDARD	0.290	11:53
BLANK TEST	0.000	11:54
EXTERNAL STANDARD	0.290	11:54
BLANK TEST	0.000	11:55
EXTERNAL STANDARD	0.290	11:55
BLANK TEST	0.000	11:56

Average = 0.2900  
 Std Dev = 0.0000

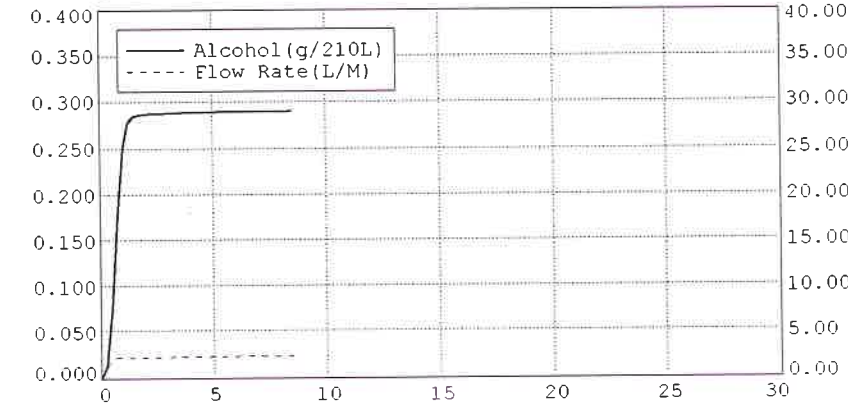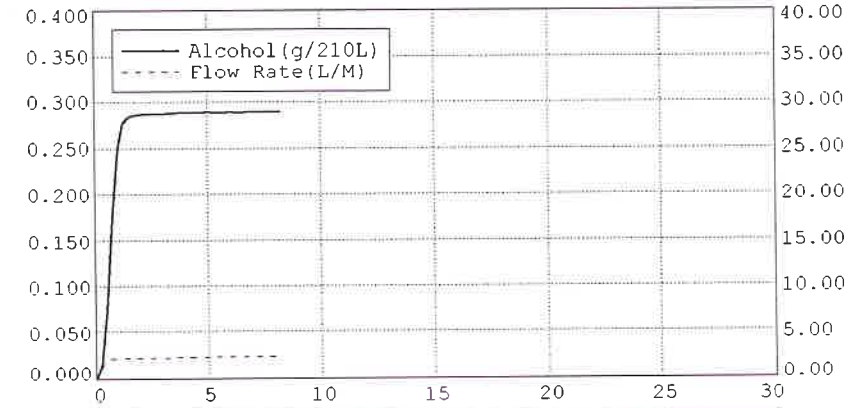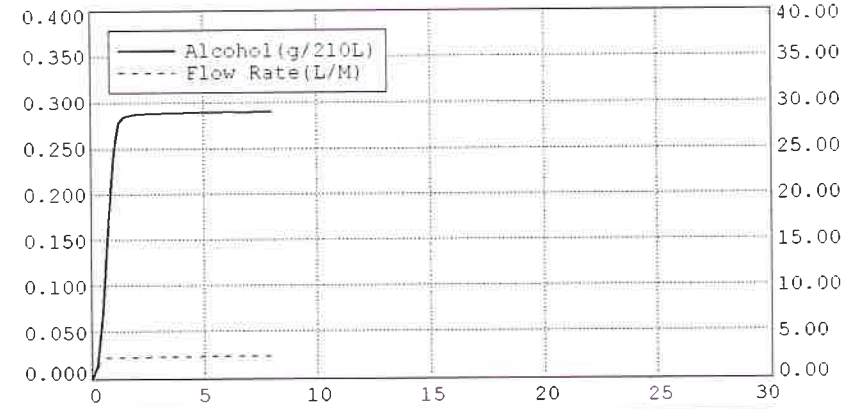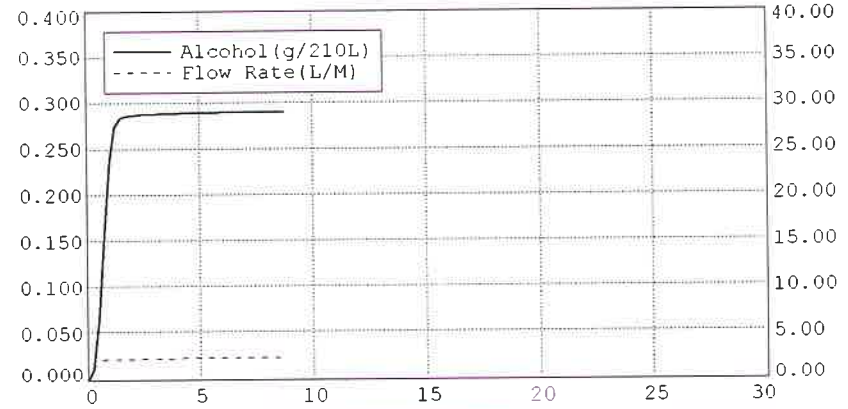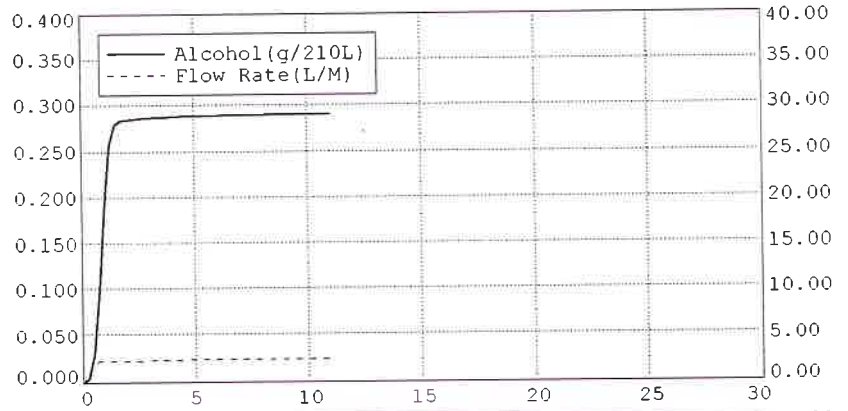

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 12:15:37


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INCOMPLETE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.17: 0.078  
LOI #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:16
BLANK TEST	0.000	12:16
INTERNAL STANDARD	VERIFIED	12:16
EXTERNAL STANDARD	0.078	12:17
BLANK TEST	0.000	12:18
SUBJECT SAMPLE	INCOMPLETE	12:20

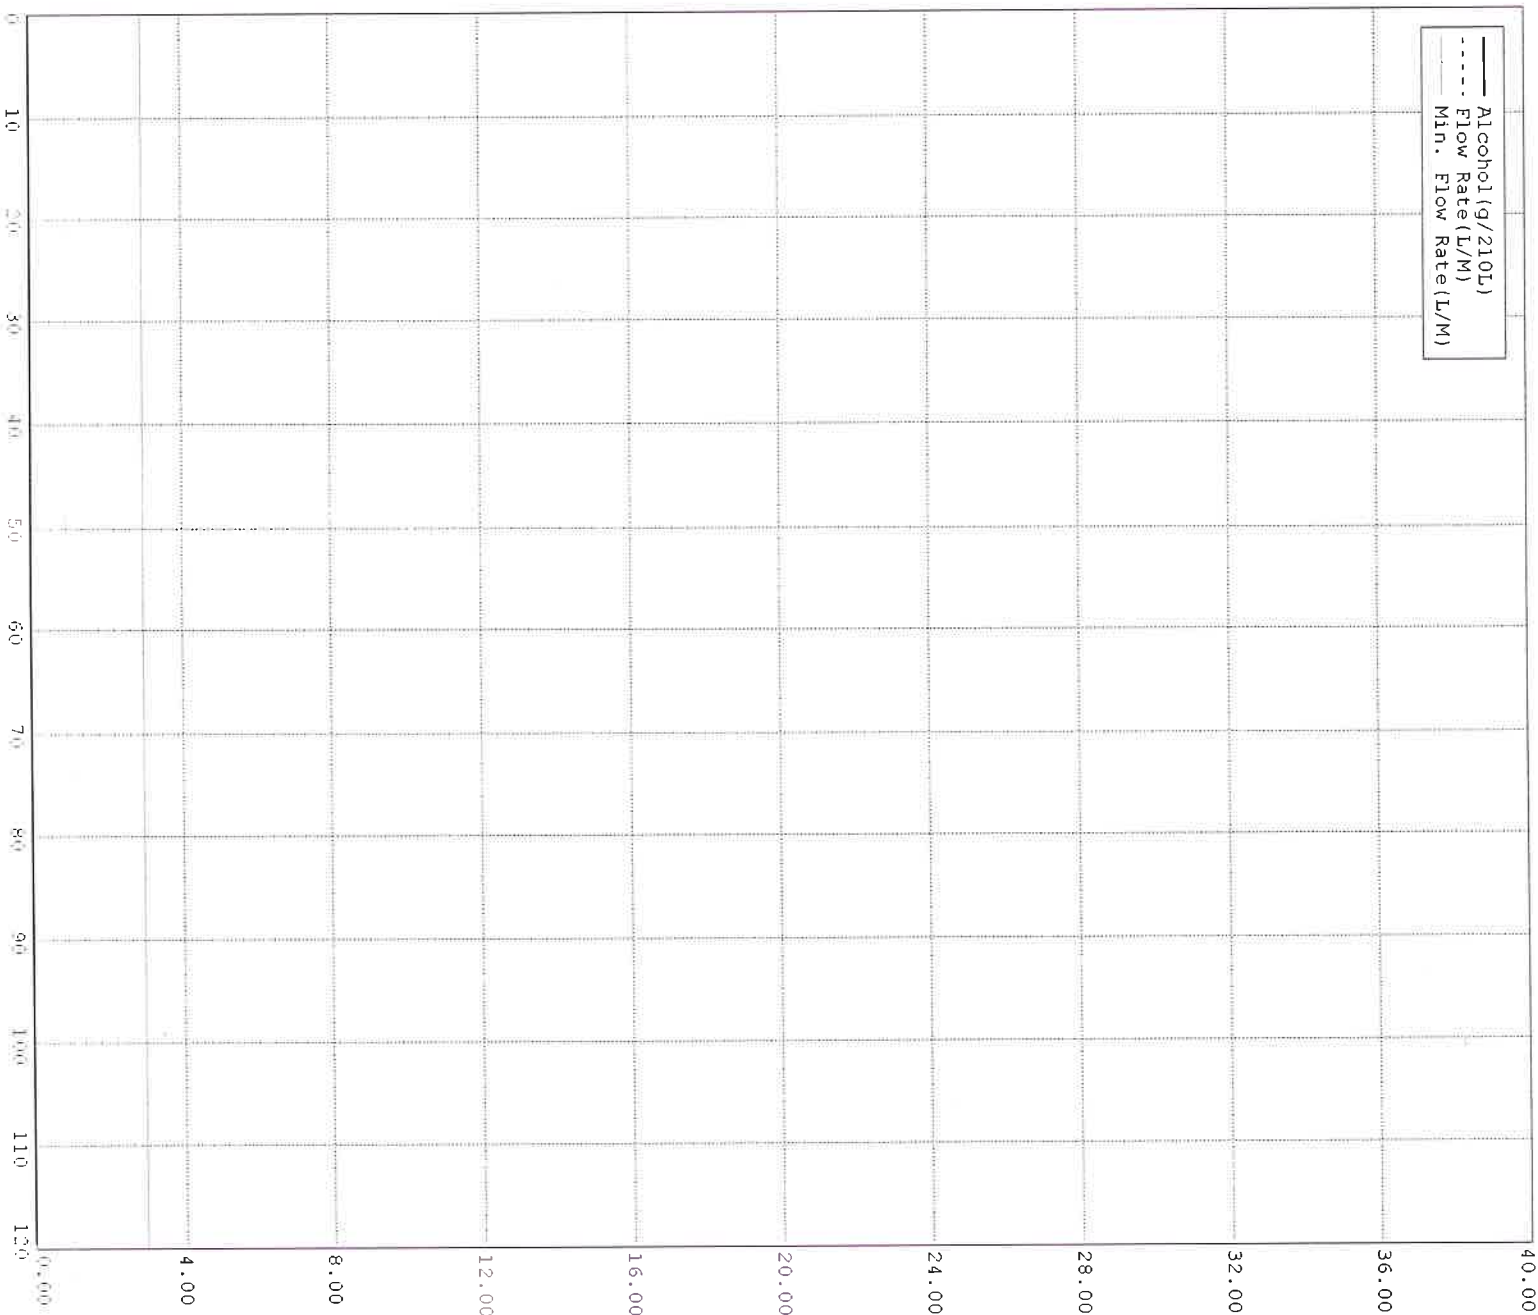

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 12:25:01


SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
INVALID  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.17: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:26
BLANK TEST	0.000	12:26
INTERNAL STANDARD	VERIFIED	12:26
EXTERNAL STANDARD	0.078	12:26
BLANK TEST	0.000	12:27
SUBJECT SAMPLE	INVALID	12:28

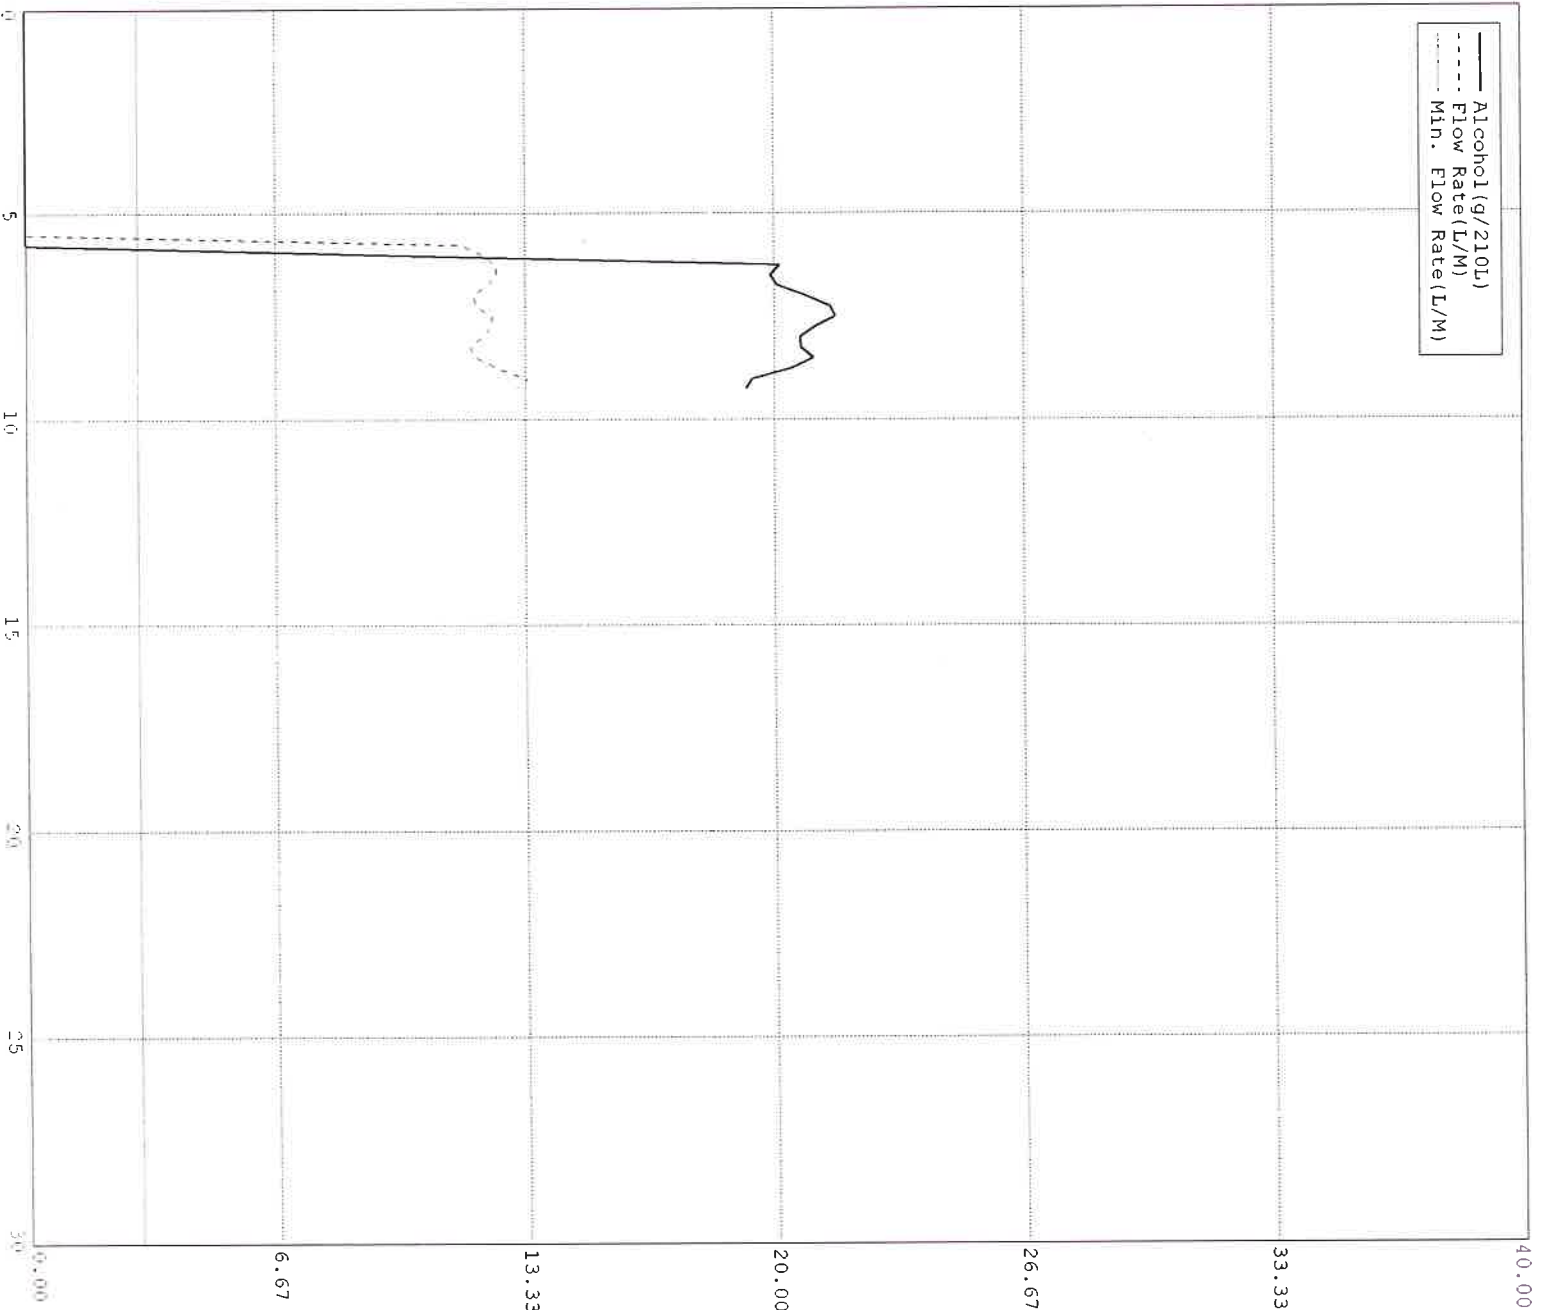

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 13:05:18

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KALJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
MAX ATTEMPTS  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.16: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:06
BLANK TEST	0.000	13:06
INTERNAL STANDARD	VERIFIED	13:06
EXTERNAL STANDARD	0.078	13:06
BLANK TEST	0.000	13:07
SUBJECT SAMPLE	XXX	13:08

Maximum Attempts Exceeded

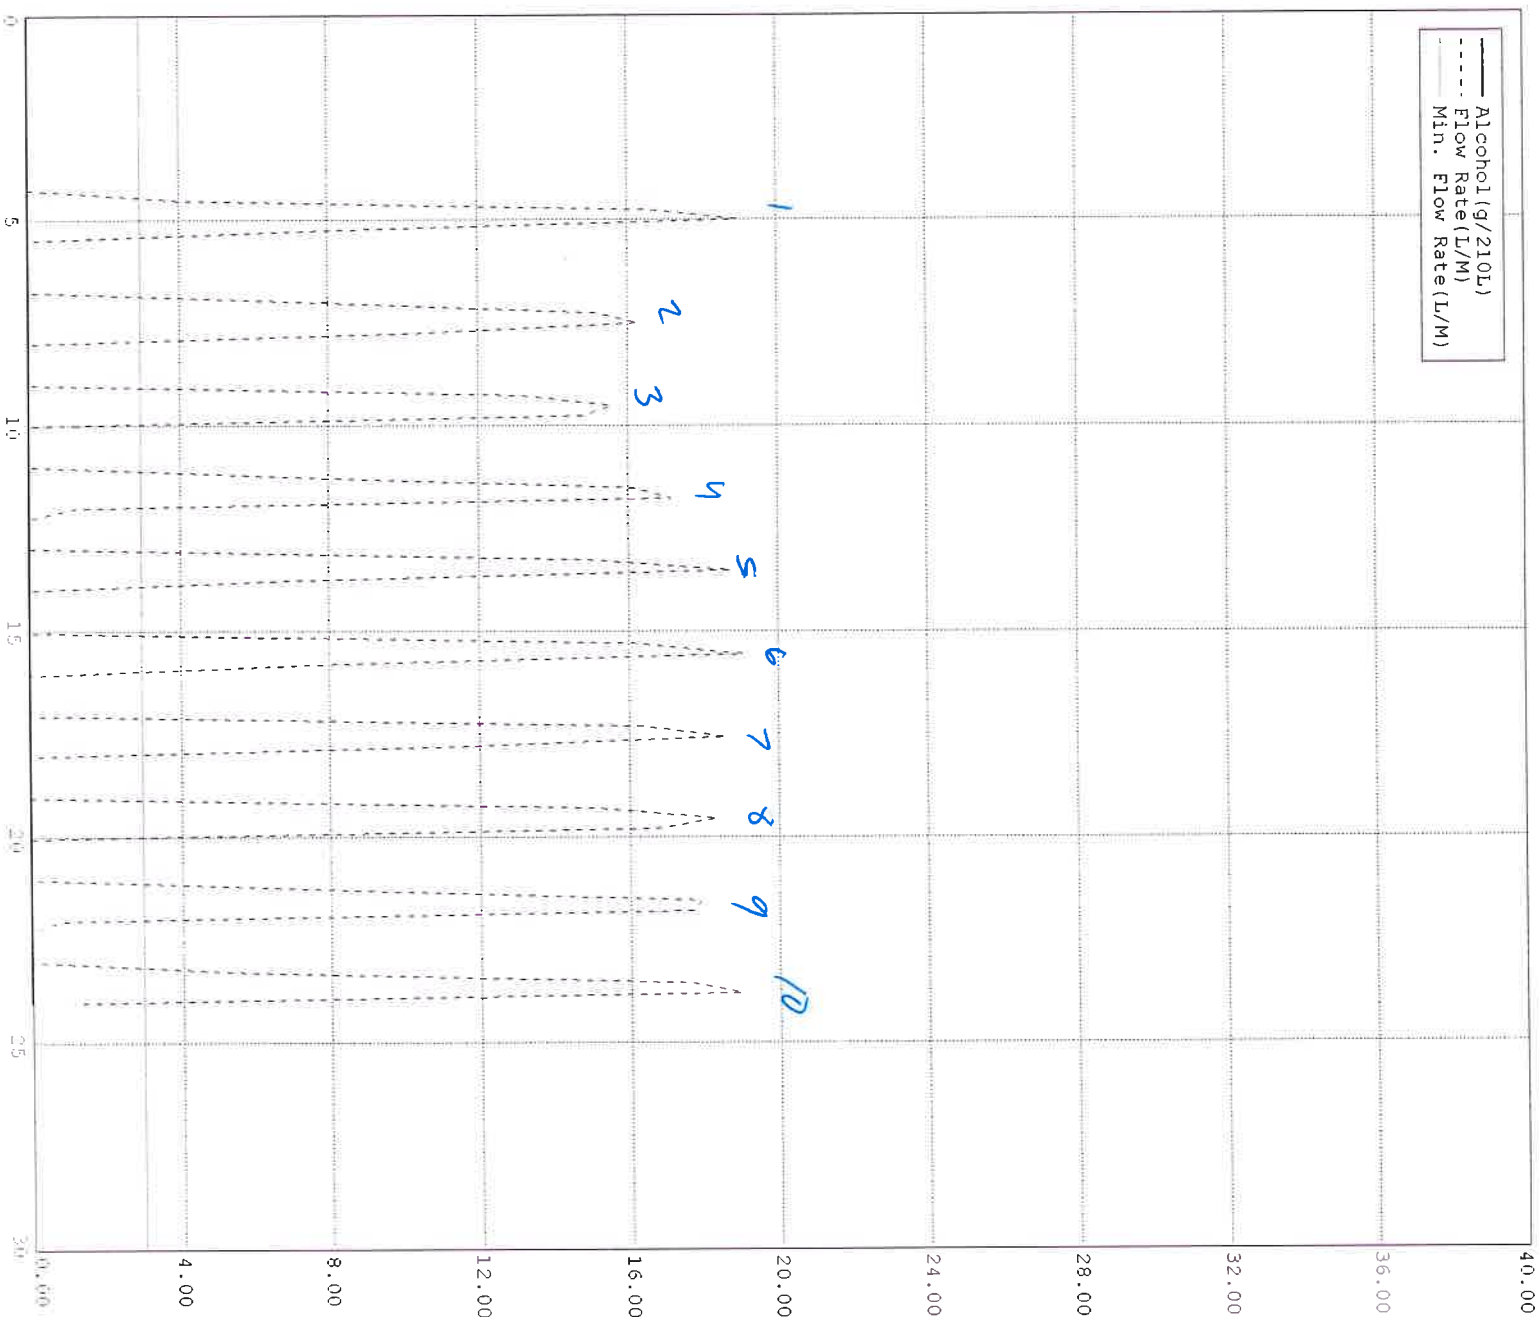



SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 13:16:12

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
RFI  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.16: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:17
BLANK TEST	0.000	13:17
INTERNAL STANDARD	VERIFIED	13:17
EXTERNAL STANDARD	0.078	13:17
BLANK TEST	0.000	13:18

RFI DETECTED

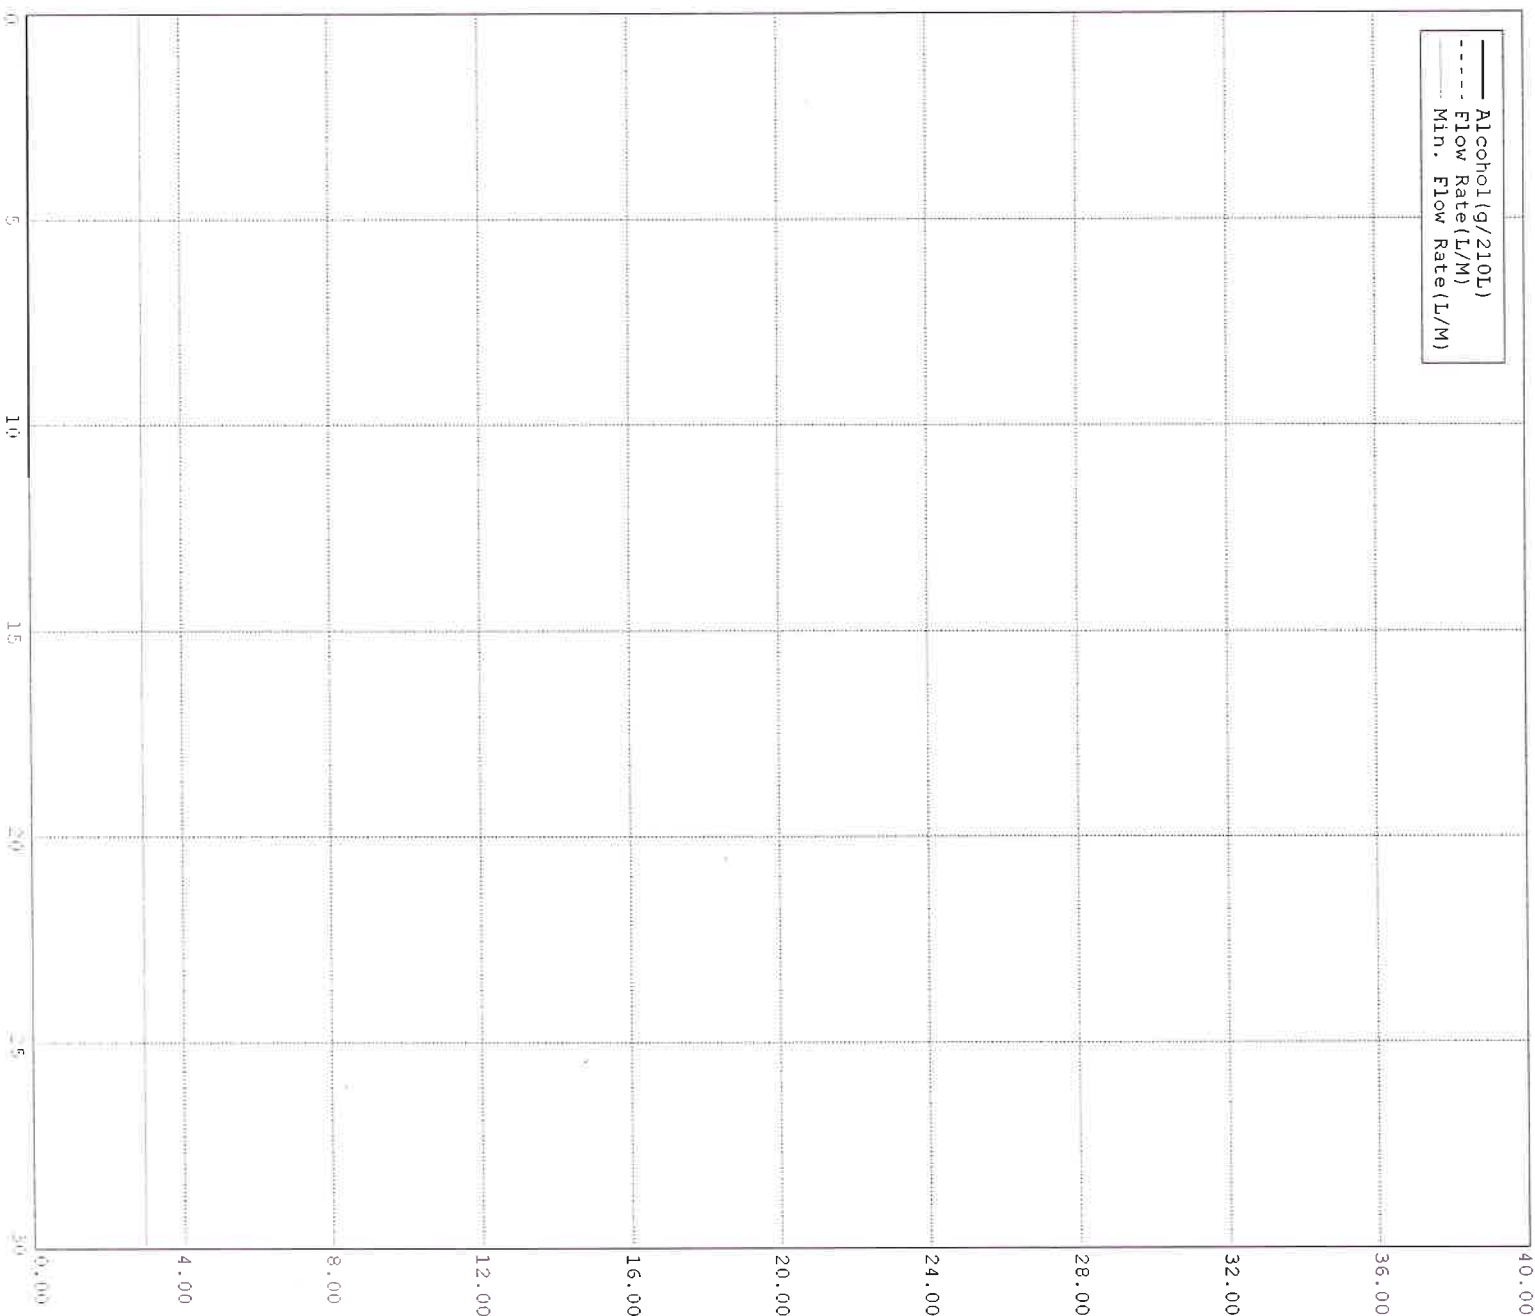

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 13:25:41

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746


DEPT/AGENCY:  
ACETONE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.16: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:26
BLANK TEST	0.000	13:27
INTERNAL STANDARD	VERIFIED	13:27
Xq = 0.081 (0.74%)	0.078	13:27
EXTERNAL STANDARD	X[1] = 0.0017	
X[1] = 0.0780 (-0.0008)	0.000	13:28
BLANK TEST	XXX	13:28
SUBJECT SAMPLE	X[1] = 0.1099 (-0.0240)	(-0.0012)

Interference Detected

Filter 2 ave: -0.0007  
Filter 3 ave: 0.0015  
KS 9/23/25

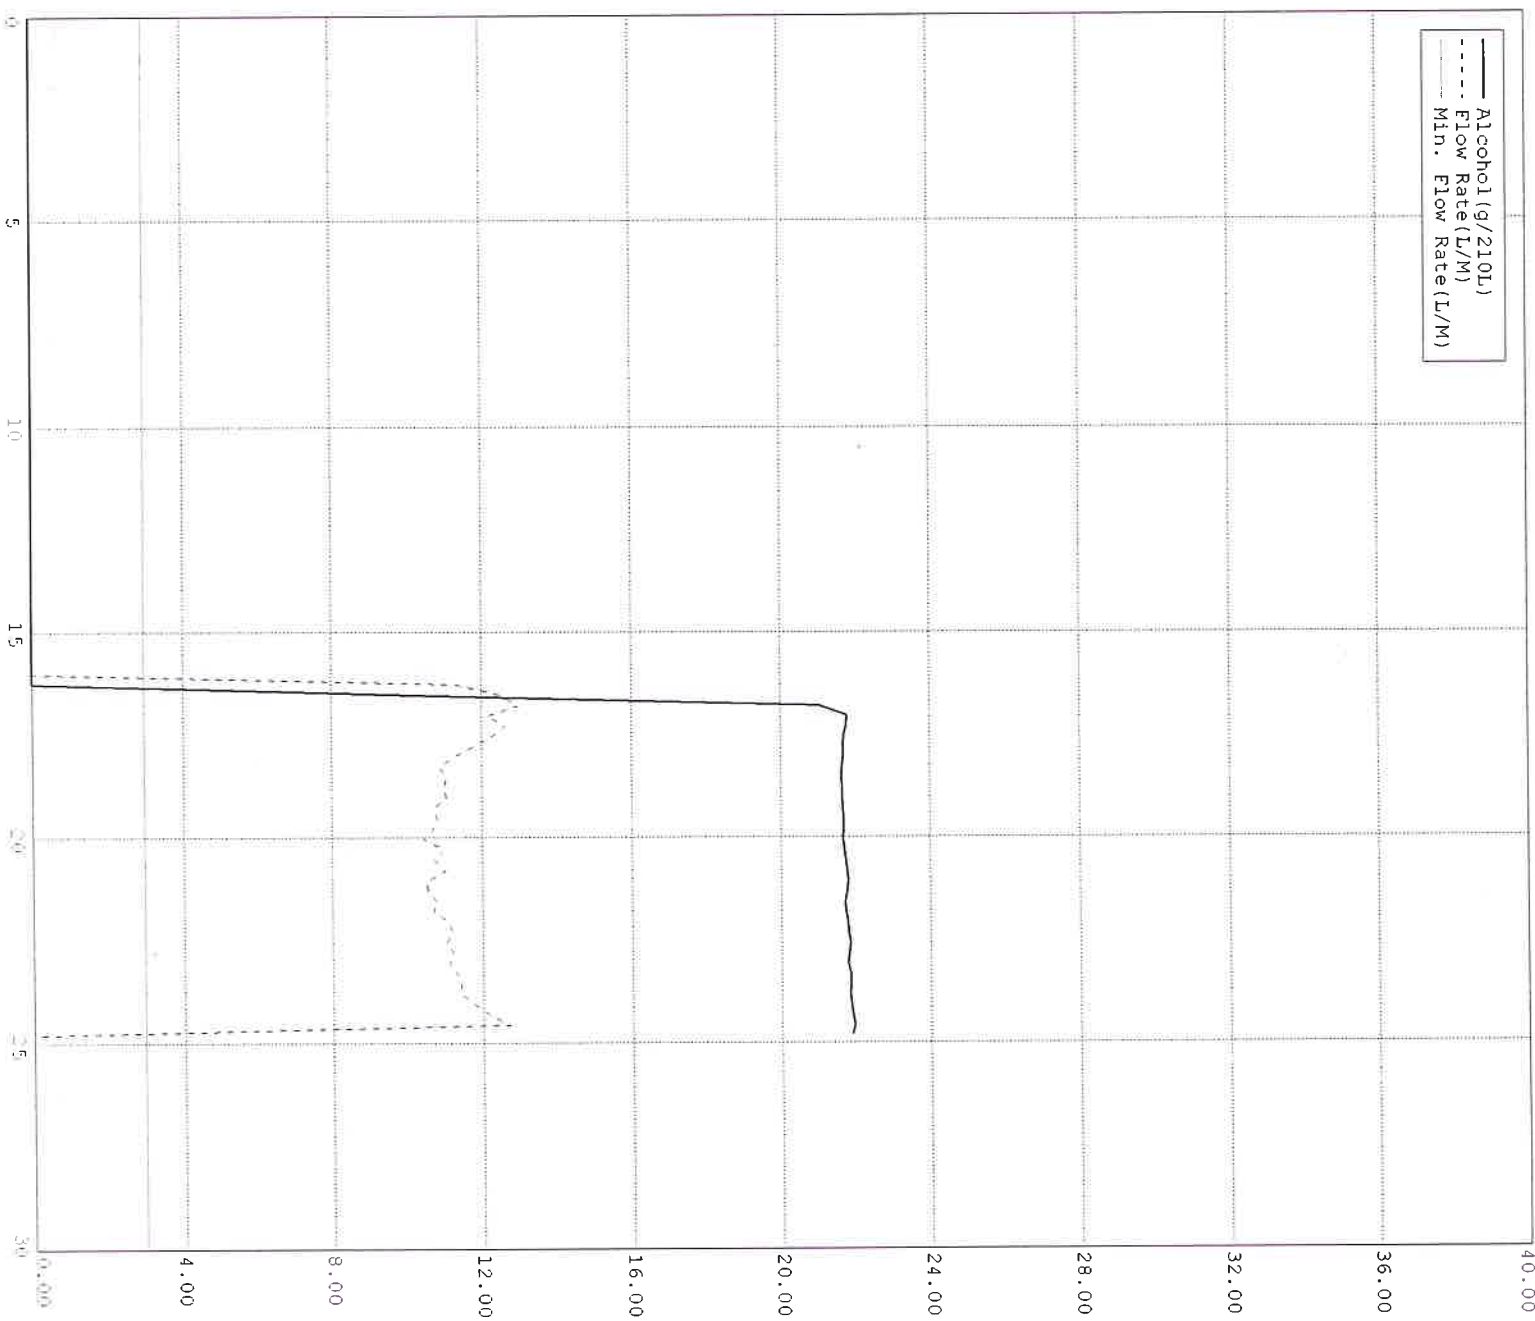

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 13:35:02

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
IPA  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.17: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:36
BLANK TEST	0.000	13:36
INTERNAL STANDARD	VERIFIED	13:36
Xq = 0.082 (0.21%)	0.078	13:36
EXTERNAL STANDARD	X[1] = 0.0777 (-0.0010)	(0.0016)
BLANK TEST	0.000	13:37
SUBJECT SAMPLE	XXX	13:38
X[1] = 0.1201 (-0.0196)	(0.0010)	

Interference Detected

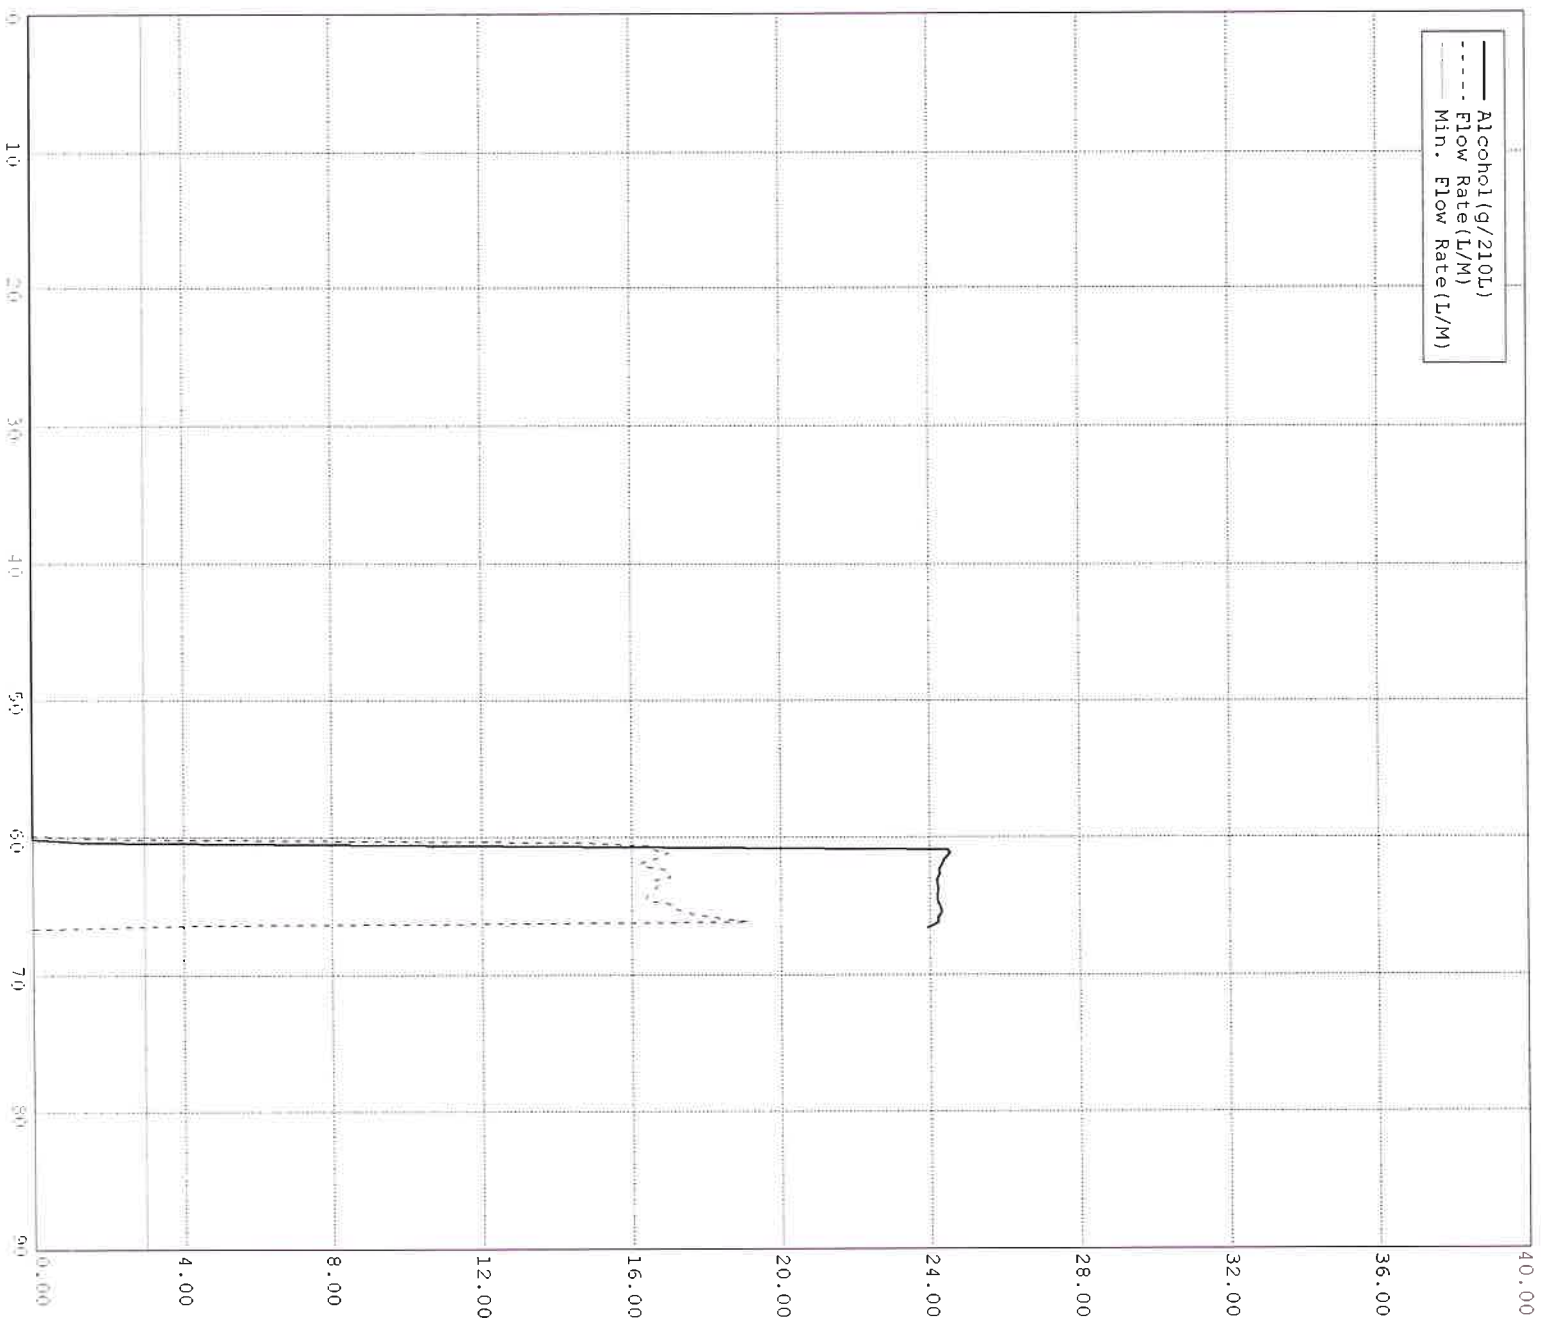

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 13:42:11

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX


OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
NEGATIVE  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 29.17: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	13:43
INTERNAL STANDARD	0.000	13:43
EXTERNAL STANDARD	0.078	13:43
Xq = 0.082 (0.53%)		
X[1] = 0.0780 (-0.0001)	(0.0017)	
INTERNAL STANDARD	0.000	13:44
EXTERNAL STANDARD	0.096	13:45
SUBJECT SAMPLE (Vol=1.64L)	(0.0000)	
X[1] = 0.0961 (-0.0004)	(0.0000)	
INTERNAL STANDARD	0.000	13:46
EXTERNAL STANDARD	0.078	13:46
X[1] = 0.0776 (-0.0007)	(0.0010)	
INTERNAL STANDARD	0.000	13:47
EXTERNAL STANDARD	0.000	13:47

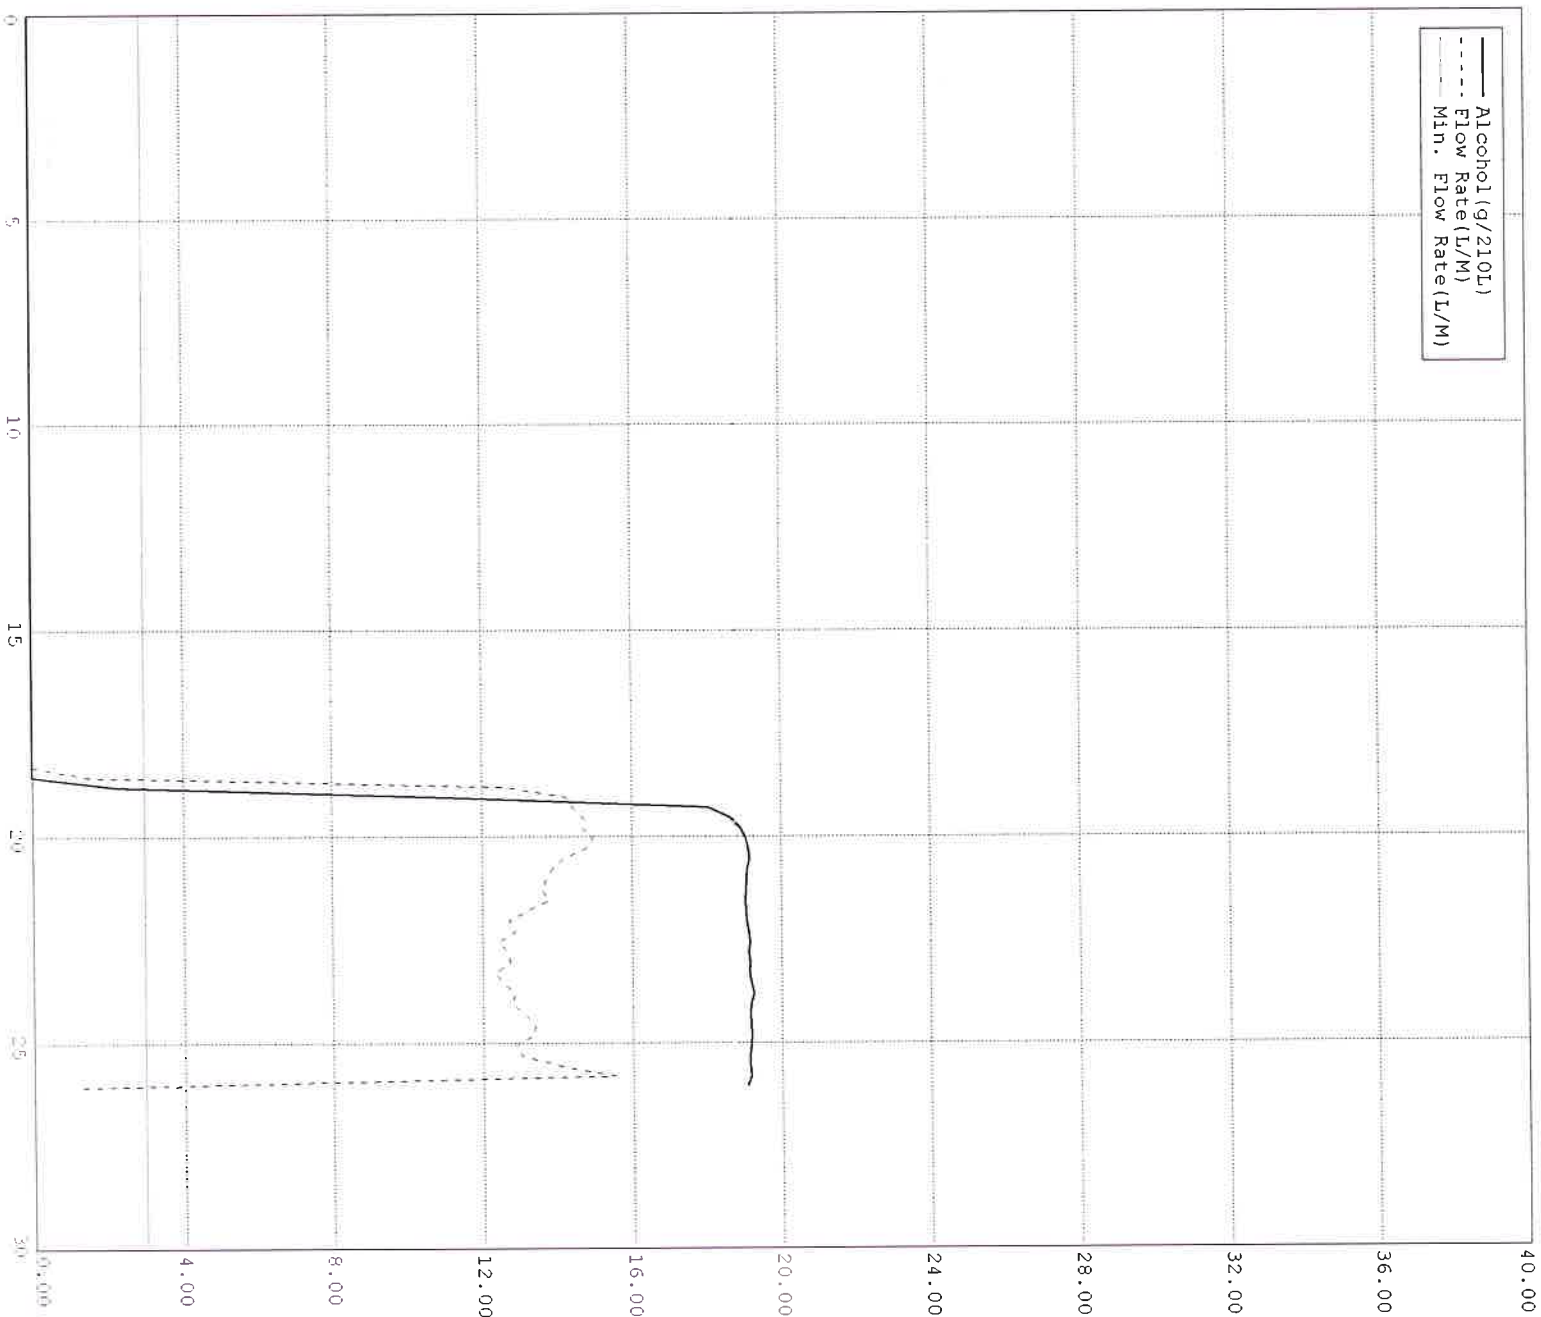

SUBJECT TEST

Alaska Department of Public Safety  
DATAMASTER dmt: 100697

Date: 09/22/2025  
Time: 14:33:45

SUBJECT NAME:  
TEST TEST  
LICENSE #: XXX

OPERATOR NAME:  
KAIJA SWISHER  
OPERATOR'S #: 10746

DEPT/AGENCY:  
NON-DRINKING TEST  
CASE/REPORT: XXX  
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION  
NOMINAL: 0.080  
TARGET AT 29.17: 0.078  
LOT #: AG335202  
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:35
BLANK TEST	0.000	14:35
INTERNAL STANDARD	VERIFIED	14:35
EXTERNAL STANDARD	0.078	14:36
BLANK TEST	0.000	14:37
SUBJECT SAMPLE (Vol=1.76L)	0.000	14:37
BLANK TEST	0.000	14:38
EXTERNAL STANDARD	0.078	14:38
BLANK TEST	0.000	14:39

