

# VERIFICATION OF CALIBRATION REPORT

of DataMaster dmt Breath Test Instrument

State of Alaska

Serial #: 100676

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Date: 10/31/2015

## External Standard Test Values

### EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080  
TARGET AT 27.73: 0.074  
LOT #: 09214080A2  
EXPIRATION: 05/01/2016  
TANK PRESSURE: 943 psi

BLANK TEST	0.000	09:32
INTERNAL STANDARD	VERIFIED	09:32
EXTERNAL STANDARD	0.071	09:32
BLANK TEST	0.000	09:33
EXTERNAL STANDARD	0.072	09:33
BLANK TEST	0.000	09:34
EXTERNAL STANDARD	0.072	09:35
BLANK TEST	0.000	09:36
EXTERNAL STANDARD	0.072	09:36
BLANK TEST	0.000	09:37
EXTERNAL STANDARD	0.072	09:37
BLANK TEST	0.000	09:38

Average = 0.0718  
Std Dev = 0.0004

## Diagnostic Check

### VERSIONS

DMT: 3.01  
PIC: 3.03  
Modem: 2.6  
Questions: 2.2

### TEMPERATURES

Sample Chamber = 48.9°C PASSED  
Breath Tube = 47.7°C PASSED

### PUMP INFO

Flow Rate = 3.912 L/M PASSED

### DETECTOR INFO

PUMP ON PASSED  
PUMP OFF PASSED

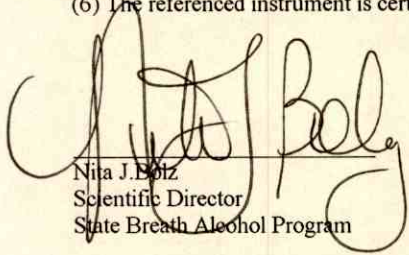
### FILTER INFO

Filter 1 PASSED  
Filter 2 PASSED  
Filter 3 PASSED

INTERNAL STANDARD PASSED


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the Breath Alcohol Program, which includes assuring that instruments are calibrated and maintaining program records.
- (5) The above is a true and accurate verification of calibration, which is performed by the instrument's software, as specified by the State Breath Alcohol Program. Verification of calibration is a regularly conducted and regularly recorded activity of the State Breath Alcohol Program.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

11/27/2015

Subscribed and sworn before me this 27<sup>th</sup> day of Nov. 20 15

  
Nikki Roth, Notary Public  
My Commission Expires With Office



CDE  
11/19/15