



State of Alaska
 Department of Public Safety
Scientific Crime Detection Laboratory

4805 Dr. Martin Luther King Jr. Ave.
 Anchorage, Alaska 99507
 David Kanaris, Chief, Forensic Laboratories



Breath Alcohol Calibration Report
Calibration Item: DataMaster DMT
Serial Number: 100361

Report Issue Date: 06/09/2025
Date Received: 2025-05-19
Condition of Item: Damaged

Method Used: DataMaster DMT Calibration / Current Breath Alcohol Procedure Manual
Calibration Range: 0.020 g/210L - 0.300 g/210L

No As-Found Data Collected

Unable to perform VOC, As Found Linearity, or Non-Drinking Subject Test due to breath hose not being up to temperature. Breath hose needs to be replaced.

As-Left Data

Nominal Values (g/210L)	Target Values (g/210L)	Lot Number	Results (g/210L)					Mean (g/210L)	Uncertainty (g/210L)
0.020	0.020	AG408002	0.020	0.020	0.020	0.020	0.019	0.020	+/- 0.002
0.040	0.039	AG407908	0.040	0.039	0.040	0.039	0.039	0.039	+/- 0.003
0.080	0.079	AG335202	0.078	0.077	0.077	0.077	0.077	0.077	+/- 0.004
0.100	0.098	AG333401	0.099	0.098	0.099	0.099	0.099	0.099	+/- 0.004
0.150	0.148	AG332004	0.146	0.145	0.145	0.145	0.145	0.145	+/- 0.006
0.300	0.295	AG427706	0.293	0.292	0.293	0.292	0.294	0.293	+/- 0.012

As Left Conditions - Barometric Pressure (inHg): 29.53 Barometer Used: VWR S/N 240680771 Temperature (C): 22.3 Relative Humidity (%): 29
 As-Left Lab Activity Date Range: 06/04/2025 - 06/05/2025

Calibration is performed using dry gas standards traceable to NIST. Standards are sourced from an external provider accredited to ISO/IEC 17025 and ISO 17034 standards. Internal instrument barometer readings are traceable to NIST. External barometers are calibrated by an external calibration provider accredited to the ISO/IEC 17025 standard.

The As-Left results listed above include the estimated measurement uncertainty with a coverage factor k=2 and an expanded coverage probability of 95%. The estimated uncertainty applies to the calibration process and not to subject breath samples.

This report applies only to the item being calibrated and shall not be reproduced, except in full, without written approval from the laboratory.

Results authorized by Kaija Swisher on 06/09/2025

kaija.swisher@alaska.gov

Technically and administratively reviewed by Carlie Glaister on 06/09/2025

Alaska Scientific Crime Detection Laboratory

DataMaster Calibration Form

Effective: 1/23/2024

Version: 4.0

Instrument #: 100361 Analyst or Technician Name: Kaija Swisher

DataMaster DMT Calibration Start Date: 6/4/25

Diagnostic Test

- Perform Diagnostic Test (View Details)
- Internal Standard Value \leq 3.00%

Technician Screen and Calibration Factors

- Adjust Voltages (if needed)
 - Lamp (2.60 V Maximum)
 - Bias
 - Cooler (2.00 V Maximum)
 - Chopper Frequency
 - Detector Voltage (-0.100V to 0.100V)
- Set RFI Sensitivity
- Adjust internal barometer reading to match NIST-traceable barometer
Barometer/Thermometer/Hygrometer S/N: 240680771
Calibration Due Date: 9/10/26
- Verify Volume Setting (1.50 L +/- 0.10 L), adjust if needed
- Print Technician Screen
- Print "Cal Factors"

Minimum Volume Test

- Perform Minimum Volume (Subject) Test: 1.4 liters (1.3 L to 1.7 L)

As Left Linearity Testing

Barometric Pressure (in Hg) 29.53 Temperature(C) 22.3 Relative Humidity(%) 29

Approved Concentrations (g/210L): 0.020, 0.040, 0.080, 0.100, 0.150, 0.300

Functional Tests

- Incomplete
- Invalid
- Interference (Volatiles) - *Print with View Details*
- Maximum Attempts Exceeded
- Radio Frequency Interference (RFI)

- 1. Acetone Reagent Lot Number: 20250603KS Expiration Date: 7/27/25
Simulator S/N: SD1200 Thermometer Verification Performed?
- 2. Isopropanol Reagent Lot Number: 20250603KS Expiration Date: 9/3/25
Simulator S/N: SD1198 Thermometer Verification Performed?
- 3. Negative (Ethanol Only) Lot Number: 23IP41233 Expiration Date: 9/3/25
Simulator S/N: SD1199 Thermometer Verification Performed?

0.100 solution exp: 9/20/2025
KS 06/05/2025

Calibrated External Thermometer S/N: 230631106

Calibration Due Date: 9/19/2025

Administrative

- Verify Stylus Calibration
- Reset Options
- Clear Memory
- Verification of Calibration (VOC)
- Perform Non-Drinking Subject Test
- Upload Instrument
- Remove Dry Gas Tank Before Shutdown
- Add Ready for Tech Review Note

Completion

Lab Work End Date: 6/4/25

Data Interpretation Date (Technician): N/A (if applicable)

Data Interpretation Date (Analyst): 6/5/25

All printed copies are uncontrolled.

Approved by: Chemistry Supervisor

DIAGNOSTIC RECORD

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 08:09:22

VERSIONS
DMT: 3.02
PIC: 3.03
Modem: 2.6
Questions: 2.2

TEMPERATURES

Sample Chamber = 48.9°C PASSED
(44.0°C - 52.0°C)
Breath Tube = 48.1°C PASSED
(38.0°C - 50.0°C)

SETTINGS

Lamp Voltage = 1.87 V PASSED
(1.17 V - 2.73 V)
Cooler Voltage = 1.94 V PASSED
(1.01 V - 2.35 V)
Bias Voltage = 79 V PASSED
(48 V - 112 V)
Chopper Freq = 530 Hz PASSED
(475 Hz - 575 Hz)
Barometer = 29.5 in

PUMP INFO

Flow Rate = 5.322 L/M PASSED
(3.500 L/M - 6.500 L/M)

DETECTOR INFO

PUMP ON PASSED
(0.002 v <= 0.010 v)
PUMP OFF PASSED
(0.002 v <= 0.010 v)

FILTER INFO

Filter 1 PASSED
Filter 2 PASSED
Filter 3 PASSED

INTERNAL STANDARD PASSED
Xq = 0.088 0.40% (0.00% - 4.00%)

Technician Screen

DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 8:34 AM

Temperatures (°C)
Sample Cell: 49.2°C
Breath Tube: 45.3°C

Current Barometer 29.5 in
Volume (Ltr) 1.51

Settings
Lamp: 1.87 V
Bias: 79 V
Cooler: 1.94 V
Chopper: 524 Hz

Voltages (V)
Flow: 1.04 V
Detector: -0.020 V

CALIBRATION FACTORS

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 04/23/2021
Time: 09:19:31

OPERATOR NAME:
NPAS TECH
CERTIFICATE #: G12921/20490

Ca = 0.1000
CAL = 0.999458 0.800 <= CAL < 1.200
b1 = 0.0003 0.0000 <= b1 < 0.0040
b2 = 0.0060 0.0010 <= b2 < 0.0100
b3 = 0.0001 0.0000 <= b3 < 0.0040
Xq = 0.0877 0.0500 <= Xq < 0.2000
a21 = 1.187326 1.050 <= a21 < 1.300
a31 = 0.501823 0.300 <= a31 < 0.800



SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 08:50:01

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
MINIMUM VOLUME TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.50: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	08:51
BLANK TEST	0.000	08:51
INTERNAL STANDARD	VERIFIED	08:51
EXTERNAL STANDARD	0.077	08:51
BLANK TEST	0.000	08:52
SUBJECT SAMPLE (Vol=1.51L)	0.000	08:53
BLANK TEST	0.000	08:53
EXTERNAL STANDARD	0.077	08:54
BLANK TEST	0.000	08:55

KS

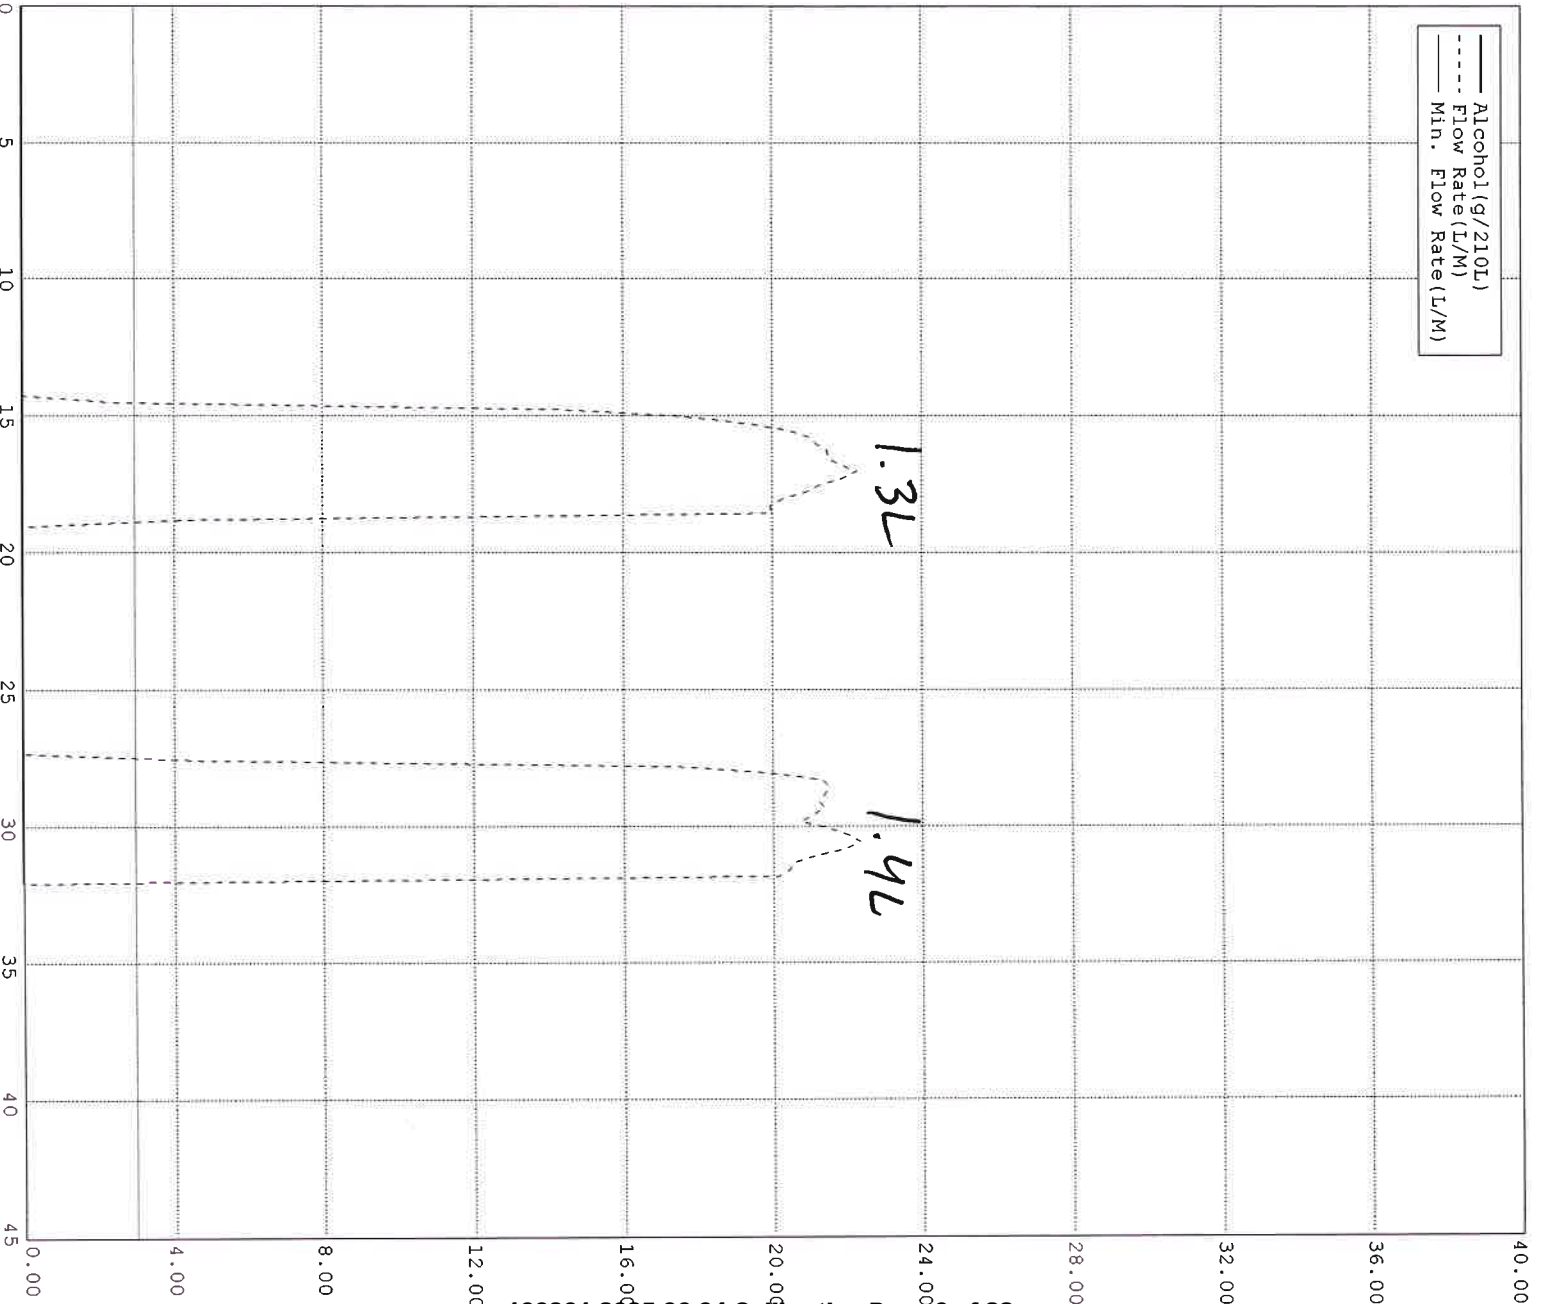

LINEARITY CHECK


Alaska Department of Public Safety
DATAMASTER dnt: 100361

Date: 06/04/2025
Time: 10:53:13

SUPERVISOR NAME:
KAITA SWISHER
OPERATOR'S #: 10746

TARGET	AVERAGE	STD. DEV.
0.020	0.0198	0.0004
0.039	0.0394	0.0005
0.079	0.0772	0.0004
0.098	0.0988	0.0004
0.148	0.1452	0.0004
0.295	0.2928	0.0008

SLOPE = 0.990789
R² = 0.999859

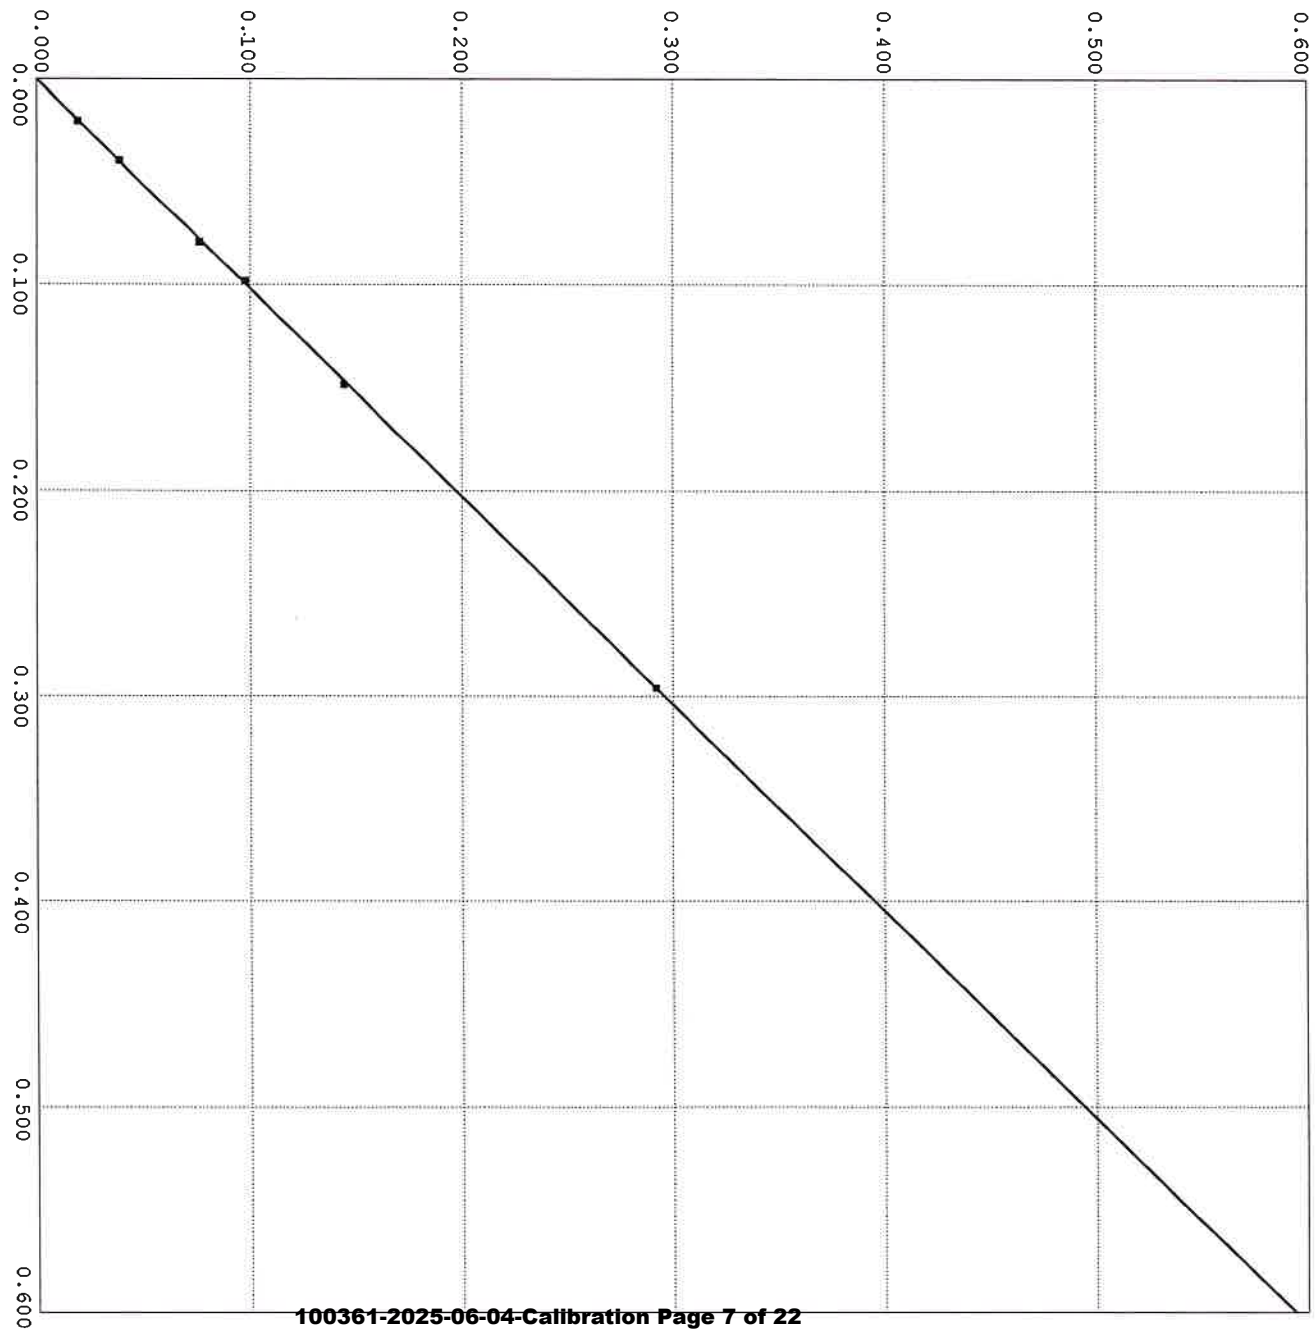

KS

LINEARITY CHECK: Control Test 1

Alaska Department of Public Safety
 DATAMASTER dmt: 100361






Date: 06/04/2025
 Time: 10:53:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.020
 TARGET AT 29.45: 0.020
 LOT #: AG408002
 EXPIRATION: 03/20/2026
 TANK PRESSURE: 841 psi

BLANK TEST	0.000	10:54
INTERNAL STANDARD	VERIFIED	10:54
EXTERNAL STANDARD	0.020	10:55
BLANK TEST	0.000	10:55
EXTERNAL STANDARD	0.020	10:56
BLANK TEST	0.000	10:57
EXTERNAL STANDARD	0.020	10:57
BLANK TEST	0.000	10:58
EXTERNAL STANDARD	0.020	10:58
BLANK TEST	0.000	10:59
EXTERNAL STANDARD	0.019	10:59
BLANK TEST	0.000	11:00

Average = 0.0198
 Std Dev = 0.0004

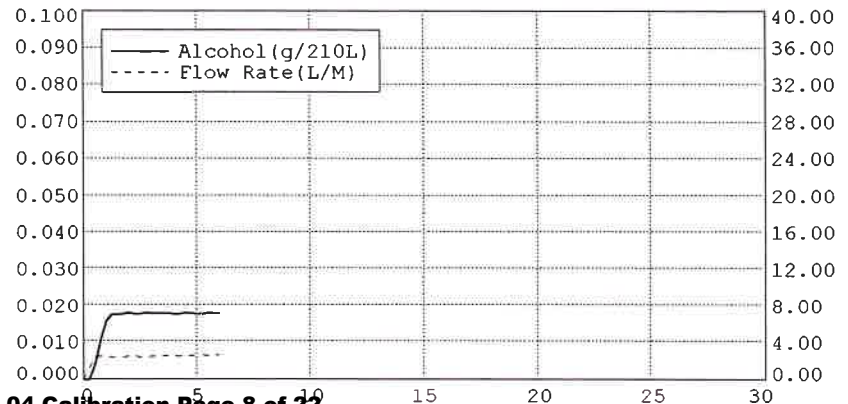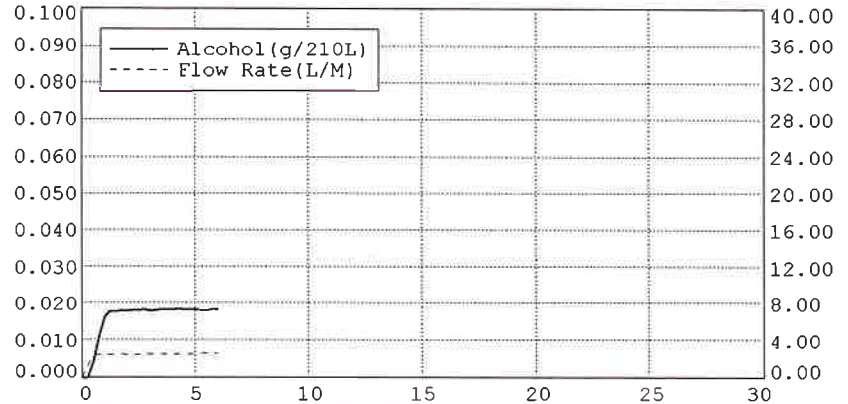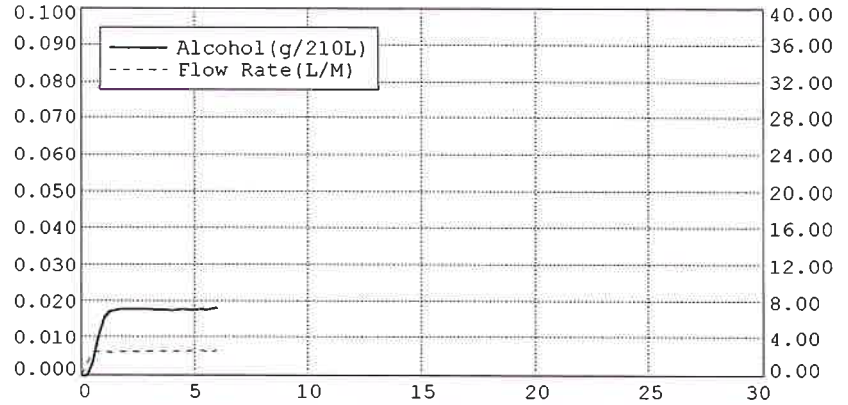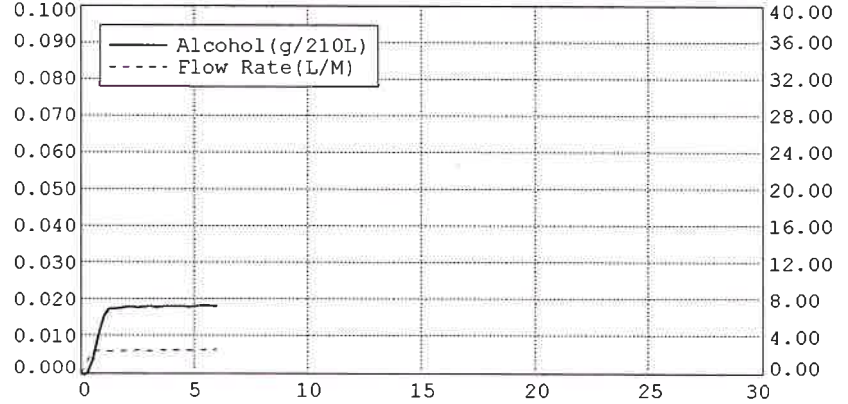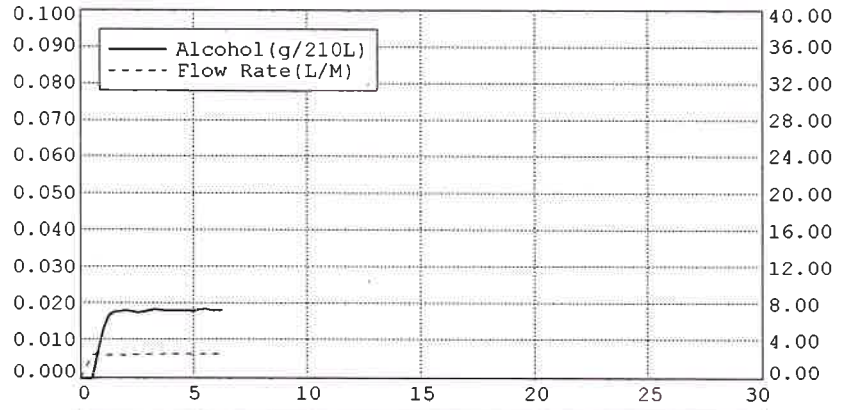

LINEARITY CHECK: Control Test 2

Alaska Department of Public Safety
DATAMASTER dmt: 100361






Date: 06/04/2025
Time: 11:02:58

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.040
TARGET AT 29.44: 0.039
LOT #: AG407908
EXPIRATION: 03/19/2026
TANK PRESSURE: 748 psi

BLANK TEST	0.000	11:04
INTERNAL STANDARD	VERIFIED	11:04
EXTERNAL STANDARD	0.040	11:04
BLANK TEST	0.000	11:05
EXTERNAL STANDARD	0.039	11:05
BLANK TEST	0.000	11:06
EXTERNAL STANDARD	0.040	11:07
BLANK TEST	0.000	11:07
EXTERNAL STANDARD	0.039	11:08
BLANK TEST	0.000	11:09
EXTERNAL STANDARD	0.039	11:09
BLANK TEST	0.000	11:10

Average = 0.0394
Std Dev = 0.0005

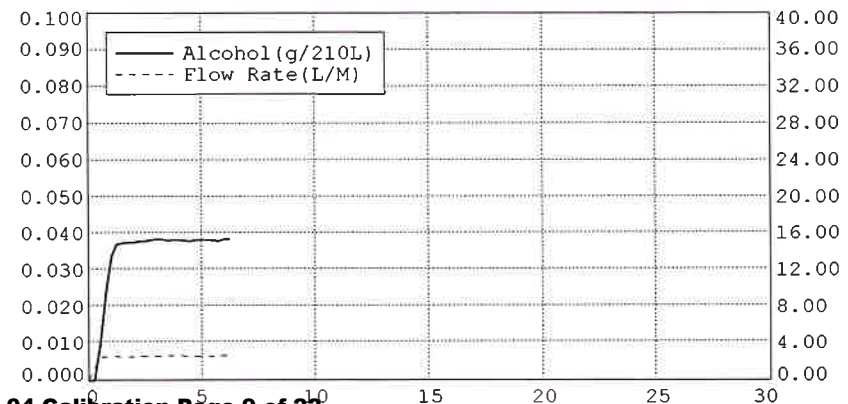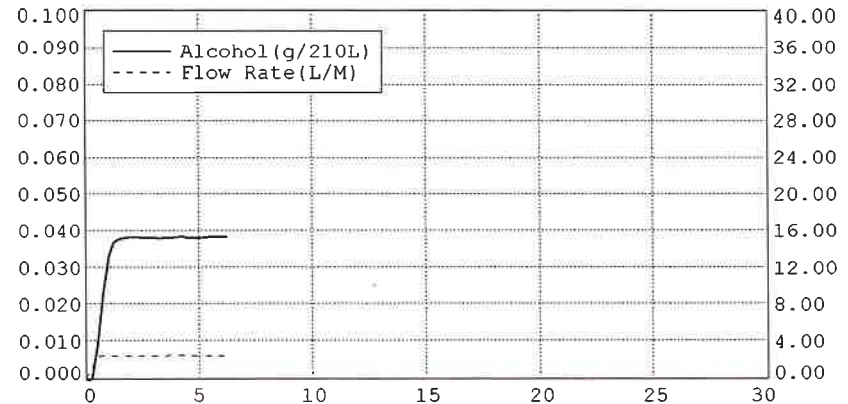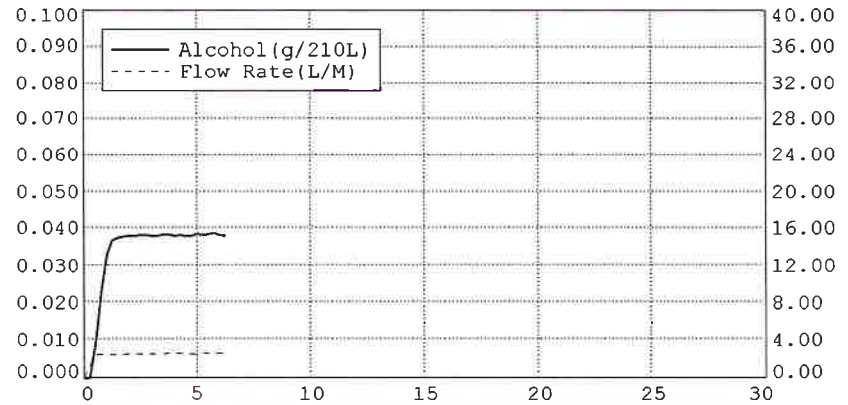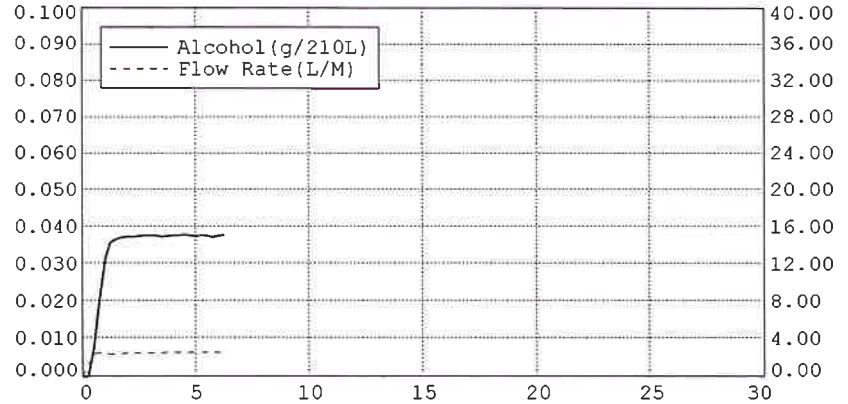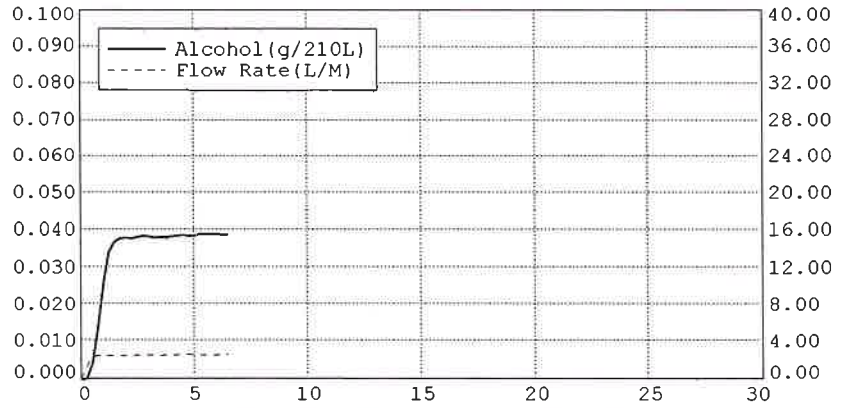

LINEARITY CHECK: Control Test 3

Alaska Department of Public Safety
 DATAMASTER dmt: 100361






Date: 06/04/2025
 Time: 11:10:45

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.080
 TARGET AT 29.43: 0.079
 LOT #: AG335202
 EXPIRATION: 12/18/2025
 TANK PRESSURE: 240 psi

BLANK TEST	0.000	11:12
INTERNAL STANDARD	VERIFIED	11:12
EXTERNAL STANDARD	0.078	11:12
BLANK TEST	0.000	11:13
EXTERNAL STANDARD	0.077	11:13
BLANK TEST	0.000	11:14
EXTERNAL STANDARD	0.077	11:14
BLANK TEST	0.000	11:15
EXTERNAL STANDARD	0.077	11:15
BLANK TEST	0.000	11:16
EXTERNAL STANDARD	0.077	11:16
BLANK TEST	0.000	11:17

Average = 0.0772
 Std Dev = 0.0004

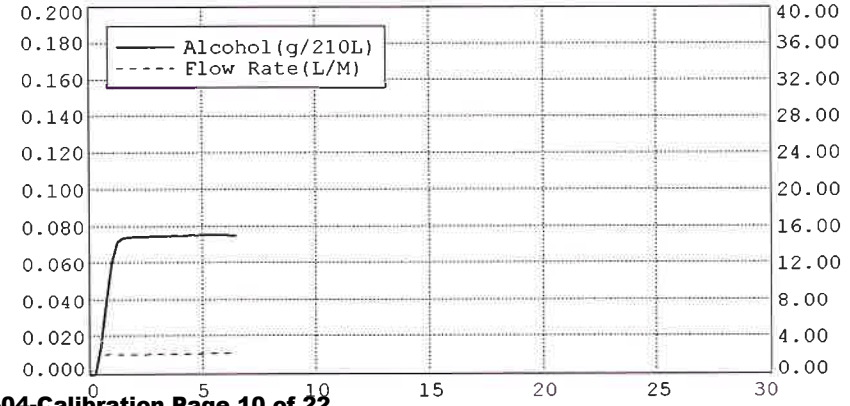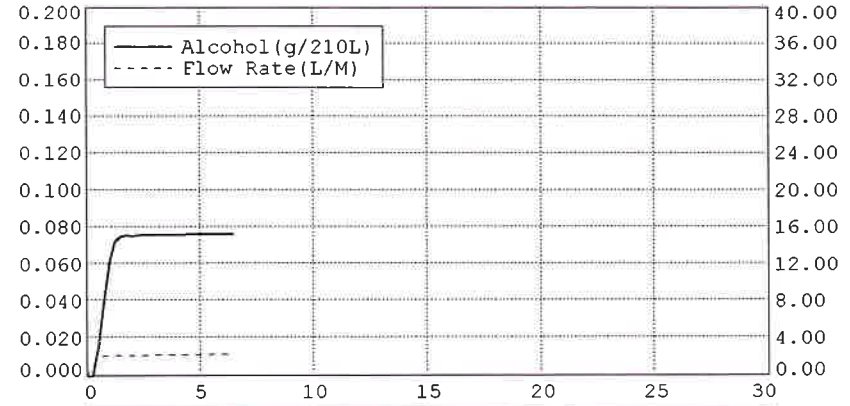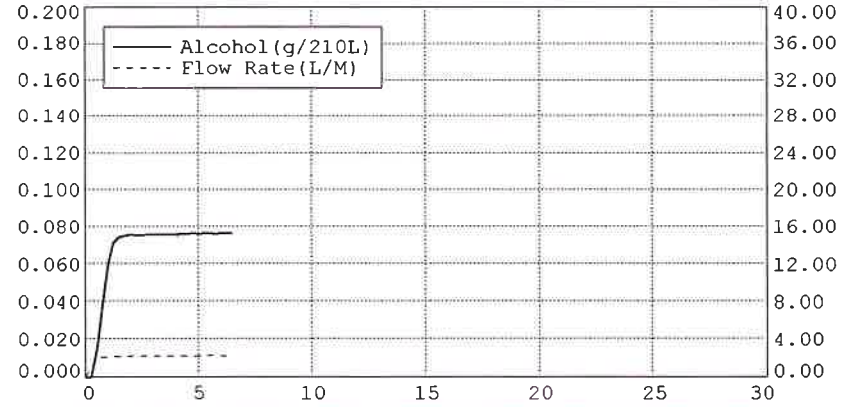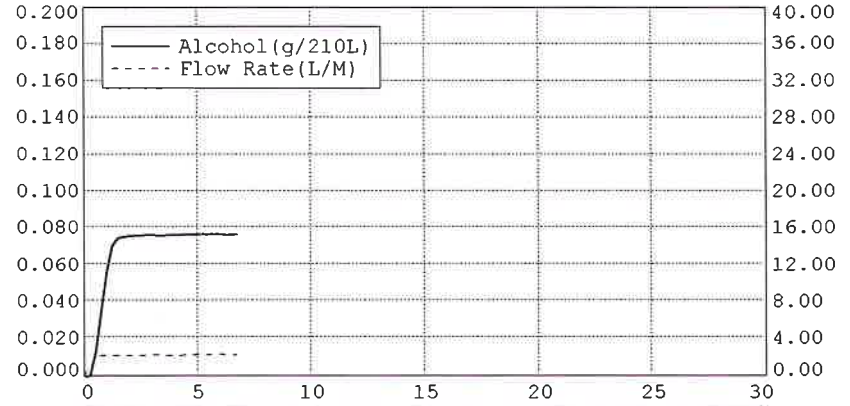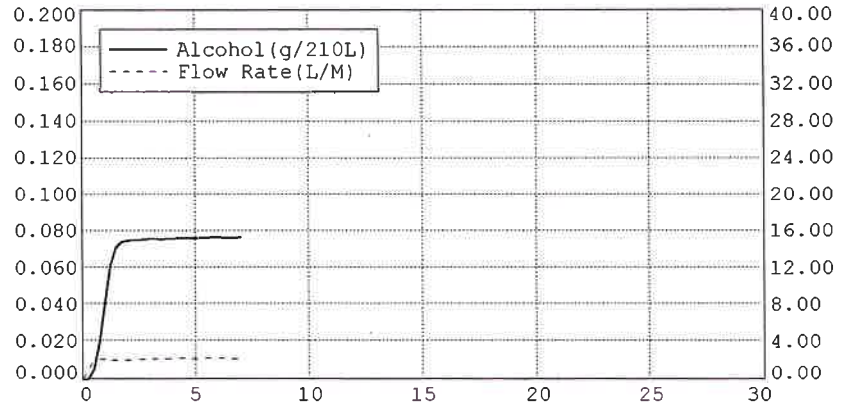

LINEARITY CHECK: Control Test 4

Alaska Department of Public Safety
 DATAMASTER dmt: 100361






Date: 06/04/2025
 Time: 11:20:15

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.100
 TARGET AT 29.44: 0.098
 LOT #: AG333401
 EXPIRATION: 11/30/2025
 TANK PRESSURE: 1078 psi

BLANK TEST	0.000	11:21
INTERNAL STANDARD	VERIFIED	11:21
EXTERNAL STANDARD	0.099	11:22
BLANK TEST	0.000	11:22
EXTERNAL STANDARD	0.098	11:23
BLANK TEST	0.000	11:24
EXTERNAL STANDARD	0.099	11:24
BLANK TEST	0.000	11:25
EXTERNAL STANDARD	0.099	11:25
BLANK TEST	0.000	11:26
EXTERNAL STANDARD	0.099	11:26
BLANK TEST	0.000	11:27

Average = 0.0988
 Std Dev = 0.0004

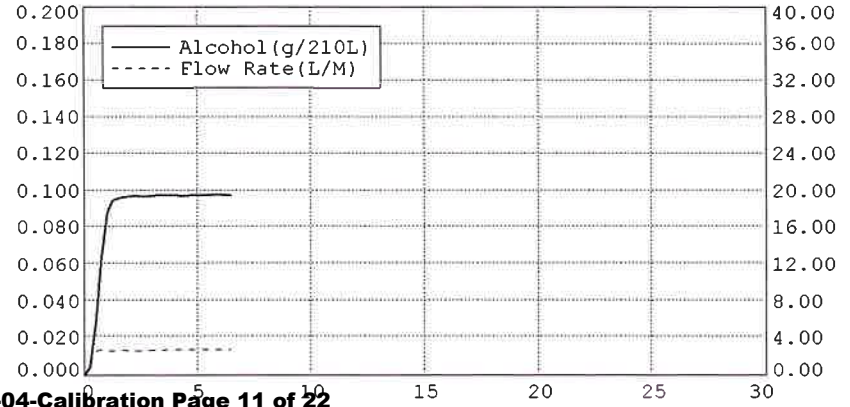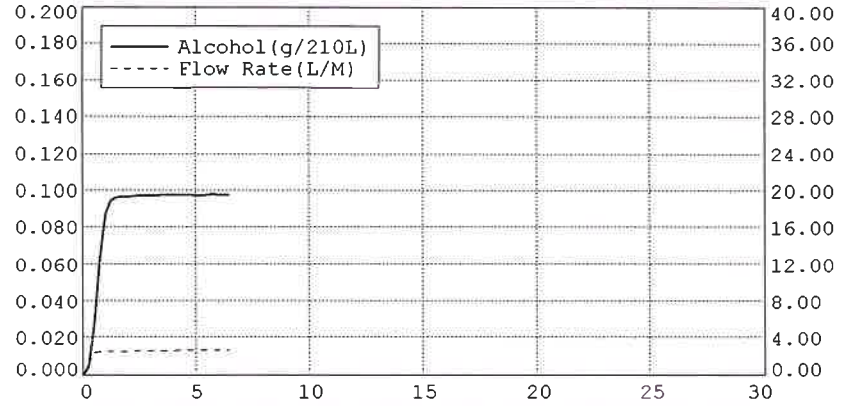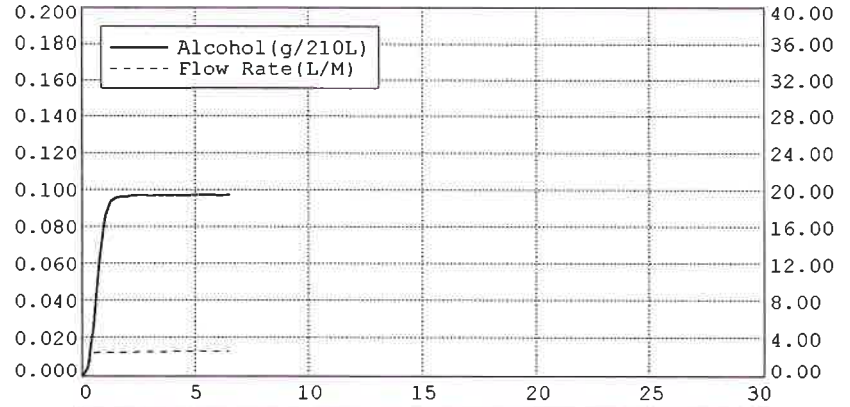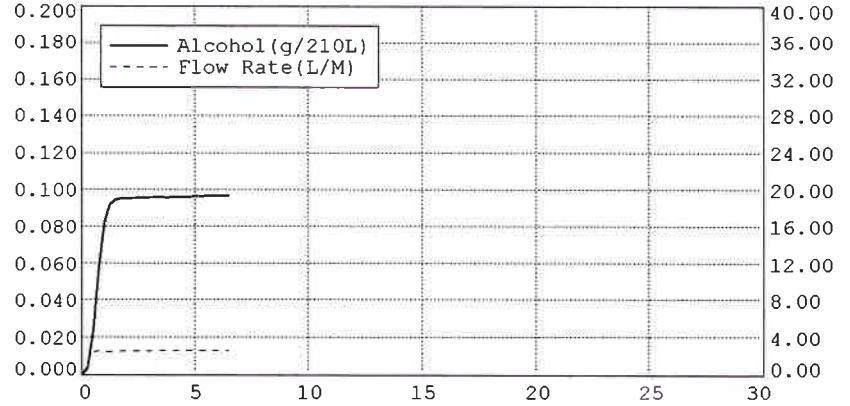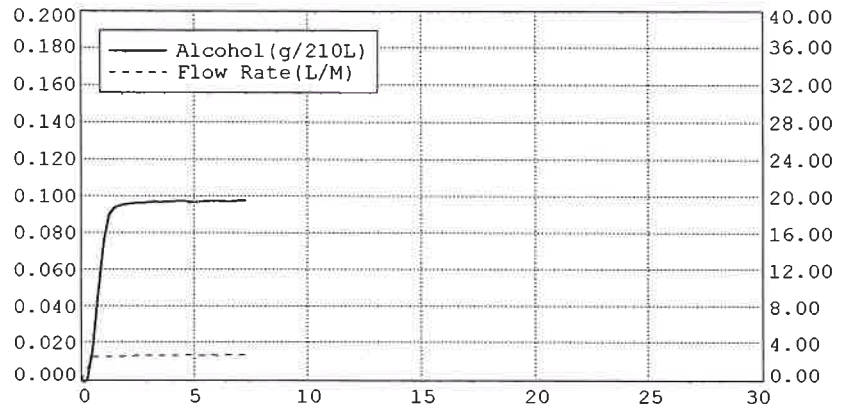

LINEARITY CHECK: Control Test 5

Alaska Department of Public Safety
 DATAMASTER dmt: 100361






Date: 06/04/2025
 Time: 11:28:25

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.150
 TARGET AT 29.43: 0.148
 LOT #: AG332004
 EXPIRATION: 11/16/2025
 TANK PRESSURE: 500 psi

BLANK TEST	0.000	11:29
INTERNAL STANDARD	VERIFIED	11:29
EXTERNAL STANDARD	0.146	11:30
BLANK TEST	0.000	11:31
EXTERNAL STANDARD	0.145	11:31
BLANK TEST	0.000	11:32
EXTERNAL STANDARD	0.145	11:32
BLANK TEST	0.000	11:33
EXTERNAL STANDARD	0.145	11:33
BLANK TEST	0.000	11:34
EXTERNAL STANDARD	0.145	11:34
BLANK TEST	0.000	11:35

Average = 0.1452
 Std Dev = 0.0004

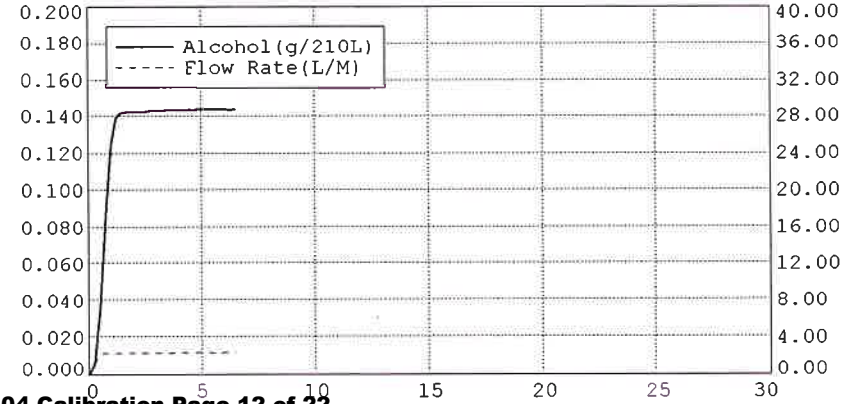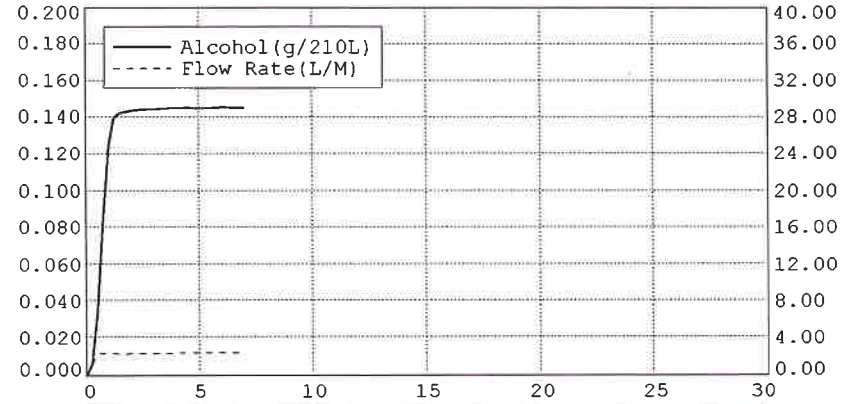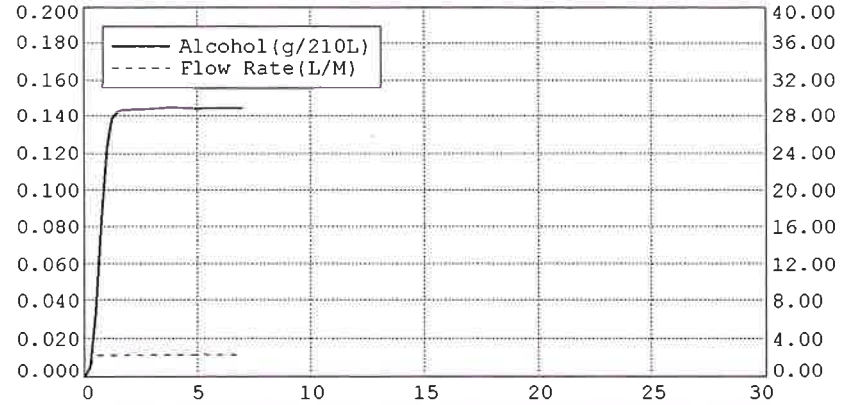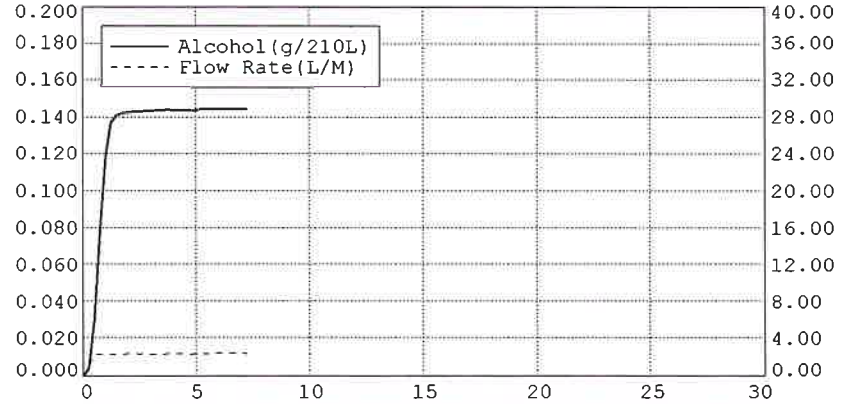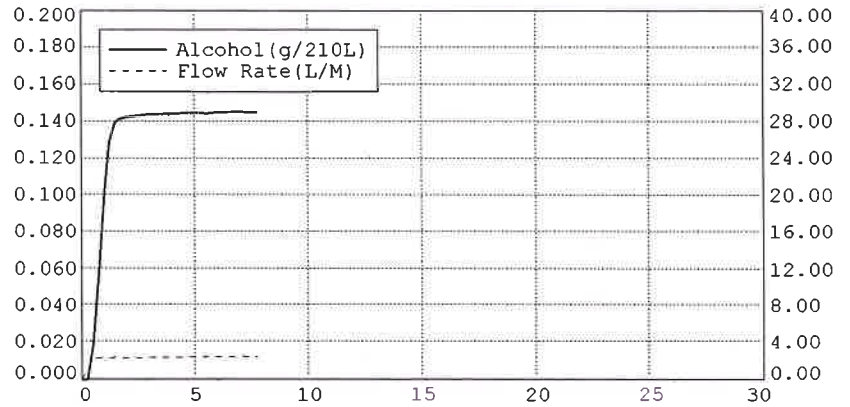

LINEARITY CHECK: Control Test 6

Alaska Department of Public Safety
DATAMASTER dmt: 100361






Date: 06/04/2025
Time: 11:46:05

EXTERNAL STANDARD INFORMATION

NOMINAL: 0.300
TARGET AT 29.43: 0.295
LOT #: AG427706
EXPIRATION: 10/03/2026
TANK PRESSURE: 344 psi

BLANK TEST	0.000	11:48
INTERNAL STANDARD	VERIFIED	11:48
EXTERNAL STANDARD	0.293	11:48
BLANK TEST	0.000	11:49
EXTERNAL STANDARD	0.292	11:49
BLANK TEST	0.000	11:50
EXTERNAL STANDARD	0.293	11:50
BLANK TEST	0.000	11:51
EXTERNAL STANDARD	0.292	11:51
BLANK TEST	0.000	11:52
EXTERNAL STANDARD	0.294	11:53
BLANK TEST	0.000	11:54

Average = 0.2928
Std Dev = 0.0008

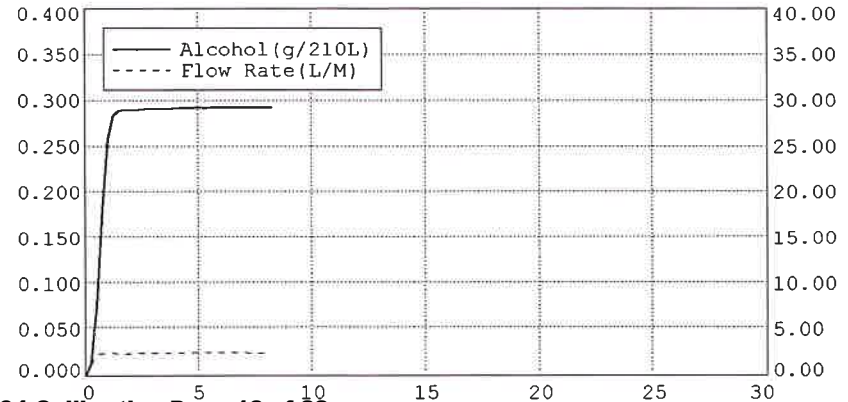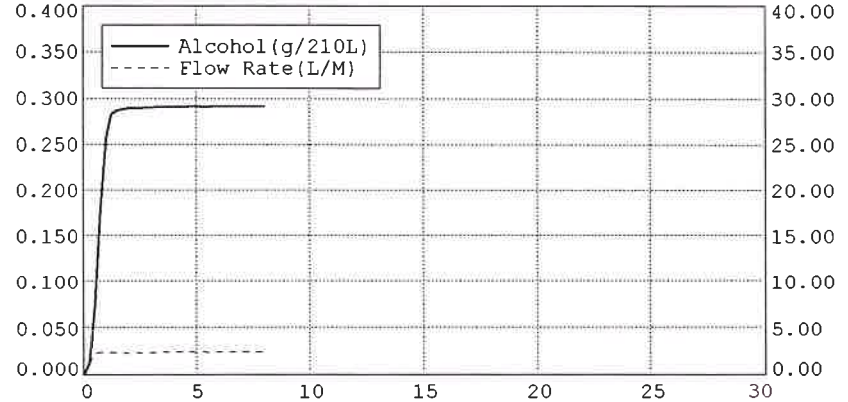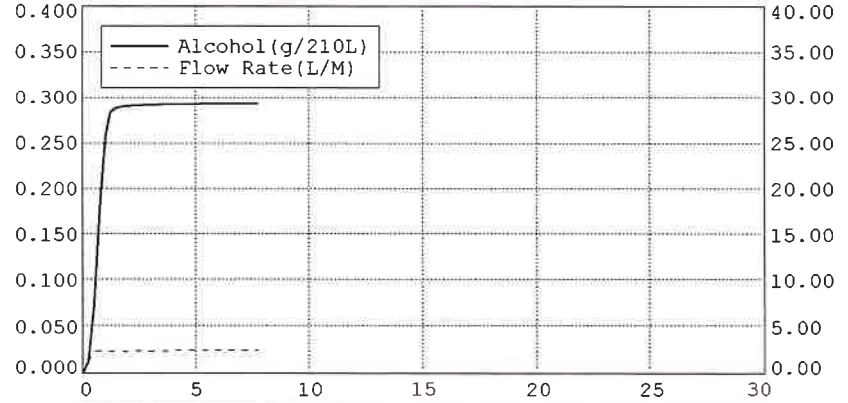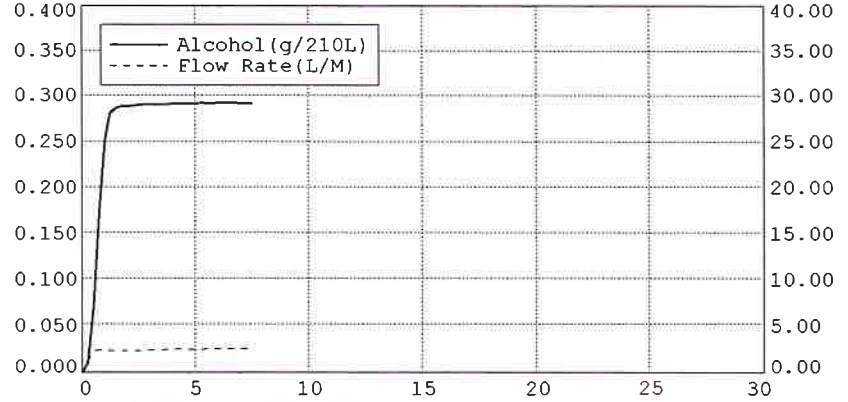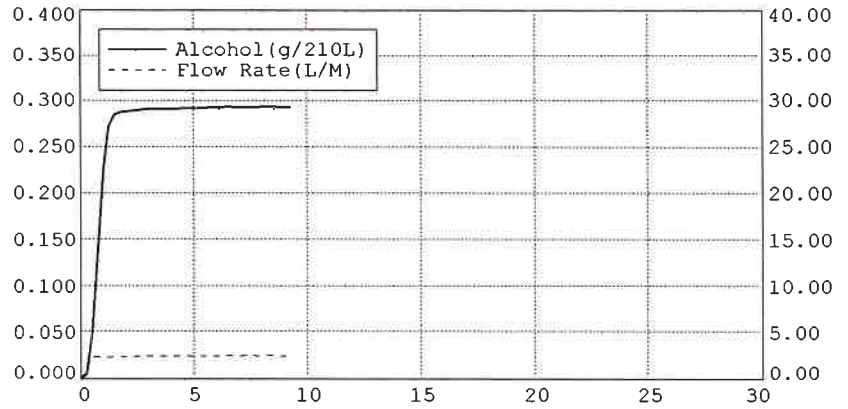

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 12:09:54

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INCOMPLETE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:12
BLANK TEST	0.000	12:12
INTERNAL STANDARD	VERIFIED	12:12
EXTERNAL STANDARD	0.078	12:13
BLANK TEST	0.000	12:14
SUBJECT SAMPLE	INCOMPLETE	12:16

KS

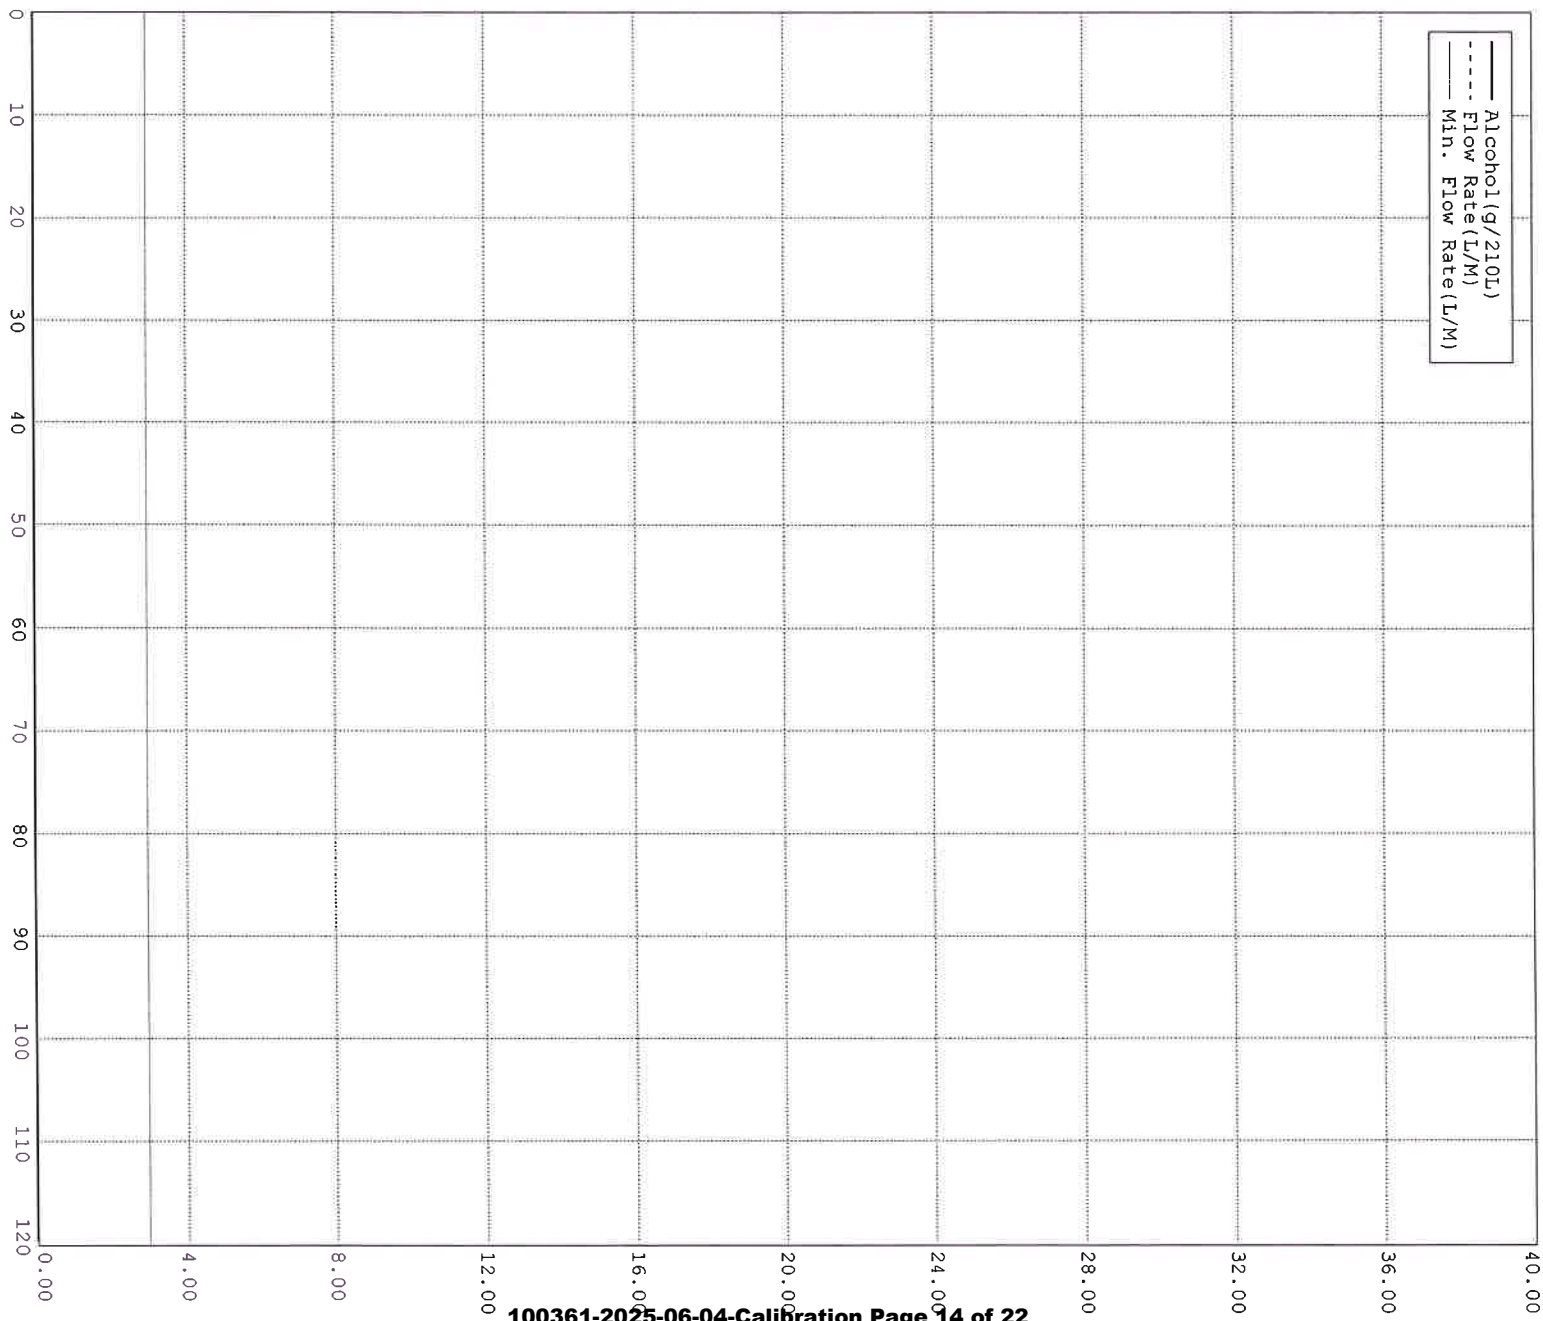

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100361

Date: 06/04/2025
Time: 12:18:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
MAX ATTEMPTS
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

TEST TYPE	PASSED	TIME
DIAGNOSTIC CHECK	0.000	12:20
INTERNAL STANDARD	VERIFIED	12:20
EXTERNAL STANDARD	0.077	12:20
BLANK TEST	0.000	12:21
SUBJECT SAMPLE	XXX	12:22

Maximum Attempts Exceeded

KS

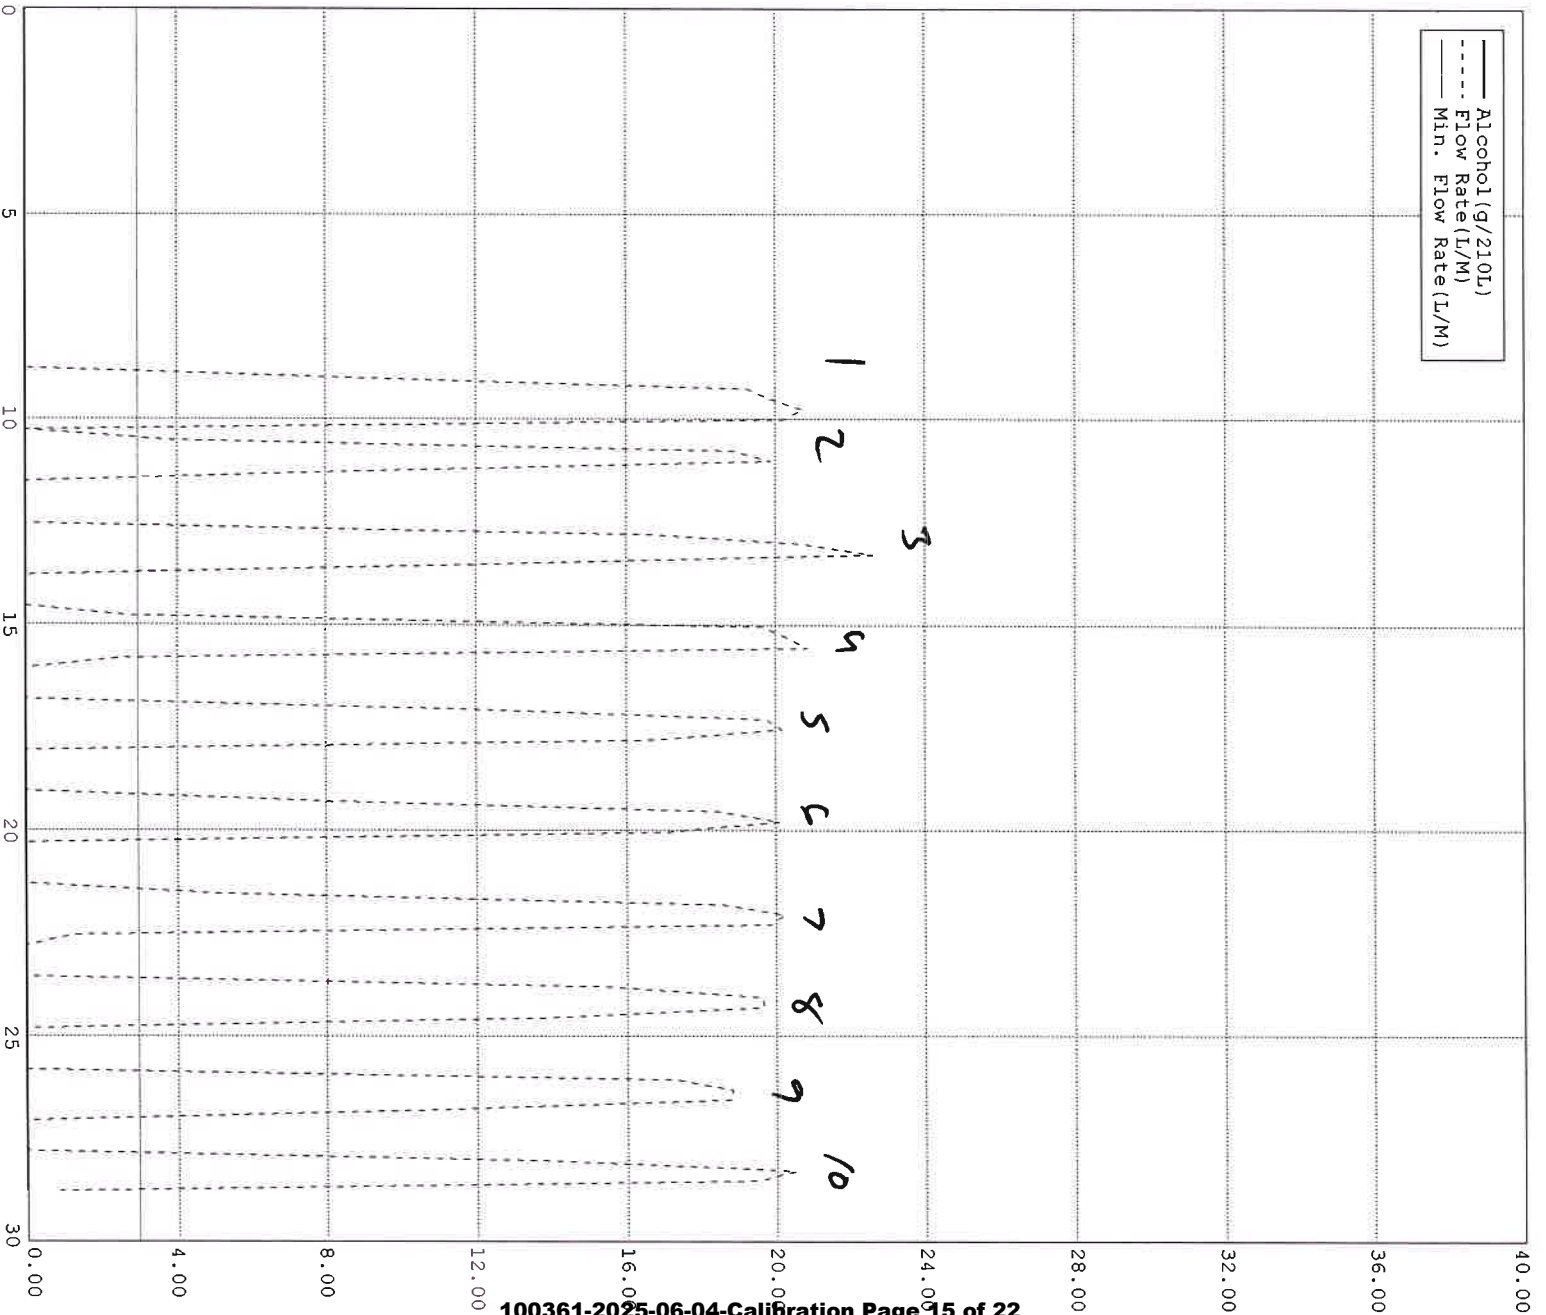

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 12:25:38

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK
BLANK TEST PASSED 12:26
INTERNAL STANDARD VERIFIED 12:27
EXTERNAL STANDARD 0.077 12:27
BLANK TEST 0.000 12:28
SUBJECT SAMPLE INVALID 12:29

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

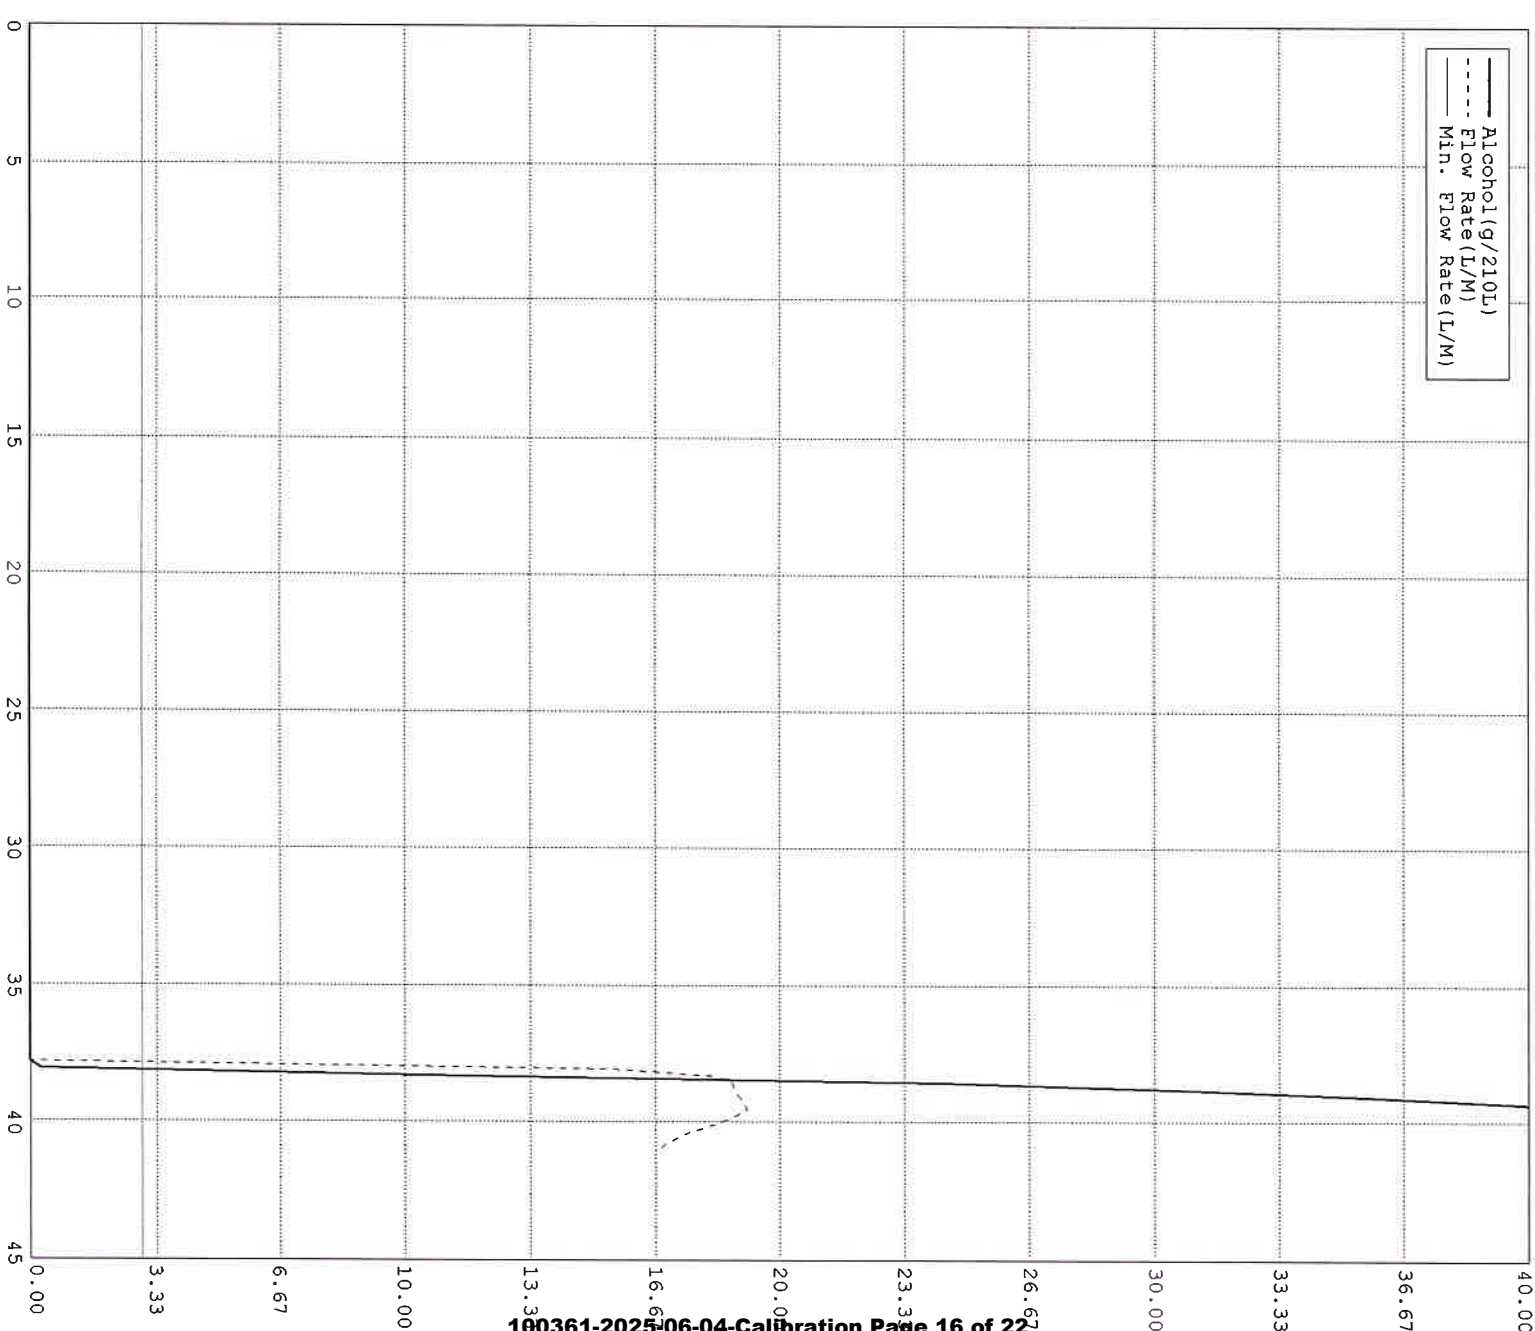

KS

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/09/2025
Time: 08:32:59

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
INVALID
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.85: 0.080
LOT #: AG335202
EXPIRATION: 12/18/2025

TEST TYPE	RESULT	TIME
DIAGNOSTIC CHECK	PASSED	08:34
BLANK TEST	0.000	08:34
INTERNAL STANDARD	VERIFIED	08:34
EXTERNAL STANDARD	0.079	08:34
BLANK TEST	0.000	08:35
SUBJECT SAMPLE	INVALID	08:36

*Invalid test return on
6/9/25 to show slope.
K5619/25*

K5

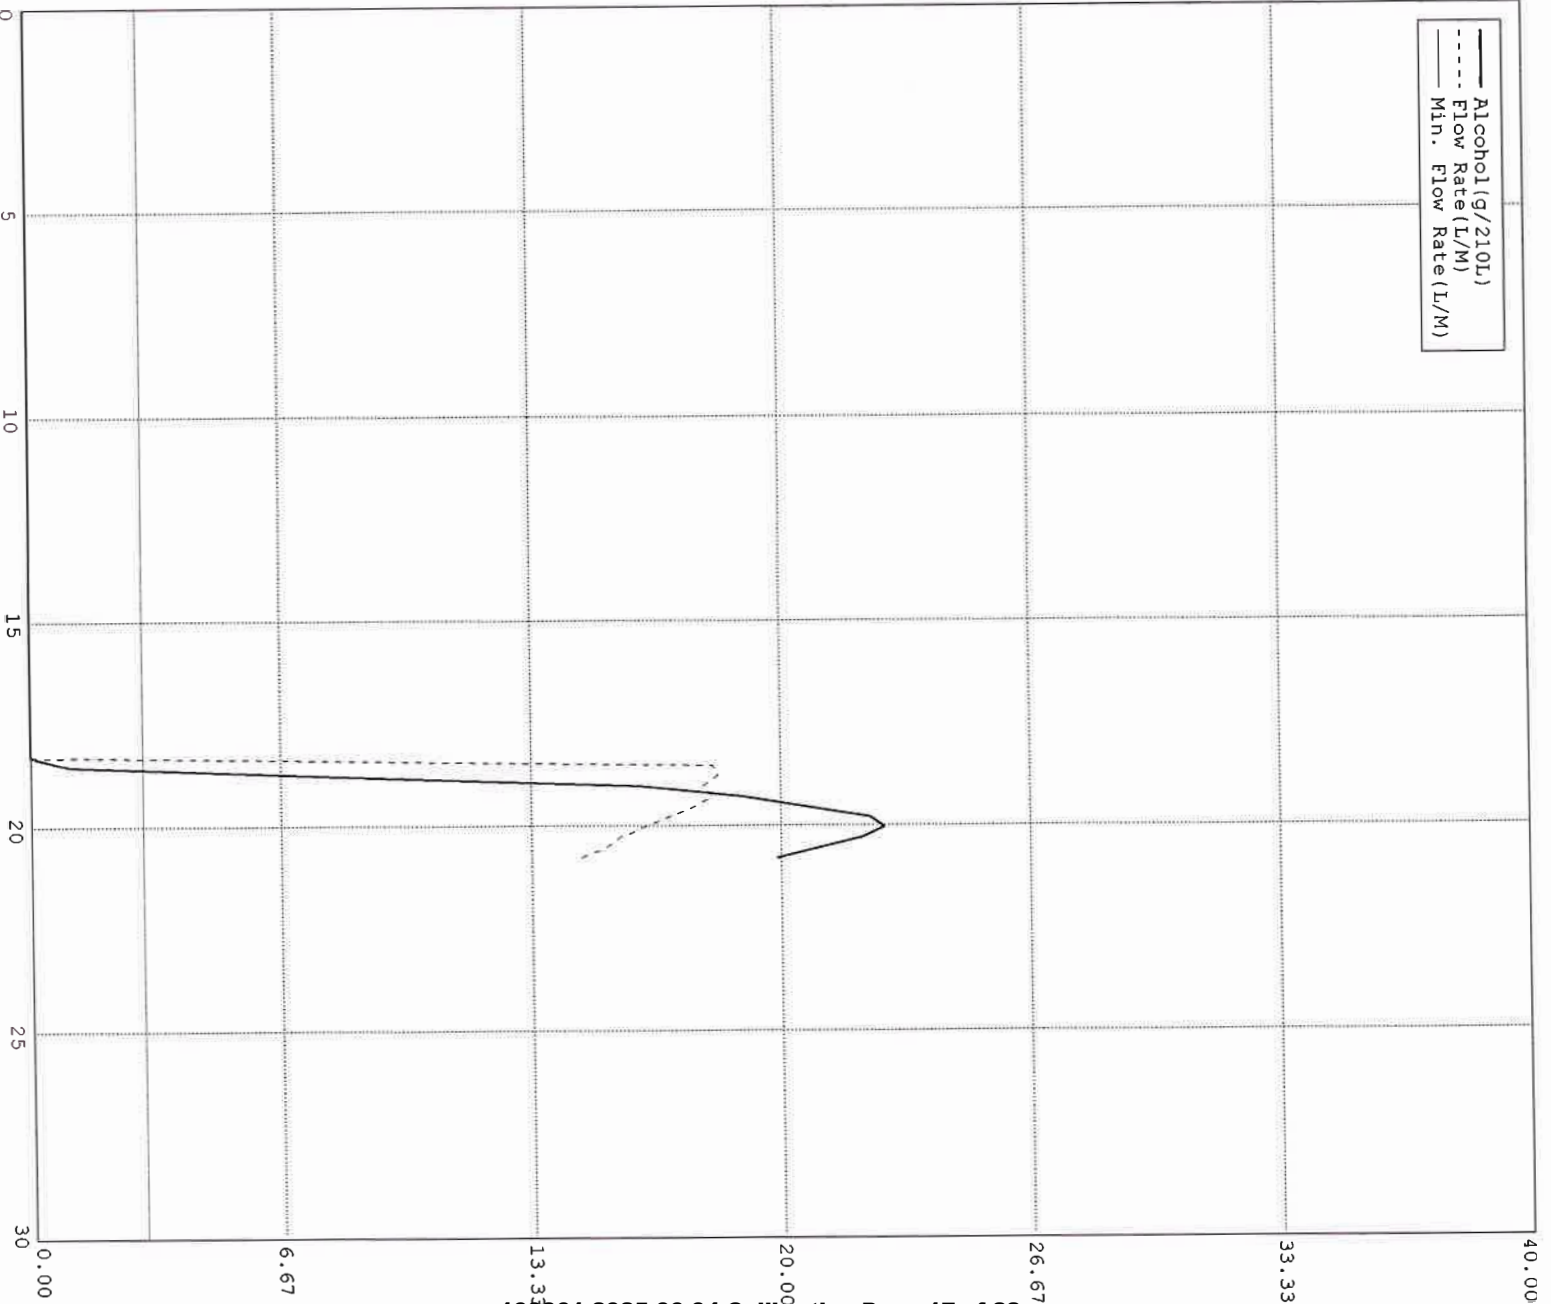

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 14:21:50

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
RFI
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:25
BLANK TEST	0.000	14:25
INTERNAL STANDARD	VERIFIED	14:25
EXTERNAL STANDARD	0.077	14:25
BLANK TEST	0.000	14:26

RFI DETECTED

KS

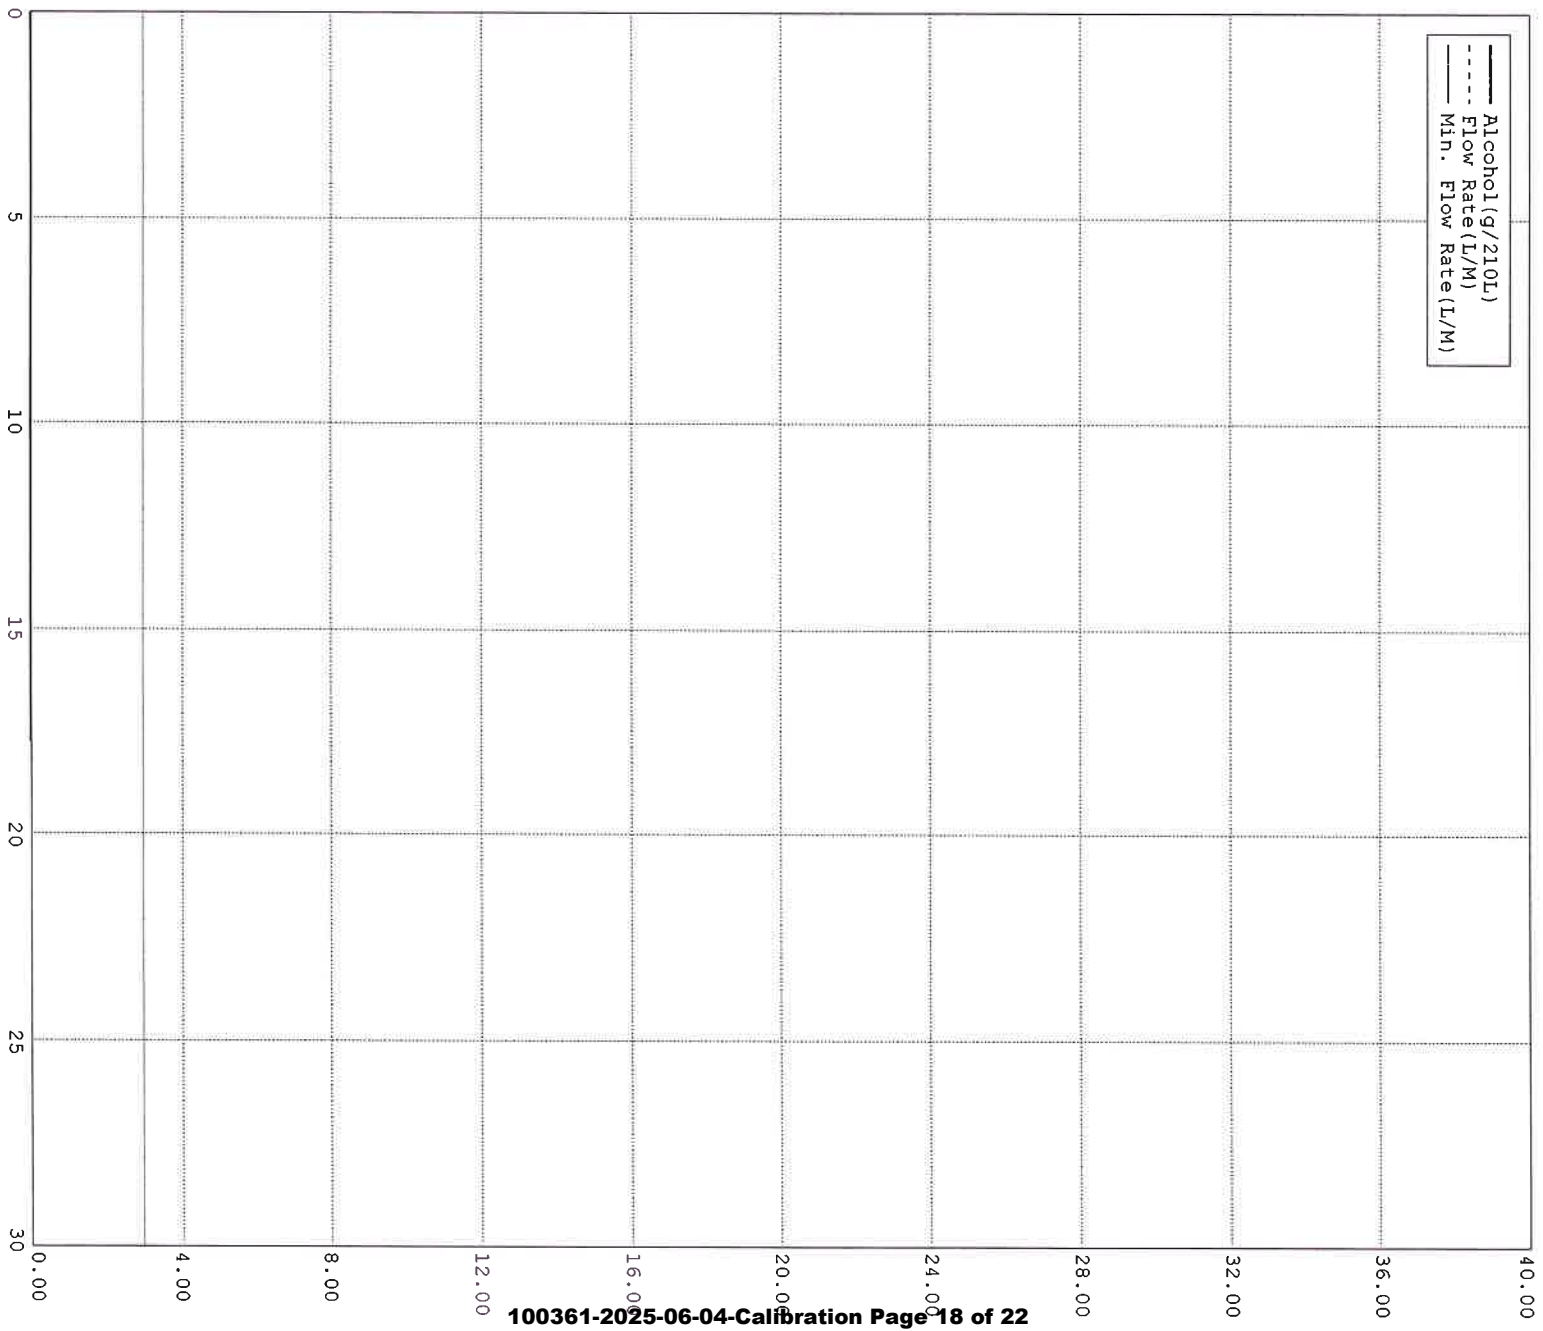

SUBJECT TEST

Alaska Department of Public Safety
DATA MASTER dmt: 100361

Date: 06/04/2025
Time: 12:38:15

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - ACETONE
CASE/REPORT: XXX
TEST TYPE: TEST


EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.42: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:39
BLANK TEST	0.000	12:39
INTERNAL STANDARD	VERIFIED	12:39
Xq = 0.088 (0.00%)		
EXTERNAL STANDARD	0.077	12:39
X[1] = 0.0767 (0.0001)	(0.0036)	
BLANK TEST	0.000	12:40
SUBJECT SAMPLE	XXX	12:41
X[1] = 0.1118 (-0.0220)	(0.0016)	

Interference Detected

F2 Average: -0.0002
F3 Average: 0.0035
KS 6/5/25

KS

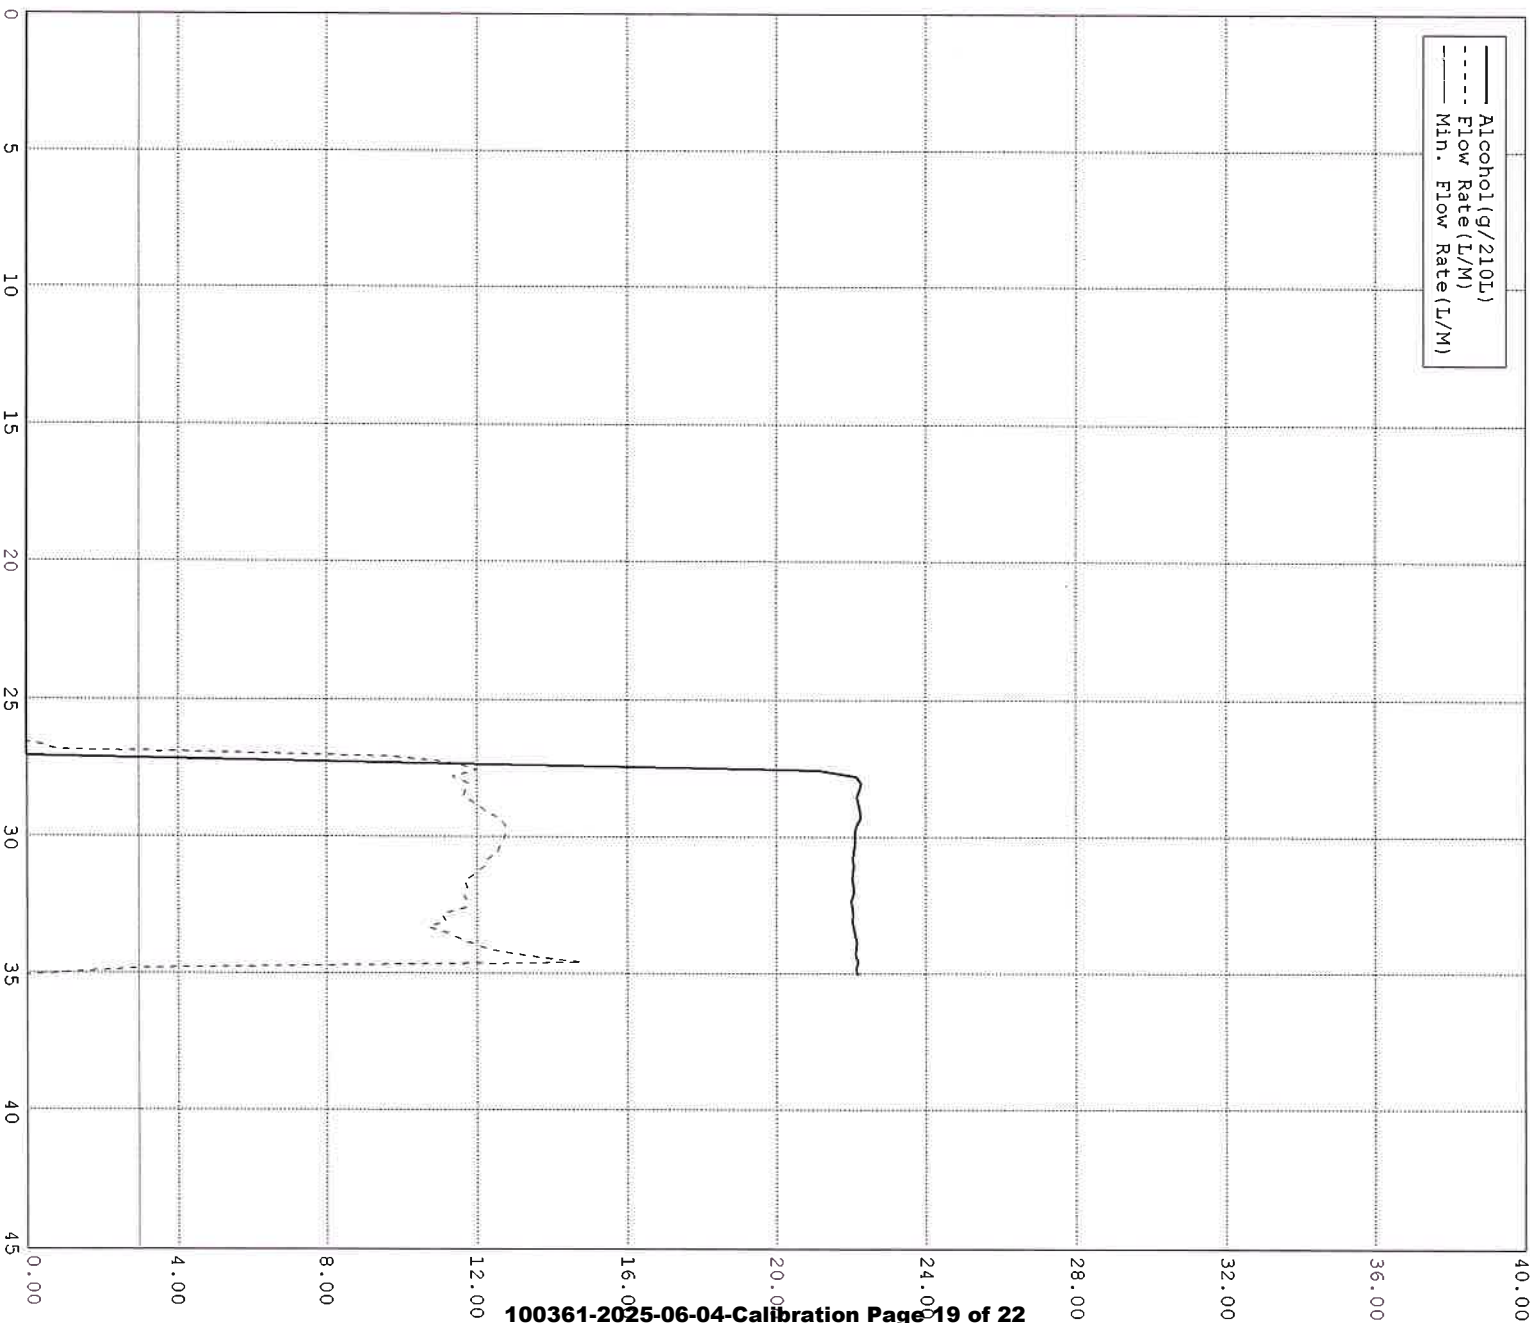

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 12:45:24

SUBJECT NAME:
TEST TEST
LICENSE #: XXX

OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746


DEPT/AGENCY:
INTERFERENCE - IPA
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:46
BLANK TEST	0.000	12:46
INTERNAL STANDARD	VERIFIED	12:47
Xq = 0.088 (0.708)		
EXTERNAL STANDARD	0.077	12:47
X[1] = 0.0771 (0.0001)	(0.0037)	
BLANK TEST	0.000	12:48
SUBJECT SAMPLE	XXX	12:48
X[1] = 0.1222 (-0.0232)	(0.0029)	

Interference Detected

KS

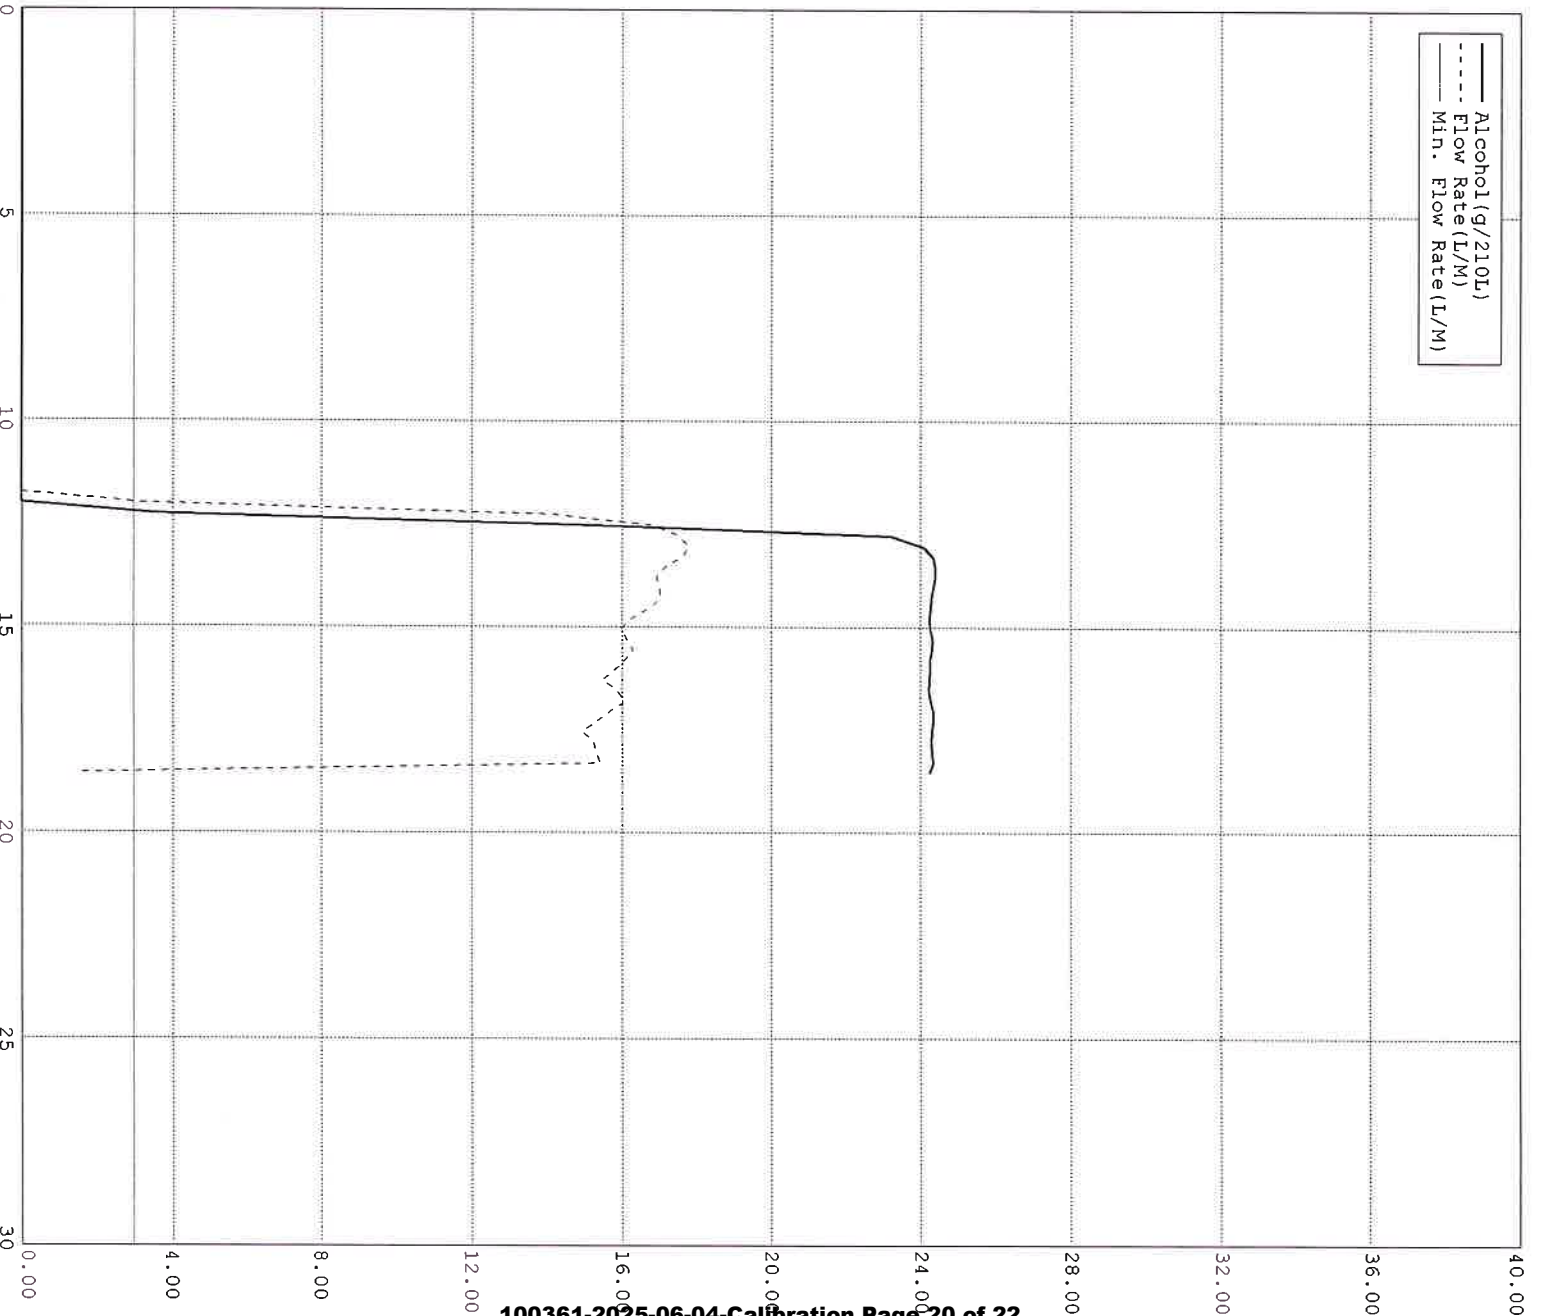

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 12:52:26

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
INTERFERENCE - NEGATIVE
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	12:53
BLANK TEST	0.000	12:53
INTERNAL STANDARD	VERIFIED	12:53
Xq = 0.089 (0.89%)		
EXTERNAL STANDARD	0.077	12:53
X[1] = 0.0774 (-0.0003)	(0.0040)	
BLANK TEST	0.000	12:54
SUBJECT SAMPLE (Vol=1.70L)	0.094	12:55
X[1] = 0.0945 (0.0010)	(0.0011)	
BLANK TEST	0.000	12:56
EXTERNAL STANDARD	0.077	12:56
X[1] = 0.0769 (-0.0005)	(0.0025)	
BLANK TEST	0.000	12:57

KCS

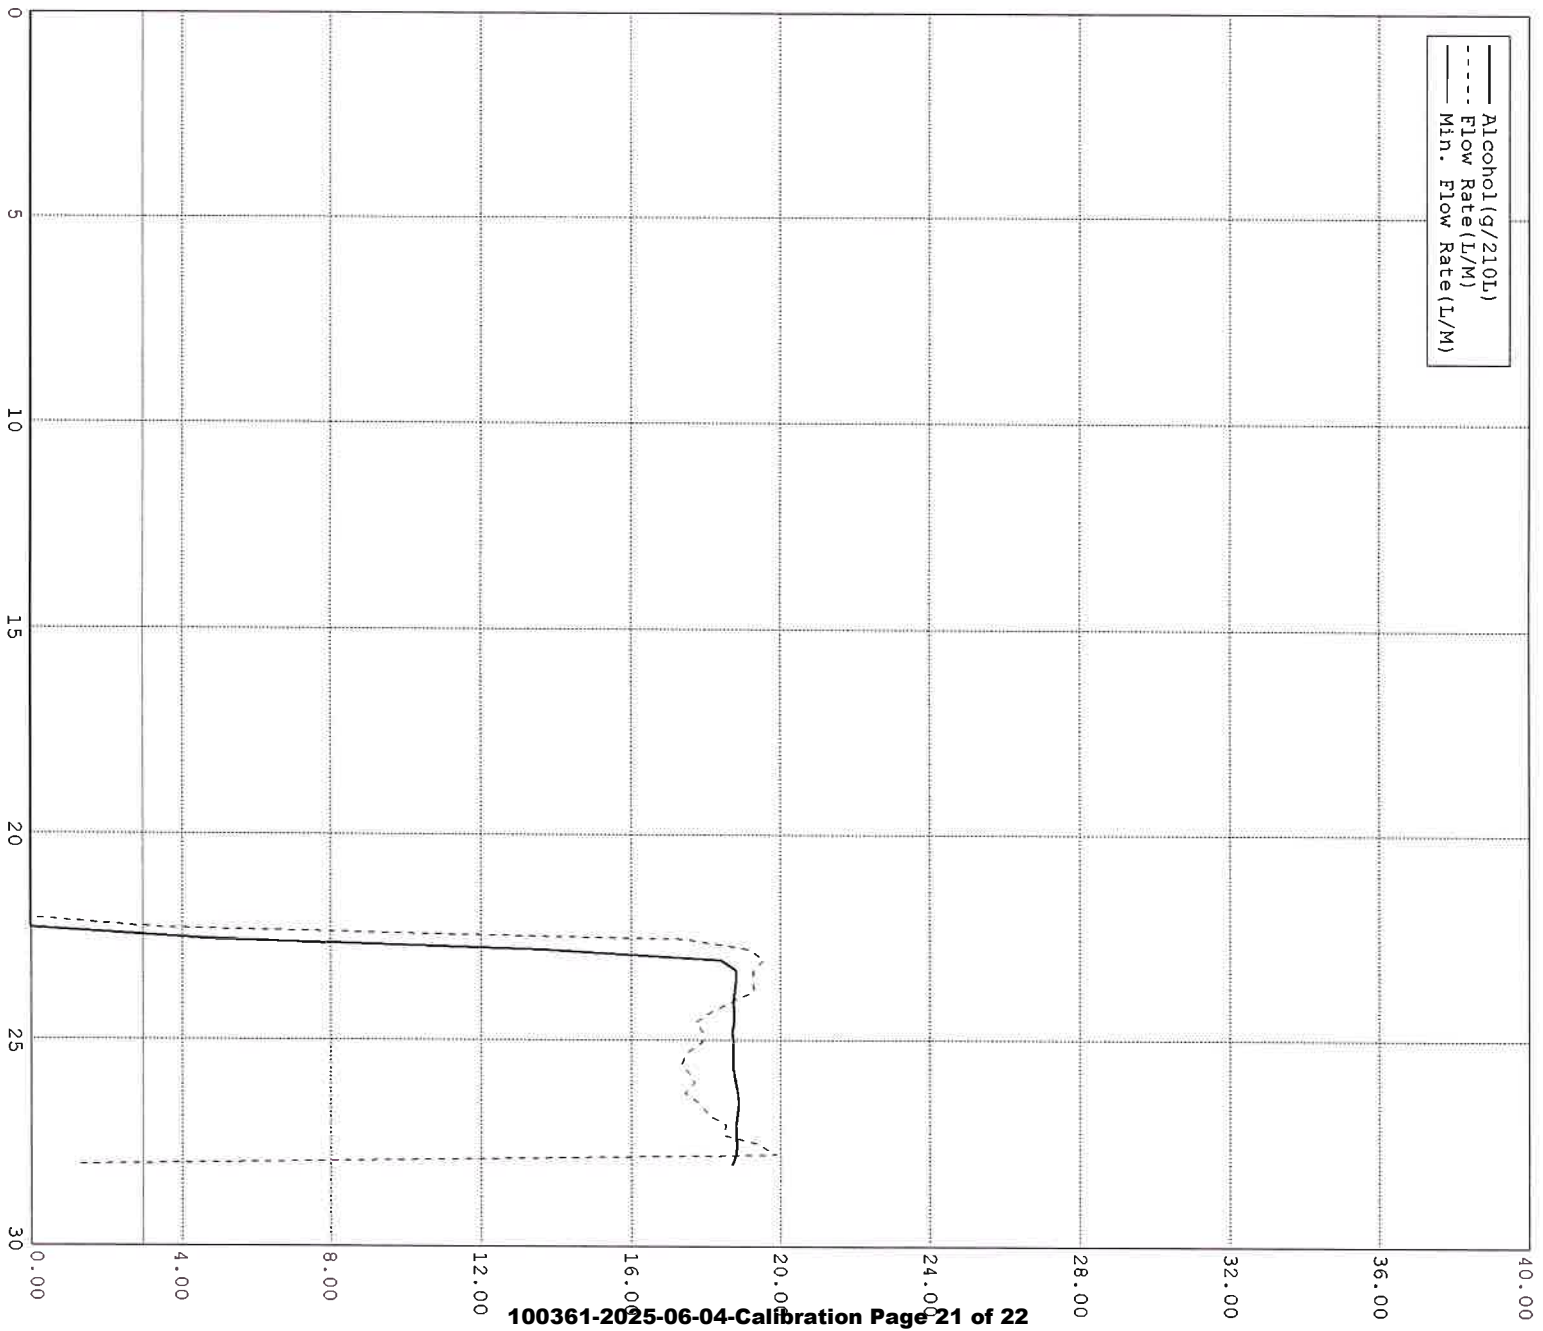

SUBJECT TEST

Alaska Department of Public Safety
DATAMASTER dmt: 100361

Date: 06/04/2025
Time: 14:56:36

SUBJECT NAME:
TEST TEST
LICENSE #: XXX


OPERATOR NAME:
KAIJA SWISHER
OPERATOR'S #: 10746

DEPT/AGENCY:
NON DRINKING SUBJECT TEST
CASE/REPORT: XXX
TEST TYPE: TEST

EXTERNAL STANDARD INFORMATION
NOMINAL: 0.080
TARGET AT 29.41: 0.079
LOT #: AG335202
EXPIRATION: 12/18/2025

DIAGNOSTIC CHECK	PASSED	14:57
BLANK TEST	0.000	14:58
INTERNAL STANDARD	VERIFIED	14:58
EXTERNAL STANDARD	0.078	14:58
BLANK TEST	0.000	14:59
SUBJECT SAMPLE (Vol=1.69L)	0.000	14:59
BLANK TEST	0.000	15:00
EXTERNAL STANDARD	0.078	15:00
BLANK TEST	0.000	15:01

Alcohol(g/210L)
Flow Rate(L/M)
Min. Flow Rate(L/M)

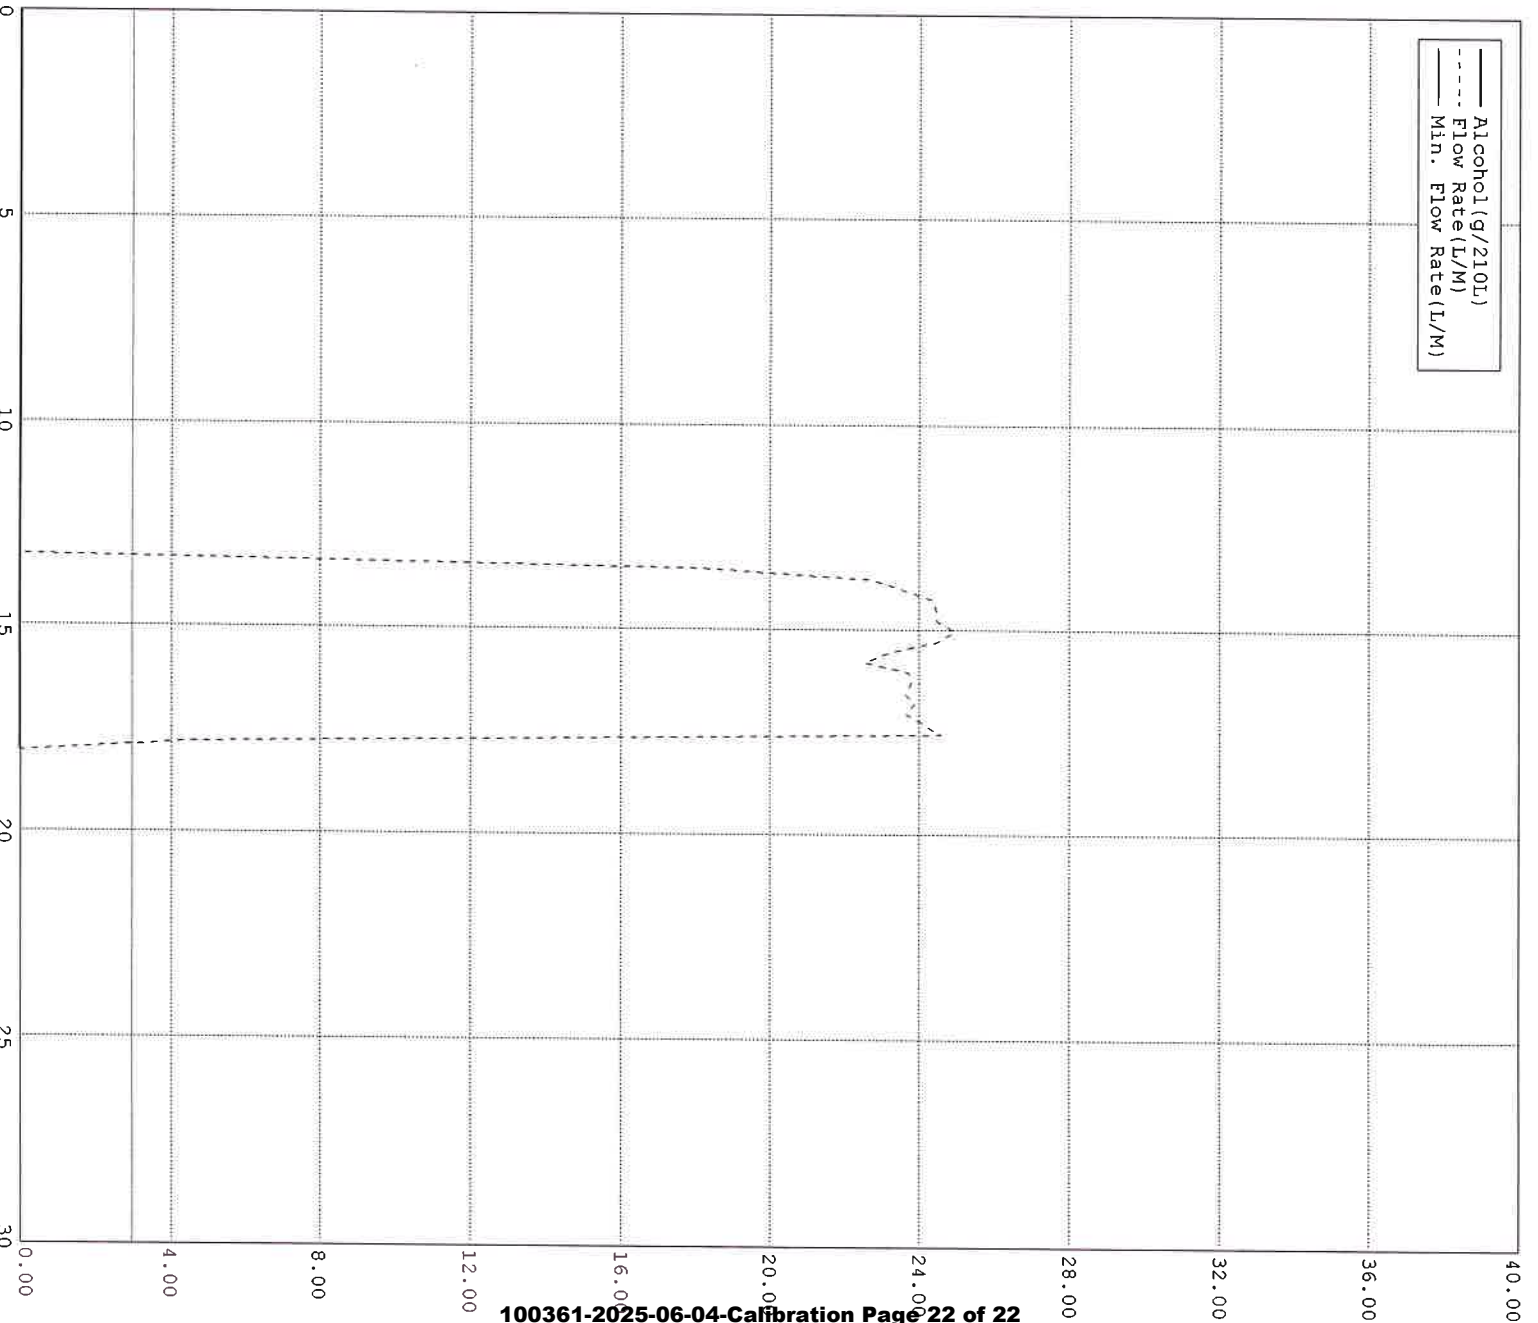

KS